

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040519\
 Data File : P0055008.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Apr 2019 1:46
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1254 LOD 40PPB
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Manual Integrations
 APPROVED

Sohil
 4/8/2019 5:25:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 04:05:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.297	3.610	895356	798361	25.799	25.017
2)	SA Decachlor...	9.912	8.578	1130277	790304	22.928	24.815
Target Compounds							
26)	L6 AR-1254-1	6.307	5.483	124493	142786	68.660	65.334
27)	L6 AR-1254-2	6.524	5.628	195442	127328	68.462	65.669
28)	L6 AR-1254-3	6.890	6.031	199474	200310	63.432	62.486
29)	L6 AR-1254-4	7.175	6.258	150013	120565	61.321	61.578m
30)	L6 AR-1254-5	7.591	6.673	149507	163459	55.780	56.861

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040519\
Data File : PO055008.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Apr 2019 1:46
Operator : SM/SJ
Sample : K1560-07
Misc : AR1254 LOD 40PPB
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 04:05:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

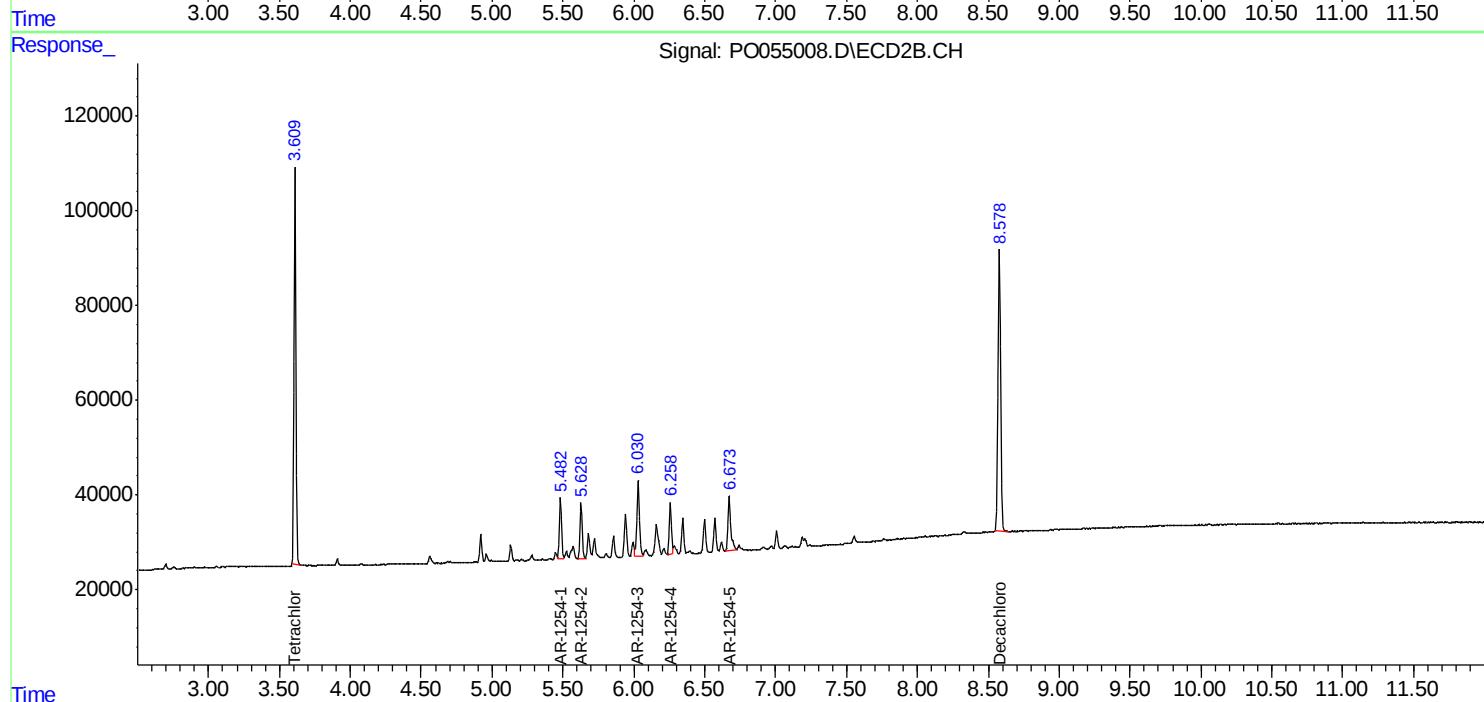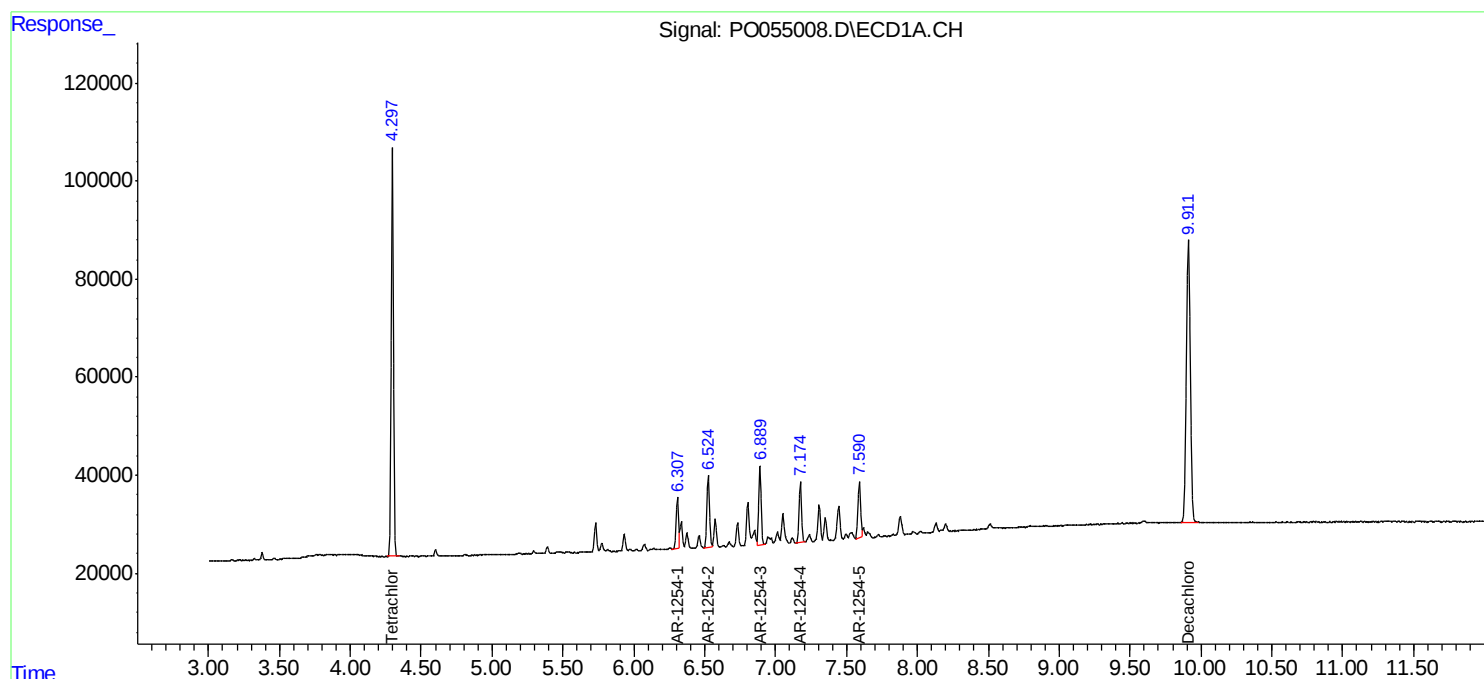

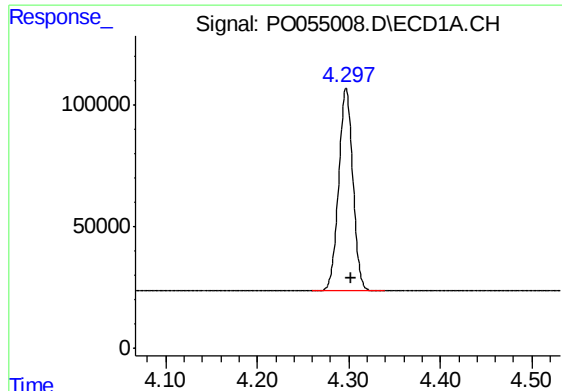


#1 Tetrachloro-m-xylene

R.T.: 4.297 min
Delta R.T.: -0.006 min
Response: 895356
Conc: 25.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:20 PM

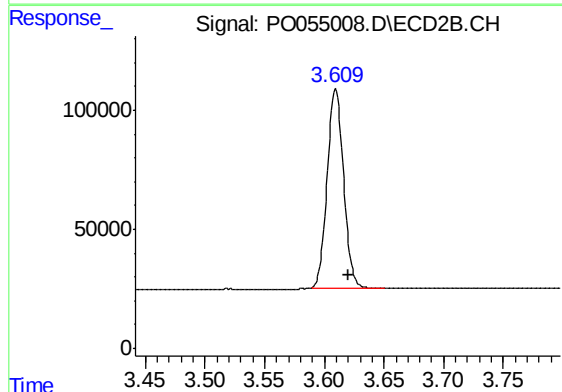


#1 Tetrachloro-m-xylene

R.T.: 3.610 min
Delta R.T.: -0.011 min
Response: 798361
Conc: 25.02 ng/ml

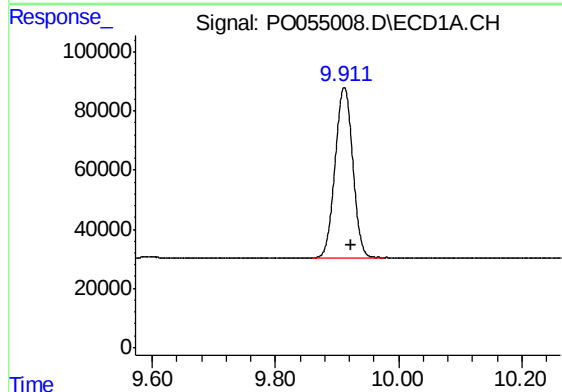


#2 Decachlorobiphenyl

R.T.: 9.912 min
Delta R.T.: -0.011 min
Response: 1130277
Conc: 22.93 ng/ml

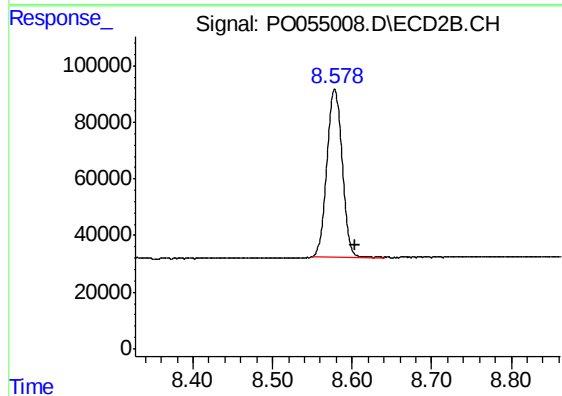

#2 Decachlorobiphenyl

R.T.: 8.578 min
Delta R.T.: -0.026 min
Response: 790304
Conc: 24.81 ng/ml

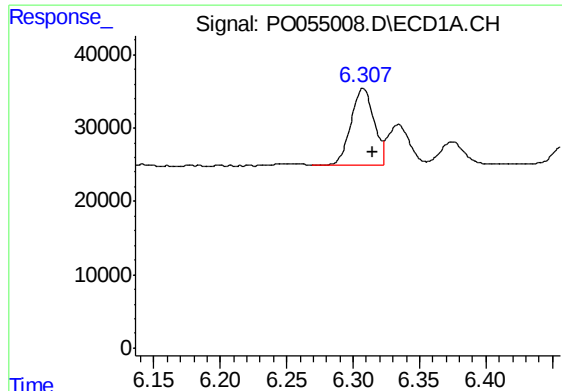


#26 AR-1254-1

R.T.: 6.307 min
Delta R.T.: -0.007 min
Response: 124493
Conc: 68.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:20 PM

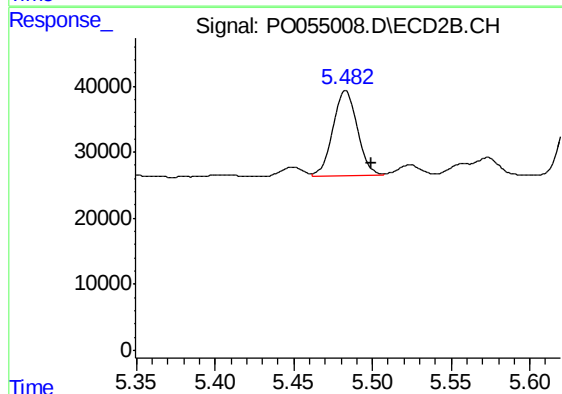


#26 AR-1254-1

R.T.: 5.483 min
Delta R.T.: -0.017 min
Response: 142786
Conc: 65.33 ng/ml

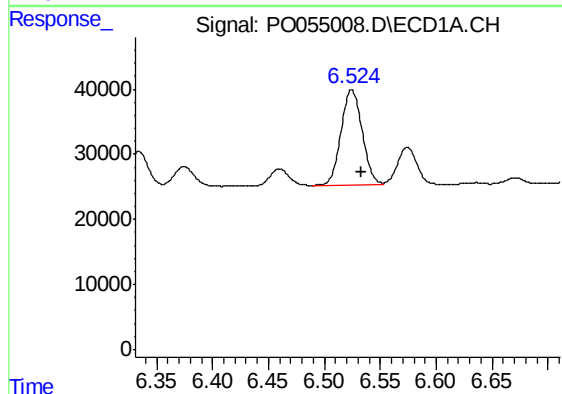


#27 AR-1254-2

R.T.: 6.524 min
Delta R.T.: -0.009 min
Response: 195442
Conc: 68.46 ng/ml

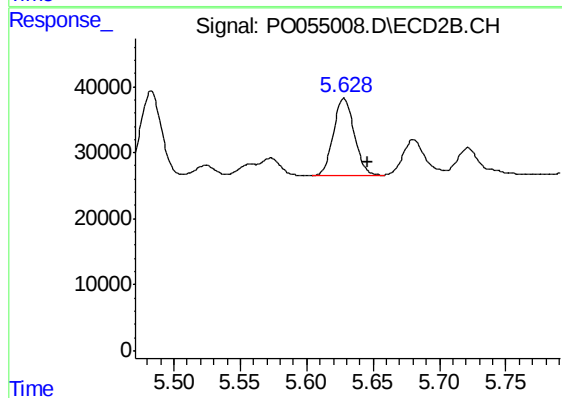

#27 AR-1254-2

R.T.: 5.628 min
Delta R.T.: -0.018 min
Response: 127328
Conc: 65.67 ng/ml

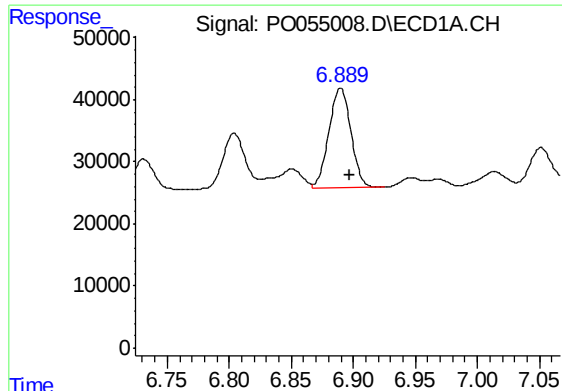


#28 AR-1254-3

R.T.: 6.890 min
Delta R.T.: -0.008 min
Response: 199474
Conc: 63.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:20 PM

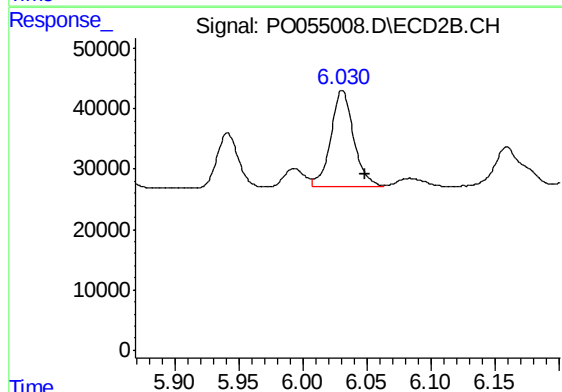


#28 AR-1254-3

R.T.: 6.031 min
Delta R.T.: -0.018 min
Response: 200310
Conc: 62.49 ng/ml

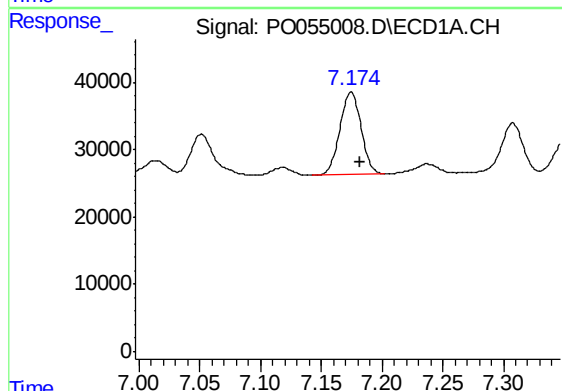


#29 AR-1254-4

R.T.: 7.175 min
Delta R.T.: -0.008 min
Response: 150013
Conc: 61.32 ng/ml

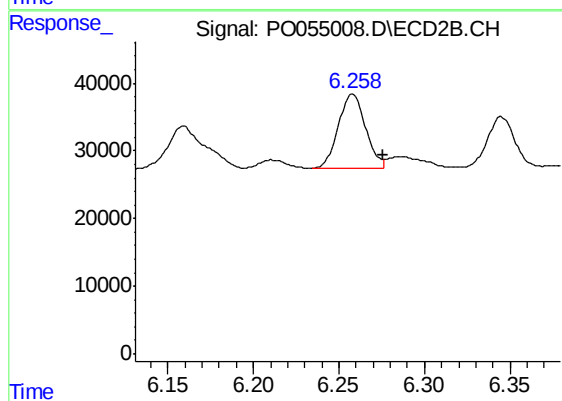

#29 AR-1254-4

R.T.: 6.258 min
Delta R.T.: -0.018 min
Response: 120565
Conc: 61.58 ng/ml m

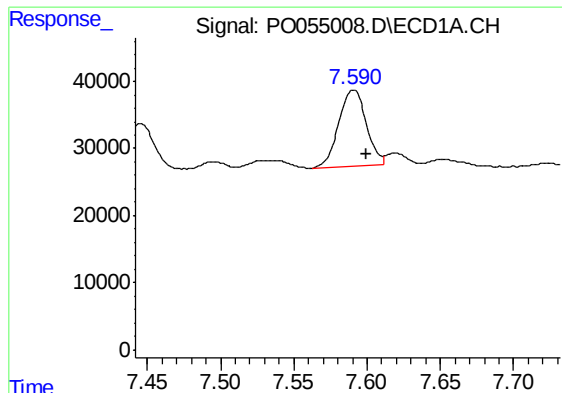


#30 AR-1254-5

R.T.: 7.591 min
Delta R.T.: -0.009 min
Response: 149507
Conc: 55.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:20 PM

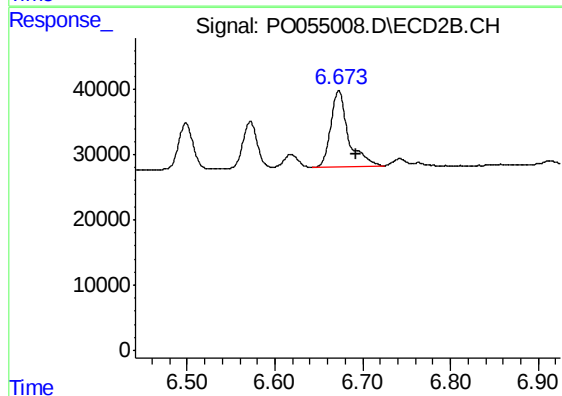

#30 AR-1254-5

R.T.: 6.673 min
Delta R.T.: -0.019 min
Response: 163459
Conc: 56.86 ng/ml