

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040519\
 Data File : P0055011.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Apr 2019 2:36
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1262 LOD 40PPB
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Manual Integrations
 APPROVED

Sohil
 4/8/2019 5:25:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 04:06:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.297	3.609	938718	858250	27.048	26.894m
2)	SA Decachlor...	9.911	8.579	1102567	774225	22.366	24.310
Target Compounds							
36)	L8 AR-1262-1	7.666	6.710	204412	186403	61.347m	62.658
37)	L8 AR-1262-2	8.200	7.208	320436	281914	54.087	57.520
38)	L8 AR-1262-3	8.497	7.491	221473	116842	53.460	56.900
39)	L8 AR-1262-4	8.583	7.554	167573	206395	52.009	56.982
40)	L8 AR-1262-5	9.207	8.045	109485	94346	50.078	58.459

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040519\
Data File : PO055011.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Apr 2019 2:36
Operator : SM/SJ
Sample : K1560-07
Misc : AR1262 LOD 40PPB
ALS Vial : 49 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 04:06:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

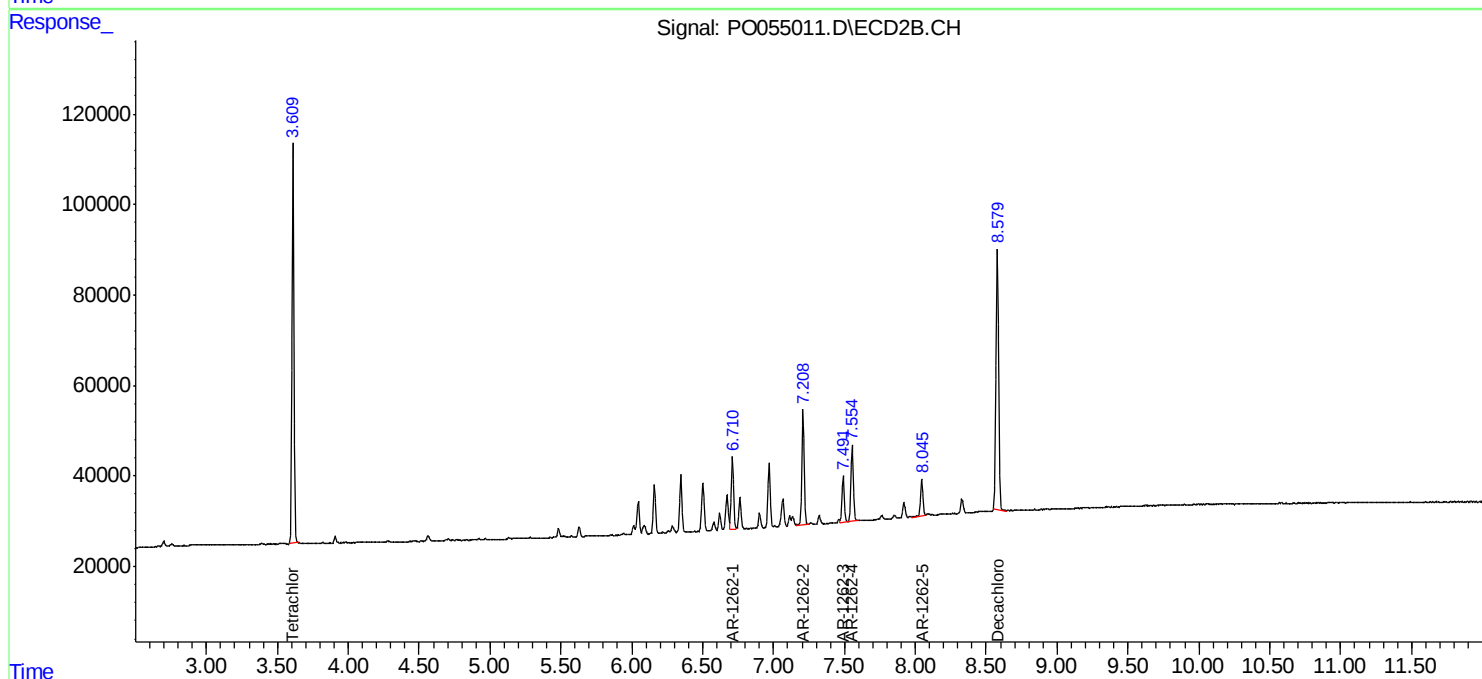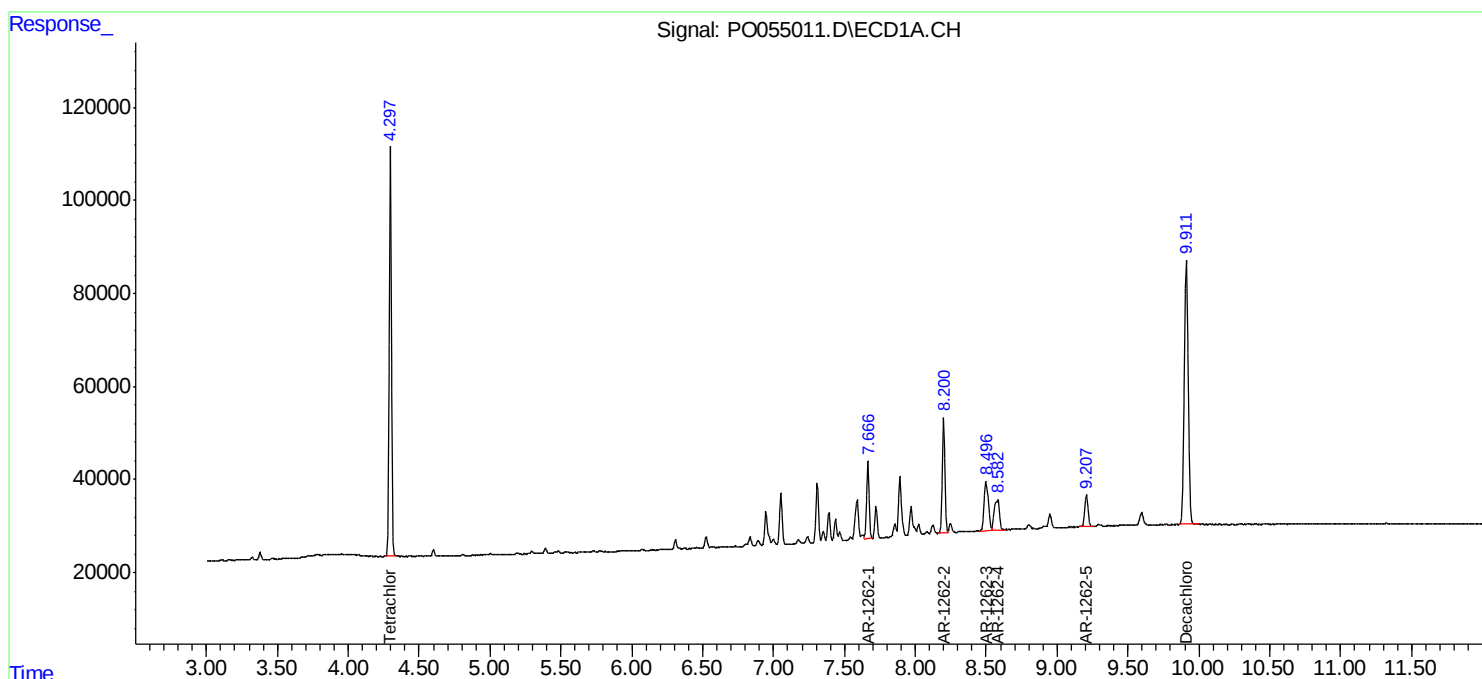

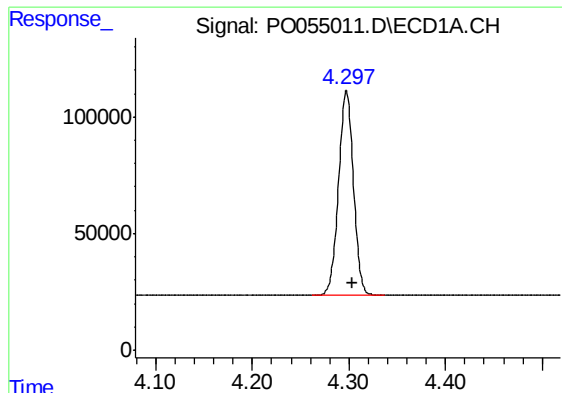


#1 Tetrachloro-m-xylene

R.T.: 4.297 min
Delta R.T.: -0.006 min
Response: 938718
Conc: 27.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:26 PM

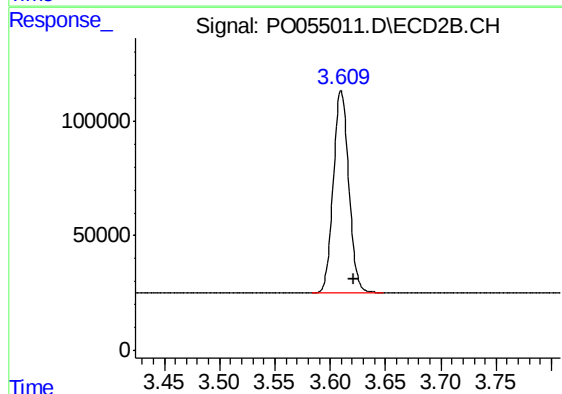


#1 Tetrachloro-m-xylene

R.T.: 3.609 min
Delta R.T.: -0.011 min
Response: 858250
Conc: 26.89 ng/ml m

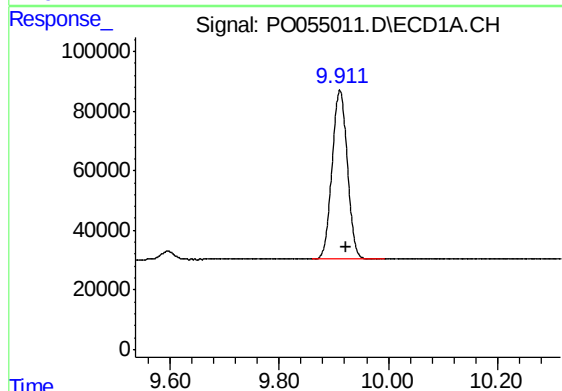


#2 Decachlorobiphenyl

R.T.: 9.911 min
Delta R.T.: -0.012 min
Response: 1102567
Conc: 22.37 ng/ml

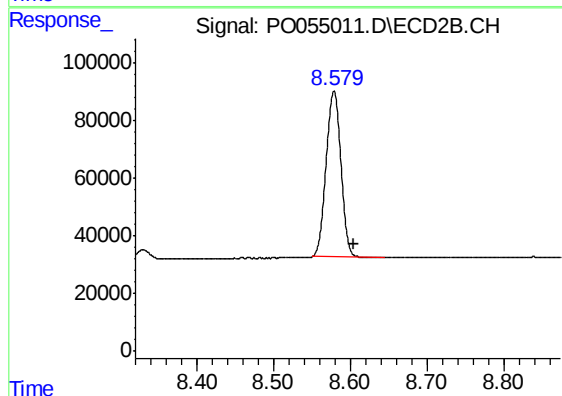

#2 Decachlorobiphenyl

R.T.: 8.579 min
Delta R.T.: -0.025 min
Response: 774225
Conc: 24.31 ng/ml

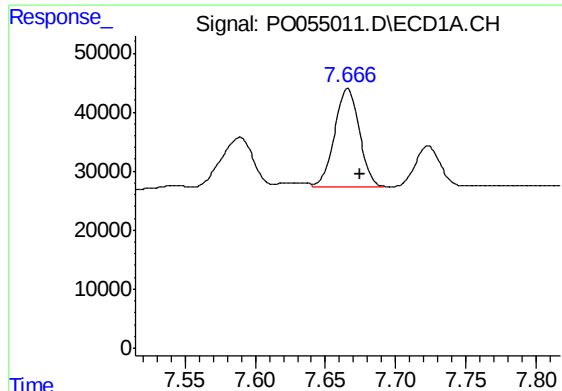


#36 AR-1262-1

R.T.: 7.666 min
Delta R.T.: -0.009 min
Response: 204412
Conc: 61.35 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:26 PM

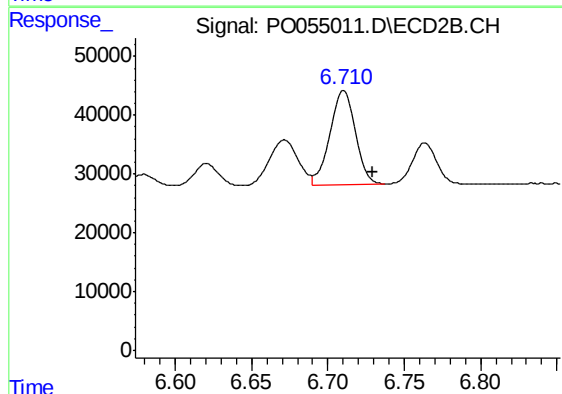


#36 AR-1262-1

R.T.: 6.710 min
Delta R.T.: -0.019 min
Response: 186403
Conc: 62.66 ng/ml

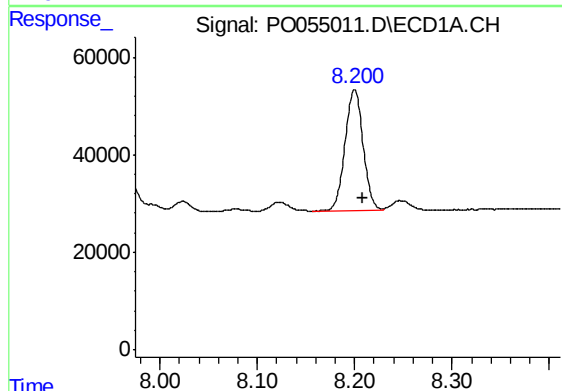


#37 AR-1262-2

R.T.: 8.200 min
Delta R.T.: -0.009 min
Response: 320436
Conc: 54.09 ng/ml

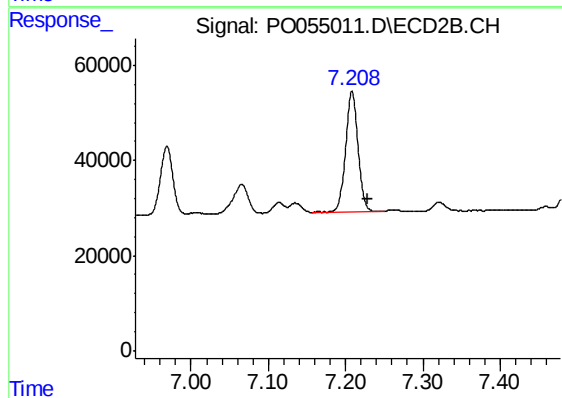

#37 AR-1262-2

R.T.: 7.208 min
Delta R.T.: -0.021 min
Response: 281914
Conc: 57.52 ng/ml

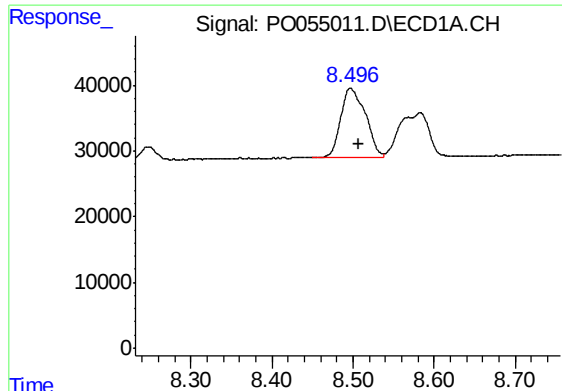


#38 AR-1262-3

R.T.: 8.497 min
Delta R.T.: -0.010 min
Response: 221473
Conc: 53.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:26 PM

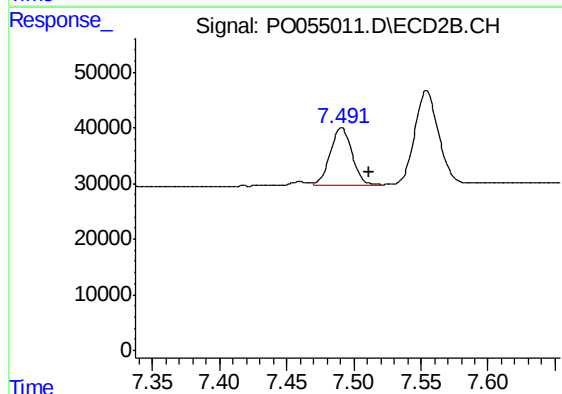


#38 AR-1262-3

R.T.: 7.491 min
Delta R.T.: -0.020 min
Response: 116842
Conc: 56.90 ng/ml

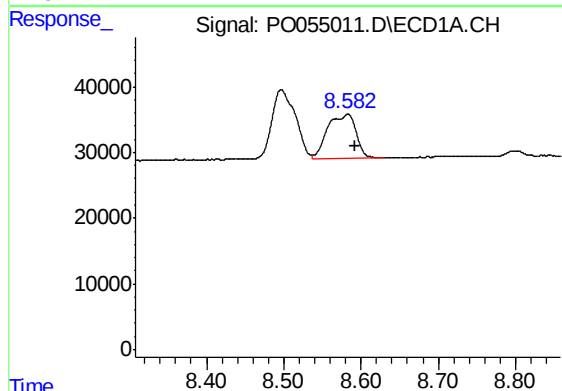


#39 AR-1262-4

R.T.: 8.583 min
Delta R.T.: -0.010 min
Response: 167573
Conc: 52.01 ng/ml

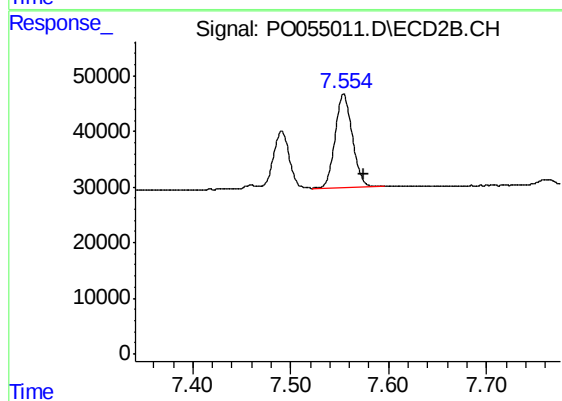

#39 AR-1262-4

R.T.: 7.554 min
Delta R.T.: -0.021 min
Response: 206395
Conc: 56.98 ng/ml

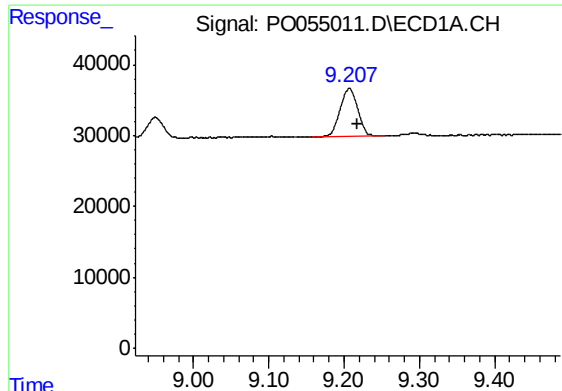


#40 AR-1262-5

R.T.: 9.207 min
Delta R.T.: -0.011 min
Response: 109485
Conc: 50.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:26 PM

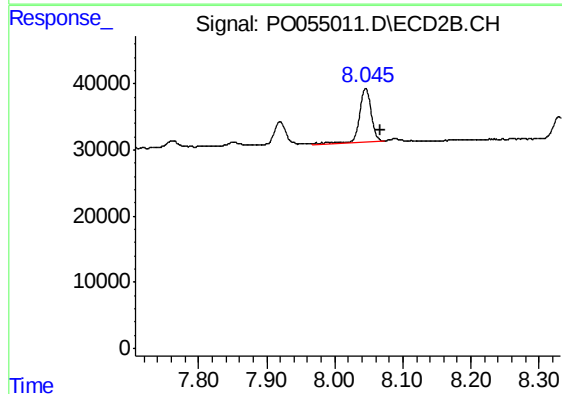

#40 AR-1262-5

R.T.: 8.045 min
Delta R.T.: -0.021 min
Response: 94346
Conc: 58.46 ng/ml