

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040519\
 Data File : P0055013.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Apr 2019 3:10
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1268 LOD 25PPB
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Manual Integrations
 APPROVED

Sohil
 4/8/2019 5:25:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 04:07:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.298	3.610	944891	843716	27.226	26.439
2) SA Decachlor...	9.913	8.579	1220082	856992	24.749	26.909
Target Compounds						
41) L9 AR-1268-1	8.495	7.491	233736	197769	32.840	34.978
42) L9 AR-1268-2	8.585	7.556	209736	177191	32.011	34.262
43) L9 AR-1268-3	8.801	7.762	175291	152472	32.179	35.430
44) L9 AR-1268-4	9.207	8.046	74844	65009	31.371	35.067
45) L9 AR-1268-5	9.596	8.330	521191	402058	31.635	35.322m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040519\
Data File : PO055013.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Apr 2019 3:10
Operator : SM/SJ
Sample : K1560-07
Misc : AR1268 LOD 25PPB
ALS Vial : 51 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 04:07:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

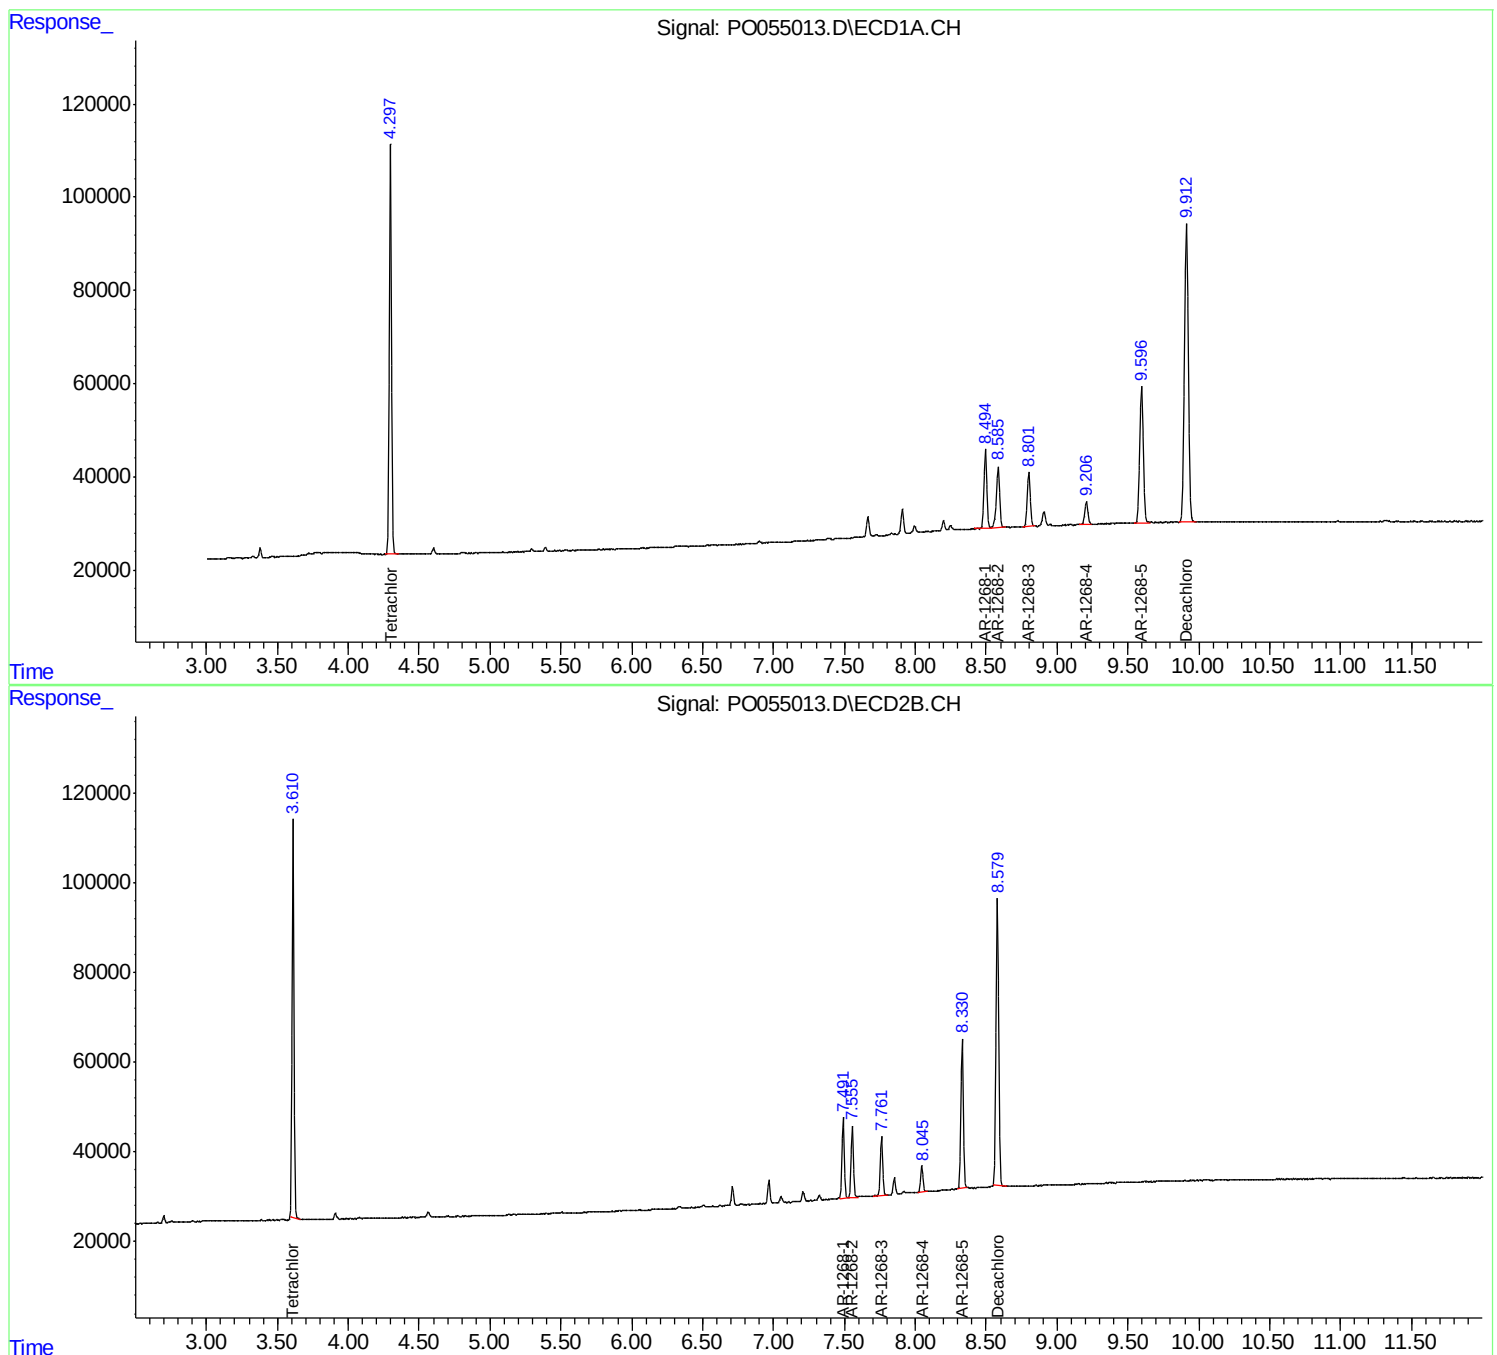

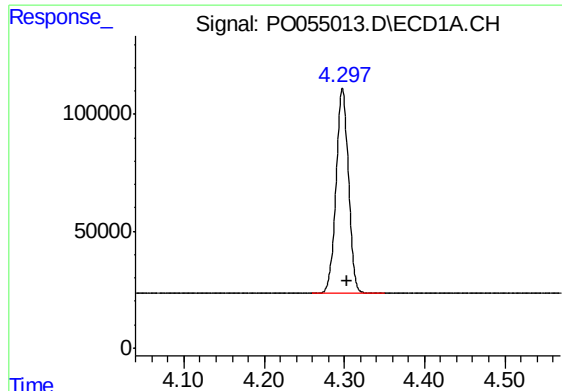


#1 Tetrachloro-m-xylene

R.T.: 4.298 min
Delta R.T.: -0.005 min
Response: 944891
Conc: 27.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:29 PM

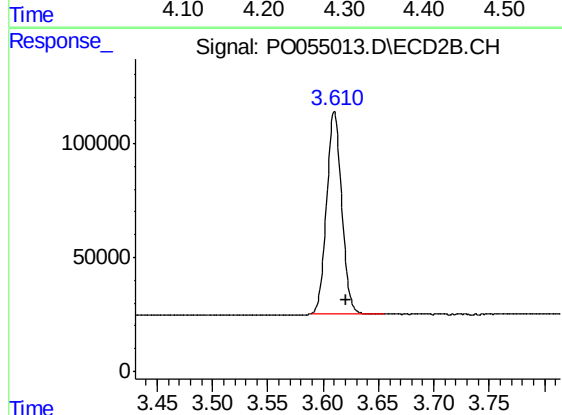


#1 Tetrachloro-m-xylene

R.T.: 3.610 min
Delta R.T.: -0.011 min
Response: 843716
Conc: 26.44 ng/ml

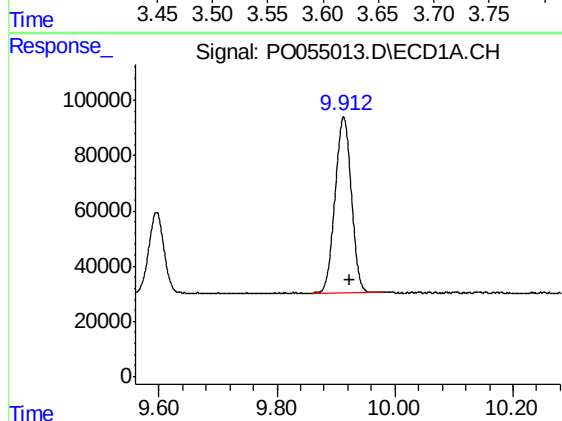


#2 Decachlorobiphenyl

R.T.: 9.913 min
Delta R.T.: -0.010 min
Response: 1220082
Conc: 24.75 ng/ml

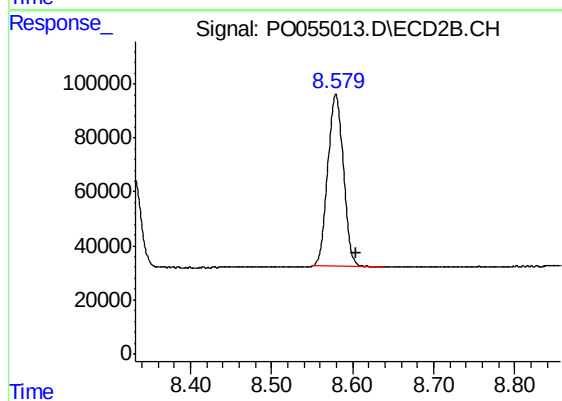

#2 Decachlorobiphenyl

R.T.: 8.579 min
Delta R.T.: -0.025 min
Response: 856992
Conc: 26.91 ng/ml

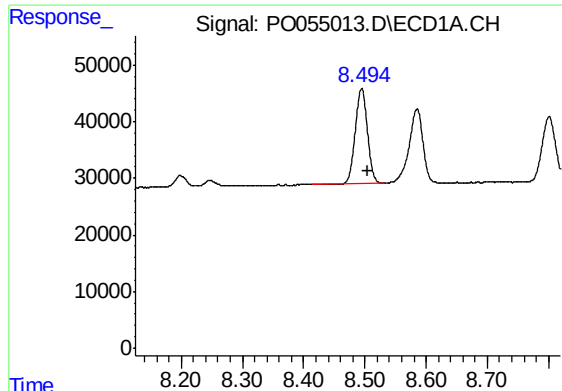


#41 AR-1268-1

R.T.: 8.495 min
Delta R.T.: -0.009 min
Response: 233736
Conc: 32.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:29 PM

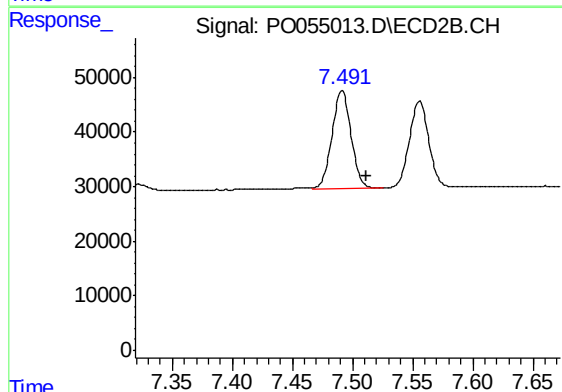


#41 AR-1268-1

R.T.: 7.491 min
Delta R.T.: -0.020 min
Response: 197769
Conc: 34.98 ng/ml

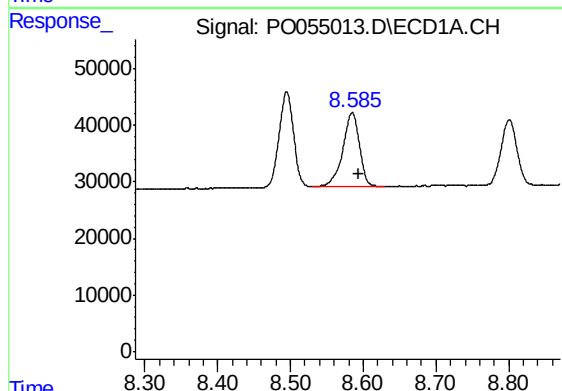


#42 AR-1268-2

R.T.: 8.585 min
Delta R.T.: -0.009 min
Response: 209736
Conc: 32.01 ng/ml

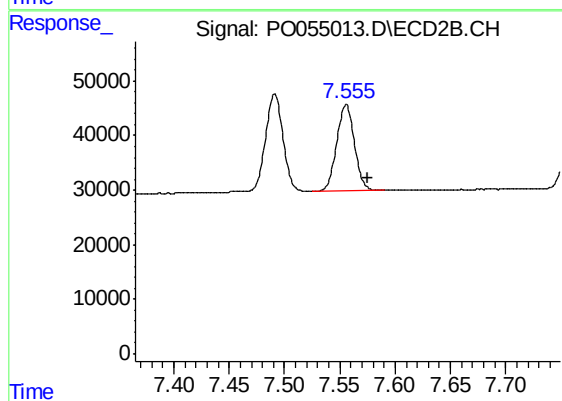

#42 AR-1268-2

R.T.: 7.556 min
Delta R.T.: -0.019 min
Response: 177191
Conc: 34.26 ng/ml

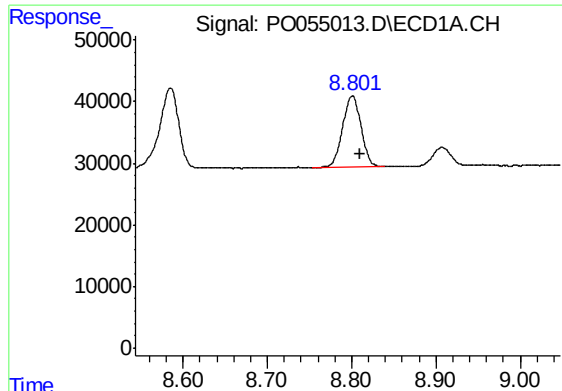


#43 AR-1268-3

R.T.: 8.801 min
Delta R.T.: -0.009 min
Response: 175291
Conc: 32.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:29 PM

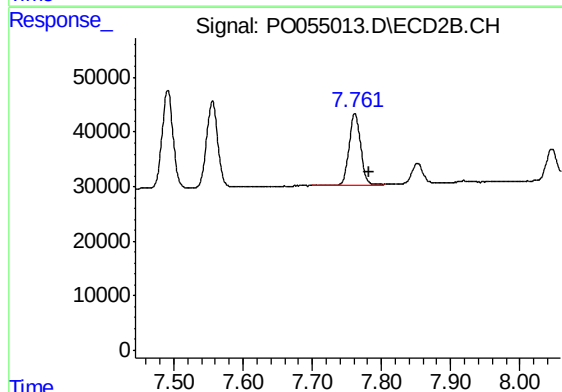


#43 AR-1268-3

R.T.: 7.762 min
Delta R.T.: -0.021 min
Response: 152472
Conc: 35.43 ng/ml

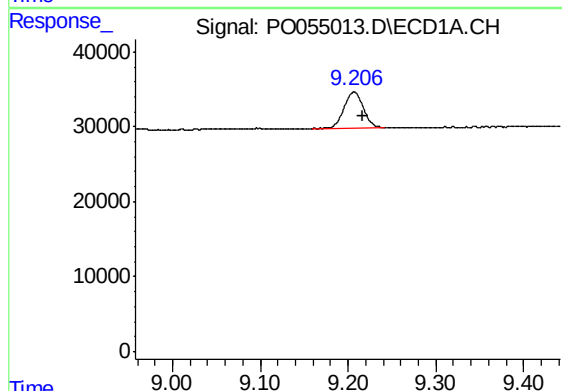


#44 AR-1268-4

R.T.: 9.207 min
Delta R.T.: -0.010 min
Response: 74844
Conc: 31.37 ng/ml

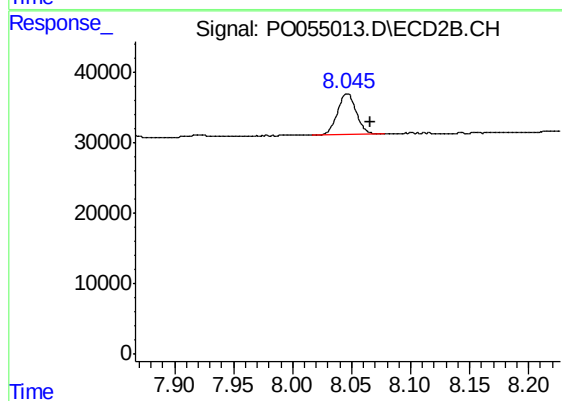

#44 AR-1268-4

R.T.: 8.046 min
Delta R.T.: -0.020 min
Response: 65009
Conc: 35.07 ng/ml

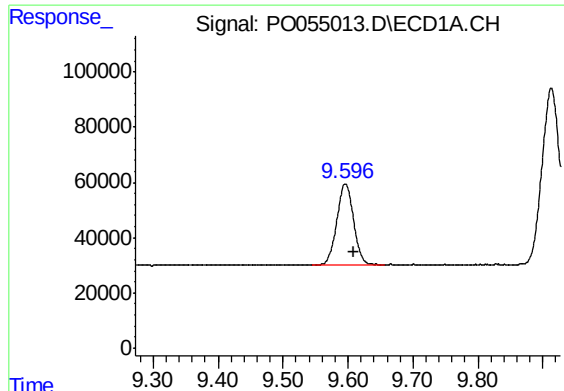


#45 AR-1268-5

R.T.: 9.596 min
Delta R.T.: -0.012 min
Response: 521191
Conc: 31.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:29 PM

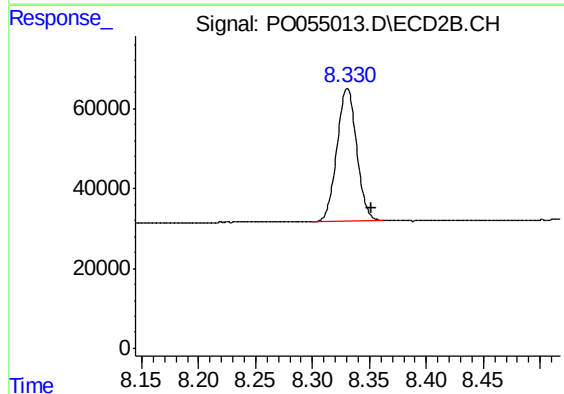

#45 AR-1268-5

R.T.: 8.330 min
Delta R.T.: -0.022 min
Response: 402058
Conc: 35.32 ng/ml m