

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040519\
 Data File : P0055014.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Apr 2019 3:27
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1268 LOQ 40PPB
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Manual Integrations
 APPROVED

Sohil
 4/8/2019 5:25:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 05:17:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.297	3.610	842938	764691	24.289	23.962m
2) SA Decachlor...	9.911	8.579	1156265	812647	23.455	25.516
Target Compounds						
41) L9 AR-1268-1	8.495	7.491	342822	285657	48.166	50.522
42) L9 AR-1268-2	8.584	7.555	303714	255705	46.354	49.444
43) L9 AR-1268-3	8.799	7.762	255510	219057	46.905	50.902
44) L9 AR-1268-4	9.206	8.045	110933	92759	46.498	50.036
45) L9 AR-1268-5	9.595	8.329	752866	573385	45.697	50.373m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040519\
Data File : PO055014.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Apr 2019 3:27
Operator : SM/SJ
Sample : K1560-07
Misc : AR1268 LOQ 40PPB
ALS Vial : 52 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 05:17:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

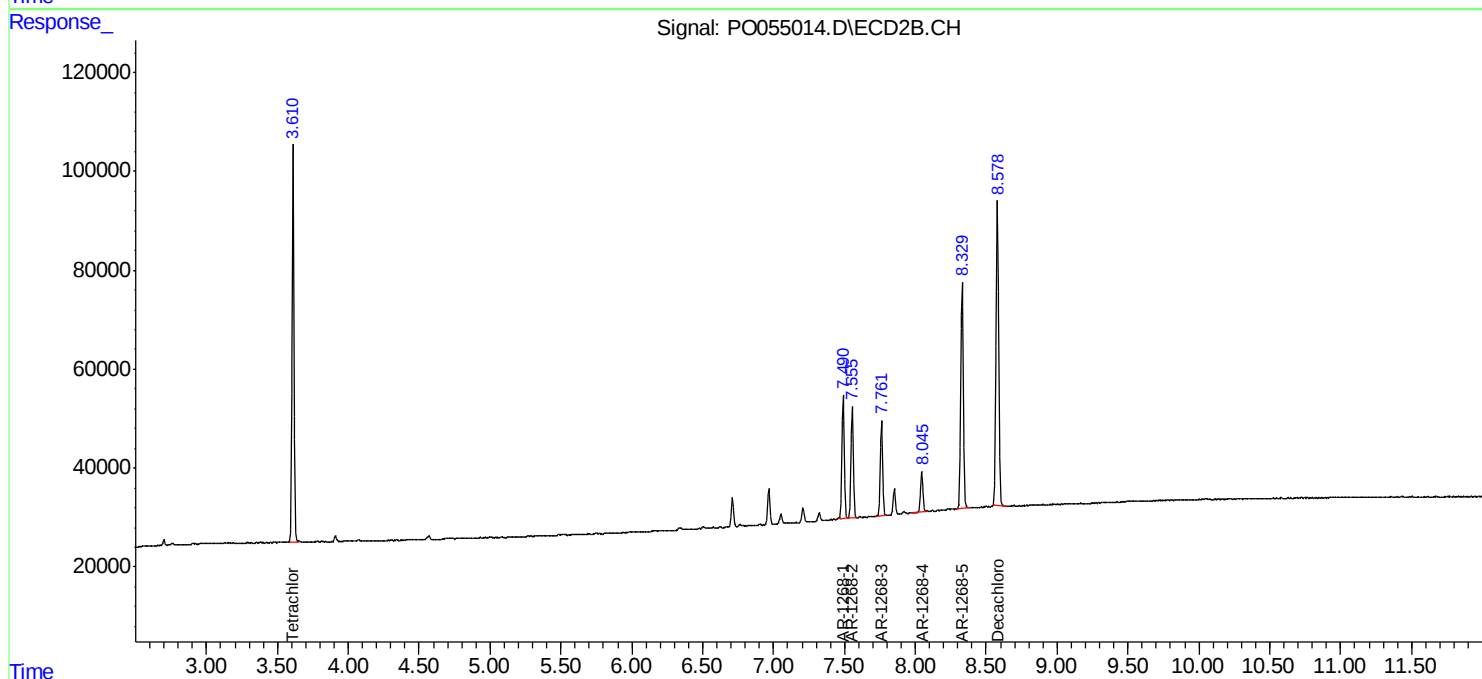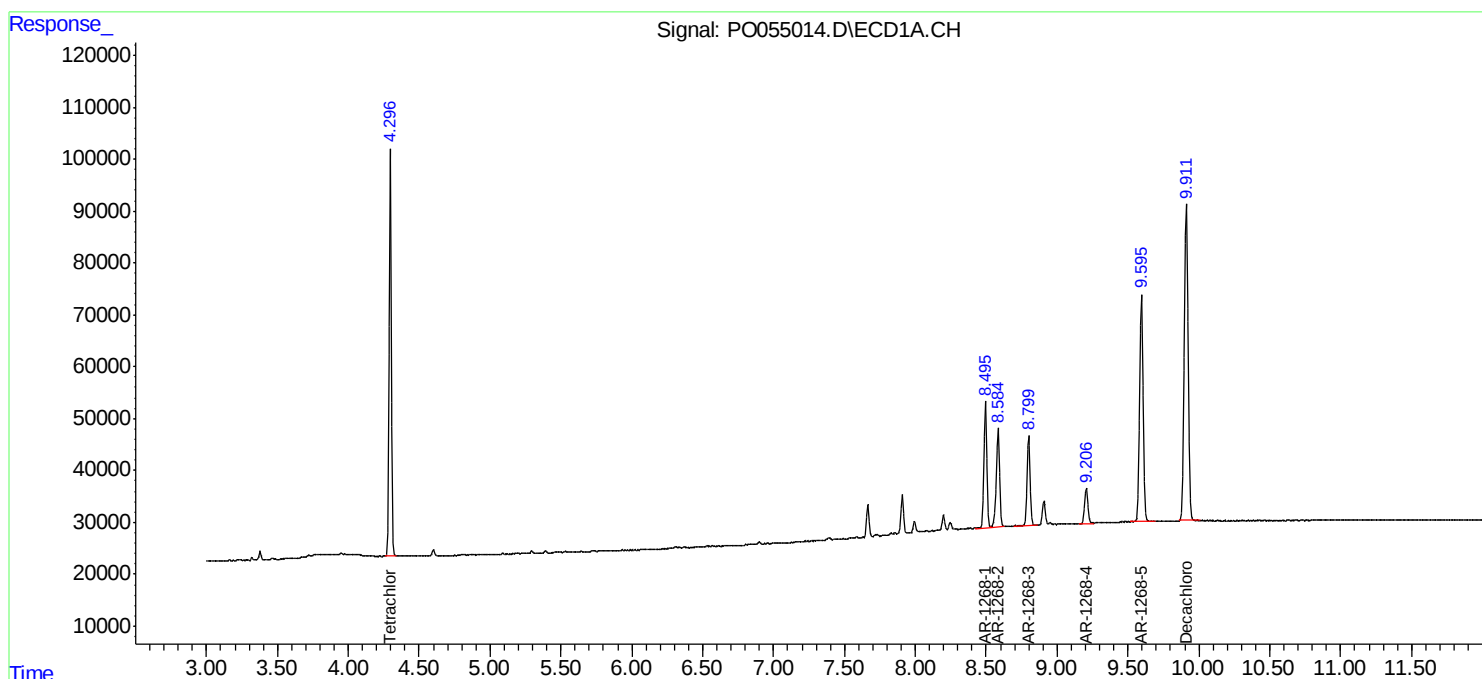

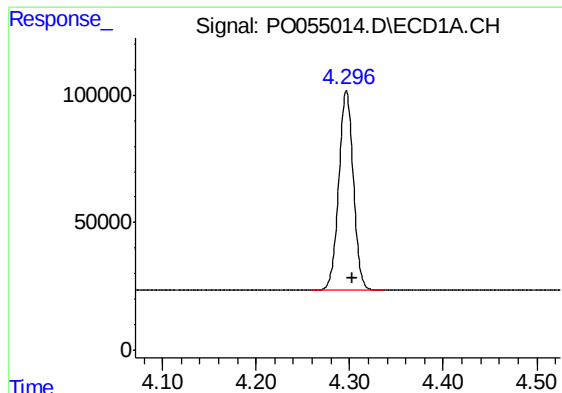


#1 Tetrachloro-m-xylene

R.T.: 4.297 min
Delta R.T.: -0.006 min
Response: 842938
Conc: 24.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:30 PM

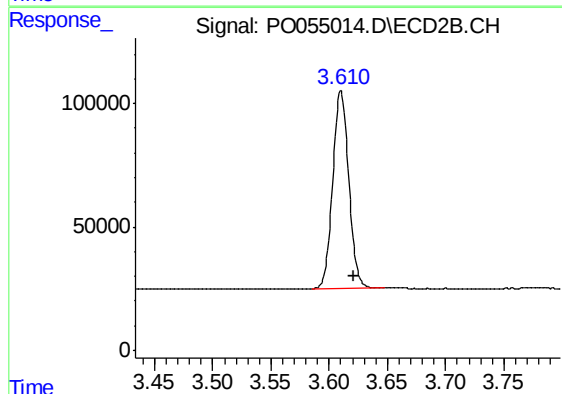


#1 Tetrachloro-m-xylene

R.T.: 3.610 min
Delta R.T.: -0.011 min
Response: 764691
Conc: 23.96 ng/ml m

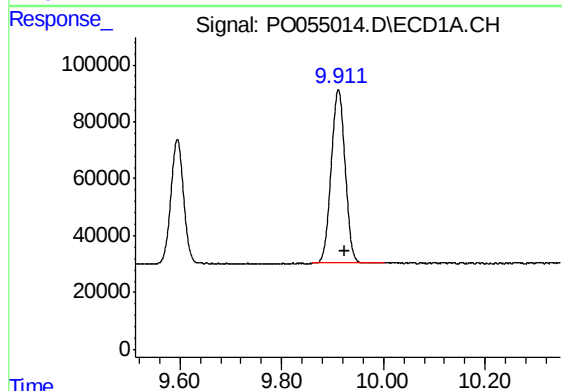


#2 Decachlorobiphenyl

R.T.: 9.911 min
Delta R.T.: -0.012 min
Response: 1156265
Conc: 23.45 ng/ml

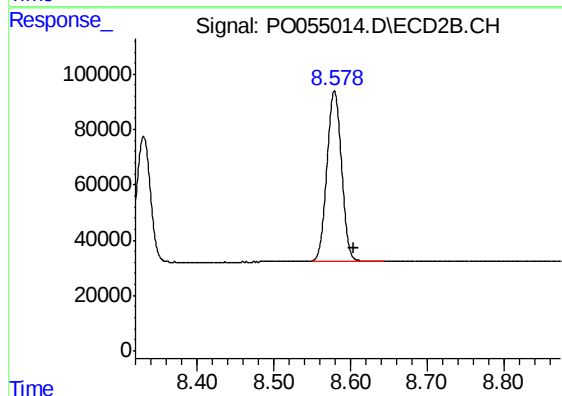

#2 Decachlorobiphenyl

R.T.: 8.579 min
Delta R.T.: -0.025 min
Response: 812647
Conc: 25.52 ng/ml

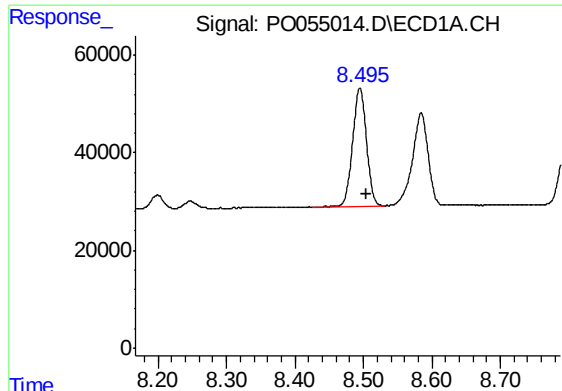


#41 AR-1268-1

R.T.: 8.495 min
Delta R.T.: -0.009 min
Response: 342822
Conc: 48.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:30 PM

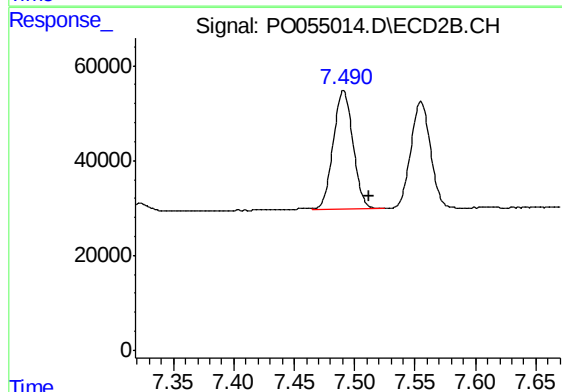


#41 AR-1268-1

R.T.: 7.491 min
Delta R.T.: -0.021 min
Response: 285657
Conc: 50.52 ng/ml

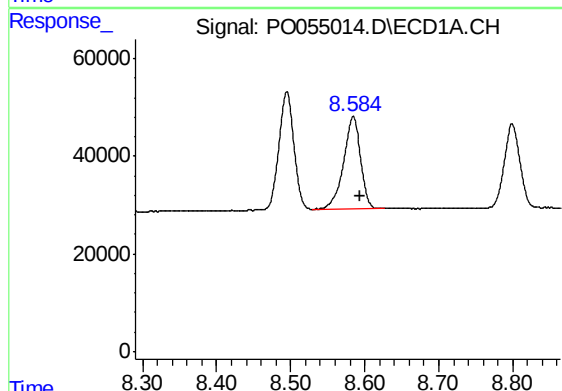


#42 AR-1268-2

R.T.: 8.584 min
Delta R.T.: -0.010 min
Response: 303714
Conc: 46.35 ng/ml

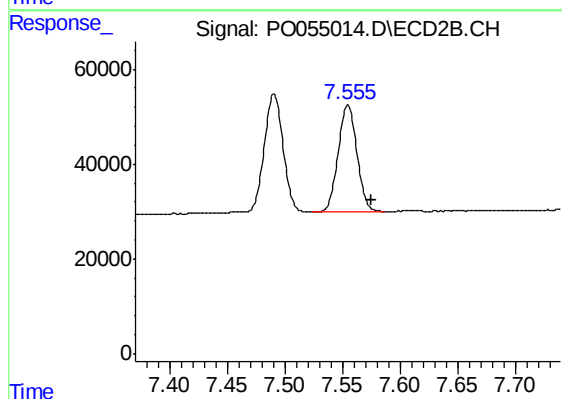

#42 AR-1268-2

R.T.: 7.555 min
Delta R.T.: -0.020 min
Response: 255705
Conc: 49.44 ng/ml

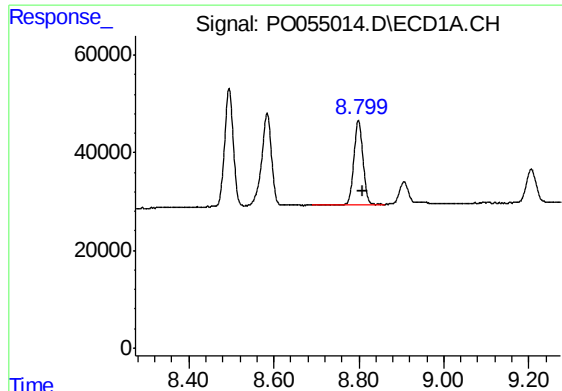


#43 AR-1268-3

R.T.: 8.799 min
Delta R.T.: -0.011 min
Response: 255510
Conc: 46.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:30 PM

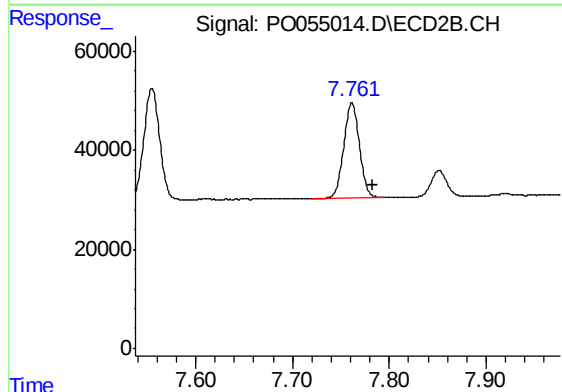


#43 AR-1268-3

R.T.: 7.762 min
Delta R.T.: -0.021 min
Response: 219057
Conc: 50.90 ng/ml

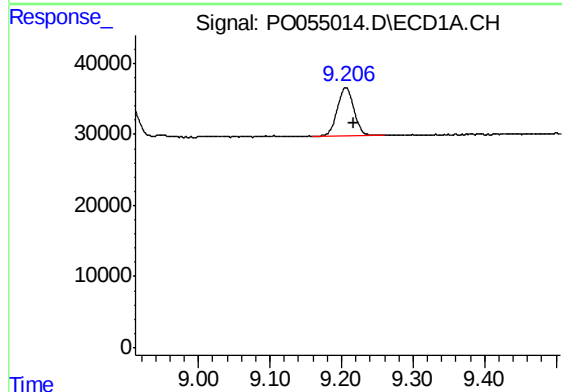


#44 AR-1268-4

R.T.: 9.206 min
Delta R.T.: -0.011 min
Response: 110933
Conc: 46.50 ng/ml

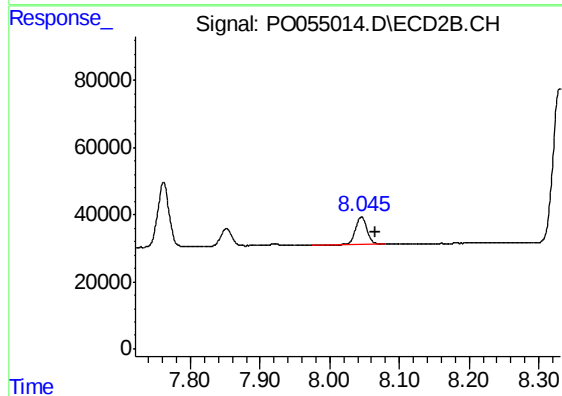

#44 AR-1268-4

R.T.: 8.045 min
Delta R.T.: -0.020 min
Response: 92759
Conc: 50.04 ng/ml

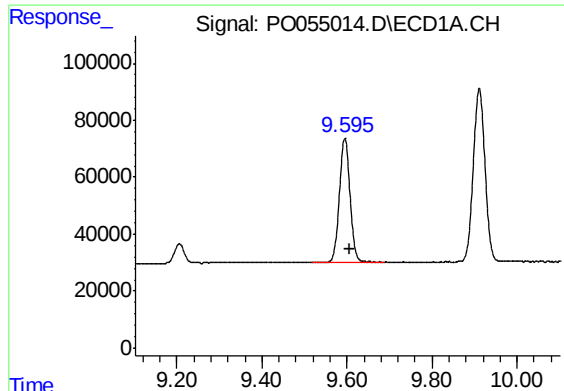


#45 AR-1268-5

R.T.: 9.595 min
Delta R.T.: -0.013 min
Response: 752866
Conc: 45.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Manual Integrations
APPROVED

Sohil
4/8/2019 5:25:30 PM

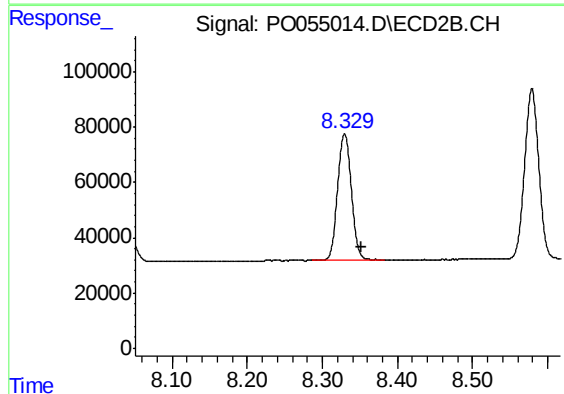

#45 AR-1268-5

R.T.: 8.329 min
Delta R.T.: -0.023 min
Response: 573385
Conc: 50.37 ng/ml m