

Data Path : P:\HPCHEM1\ECD_0\Data\P0040618\
Data File : P0043662.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Apr 2018 10:43
Operator : SM/UA
Sample : J2265-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PF-7

Manual Integrations
APPROVED

ugo
4/9/2018 1:02:14 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 11:16:13 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0040418.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 04 15:17:57 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.067	3.325	3692519	4950807	20.770	18.426
2) SA Decachlor...	9.406	8.084	2187833	2853532	12.141m	12.172

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0040618\
Data File : P0043662.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Apr 2018 10:43
Operator : SM/UA
Sample : J2265-06
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
PF-7


Manual Integrations
APPROVED

ugo
4/9/2018 1:02:14 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 11:16:13 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0040418.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 04 15:17:57 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

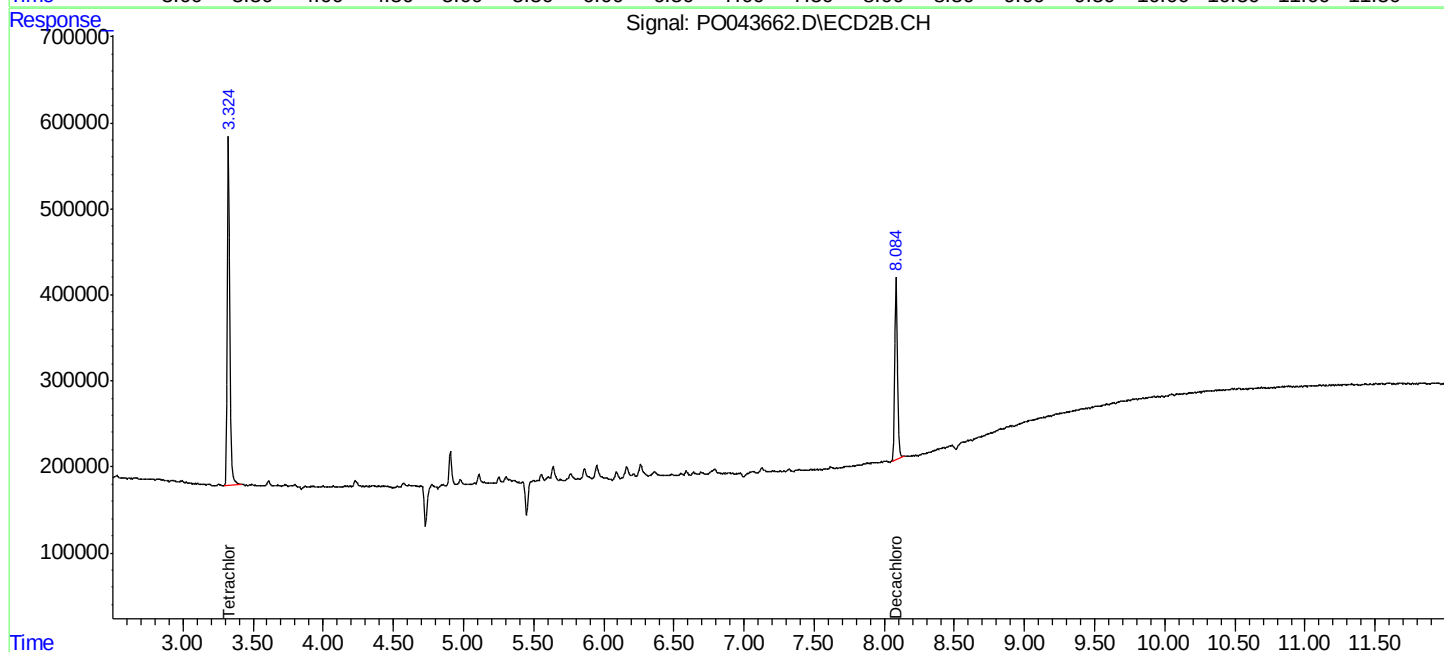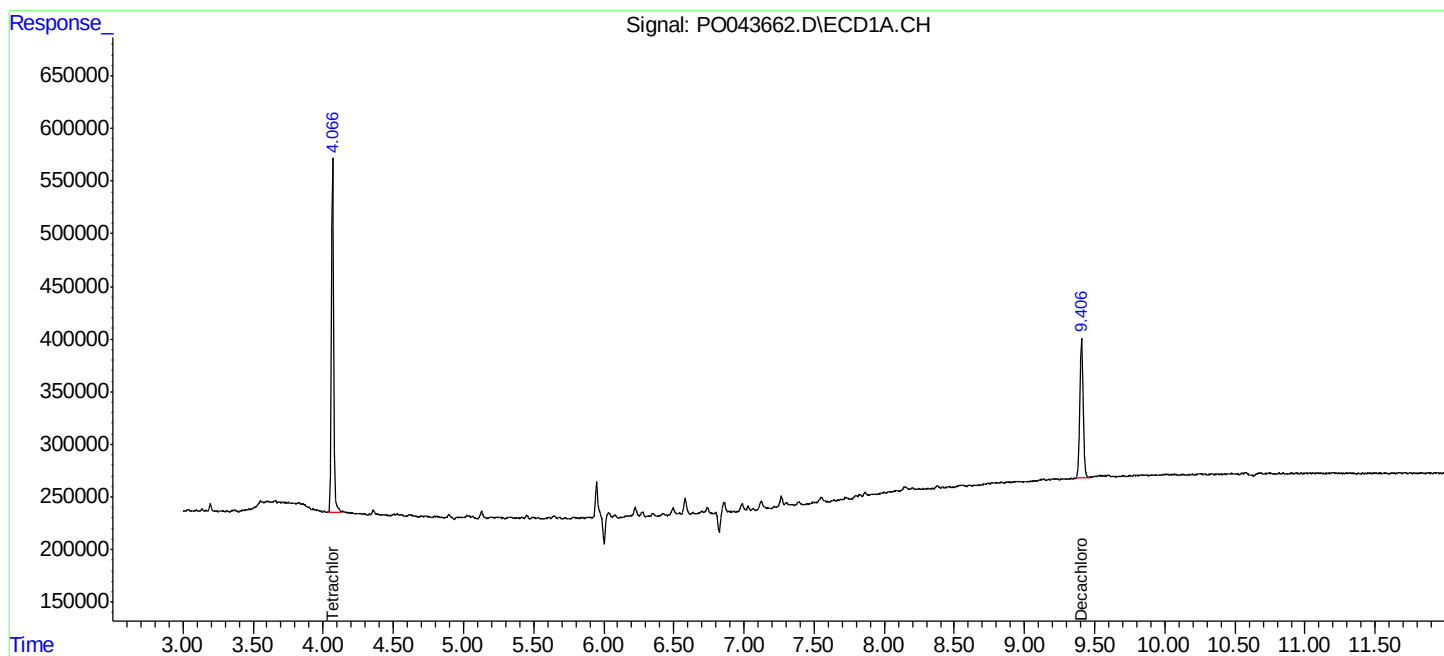

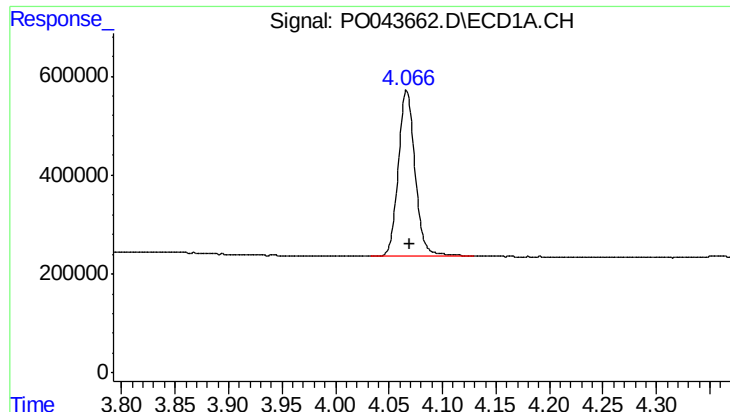


#1 Tetrachloro-m-xylene

R.T.: 4.067 min
Delta R.T.: -0.003 min
Response: 3692519
Conc: 20.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
PF-7


Manual Integrations
APPROVED

ugo
4/9/2018 1:02:14 PM

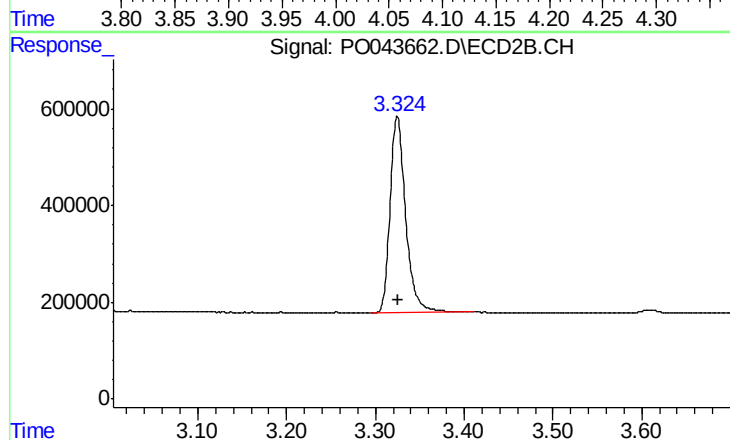


#1 Tetrachloro-m-xylene

R.T.: 3.325 min
Delta R.T.: -0.002 min
Response: 4950807
Conc: 18.43 ng/ml

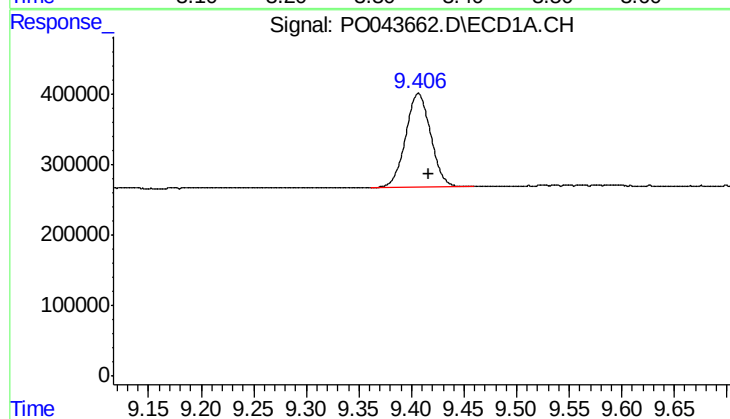

#2 Decachlorobiphenyl

R.T.: 9.406 min
Delta R.T.: -0.011 min
Response: 2187833
Conc: 12.14 ng/ml m

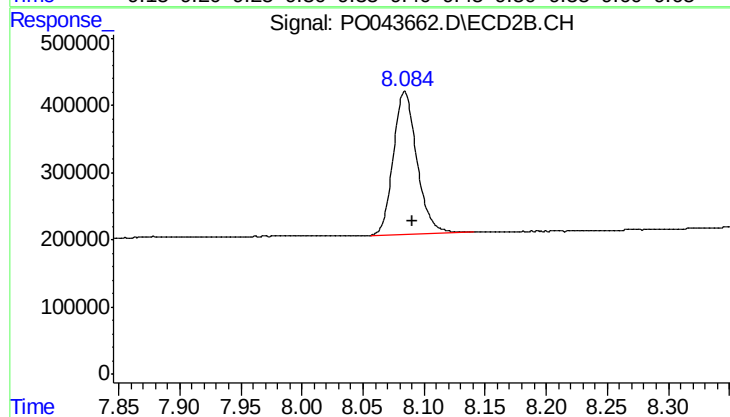

#2 Decachlorobiphenyl

R.T.: 8.084 min
Delta R.T.: -0.006 min
Response: 2853532
Conc: 12.17 ng/ml