

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040620\
 Data File : P0067678.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Apr 2020 9:58
 Operator : DD\AJ
 Sample : L2108-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-70-71-COMP

Manual Integrations
 APPROVED

Sohil
 4/7/2020 1:34:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 12:36:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.933	3.942	565083	809934	23.729	24.165
2) SA Decachlor...	10.911	9.226	720296	831019	21.158m	20.099m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040620\
Data File : P0067678.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Apr 2020 9:58
Operator : DD\AJ
Sample : L2108-05
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-70-71-COMP


Manual Integrations
APPROVED

Sohil
4/7/2020 1:34:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 12:36:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

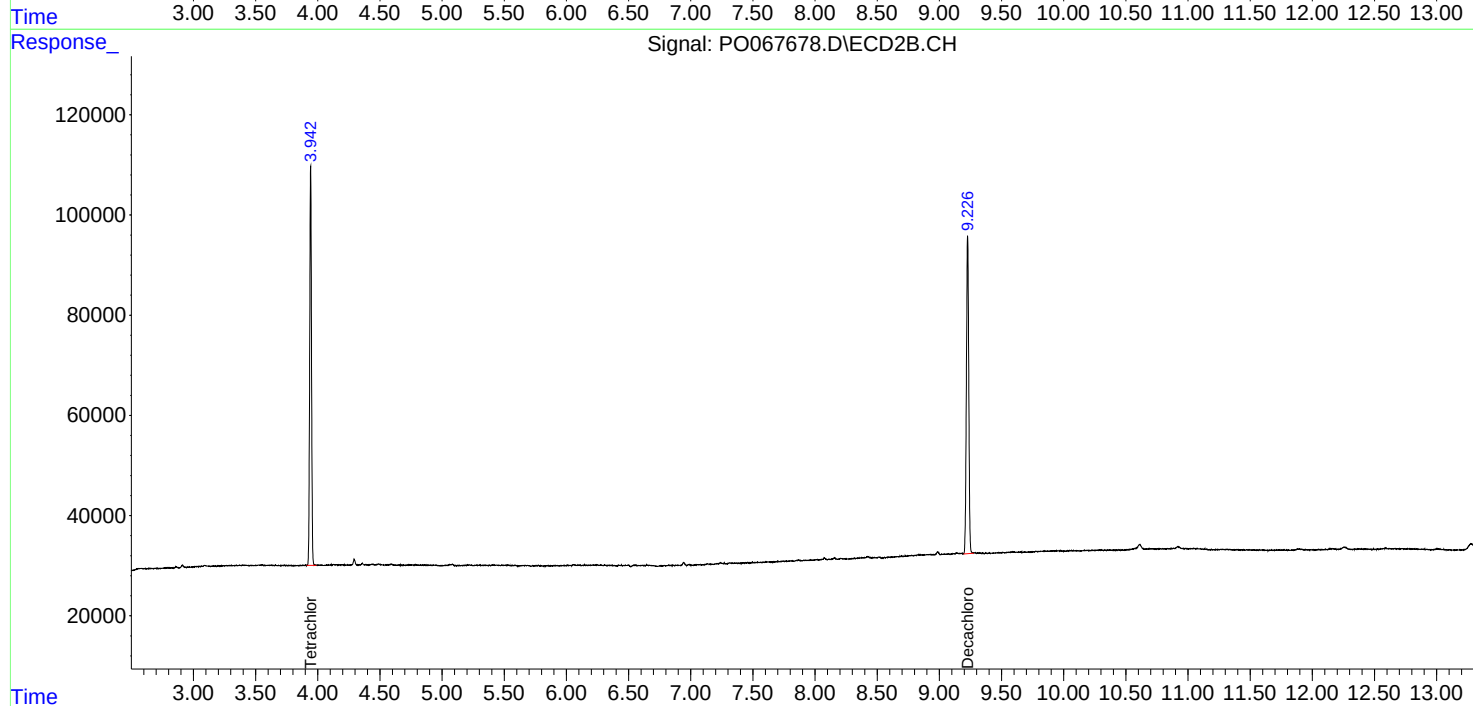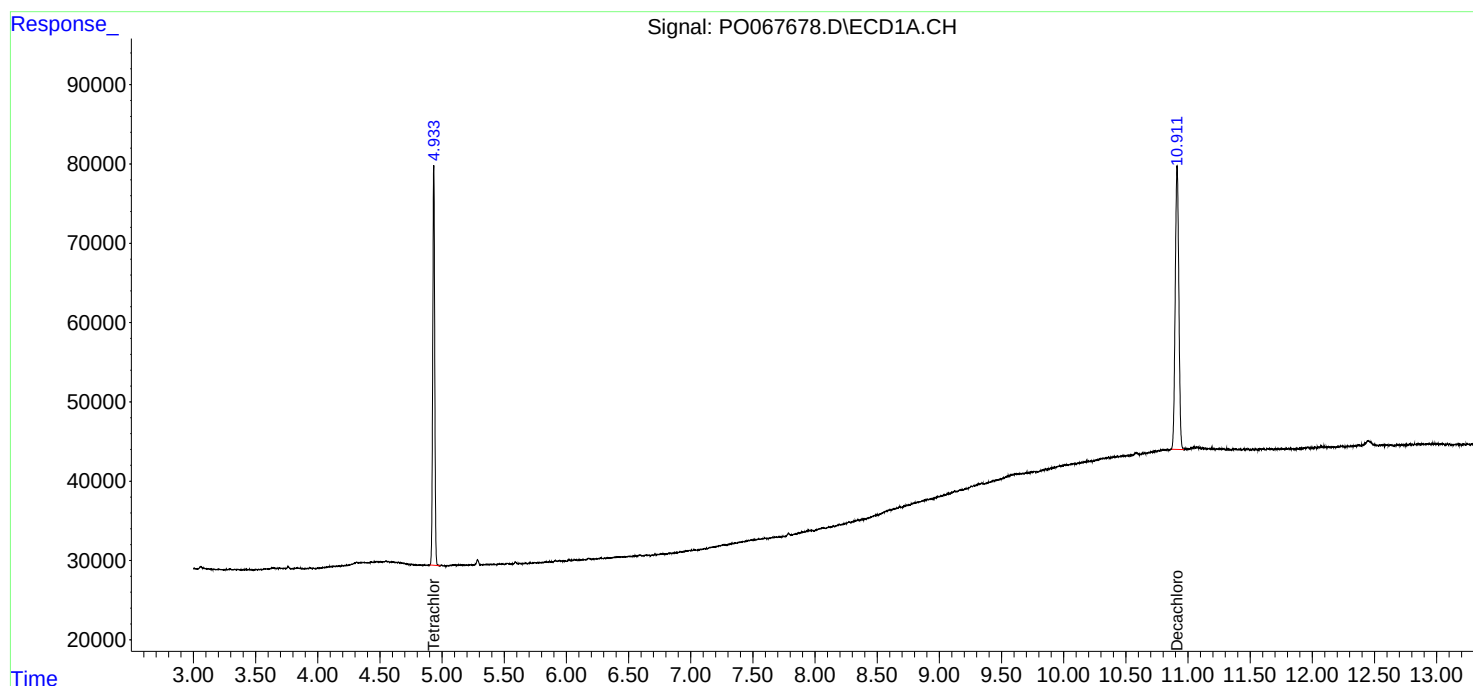

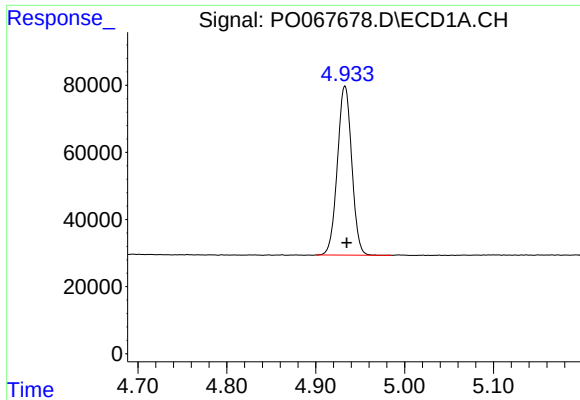


#1 Tetrachloro-m-xylene

R.T.: 4.933 min
Delta R.T.: -0.002 min
Response: 565083
Conc: 23.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-70-71-COMP


Manual Integrations
APPROVED

Sohil
4/7/2020 1:34:29 PM

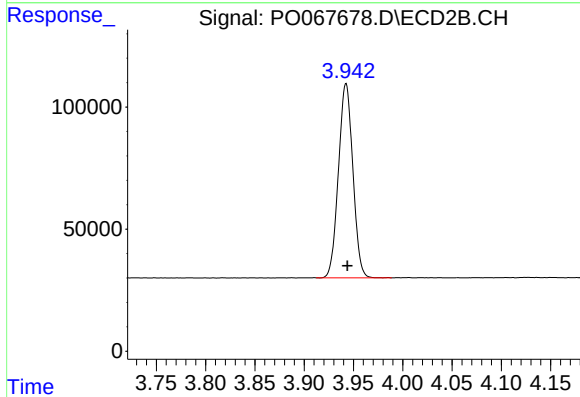


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: -0.001 min
Response: 809934
Conc: 24.16 ng/ml

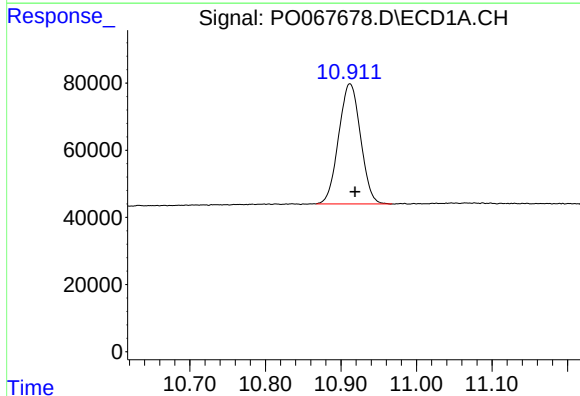

#2 Decachlorobiphenyl

R.T.: 10.911 min
Delta R.T.: -0.007 min
Response: 720296
Conc: 21.16 ng/ml m

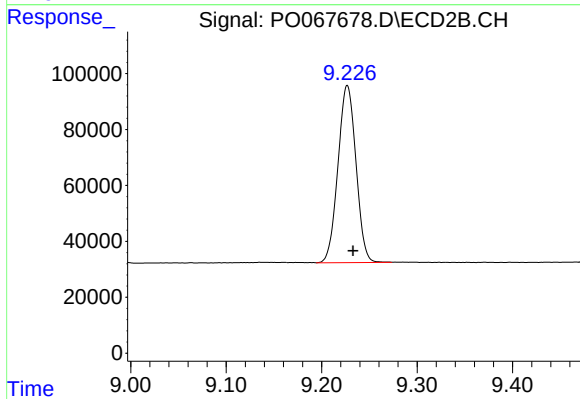

#2 Decachlorobiphenyl

R.T.: 9.226 min
Delta R.T.: -0.007 min
Response: 831019
Conc: 20.10 ng/ml m