

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040620\
 Data File : P0067686.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Apr 2020 12:15
 Operator : DD\AJ
 Sample : L2148-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-GF-02-055-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 13:42:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.933	3.942	635775	911840	26.697	27.205
2) SA Decachlor...	10.911	9.226	752456	821848	22.103	19.877

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040620\
Data File : P0067686.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Apr 2020 12:15
Operator : DD\AJ
Sample : L2148-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-055-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 13:42:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

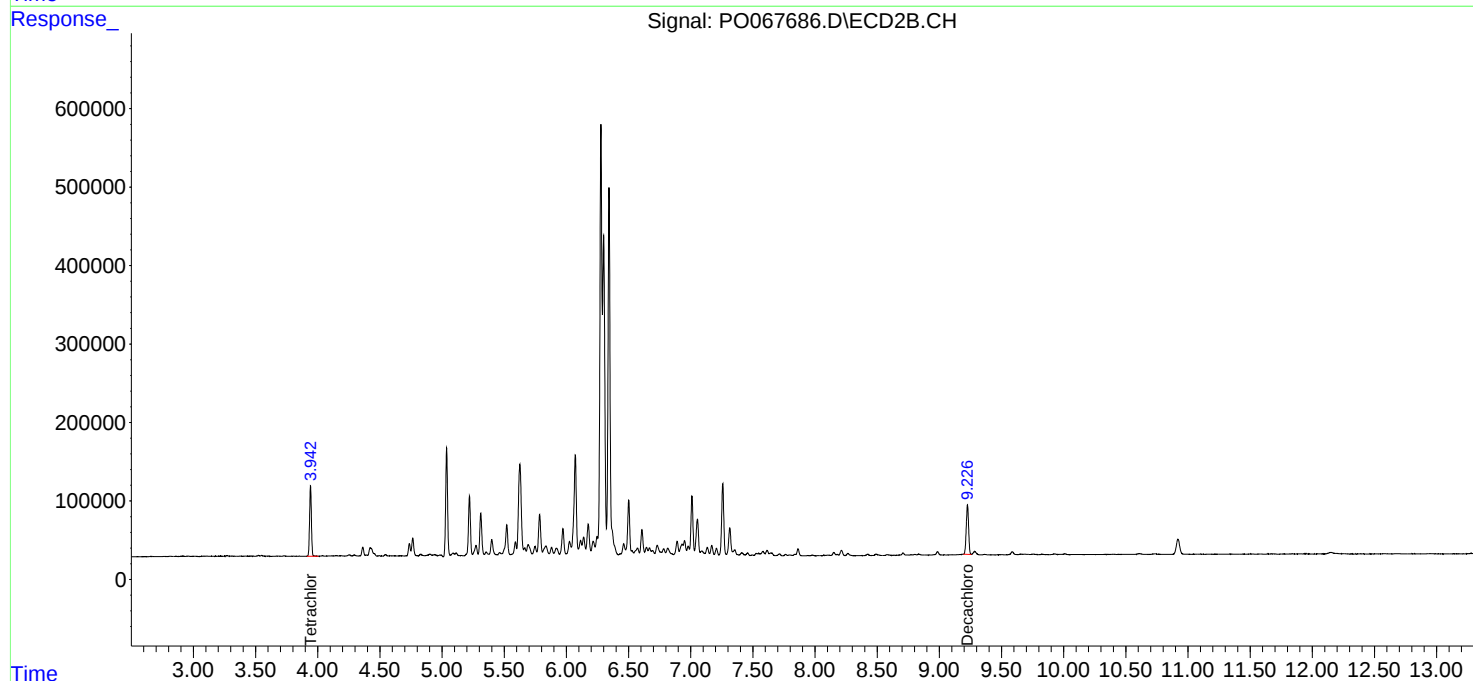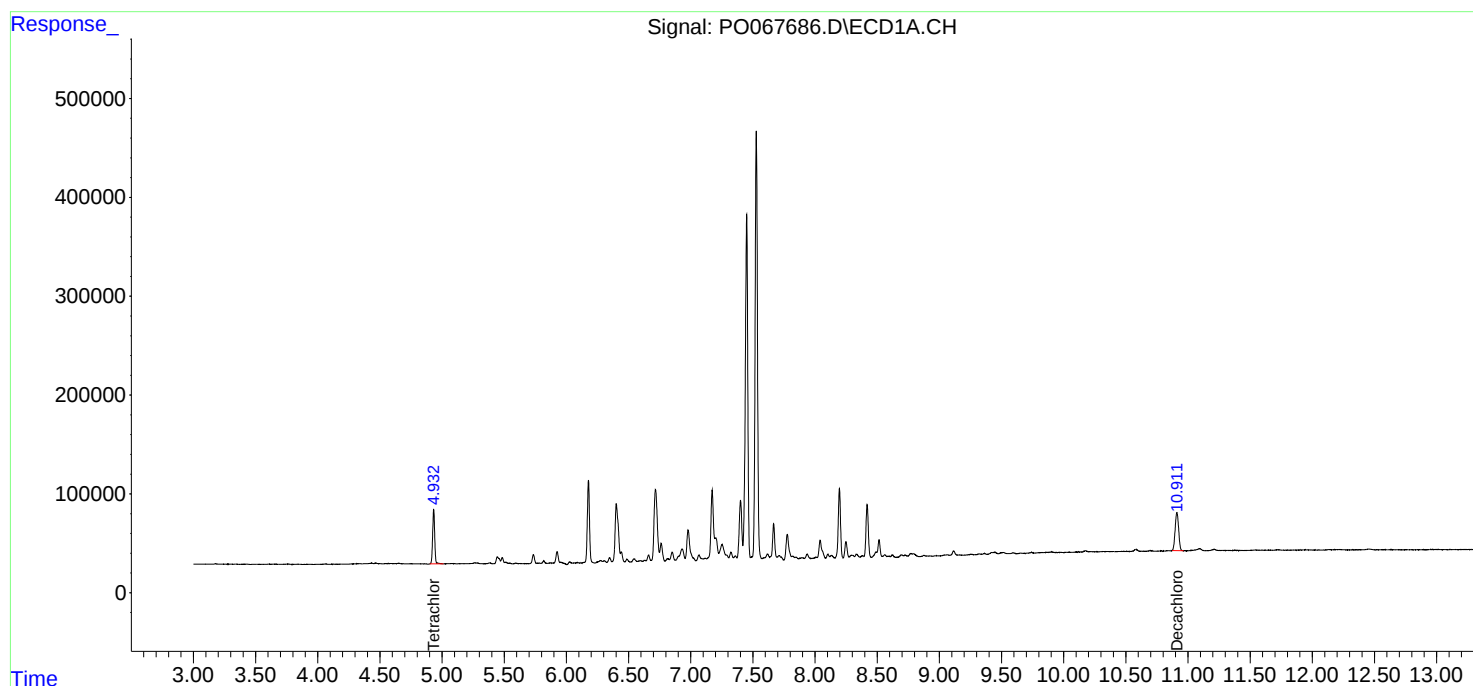


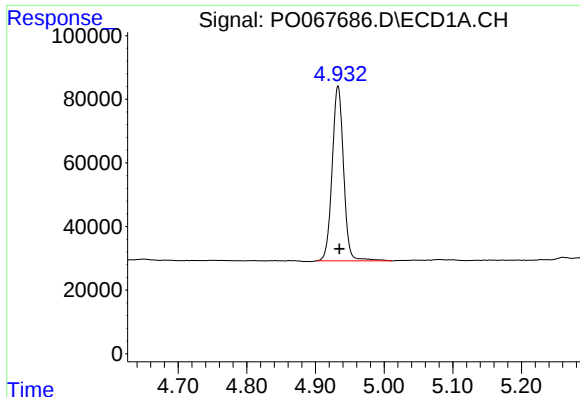

#1 Tetrachloro-m-xylene


R.T.: 4.933 min
Delta R.T.: -0.002 min
Response: 635775
Conc: 26.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-055-A

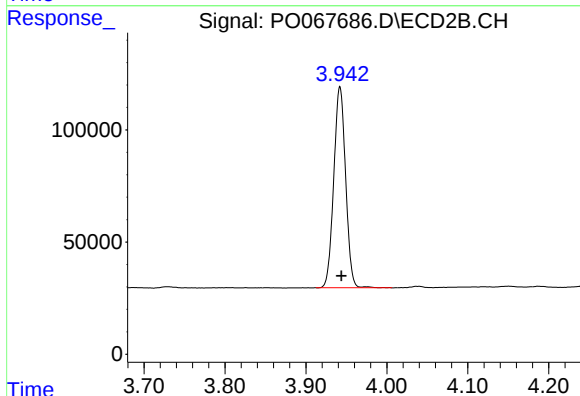


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: -0.002 min
Response: 911840
Conc: 27.21 ng/ml

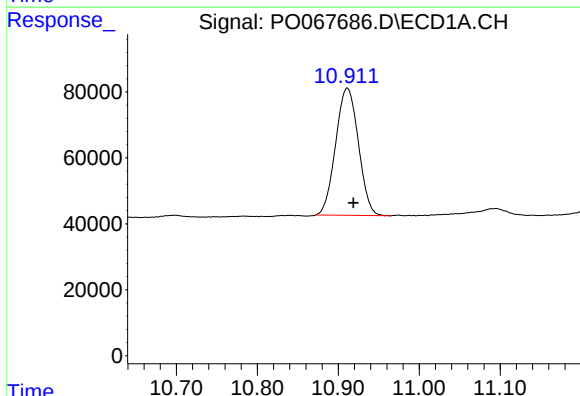

#2 Decachlorobiphenyl

R.T.: 10.911 min
Delta R.T.: -0.008 min
Response: 752456
Conc: 22.10 ng/ml

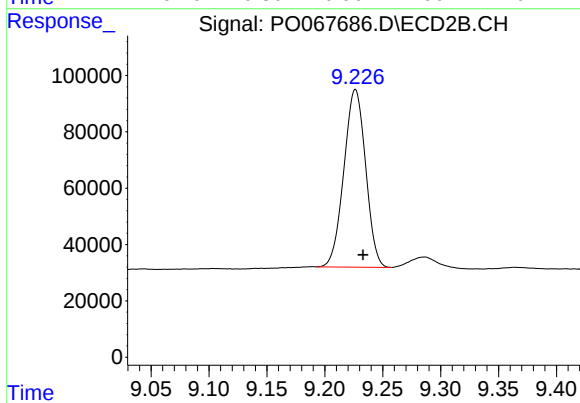

#2 Decachlorobiphenyl

R.T.: 9.226 min
Delta R.T.: -0.007 min
Response: 821848
Conc: 19.88 ng/ml