

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040620\
 Data File : P0067695.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Apr 2020 14:54
 Operator : DD\AJ
 Sample : L2110-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AU-05-040220

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 17:15:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.932	3.942	606544	889068	25.470	26.526
2)	SA Decachlor...	10.912	9.228	744272	803897	21.862	19.443

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040620\
Data File : P0067695.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Apr 2020 14:54
Operator : DD\AJ
Sample : L2110-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AU-05-040220

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 17:15:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

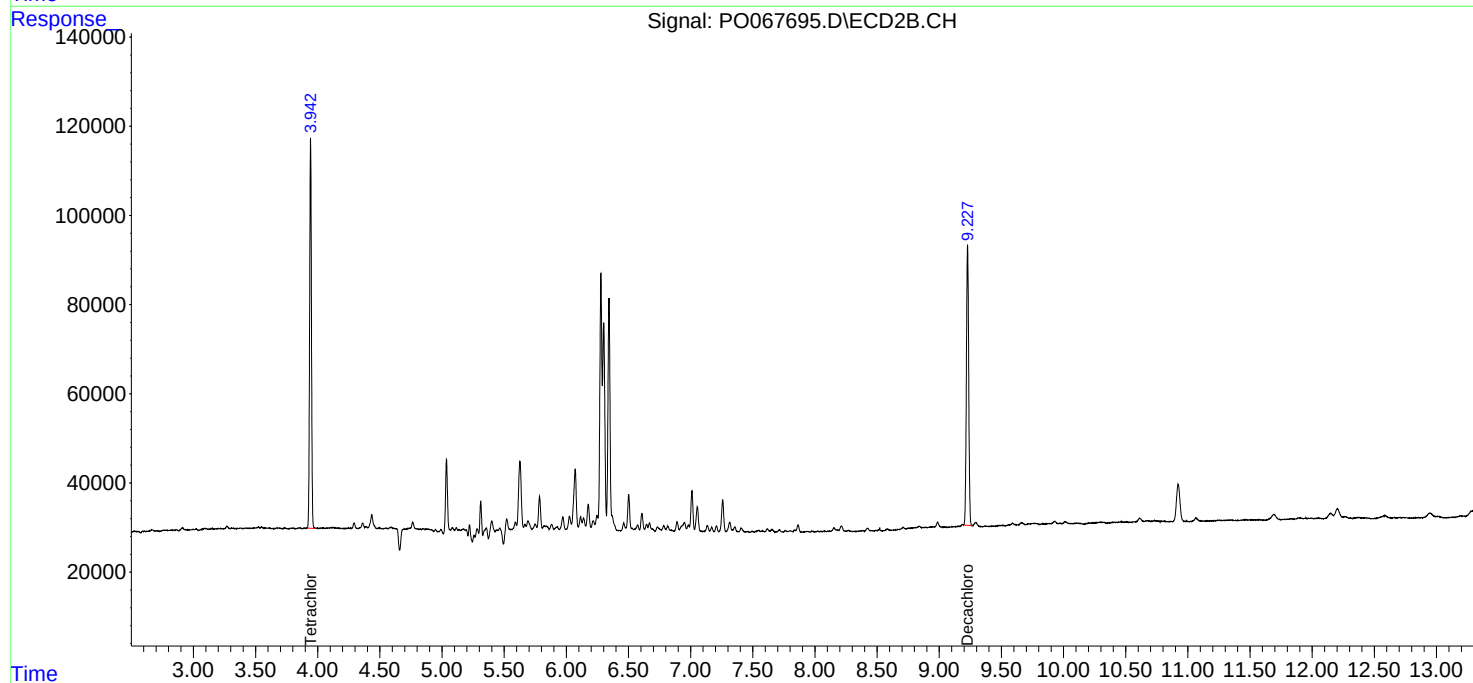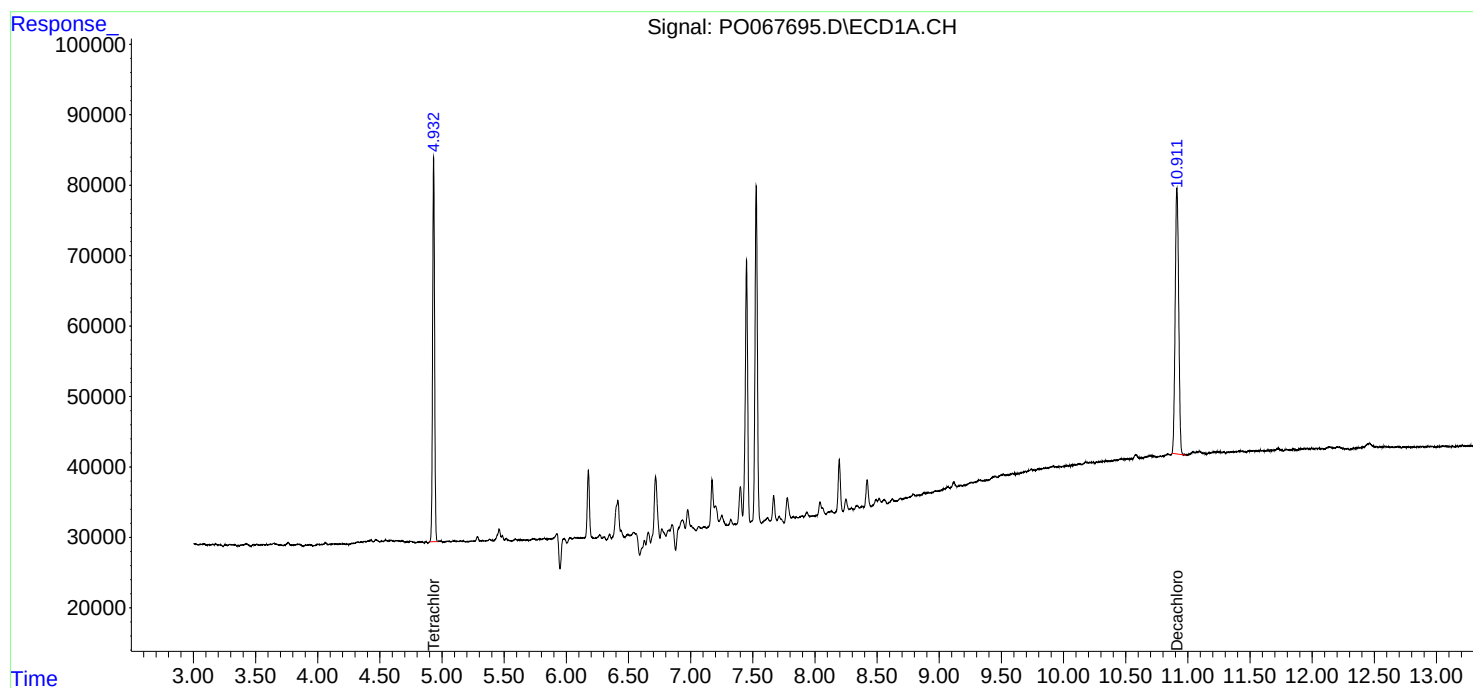


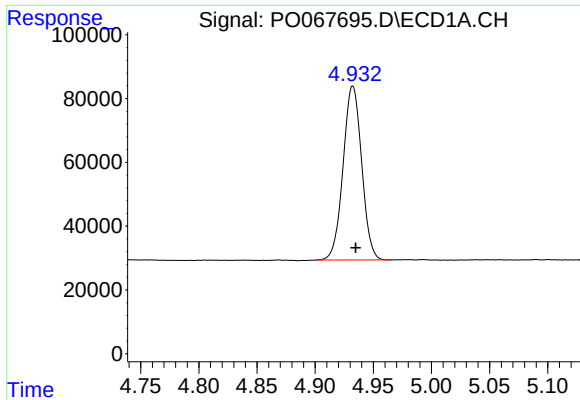

#1 Tetrachloro-m-xylene


R.T.: 4.932 min
Delta R.T.: -0.003 min
Response: 606544
Conc: 25.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
AU-05-040220

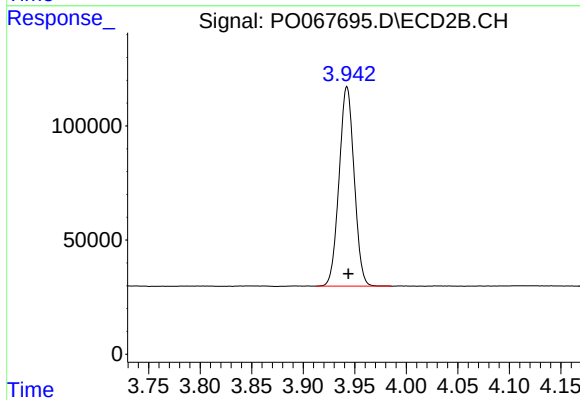


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: -0.001 min
Response: 889068
Conc: 26.53 ng/ml

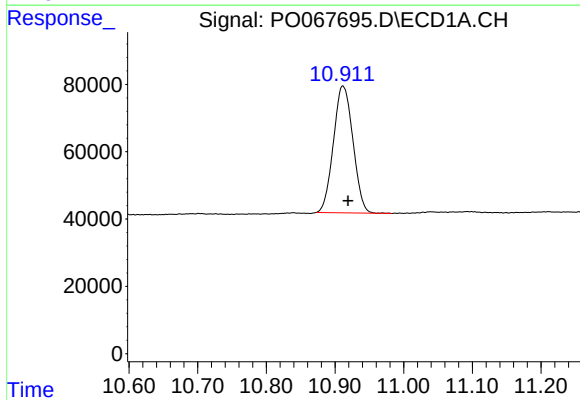

#2 Decachlorobiphenyl

R.T.: 10.912 min
Delta R.T.: -0.007 min
Response: 744272
Conc: 21.86 ng/ml

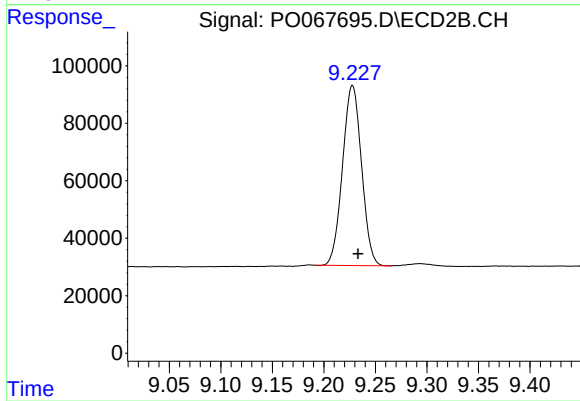

#2 Decachlorobiphenyl

R.T.: 9.228 min
Delta R.T.: -0.005 min
Response: 803897
Conc: 19.44 ng/ml