

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040720\
 Data File : P0067710.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Apr 2020 11:54
 Operator : DD\AJ
 Sample : L2166-19MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-45-COMPMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 14:48:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.932	3.942	629277	927075	26.425	27.660
2)	SA Decachlor...	10.911	9.228	745420	823089	21.896	19.907
Target Compounds							
3)	L1 AR-1016-1	6.251	5.197	258624	383923	250.791	261.899
4)	L1 AR-1016-2	6.275	5.217	356297	510597	252.525	260.645
5)	L1 AR-1016-3	6.341	5.407	215680	279348	245.374	267.097
6)	L1 AR-1016-4	6.448	5.460	172619	225263	244.789	252.515
7)	L1 AR-1016-5	6.762	5.688	170919	275949	237.704	243.854
8)	L2 AR-1221-1	0.000	4.198	0	35839	N.D.	80.653 #
9)	L2 AR-1221-2	5.282	4.298	33993	53183	146.152	168.644
10)	L2 AR-1221-3	5.369	4.387	129792	195541	172.758	199.178
11)	L3 AR-1232-1	5.369	4.387	129792	195541	252.088	282.546
12)	L3 AR-1232-2	5.957	5.217	184392	510597	687.322	703.916
13)	L3 AR-1232-3	6.275	5.407	356297	279348	679.731	724.708
14)	L3 AR-1232-4	6.448	5.504	172619	271932	671.474	768.675
15)	L3 AR-1232-5	6.546	5.688	143681	275949	767.070	722.123
16)	L4 AR-1242-1	6.251	5.197	258624	383923	376.695	391.296
17)	L4 AR-1242-2	6.275	5.217	356297	510597	379.208	391.862
18)	L4 AR-1242-3	6.341	5.407	215680	279348	368.038	390.655
19)	L4 AR-1242-4	6.448	5.504	172619	271932	367.032	377.783
20)	L4 AR-1242-5	7.230	6.067	25164	226596	47.104	242.157 #
21)	L5 AR-1248-1	6.251	5.197	258624	383923	482.047	491.445
22)	L5 AR-1248-2	6.546	5.460	143681	225263	204.212	223.865
23)	L5 AR-1248-3	6.762	5.504	170919	271932	210.009	265.863 #
24)	L5 AR-1248-4	7.190	5.688	28963	275949	30.699	221.420 #
25)	L5 AR-1248-5	7.230	6.110	25164	37941	27.923	30.660
26)	L6 AR-1254-1	7.159	6.067	135601	226596	109.789	88.371
27)	L6 AR-1254-2	7.387	6.227	147100	240751	74.796	105.562 #
28)	L6 AR-1254-3	7.769	6.665	84135	410720	40.545	112.491 #
29)	L6 AR-1254-4	8.062	6.885	60441	48383	37.108	20.070 #
30)	L6 AR-1254-5	8.489	7.313	484500	752471	282.387	225.445
31)	L7 AR-1260-1	7.935	6.783	340265	528111	251.781	251.909
32)	L7 AR-1260-2	8.199	6.981	423683	640727	250.971	249.529
33)	L7 AR-1260-3	8.562	7.135	261300	574587	200.463	238.946
34)	L7 AR-1260-4	8.793	7.618	315628	431077	205.380	205.109
35)	L7 AR-1260-5	9.115	7.864	619204	975330	196.285	192.657
36)	L8 AR-1262-1	8.562	7.313	261300	752471	155.864	543.017 #
37)	L8 AR-1262-2	9.115	7.864	619204	975330	215.790	213.323
38)	L8 AR-1262-3	9.444	8.151	413360	222466	198.650	113.188 #
39)	L8 AR-1262-4	9.496	8.213	226436	713180	143.100	208.047 #
40)	L8 AR-1262-5	10.174	8.710	180063	222958	152.715	131.164
41)	L9 AR-1268-1	9.444	8.151	413360	222466	111.865	41.346 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040720\
 Data File : P0067710.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Apr 2020 11:54
 Operator : DD\AJ
 Sample : L2166-19MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-45-COMPMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 14:48:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	9.496	8.213	226436	713180	65.331	144.441 #
43) L9	AR-1268-3	0.000	8.424	0	21029	N.D.	5.017 #
44) L9	AR-1268-4	10.174	8.710	180063	222958	129.708	115.231
45) L9	AR-1268-5	10.581	8.987	58942	73158	5.945	5.673



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO040720\
Data File : PO067710.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Apr 2020 11:54
Operator : DD\AJ
Sample : L2166-19MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
TP-45-COMPMS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 14:48:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

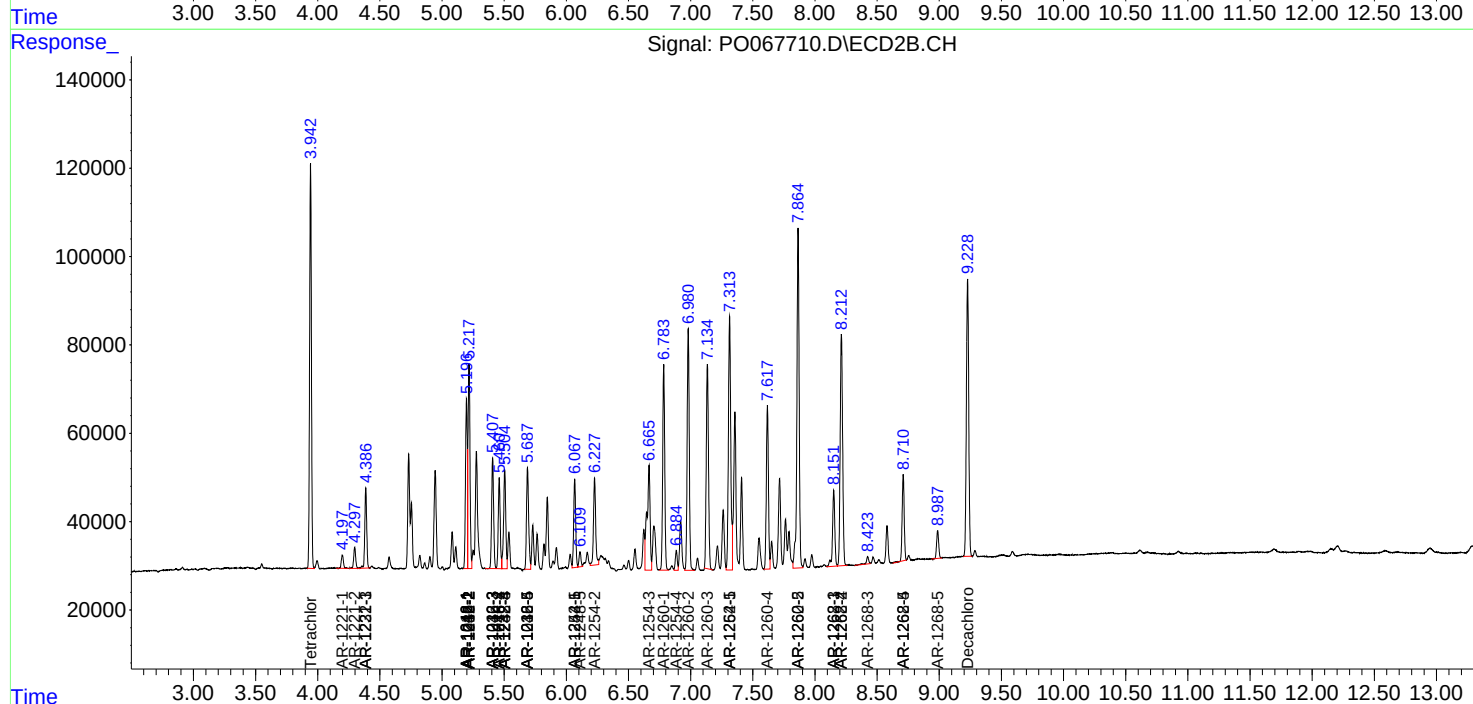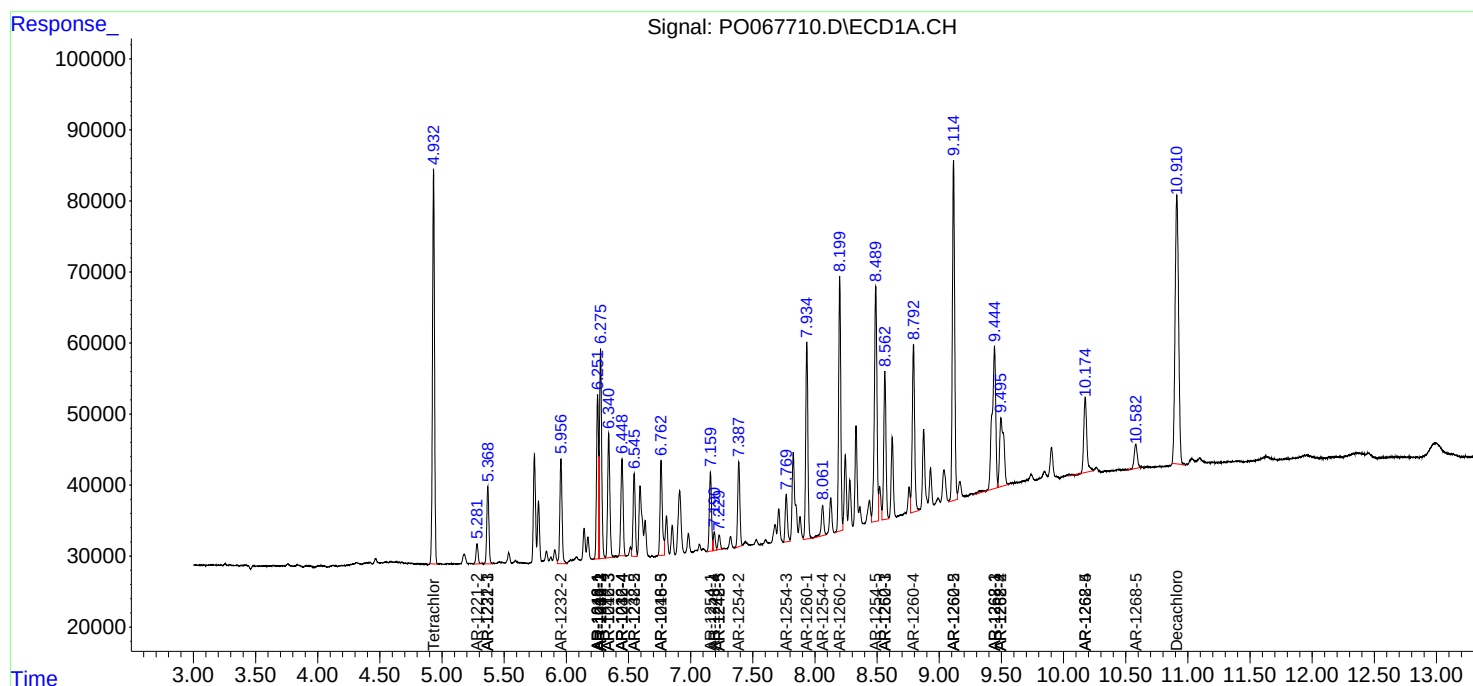


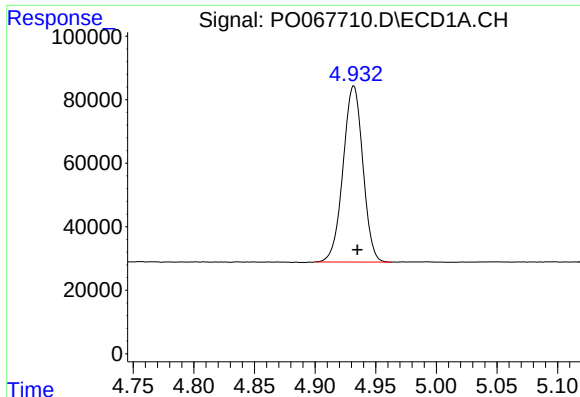

#1 Tetrachloro-m-xylene


R.T.: 4.932 min
Delta R.T.: -0.003 min
Response: 629277
Conc: 26.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

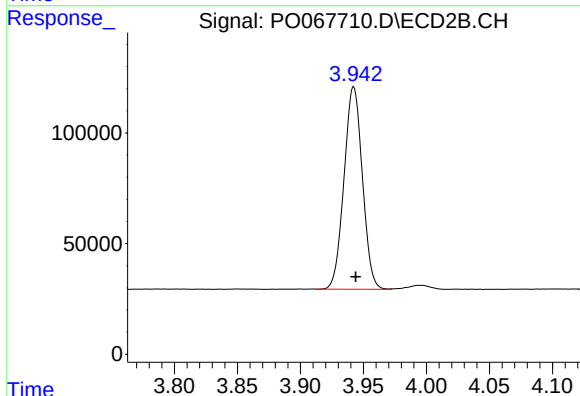


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: -0.002 min
Response: 927075
Conc: 27.66 ng/ml

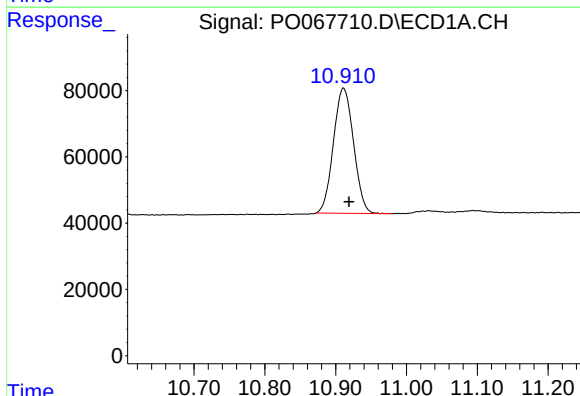


#2 Decachlorobiphenyl

R.T.: 10.911 min
Delta R.T.: -0.008 min
Response: 745420
Conc: 21.90 ng/ml

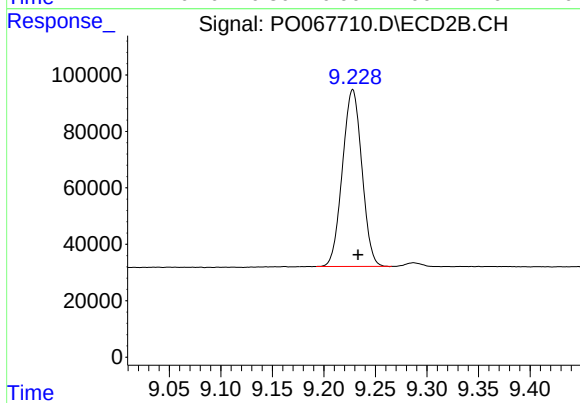

#2 Decachlorobiphenyl


R.T.: 9.228 min
Delta R.T.: -0.005 min
Response: 823089
Conc: 19.91 ng/ml

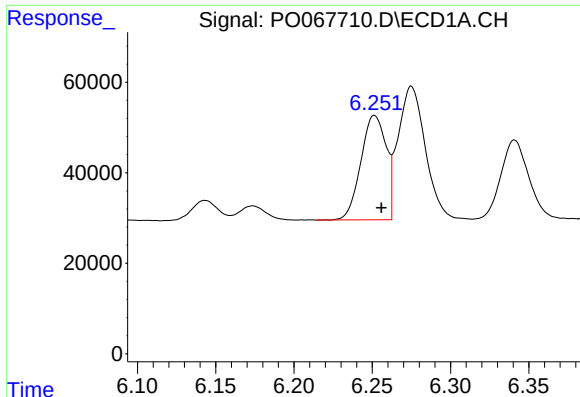

#3 AR-1016-1


R.T.: 6.251 min
Delta R.T.: -0.004 min
Response: 258624
Conc: 250.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

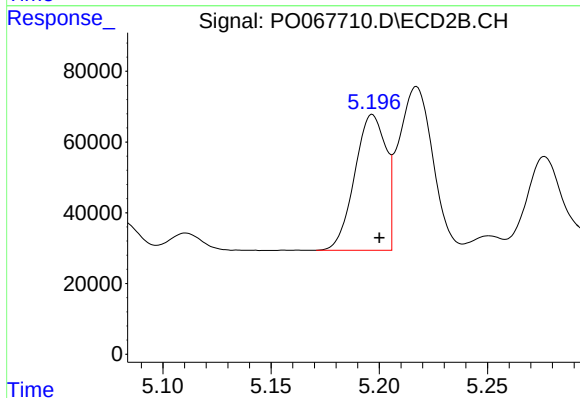


#3 AR-1016-1

R.T.: 5.197 min
Delta R.T.: -0.003 min
Response: 383923
Conc: 261.90 ng/ml

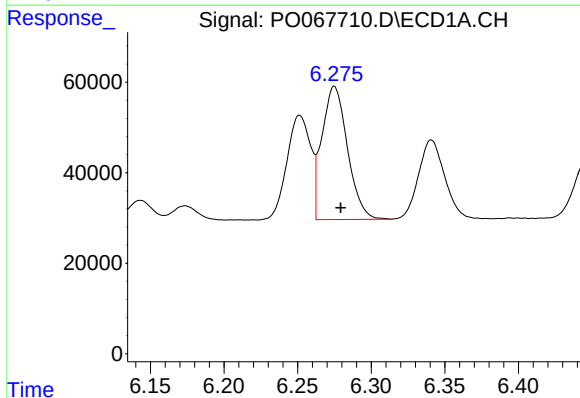


#4 AR-1016-2

R.T.: 6.275 min
Delta R.T.: -0.004 min
Response: 356297
Conc: 252.52 ng/ml

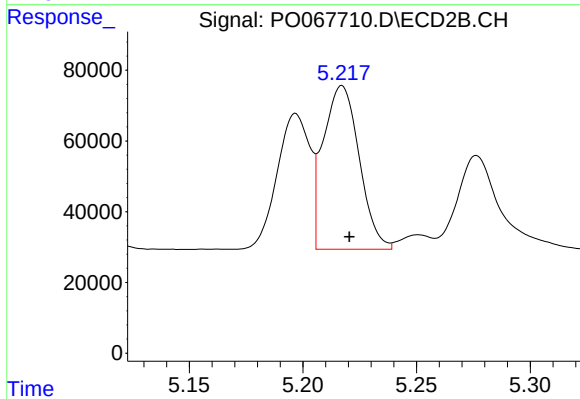

#4 AR-1016-2


R.T.: 5.217 min
Delta R.T.: -0.003 min
Response: 510597
Conc: 260.64 ng/ml

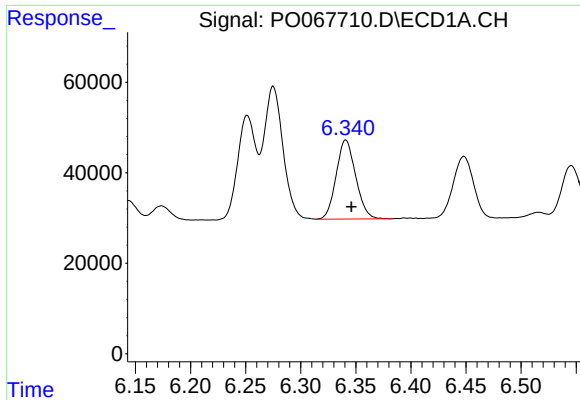

#5 AR-1016-3


R.T.: 6.341 min
Delta R.T.: -0.005 min
Response: 215680
Conc: 245.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

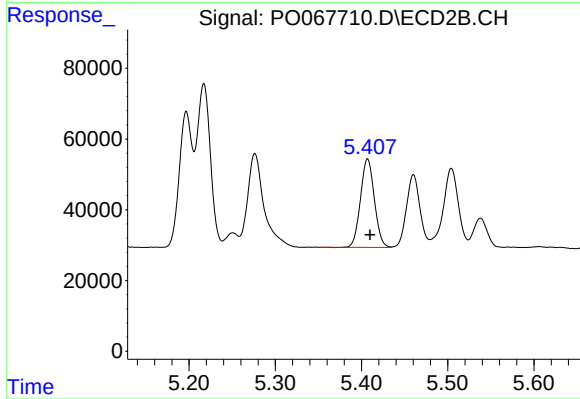


#5 AR-1016-3

R.T.: 5.407 min
Delta R.T.: -0.003 min
Response: 279348
Conc: 267.10 ng/ml

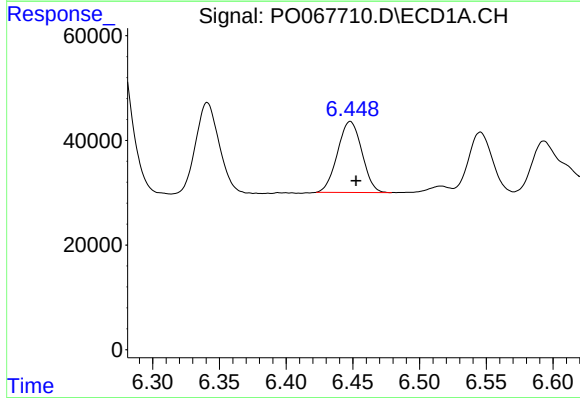


#6 AR-1016-4

R.T.: 6.448 min
Delta R.T.: -0.004 min
Response: 172619
Conc: 244.79 ng/ml

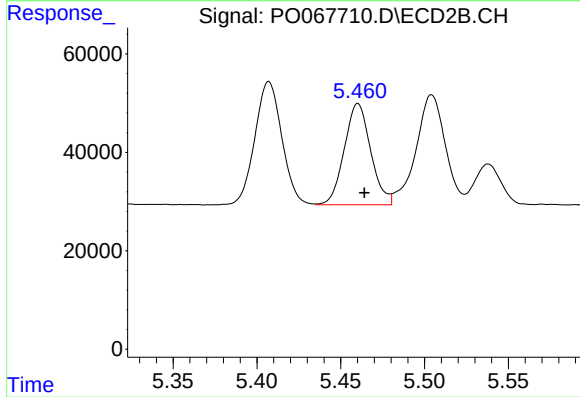

#6 AR-1016-4


R.T.: 5.460 min
Delta R.T.: -0.004 min
Response: 225263
Conc: 252.51 ng/ml

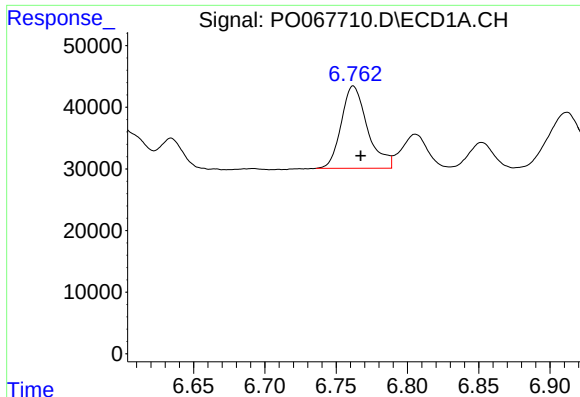

#7 AR-1016-5


R.T.: 6.762 min
Delta R.T.: -0.005 min
Response: 170919
Conc: 237.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

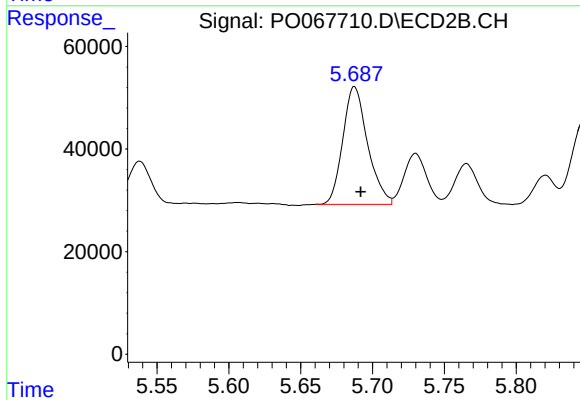


#7 AR-1016-5

R.T.: 5.688 min
Delta R.T.: -0.004 min
Response: 275949
Conc: 243.85 ng/ml

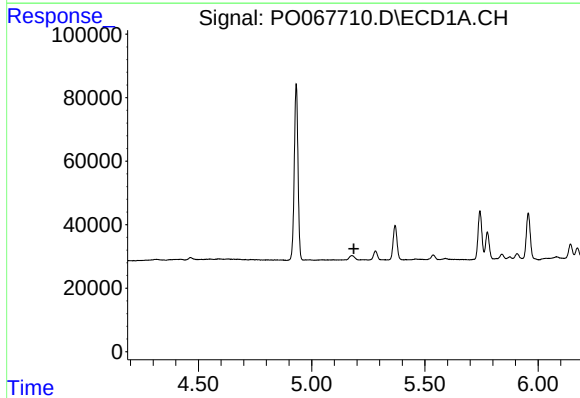


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 5.187 min
Response: 0
Conc: N.D.

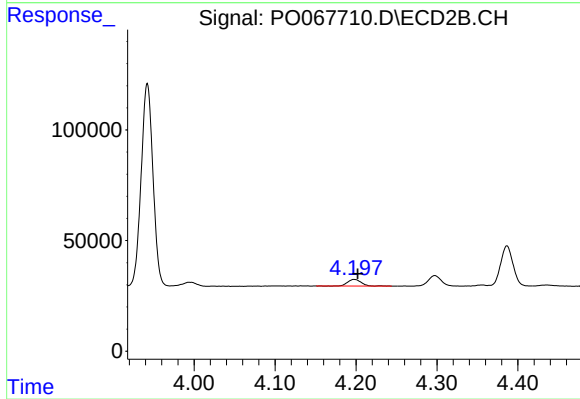

#8 AR-1221-1


R.T.: 4.198 min
Delta R.T.: -0.004 min
Response: 35839
Conc: 80.65 ng/ml

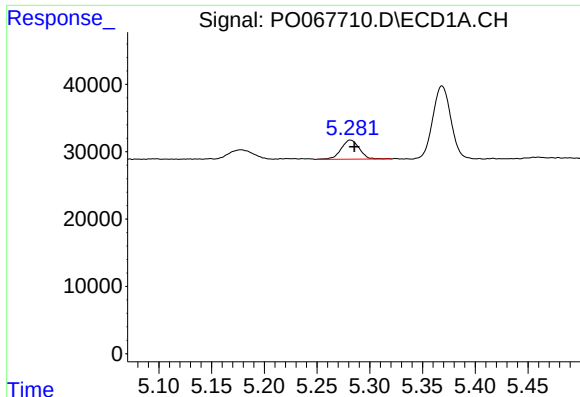

#9 AR-1221-2


R.T.: 5.282 min
Delta R.T.: -0.004 min
Response: 33993
Conc: 146.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

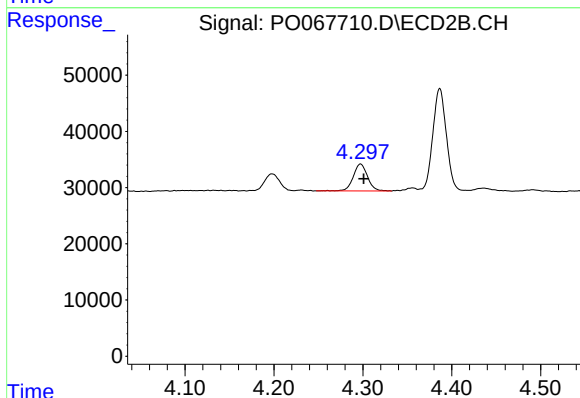


#9 AR-1221-2

R.T.: 4.298 min
Delta R.T.: -0.003 min
Response: 53183
Conc: 168.64 ng/ml

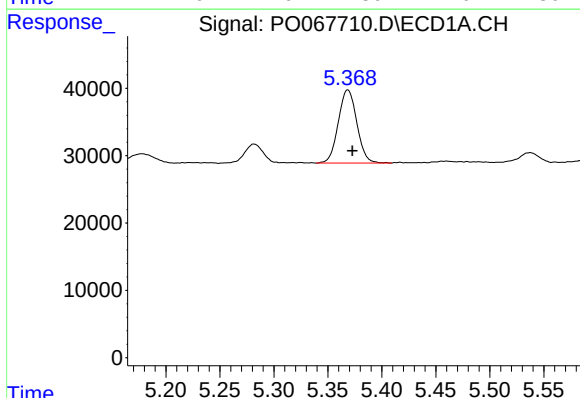


#10 AR-1221-3

R.T.: 5.369 min
Delta R.T.: -0.004 min
Response: 129792
Conc: 172.76 ng/ml

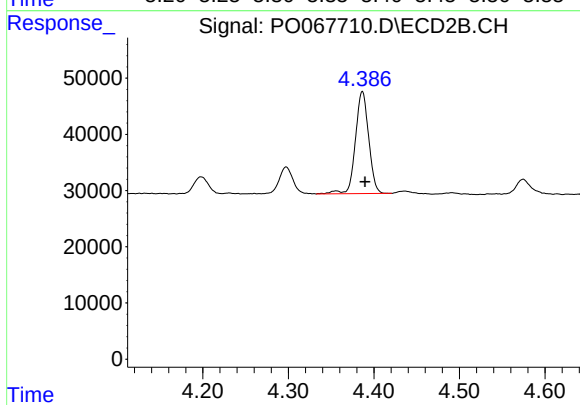

#10 AR-1221-3


R.T.: 4.387 min
Delta R.T.: -0.003 min
Response: 195541
Conc: 199.18 ng/ml

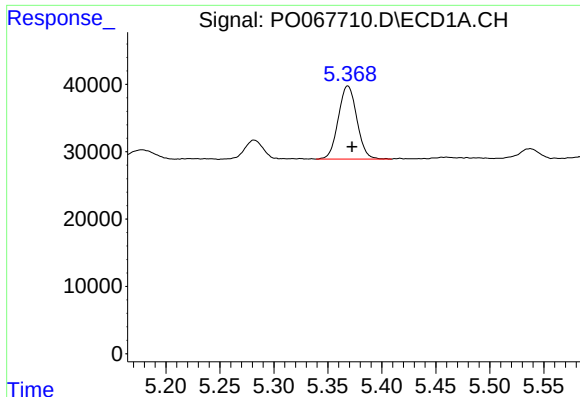

#11 AR-1232-1


R.T.: 5.369 min
Delta R.T.: -0.004 min
Response: 129792
Conc: 252.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

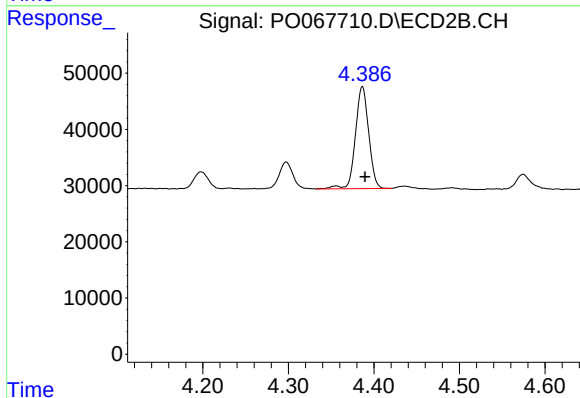


#11 AR-1232-1

R.T.: 4.387 min
Delta R.T.: -0.003 min
Response: 195541
Conc: 282.55 ng/ml

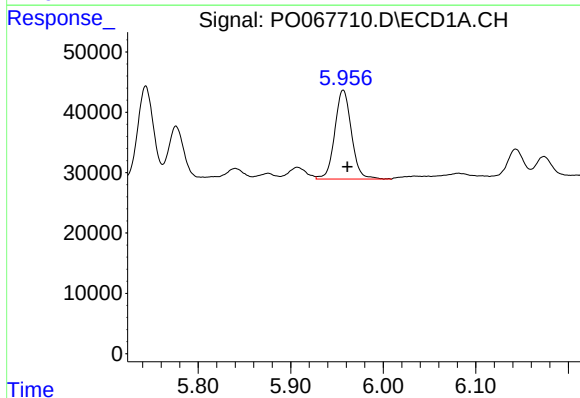


#12 AR-1232-2

R.T.: 5.957 min
Delta R.T.: -0.004 min
Response: 184392
Conc: 687.32 ng/ml

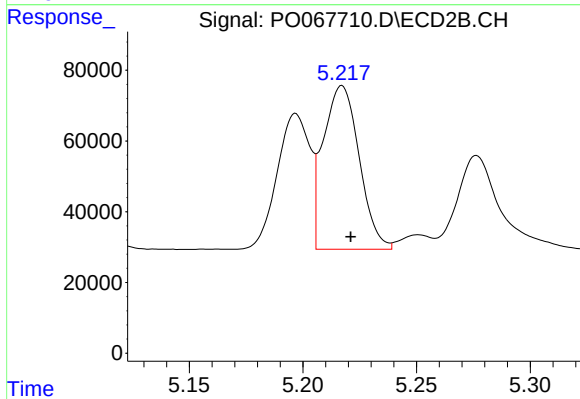

#12 AR-1232-2


R.T.: 5.217 min
Delta R.T.: -0.004 min
Response: 510597
Conc: 703.92 ng/ml

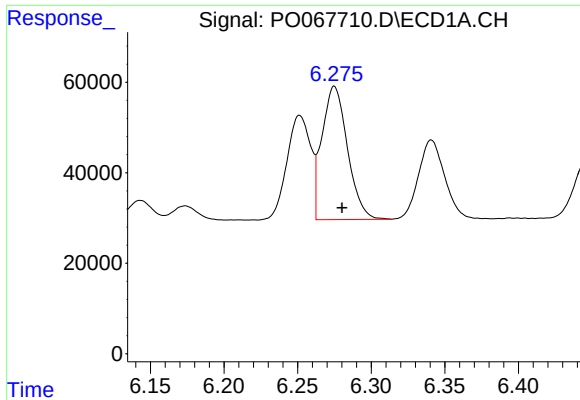

#13 AR-1232-3


R.T.: 6.275 min
Delta R.T.: -0.005 min
Response: 356297
Conc: 679.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

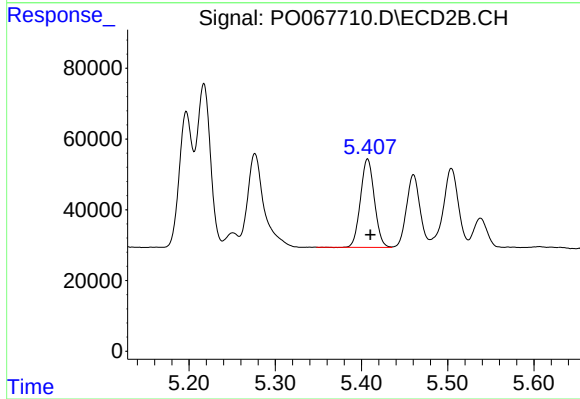


#13 AR-1232-3

R.T.: 5.407 min
Delta R.T.: -0.003 min
Response: 279348
Conc: 724.71 ng/ml

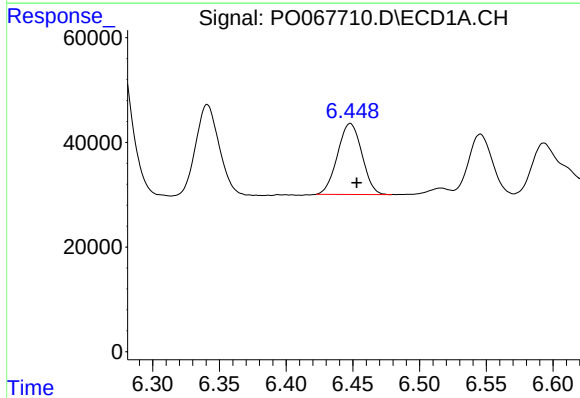


#14 AR-1232-4

R.T.: 6.448 min
Delta R.T.: -0.005 min
Response: 172619
Conc: 671.47 ng/ml

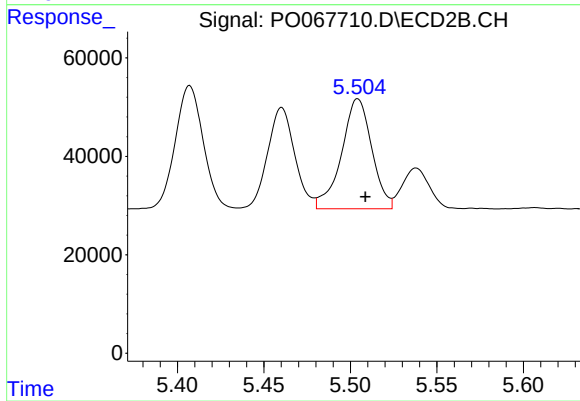

#14 AR-1232-4


R.T.: 5.504 min
Delta R.T.: -0.004 min
Response: 271932
Conc: 768.68 ng/ml

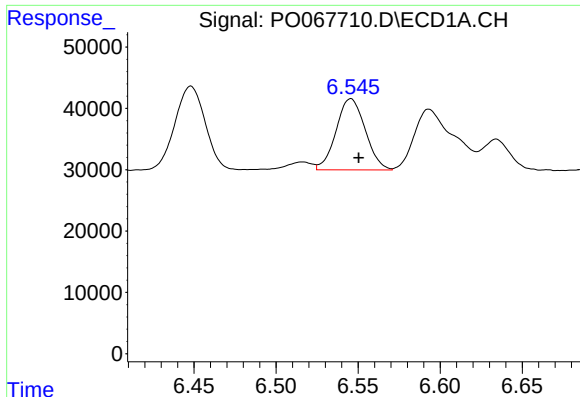

#15 AR-1232-5


R.T.: 6.546 min
Delta R.T.: -0.005 min
Response: 143681
Conc: 767.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

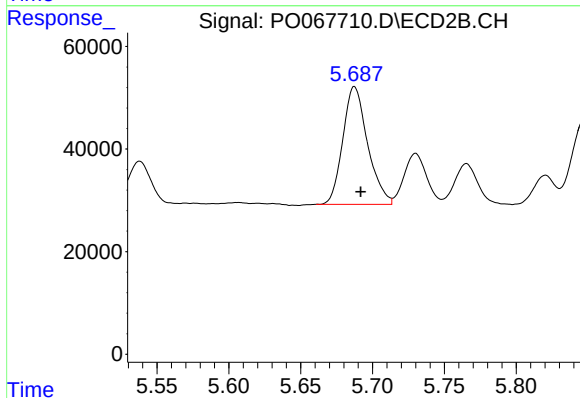


#15 AR-1232-5

R.T.: 5.688 min
Delta R.T.: -0.004 min
Response: 275949
Conc: 722.12 ng/ml

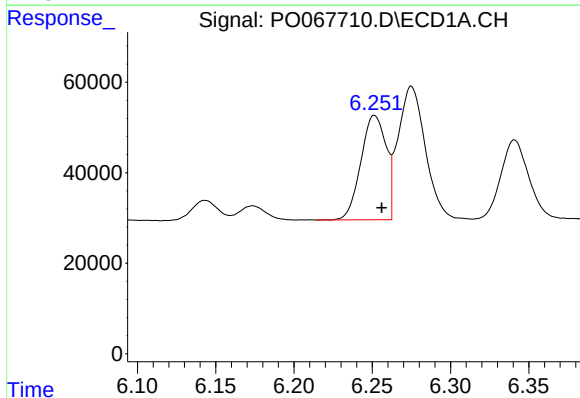


#16 AR-1242-1

R.T.: 6.251 min
Delta R.T.: -0.005 min
Response: 258624
Conc: 376.70 ng/ml

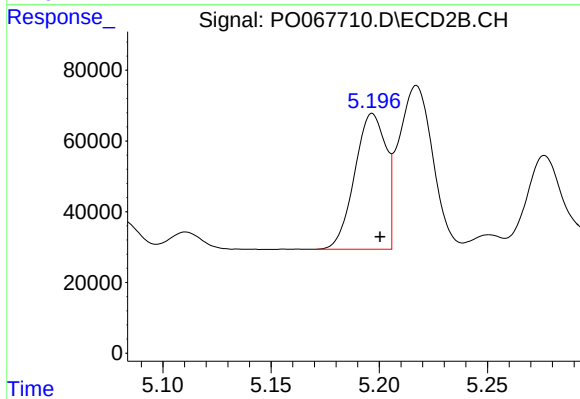

#16 AR-1242-1


R.T.: 5.197 min
Delta R.T.: -0.003 min
Response: 383923
Conc: 391.30 ng/ml

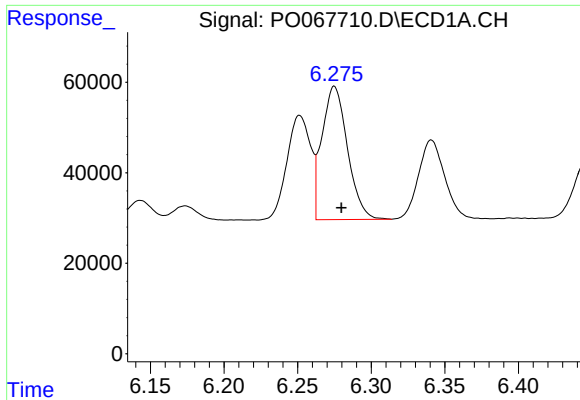

#17 AR-1242-2


R.T.: 6.275 min
Delta R.T.: -0.005 min
Response: 356297
Conc: 379.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

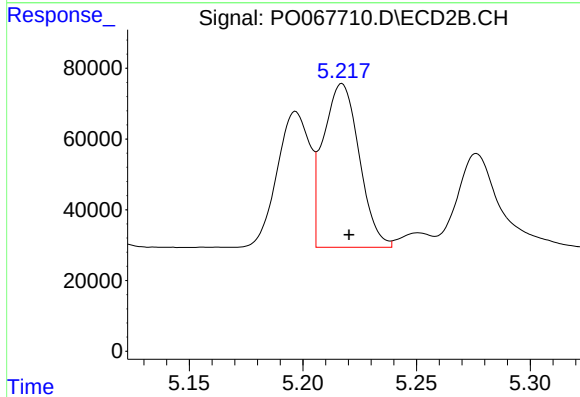


#17 AR-1242-2

R.T.: 5.217 min
Delta R.T.: -0.003 min
Response: 510597
Conc: 391.86 ng/ml

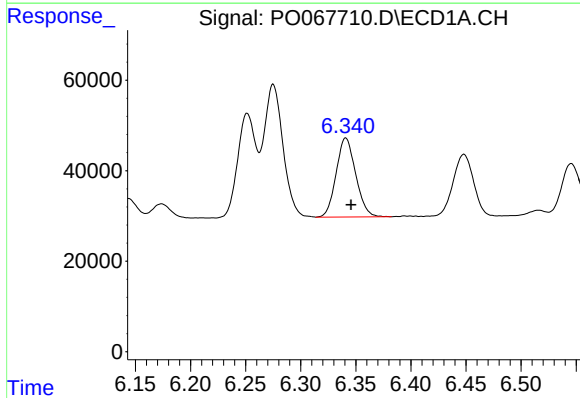


#18 AR-1242-3

R.T.: 6.341 min
Delta R.T.: -0.005 min
Response: 215680
Conc: 368.04 ng/ml

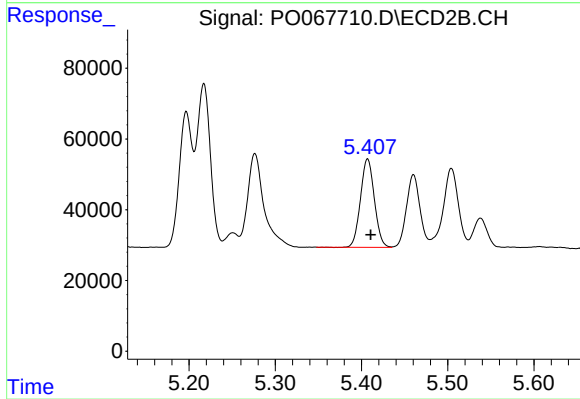

#18 AR-1242-3


R.T.: 5.407 min
Delta R.T.: -0.003 min
Response: 279348
Conc: 390.65 ng/ml

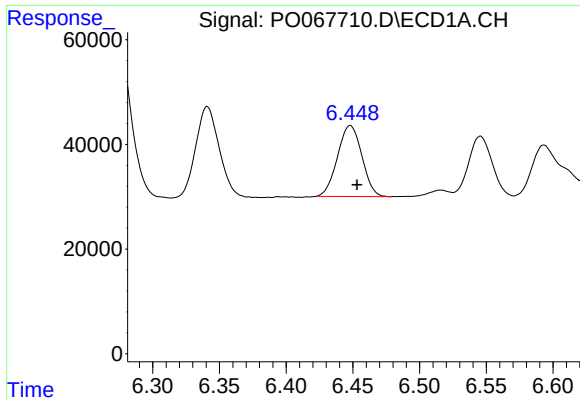

#19 AR-1242-4


R.T.: 6.448 min
Delta R.T.: -0.005 min
Response: 172619
Conc: 367.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

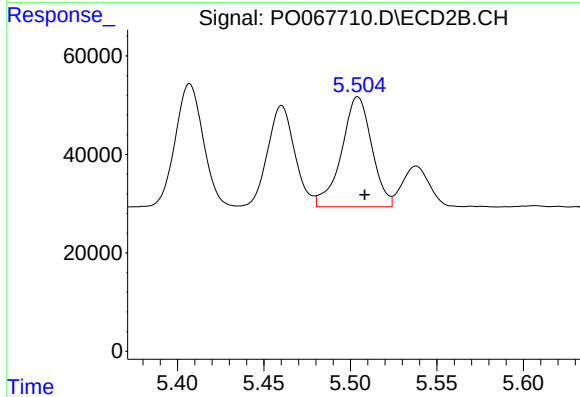


#19 AR-1242-4

R.T.: 5.504 min
Delta R.T.: -0.004 min
Response: 271932
Conc: 377.78 ng/ml

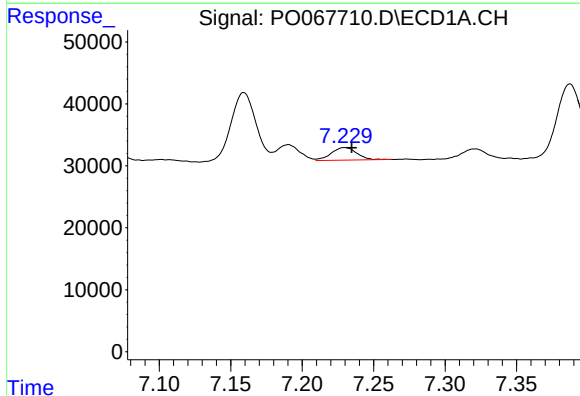


#20 AR-1242-5

R.T.: 7.230 min
Delta R.T.: -0.005 min
Response: 25164
Conc: 47.10 ng/ml

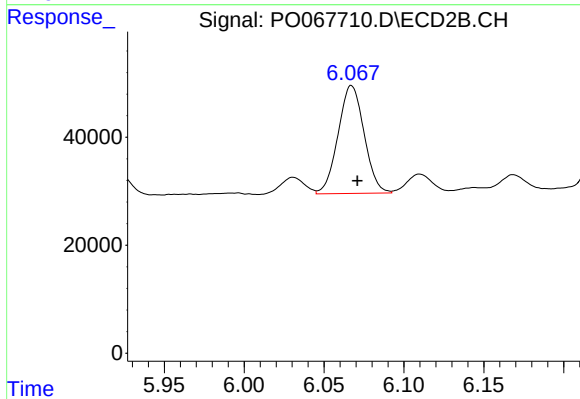

#20 AR-1242-5


R.T.: 6.067 min
Delta R.T.: -0.004 min
Response: 226596
Conc: 242.16 ng/ml

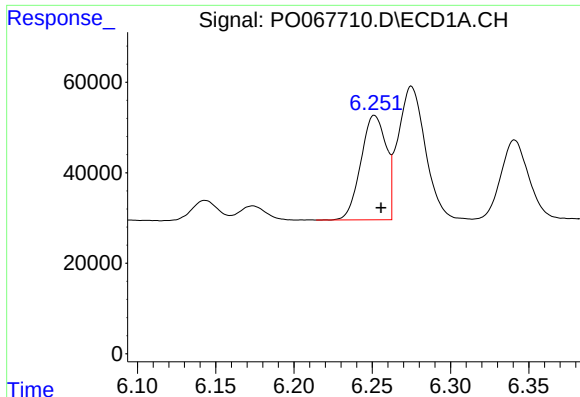

#21 AR-1248-1


R.T.: 6.251 min
Delta R.T.: -0.004 min
Response: 258624
Conc: 482.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

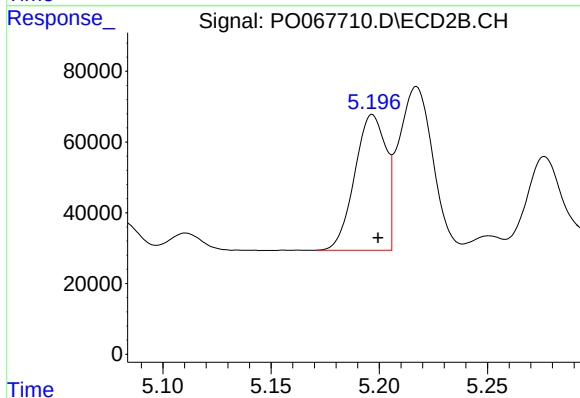


#21 AR-1248-1

R.T.: 5.197 min
Delta R.T.: -0.002 min
Response: 383923
Conc: 491.45 ng/ml

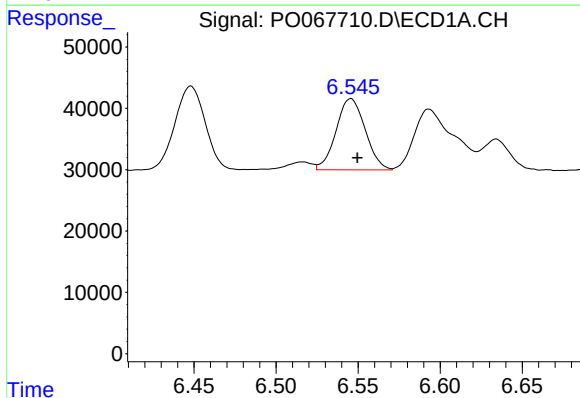


#22 AR-1248-2

R.T.: 6.546 min
Delta R.T.: -0.004 min
Response: 143681
Conc: 204.21 ng/ml

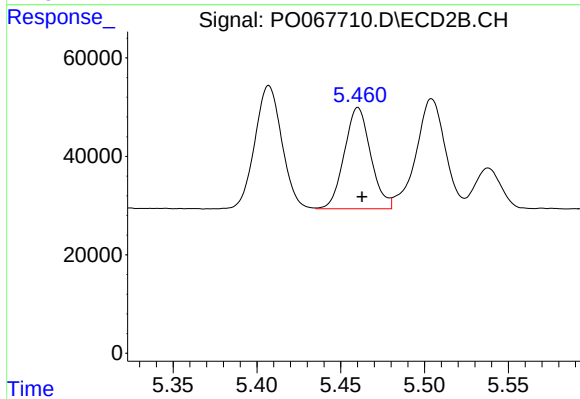

#22 AR-1248-2


R.T.: 5.460 min
Delta R.T.: -0.003 min
Response: 225263
Conc: 223.87 ng/ml

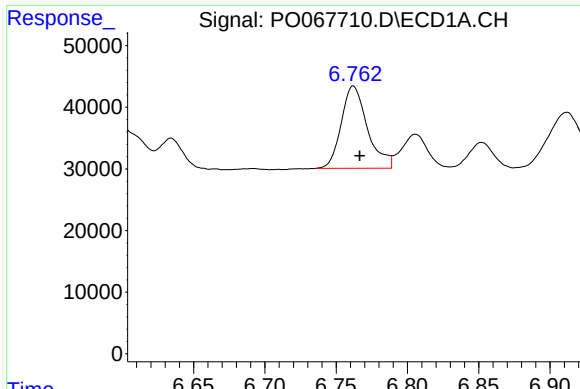

#23 AR-1248-3


R.T.: 6.762 min
Delta R.T.: -0.005 min
Response: 170919
Conc: 210.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

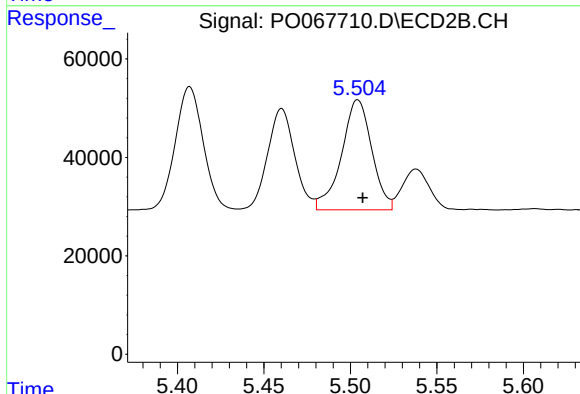


#23 AR-1248-3

R.T.: 5.504 min
Delta R.T.: -0.003 min
Response: 271932
Conc: 265.86 ng/ml

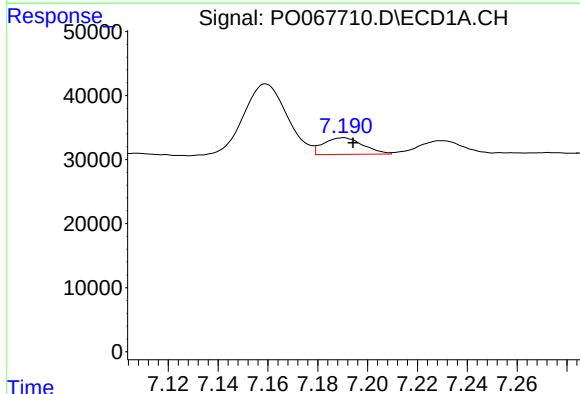


#24 AR-1248-4

R.T.: 7.190 min
Delta R.T.: -0.004 min
Response: 28963
Conc: 30.70 ng/ml

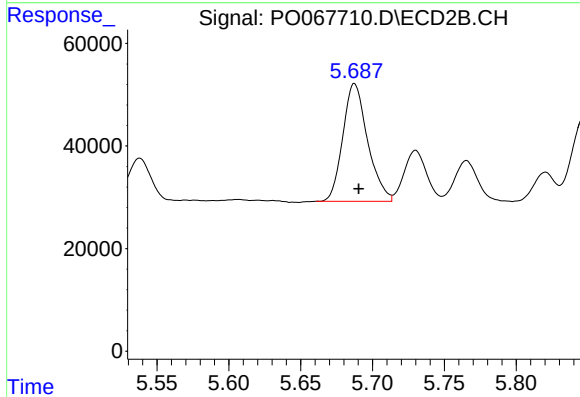

#24 AR-1248-4


R.T.: 5.688 min
Delta R.T.: -0.003 min
Response: 275949
Conc: 221.42 ng/ml

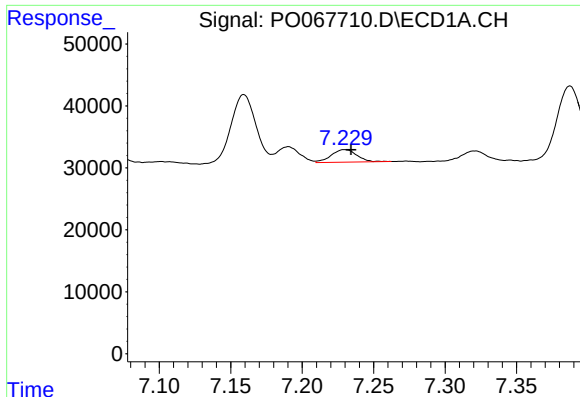

#25 AR-1248-5


R.T.: 7.230 min
Delta R.T.: -0.004 min
Response: 25164
Conc: 27.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

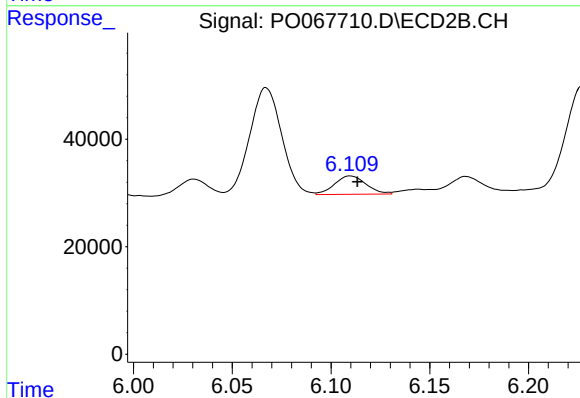


#25 AR-1248-5

R.T.: 6.110 min
Delta R.T.: -0.003 min
Response: 37941
Conc: 30.66 ng/ml

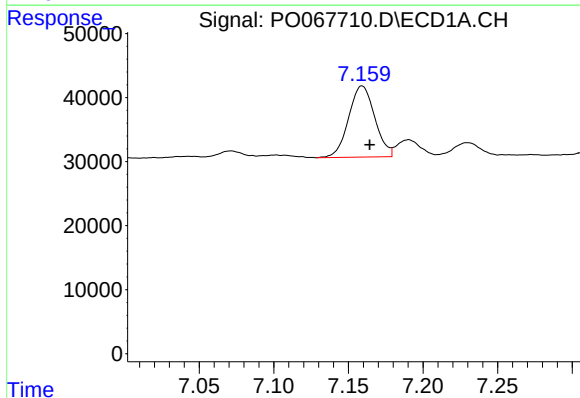


#26 AR-1254-1

R.T.: 7.159 min
Delta R.T.: -0.005 min
Response: 135601
Conc: 109.79 ng/ml

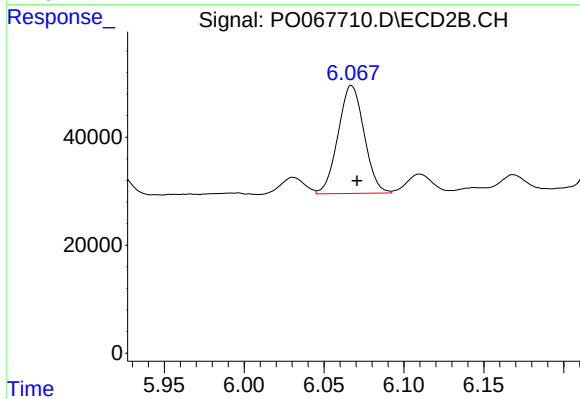

#26 AR-1254-1


R.T.: 6.067 min
Delta R.T.: -0.003 min
Response: 226596
Conc: 88.37 ng/ml

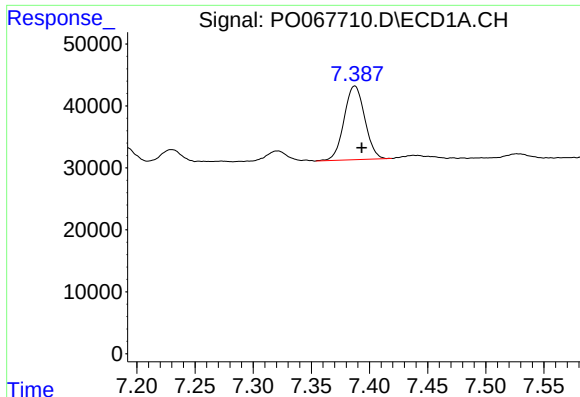

#27 AR-1254-2


R.T.: 7.387 min
Delta R.T.: -0.006 min
Response: 147100
Conc: 74.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

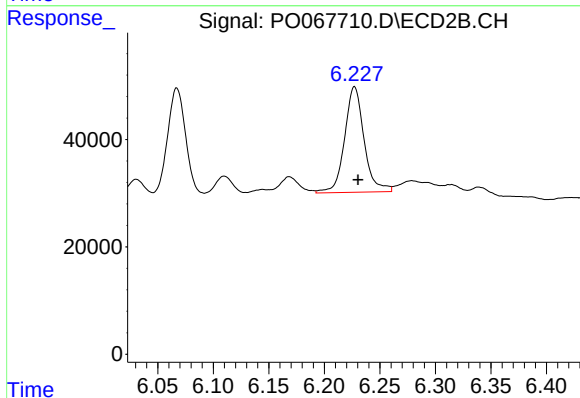


#27 AR-1254-2

R.T.: 6.227 min
Delta R.T.: -0.003 min
Response: 240751
Conc: 105.56 ng/ml

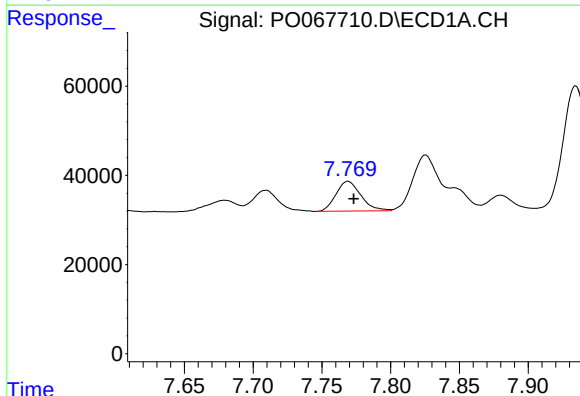


#28 AR-1254-3

R.T.: 7.769 min
Delta R.T.: -0.004 min
Response: 84135
Conc: 40.55 ng/ml

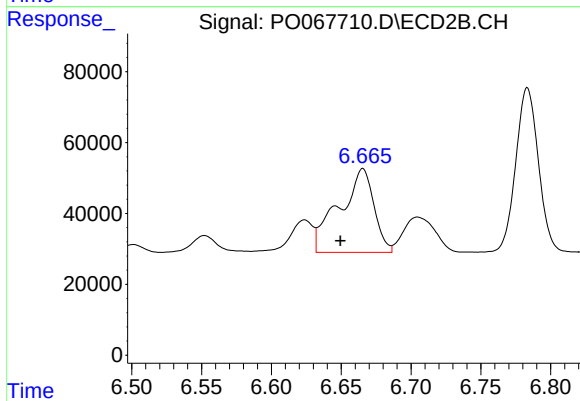

#28 AR-1254-3


R.T.: 6.665 min
Delta R.T.: 0.016 min
Response: 410720
Conc: 112.49 ng/ml

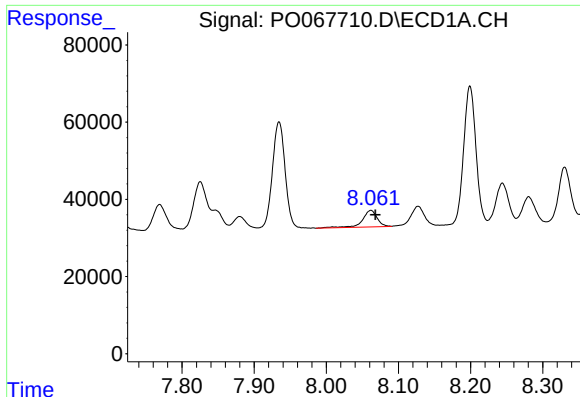

#29 AR-1254-4


R.T.: 8.062 min
Delta R.T.: -0.006 min
Response: 60441
Conc: 37.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

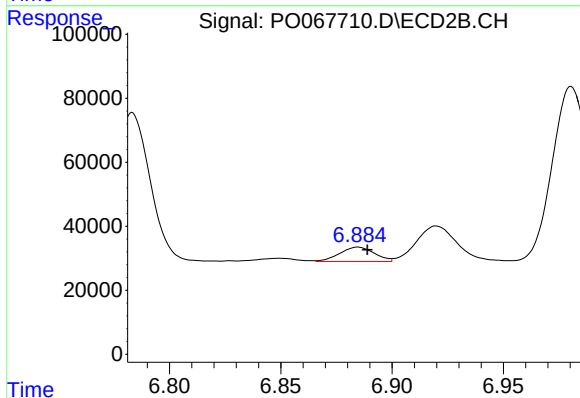


#29 AR-1254-4

R.T.: 6.885 min
Delta R.T.: -0.004 min
Response: 48383
Conc: 20.07 ng/ml

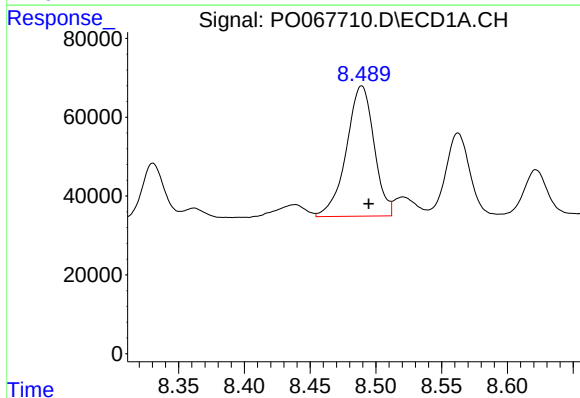


#30 AR-1254-5

R.T.: 8.489 min
Delta R.T.: -0.005 min
Response: 484500
Conc: 282.39 ng/ml

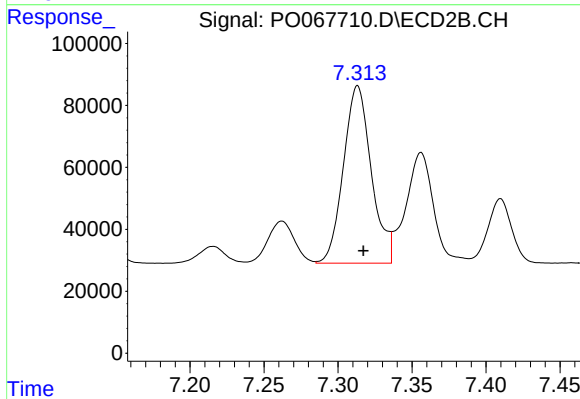

#30 AR-1254-5


R.T.: 7.313 min
Delta R.T.: -0.004 min
Response: 752471
Conc: 225.44 ng/ml

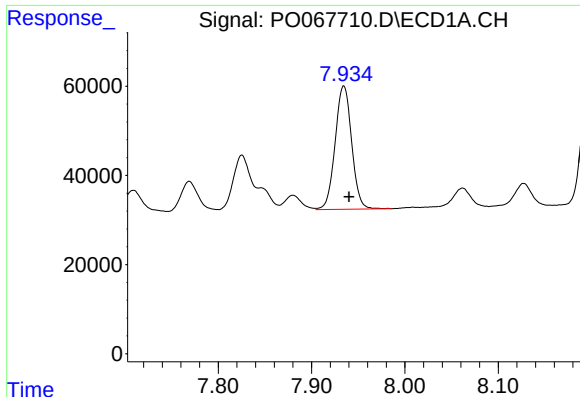

#31 AR-1260-1


R.T.: 7.935 min
Delta R.T.: -0.005 min
Response: 340265
Conc: 251.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

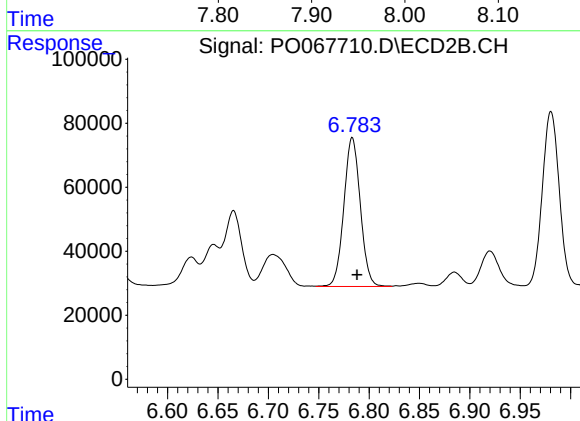


#31 AR-1260-1

R.T.: 6.783 min
Delta R.T.: -0.005 min
Response: 528111
Conc: 251.91 ng/ml

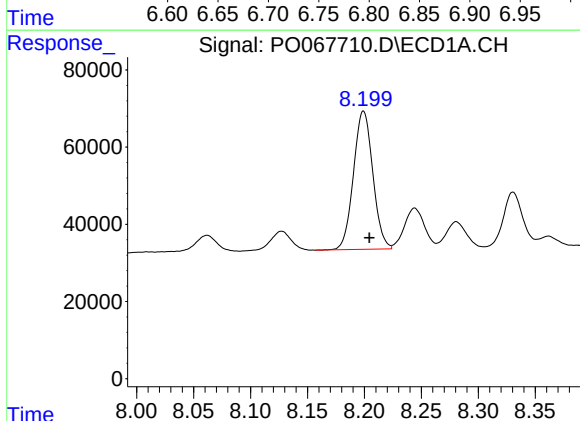


#32 AR-1260-2

R.T.: 8.199 min
Delta R.T.: -0.005 min
Response: 423683
Conc: 250.97 ng/ml

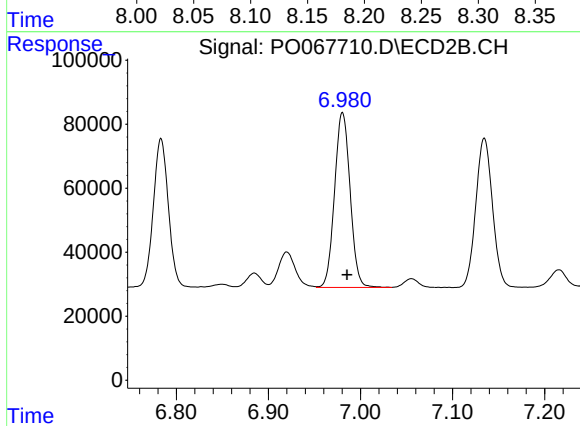

#32 AR-1260-2


R.T.: 6.981 min
Delta R.T.: -0.005 min
Response: 640727
Conc: 249.53 ng/ml

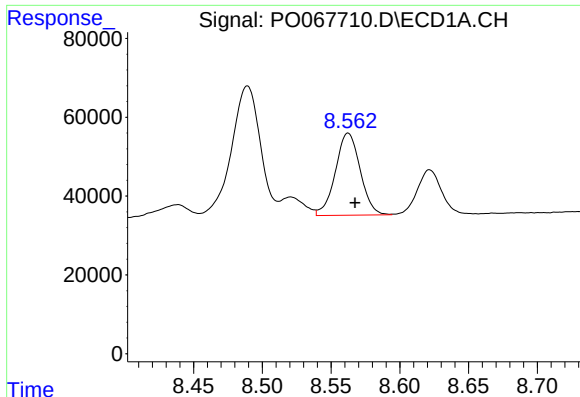

#33 AR-1260-3


R.T.: 8.562 min
Delta R.T.: -0.005 min
Response: 261300
Conc: 200.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

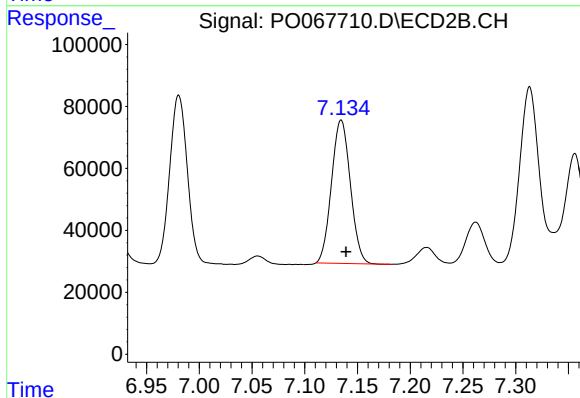


#33 AR-1260-3

R.T.: 7.135 min
Delta R.T.: -0.005 min
Response: 574587
Conc: 238.95 ng/ml

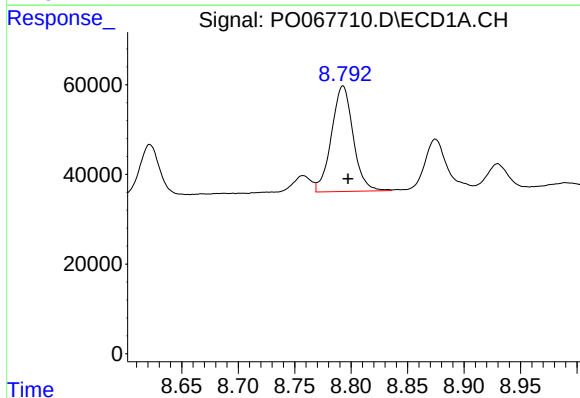


#34 AR-1260-4

R.T.: 8.793 min
Delta R.T.: -0.005 min
Response: 315628
Conc: 205.38 ng/ml

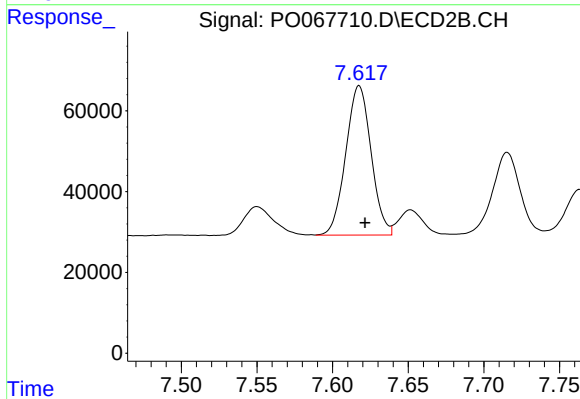

#34 AR-1260-4


R.T.: 7.618 min
Delta R.T.: -0.004 min
Response: 431077
Conc: 205.11 ng/ml

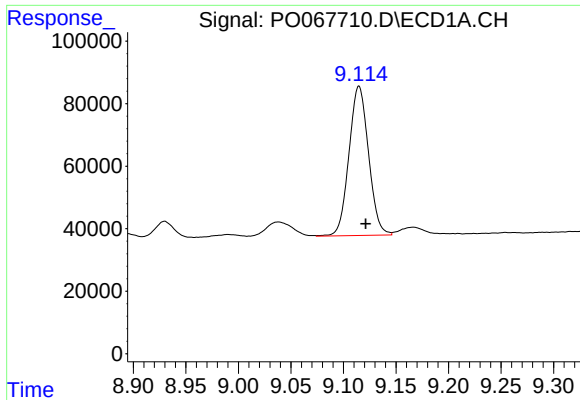

#35 AR-1260-5


R.T.: 9.115 min
Delta R.T.: -0.007 min
Response: 619204
Conc: 196.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

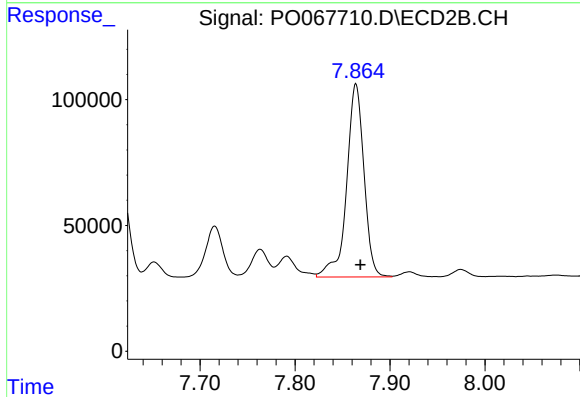


#35 AR-1260-5

R.T.: 7.864 min
Delta R.T.: -0.004 min
Response: 975330
Conc: 192.66 ng/ml

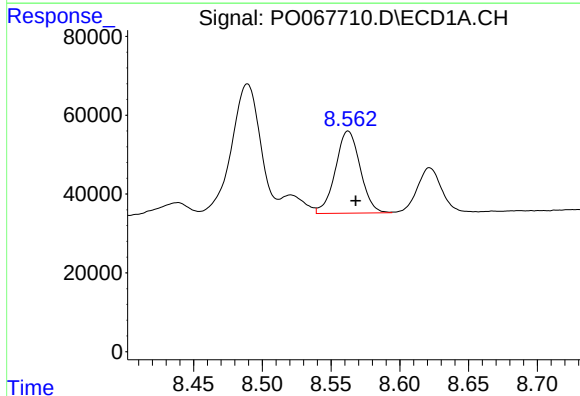


#36 AR-1262-1

R.T.: 8.562 min
Delta R.T.: -0.005 min
Response: 261300
Conc: 155.86 ng/ml

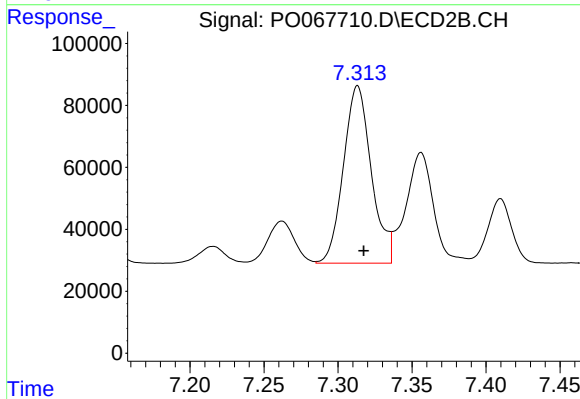

#36 AR-1262-1


R.T.: 7.313 min
Delta R.T.: -0.004 min
Response: 752471
Conc: 543.02 ng/ml

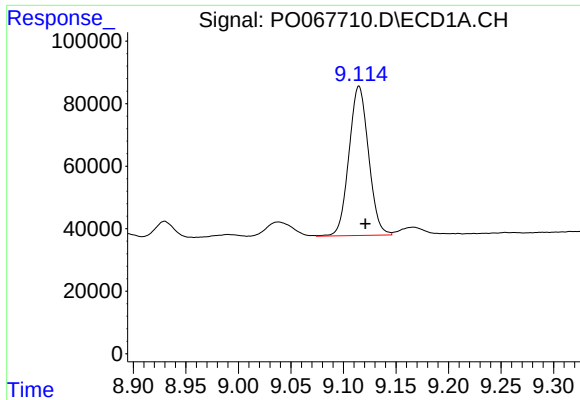

#37 AR-1262-2


R.T.: 9.115 min
Delta R.T.: -0.006 min
Response: 619204
Conc: 215.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

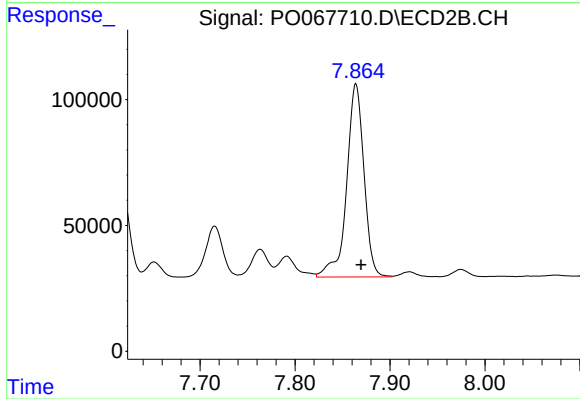


#37 AR-1262-2

R.T.: 7.864 min
Delta R.T.: -0.005 min
Response: 975330
Conc: 213.32 ng/ml

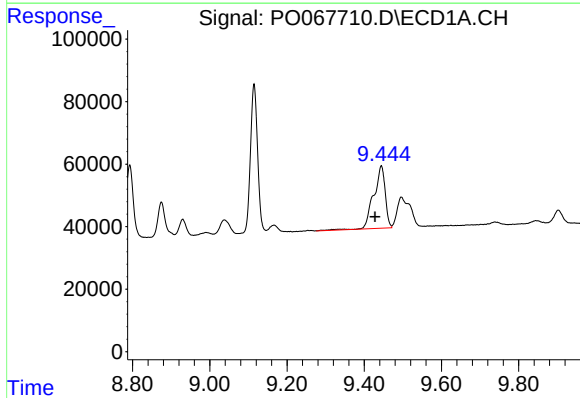


#38 AR-1262-3

R.T.: 9.444 min
Delta R.T.: 0.016 min
Response: 413360
Conc: 198.65 ng/ml

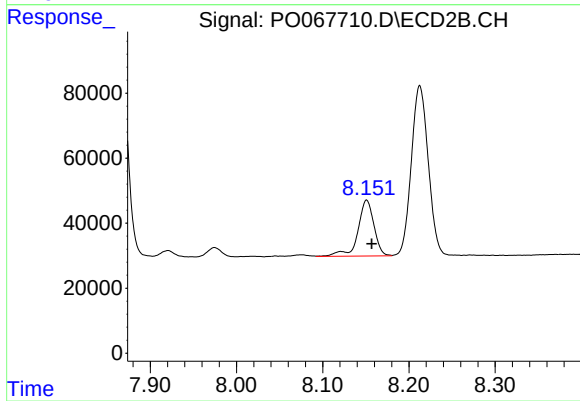

#38 AR-1262-3


R.T.: 8.151 min
Delta R.T.: -0.006 min
Response: 222466
Conc: 113.19 ng/ml

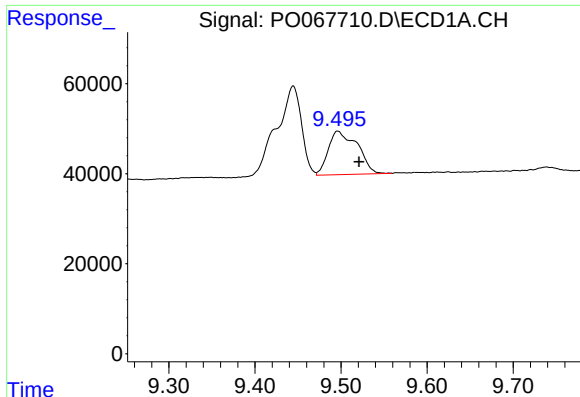

#39 AR-1262-4


R.T.: 9.496 min
Delta R.T.: -0.025 min
Response: 226436
Conc: 143.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

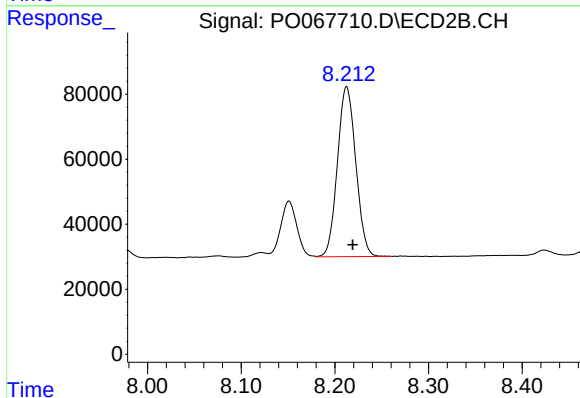


#39 AR-1262-4

R.T.: 8.213 min
Delta R.T.: -0.007 min
Response: 713180
Conc: 208.05 ng/ml

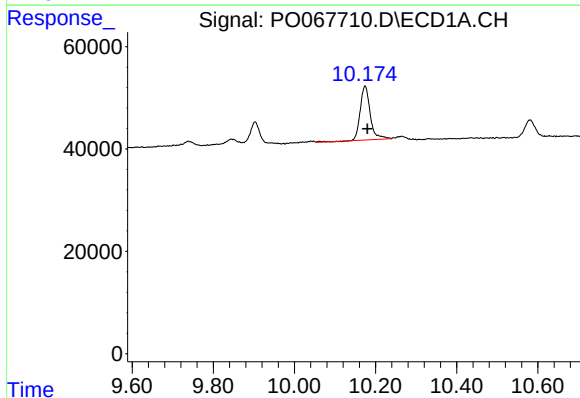


#40 AR-1262-5

R.T.: 10.174 min
Delta R.T.: -0.006 min
Response: 180063
Conc: 152.71 ng/ml

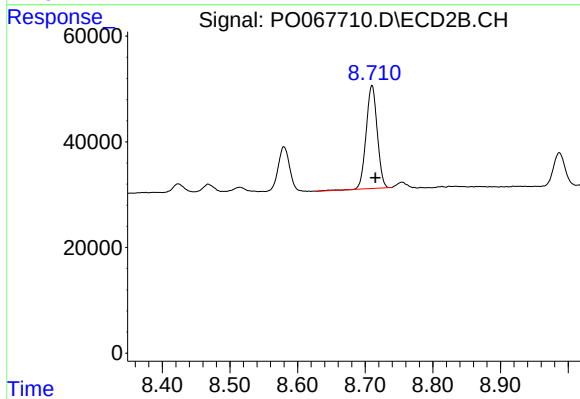

#40 AR-1262-5


R.T.: 8.710 min
Delta R.T.: -0.005 min
Response: 222958
Conc: 131.16 ng/ml

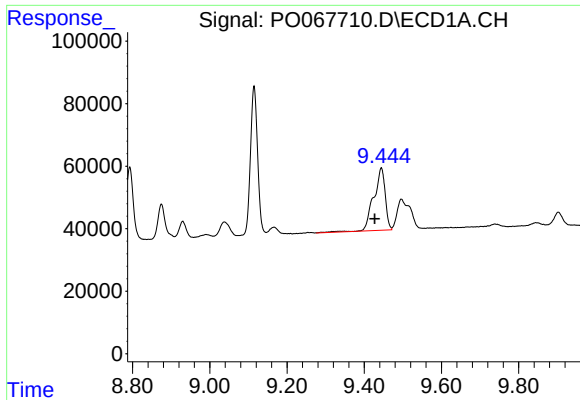

#41 AR-1268-1


R.T.: 9.444 min
Delta R.T.: 0.017 min
Response: 413360
Conc: 111.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

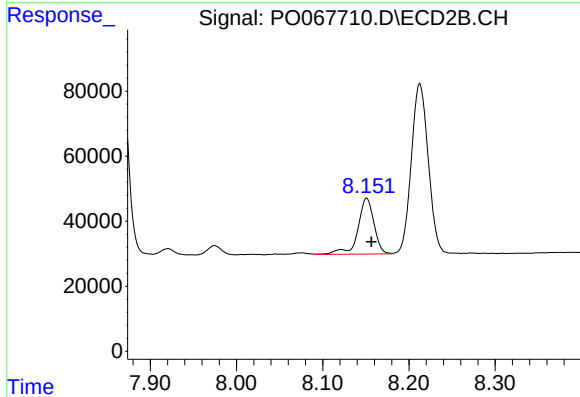


#41 AR-1268-1

R.T.: 8.151 min
Delta R.T.: -0.005 min
Response: 222466
Conc: 41.35 ng/ml

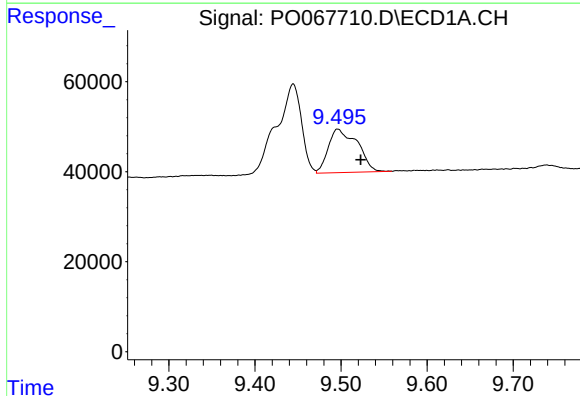


#42 AR-1268-2

R.T.: 9.496 min
Delta R.T.: -0.027 min
Response: 226436
Conc: 65.33 ng/ml

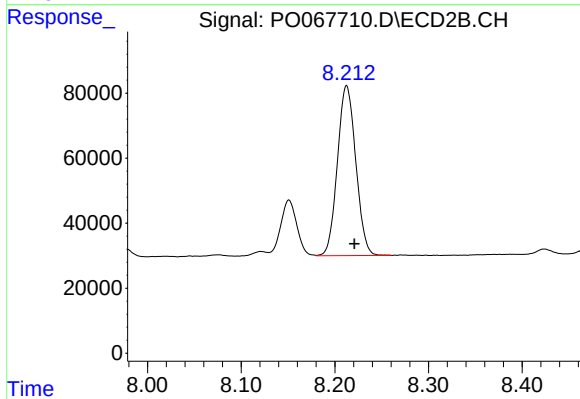

#42 AR-1268-2


R.T.: 8.213 min
Delta R.T.: -0.008 min
Response: 713180
Conc: 144.44 ng/ml

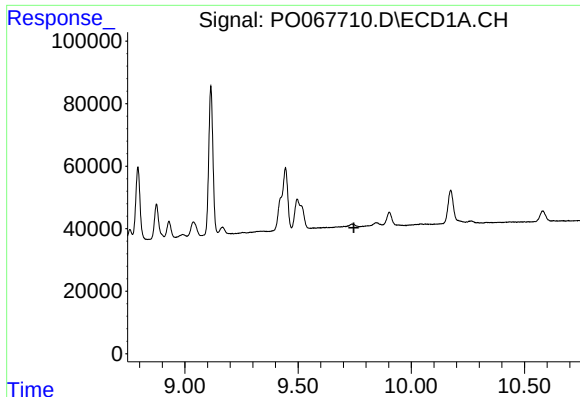

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.746 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

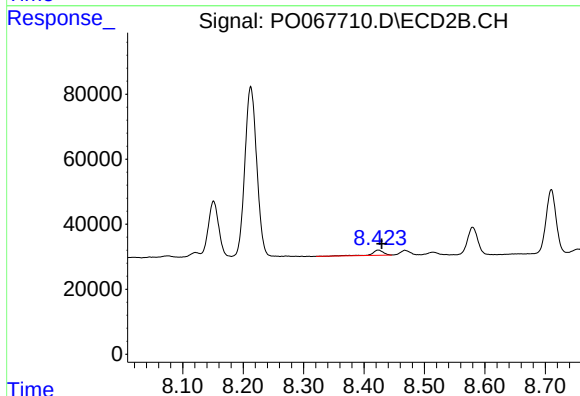


#43 AR-1268-3

R.T.: 8.424 min
Delta R.T.: -0.006 min
Response: 21029
Conc: 5.02 ng/ml

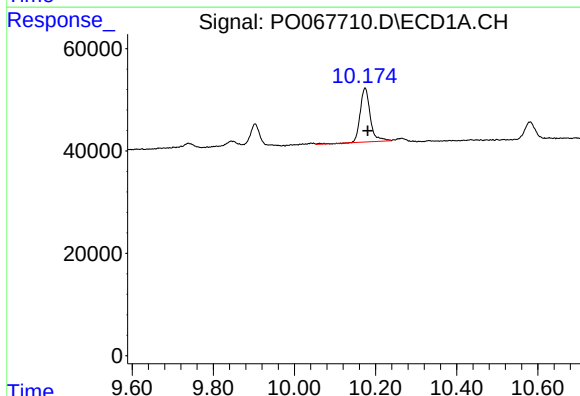


#44 AR-1268-4

R.T.: 10.174 min
Delta R.T.: -0.006 min
Response: 180063
Conc: 129.71 ng/ml

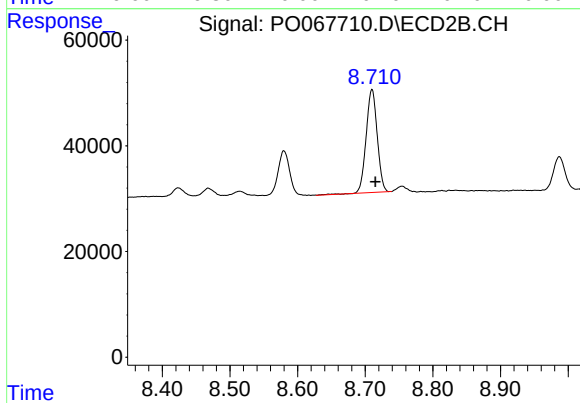

#44 AR-1268-4


R.T.: 8.710 min
Delta R.T.: -0.005 min
Response: 222958
Conc: 115.23 ng/ml

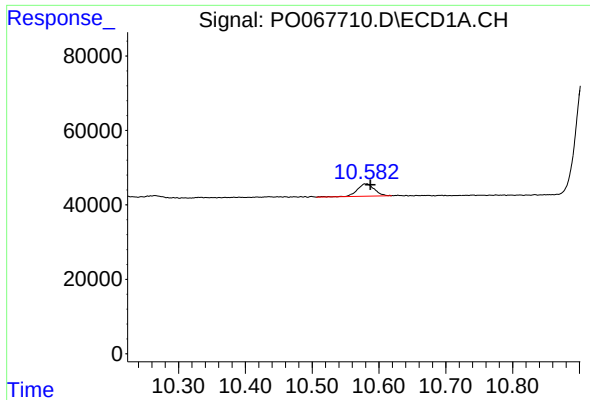

#45 AR-1268-5

R.T.: 10.581 min
Delta R.T.: -0.007 min
Response: 58942
Conc: 5.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMS

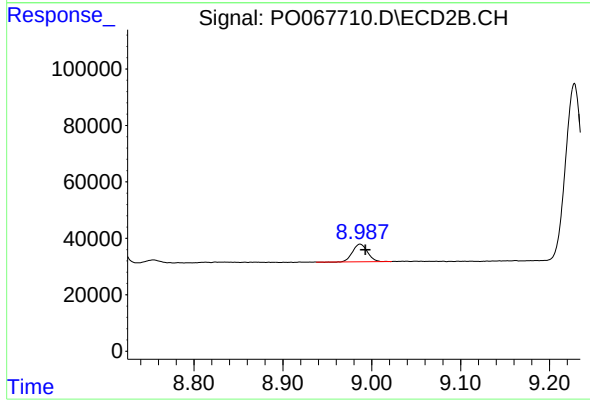

#45 AR-1268-5

R.T.: 8.987 min
Delta R.T.: -0.006 min
Response: 73158
Conc: 5.67 ng/ml