

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040720\
 Data File : P0067711.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Apr 2020 12:11
 Operator : DD\AJ
 Sample : L2166-19MSD
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-45-COMPMSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 14:49:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.932	3.942	635855	938759	26.701	28.008
2)	SA Decachlor...	10.911	9.227	748978	826820	22.000	19.998
Target Compounds							
3)	L1 AR-1016-1	6.252	5.197	258540	387912	250.709	264.620
4)	L1 AR-1016-2	6.275	5.217	362285	515062	256.769	262.924
5)	L1 AR-1016-3	6.341	5.407	218720	281891	248.833	269.529
6)	L1 AR-1016-4	6.449	5.460	174302	226091	247.177	253.442
7)	L1 AR-1016-5	6.763	5.688	174260	271813	242.351	240.199
8)	L2 AR-1221-1	0.000	4.198	0	38392	N.D.	86.397 #
9)	L2 AR-1221-2	5.282	4.297	33031	53953	142.013	171.083
10)	L2 AR-1221-3	5.369	4.387	129380	199028	172.209	202.729
11)	L3 AR-1232-1	5.369	4.387	129380	199028	251.288	287.585
12)	L3 AR-1232-2	5.957	5.217	183073	515062	682.403	710.071
13)	L3 AR-1232-3	6.275	5.407	362285	281891	691.156	731.306
14)	L3 AR-1232-4	6.449	5.505	174302	274425	678.023	775.722
15)	L3 AR-1232-5	6.547	5.688	143582	271813	766.537	711.301
16)	L4 AR-1242-1	6.252	5.197	258540	387912	376.572	395.362
17)	L4 AR-1242-2	6.275	5.217	362285	515062	385.582	395.289
18)	L4 AR-1242-3	6.341	5.407	218720	281891	373.226	394.212
19)	L4 AR-1242-4	6.449	5.505	174302	274425	370.612	381.246
20)	L4 AR-1242-5	7.230	6.067	28691	230559	53.707	246.392 #
21)	L5 AR-1248-1	6.252	5.197	258540	387912	481.889	496.552
22)	L5 AR-1248-2	6.547	5.460	143582	226091	204.071	224.688
23)	L5 AR-1248-3	6.763	5.505	174260	274425	214.115	268.300 #
24)	L5 AR-1248-4	7.191	5.688	36113	271813	38.278	218.102 #
25)	L5 AR-1248-5	7.230	6.111	28691	38030	31.837	30.732
26)	L6 AR-1254-1	7.160	6.067	153850	230559	124.564	89.917 #
27)	L6 AR-1254-2	7.388	6.228	147632	236017	75.066	103.486 #
28)	L6 AR-1254-3	7.770	6.666	87792	427511	42.308	117.090 #
29)	L6 AR-1254-4	8.062	6.886	70370	52841	43.203	21.920 #
30)	L6 AR-1254-5	8.489	7.314	496972	761517	289.656	228.155
31)	L7 AR-1260-1	7.935	6.784	363192	550229	268.746	262.460
32)	L7 AR-1260-2	8.200	6.981	436925	648505	258.815	252.558
33)	L7 AR-1260-3	8.563	7.135	272593	586883	209.126	244.059
34)	L7 AR-1260-4	8.793	7.618	323229	431704	210.326	205.407
35)	L7 AR-1260-5	9.115	7.865	621687	981827	197.072	193.940
36)	L8 AR-1262-1	8.563	7.314	272593	761517	162.600	549.545 #
37)	L8 AR-1262-2	9.115	7.865	621687	981827	216.655	214.744
38)	L8 AR-1262-3	9.445	8.152	423230	219042	203.394	111.446 #
39)	L8 AR-1262-4	9.497	8.213	230860	717418	145.896	209.284 #
40)	L8 AR-1262-5	10.174	8.710	204321	219416	173.288	129.081 #
41)	L9 AR-1268-1	9.445	8.152	423230	219042	114.537	40.709 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040720\
 Data File : P0067711.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Apr 2020 12:11
 Operator : DD\AJ
 Sample : L2166-19MSD
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-45-COMPMSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 14:49:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	9.497	8.213	230860	717418	66.608	145.299 #
43) L9	AR-1268-3	0.000	8.425	0	16034	N.D.	3.825 #
44) L9	AR-1268-4	10.174	8.710	204321	219416	147.182	113.401
45) L9	AR-1268-5	10.582	8.987	60533	74330	6.105	5.764



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040720\
Data File : P0067711.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Apr 2020 12:11
Operator : DD\AJ
Sample : L2166-19MSD
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 14:49:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

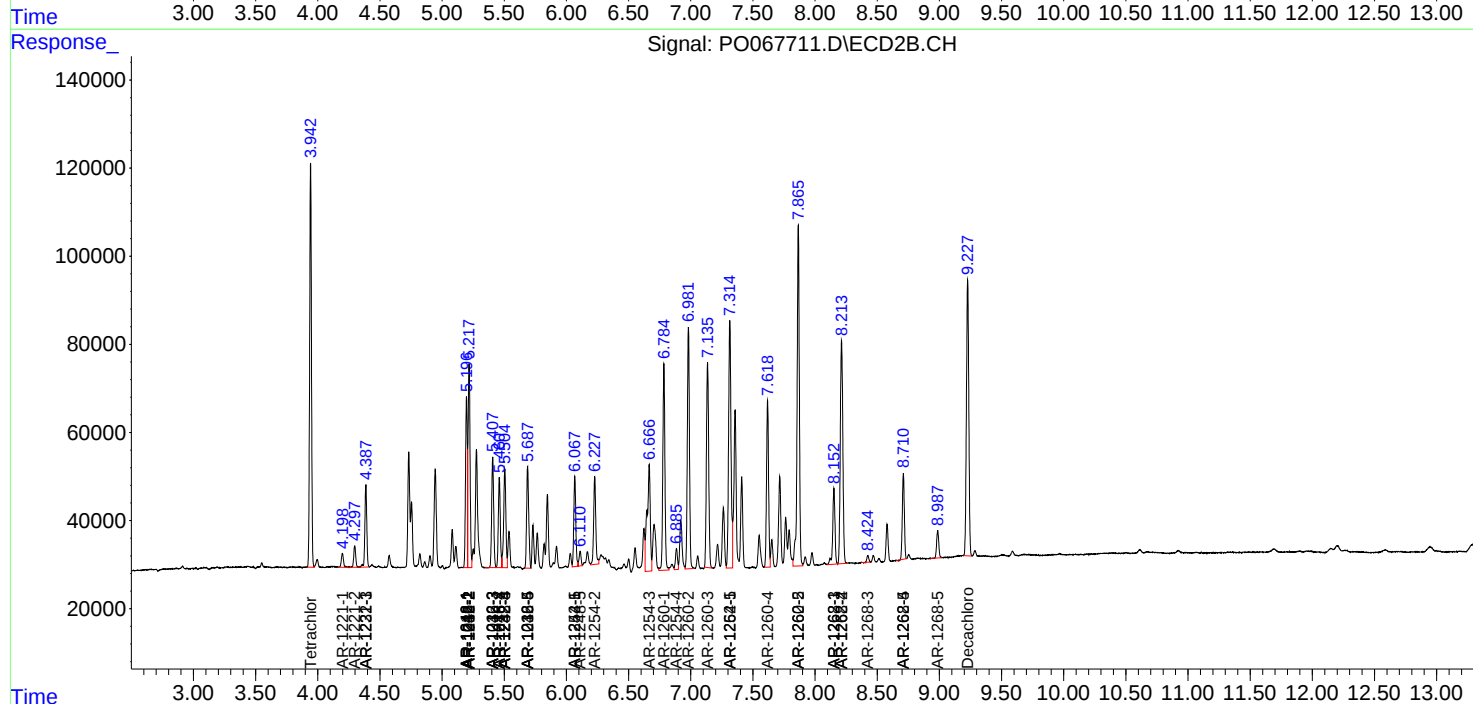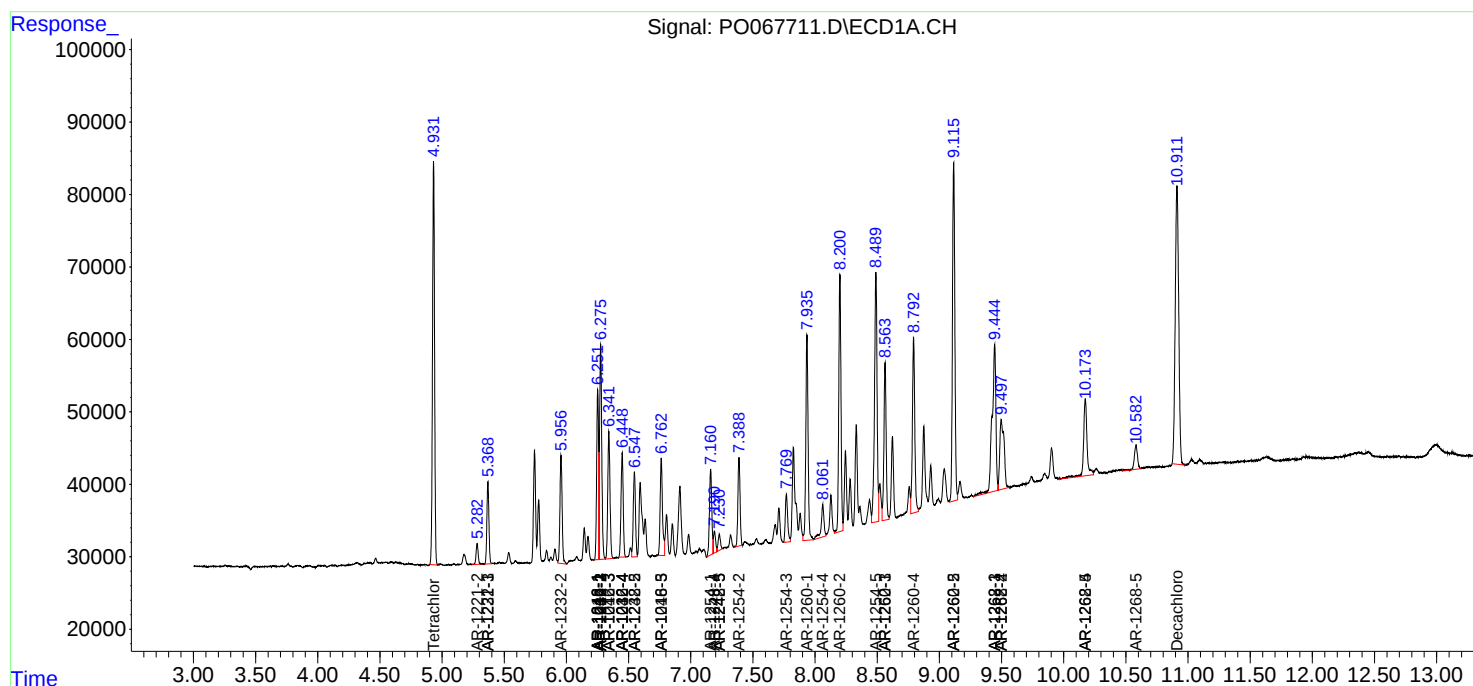


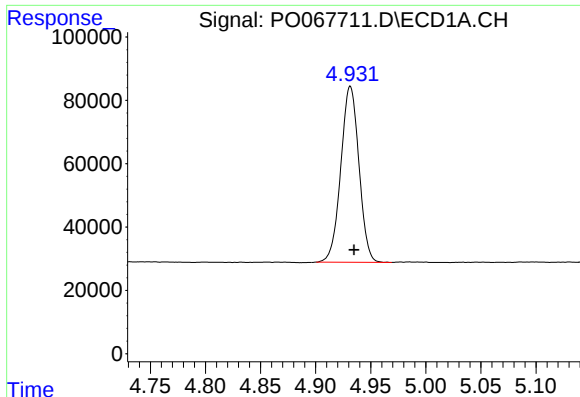

#1 Tetrachloro-m-xylene


R.T.: 4.932 min
Delta R.T.: -0.003 min
Response: 635855
Conc: 26.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

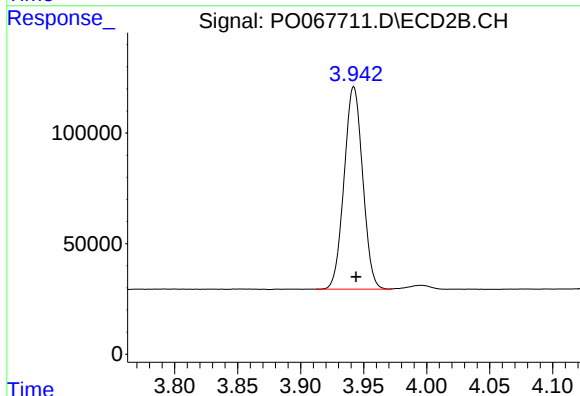


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: -0.002 min
Response: 938759
Conc: 28.01 ng/ml

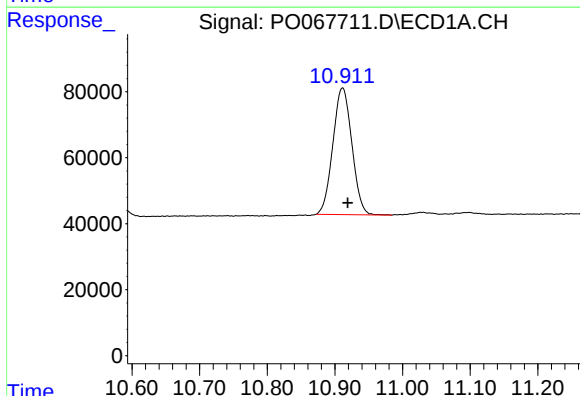


#2 Decachlorobiphenyl

R.T.: 10.911 min
Delta R.T.: -0.007 min
Response: 748978
Conc: 22.00 ng/ml

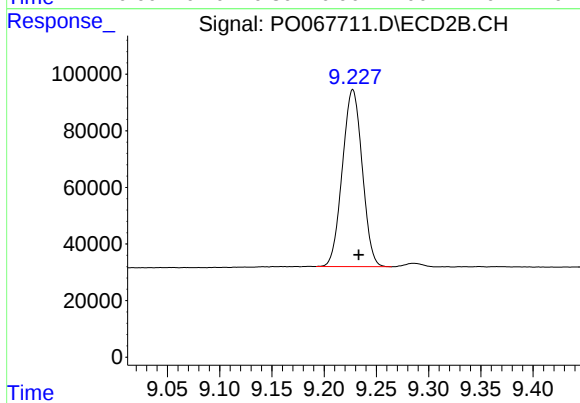

#2 Decachlorobiphenyl


R.T.: 9.227 min
Delta R.T.: -0.006 min
Response: 826820
Conc: 20.00 ng/ml

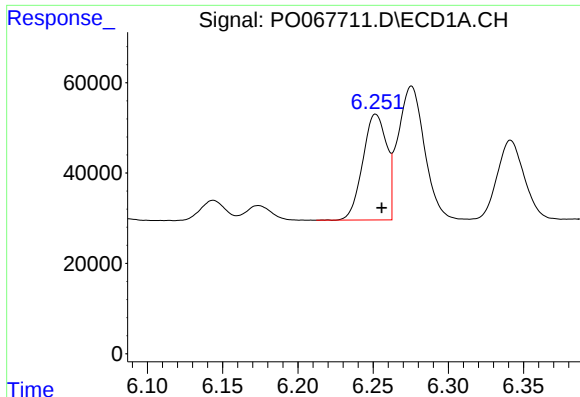

#3 AR-1016-1


R.T.: 6.252 min
Delta R.T.: -0.004 min
Response: 258540
Conc: 250.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

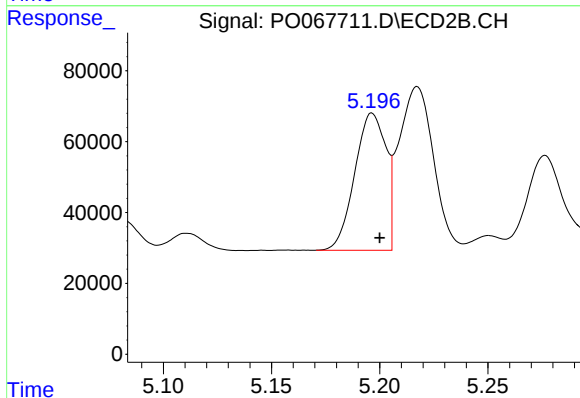


#3 AR-1016-1

R.T.: 5.197 min
Delta R.T.: -0.003 min
Response: 387912
Conc: 264.62 ng/ml

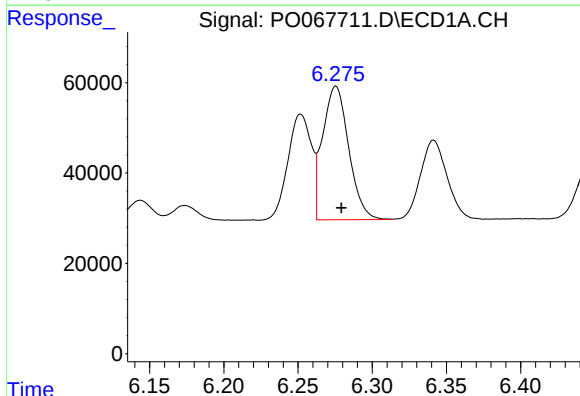


#4 AR-1016-2

R.T.: 6.275 min
Delta R.T.: -0.004 min
Response: 362285
Conc: 256.77 ng/ml

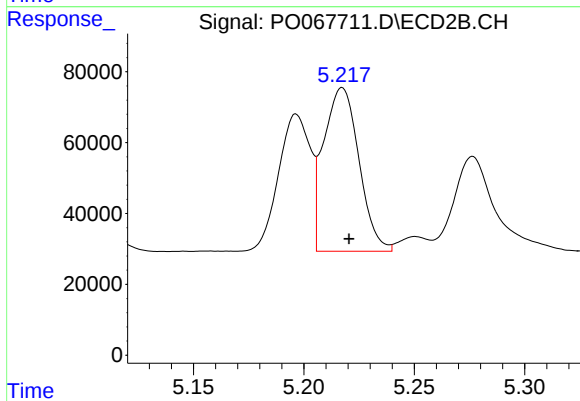

#4 AR-1016-2


R.T.: 5.217 min
Delta R.T.: -0.003 min
Response: 515062
Conc: 262.92 ng/ml

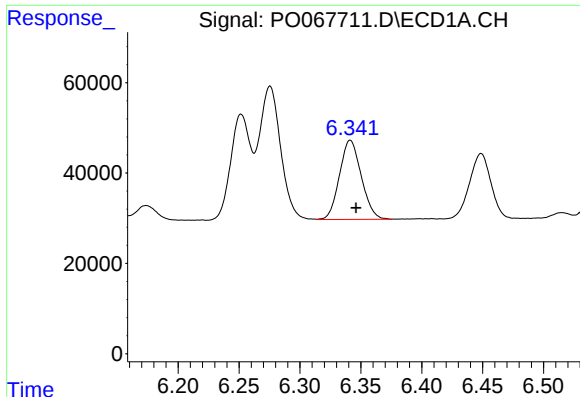

#5 AR-1016-3


R.T.: 6.341 min
Delta R.T.: -0.005 min
Response: 218720
Conc: 248.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

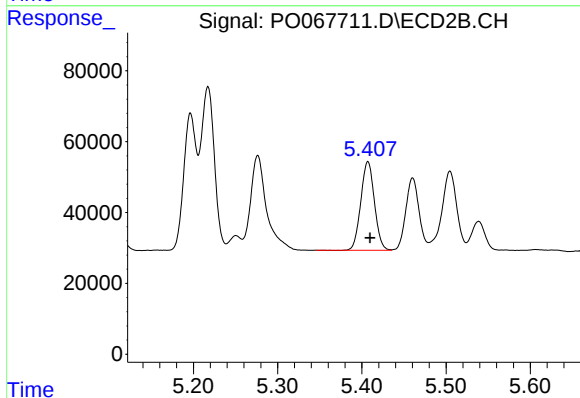


#5 AR-1016-3

R.T.: 5.407 min
Delta R.T.: -0.003 min
Response: 281891
Conc: 269.53 ng/ml

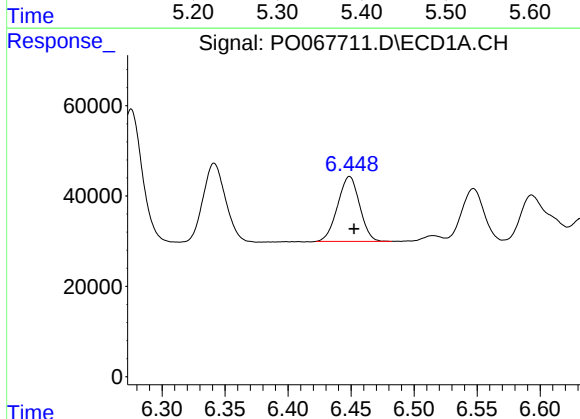


#6 AR-1016-4

R.T.: 6.449 min
Delta R.T.: -0.003 min
Response: 174302
Conc: 247.18 ng/ml

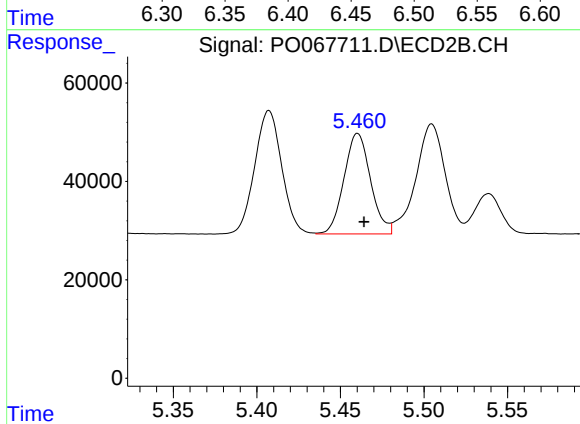

#6 AR-1016-4


R.T.: 5.460 min
Delta R.T.: -0.004 min
Response: 226091
Conc: 253.44 ng/ml

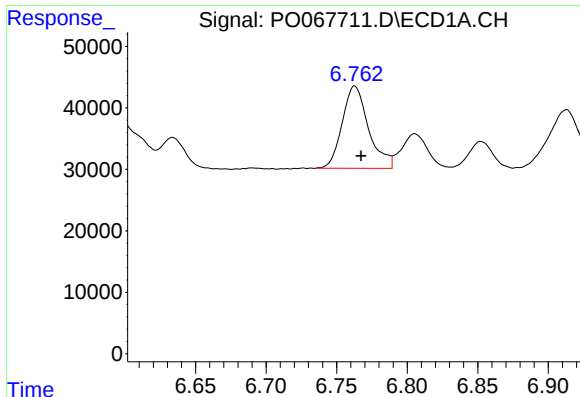

#7 AR-1016-5


R.T.: 6.763 min
Delta R.T.: -0.004 min
Response: 174260
Conc: 242.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

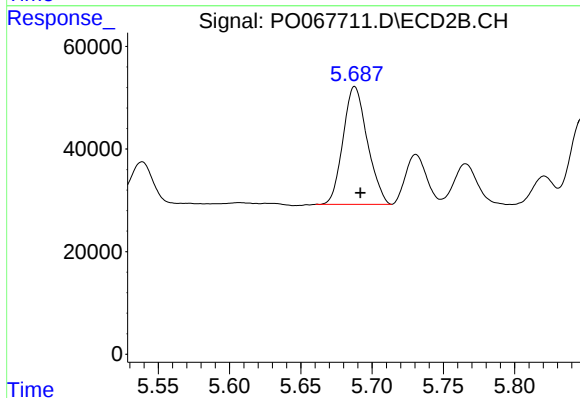


#7 AR-1016-5

R.T.: 5.688 min
Delta R.T.: -0.004 min
Response: 271813
Conc: 240.20 ng/ml

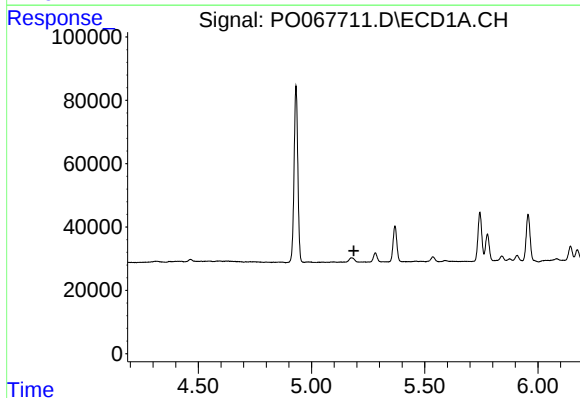


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 5.187 min
Response: 0
Conc: N.D.

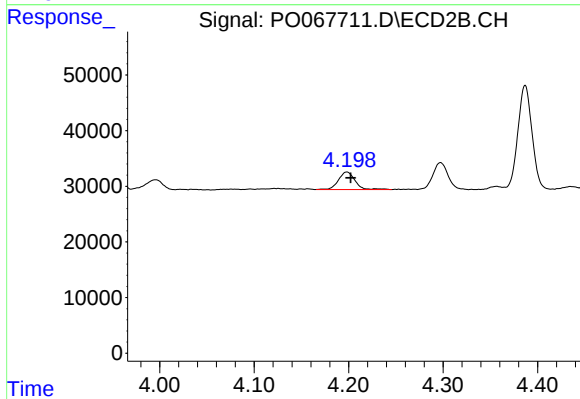

#8 AR-1221-1


R.T.: 4.198 min
Delta R.T.: -0.004 min
Response: 38392
Conc: 86.40 ng/ml

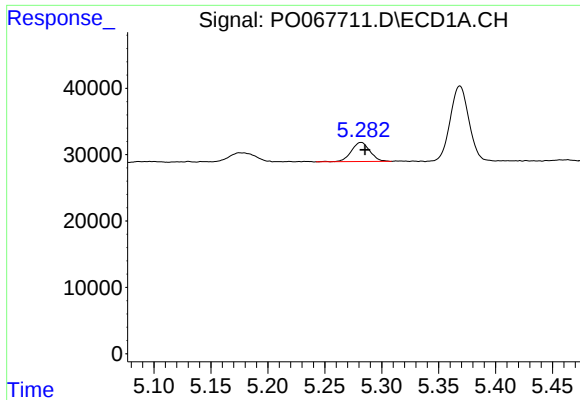

#9 AR-1221-2


R.T.: 5.282 min
Delta R.T.: -0.004 min
Response: 33031
Conc: 142.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

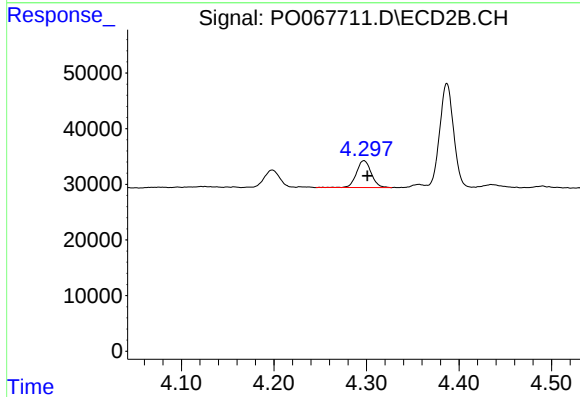


#9 AR-1221-2

R.T.: 4.297 min
Delta R.T.: -0.004 min
Response: 53953
Conc: 171.08 ng/ml

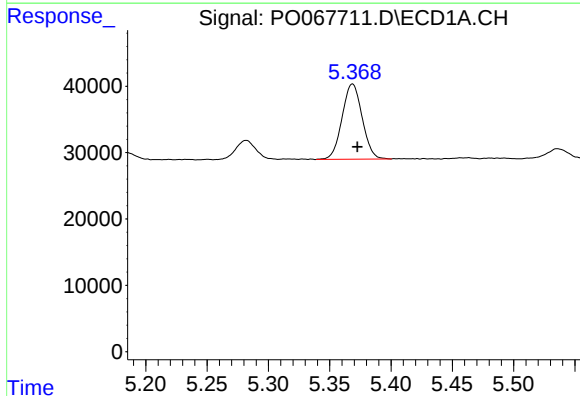


#10 AR-1221-3

R.T.: 5.369 min
Delta R.T.: -0.004 min
Response: 129380
Conc: 172.21 ng/ml

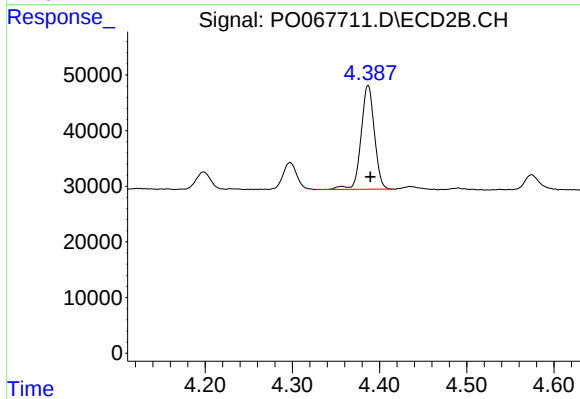

#10 AR-1221-3


R.T.: 4.387 min
Delta R.T.: -0.003 min
Response: 199028
Conc: 202.73 ng/ml

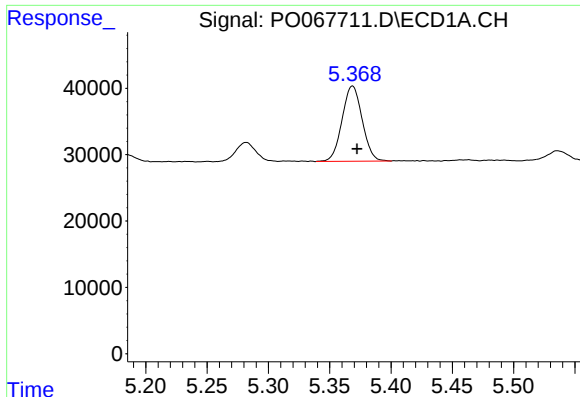

#11 AR-1232-1


R.T.: 5.369 min
Delta R.T.: -0.004 min
Response: 129380
Conc: 251.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

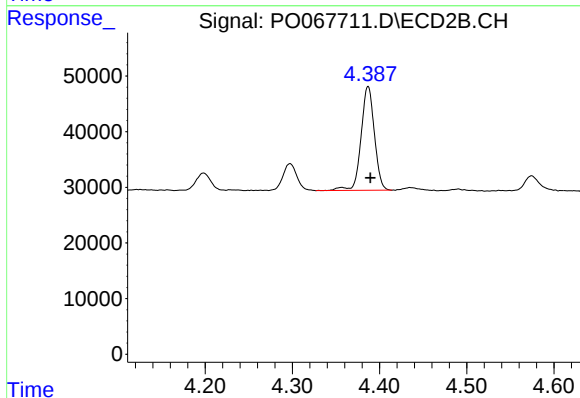


#11 AR-1232-1

R.T.: 4.387 min
Delta R.T.: -0.003 min
Response: 199028
Conc: 287.58 ng/ml

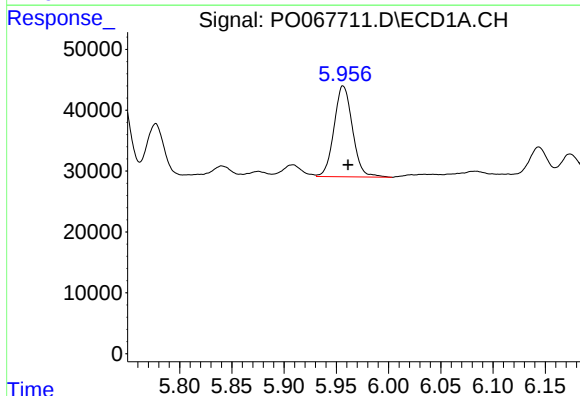


#12 AR-1232-2

R.T.: 5.957 min
Delta R.T.: -0.005 min
Response: 183073
Conc: 682.40 ng/ml

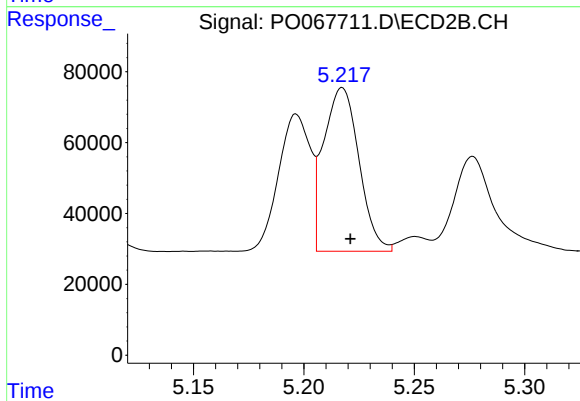

#12 AR-1232-2


R.T.: 5.217 min
Delta R.T.: -0.004 min
Response: 515062
Conc: 710.07 ng/ml

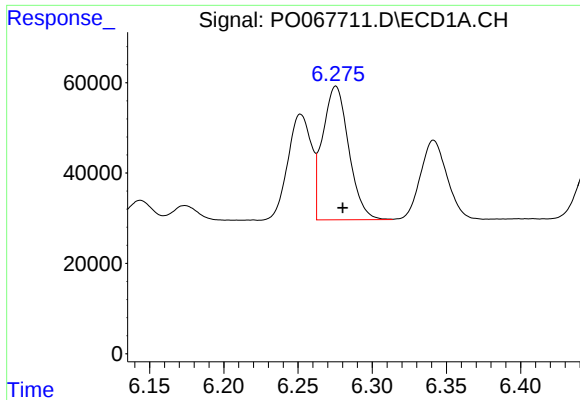

#13 AR-1232-3


R.T.: 6.275 min
Delta R.T.: -0.005 min
Response: 362285
Conc: 691.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

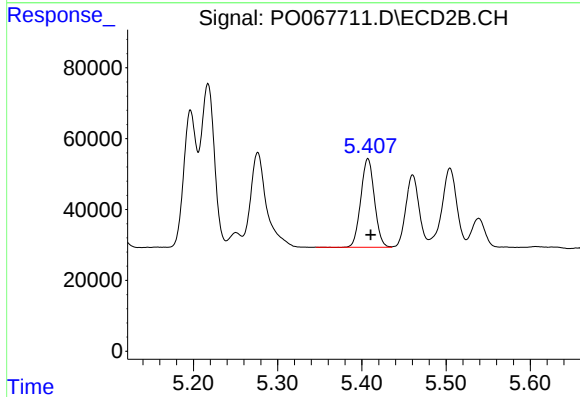


#13 AR-1232-3

R.T.: 5.407 min
Delta R.T.: -0.003 min
Response: 281891
Conc: 731.31 ng/ml

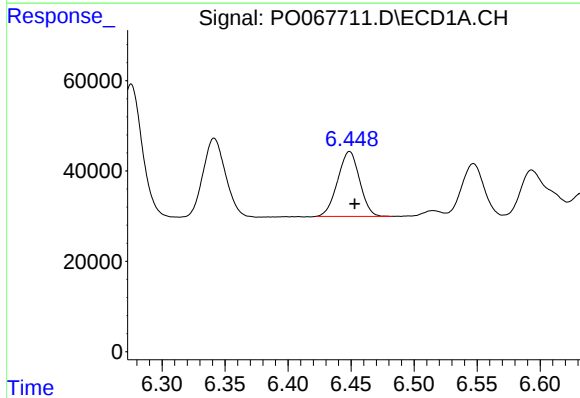


#14 AR-1232-4

R.T.: 6.449 min
Delta R.T.: -0.004 min
Response: 174302
Conc: 678.02 ng/ml

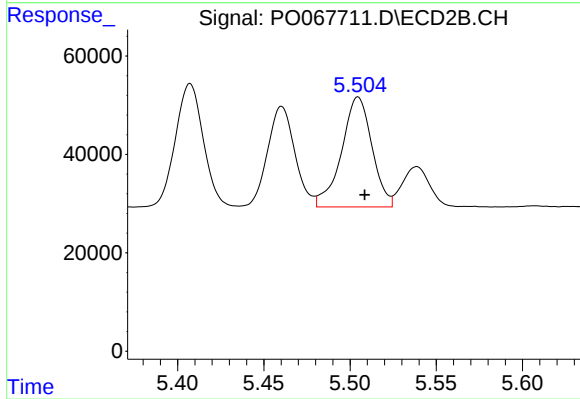

#14 AR-1232-4


R.T.: 5.505 min
Delta R.T.: -0.004 min
Response: 274425
Conc: 775.72 ng/ml

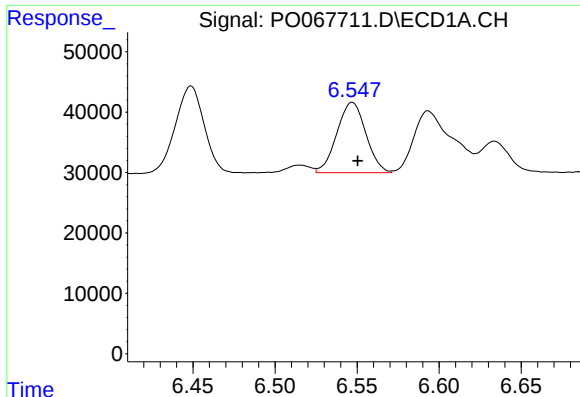

#15 AR-1232-5


R.T.: 6.547 min
Delta R.T.: -0.003 min
Response: 143582
Conc: 766.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

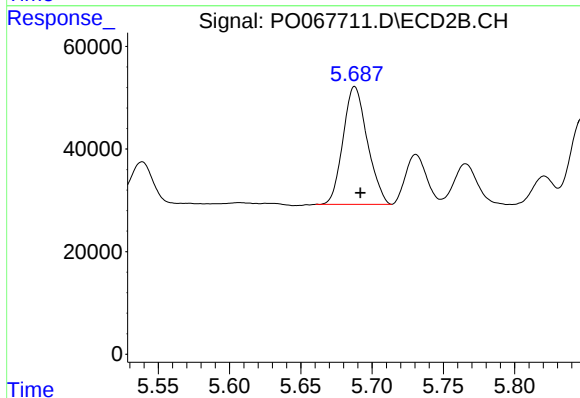


#15 AR-1232-5

R.T.: 5.688 min
Delta R.T.: -0.004 min
Response: 271813
Conc: 711.30 ng/ml

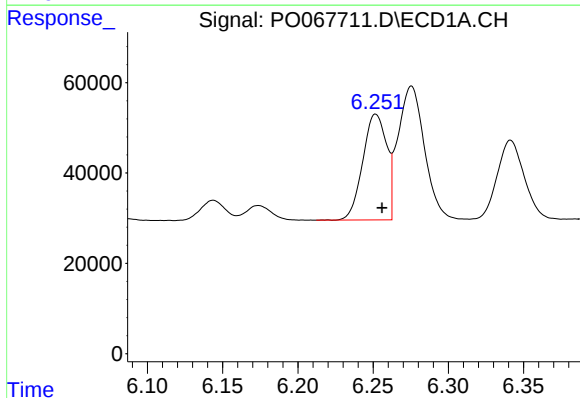


#16 AR-1242-1

R.T.: 6.252 min
Delta R.T.: -0.004 min
Response: 258540
Conc: 376.57 ng/ml

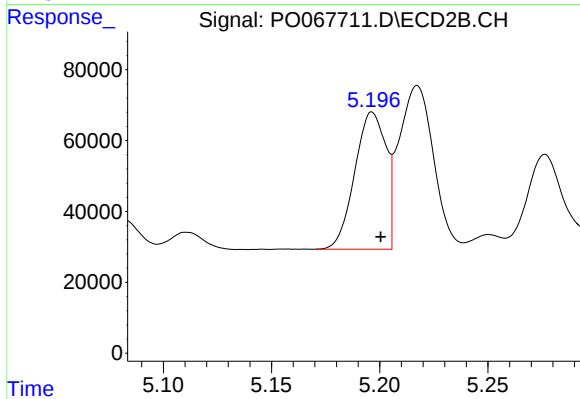

#16 AR-1242-1


R.T.: 5.197 min
Delta R.T.: -0.004 min
Response: 387912
Conc: 395.36 ng/ml

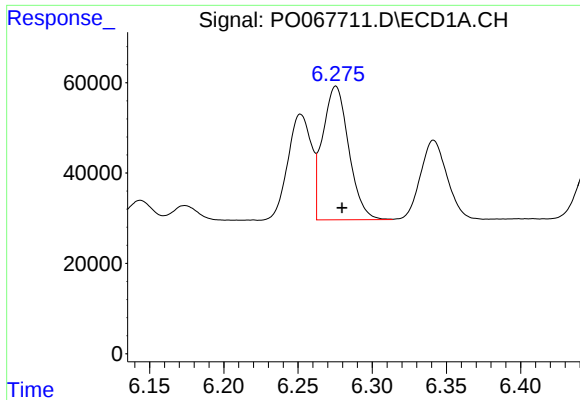

#17 AR-1242-2


R.T.: 6.275 min
Delta R.T.: -0.004 min
Response: 362285
Conc: 385.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

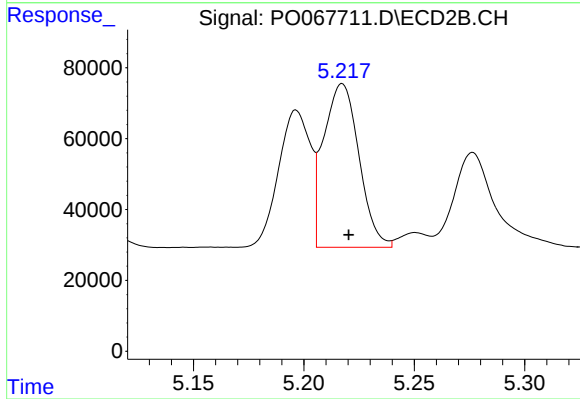


#17 AR-1242-2

R.T.: 5.217 min
Delta R.T.: -0.003 min
Response: 515062
Conc: 395.29 ng/ml

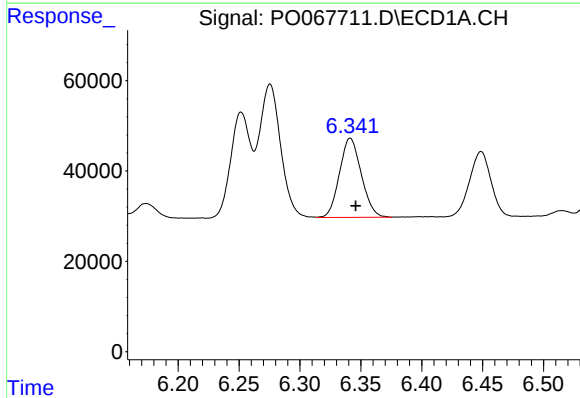


#18 AR-1242-3

R.T.: 6.341 min
Delta R.T.: -0.004 min
Response: 218720
Conc: 373.23 ng/ml

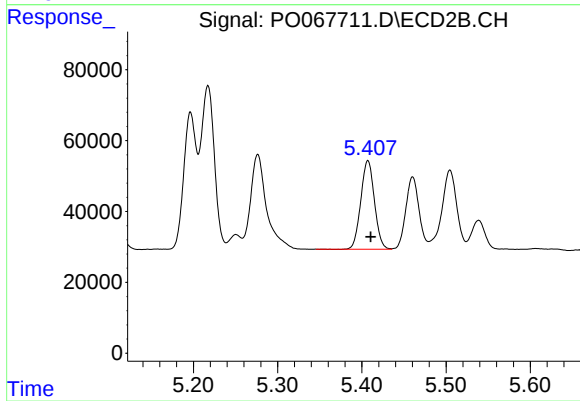

#18 AR-1242-3


R.T.: 5.407 min
Delta R.T.: -0.003 min
Response: 281891
Conc: 394.21 ng/ml

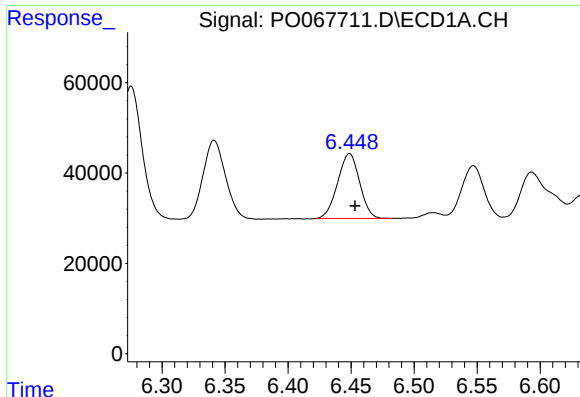

#19 AR-1242-4


R.T.: 6.449 min
Delta R.T.: -0.004 min
Response: 174302
Conc: 370.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

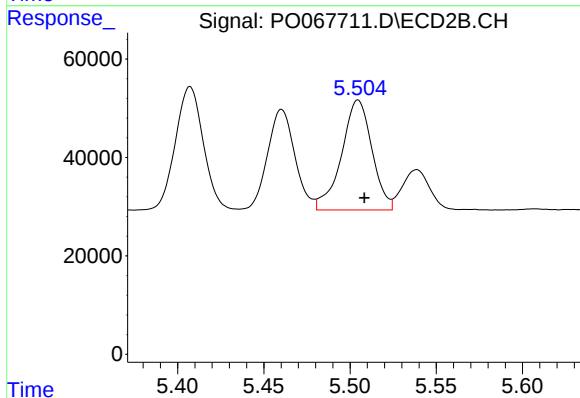


#19 AR-1242-4

R.T.: 5.505 min
Delta R.T.: -0.004 min
Response: 274425
Conc: 381.25 ng/ml

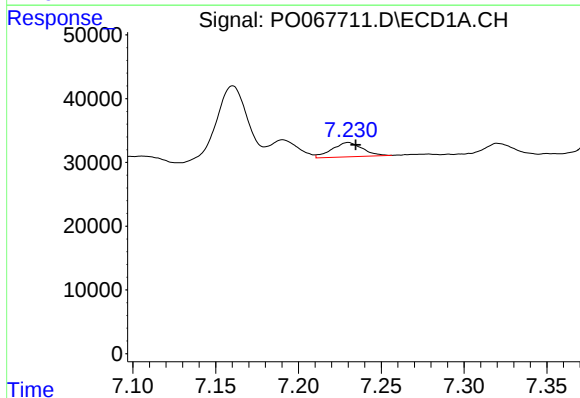


#20 AR-1242-5

R.T.: 7.230 min
Delta R.T.: -0.005 min
Response: 28691
Conc: 53.71 ng/ml

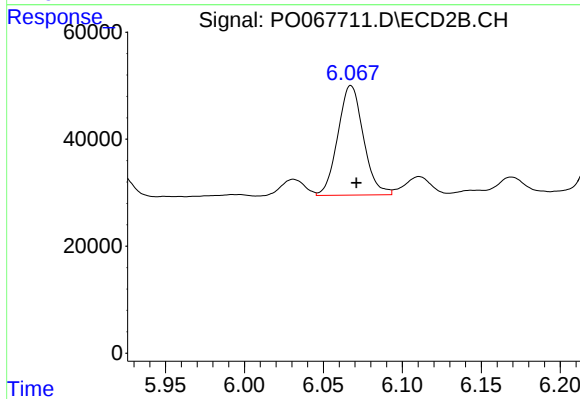

#20 AR-1242-5


R.T.: 6.067 min
Delta R.T.: -0.003 min
Response: 230559
Conc: 246.39 ng/ml

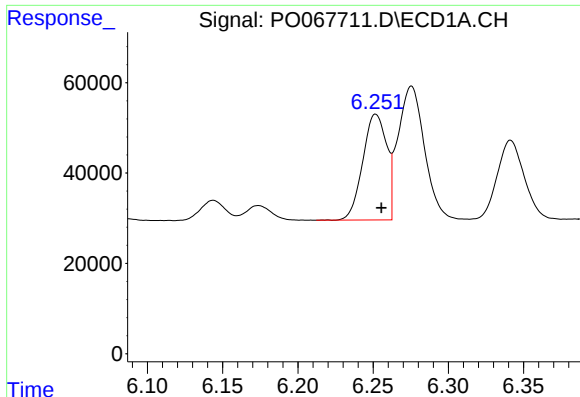

#21 AR-1248-1


R.T.: 6.252 min
Delta R.T.: -0.004 min
Response: 258540
Conc: 481.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

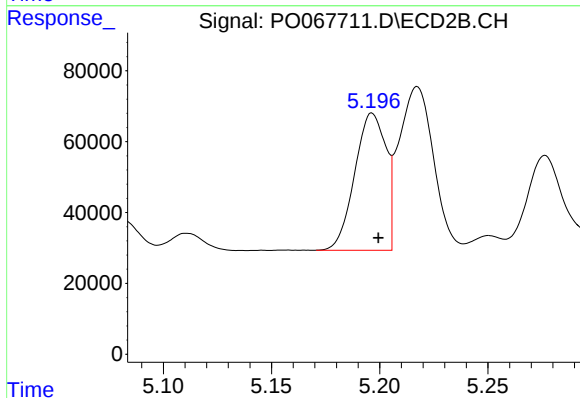


#21 AR-1248-1

R.T.: 5.197 min
Delta R.T.: -0.003 min
Response: 387912
Conc: 496.55 ng/ml

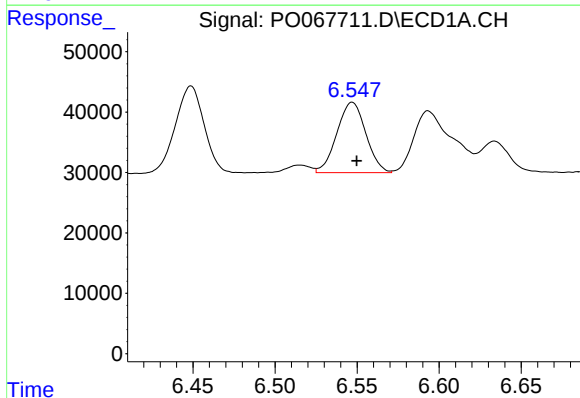


#22 AR-1248-2

R.T.: 6.547 min
Delta R.T.: -0.003 min
Response: 143582
Conc: 204.07 ng/ml

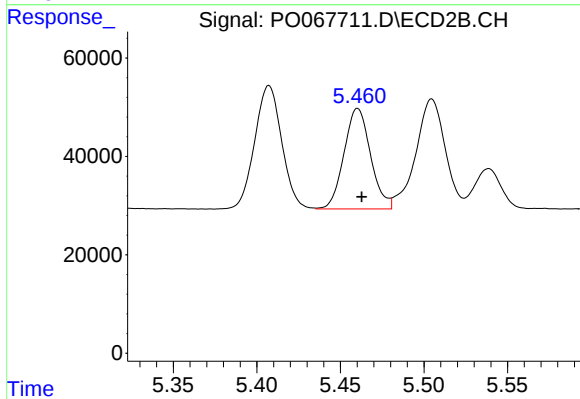

#22 AR-1248-2


R.T.: 5.460 min
Delta R.T.: -0.002 min
Response: 226091
Conc: 224.69 ng/ml

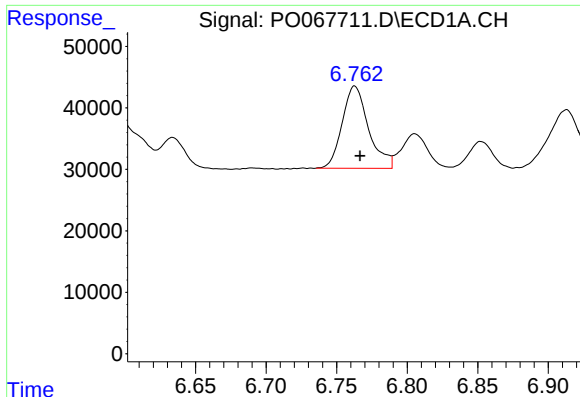

#23 AR-1248-3


R.T.: 6.763 min
Delta R.T.: -0.004 min
Response: 174260
Conc: 214.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

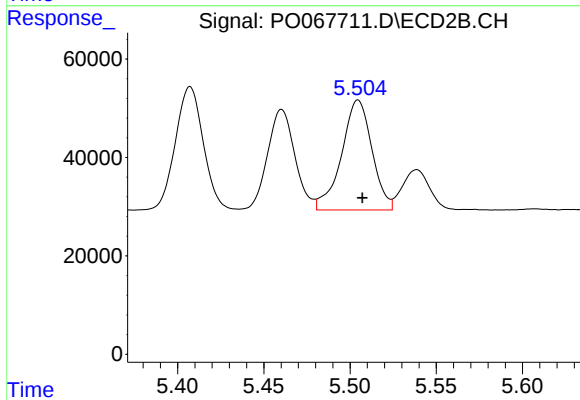


#23 AR-1248-3

R.T.: 5.505 min
Delta R.T.: -0.003 min
Response: 274425
Conc: 268.30 ng/ml

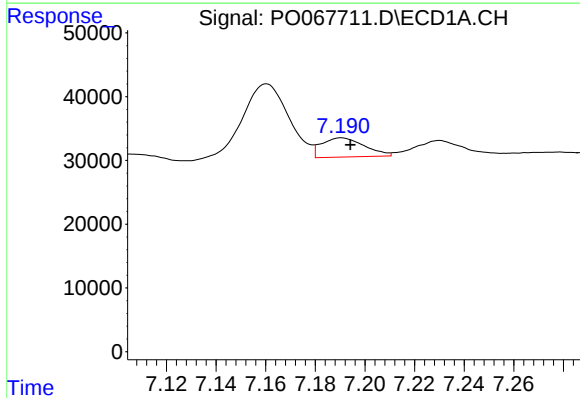


#24 AR-1248-4

R.T.: 7.191 min
Delta R.T.: -0.004 min
Response: 36113
Conc: 38.28 ng/ml

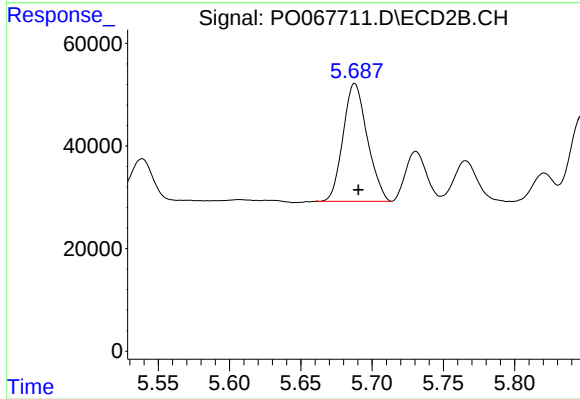

#24 AR-1248-4


R.T.: 5.688 min
Delta R.T.: -0.003 min
Response: 271813
Conc: 218.10 ng/ml

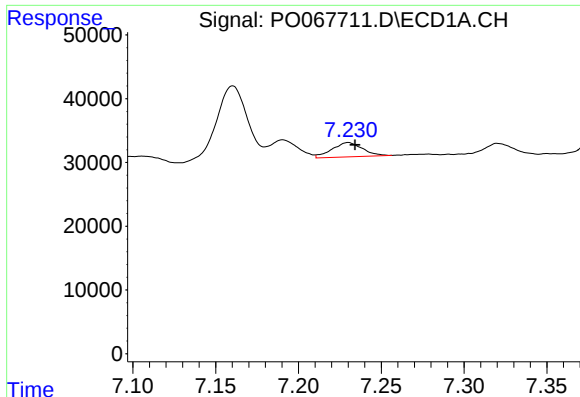

#25 AR-1248-5


R.T.: 7.230 min
Delta R.T.: -0.004 min
Response: 28691
Conc: 31.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

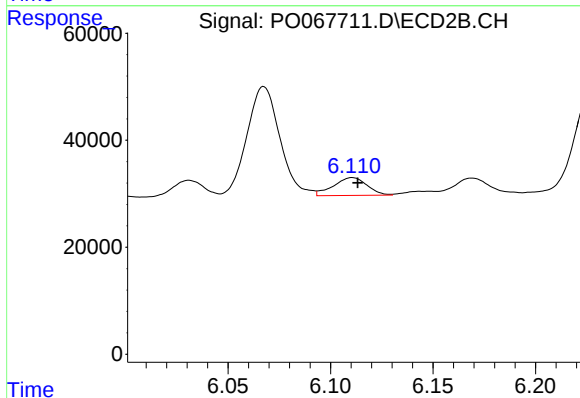


#25 AR-1248-5

R.T.: 6.111 min
Delta R.T.: -0.003 min
Response: 38030
Conc: 30.73 ng/ml

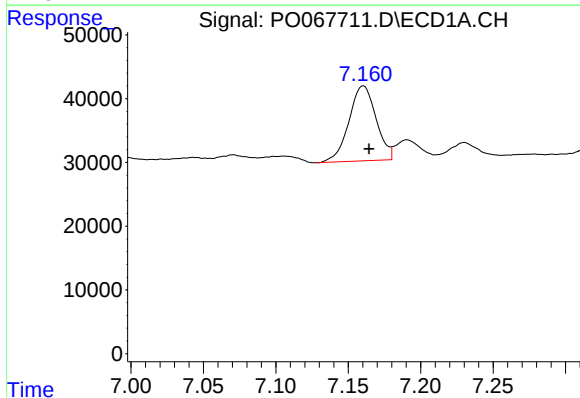


#26 AR-1254-1

R.T.: 7.160 min
Delta R.T.: -0.004 min
Response: 153850
Conc: 124.56 ng/ml

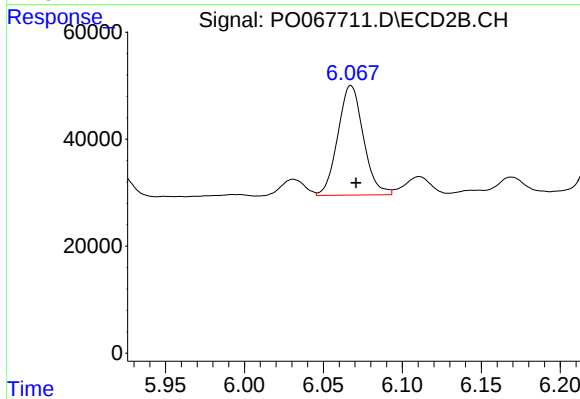

#26 AR-1254-1


R.T.: 6.067 min
Delta R.T.: -0.003 min
Response: 230559
Conc: 89.92 ng/ml

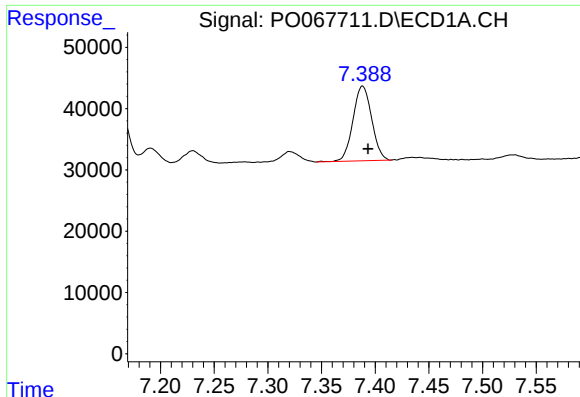

#27 AR-1254-2


R.T.: 7.388 min
Delta R.T.: -0.005 min
Response: 147632
Conc: 75.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

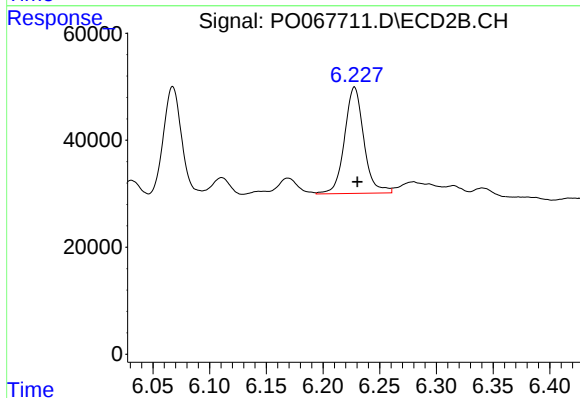


#27 AR-1254-2

R.T.: 6.228 min
Delta R.T.: -0.003 min
Response: 236017
Conc: 103.49 ng/ml

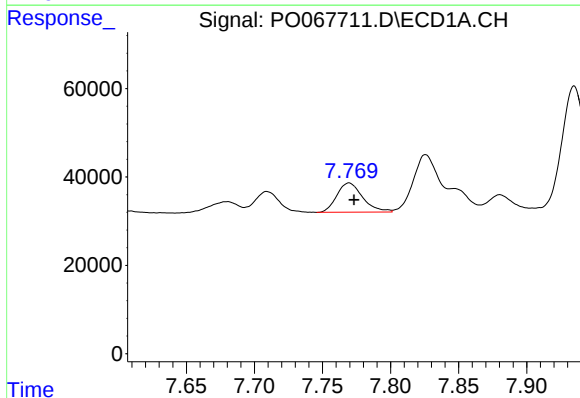


#28 AR-1254-3

R.T.: 7.770 min
Delta R.T.: -0.004 min
Response: 87792
Conc: 42.31 ng/ml

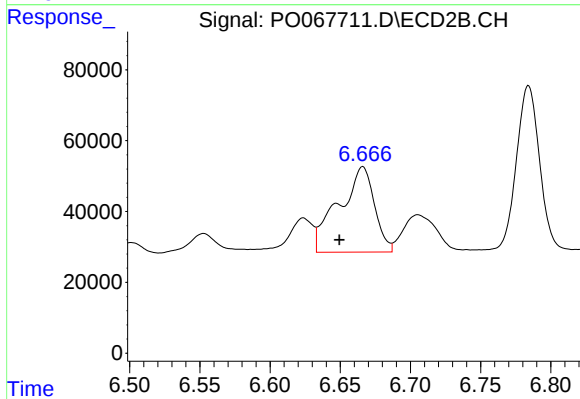

#28 AR-1254-3


R.T.: 6.666 min
Delta R.T.: 0.017 min
Response: 427511
Conc: 117.09 ng/ml

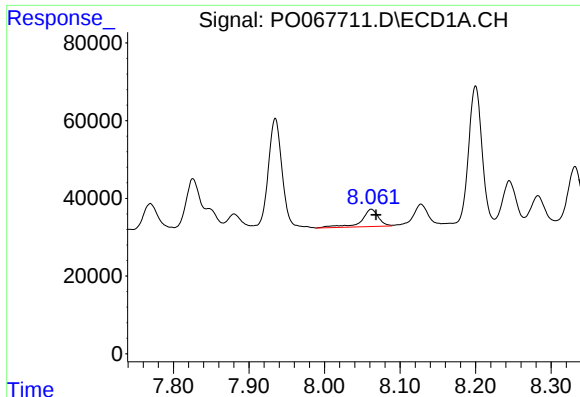

#29 AR-1254-4


R.T.: 8.062 min
Delta R.T.: -0.006 min
Response: 70370
Conc: 43.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

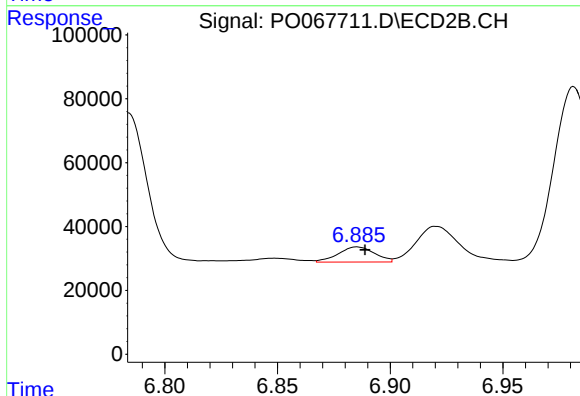


#29 AR-1254-4

R.T.: 6.886 min
Delta R.T.: -0.003 min
Response: 52841
Conc: 21.92 ng/ml

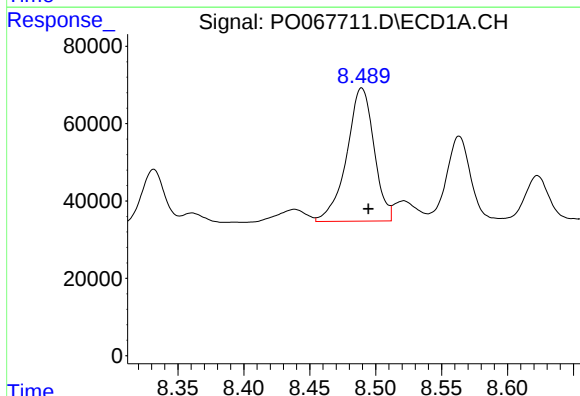


#30 AR-1254-5

R.T.: 8.489 min
Delta R.T.: -0.005 min
Response: 496972
Conc: 289.66 ng/ml

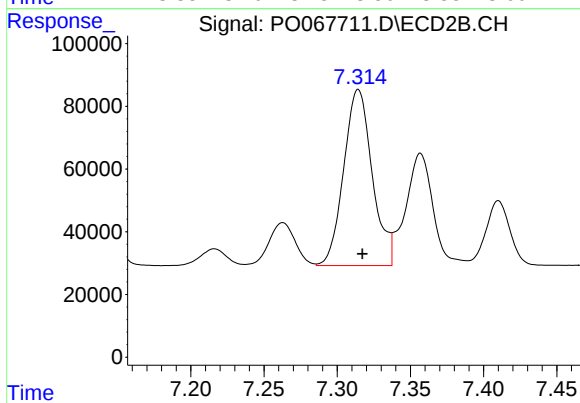

#30 AR-1254-5


R.T.: 7.314 min
Delta R.T.: -0.003 min
Response: 761517
Conc: 228.15 ng/ml

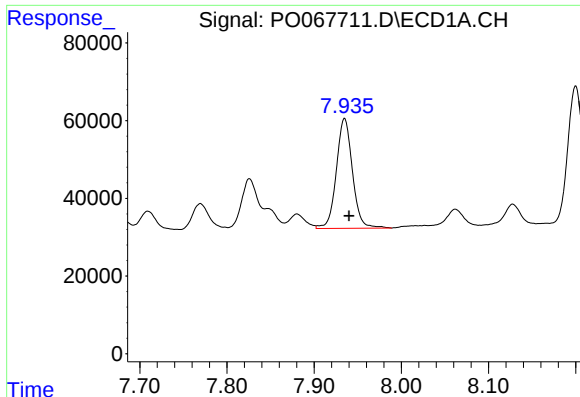

#31 AR-1260-1


R.T.: 7.935 min
Delta R.T.: -0.005 min
Response: 363192
Conc: 268.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

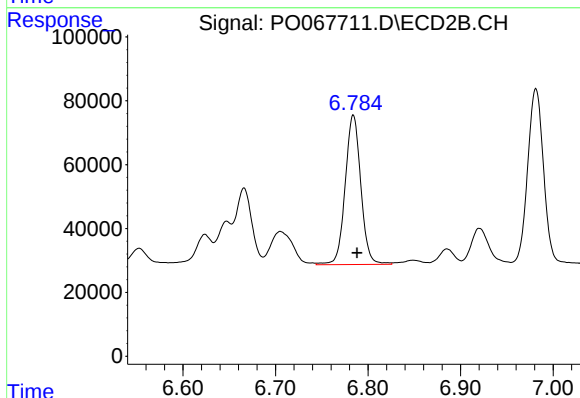


#31 AR-1260-1

R.T.: 6.784 min
Delta R.T.: -0.004 min
Response: 550229
Conc: 262.46 ng/ml

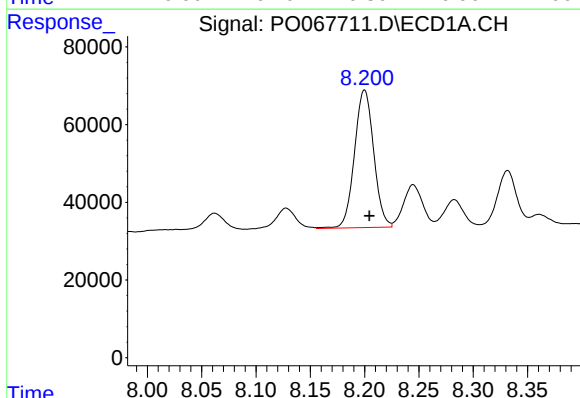


#32 AR-1260-2

R.T.: 8.200 min
Delta R.T.: -0.005 min
Response: 436925
Conc: 258.82 ng/ml

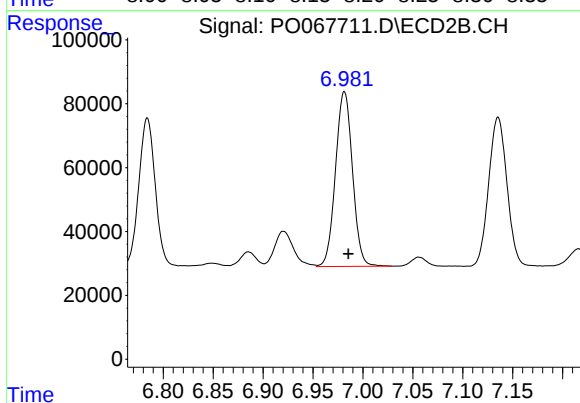

#32 AR-1260-2


R.T.: 6.981 min
Delta R.T.: -0.004 min
Response: 648505
Conc: 252.56 ng/ml

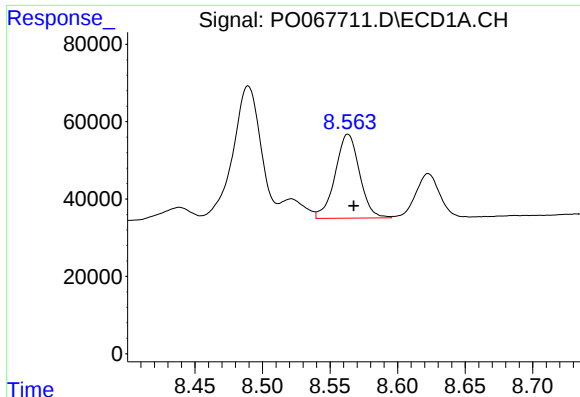

#33 AR-1260-3


R.T.: 8.563 min
Delta R.T.: -0.004 min
Response: 272593
Conc: 209.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

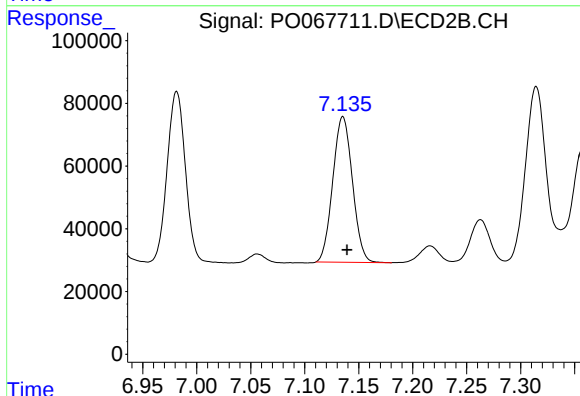


#33 AR-1260-3

R.T.: 7.135 min
Delta R.T.: -0.004 min
Response: 586883
Conc: 244.06 ng/ml

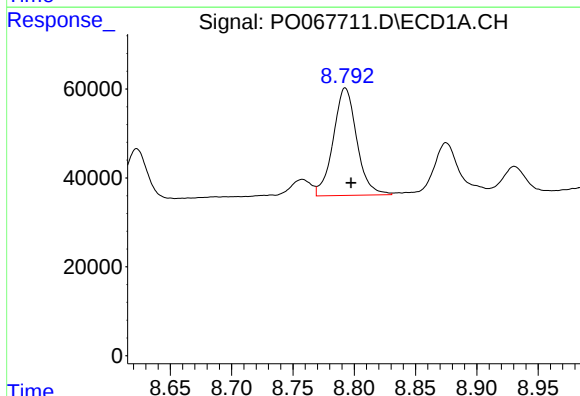


#34 AR-1260-4

R.T.: 8.793 min
Delta R.T.: -0.005 min
Response: 323229
Conc: 210.33 ng/ml

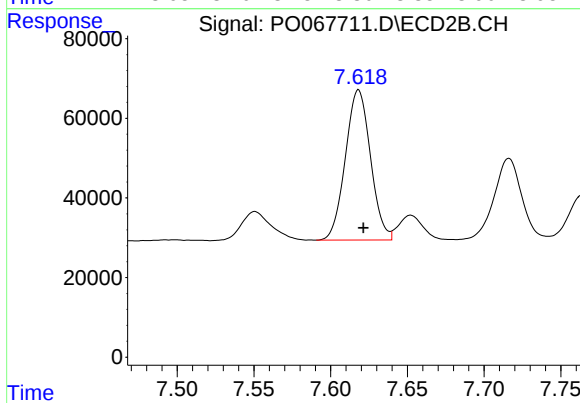

#34 AR-1260-4


R.T.: 7.618 min
Delta R.T.: -0.003 min
Response: 431704
Conc: 205.41 ng/ml

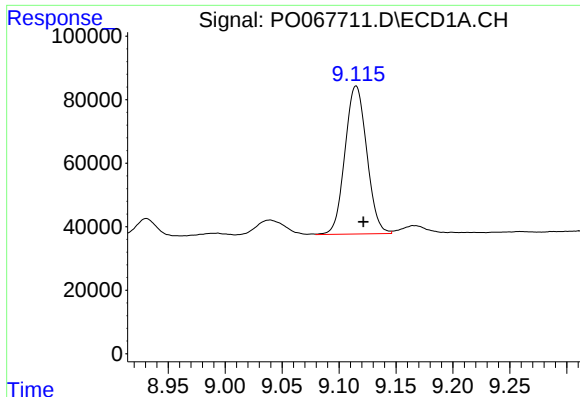

#35 AR-1260-5


R.T.: 9.115 min
Delta R.T.: -0.006 min
Response: 621687
Conc: 197.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

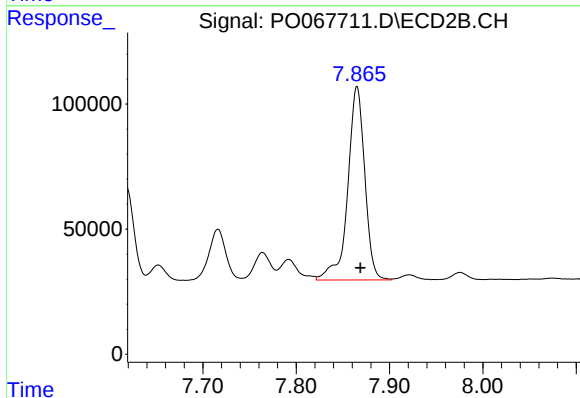


#35 AR-1260-5

R.T.: 7.865 min
Delta R.T.: -0.004 min
Response: 981827
Conc: 193.94 ng/ml

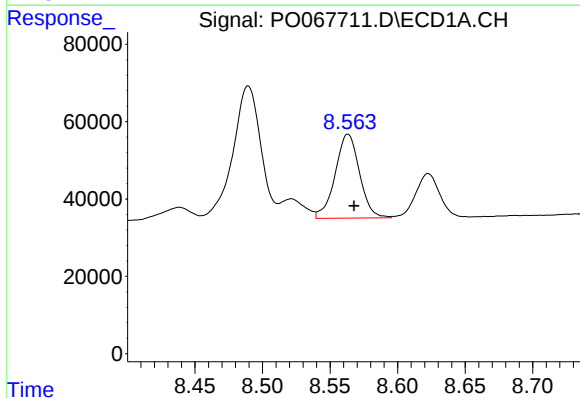


#36 AR-1262-1

R.T.: 8.563 min
Delta R.T.: -0.005 min
Response: 272593
Conc: 162.60 ng/ml

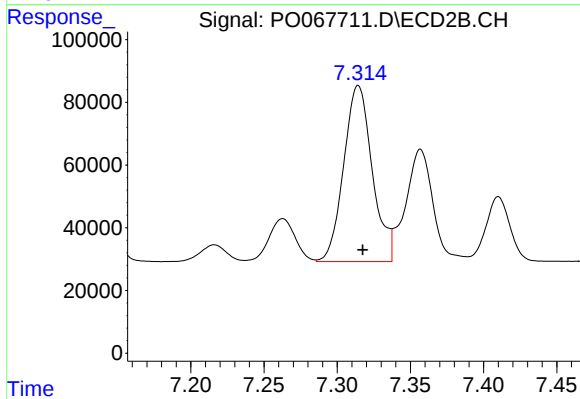

#36 AR-1262-1


R.T.: 7.314 min
Delta R.T.: -0.003 min
Response: 761517
Conc: 549.55 ng/ml

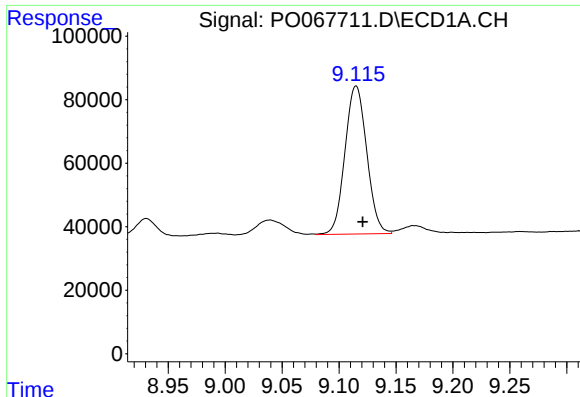

#37 AR-1262-2


R.T.: 9.115 min
Delta R.T.: -0.006 min
Response: 621687
Conc: 216.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

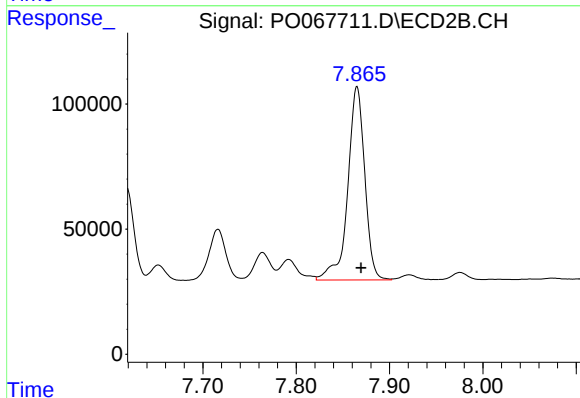


#37 AR-1262-2

R.T.: 7.865 min
Delta R.T.: -0.004 min
Response: 981827
Conc: 214.74 ng/ml

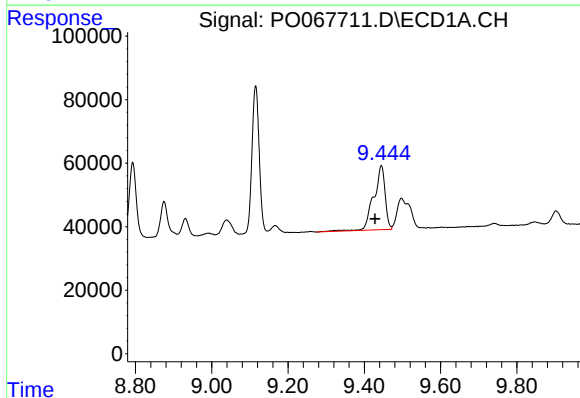


#38 AR-1262-3

R.T.: 9.445 min
Delta R.T.: 0.017 min
Response: 423230
Conc: 203.39 ng/ml

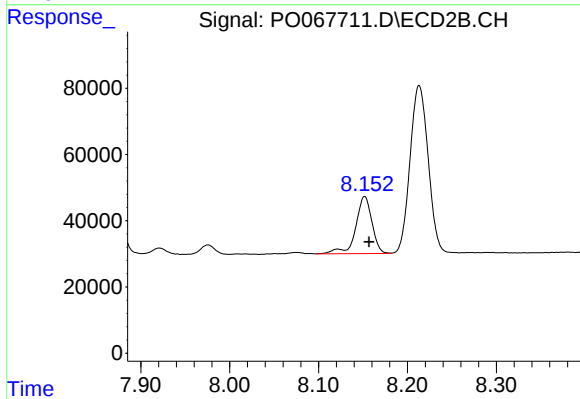

#38 AR-1262-3


R.T.: 8.152 min
Delta R.T.: -0.005 min
Response: 219042
Conc: 111.45 ng/ml

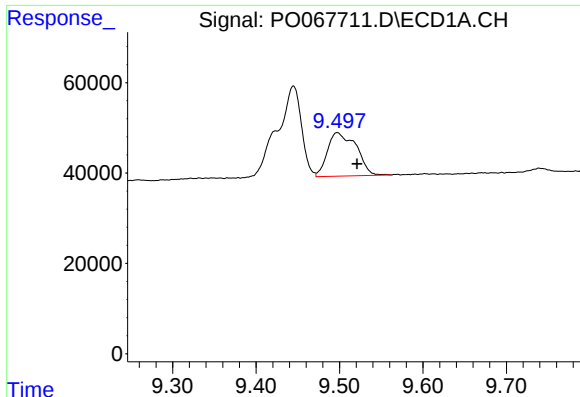

#39 AR-1262-4


R.T.: 9.497 min
Delta R.T.: -0.024 min
Response: 230860
Conc: 145.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

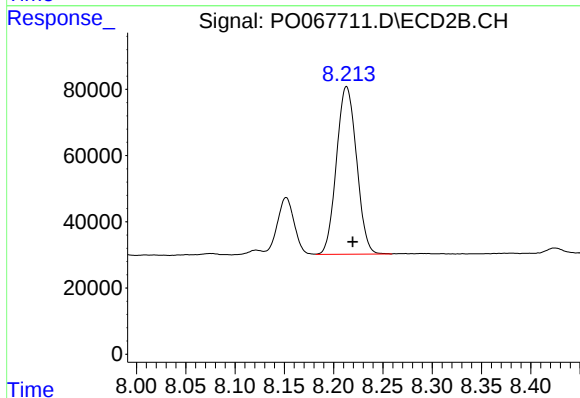


#39 AR-1262-4

R.T.: 8.213 min
Delta R.T.: -0.006 min
Response: 717418
Conc: 209.28 ng/ml

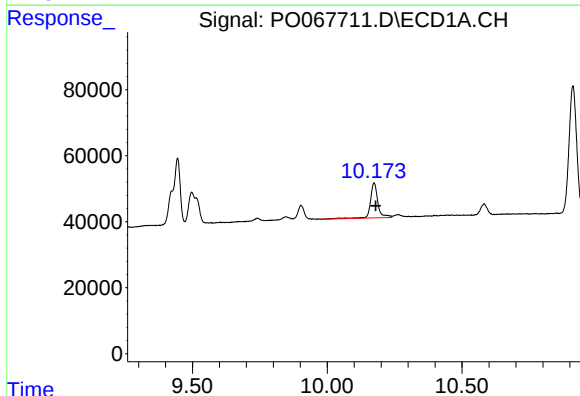


#40 AR-1262-5

R.T.: 10.174 min
Delta R.T.: -0.006 min
Response: 204321
Conc: 173.29 ng/ml

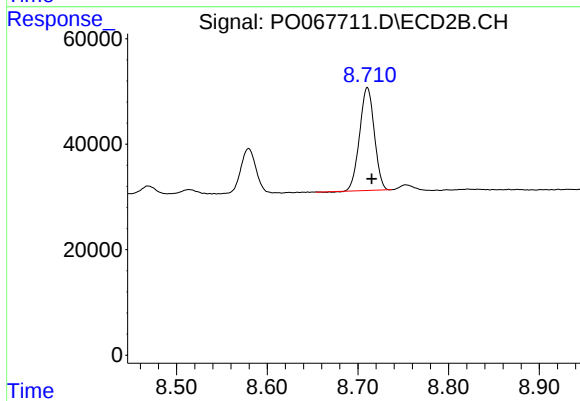

#40 AR-1262-5


R.T.: 8.710 min
Delta R.T.: -0.005 min
Response: 219416
Conc: 129.08 ng/ml

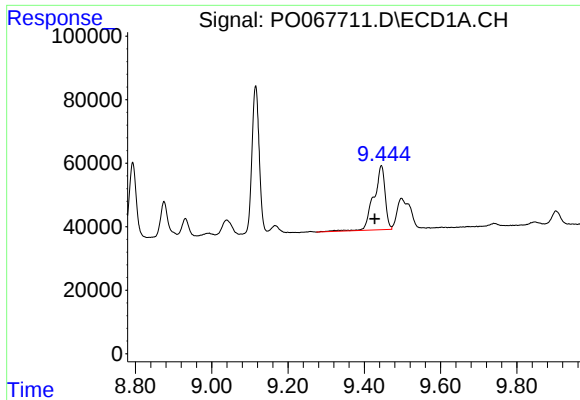

#41 AR-1268-1


R.T.: 9.445 min
Delta R.T.: 0.017 min
Response: 423230
Conc: 114.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

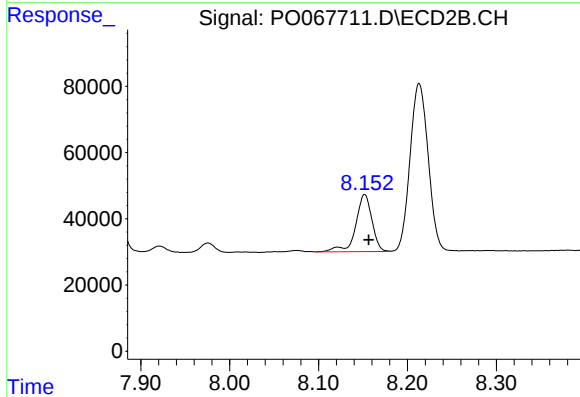


#41 AR-1268-1

R.T.: 8.152 min
Delta R.T.: -0.005 min
Response: 219042
Conc: 40.71 ng/ml

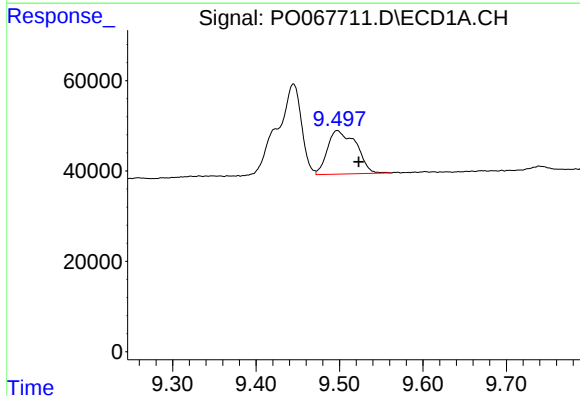


#42 AR-1268-2

R.T.: 9.497 min
Delta R.T.: -0.026 min
Response: 230860
Conc: 66.61 ng/ml

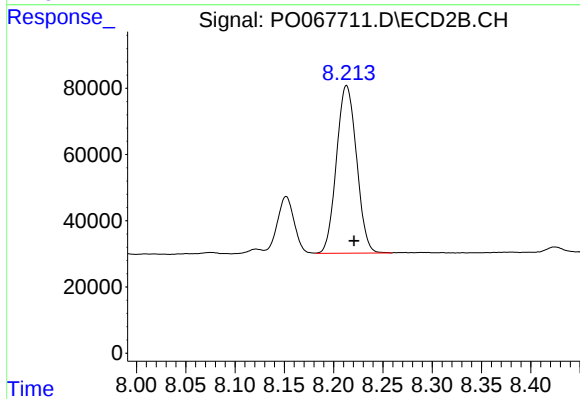

#42 AR-1268-2


R.T.: 8.213 min
Delta R.T.: -0.008 min
Response: 717418
Conc: 145.30 ng/ml

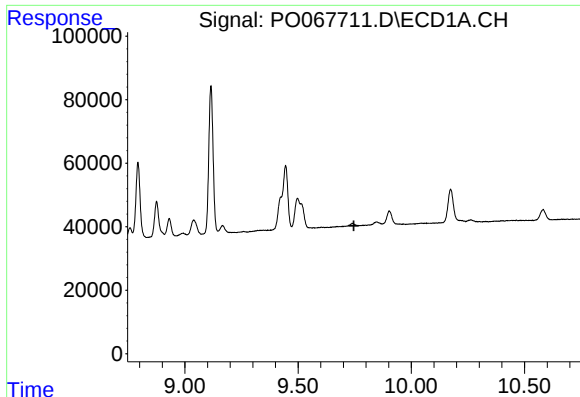

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.746 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

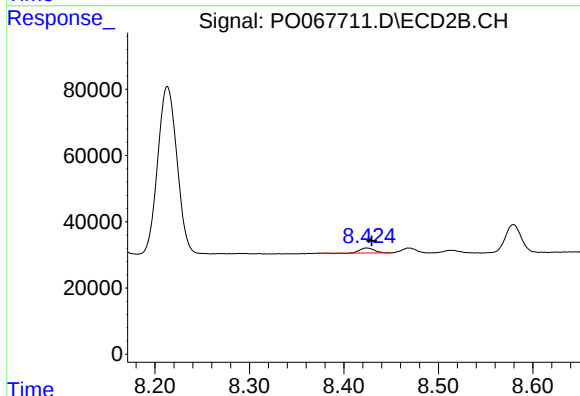


#43 AR-1268-3

R.T.: 8.425 min
Delta R.T.: -0.005 min
Response: 16034
Conc: 3.83 ng/ml

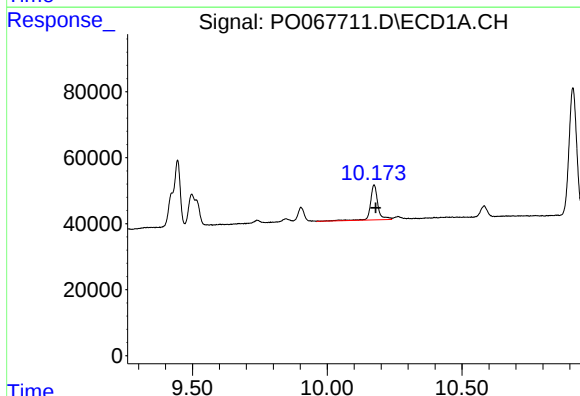


#44 AR-1268-4

R.T.: 10.174 min
Delta R.T.: -0.007 min
Response: 204321
Conc: 147.18 ng/ml

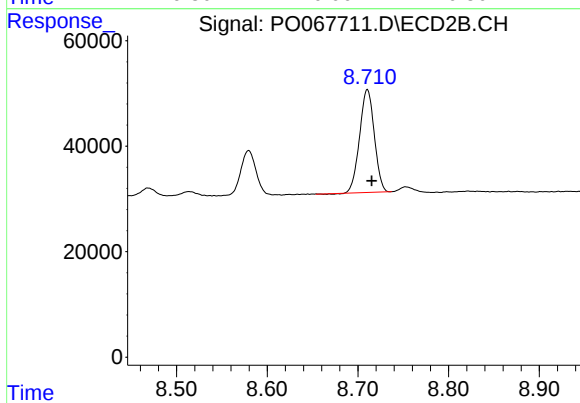

#44 AR-1268-4


R.T.: 8.710 min
Delta R.T.: -0.005 min
Response: 219416
Conc: 113.40 ng/ml

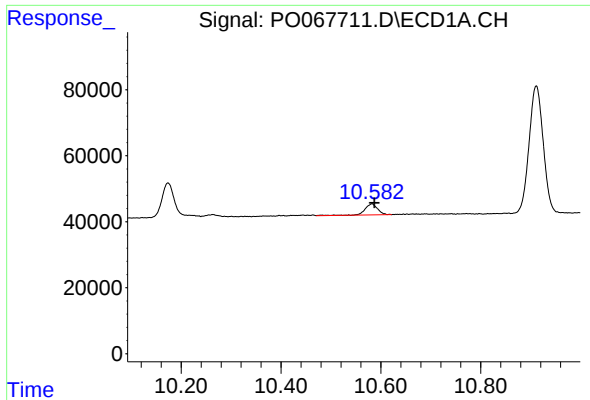

#45 AR-1268-5

R.T.: 10.582 min
Delta R.T.: -0.005 min
Response: 60533
Conc: 6.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-45-COMPMSD

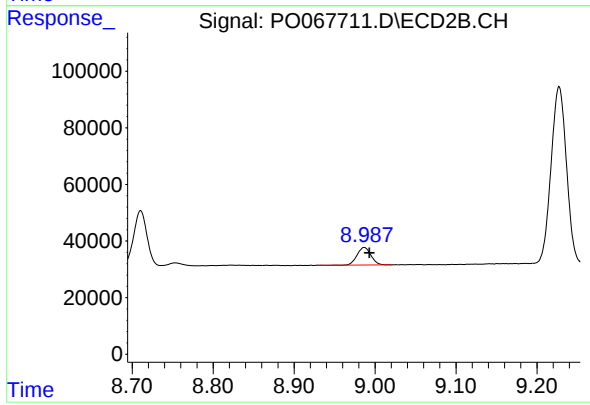

#45 AR-1268-5

R.T.: 8.987 min
Delta R.T.: -0.006 min
Response: 74330
Conc: 5.76 ng/ml