

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040720\
 Data File : P0067726.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Apr 2020 16:56
 Operator : DD\AJ
 Sample : L2151-02
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MH-720

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 17:54:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.932	3.943	509163	750318	21.381	22.386
2)	SA Decachlor...	10.912	9.228	613772	719737	18.029	17.408
Target Compounds							
32)	L7 AR-1260-2	8.218	0.000	24713	0	14.639	N.D. #
33)	L7 AR-1260-3	8.574	7.136	13186	72401	10.116	30.108 #
34)	L7 AR-1260-4	8.801	0.000	16154	0	10.511	N.D. #
35)	L7 AR-1260-5	9.121	0.000	33877	0	10.739	N.D. #
36)	L8 AR-1262-1	8.574	0.000	13186	0	7.865	N.D. #
37)	L8 AR-1262-2	9.121	0.000	33877	0	11.806	N.D. #
38)	L8 AR-1262-3	9.401	0.000	29347	0	14.103	N.D. #
41)	L9 AR-1268-1	9.401	0.000	29347	0	7.942	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040720\
Data File : P0067726.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Apr 2020 16:56
Operator : DD\AJ
Sample : L2151-02
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
MH-720

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 17:54:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

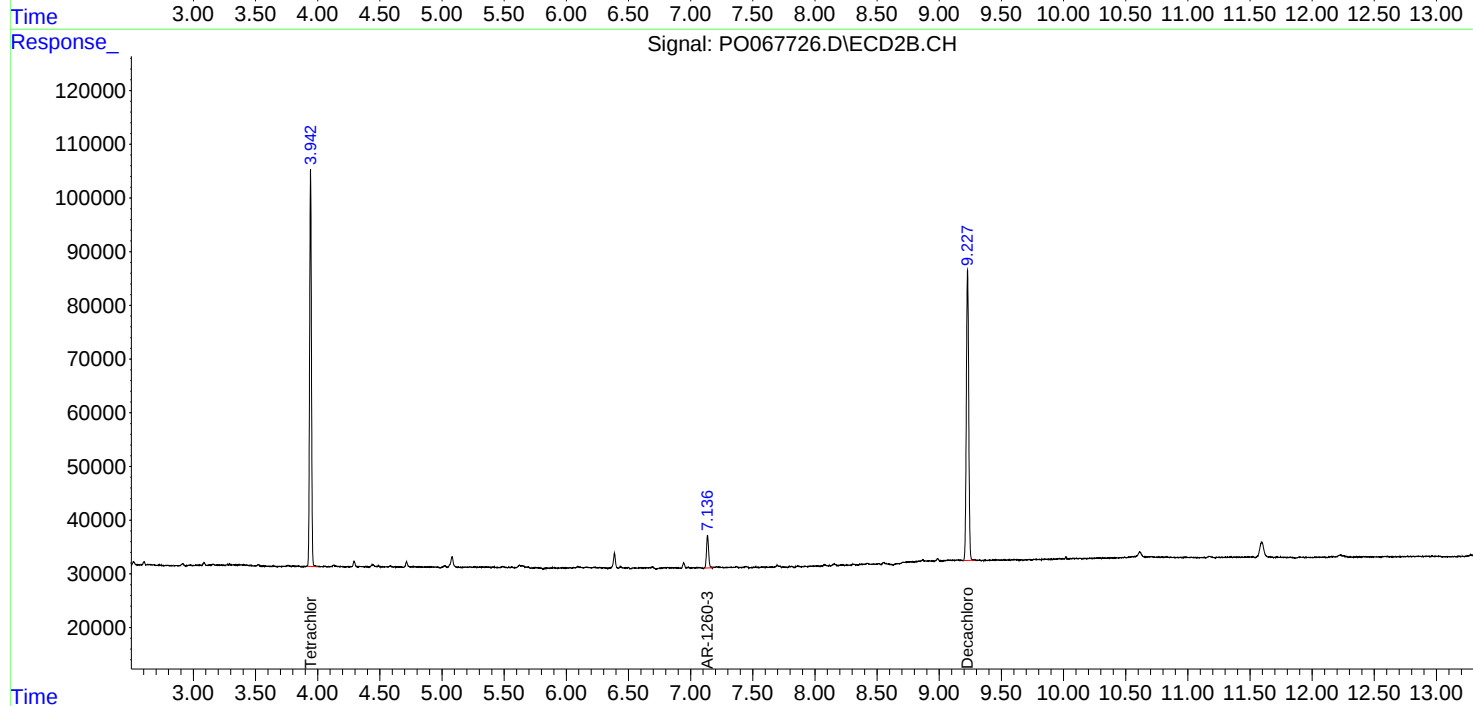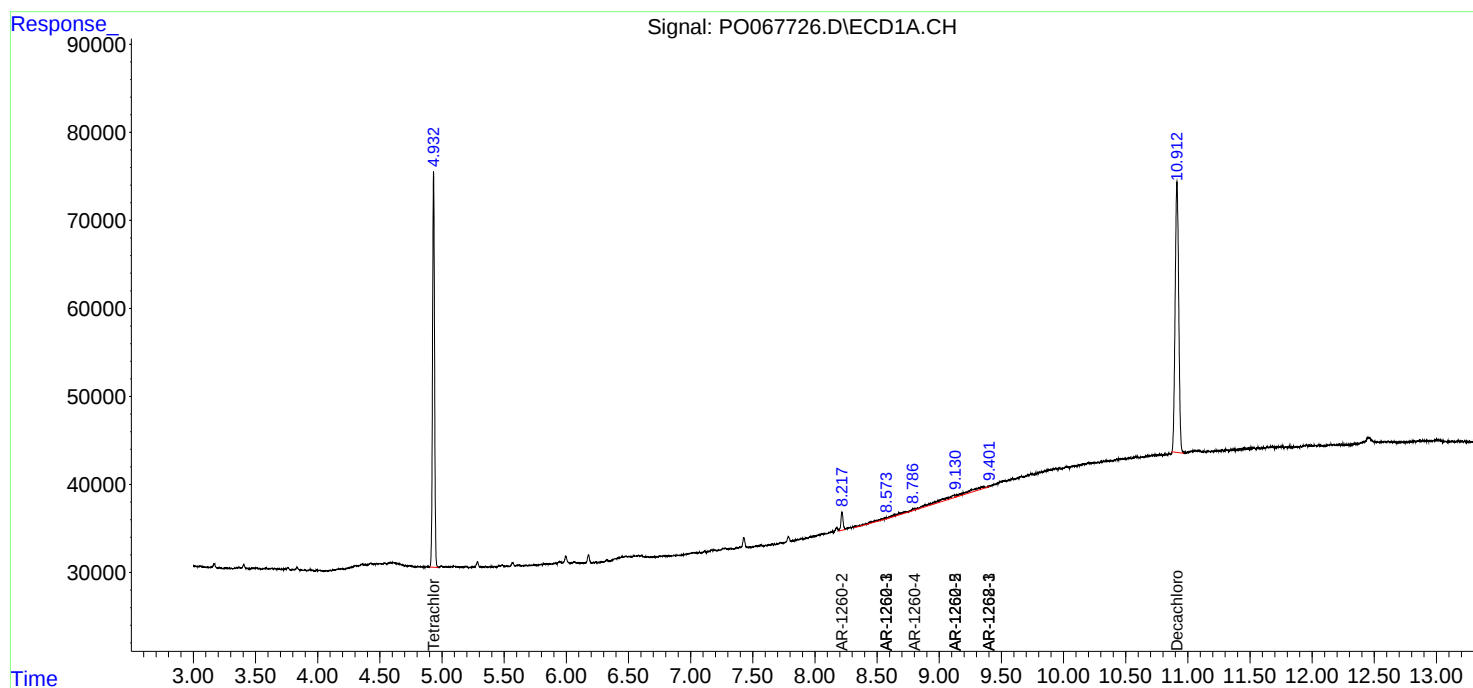


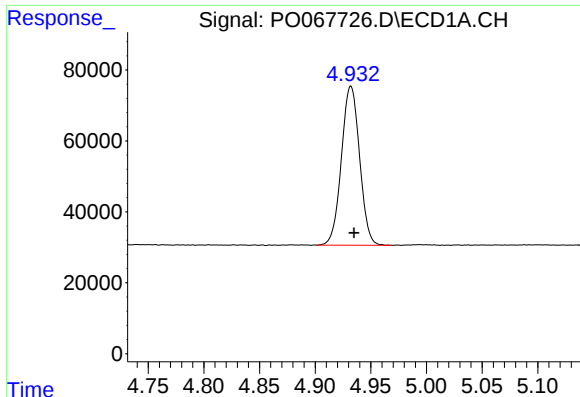

#1 Tetrachloro-m-xylene


R.T.: 4.932 min
Delta R.T.: -0.003 min
Response: 509163
Conc: 21.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
MH-720

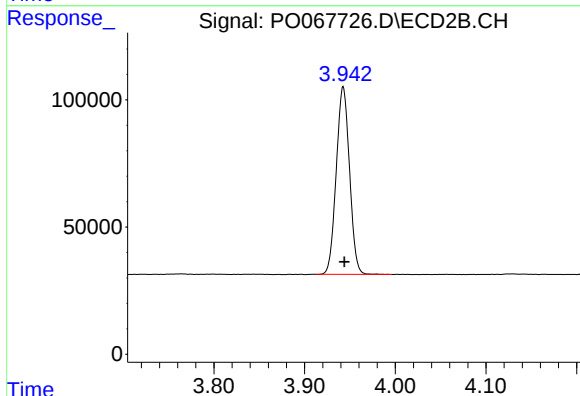


#1 Tetrachloro-m-xylene

R.T.: 3.943 min
Delta R.T.: -0.001 min
Response: 750318
Conc: 22.39 ng/ml

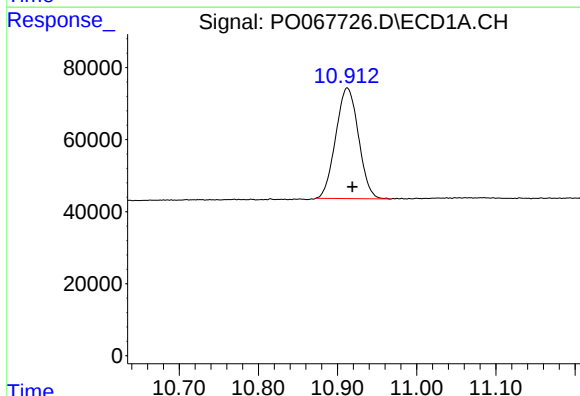


#2 Decachlorobiphenyl

R.T.: 10.912 min
Delta R.T.: -0.006 min
Response: 613772
Conc: 18.03 ng/ml

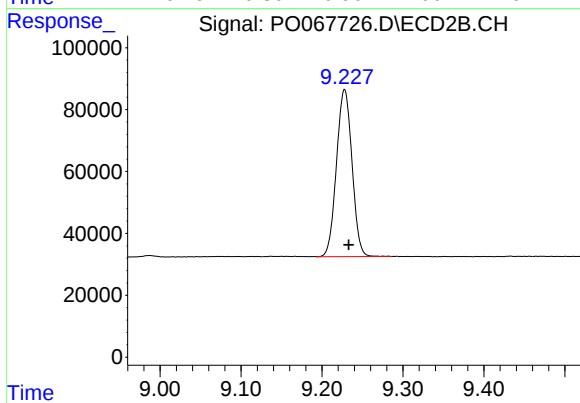

#2 Decachlorobiphenyl


R.T.: 9.228 min
Delta R.T.: -0.005 min
Response: 719737
Conc: 17.41 ng/ml

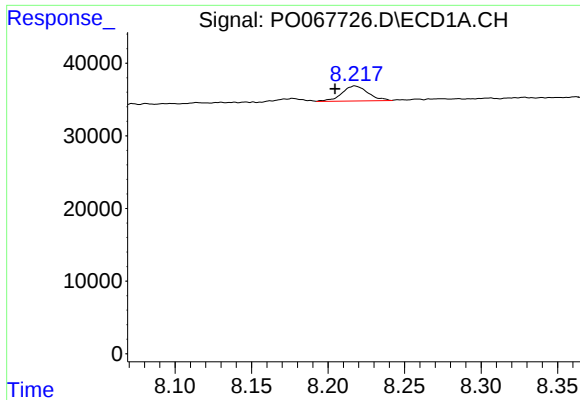

#32 AR-1260-2


R.T.: 8.218 min
Delta R.T.: 0.013 min
Response: 24713
Conc: 14.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
MH-720

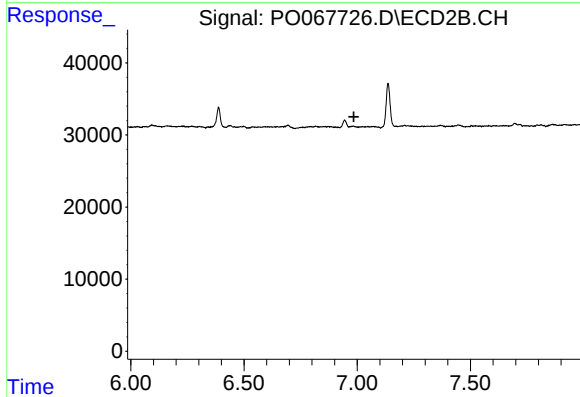


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.985 min
Response: 0
Conc: N.D.

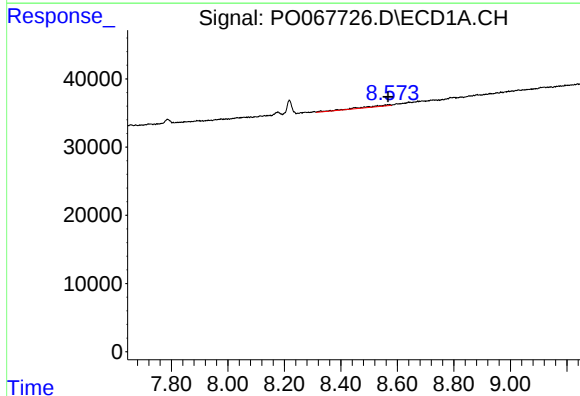


#33 AR-1260-3

R.T.: 8.574 min
Delta R.T.: 0.007 min
Response: 13186
Conc: 10.12 ng/ml

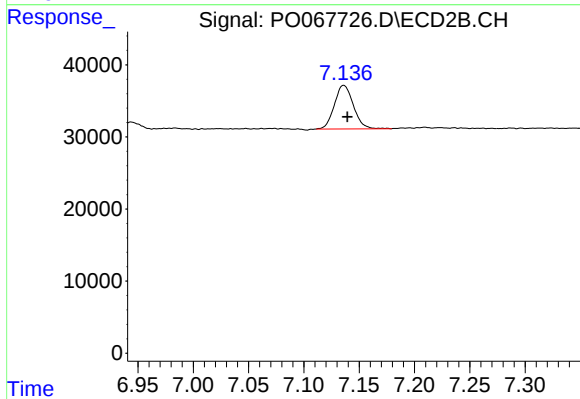

#33 AR-1260-3


R.T.: 7.136 min
Delta R.T.: -0.003 min
Response: 72401
Conc: 30.11 ng/ml

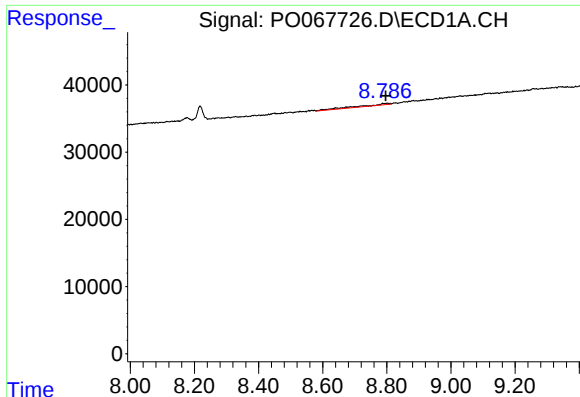

#34 AR-1260-4


R.T.: 8.801 min
Delta R.T.: 0.004 min
Response: 16154
Conc: 10.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
MH-720

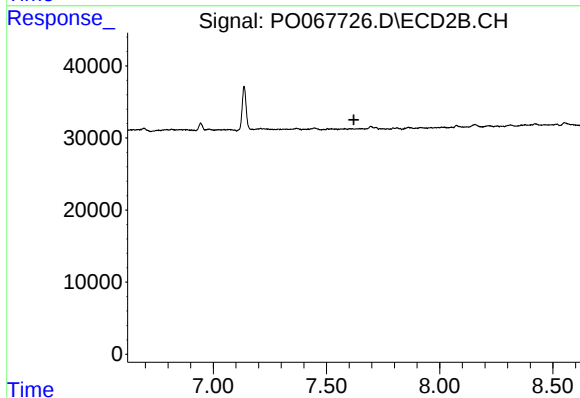


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.621 min
Response: 0
Conc: N.D.

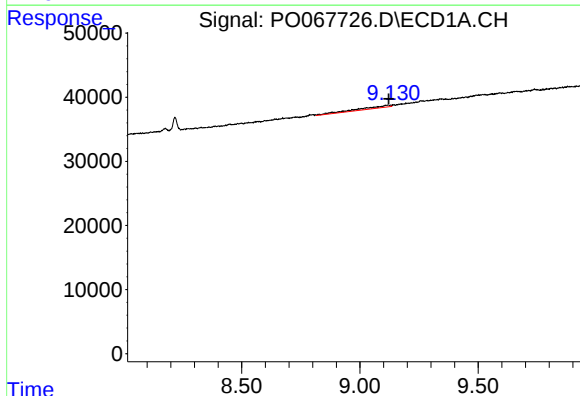


#35 AR-1260-5

R.T.: 9.121 min
Delta R.T.: 0.000 min
Response: 33877
Conc: 10.74 ng/ml

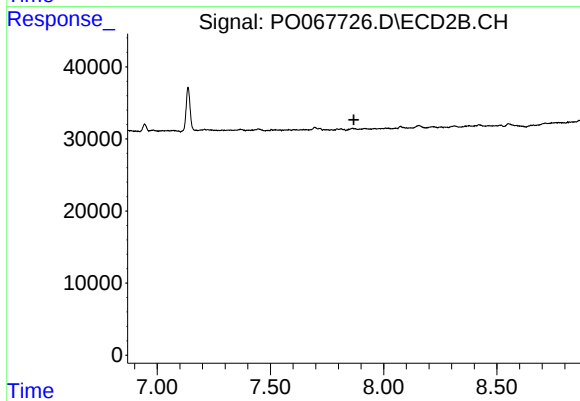

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 7.869 min
Response: 0
Conc: N.D.

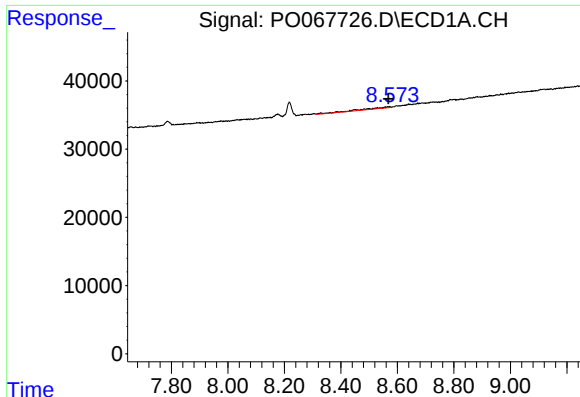

#36 AR-1262-1


R.T.: 8.574 min
Delta R.T.: 0.006 min
Response: 13186
Conc: 7.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
MH-720

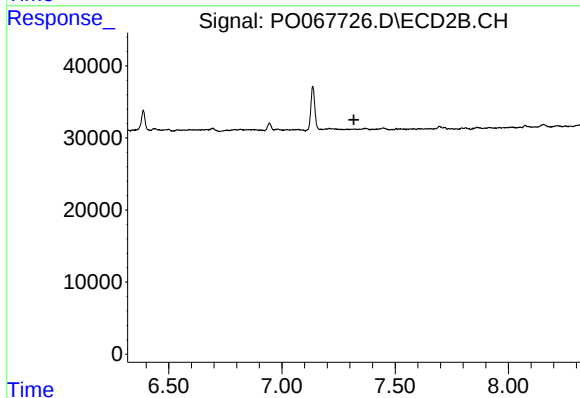


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.317 min
Response: 0
Conc: N.D.

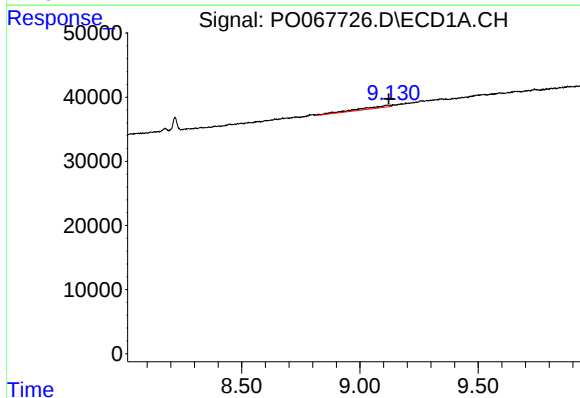


#37 AR-1262-2

R.T.: 9.121 min
Delta R.T.: 0.000 min
Response: 33877
Conc: 11.81 ng/ml

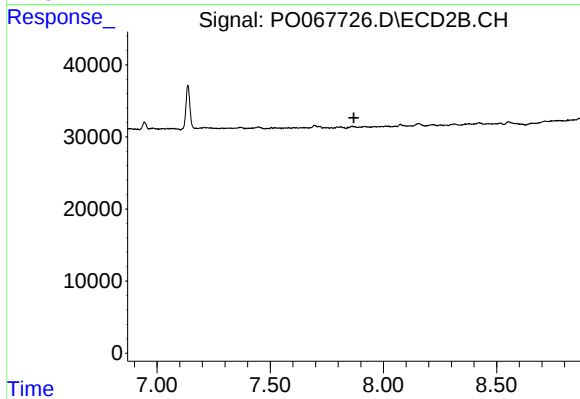

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.869 min
Response: 0
Conc: N.D.

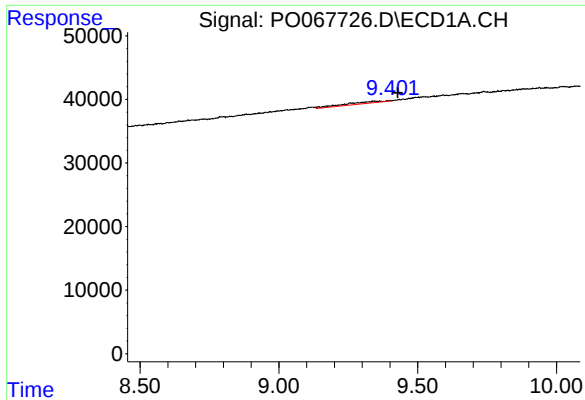

#38 AR-1262-3


R.T.: 9.401 min
Delta R.T.: -0.027 min
Response: 29347
Conc: 14.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
MH-720

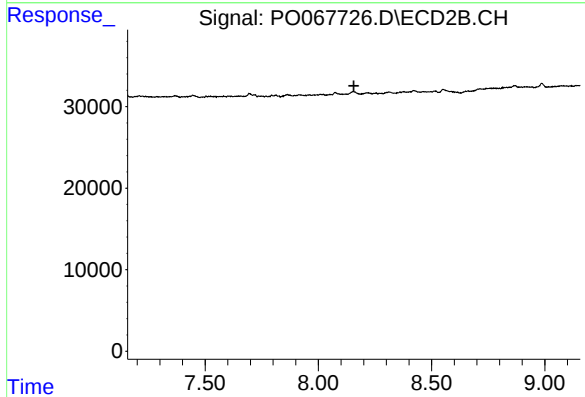


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.157 min
Response: 0
Conc: N.D.

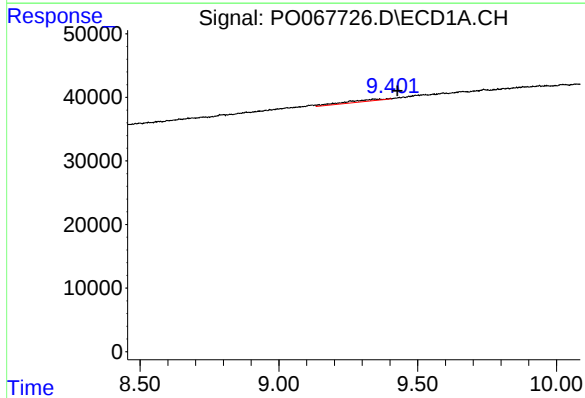

#41 AR-1268-1

R.T.: 9.401 min
Delta R.T.: -0.026 min
Response: 29347
Conc: 7.94 ng/ml

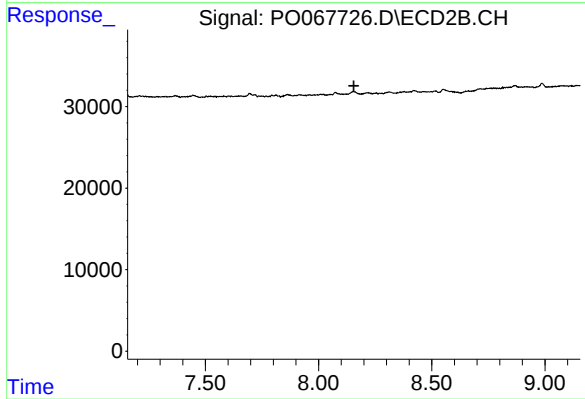

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.156 min
Response: 0
Conc: N.D.