

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040720\
 Data File : P0067731.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Apr 2020 18:37
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 18:58:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.931	3.942	495833	727047	20.821	21.692
2) SA Decachlor...	10.911	9.228	659495	784236	19.372	18.968
Target Compounds						
20) L4 AR-1242-5	7.167	6.092	35047	27851	65.604	29.764 #
24) L5 AR-1248-4	7.167	0.000	35047	0	37.148	N.D. #
25) L5 AR-1248-5	7.167	6.092	35047	27851	38.890	22.506 #
26) L6 AR-1254-1	7.167	6.092	35047	27851	28.376	10.862 #
38) L8 AR-1262-3	9.439	0.000	69716	0	33.504	N.D. #
41) L9 AR-1268-1	9.439	0.000	69716	0	18.867	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040720\
Data File : PO067731.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Apr 2020 18:37
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 18:58:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

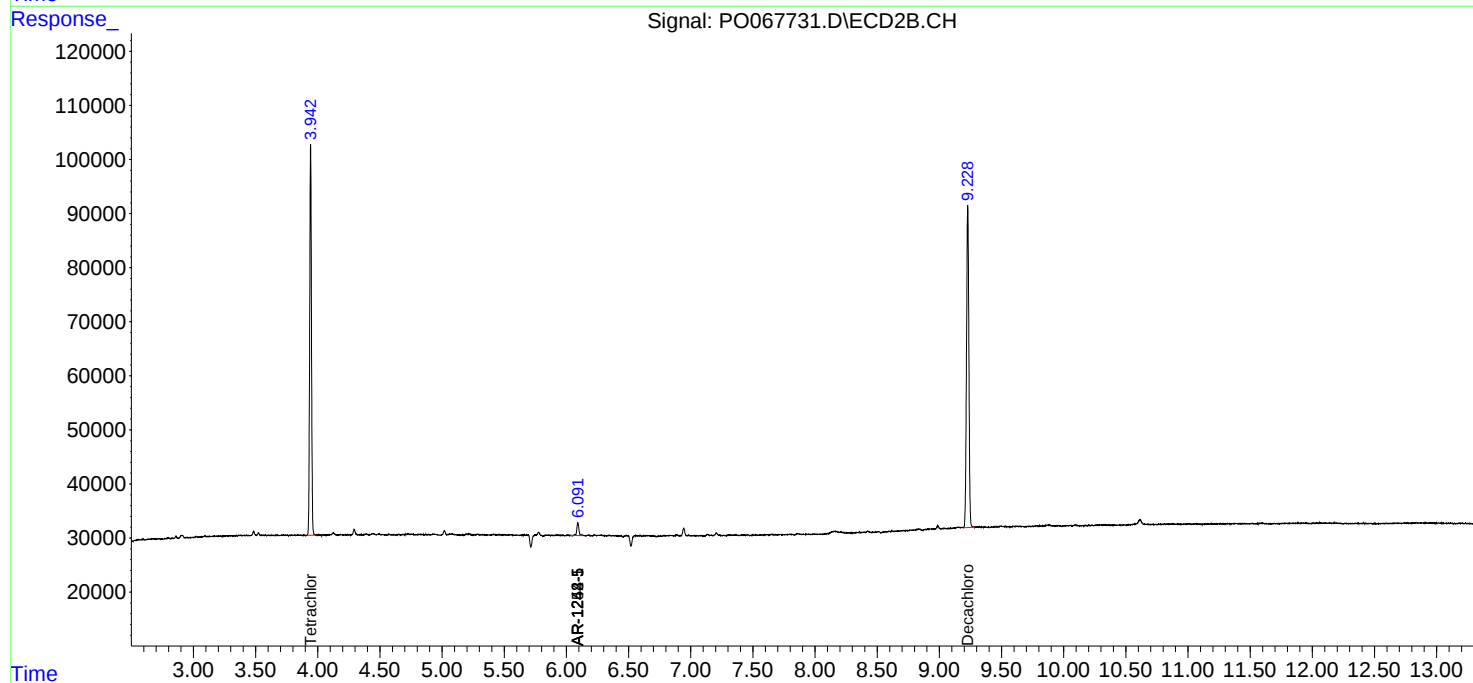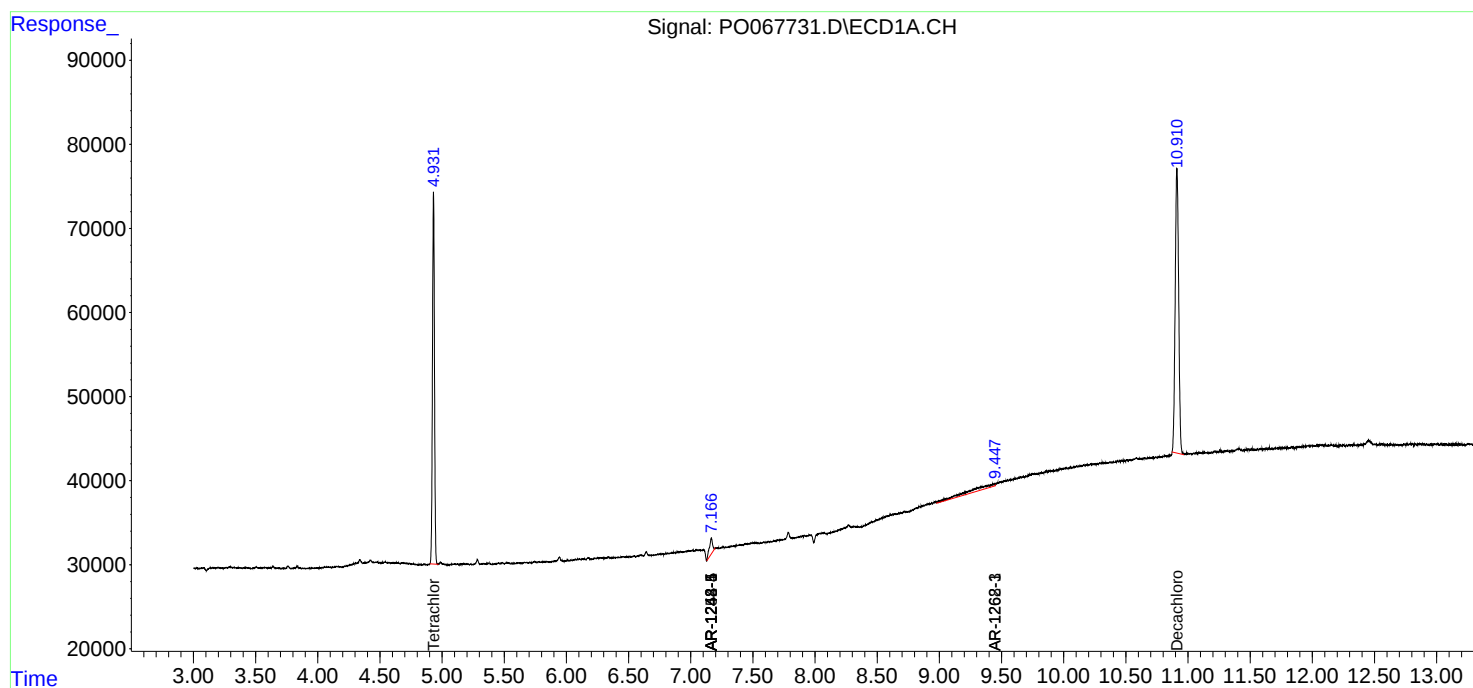


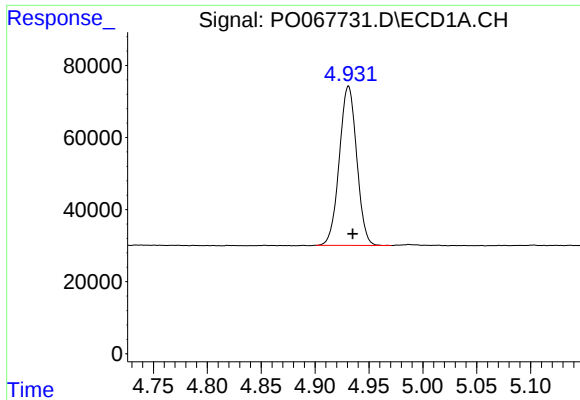

#1 Tetrachloro-m-xylene


R.T.: 4.931 min
Delta R.T.: -0.004 min
Response: 495833
Conc: 20.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

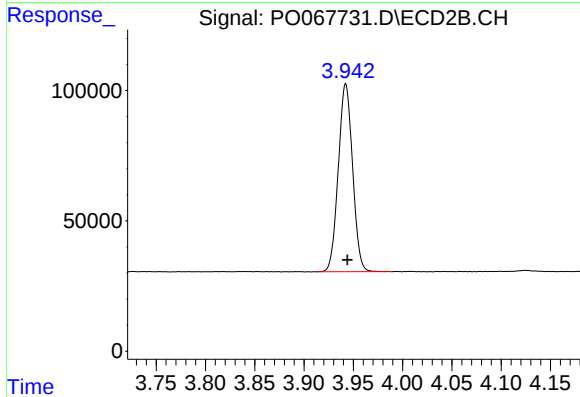


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: -0.001 min
Response: 727047
Conc: 21.69 ng/ml

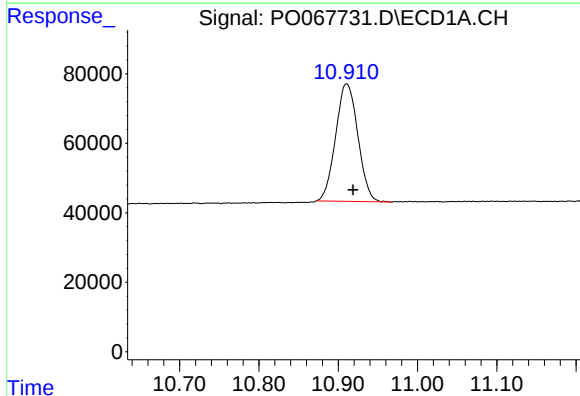


#2 Decachlorobiphenyl

R.T.: 10.911 min
Delta R.T.: -0.008 min
Response: 659495
Conc: 19.37 ng/ml

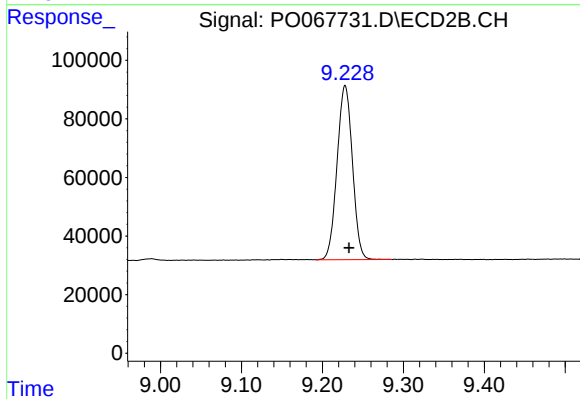

#2 Decachlorobiphenyl


R.T.: 9.228 min
Delta R.T.: -0.005 min
Response: 784236
Conc: 18.97 ng/ml

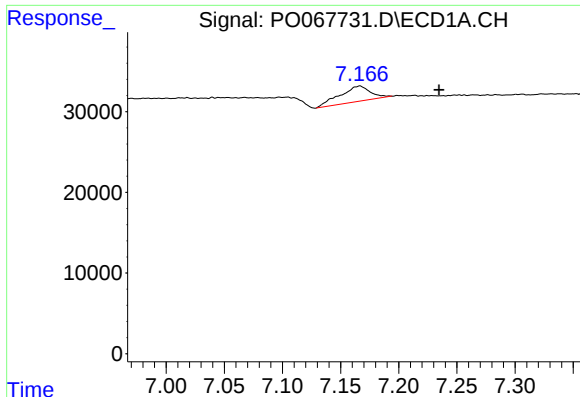

#20 AR-1242-5


R.T.: 7.167 min
Delta R.T.: -0.068 min
Response: 35047
Conc: 65.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

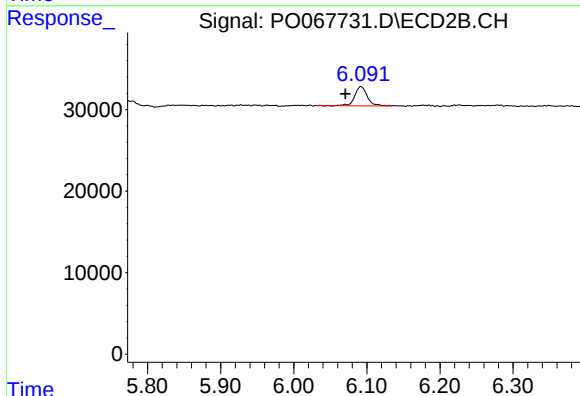


#20 AR-1242-5

R.T.: 6.092 min
Delta R.T.: 0.021 min
Response: 27851
Conc: 29.76 ng/ml

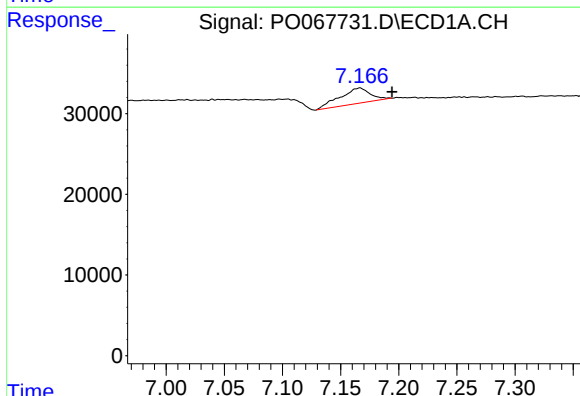


#24 AR-1248-4

R.T.: 7.167 min
Delta R.T.: -0.028 min
Response: 35047
Conc: 37.15 ng/ml

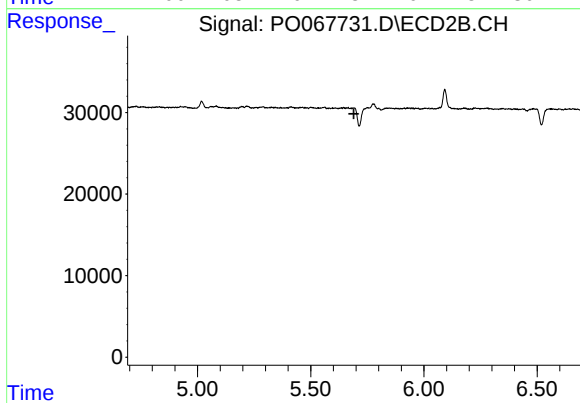

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.690 min
Response: 0
Conc: N.D.

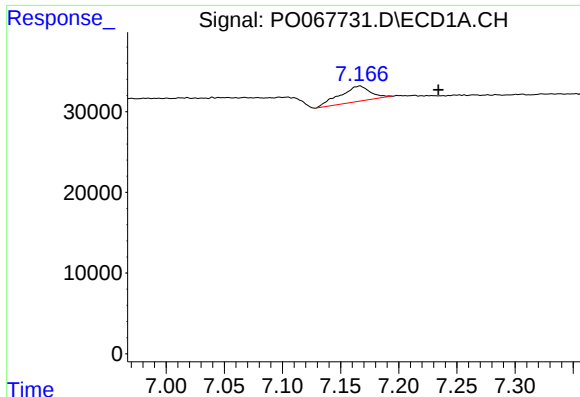

#25 AR-1248-5


R.T.: 7.167 min
Delta R.T.: -0.068 min
Response: 35047
Conc: 38.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

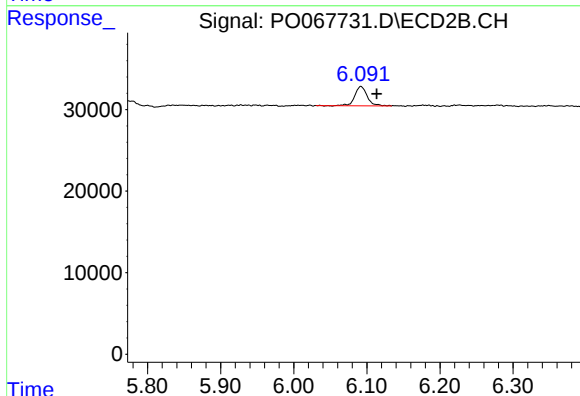


#25 AR-1248-5

R.T.: 6.092 min
Delta R.T.: -0.021 min
Response: 27851
Conc: 22.51 ng/ml

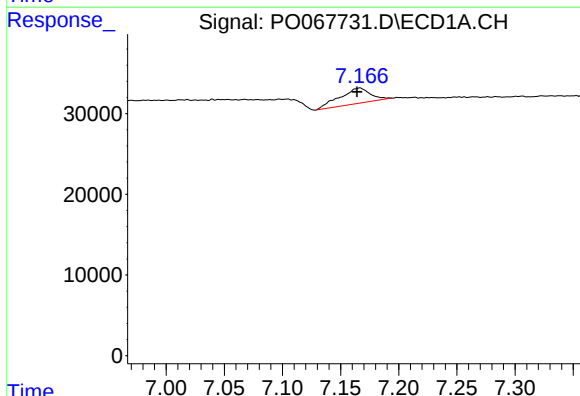


#26 AR-1254-1

R.T.: 7.167 min
Delta R.T.: 0.002 min
Response: 35047
Conc: 28.38 ng/ml

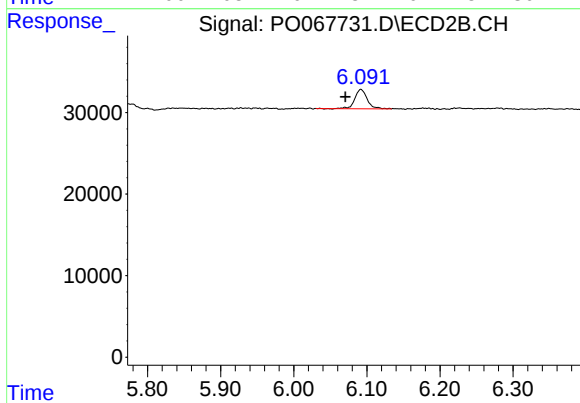

#26 AR-1254-1


R.T.: 6.092 min
Delta R.T.: 0.021 min
Response: 27851
Conc: 10.86 ng/ml

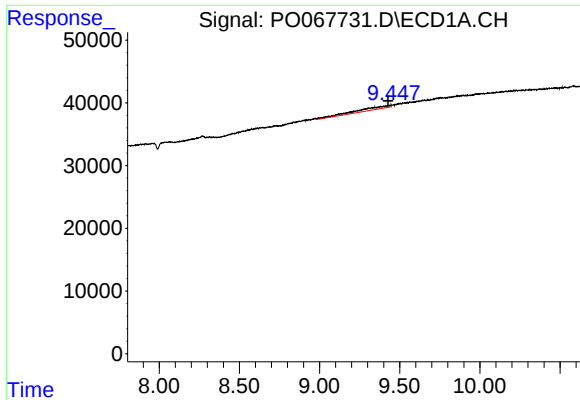

#38 AR-1262-3


R.T.: 9.439 min
Delta R.T.: 0.011 min
Response: 69716
Conc: 33.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

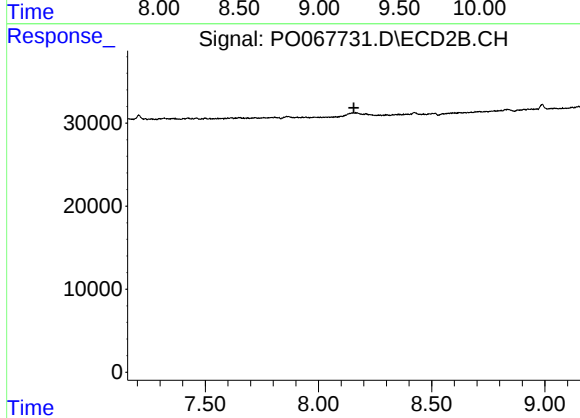


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.157 min
Response: 0
Conc: N.D.

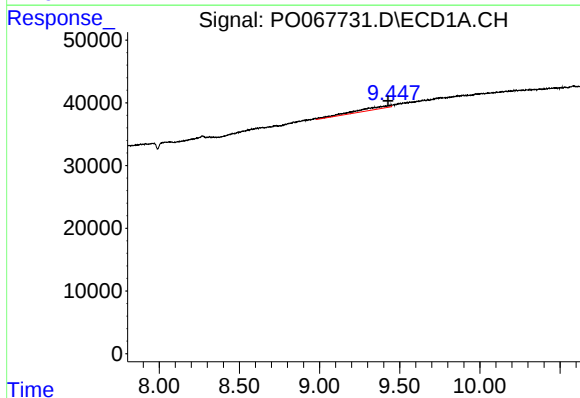

#41 AR-1268-1

R.T.: 9.439 min
Delta R.T.: 0.011 min
Response: 69716
Conc: 18.87 ng/ml

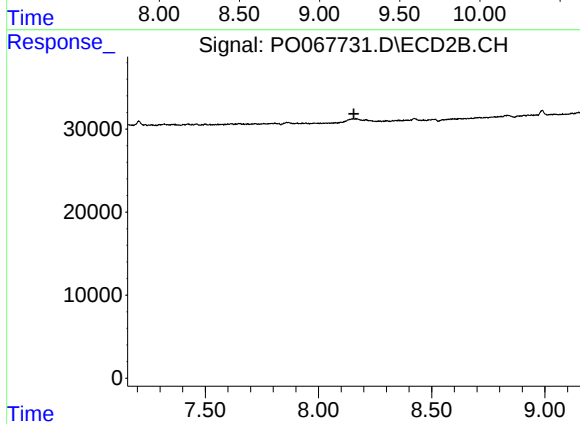

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.156 min
Response: 0
Conc: N.D.