

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040720\
 Data File : P0067707.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Apr 2020 11:03
 Operator : DD\AJ
 Sample : L2166-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-47-COMP

Manual Integrations
 APPROVED

Sohil
 4/8/2020 10:09:19 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 14:47:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.929	3.941	616561	916924	25.891	27.357
2) SA Decachlor...	10.908	9.226	738918	816714	21.705m	19.753

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040720\
Data File : P0067707.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Apr 2020 11:03
Operator : DD\AJ
Sample : L2166-05
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-47-COMP


Manual Integrations
APPROVED

Sohil
4/8/2020 10:09:19 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 14:47:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

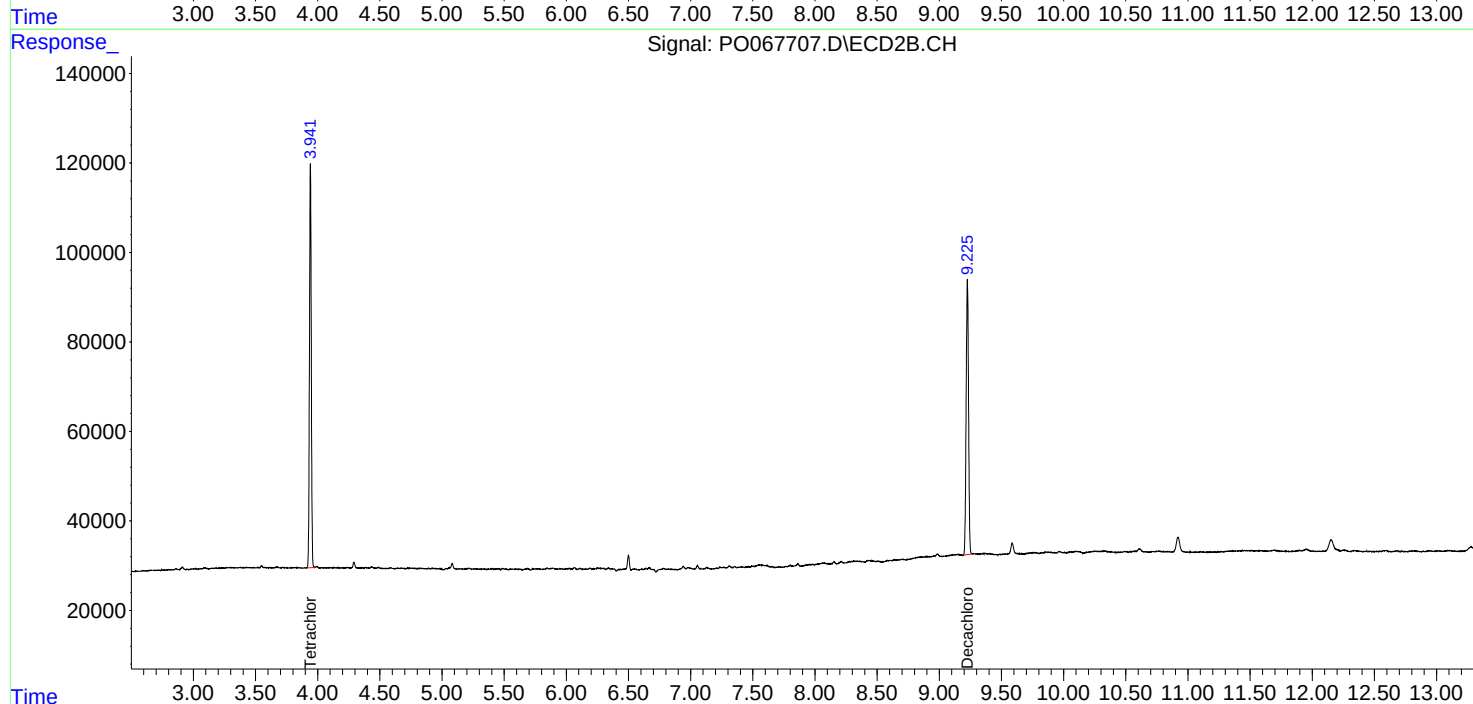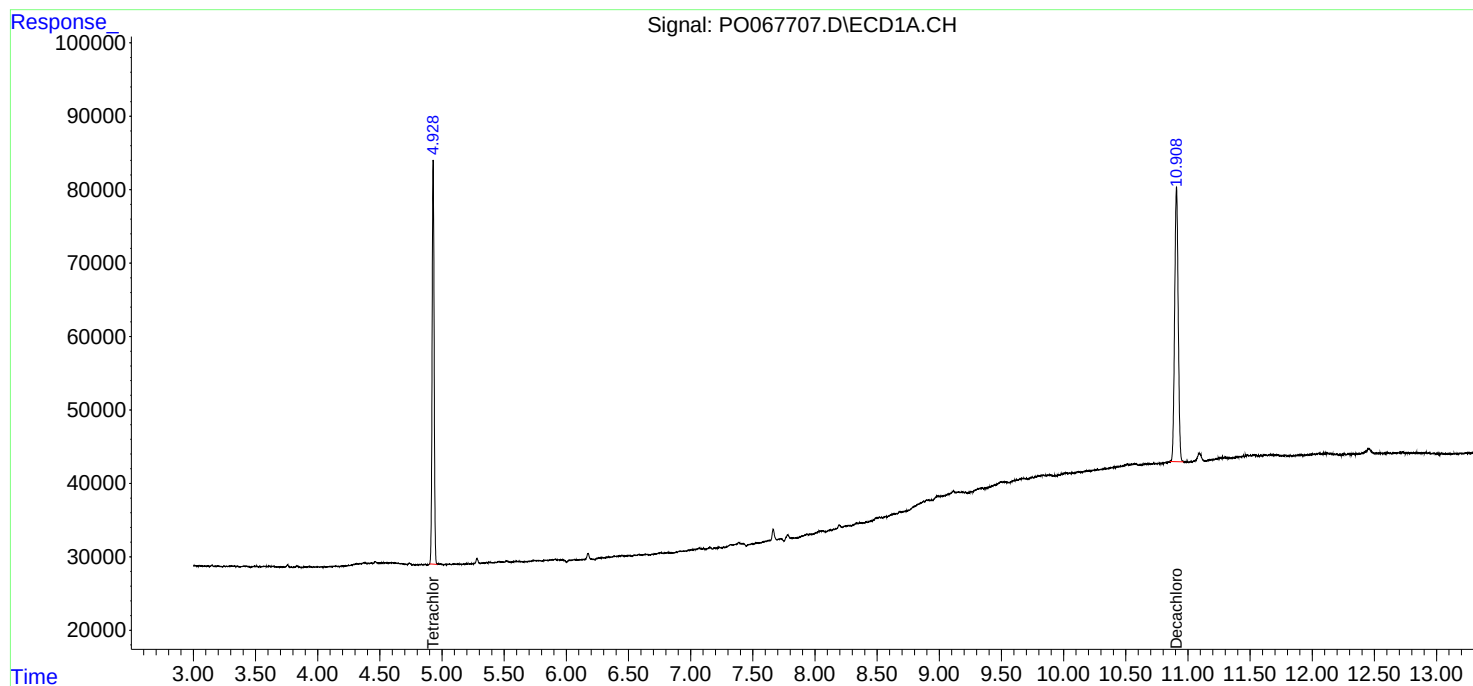

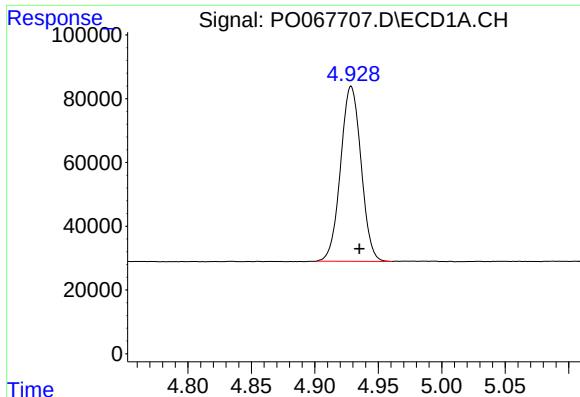


#1 Tetrachloro-m-xylene

R.T.: 4.929 min
Delta R.T.: -0.006 min
Response: 616561
Conc: 25.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-47-COMP


Manual Integrations
APPROVED

Sohil
4/8/2020 10:09:19 AM

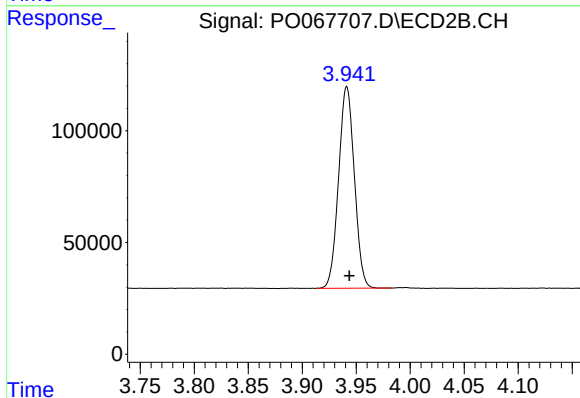


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: -0.002 min
Response: 916924
Conc: 27.36 ng/ml

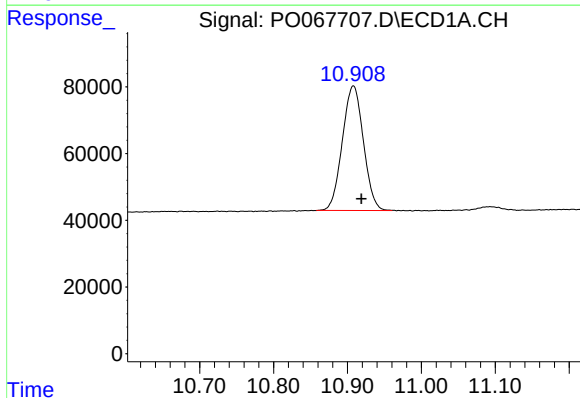

#2 Decachlorobiphenyl

R.T.: 10.908 min
Delta R.T.: -0.011 min
Response: 738918
Conc: 21.70 ng/ml m

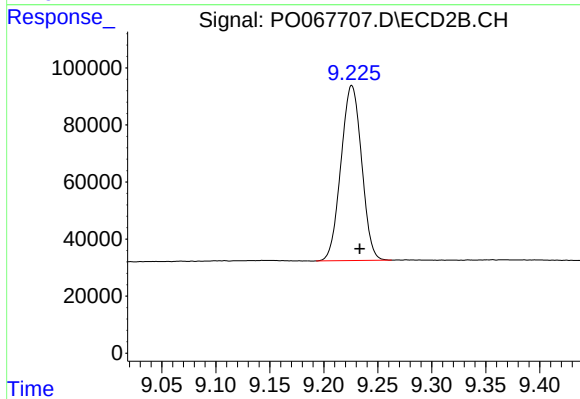

#2 Decachlorobiphenyl

R.T.: 9.226 min
Delta R.T.: -0.007 min
Response: 816714
Conc: 19.75 ng/ml