

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040720\
 Data File : P0067721.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Apr 2020 15:31
 Operator : DD\AJ
 Sample : PB128074BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB128074BL

Manual Integrations
 APPROVED

Sohil
 4/8/2020 10:09:23 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 17:52:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.932	3.942	583849	862599	24.517	25.736
2) SA Decachlor...	10.911	9.227	772980	882660	22.706m	21.348

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040720\
Data File : P0067721.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Apr 2020 15:31
Operator : DD\AJ
Sample : PB128074BL
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB128074BL


Manual Integrations
APPROVED

Sohil
4/8/2020 10:09:23 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 17:52:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

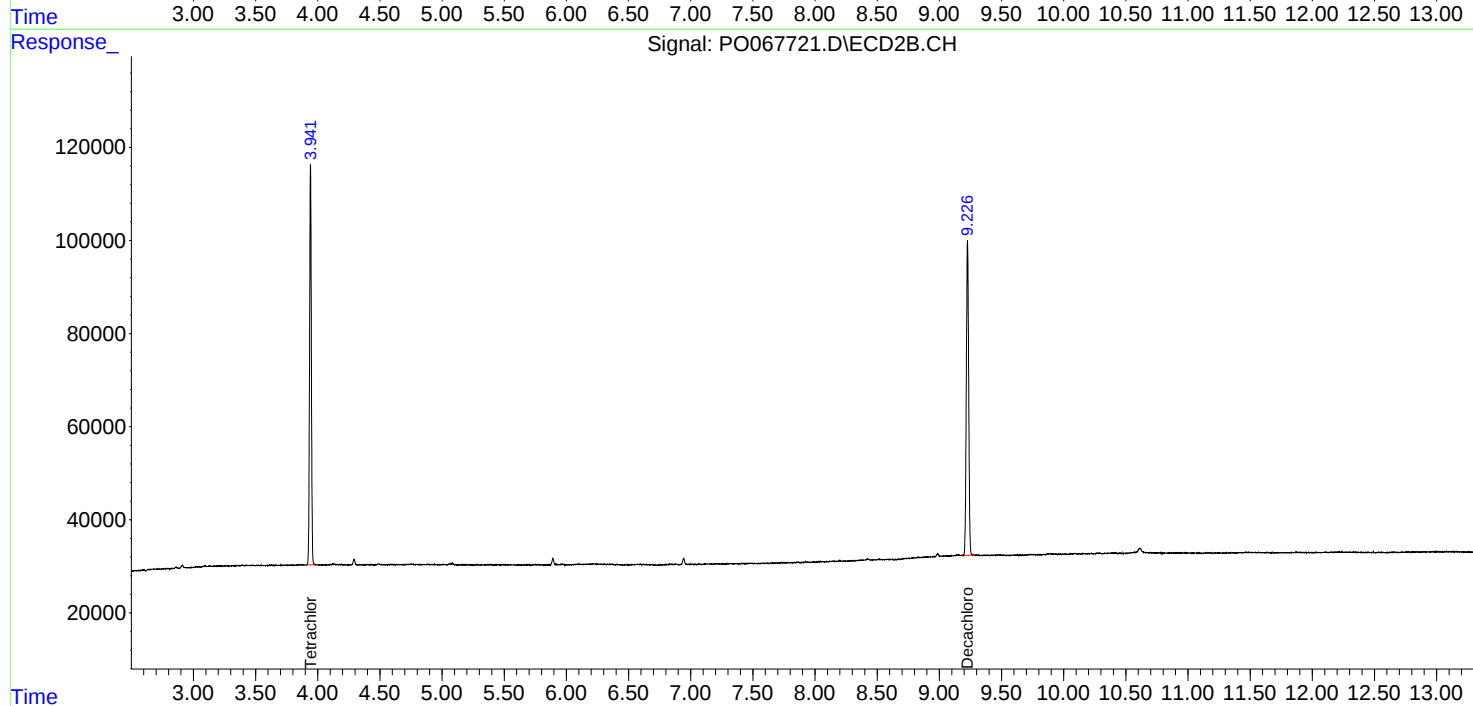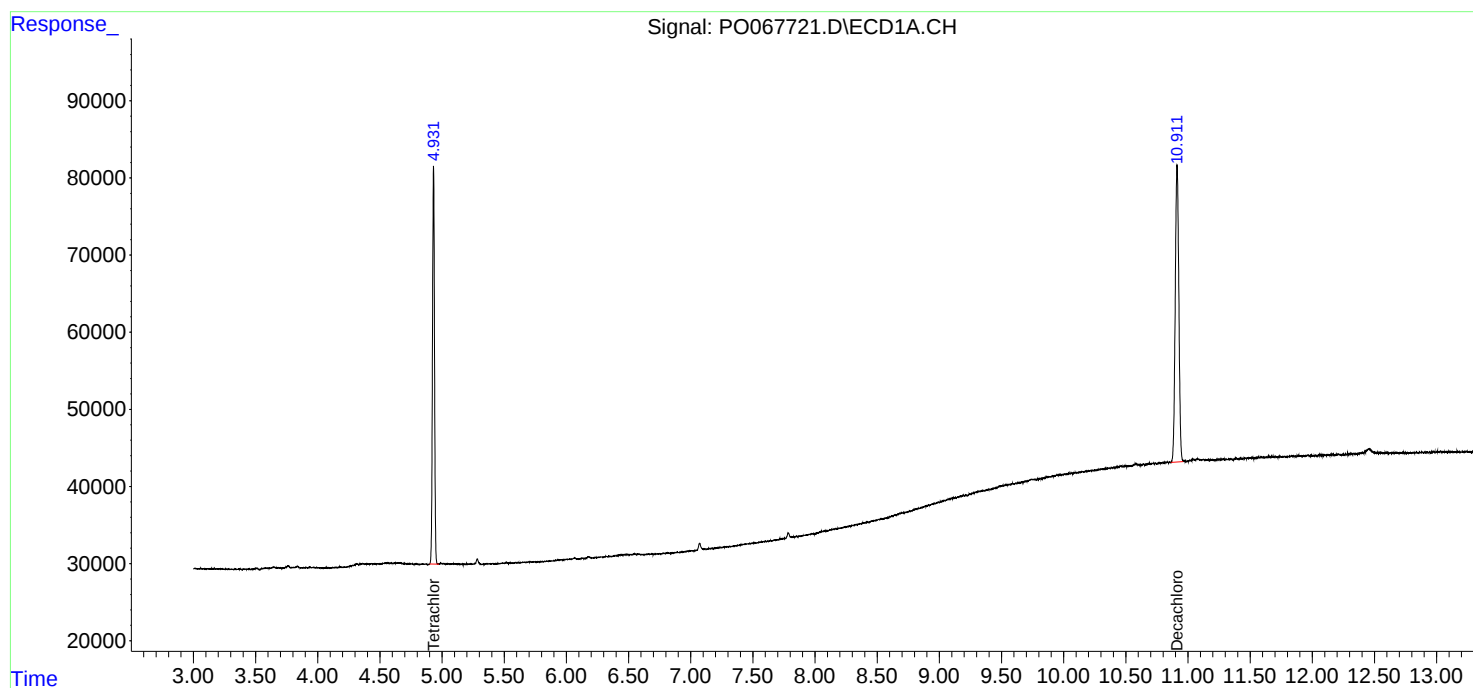

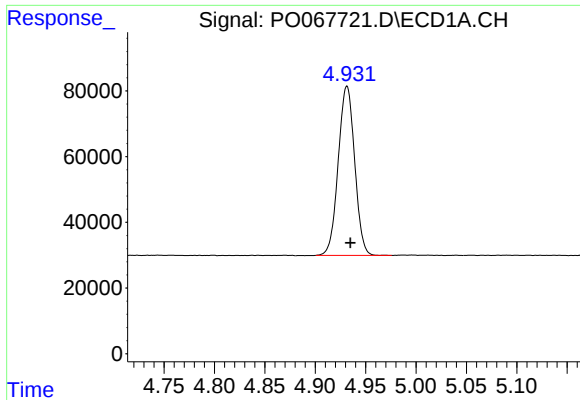


#1 Tetrachloro-m-xylene

R.T.: 4.932 min
Delta R.T.: -0.003 min
Response: 583849
Conc: 24.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB128074BL


Manual Integrations
APPROVED

Sohil
4/8/2020 10:09:23 AM

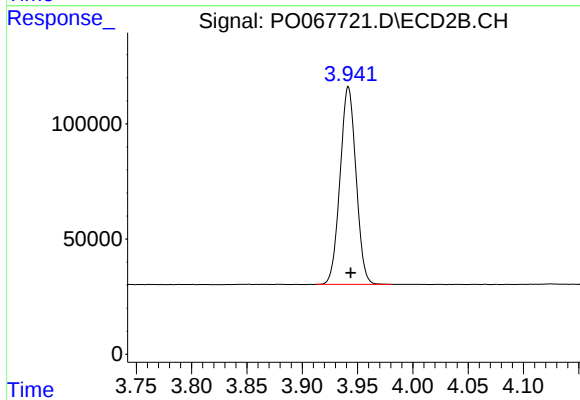


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: -0.002 min
Response: 862599
Conc: 25.74 ng/ml

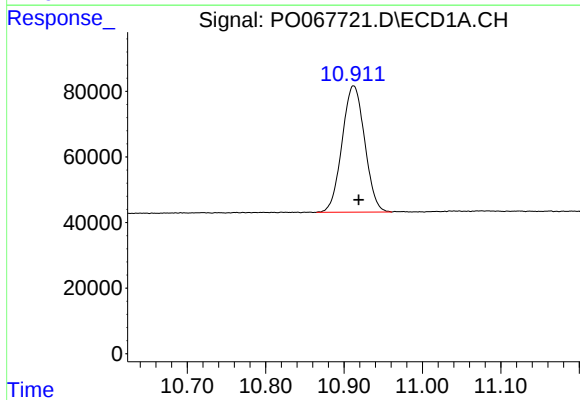

#2 Decachlorobiphenyl

R.T.: 10.911 min
Delta R.T.: -0.007 min
Response: 772980
Conc: 22.71 ng/ml m

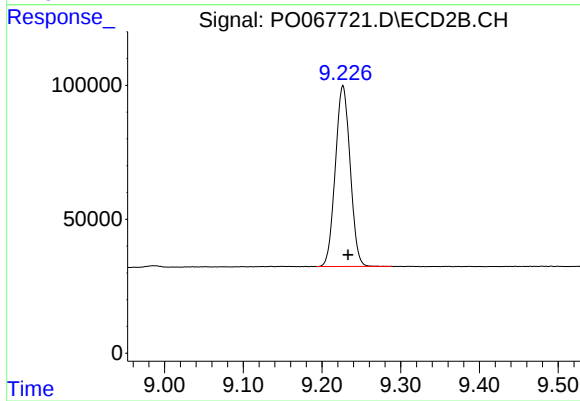

#2 Decachlorobiphenyl

R.T.: 9.227 min
Delta R.T.: -0.007 min
Response: 882660
Conc: 21.35 ng/ml