

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040819\
 Data File : P0055024.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Apr 2019 10:08
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1660 LOD 25PPB
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 07:34:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.315	3.611	1429789	1395711	41.198	43.736
2)	SA Decachlor...	9.941	8.586	1398190	965901	28.362	30.328
Target Compounds							
3)	L1 AR-1016-1	5.477	4.709	99620	115016	55.362	72.731 #
4)	L1 AR-1016-2	5.477	4.709	99620	115016	40.110	53.677 #
5)	L1 AR-1016-3	5.561	4.883	91232	63360	57.990	52.440
6)	L1 AR-1016-4	5.659	4.924	75059	52149	57.601	51.606
7)	L1 AR-1016-5	5.951	5.136	80881	62927	60.619	48.279
9)	L2 AR-1221-2	4.616	3.910	30704	27829	90.542	92.827
10)	L2 AR-1221-3	4.685	3.984	51300	42626	49.385	46.243
11)	L3 AR-1232-1	4.685	3.984	51300	42626	59.585	56.842
12)	L3 AR-1232-2	5.211	4.709	71337	115016	145.842	133.568
13)	L3 AR-1232-3	5.477	4.883	99620	63360	101.933	130.756 #
14)	L3 AR-1232-4	5.659	4.966	75059	63173	146.642	143.771
15)	L3 AR-1232-5	5.749	5.136	67673	62927	162.678	129.383
16)	L4 AR-1242-1	5.477	4.709	99620	115016	71.706	93.683 #
17)	L4 AR-1242-2	5.477	4.709	99620	115016	52.062	69.403 #
18)	L4 AR-1242-3	5.561	4.883	91232	63360	73.607	66.883
19)	L4 AR-1242-4	5.659	4.966	75059	63173	73.620	66.097
20)	L4 AR-1242-5	6.392	5.487	21799	66567	18.058	54.124 #
21)	L5 AR-1248-1	5.477	4.709	99620	115016	99.652	131.031 #
22)	L5 AR-1248-2	5.749	4.924	67673	52149	46.597	43.150
23)	L5 AR-1248-3	5.951	4.966	80881	63173	50.640	50.628
24)	L5 AR-1248-4	6.354	5.136	26182	62927	13.938	41.318 #
25)	L5 AR-1248-5	6.392	5.527	21799	18989	12.159	12.737
26)	L6 AR-1254-1	6.327	5.487	85574	66567	47.195	30.459 #
27)	L6 AR-1254-2	6.543	5.632	61524	48402	21.551	24.963
28)	L6 AR-1254-3	6.914	6.049	80408	88755	25.569	27.687
29)	L6 AR-1254-4	7.192	6.290	21414	26265	8.753	13.415 #
30)	L6 AR-1254-5	7.609	6.677	184515	149402	68.841	51.971
31)	L7 AR-1260-1	7.071	6.164	147985	125488	58.896	54.606
32)	L7 AR-1260-2	7.327	6.349	166152	176442	53.537	64.096
33)	L7 AR-1260-3	7.684	6.504	118121	132349	48.127	51.340
34)	L7 AR-1260-4	7.908	6.974	133182	100771	48.150	47.351
35)	L7 AR-1260-5	8.219	7.213	233856	219084	42.147	45.745
36)	L8 AR-1262-1	7.684	6.715	118121	114492	35.450	38.485
37)	L8 AR-1262-2	8.219	7.213	233856	219084	39.473	44.701
38)	L8 AR-1262-3	8.531	7.496	178495	52970	43.086	25.796 #
39)	L8 AR-1262-4	8.584	7.559	98139	158954	30.459	43.884 #
40)	L8 AR-1262-5	9.231	8.052	64640	52737	29.566	32.677
41)	L9 AR-1268-1	8.531	7.496	178495	52970	25.078	9.368 #
42)	L9 AR-1268-2	8.584	7.559	98139	158954	14.978	30.736 #
44)	L9 AR-1268-4	9.231	8.052	64640	52737	27.094	28.447

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040819\
Data File : P0055024.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Apr 2019 10:08
Operator : SM/SJ
Sample : K1560-07
Misc : AR1660 LOD 25PPB
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 07:34:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
45) L9	AR-1268-5	9.624	8.336	25885	17315	1.571	1.521



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040819\
Data File : PO055024.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Apr 2019 10:08
Operator : SM/SJ
Sample : K1560-07
Misc : AR1660 LOD 25PPB
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 07:34:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

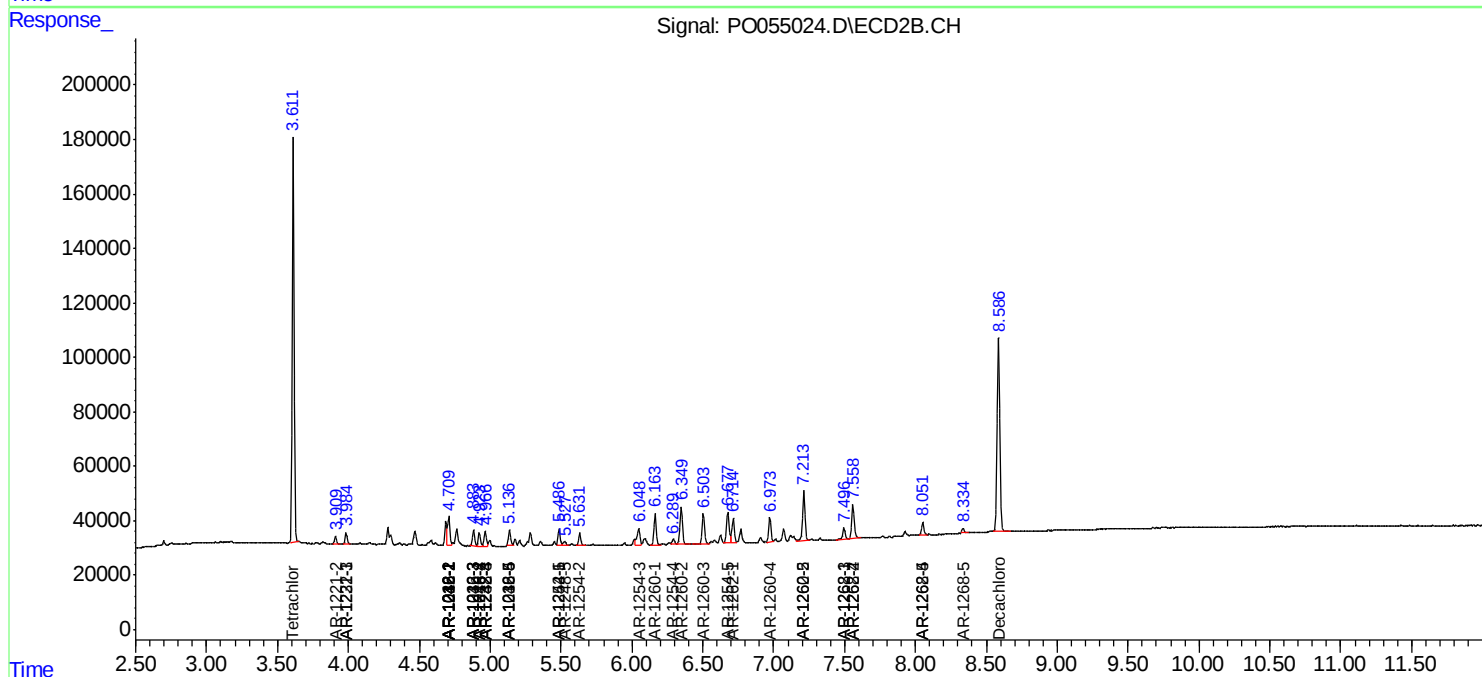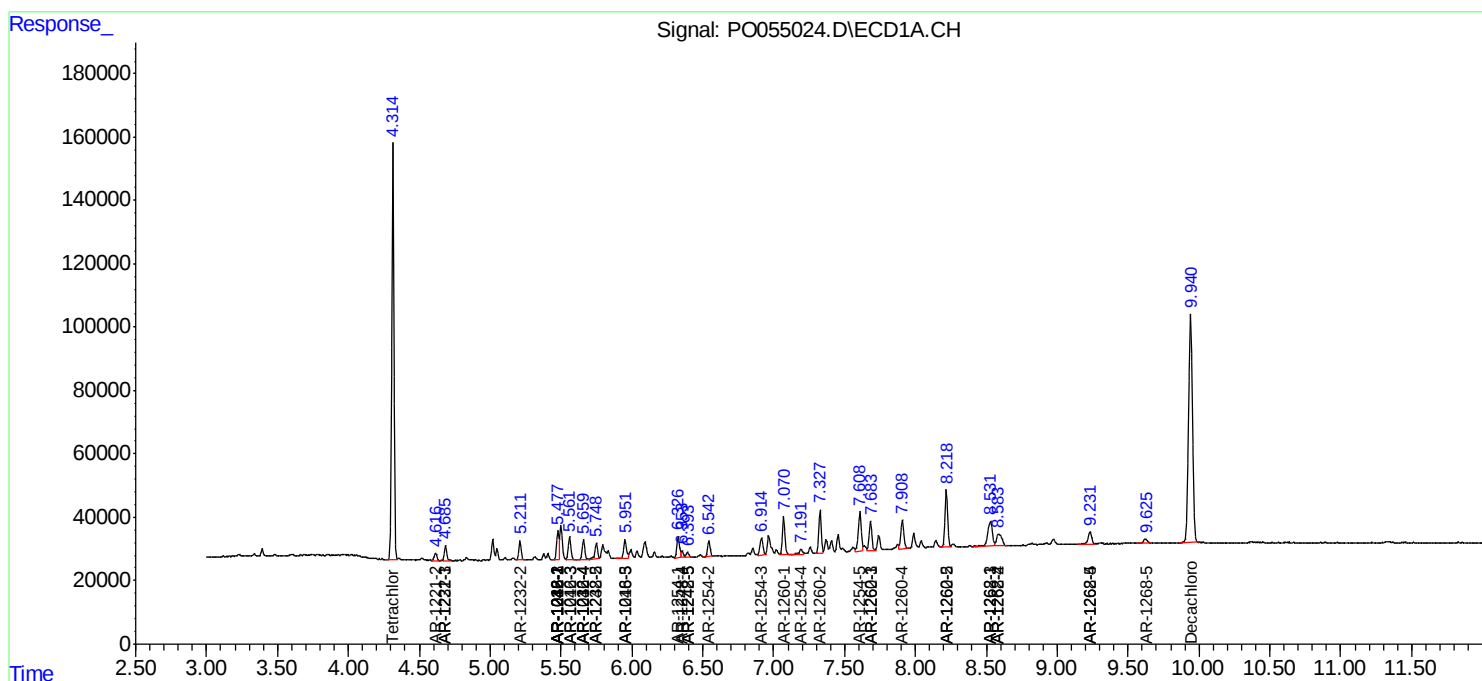


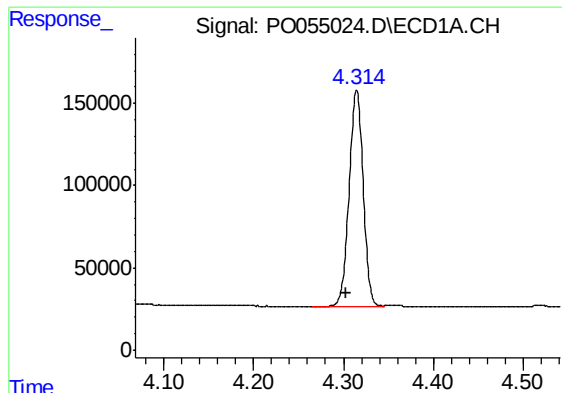

#1 Tetrachloro-m-xylene


R.T.: 4.315 min
Delta R.T.: 0.012 min
Response: 1429789
Conc: 41.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: -0.010 min
Response: 1395711
Conc: 43.74 ng/ml




#2 Decachlorobiphenyl

R.T.: 9.941 min
Delta R.T.: 0.018 min
Response: 1398190
Conc: 28.36 ng/ml

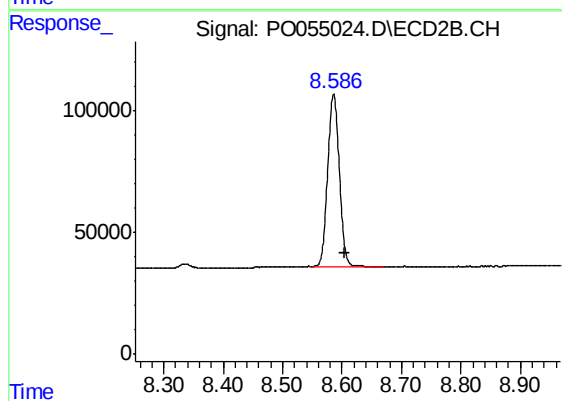

#2 Decachlorobiphenyl


R.T.: 8.586 min
Delta R.T.: -0.018 min
Response: 965901
Conc: 30.33 ng/ml

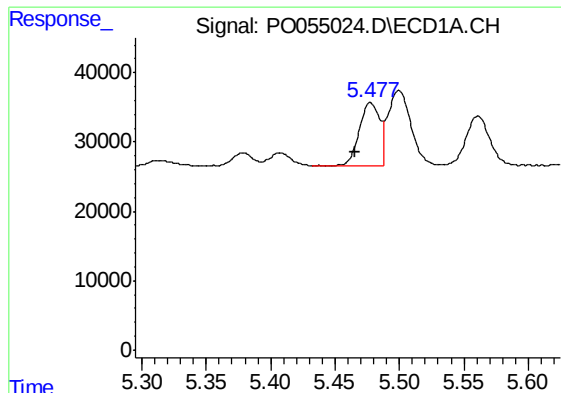

#3 AR-1016-1


R.T.: 5.477 min
Delta R.T.: 0.012 min
Response: 99620
Conc: 55.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

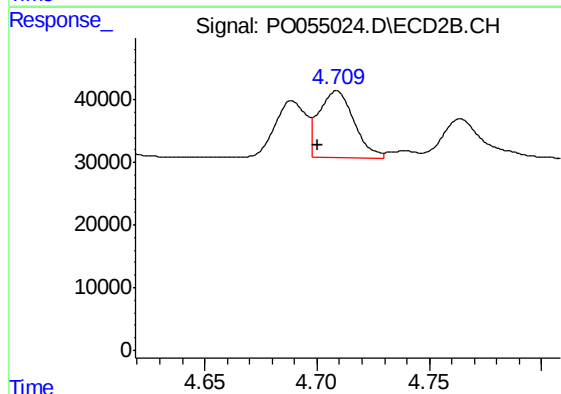


#3 AR-1016-1

R.T.: 4.709 min
Delta R.T.: 0.008 min
Response: 115016
Conc: 72.73 ng/ml

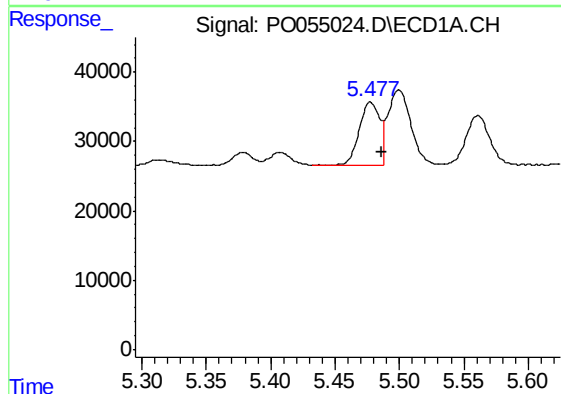


#4 AR-1016-2

R.T.: 5.477 min
Delta R.T.: -0.009 min
Response: 99620
Conc: 40.11 ng/ml

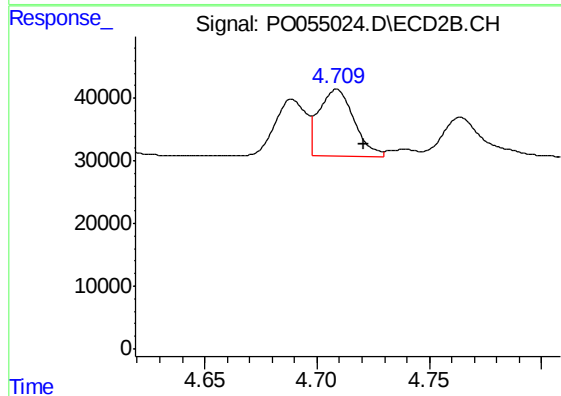

#4 AR-1016-2


R.T.: 4.709 min
Delta R.T.: -0.012 min
Response: 115016
Conc: 53.68 ng/ml

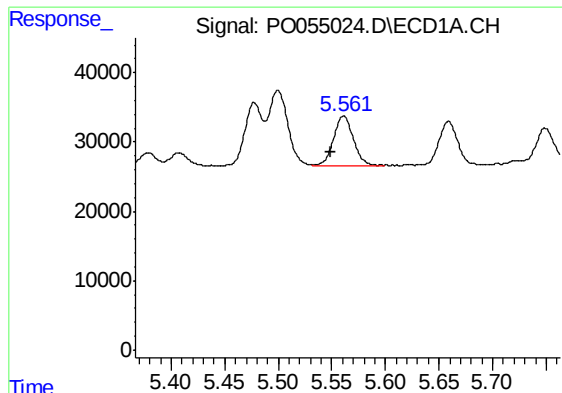

#5 AR-1016-3


R.T.: 5.561 min
Delta R.T.: 0.013 min
Response: 91232
Conc: 57.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

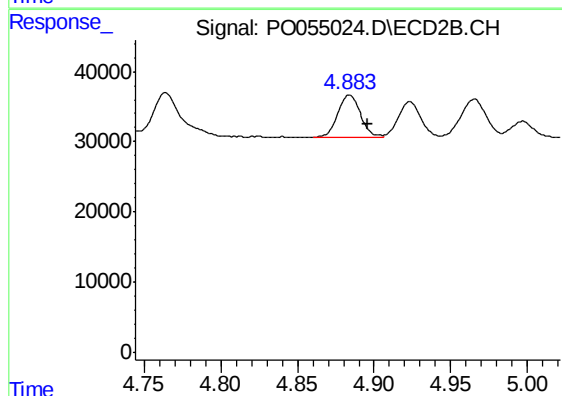


#5 AR-1016-3

R.T.: 4.883 min
Delta R.T.: -0.012 min
Response: 63360
Conc: 52.44 ng/ml

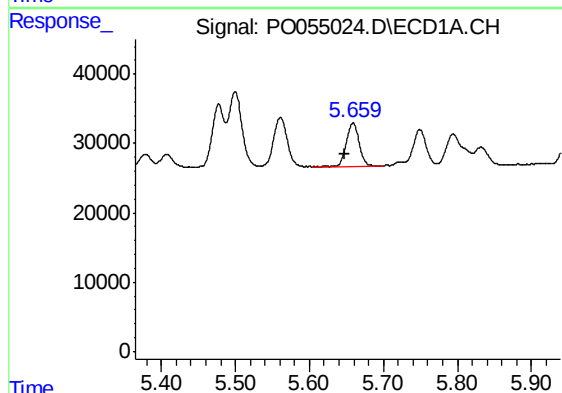


#6 AR-1016-4

R.T.: 5.659 min
Delta R.T.: 0.012 min
Response: 75059
Conc: 57.60 ng/ml

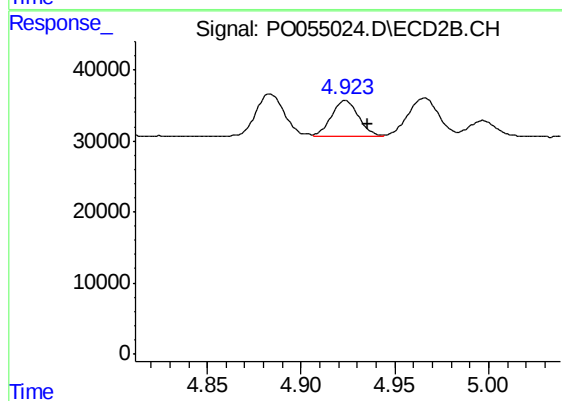

#6 AR-1016-4


R.T.: 4.924 min
Delta R.T.: -0.012 min
Response: 52149
Conc: 51.61 ng/ml

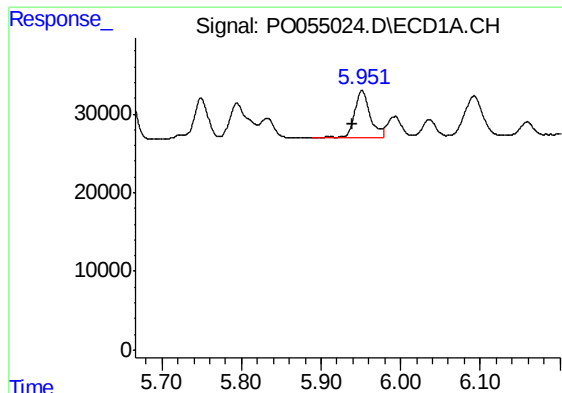

#7 AR-1016-5


R.T.: 5.951 min
Delta R.T.: 0.011 min
Response: 80881
Conc: 60.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#7 AR-1016-5

R.T.: 5.136 min
Delta R.T.: -0.012 min
Response: 62927
Conc: 48.28 ng/ml

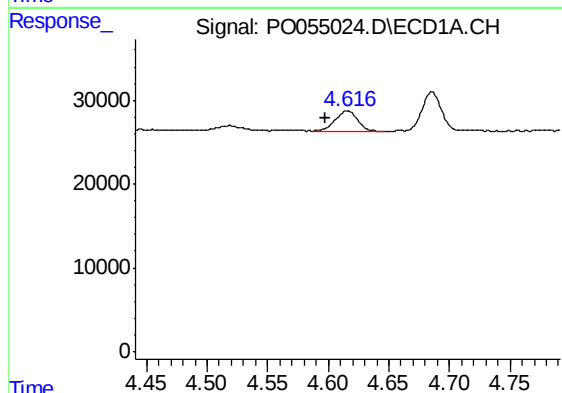


#9 AR-1221-2

R.T.: 4.616 min
Delta R.T.: 0.018 min
Response: 30704
Conc: 90.54 ng/ml

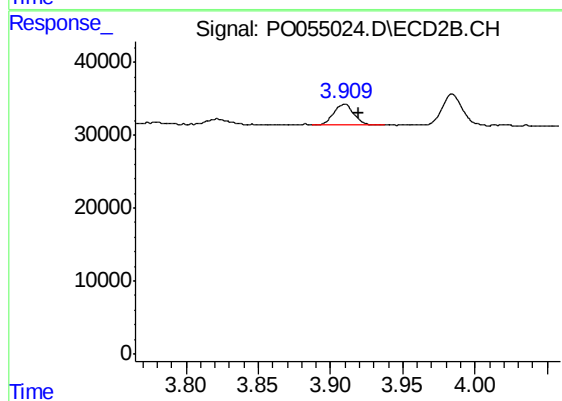

#9 AR-1221-2


R.T.: 3.910 min
Delta R.T.: -0.010 min
Response: 27829
Conc: 92.83 ng/ml

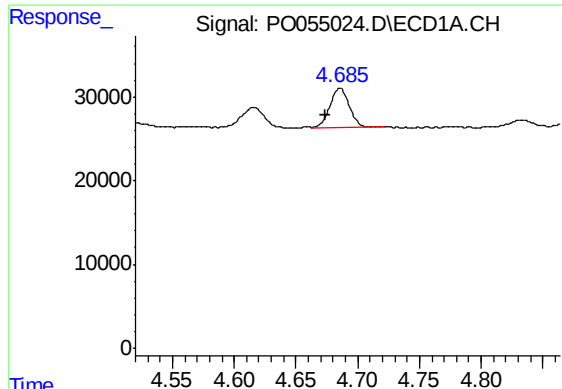

#10 AR-1221-3


R.T.: 4.685 min
Delta R.T.: 0.012 min
Response: 51300
Conc: 49.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#10 AR-1221-3

R.T.: 3.984 min
Delta R.T.: -0.012 min
Response: 42626
Conc: 46.24 ng/ml




#11 AR-1232-1

R.T.: 4.685 min
Delta R.T.: 0.011 min
Response: 51300
Conc: 59.58 ng/ml

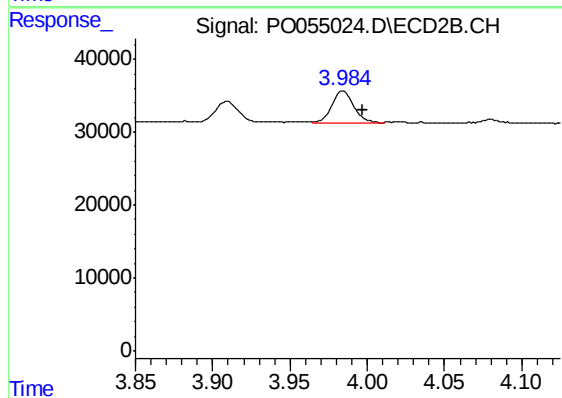

#11 AR-1232-1


R.T.: 3.984 min
Delta R.T.: -0.012 min
Response: 42626
Conc: 56.84 ng/ml



#12 AR-1232-2


R.T.: 5.211 min
Delta R.T.: 0.012 min
Response: 71337
Conc: 145.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#12 AR-1232-2

R.T.: 4.709 min
Delta R.T.: -0.012 min
Response: 115016
Conc: 133.57 ng/ml




#13 AR-1232-3

R.T.: 5.477 min
Delta R.T.: -0.011 min
Response: 99620
Conc: 101.93 ng/ml

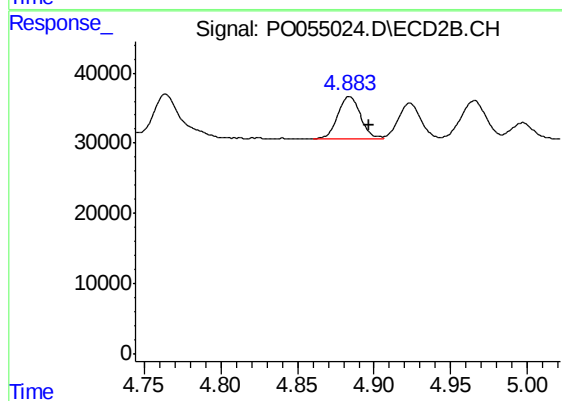

#13 AR-1232-3


R.T.: 4.883 min
Delta R.T.: -0.013 min
Response: 63360
Conc: 130.76 ng/ml

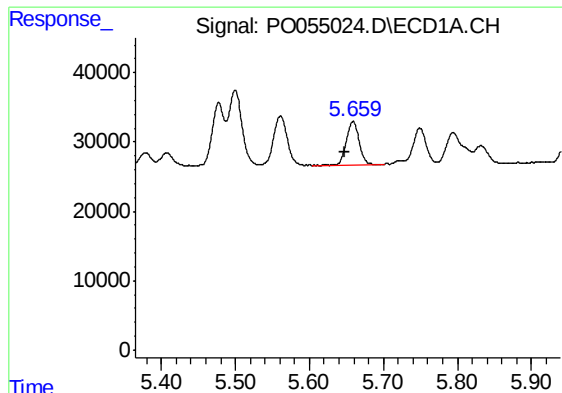

#14 AR-1232-4


R.T.: 5.659 min
Delta R.T.: 0.011 min
Response: 75059
Conc: 146.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

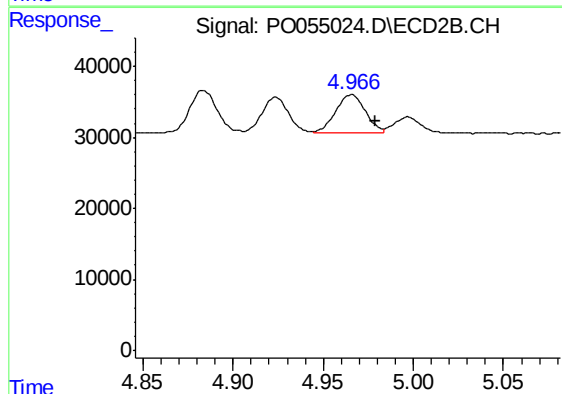


#14 AR-1232-4

R.T.: 4.966 min
Delta R.T.: -0.013 min
Response: 63173
Conc: 143.77 ng/ml

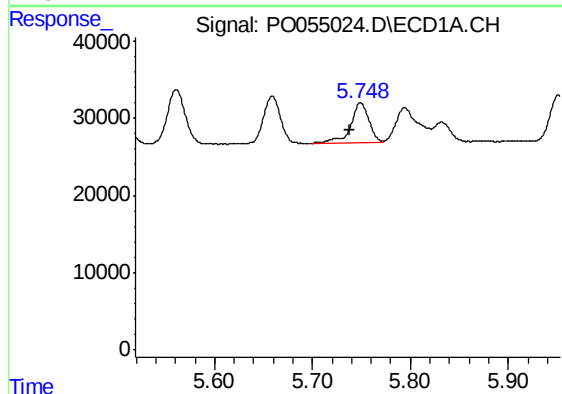


#15 AR-1232-5

R.T.: 5.749 min
Delta R.T.: 0.010 min
Response: 67673
Conc: 162.68 ng/ml

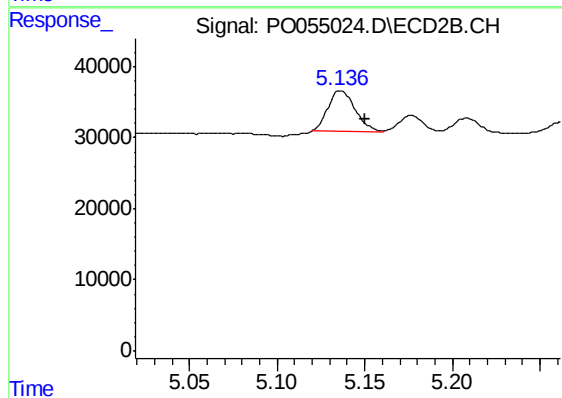

#15 AR-1232-5


R.T.: 5.136 min
Delta R.T.: -0.014 min
Response: 62927
Conc: 129.38 ng/ml



#16 AR-1242-1


R.T.: 5.477 min
Delta R.T.: 0.012 min
Response: 99620
Conc: 71.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#16 AR-1242-1

R.T.: 4.709 min
Delta R.T.: 0.008 min
Response: 115016
Conc: 93.68 ng/ml




#17 AR-1242-2

R.T.: 5.477 min
Delta R.T.: -0.010 min
Response: 99620
Conc: 52.06 ng/ml

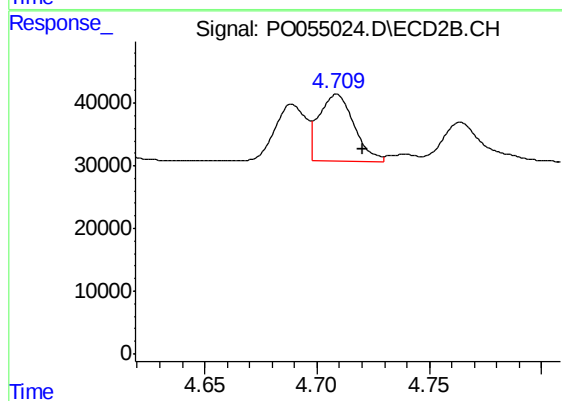

#17 AR-1242-2


R.T.: 4.709 min
Delta R.T.: -0.011 min
Response: 115016
Conc: 69.40 ng/ml



#18 AR-1242-3


R.T.: 5.561 min
Delta R.T.: 0.012 min
Response: 91232
Conc: 73.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

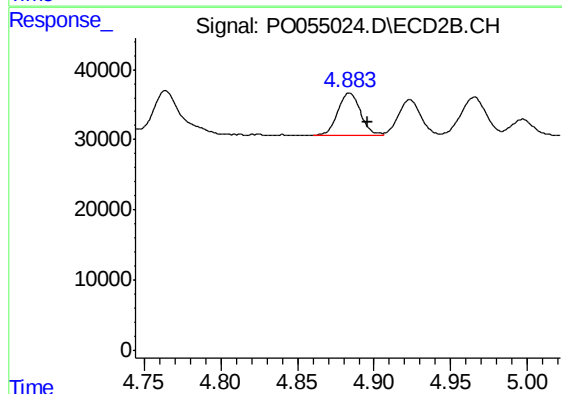


#18 AR-1242-3

R.T.: 4.883 min
Delta R.T.: -0.012 min
Response: 63360
Conc: 66.88 ng/ml




#19 AR-1242-4

R.T.: 5.659 min
Delta R.T.: 0.012 min
Response: 75059
Conc: 73.62 ng/ml

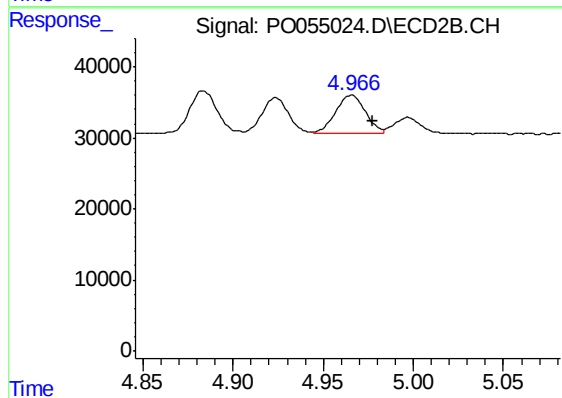

#19 AR-1242-4


R.T.: 4.966 min
Delta R.T.: -0.012 min
Response: 63173
Conc: 66.10 ng/ml

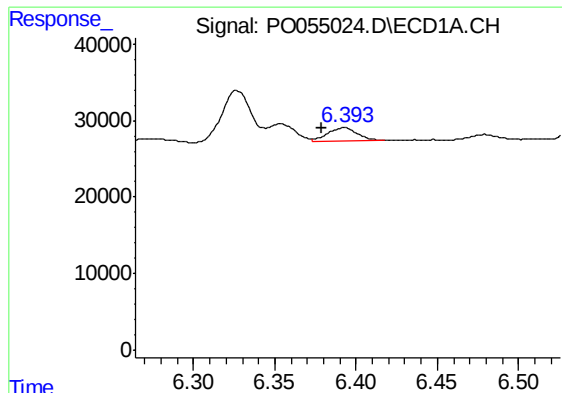

#20 AR-1242-5


R.T.: 6.392 min
Delta R.T.: 0.013 min
Response: 21799
Conc: 18.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

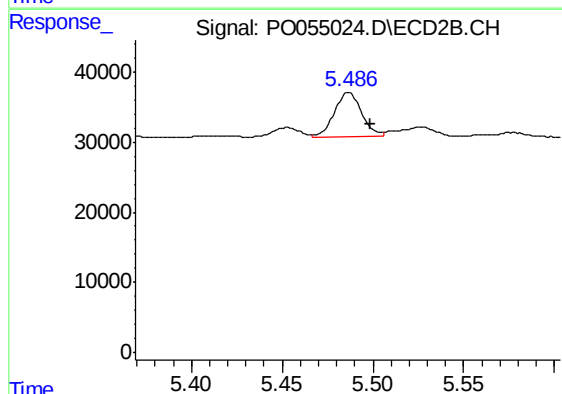


#20 AR-1242-5

R.T.: 5.487 min
Delta R.T.: -0.012 min
Response: 66567
Conc: 54.12 ng/ml

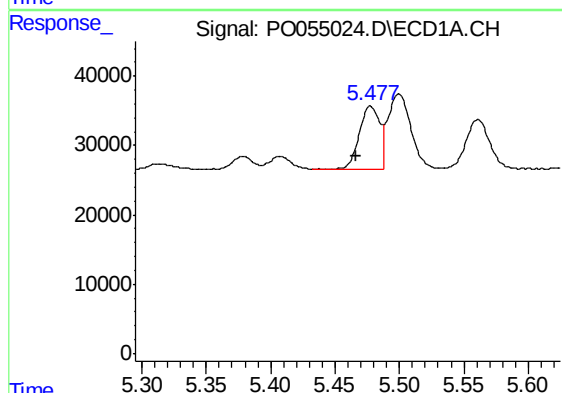


#21 AR-1248-1

R.T.: 5.477 min
Delta R.T.: 0.011 min
Response: 99620
Conc: 99.65 ng/ml

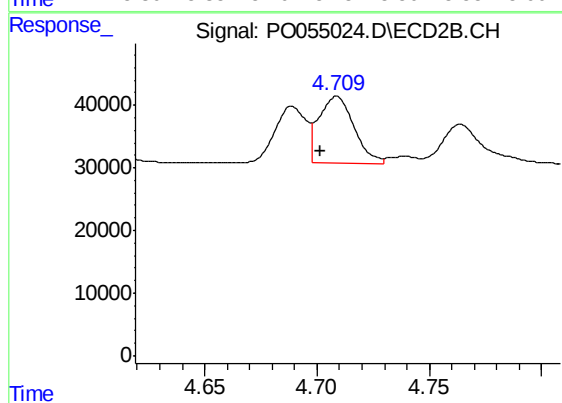

#21 AR-1248-1


R.T.: 4.709 min
Delta R.T.: 0.008 min
Response: 115016
Conc: 131.03 ng/ml

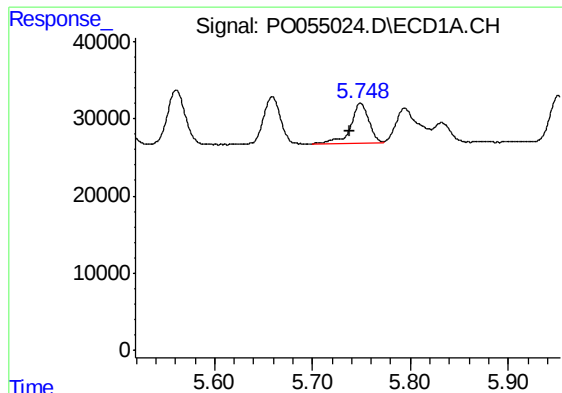

#22 AR-1248-2


R.T.: 5.749 min
Delta R.T.: 0.011 min
Response: 67673
Conc: 46.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

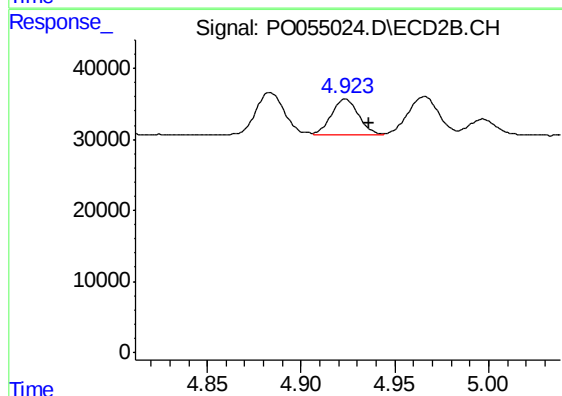


#22 AR-1248-2

R.T.: 4.924 min
Delta R.T.: -0.013 min
Response: 52149
Conc: 43.15 ng/ml

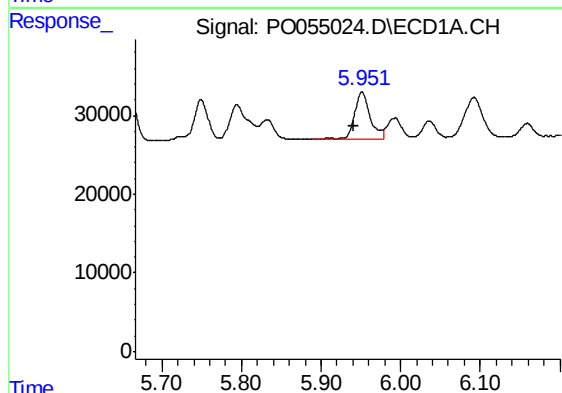


#23 AR-1248-3

R.T.: 5.951 min
Delta R.T.: 0.011 min
Response: 80881
Conc: 50.64 ng/ml

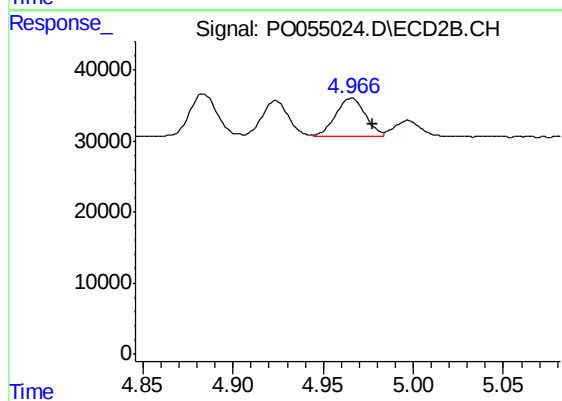

#23 AR-1248-3


R.T.: 4.966 min
Delta R.T.: -0.011 min
Response: 63173
Conc: 50.63 ng/ml



#24 AR-1248-4


R.T.: 6.354 min
Delta R.T.: 0.011 min
Response: 26182
Conc: 13.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#24 AR-1248-4

R.T.: 5.136 min
Delta R.T.: -0.013 min
Response: 62927
Conc: 41.32 ng/ml




#25 AR-1248-5

R.T.: 6.392 min
Delta R.T.: 0.012 min
Response: 21799
Conc: 12.16 ng/ml

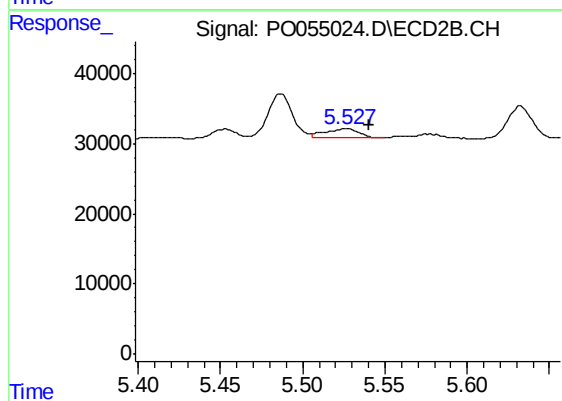

#25 AR-1248-5


R.T.: 5.527 min
Delta R.T.: -0.013 min
Response: 18989
Conc: 12.74 ng/ml

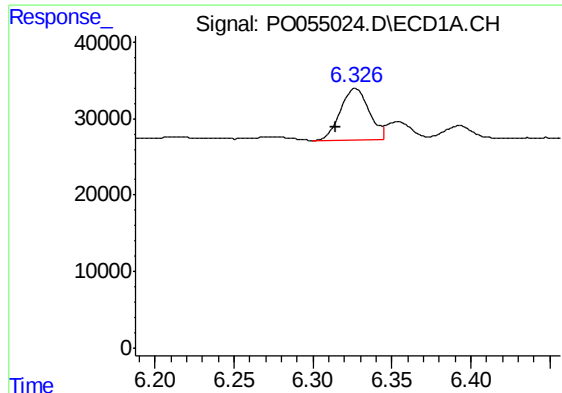

#26 AR-1254-1


R.T.: 6.327 min
Delta R.T.: 0.012 min
Response: 85574
Conc: 47.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

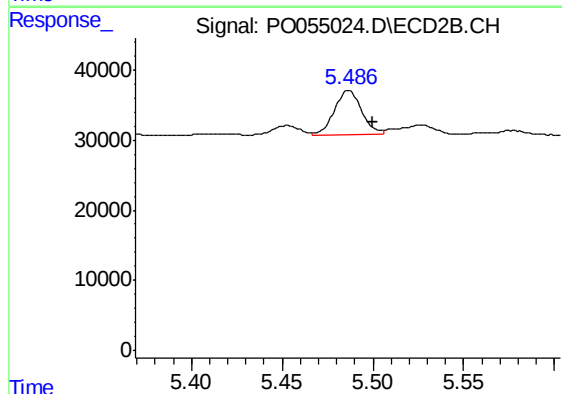


#26 AR-1254-1

R.T.: 5.487 min
Delta R.T.: -0.013 min
Response: 66567
Conc: 30.46 ng/ml

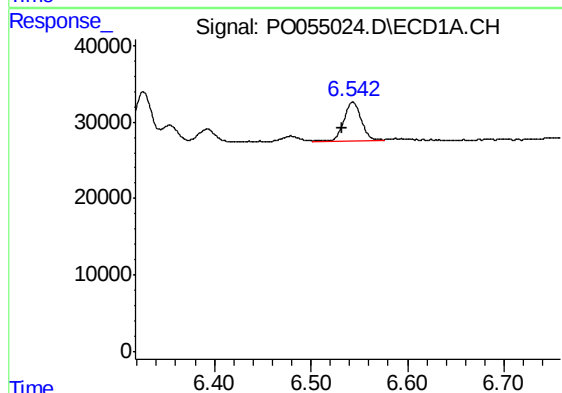


#27 AR-1254-2

R.T.: 6.543 min
Delta R.T.: 0.010 min
Response: 61524
Conc: 21.55 ng/ml

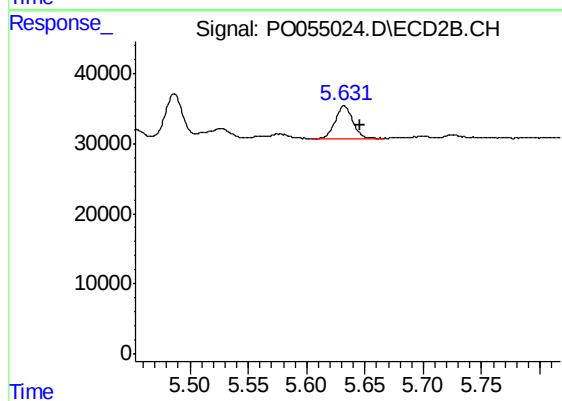

#27 AR-1254-2


R.T.: 5.632 min
Delta R.T.: -0.014 min
Response: 48402
Conc: 24.96 ng/ml



#28 AR-1254-3


R.T.: 6.914 min
Delta R.T.: 0.017 min
Response: 80408
Conc: 25.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#28 AR-1254-3

R.T.: 6.049 min
Delta R.T.: 0.000 min
Response: 88755
Conc: 27.69 ng/ml

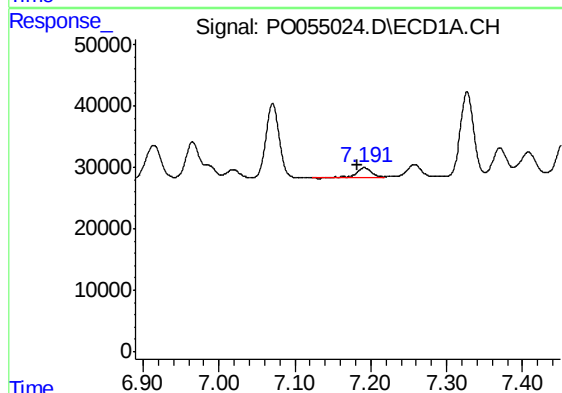


#29 AR-1254-4

R.T.: 7.192 min
Delta R.T.: 0.010 min
Response: 21414
Conc: 8.75 ng/ml

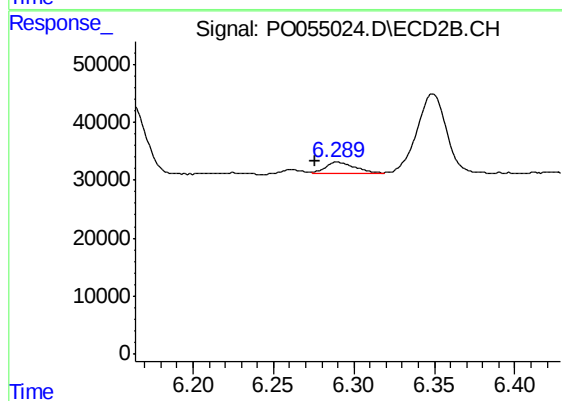

#29 AR-1254-4


R.T.: 6.290 min
Delta R.T.: 0.014 min
Response: 26265
Conc: 13.41 ng/ml



#30 AR-1254-5


R.T.: 7.609 min
Delta R.T.: 0.009 min
Response: 184515
Conc: 68.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#30 AR-1254-5

R.T.: 6.677 min
Delta R.T.: -0.015 min
Response: 149402
Conc: 51.97 ng/ml




#31 AR-1260-1

R.T.: 7.071 min
Delta R.T.: 0.011 min
Response: 147985
Conc: 58.90 ng/ml

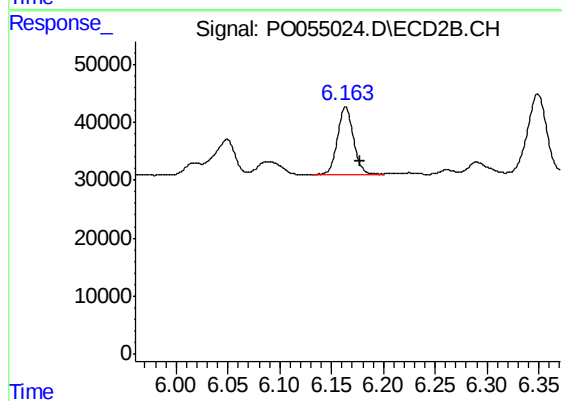

#31 AR-1260-1


R.T.: 6.164 min
Delta R.T.: -0.014 min
Response: 125488
Conc: 54.61 ng/ml



#32 AR-1260-2


R.T.: 7.327 min
Delta R.T.: 0.011 min
Response: 166152
Conc: 53.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#32 AR-1260-2

R.T.: 6.349 min
Delta R.T.: -0.014 min
Response: 176442
Conc: 64.10 ng/ml

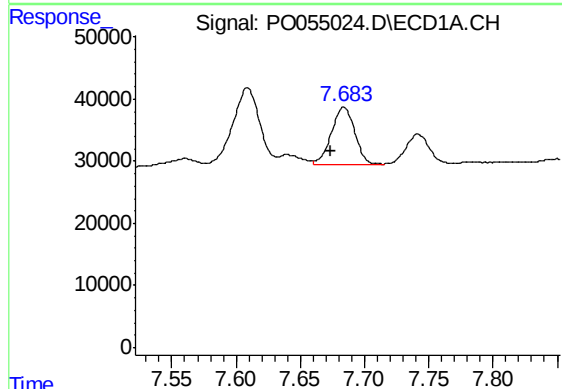


#33 AR-1260-3

R.T.: 7.684 min
Delta R.T.: 0.010 min
Response: 118121
Conc: 48.13 ng/ml

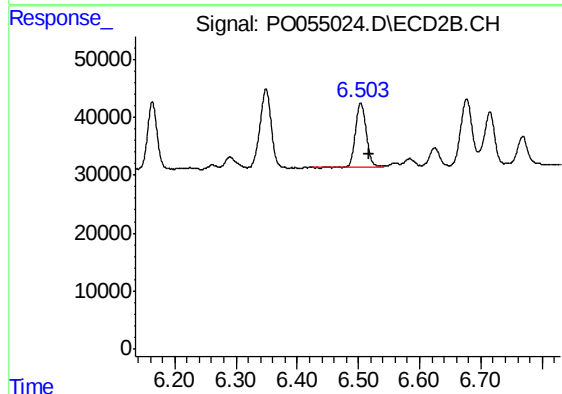

#33 AR-1260-3


R.T.: 6.504 min
Delta R.T.: -0.014 min
Response: 132349
Conc: 51.34 ng/ml



#34 AR-1260-4


R.T.: 7.908 min
Delta R.T.: 0.011 min
Response: 133182
Conc: 48.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

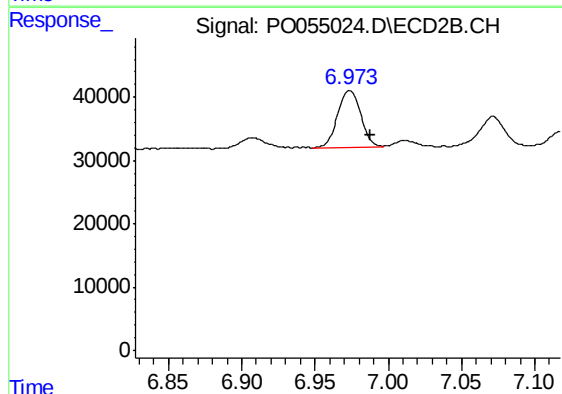


#34 AR-1260-4

R.T.: 6.974 min
Delta R.T.: -0.014 min
Response: 100771
Conc: 47.35 ng/ml




#35 AR-1260-5

R.T.: 8.219 min
Delta R.T.: 0.011 min
Response: 233856
Conc: 42.15 ng/ml

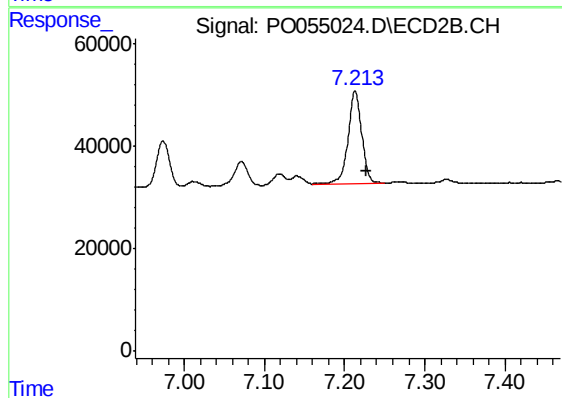

#35 AR-1260-5


R.T.: 7.213 min
Delta R.T.: -0.014 min
Response: 219084
Conc: 45.74 ng/ml



#36 AR-1262-1


R.T.: 7.684 min
Delta R.T.: 0.009 min
Response: 118121
Conc: 35.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#36 AR-1262-1

R.T.: 6.715 min
Delta R.T.: -0.015 min
Response: 114492
Conc: 38.49 ng/ml

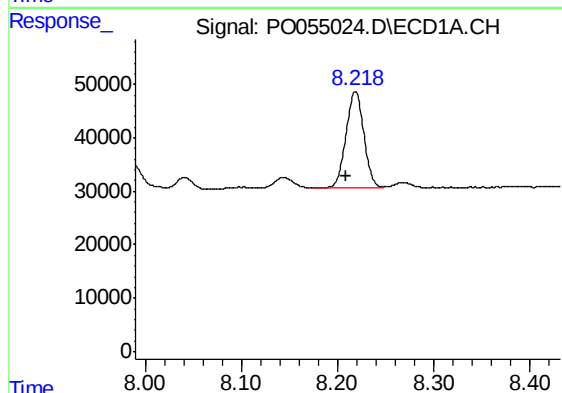


#37 AR-1262-2

R.T.: 8.219 min
Delta R.T.: 0.010 min
Response: 233856
Conc: 39.47 ng/ml

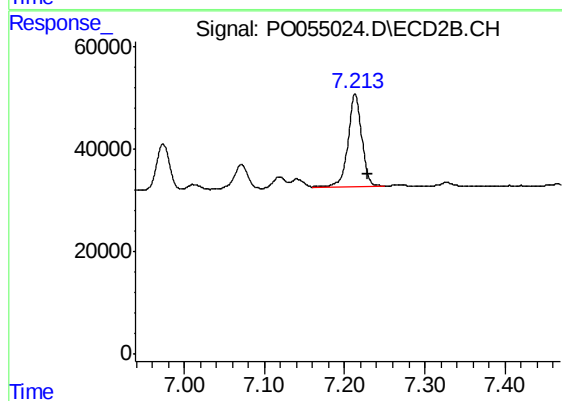

#37 AR-1262-2


R.T.: 7.213 min
Delta R.T.: -0.015 min
Response: 219084
Conc: 44.70 ng/ml



#38 AR-1262-3


R.T.: 8.531 min
Delta R.T.: 0.024 min
Response: 178495
Conc: 43.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

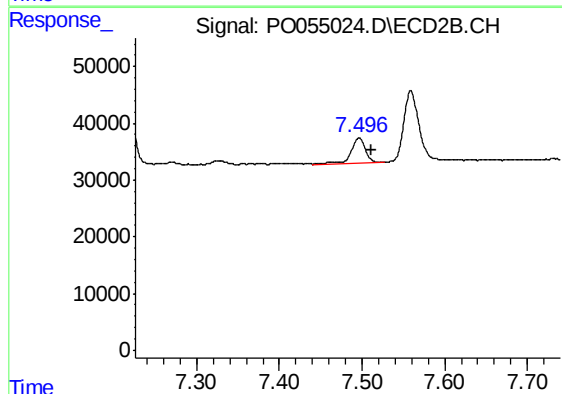


#38 AR-1262-3

R.T.: 7.496 min
Delta R.T.: -0.015 min
Response: 52970
Conc: 25.80 ng/ml




#39 AR-1262-4

R.T.: 8.584 min
Delta R.T.: -0.009 min
Response: 98139
Conc: 30.46 ng/ml

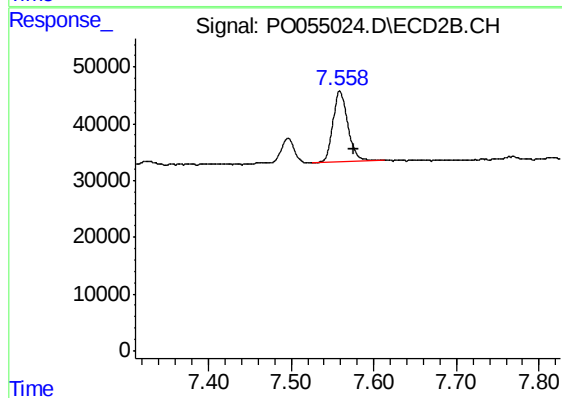

#39 AR-1262-4


R.T.: 7.559 min
Delta R.T.: -0.016 min
Response: 158954
Conc: 43.88 ng/ml



#40 AR-1262-5


R.T.: 9.231 min
Delta R.T.: 0.013 min
Response: 64640
Conc: 29.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#40 AR-1262-5

R.T.: 8.052 min
Delta R.T.: -0.015 min
Response: 52737
Conc: 32.68 ng/ml

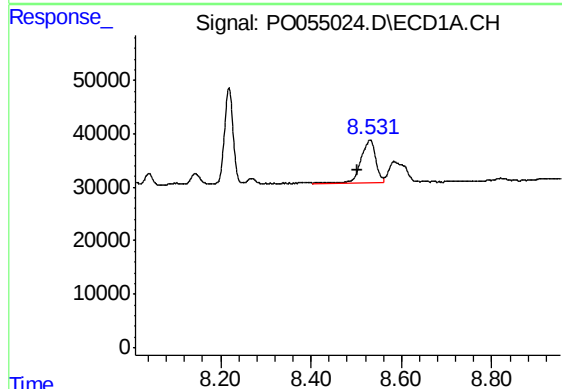


#41 AR-1268-1

R.T.: 8.531 min
Delta R.T.: 0.027 min
Response: 178495
Conc: 25.08 ng/ml

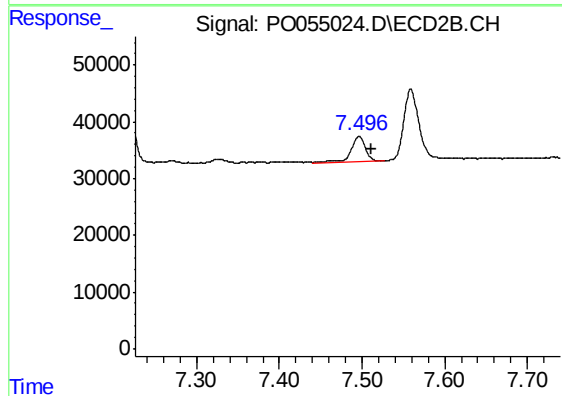

#41 AR-1268-1


R.T.: 7.496 min
Delta R.T.: -0.015 min
Response: 52970
Conc: 9.37 ng/ml



#42 AR-1268-2


R.T.: 8.584 min
Delta R.T.: -0.011 min
Response: 98139
Conc: 14.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#42 AR-1268-2

R.T.: 7.559 min
Delta R.T.: -0.016 min
Response: 158954
Conc: 30.74 ng/ml




#44 AR-1268-4

R.T.: 9.231 min
Delta R.T.: 0.014 min
Response: 64640
Conc: 27.09 ng/ml

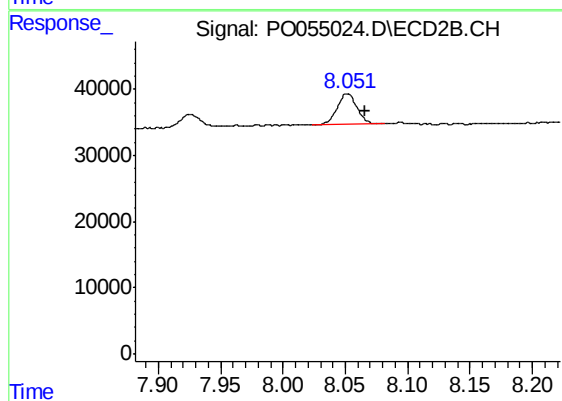

#44 AR-1268-4


R.T.: 8.052 min
Delta R.T.: -0.014 min
Response: 52737
Conc: 28.45 ng/ml

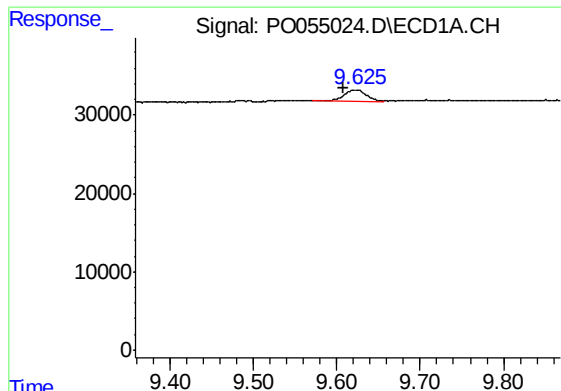

#45 AR-1268-5

R.T.: 9.624 min
Delta R.T.: 0.017 min
Response: 25885
Conc: 1.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

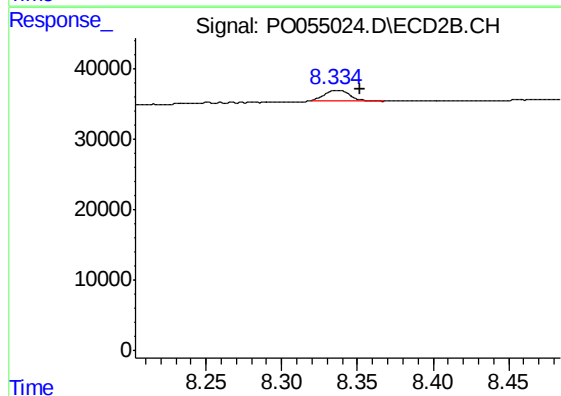

#45 AR-1268-5

R.T.: 8.336 min
Delta R.T.: -0.016 min
Response: 17315
Conc: 1.52 ng/ml