

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040819\
 Data File : P0055025.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Apr 2019 10:25
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1660 LOD 40PPB
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 06:47:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.300	3.611	1236970	1156390	35.642	36.236
2)	SA Decachlor...	9.920	8.582	1259792	876741	25.555	27.529
Target Compounds							
3)	L1 AR-1016-1	5.463	4.707	135283	161619	75.181	102.200 #
4)	L1 AR-1016-2	5.485	4.707	184768	161619	74.393	75.426
5)	L1 AR-1016-3	5.546	4.882	124370	88780	79.053	73.480
6)	L1 AR-1016-4	5.645	4.922	101461	73335	77.863	72.570
7)	L1 AR-1016-5	5.937	5.135	102269	79221	76.648	60.780
8)	L2 AR-1221-1	0.000	3.823	0	10141	N.D.	26.082 #
9)	L2 AR-1221-2	4.600	3.908	33368	27874	98.397	92.979
10)	L2 AR-1221-3	4.672	3.983	70291	57660	67.667	62.553
11)	L3 AR-1232-1	4.672	3.983	70291	57660	81.642	76.891
12)	L3 AR-1232-2	5.197	4.707	96772	161619	197.842	187.688
13)	L3 AR-1232-3	5.485	4.882	184768	88780	189.060	183.216
14)	L3 AR-1232-4	5.645	4.994	101461	31503	198.223	71.696 #
15)	L3 AR-1232-5	5.734	5.135	97036	79221	233.260	162.886 #
16)	L4 AR-1242-1	5.463	4.707	135283	161619	97.376	131.642 #
17)	L4 AR-1242-2	5.485	4.707	184768	161619	96.562	97.524
18)	L4 AR-1242-3	5.546	4.882	124370	88780	100.343	93.716
19)	L4 AR-1242-4	5.645	4.963	101461	89133	99.516	93.260
20)	L4 AR-1242-5	6.377	5.484	29244	96487	24.225	78.451 #
21)	L5 AR-1248-1	5.463	4.707	135283	161619	135.327	184.123 #
22)	L5 AR-1248-2	5.734	4.922	97036	73335	66.815	60.680
23)	L5 AR-1248-3	5.937	4.963	102269	89133	64.031	71.433
24)	L5 AR-1248-4	6.339	5.135	36689	79221	19.531	52.017 #
25)	L5 AR-1248-5	6.377	5.525	29244	25649	16.312	17.204
26)	L6 AR-1254-1	6.311	5.484	104850	96487	57.827	44.149
27)	L6 AR-1254-2	6.529	5.630	88349	68862	30.948	35.515
28)	L6 AR-1254-3	6.896	6.047	58680	126974	18.660	39.609 #
29)	L6 AR-1254-4	7.179	6.287	29158	40350	11.919	20.608 #
30)	L6 AR-1254-5	7.595	6.674	256222	210957	95.595	73.384
31)	L7 AR-1260-1	7.057	6.161	203313	178054	80.916	77.480
32)	L7 AR-1260-2	7.314	6.347	243907	218672	78.590	79.437
33)	L7 AR-1260-3	7.671	6.501	163032	192175	66.426	74.547
34)	L7 AR-1260-4	7.895	6.971	184975	147045	66.874	69.095
35)	L7 AR-1260-5	8.205	7.210	328898	300229	59.276	62.687
36)	L8 AR-1262-1	7.671	6.712	163032	159412	48.928	53.585
37)	L8 AR-1262-2	8.205	7.210	328898	300229	55.516	61.257
38)	L8 AR-1262-3	8.517	7.493	209213	71802	50.501	34.966 #
39)	L8 AR-1262-4	8.571	7.556	128293	217081	39.818	59.932 #
40)	L8 AR-1262-5	9.214	8.048	87962	78676	40.234	48.749
41)	L9 AR-1268-1	8.517	7.493	209213	71802	29.394	12.699 #
42)	L9 AR-1268-2	8.571	7.556	128293	217081	19.581	41.976 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040819\
 Data File : P0055025.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Apr 2019 10:25
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1660 LOD 40PPB
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 06:47:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	0.000	7.765	0	11942	N.D.	2.775 #
44) L9	AR-1268-4	9.214	8.048	87962	78676	36.869	42.439
45) L9	AR-1268-5	9.605	8.332	31911	16096	1.937	1.414 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040819\
Data File : PO055025.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Apr 2019 10:25
Operator : SM/SJ
Sample : K1560-07
Misc : AR1660 LOD 40PPB
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 06:47:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

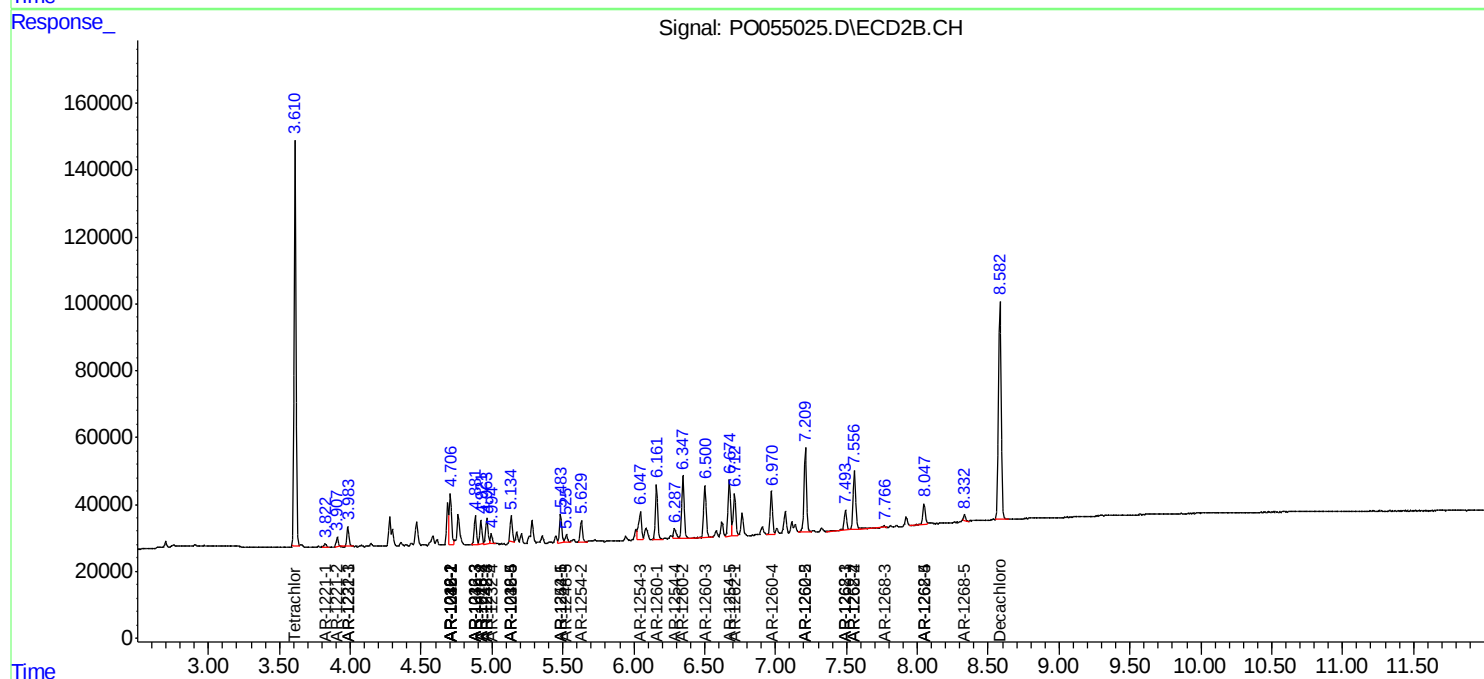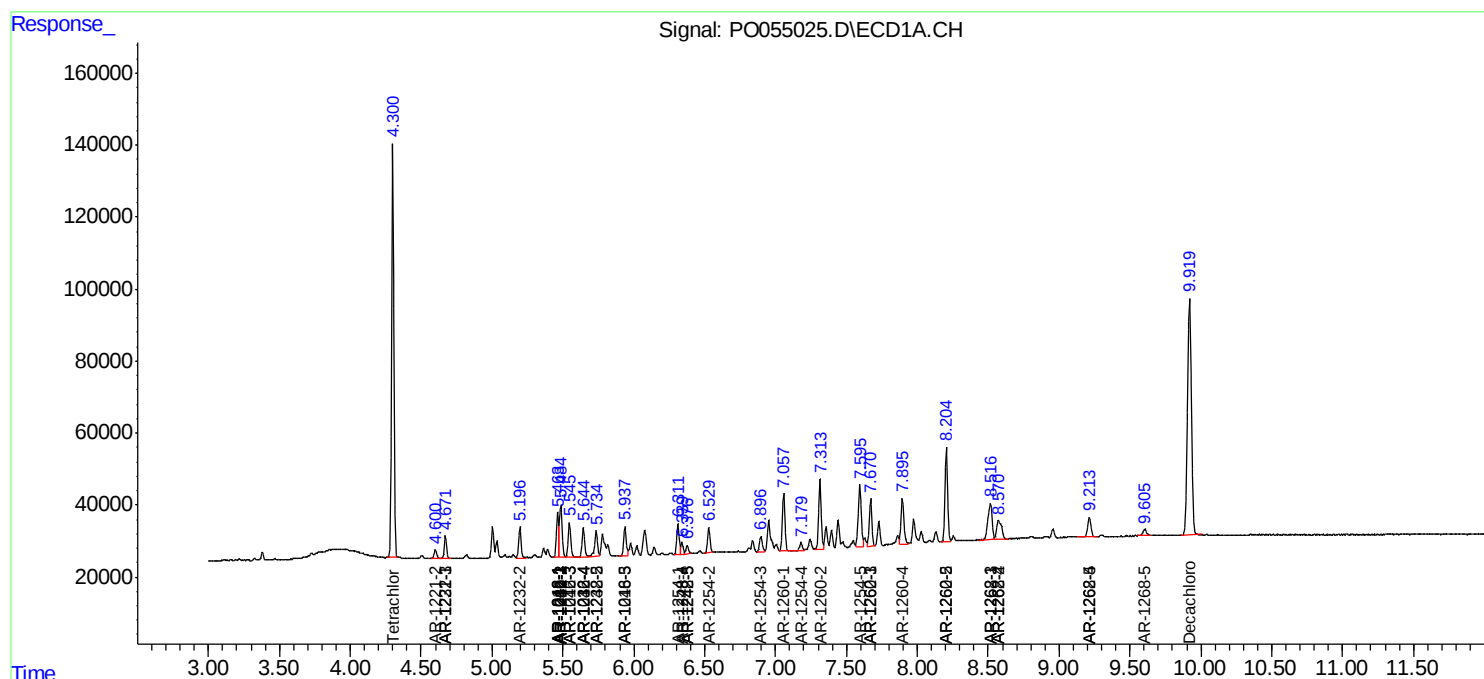




#1 Tetrachloro-m-xylene


R.T.: 4.300 min
Delta R.T.: -0.003 min
Response: 1236970
Conc: 35.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: -0.010 min
Response: 1156390
Conc: 36.24 ng/ml

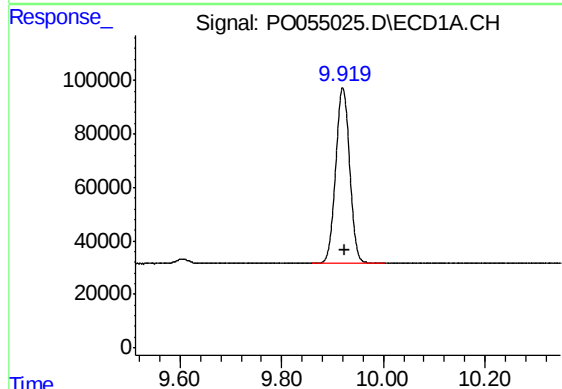


#2 Decachlorobiphenyl

R.T.: 9.920 min
Delta R.T.: -0.003 min
Response: 1259792
Conc: 25.55 ng/ml

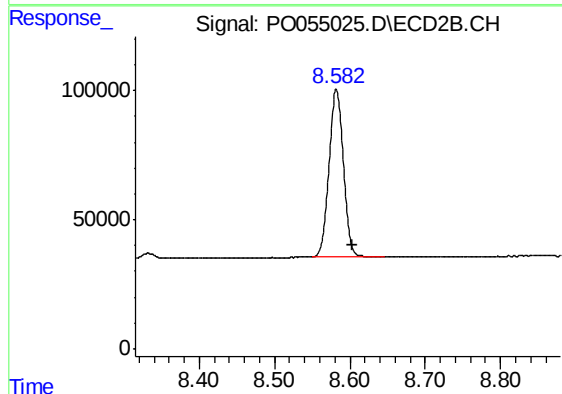

#2 Decachlorobiphenyl


R.T.: 8.582 min
Delta R.T.: -0.022 min
Response: 876741
Conc: 27.53 ng/ml

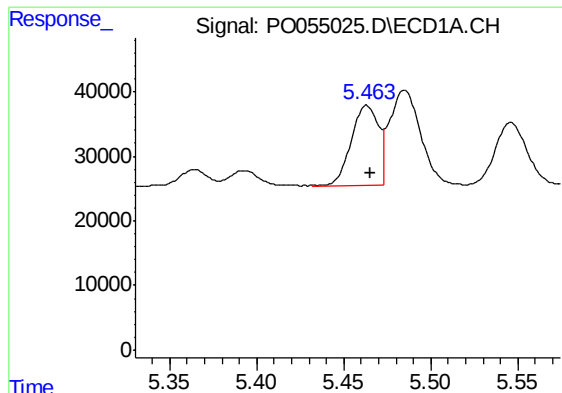

#3 AR-1016-1


R.T.: 5.463 min
Delta R.T.: -0.002 min
Response: 135283
Conc: 75.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

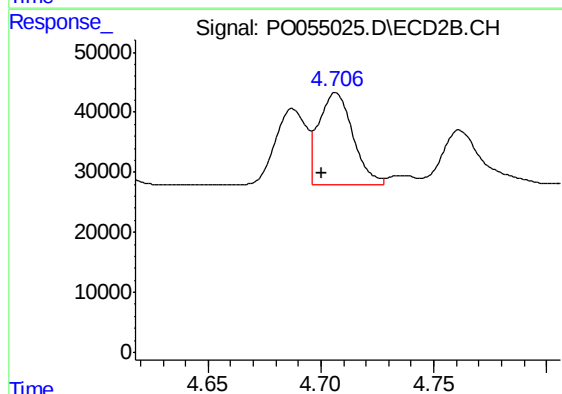


#3 AR-1016-1

R.T.: 4.707 min
Delta R.T.: 0.006 min
Response: 161619
Conc: 102.20 ng/ml

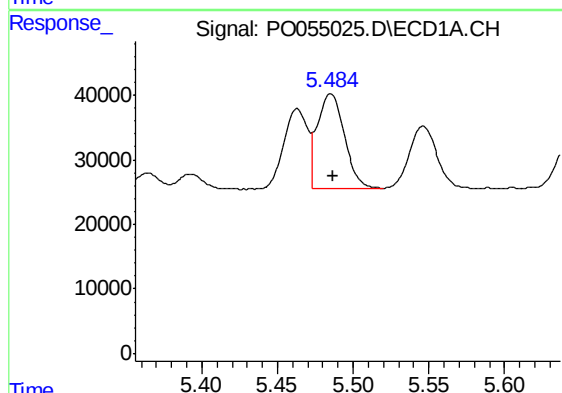


#4 AR-1016-2

R.T.: 5.485 min
Delta R.T.: -0.002 min
Response: 184768
Conc: 74.39 ng/ml

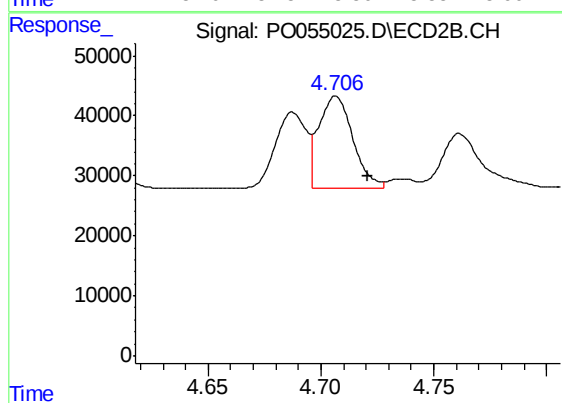

#4 AR-1016-2


R.T.: 4.707 min
Delta R.T.: -0.014 min
Response: 161619
Conc: 75.43 ng/ml



#5 AR-1016-3


R.T.: 5.546 min
Delta R.T.: -0.002 min
Response: 124370
Conc: 79.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

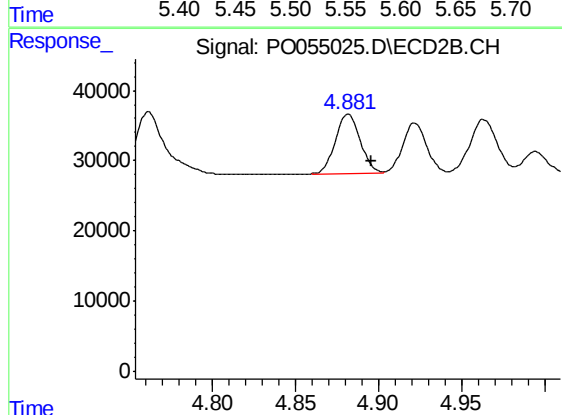


#5 AR-1016-3

R.T.: 4.882 min
Delta R.T.: -0.014 min
Response: 88780
Conc: 73.48 ng/ml

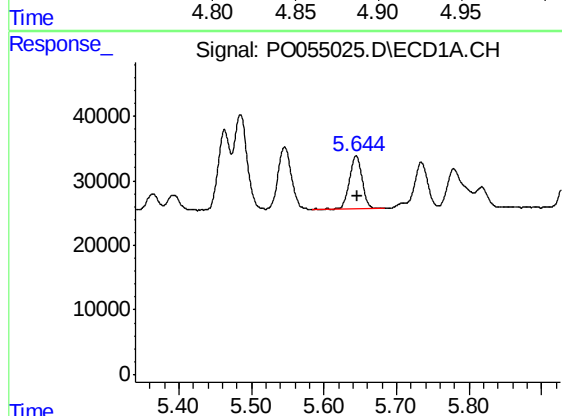


#6 AR-1016-4

R.T.: 5.645 min
Delta R.T.: -0.002 min
Response: 101461
Conc: 77.86 ng/ml

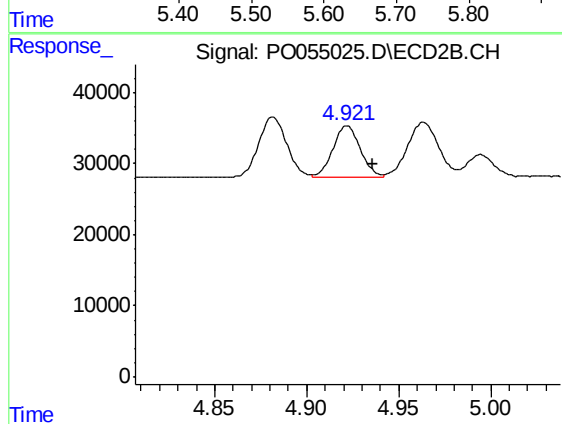

#6 AR-1016-4


R.T.: 4.922 min
Delta R.T.: -0.014 min
Response: 73335
Conc: 72.57 ng/ml



#7 AR-1016-5


R.T.: 5.937 min
Delta R.T.: -0.002 min
Response: 102269
Conc: 76.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#7 AR-1016-5

R.T.: 5.135 min
Delta R.T.: -0.014 min
Response: 79221
Conc: 60.78 ng/ml




#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.512 min
Response: 0
Conc: N.D.

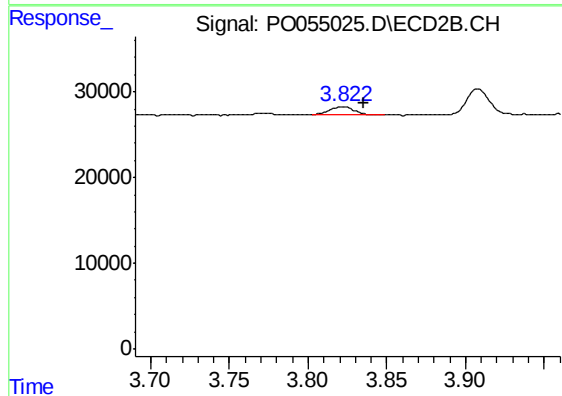

#8 AR-1221-1


R.T.: 3.823 min
Delta R.T.: -0.013 min
Response: 10141
Conc: 26.08 ng/ml

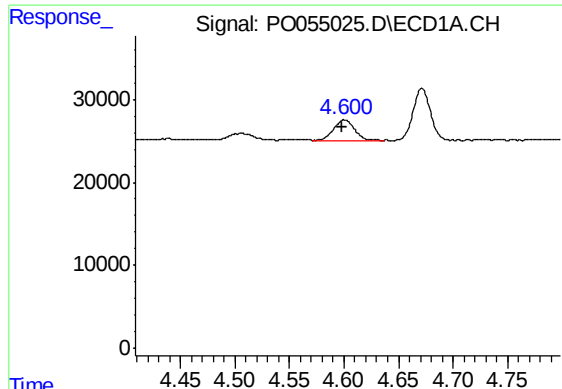

#9 AR-1221-2


R.T.: 4.600 min
Delta R.T.: 0.002 min
Response: 33368
Conc: 98.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

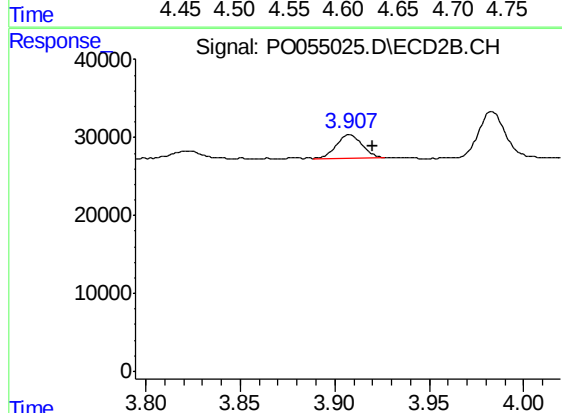


#9 AR-1221-2

R.T.: 3.908 min
Delta R.T.: -0.012 min
Response: 27874
Conc: 92.98 ng/ml

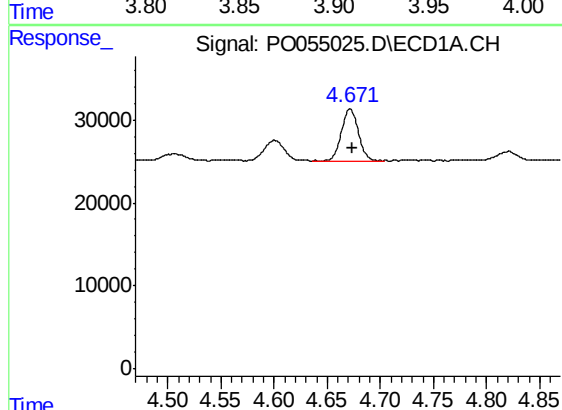


#10 AR-1221-3

R.T.: 4.672 min
Delta R.T.: -0.002 min
Response: 70291
Conc: 67.67 ng/ml

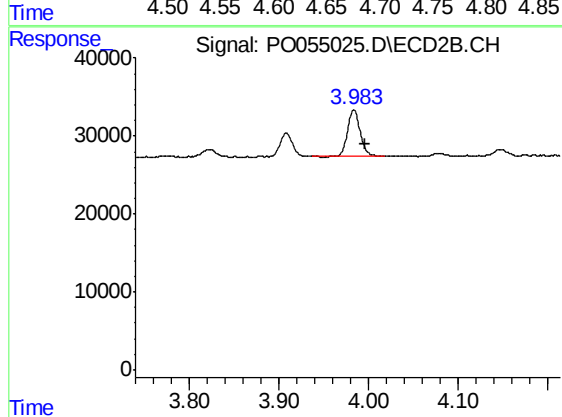

#10 AR-1221-3


R.T.: 3.983 min
Delta R.T.: -0.013 min
Response: 57660
Conc: 62.55 ng/ml

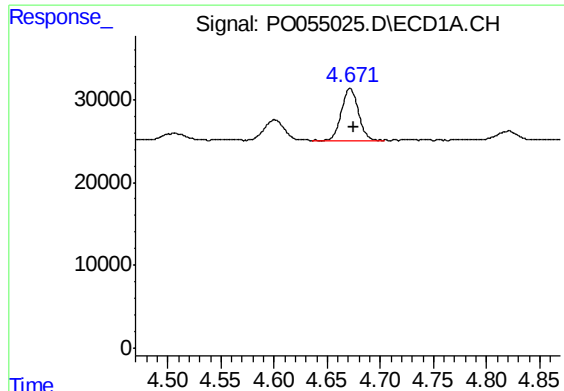

#11 AR-1232-1


R.T.: 4.672 min
Delta R.T.: -0.003 min
Response: 70291
Conc: 81.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

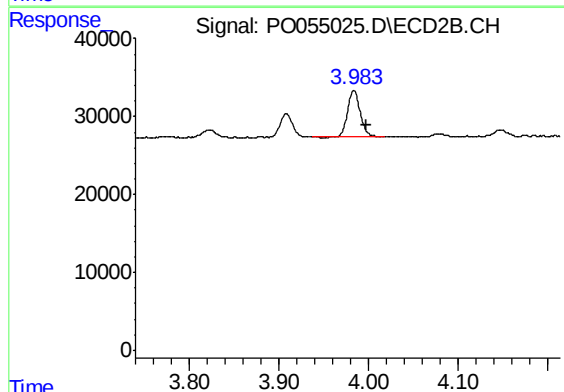


#11 AR-1232-1

R.T.: 3.983 min
Delta R.T.: -0.013 min
Response: 57660
Conc: 76.89 ng/ml

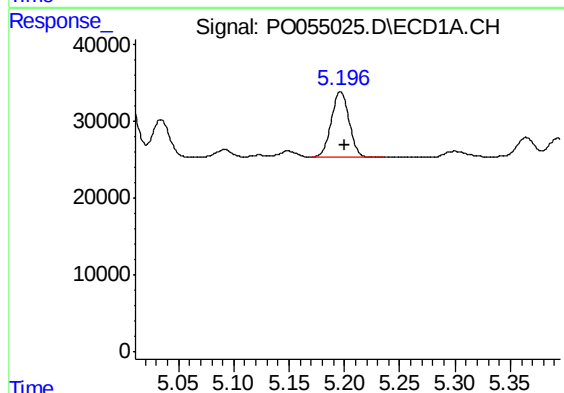


#12 AR-1232-2

R.T.: 5.197 min
Delta R.T.: -0.003 min
Response: 96772
Conc: 197.84 ng/ml

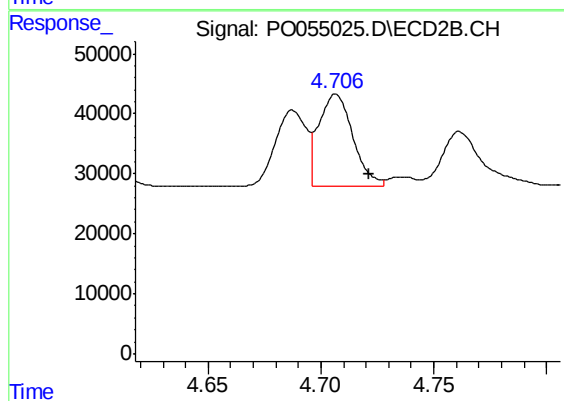

#12 AR-1232-2


R.T.: 4.707 min
Delta R.T.: -0.014 min
Response: 161619
Conc: 187.69 ng/ml

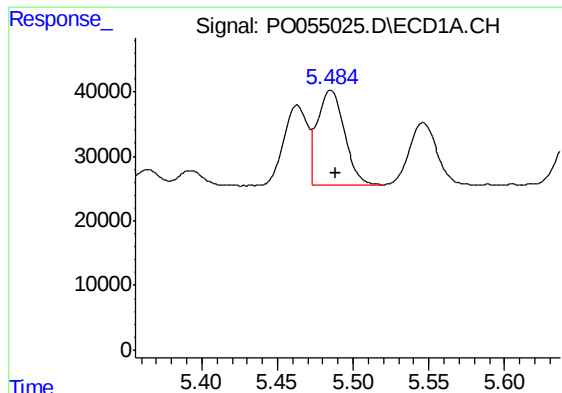

#13 AR-1232-3


R.T.: 5.485 min
Delta R.T.: -0.003 min
Response: 184768
Conc: 189.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

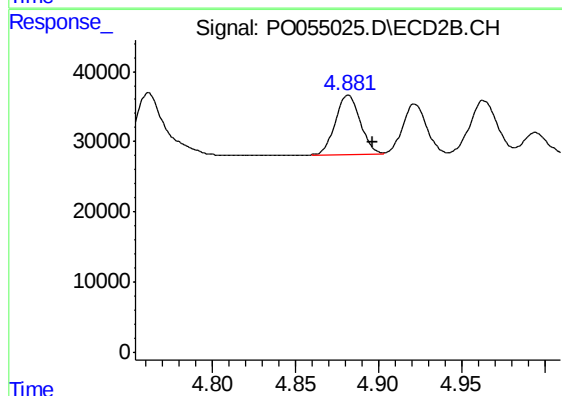


#13 AR-1232-3

R.T.: 4.882 min
Delta R.T.: -0.015 min
Response: 88780
Conc: 183.22 ng/ml

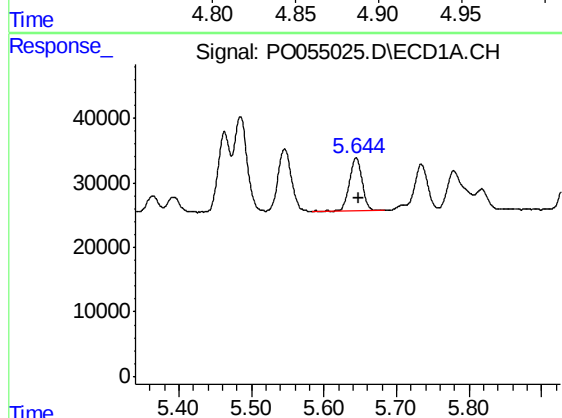


#14 AR-1232-4

R.T.: 5.645 min
Delta R.T.: -0.003 min
Response: 101461
Conc: 198.22 ng/ml

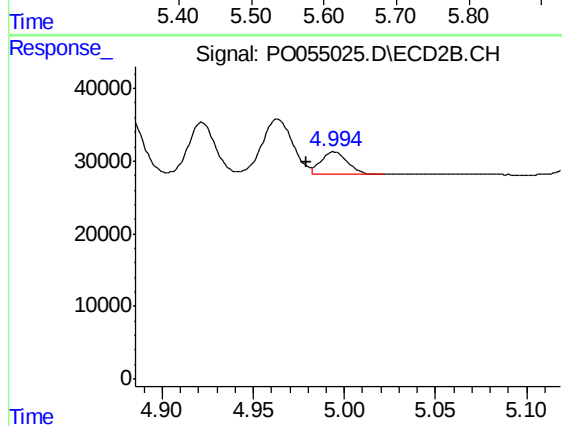

#14 AR-1232-4


R.T.: 4.994 min
Delta R.T.: 0.016 min
Response: 31503
Conc: 71.70 ng/ml



#15 AR-1232-5


R.T.: 5.734 min
Delta R.T.: -0.004 min
Response: 97036
Conc: 233.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#15 AR-1232-5

R.T.: 5.135 min
Delta R.T.: -0.015 min
Response: 79221
Conc: 162.89 ng/ml




#16 AR-1242-1

R.T.: 5.463 min
Delta R.T.: -0.002 min
Response: 135283
Conc: 97.38 ng/ml

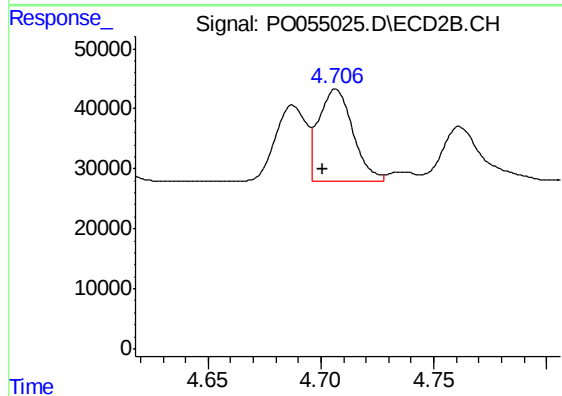

#16 AR-1242-1


R.T.: 4.707 min
Delta R.T.: 0.006 min
Response: 161619
Conc: 131.64 ng/ml



#17 AR-1242-2


R.T.: 5.485 min
Delta R.T.: -0.002 min
Response: 184768
Conc: 96.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#17 AR-1242-2

R.T.: 4.707 min
Delta R.T.: -0.014 min
Response: 161619
Conc: 97.52 ng/ml




#18 AR-1242-3

R.T.: 5.546 min
Delta R.T.: -0.003 min
Response: 124370
Conc: 100.34 ng/ml

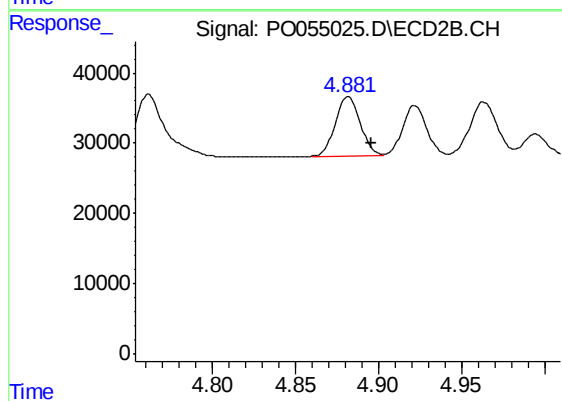

#18 AR-1242-3


R.T.: 4.882 min
Delta R.T.: -0.014 min
Response: 88780
Conc: 93.72 ng/ml



#19 AR-1242-4


R.T.: 5.645 min
Delta R.T.: -0.002 min
Response: 101461
Conc: 99.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#19 AR-1242-4

R.T.: 4.963 min
Delta R.T.: -0.015 min
Response: 89133
Conc: 93.26 ng/ml




#20 AR-1242-5

R.T.: 6.377 min
Delta R.T.: -0.002 min
Response: 29244
Conc: 24.23 ng/ml

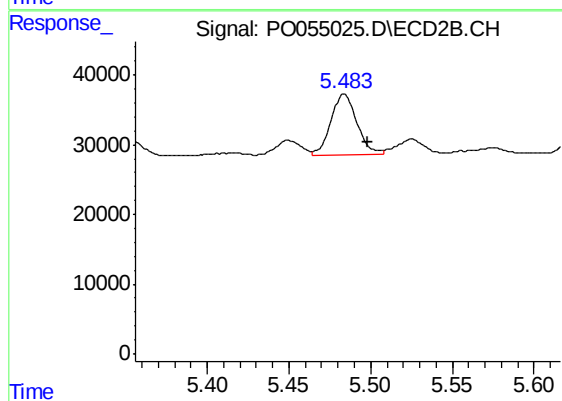

#20 AR-1242-5


R.T.: 5.484 min
Delta R.T.: -0.015 min
Response: 96487
Conc: 78.45 ng/ml



#21 AR-1248-1


R.T.: 5.463 min
Delta R.T.: -0.003 min
Response: 135283
Conc: 135.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#21 AR-1248-1

R.T.: 4.707 min
Delta R.T.: 0.005 min
Response: 161619
Conc: 184.12 ng/ml




#22 AR-1248-2

R.T.: 5.734 min
Delta R.T.: -0.003 min
Response: 97036
Conc: 66.81 ng/ml

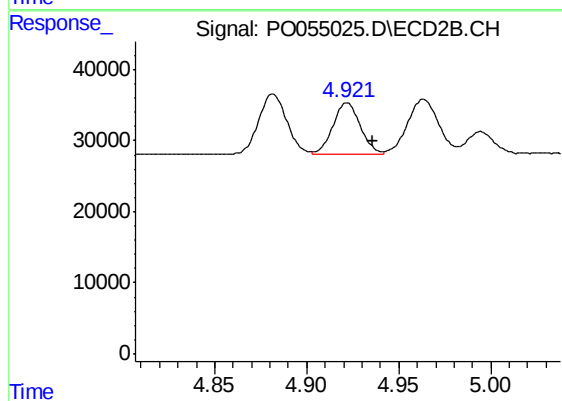

#22 AR-1248-2


R.T.: 4.922 min
Delta R.T.: -0.014 min
Response: 73335
Conc: 60.68 ng/ml

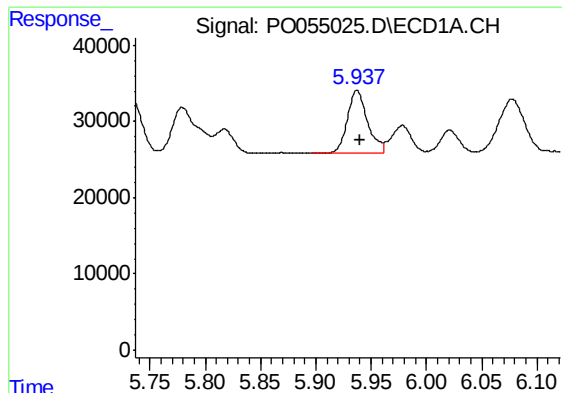

#23 AR-1248-3


R.T.: 5.937 min
Delta R.T.: -0.003 min
Response: 102269
Conc: 64.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

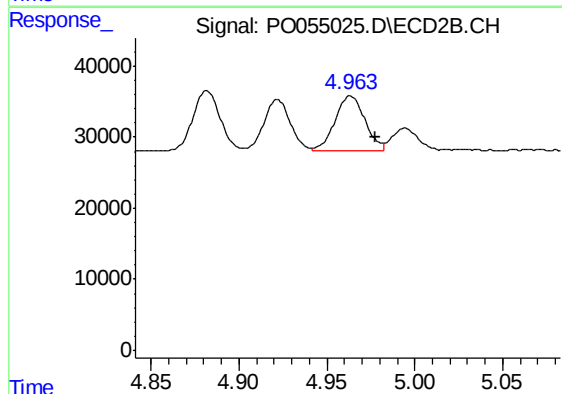


#23 AR-1248-3

R.T.: 4.963 min
Delta R.T.: -0.014 min
Response: 89133
Conc: 71.43 ng/ml

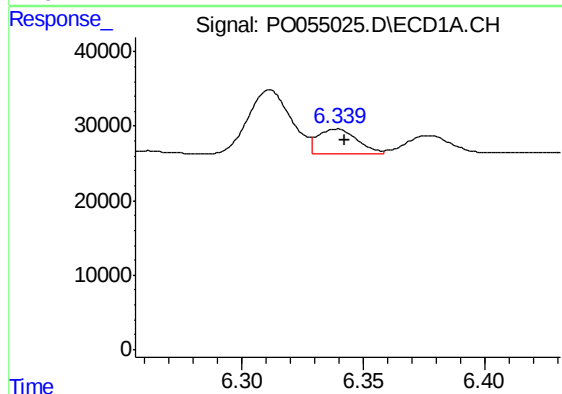


#24 AR-1248-4

R.T.: 6.339 min
Delta R.T.: -0.003 min
Response: 36689
Conc: 19.53 ng/ml

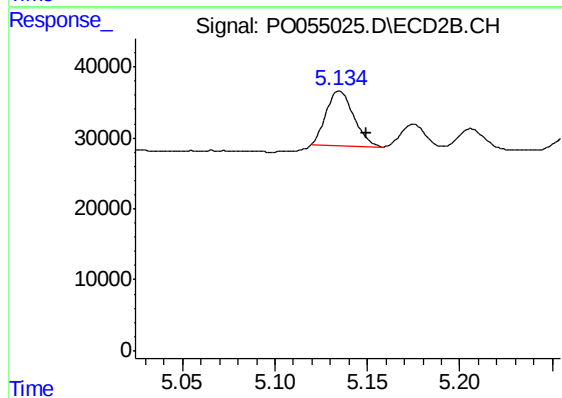

#24 AR-1248-4


R.T.: 5.135 min
Delta R.T.: -0.015 min
Response: 79221
Conc: 52.02 ng/ml



#25 AR-1248-5


R.T.: 6.377 min
Delta R.T.: -0.003 min
Response: 29244
Conc: 16.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#25 AR-1248-5

R.T.: 5.525 min
Delta R.T.: -0.015 min
Response: 25649
Conc: 17.20 ng/ml

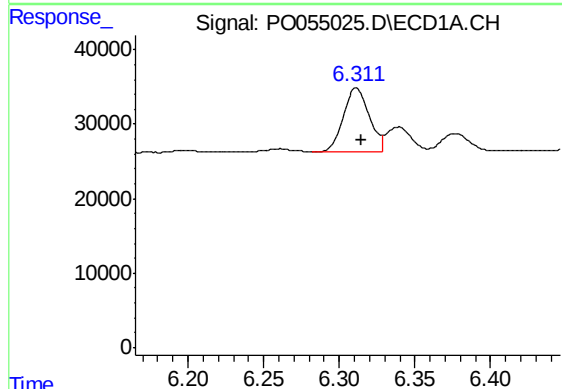


#26 AR-1254-1

R.T.: 6.311 min
Delta R.T.: -0.003 min
Response: 104850
Conc: 57.83 ng/ml

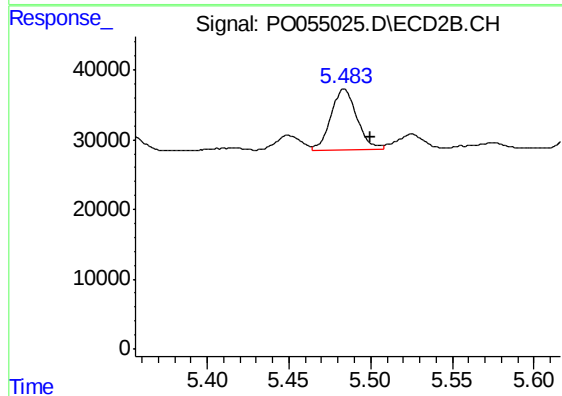

#26 AR-1254-1


R.T.: 5.484 min
Delta R.T.: -0.016 min
Response: 96487
Conc: 44.15 ng/ml

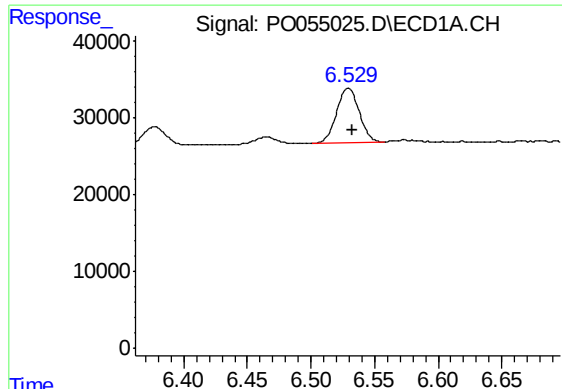

#27 AR-1254-2


R.T.: 6.529 min
Delta R.T.: -0.004 min
Response: 88349
Conc: 30.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#27 AR-1254-2

R.T.: 5.630 min
Delta R.T.: -0.016 min
Response: 68862
Conc: 35.52 ng/ml




#28 AR-1254-3

R.T.: 6.896 min
Delta R.T.: 0.000 min
Response: 58680
Conc: 18.66 ng/ml

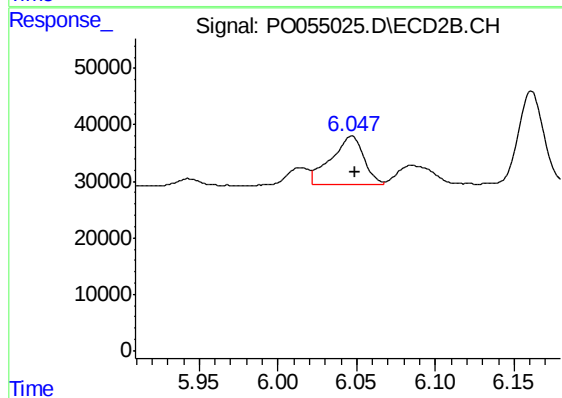

#28 AR-1254-3


R.T.: 6.047 min
Delta R.T.: -0.002 min
Response: 126974
Conc: 39.61 ng/ml

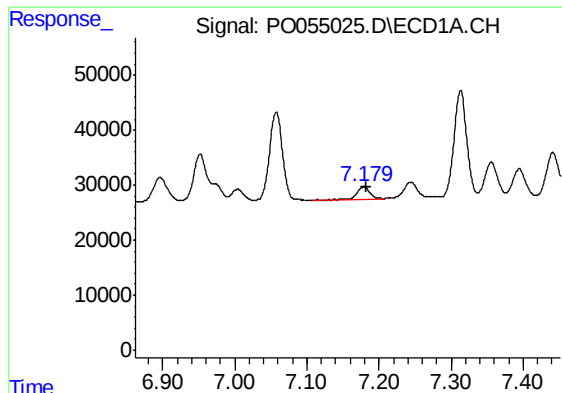

#29 AR-1254-4


R.T.: 7.179 min
Delta R.T.: -0.003 min
Response: 29158
Conc: 11.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

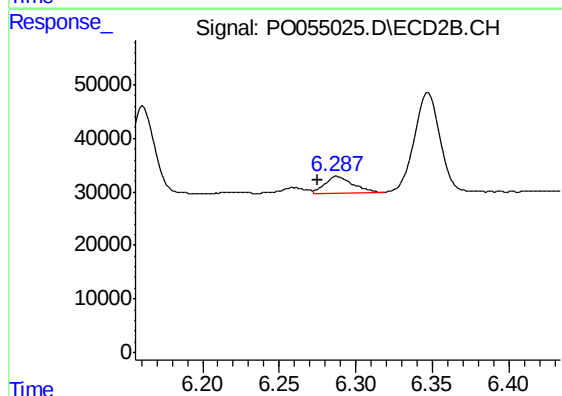


#29 AR-1254-4

R.T.: 6.287 min
Delta R.T.: 0.012 min
Response: 40350
Conc: 20.61 ng/ml

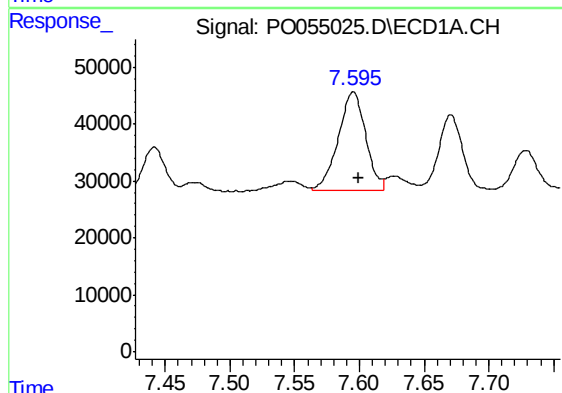


#30 AR-1254-5

R.T.: 7.595 min
Delta R.T.: -0.004 min
Response: 256222
Conc: 95.59 ng/ml

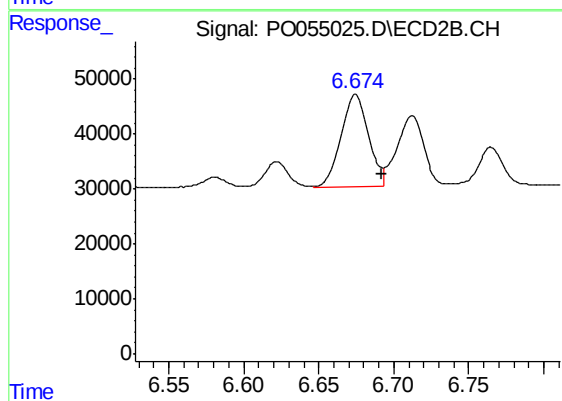

#30 AR-1254-5


R.T.: 6.674 min
Delta R.T.: -0.018 min
Response: 210957
Conc: 73.38 ng/ml



#31 AR-1260-1


R.T.: 7.057 min
Delta R.T.: -0.002 min
Response: 203313
Conc: 80.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#31 AR-1260-1

R.T.: 6.161 min
Delta R.T.: -0.016 min
Response: 178054
Conc: 77.48 ng/ml




#32 AR-1260-2

R.T.: 7.314 min
Delta R.T.: -0.003 min
Response: 243907
Conc: 78.59 ng/ml

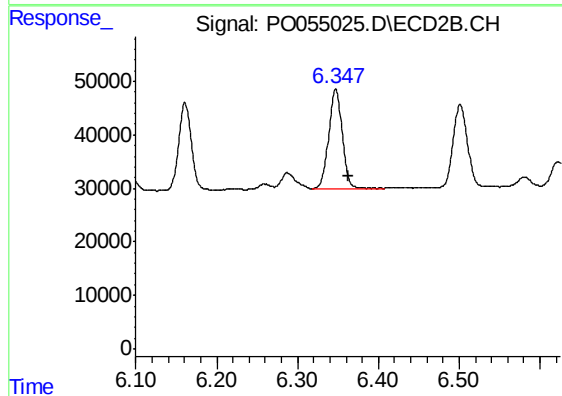

#32 AR-1260-2


R.T.: 6.347 min
Delta R.T.: -0.016 min
Response: 218672
Conc: 79.44 ng/ml



#33 AR-1260-3


R.T.: 7.671 min
Delta R.T.: -0.003 min
Response: 163032
Conc: 66.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#33 AR-1260-3

R.T.: 6.501 min
Delta R.T.: -0.017 min
Response: 192175
Conc: 74.55 ng/ml




#34 AR-1260-4

R.T.: 7.895 min
Delta R.T.: -0.002 min
Response: 184975
Conc: 66.87 ng/ml

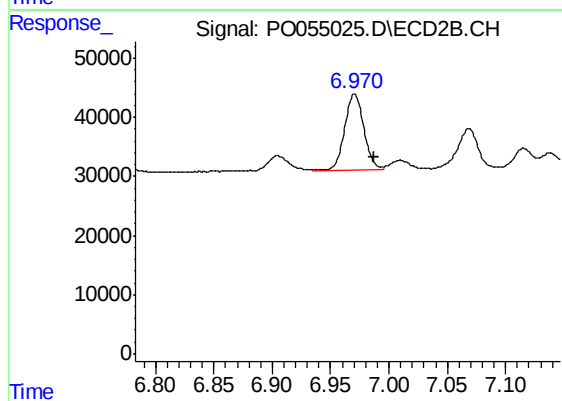

#34 AR-1260-4


R.T.: 6.971 min
Delta R.T.: -0.017 min
Response: 147045
Conc: 69.09 ng/ml



#35 AR-1260-5


R.T.: 8.205 min
Delta R.T.: -0.002 min
Response: 328898
Conc: 59.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

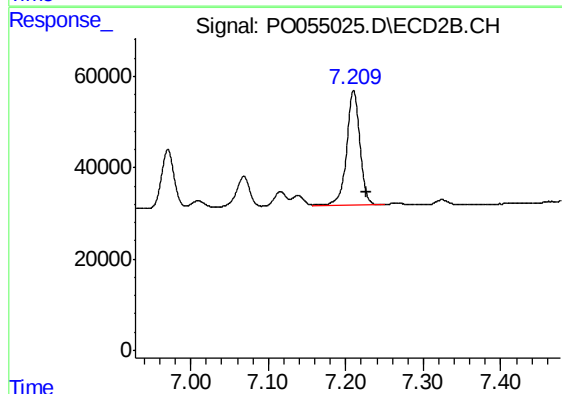


#35 AR-1260-5

R.T.: 7.210 min
Delta R.T.: -0.017 min
Response: 300229
Conc: 62.69 ng/ml




#36 AR-1262-1

R.T.: 7.671 min
Delta R.T.: -0.004 min
Response: 163032
Conc: 48.93 ng/ml

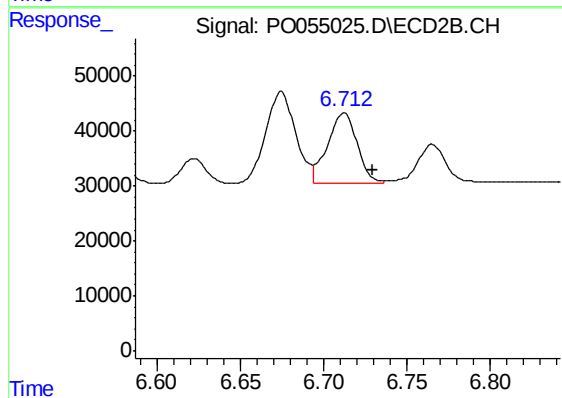

#36 AR-1262-1


R.T.: 6.712 min
Delta R.T.: -0.018 min
Response: 159412
Conc: 53.58 ng/ml

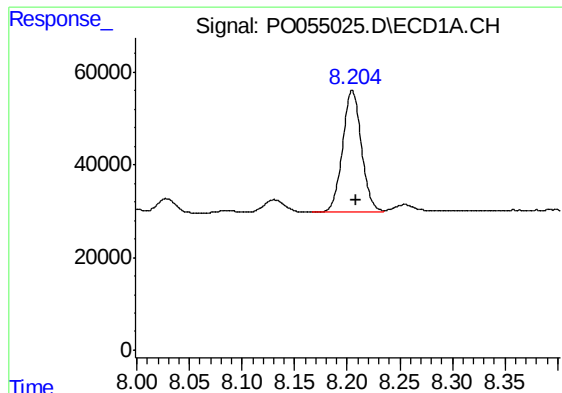

#37 AR-1262-2


R.T.: 8.205 min
Delta R.T.: -0.004 min
Response: 328898
Conc: 55.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

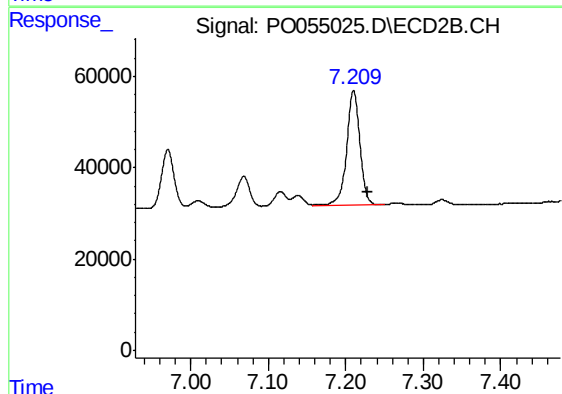


#37 AR-1262-2

R.T.: 7.210 min
Delta R.T.: -0.019 min
Response: 300229
Conc: 61.26 ng/ml




#38 AR-1262-3

R.T.: 8.517 min
Delta R.T.: 0.011 min
Response: 209213
Conc: 50.50 ng/ml

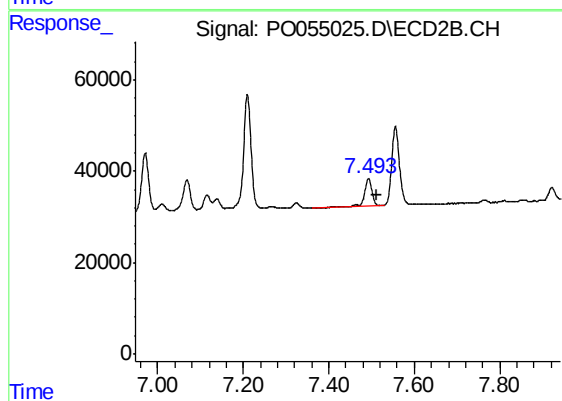

#38 AR-1262-3


R.T.: 7.493 min
Delta R.T.: -0.018 min
Response: 71802
Conc: 34.97 ng/ml



#39 AR-1262-4


R.T.: 8.571 min
Delta R.T.: -0.022 min
Response: 128293
Conc: 39.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#39 AR-1262-4

R.T.: 7.556 min
Delta R.T.: -0.019 min
Response: 217081
Conc: 59.93 ng/ml

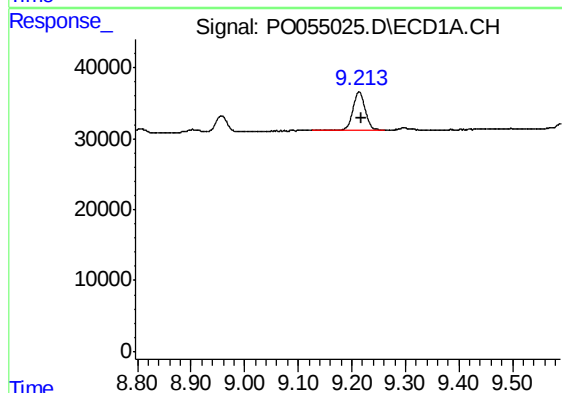


#40 AR-1262-5

R.T.: 9.214 min
Delta R.T.: -0.004 min
Response: 87962
Conc: 40.23 ng/ml

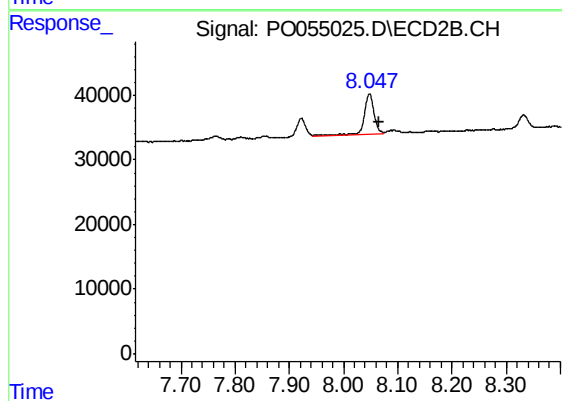

#40 AR-1262-5


R.T.: 8.048 min
Delta R.T.: -0.018 min
Response: 78676
Conc: 48.75 ng/ml



#41 AR-1268-1


R.T.: 8.517 min
Delta R.T.: 0.013 min
Response: 209213
Conc: 29.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#41 AR-1268-1

R.T.: 7.493 min
Delta R.T.: -0.018 min
Response: 71802
Conc: 12.70 ng/ml




#42 AR-1268-2

R.T.: 8.571 min
Delta R.T.: -0.023 min
Response: 128293
Conc: 19.58 ng/ml

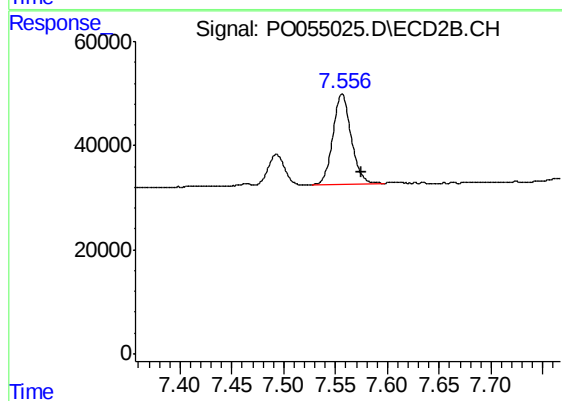

#42 AR-1268-2


R.T.: 7.556 min
Delta R.T.: -0.019 min
Response: 217081
Conc: 41.98 ng/ml



#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.810 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

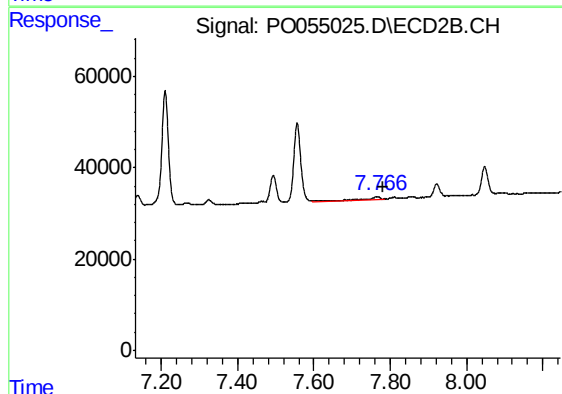


#43 AR-1268-3

R.T.: 7.765 min
Delta R.T.: -0.018 min
Response: 11942
Conc: 2.77 ng/ml

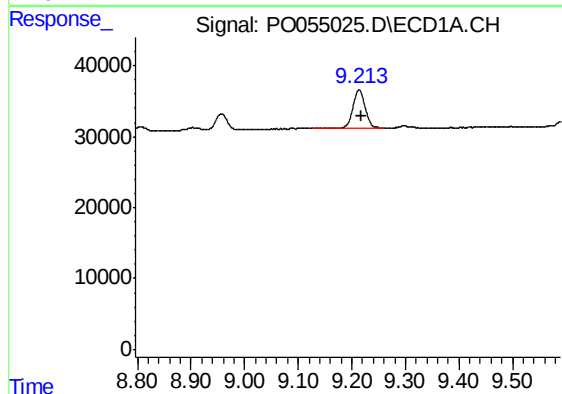


#44 AR-1268-4

R.T.: 9.214 min
Delta R.T.: -0.003 min
Response: 87962
Conc: 36.87 ng/ml

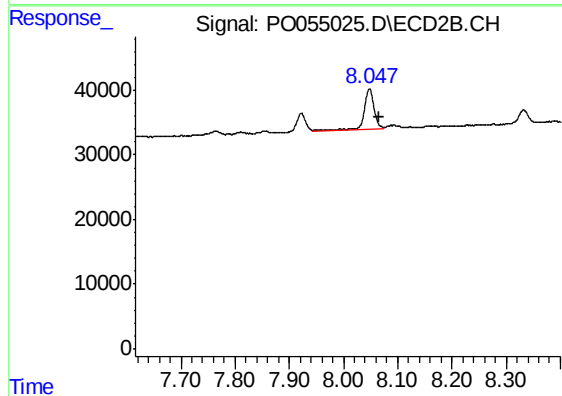

#44 AR-1268-4


R.T.: 8.048 min
Delta R.T.: -0.018 min
Response: 78676
Conc: 42.44 ng/ml

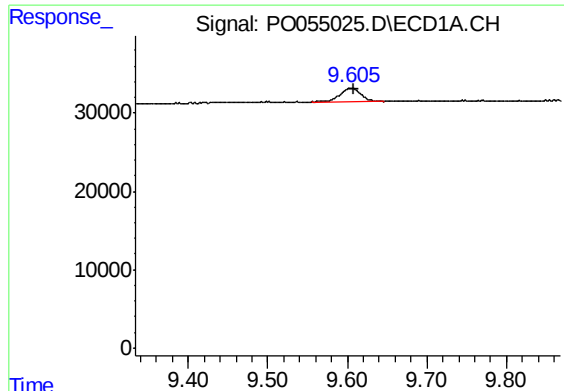

#45 AR-1268-5

R.T.: 9.605 min
Delta R.T.: -0.003 min
Response: 31911
Conc: 1.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

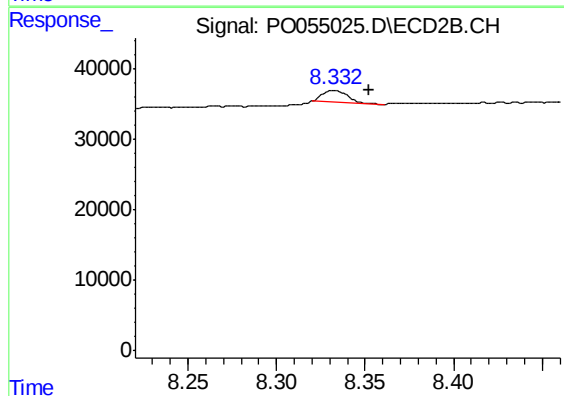

#45 AR-1268-5

R.T.: 8.332 min
Delta R.T.: -0.020 min
Response: 16096
Conc: 1.41 ng/ml