

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040819\
 Data File : P0055034.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Apr 2019 12:58
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1242 LOD 40PPB
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 06:51:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.299	3.611	1259445	1176305	36.290	36.860
2)	SA Decachlor...	9.917	8.581	1248778	862715	25.331	27.088
Target Compounds							
3)	L1 AR-1016-1	5.462	4.707	159056	128754	88.393	81.418
4)	L1 AR-1016-2	5.482	4.707	246863	128754	99.394	60.088 #
5)	L1 AR-1016-3	5.544	4.881	231098	65071	146.892	53.857 #
6)	L1 AR-1016-4	5.642	4.922	254204	55672	195.079	55.092 #
7)	L1 AR-1016-5	5.935	5.135	220878	90544	165.544	69.468 #
8)	L2 AR-1221-1	0.000	3.823	0	26658	N.D.	68.566 #
9)	L2 AR-1221-2	4.600	3.909	30906	37476	91.137	125.005 #
10)	L2 AR-1221-3	4.669	3.984	47337	52495	45.570	56.950
11)	L3 AR-1232-1	4.669	3.984	47337	52495	54.982	70.003 #
12)	L3 AR-1232-2	5.194	4.707	120050	128754	245.432	149.522 #
13)	L3 AR-1232-3	5.482	4.881	246863	65071	252.596	134.289 #
14)	L3 AR-1232-4	5.642	4.963	254204	78371	496.634	178.360 #
15)	L3 AR-1232-5	5.732	5.135	242829	90544	583.727	186.167 #
16)	L4 AR-1242-1	5.462	4.707	159056	128754	114.487	104.873
17)	L4 AR-1242-2	5.482	4.707	246863	128754	129.013	77.693 #
18)	L4 AR-1242-3	5.544	4.881	231098	65071	186.451	68.689 #
19)	L4 AR-1242-4	5.642	4.963	254204	78371	249.330	81.999 #
20)	L4 AR-1242-5	6.373	5.510	133269	2652854	110.398	2156.982 #
21)	L5 AR-1248-1	5.462	4.707	159056	128754	159.108	146.682
22)	L5 AR-1248-2	5.732	4.922	242829	55672	167.202	46.065 #
23)	L5 AR-1248-3	5.935	4.963	220878	78371	138.294	62.808 #
24)	L5 AR-1248-4	6.312	5.135	3749501	90544	1995.962	59.452 #
25)	L5 AR-1248-5	6.373	5.510	133269	2652854	74.335	1779.395 #
26)	L6 AR-1254-1	6.312	5.510	3749501	2652854	2067.912	1213.861 #
27)	L6 AR-1254-2	6.532	5.631	114439	125024	40.087	64.480 #
28)	L6 AR-1254-3	6.900	6.032	1717332	65898	546.101	20.557 #
29)	L6 AR-1254-4	7.177	6.259	62539	20509	25.564	10.475 #
30)	L6 AR-1254-5	7.624	6.677	119262	192066	44.496	66.812 #
31)	L7 AR-1260-1	7.016	6.177	32691	24463	13.011	10.645
32)	L7 AR-1260-2	7.377	6.336	228826	1372341	73.731	498.533 #
33)	L7 AR-1260-3	7.685	6.540	107055	230287	43.618	89.331 #
34)	L7 AR-1260-4	7.897	6.960	109538	269293	39.601	126.537 #
35)	L7 AR-1260-5	0.000	7.218	0	111772	N.D.	23.338 #
36)	L8 AR-1262-1	7.685	6.748	107055	87165	32.129	29.300
37)	L8 AR-1262-2	0.000	7.218	0	111772	N.D.	22.805 #
38)	L8 AR-1262-3	0.000	7.527	0	26107124	N.D.	12713.760 #
39)	L8 AR-1262-4	0.000	7.527	0	26107124	N.D.	7207.680 #
40)	L8 AR-1262-5	9.182	8.085	25521	15786	11.673	9.781
41)	L9 AR-1268-1	0.000	7.527	0	26107124	N.D.	4617.338 #
42)	L9 AR-1268-2	0.000	7.527	0	26107124	N.D.	5048.191 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040819\
 Data File : P0055034.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Apr 2019 12:58
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1242 LOD 40PPB
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 06:51:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	8.791	7.790	238655	19086	43.810	4.435 #
44) L9	AR-1268-4	9.182	8.085	25521	15786	10.697	8.515
45) L9	AR-1268-5	9.651	8.305	56325	9260	3.419	0.814 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040819\
Data File : PO055034.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Apr 2019 12:58
Operator : SM/SJ
Sample : K1560-07
Misc : AR1242 LOD 40PPB
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 06:51:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

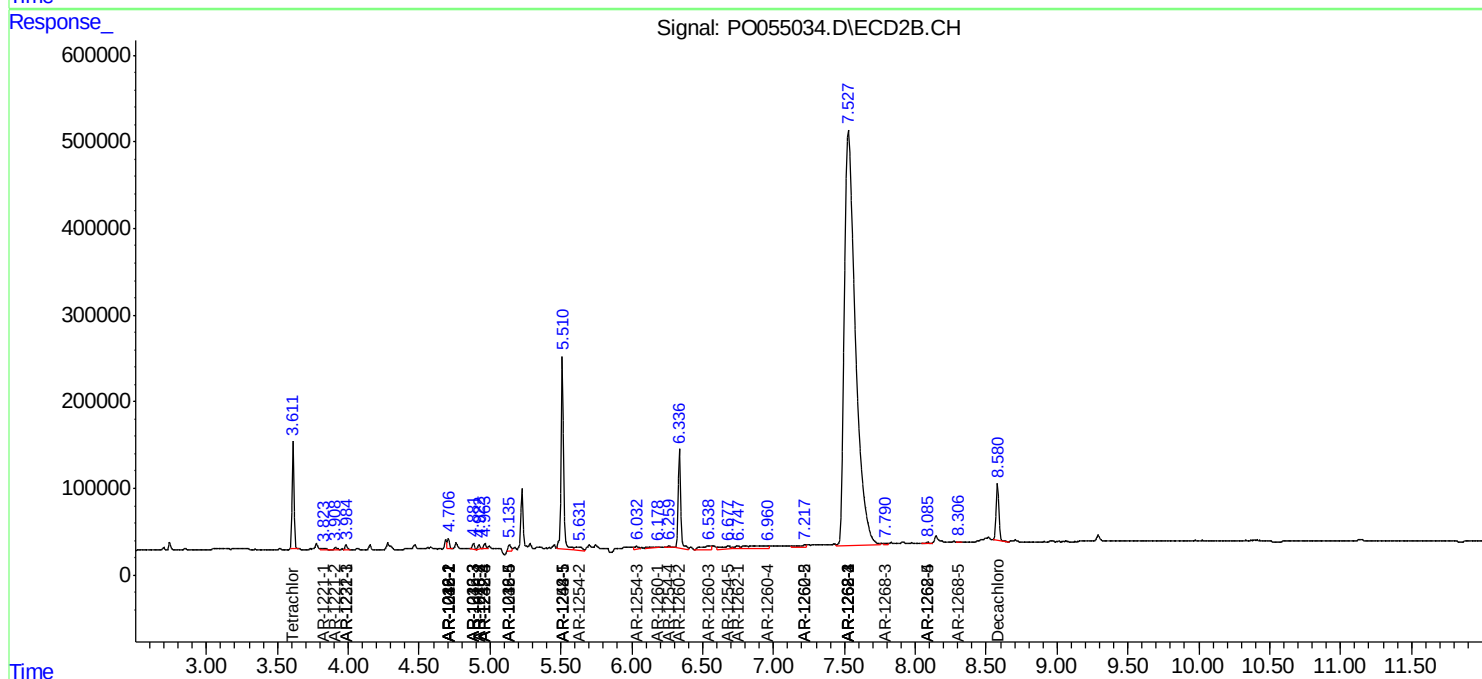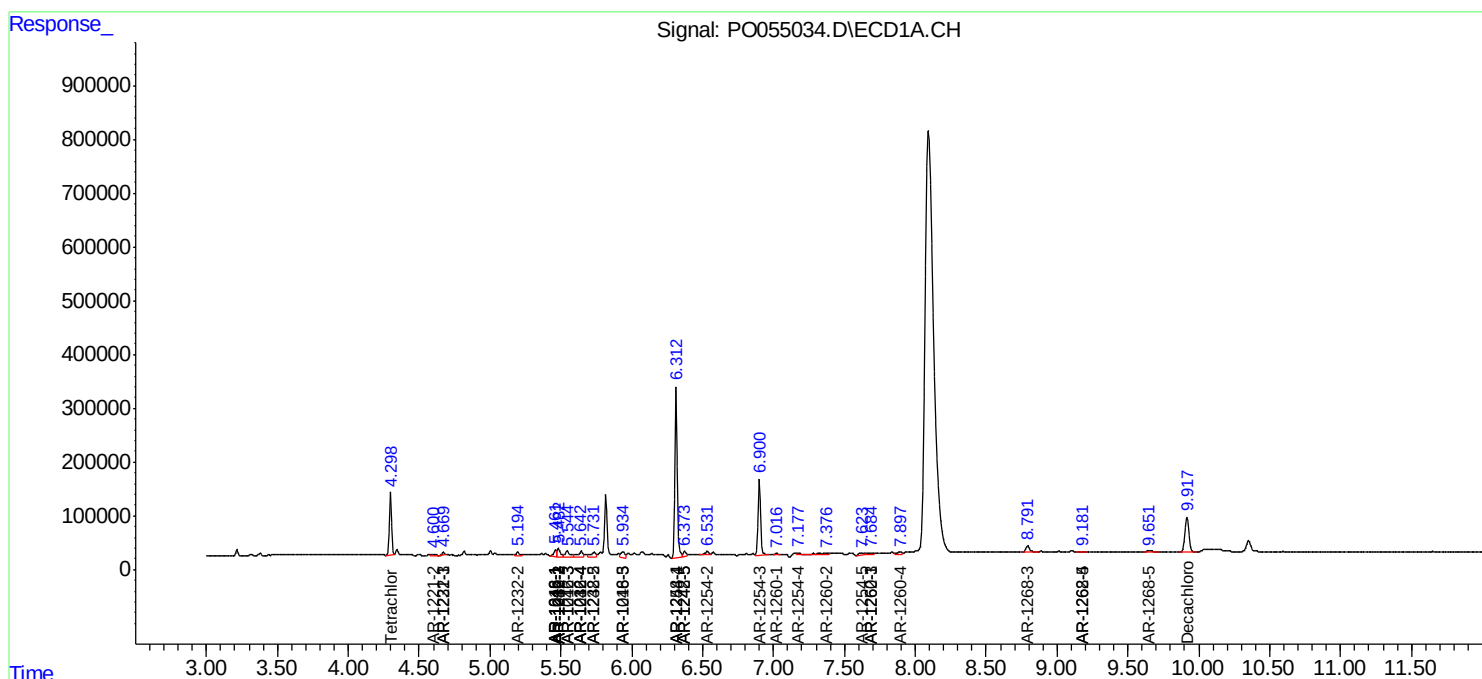


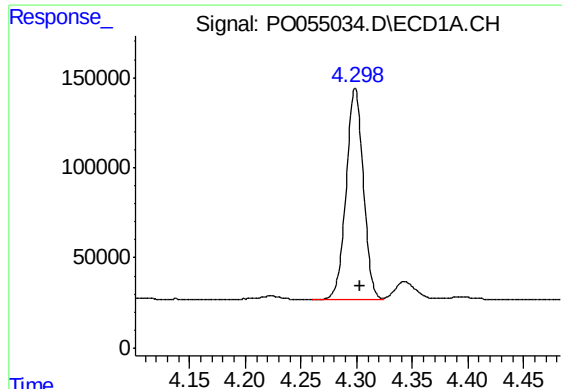

#1 Tetrachloro-m-xylene


R.T.: 4.299 min
Delta R.T.: -0.004 min
Response: 1259445
Conc: 36.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: -0.010 min
Response: 1176305
Conc: 36.86 ng/ml




#2 Decachlorobiphenyl

R.T.: 9.917 min
Delta R.T.: -0.006 min
Response: 1248778
Conc: 25.33 ng/ml

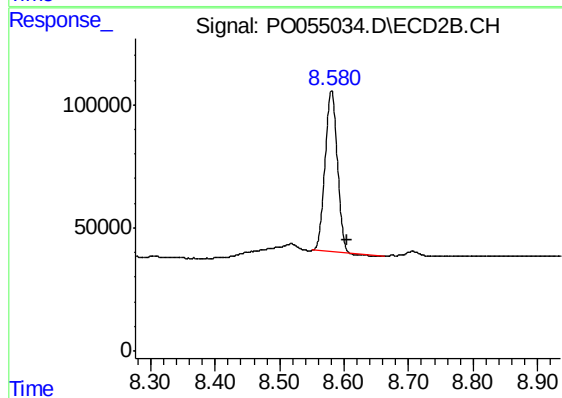

#2 Decachlorobiphenyl


R.T.: 8.581 min
Delta R.T.: -0.024 min
Response: 862715
Conc: 27.09 ng/ml



#3 AR-1016-1


R.T.: 5.462 min
Delta R.T.: -0.004 min
Response: 159056
Conc: 88.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#3 AR-1016-1

R.T.: 4.707 min
Delta R.T.: 0.006 min
Response: 128754
Conc: 81.42 ng/ml




#4 AR-1016-2

R.T.: 5.482 min
Delta R.T.: -0.005 min
Response: 246863
Conc: 99.39 ng/ml

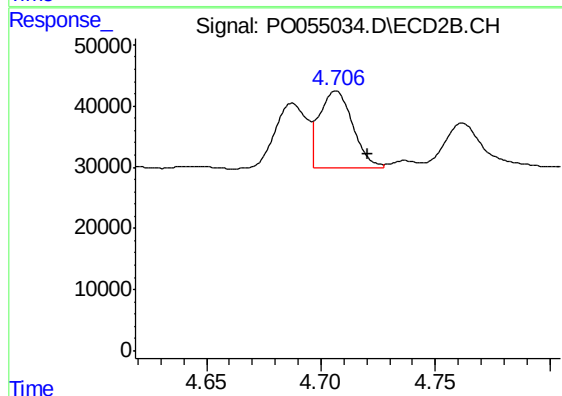

#4 AR-1016-2


R.T.: 4.707 min
Delta R.T.: -0.014 min
Response: 128754
Conc: 60.09 ng/ml



#5 AR-1016-3


R.T.: 5.544 min
Delta R.T.: -0.004 min
Response: 231098
Conc: 146.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#5 AR-1016-3

R.T.: 4.881 min
Delta R.T.: -0.014 min
Response: 65071
Conc: 53.86 ng/ml




#6 AR-1016-4

R.T.: 5.642 min
Delta R.T.: -0.005 min
Response: 254204
Conc: 195.08 ng/ml

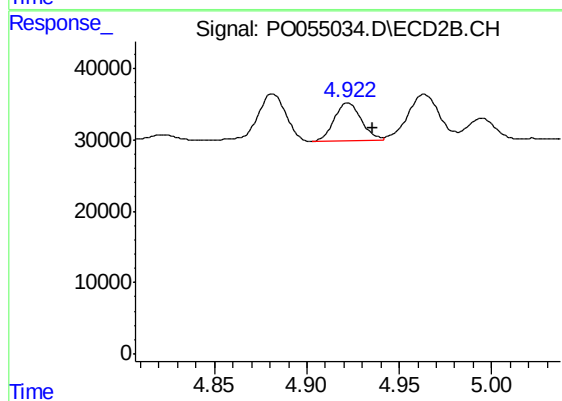

#6 AR-1016-4


R.T.: 4.922 min
Delta R.T.: -0.013 min
Response: 55672
Conc: 55.09 ng/ml



#7 AR-1016-5


R.T.: 5.935 min
Delta R.T.: -0.005 min
Response: 220878
Conc: 165.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#7 AR-1016-5

R.T.: 5.135 min
Delta R.T.: -0.013 min
Response: 90544
Conc: 69.47 ng/ml




#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.512 min
Response: 0
Conc: N.D.

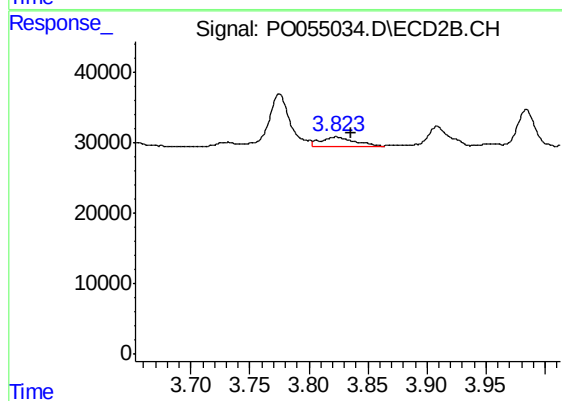

#8 AR-1221-1


R.T.: 3.823 min
Delta R.T.: -0.012 min
Response: 26658
Conc: 68.57 ng/ml



#9 AR-1221-2


R.T.: 4.600 min
Delta R.T.: 0.003 min
Response: 30906
Conc: 91.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

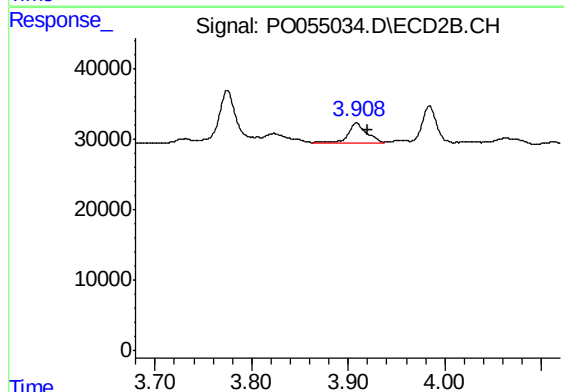


#9 AR-1221-2

R.T.: 3.909 min
Delta R.T.: -0.011 min
Response: 37476
Conc: 125.01 ng/ml




#10 AR-1221-3

R.T.: 4.669 min
Delta R.T.: -0.004 min
Response: 47337
Conc: 45.57 ng/ml

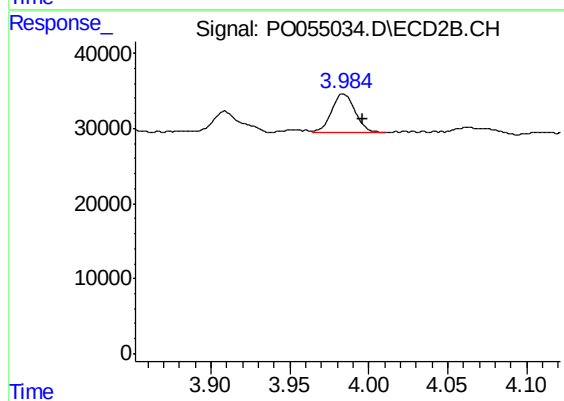

#10 AR-1221-3


R.T.: 3.984 min
Delta R.T.: -0.012 min
Response: 52495
Conc: 56.95 ng/ml

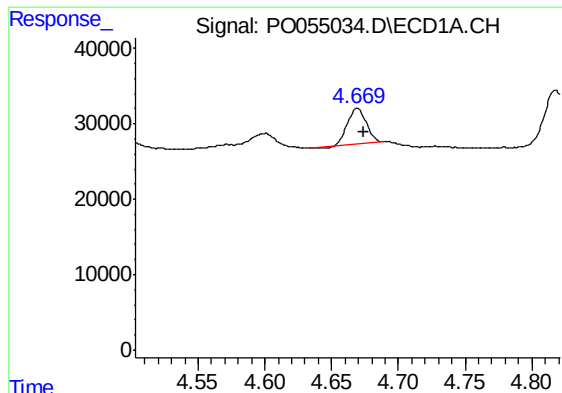

#11 AR-1232-1


R.T.: 4.669 min
Delta R.T.: -0.005 min
Response: 47337
Conc: 54.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

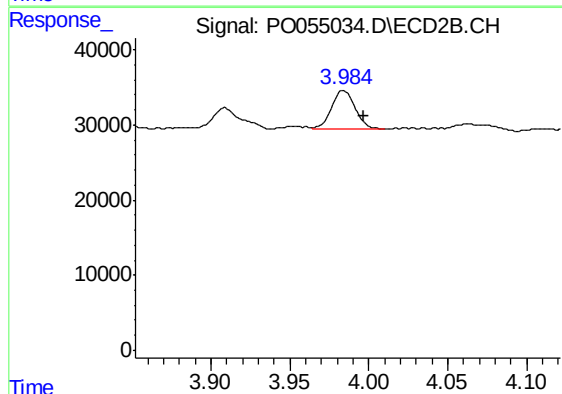


#11 AR-1232-1

R.T.: 3.984 min
Delta R.T.: -0.013 min
Response: 52495
Conc: 70.00 ng/ml

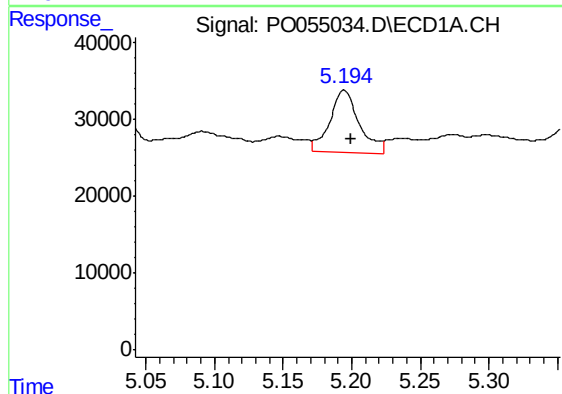


#12 AR-1232-2

R.T.: 5.194 min
Delta R.T.: -0.005 min
Response: 120050
Conc: 245.43 ng/ml

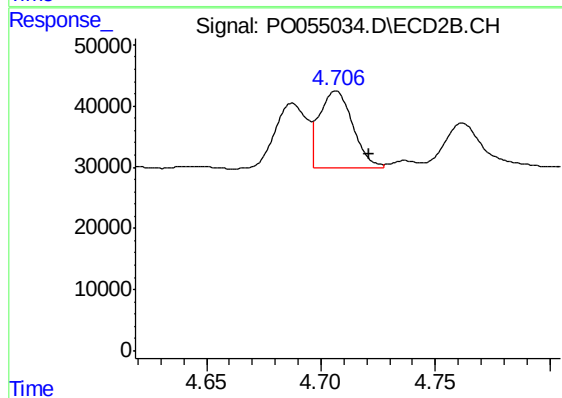

#12 AR-1232-2


R.T.: 4.707 min
Delta R.T.: -0.014 min
Response: 128754
Conc: 149.52 ng/ml



#13 AR-1232-3


R.T.: 5.482 min
Delta R.T.: -0.006 min
Response: 246863
Conc: 252.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#13 AR-1232-3

R.T.: 4.881 min
Delta R.T.: -0.016 min
Response: 65071
Conc: 134.29 ng/ml

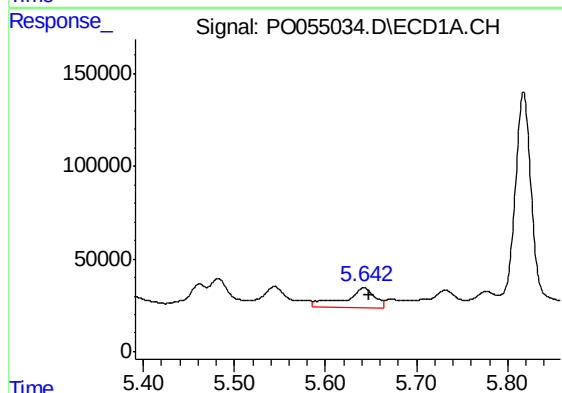


#14 AR-1232-4

R.T.: 5.642 min
Delta R.T.: -0.006 min
Response: 254204
Conc: 496.63 ng/ml

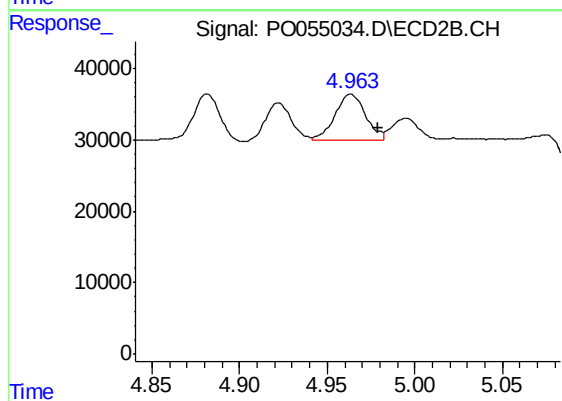

#14 AR-1232-4


R.T.: 4.963 min
Delta R.T.: -0.016 min
Response: 78371
Conc: 178.36 ng/ml

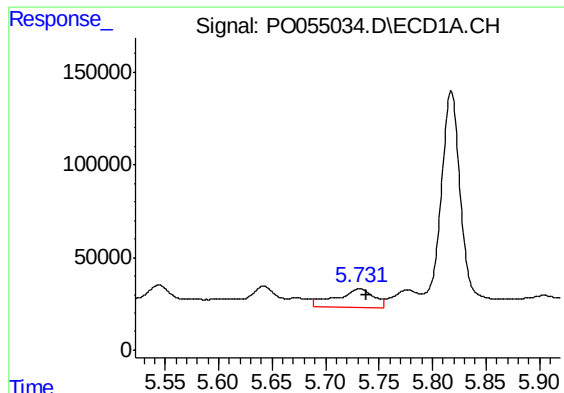

#15 AR-1232-5


R.T.: 5.732 min
Delta R.T.: -0.007 min
Response: 242829
Conc: 583.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

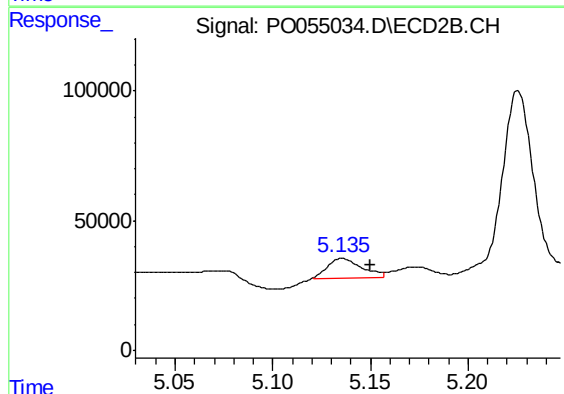


#15 AR-1232-5

R.T.: 5.135 min
Delta R.T.: -0.015 min
Response: 90544
Conc: 186.17 ng/ml

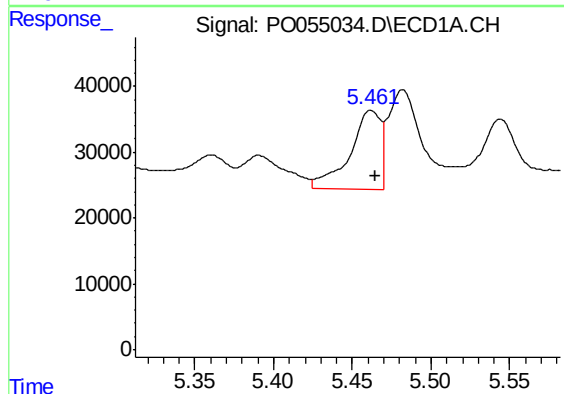


#16 AR-1242-1

R.T.: 5.462 min
Delta R.T.: -0.003 min
Response: 159056
Conc: 114.49 ng/ml

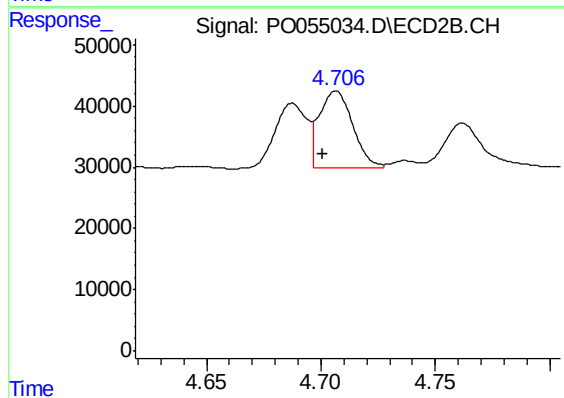

#16 AR-1242-1


R.T.: 4.707 min
Delta R.T.: 0.006 min
Response: 128754
Conc: 104.87 ng/ml



#17 AR-1242-2


R.T.: 5.482 min
Delta R.T.: -0.005 min
Response: 246863
Conc: 129.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#17 AR-1242-2

R.T.: 4.707 min
Delta R.T.: -0.014 min
Response: 128754
Conc: 77.69 ng/ml




#18 AR-1242-3

R.T.: 5.544 min
Delta R.T.: -0.005 min
Response: 231098
Conc: 186.45 ng/ml

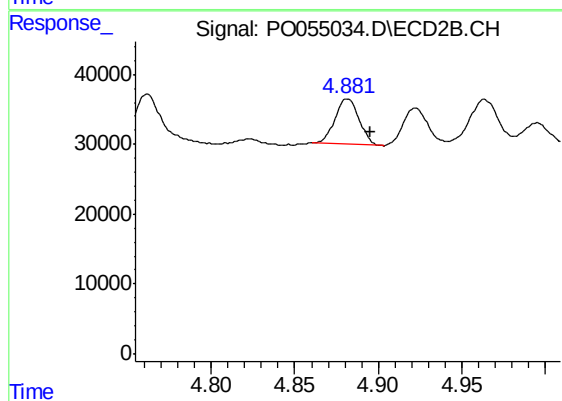

#18 AR-1242-3


R.T.: 4.881 min
Delta R.T.: -0.014 min
Response: 65071
Conc: 68.69 ng/ml

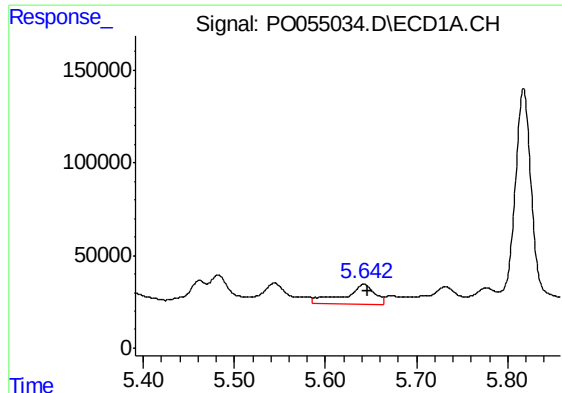

#19 AR-1242-4


R.T.: 5.642 min
Delta R.T.: -0.004 min
Response: 254204
Conc: 249.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

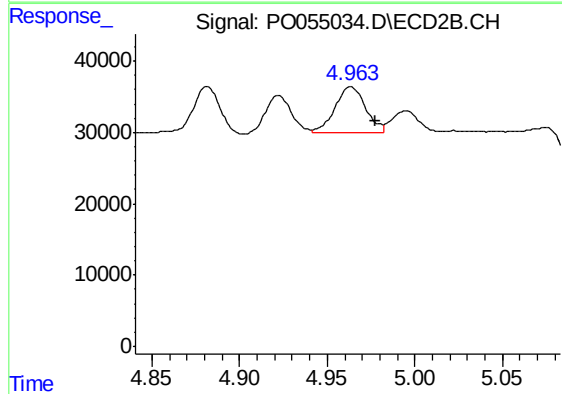


#19 AR-1242-4

R.T.: 4.963 min
Delta R.T.: -0.015 min
Response: 78371
Conc: 82.00 ng/ml

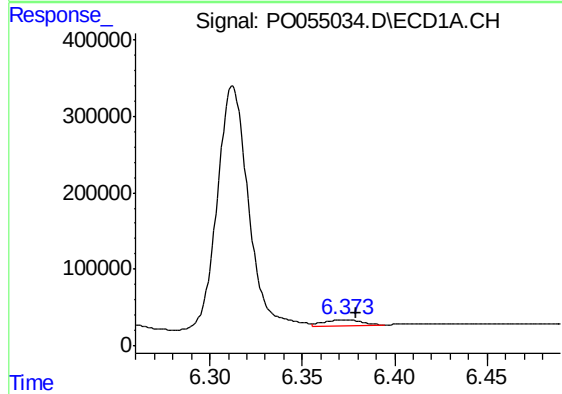


#20 AR-1242-5

R.T.: 6.373 min
Delta R.T.: -0.006 min
Response: 133269
Conc: 110.40 ng/ml

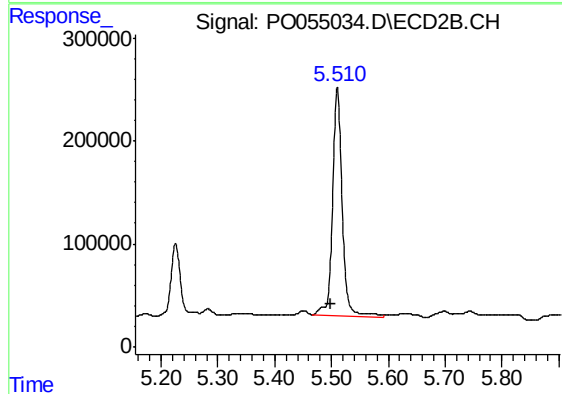

#20 AR-1242-5


R.T.: 5.510 min
Delta R.T.: 0.012 min
Response: 2652854
Conc: 2156.98 ng/ml



#21 AR-1248-1


R.T.: 5.462 min
Delta R.T.: -0.004 min
Response: 159056
Conc: 159.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#21 AR-1248-1

R.T.: 4.707 min
Delta R.T.: 0.006 min
Response: 128754
Conc: 146.68 ng/ml




#22 AR-1248-2

R.T.: 5.732 min
Delta R.T.: -0.006 min
Response: 242829
Conc: 167.20 ng/ml

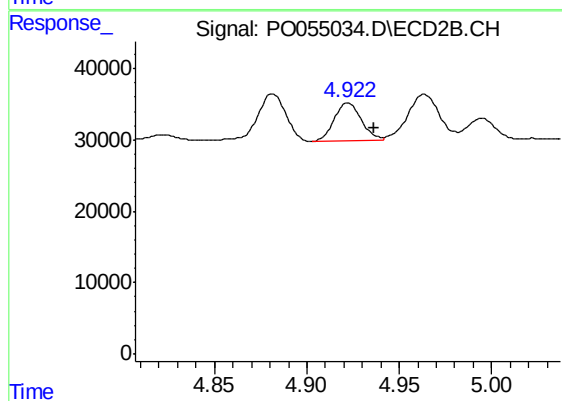

#22 AR-1248-2


R.T.: 4.922 min
Delta R.T.: -0.014 min
Response: 55672
Conc: 46.07 ng/ml



#23 AR-1248-3


R.T.: 5.935 min
Delta R.T.: -0.005 min
Response: 220878
Conc: 138.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

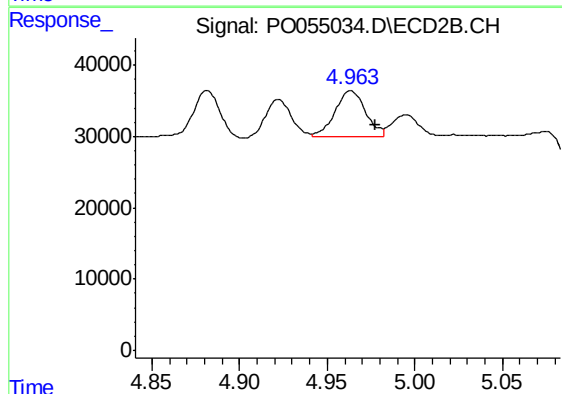


#23 AR-1248-3

R.T.: 4.963 min
Delta R.T.: -0.014 min
Response: 78371
Conc: 62.81 ng/ml

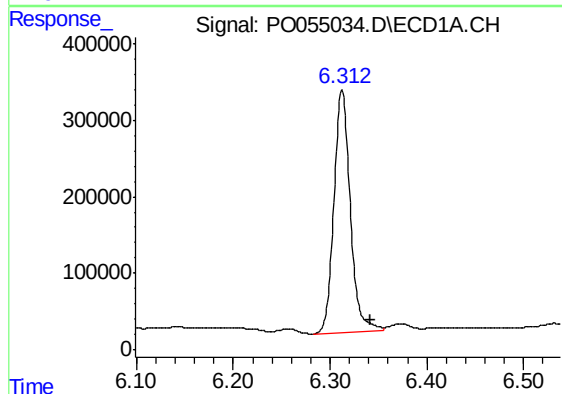


#24 AR-1248-4

R.T.: 6.312 min
Delta R.T.: -0.030 min
Response: 3749501
Conc: 1995.96 ng/ml

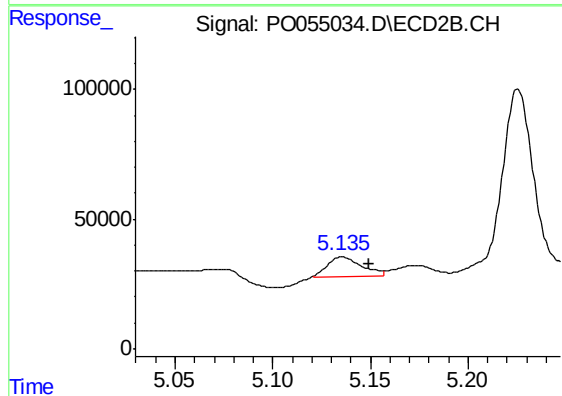

#24 AR-1248-4


R.T.: 5.135 min
Delta R.T.: -0.014 min
Response: 90544
Conc: 59.45 ng/ml



#25 AR-1248-5


R.T.: 6.373 min
Delta R.T.: -0.007 min
Response: 133269
Conc: 74.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#25 AR-1248-5

R.T.: 5.510 min
Delta R.T.: -0.030 min
Response: 2652854
Conc: 1779.40 ng/ml




#26 AR-1254-1

R.T.: 6.312 min
Delta R.T.: -0.002 min
Response: 3749501
Conc: 2067.91 ng/ml

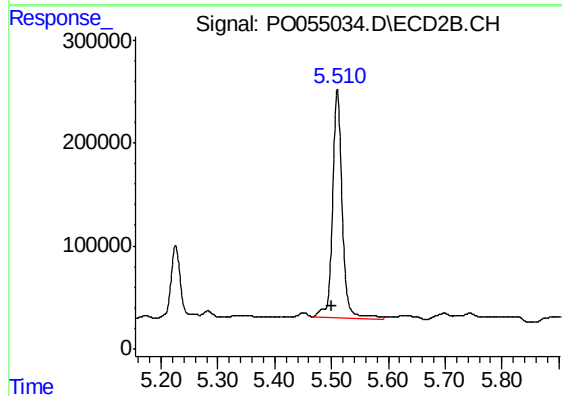

#26 AR-1254-1


R.T.: 5.510 min
Delta R.T.: 0.010 min
Response: 2652854
Conc: 1213.86 ng/ml



#27 AR-1254-2


R.T.: 6.532 min
Delta R.T.: -0.001 min
Response: 114439
Conc: 40.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#27 AR-1254-2

R.T.: 5.631 min
Delta R.T.: -0.015 min
Response: 125024
Conc: 64.48 ng/ml

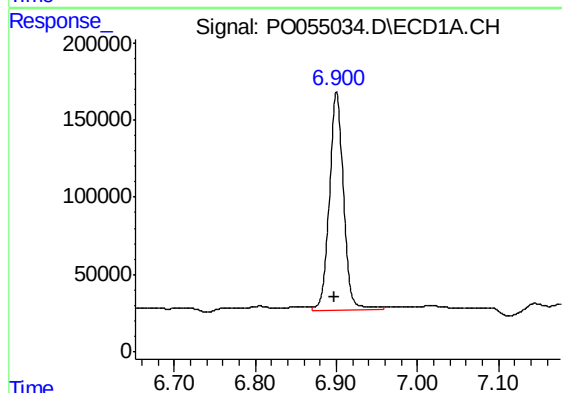


#28 AR-1254-3

R.T.: 6.900 min
Delta R.T.: 0.003 min
Response: 1717332
Conc: 546.10 ng/ml

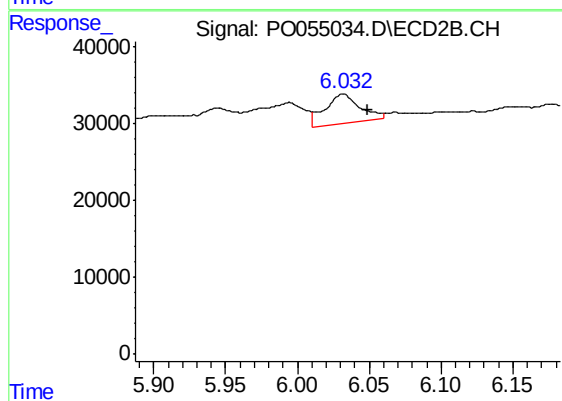

#28 AR-1254-3


R.T.: 6.032 min
Delta R.T.: -0.017 min
Response: 65898
Conc: 20.56 ng/ml



#29 AR-1254-4


R.T.: 7.177 min
Delta R.T.: -0.005 min
Response: 62539
Conc: 25.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#29 AR-1254-4

R.T.: 6.259 min
Delta R.T.: -0.016 min
Response: 20509
Conc: 10.47 ng/ml




#30 AR-1254-5

R.T.: 7.624 min
Delta R.T.: 0.024 min
Response: 119262
Conc: 44.50 ng/ml

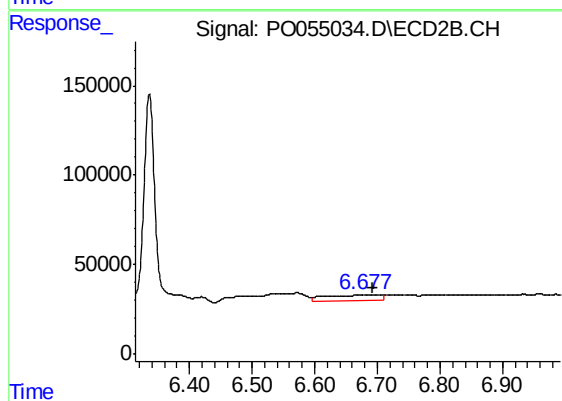

#30 AR-1254-5


R.T.: 6.677 min
Delta R.T.: -0.015 min
Response: 192066
Conc: 66.81 ng/ml



#31 AR-1260-1


R.T.: 7.016 min
Delta R.T.: -0.043 min
Response: 32691
Conc: 13.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019




#31 AR-1260-1

R.T.: 6.177 min
Delta R.T.: 0.000 min
Response: 24463
Conc: 10.64 ng/ml




#32 AR-1260-2

R.T.: 7.377 min
Delta R.T.: 0.061 min
Response: 228826
Conc: 73.73 ng/ml

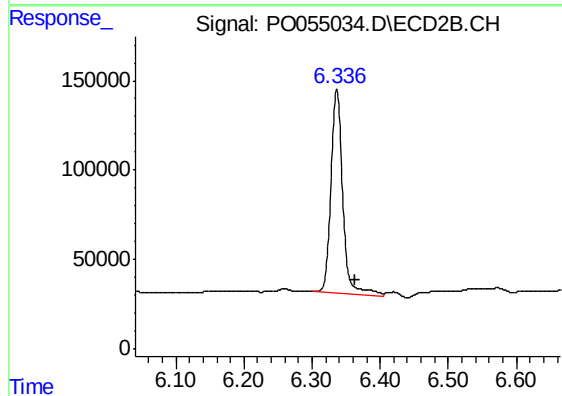

#32 AR-1260-2


R.T.: 6.336 min
Delta R.T.: -0.027 min
Response: 1372341
Conc: 498.53 ng/ml

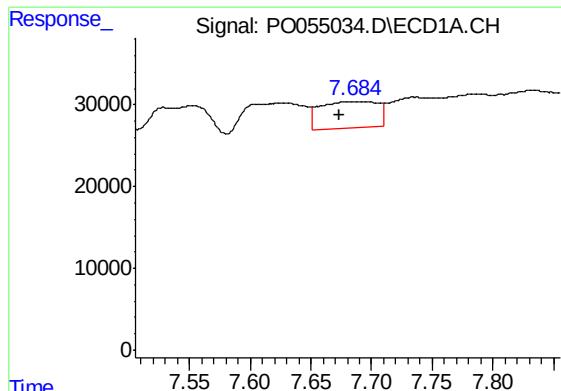

#33 AR-1260-3


R.T.: 7.685 min
Delta R.T.: 0.011 min
Response: 107055
Conc: 43.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

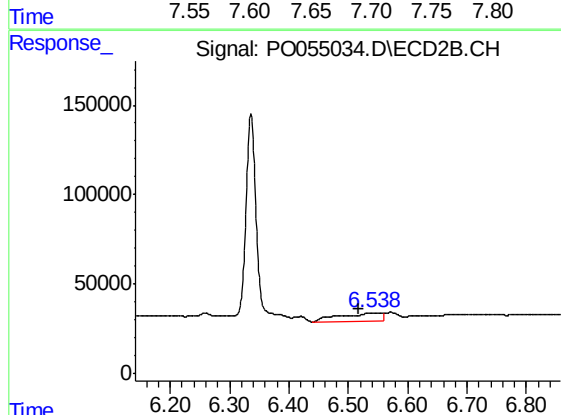


#33 AR-1260-3

R.T.: 6.540 min
Delta R.T.: 0.022 min
Response: 230287
Conc: 89.33 ng/ml

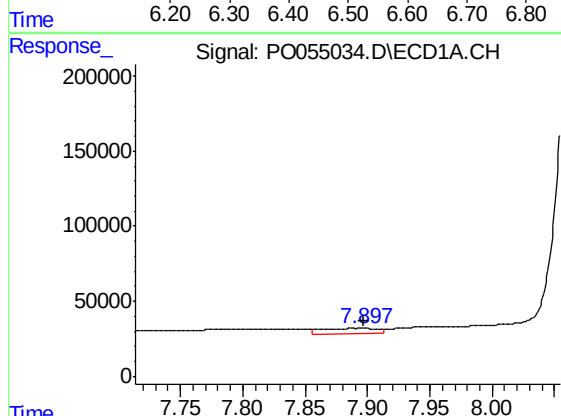


#34 AR-1260-4

R.T.: 7.897 min
Delta R.T.: 0.000 min
Response: 109538
Conc: 39.60 ng/ml

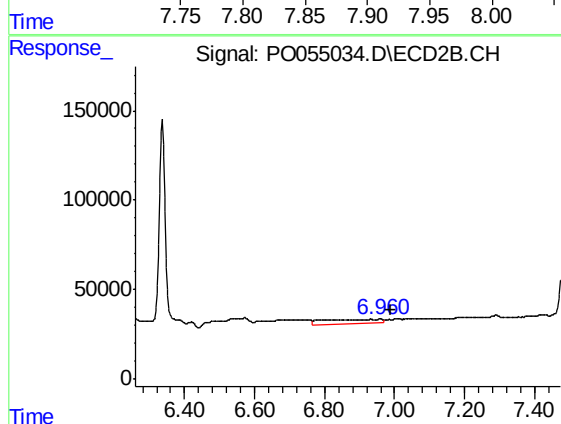

#34 AR-1260-4


R.T.: 6.960 min
Delta R.T.: -0.027 min
Response: 269293
Conc: 126.54 ng/ml



#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.207 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

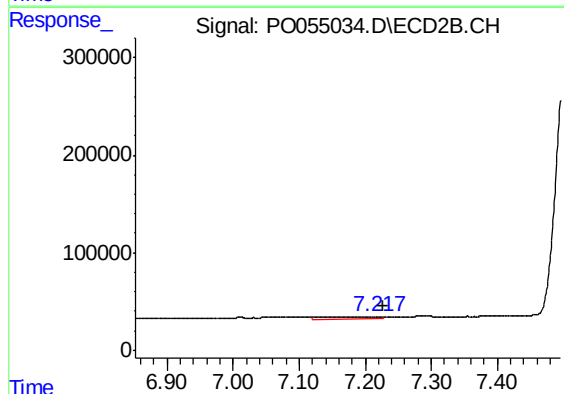


#35 AR-1260-5

R.T.: 7.218 min
Delta R.T.: -0.009 min
Response: 111772
Conc: 23.34 ng/ml




#36 AR-1262-1

R.T.: 7.685 min
Delta R.T.: 0.010 min
Response: 107055
Conc: 32.13 ng/ml

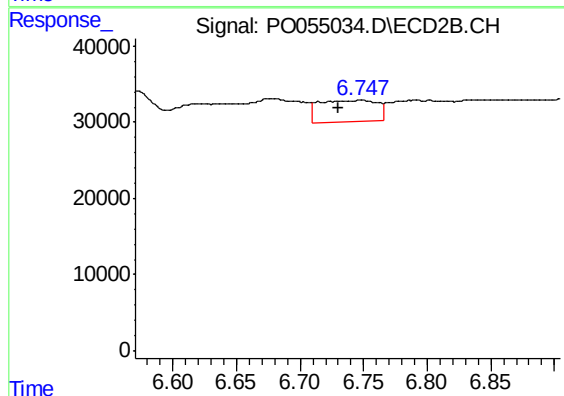

#36 AR-1262-1


R.T.: 6.748 min
Delta R.T.: 0.018 min
Response: 87165
Conc: 29.30 ng/ml



#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 8.209 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

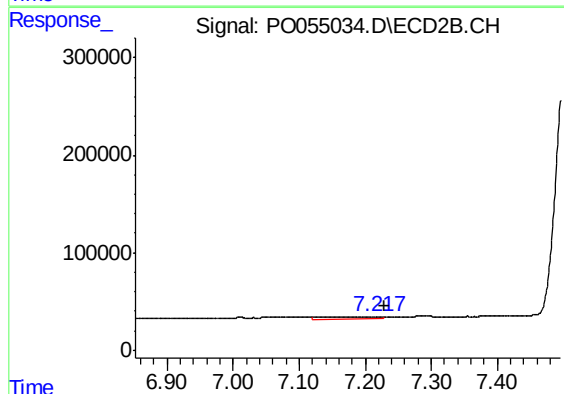


#37 AR-1262-2

R.T.: 7.218 min
Delta R.T.: -0.011 min
Response: 111772
Conc: 22.81 ng/ml




#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.507 min
Response: 0
Conc: N.D.

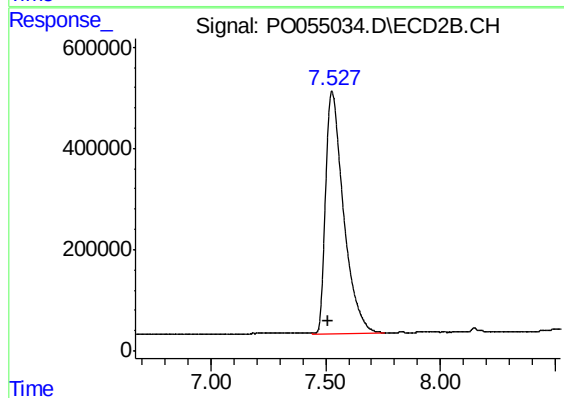

#38 AR-1262-3


R.T.: 7.527 min
Delta R.T.: 0.015 min
Response: 26107124
Conc: 12713.76 ng/ml



#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.593 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

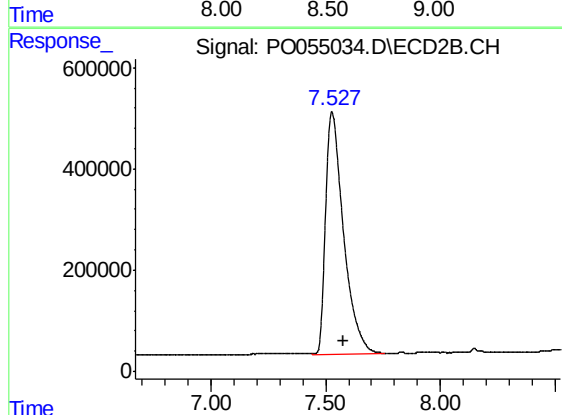


#39 AR-1262-4

R.T.: 7.527 min
Delta R.T.: -0.048 min
Response: 26107124
Conc: 7207.68 ng/ml

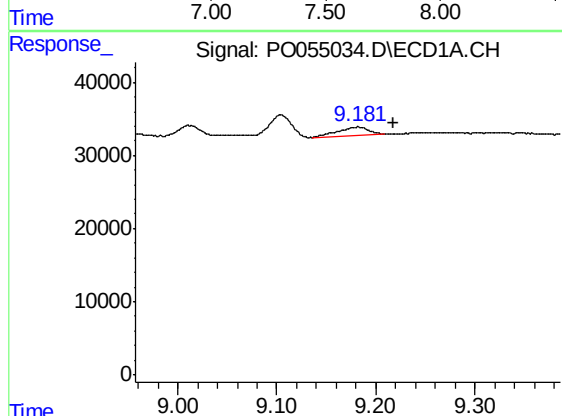


#40 AR-1262-5

R.T.: 9.182 min
Delta R.T.: -0.036 min
Response: 25521
Conc: 11.67 ng/ml

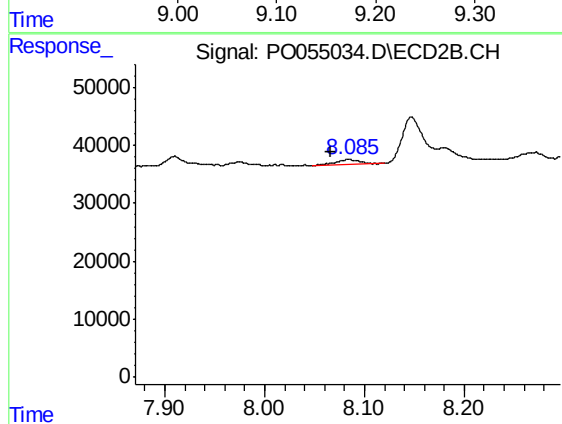

#40 AR-1262-5


R.T.: 8.085 min
Delta R.T.: 0.018 min
Response: 15786
Conc: 9.78 ng/ml



#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 8.504 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

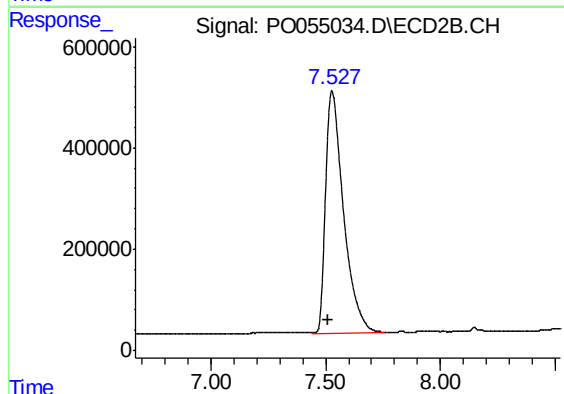


#41 AR-1268-1

R.T.: 7.527 min
Delta R.T.: 0.015 min
Response: 26107124
Conc: 4617.34 ng/ml




#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.594 min
Response: 0
Conc: N.D.

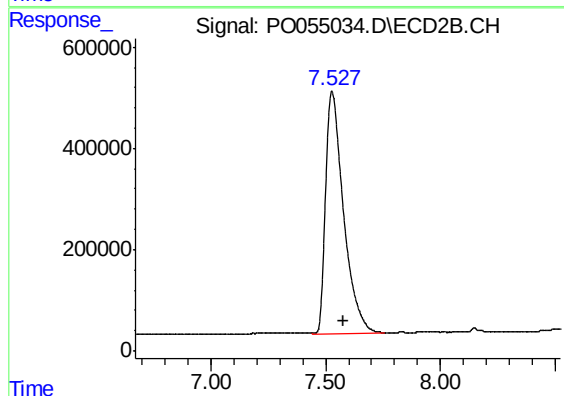

#42 AR-1268-2


R.T.: 7.527 min
Delta R.T.: -0.049 min
Response: 26107124
Conc: 5048.19 ng/ml



#43 AR-1268-3


R.T.: 8.791 min
Delta R.T.: -0.019 min
Response: 238655
Conc: 43.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

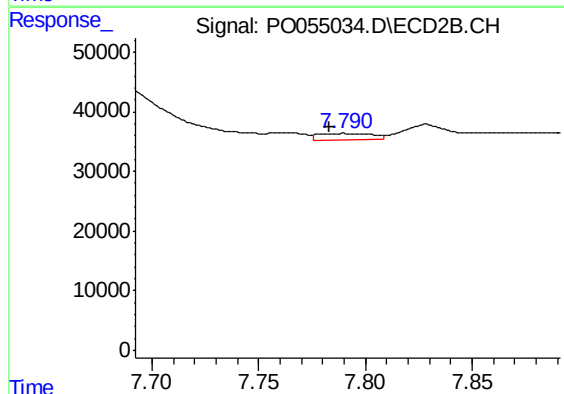


#43 AR-1268-3

R.T.: 7.790 min
Delta R.T.: 0.007 min
Response: 19086
Conc: 4.43 ng/ml




#44 AR-1268-4

R.T.: 9.182 min
Delta R.T.: -0.035 min
Response: 25521
Conc: 10.70 ng/ml

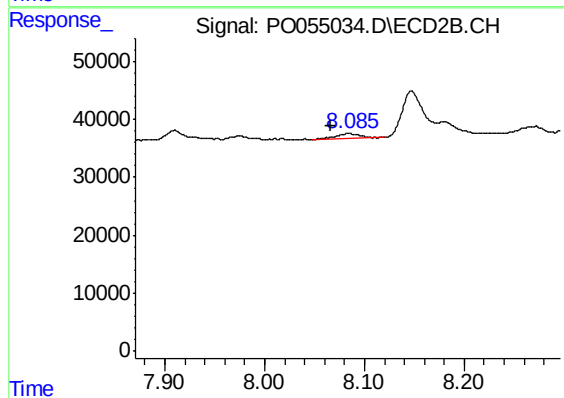

#44 AR-1268-4


R.T.: 8.085 min
Delta R.T.: 0.019 min
Response: 15786
Conc: 8.52 ng/ml

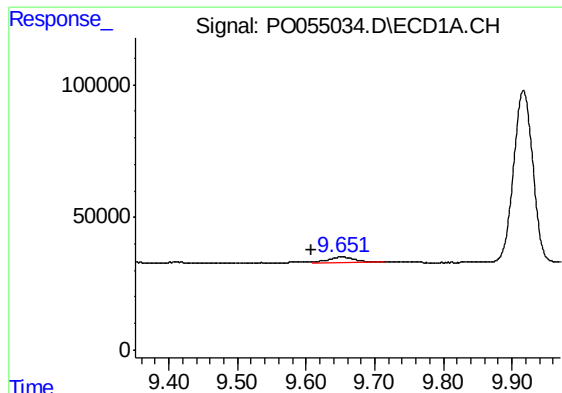

#45 AR-1268-5

R.T.: 9.651 min
Delta R.T.: 0.043 min
Response: 56325
Conc: 3.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

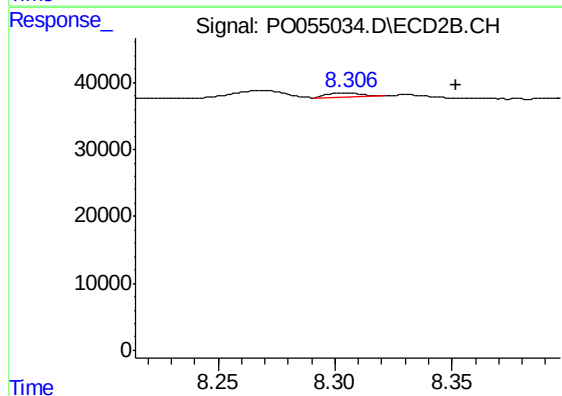

#45 AR-1268-5

R.T.: 8.305 min
Delta R.T.: -0.047 min
Response: 9260
Conc: 0.81 ng/ml