

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040819\
 Data File : P0055027.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Apr 2019 10:59
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1221 LOD 25PPB
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 06:48:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.299	3.611	1295477	1202855	37.328	37.692
2) SA Decachlor...	9.916	8.581	1314684	928713	26.668	29.161
Target Compounds						
8) L2 AR-1221-1	4.507	3.824	41724	35785	95.571	92.041
9) L2 AR-1221-2	4.596	3.908	48143	43414	141.964	144.814
10) L2 AR-1221-3	4.670	3.984	103365	87459	99.506	94.881



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040819\
Data File : PO055027.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Apr 2019 10:59
Operator : SM/SJ
Sample : K1560-07
Misc : AR1221 LOD 25PPB
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 06:48:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

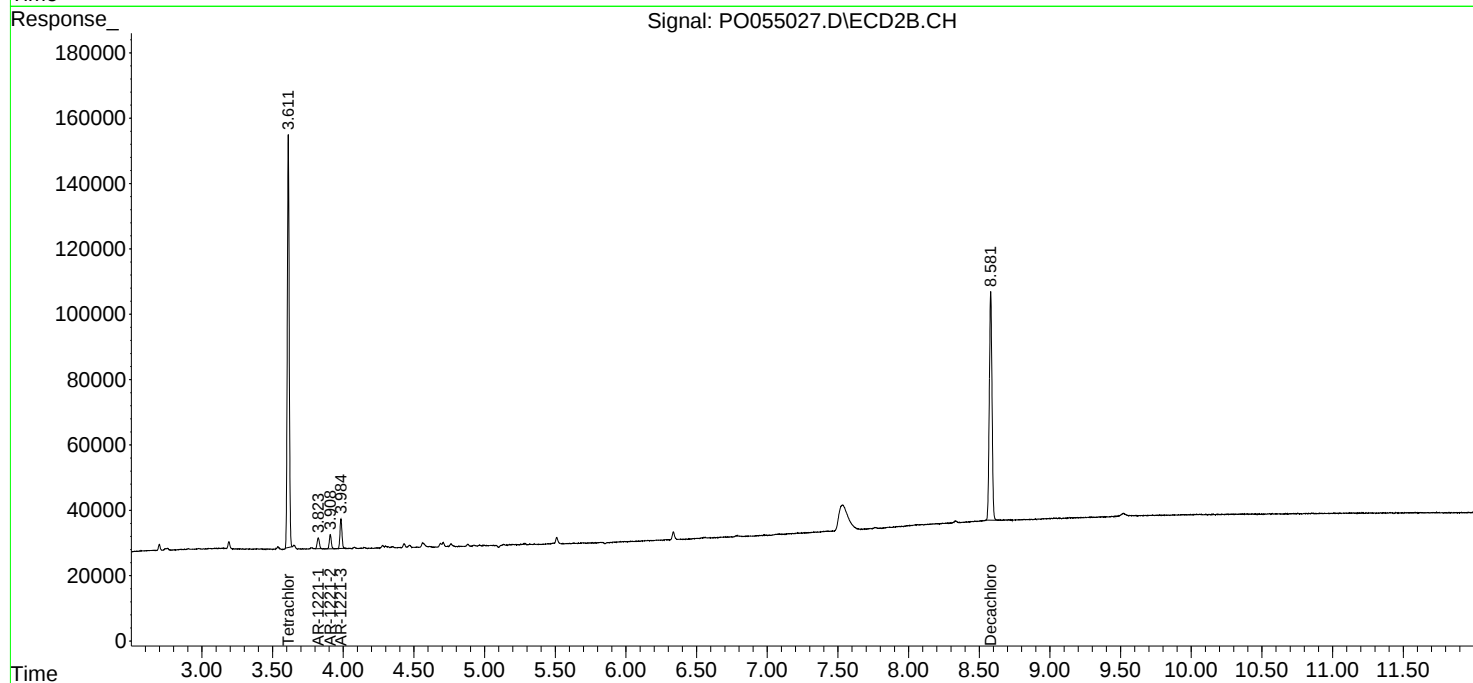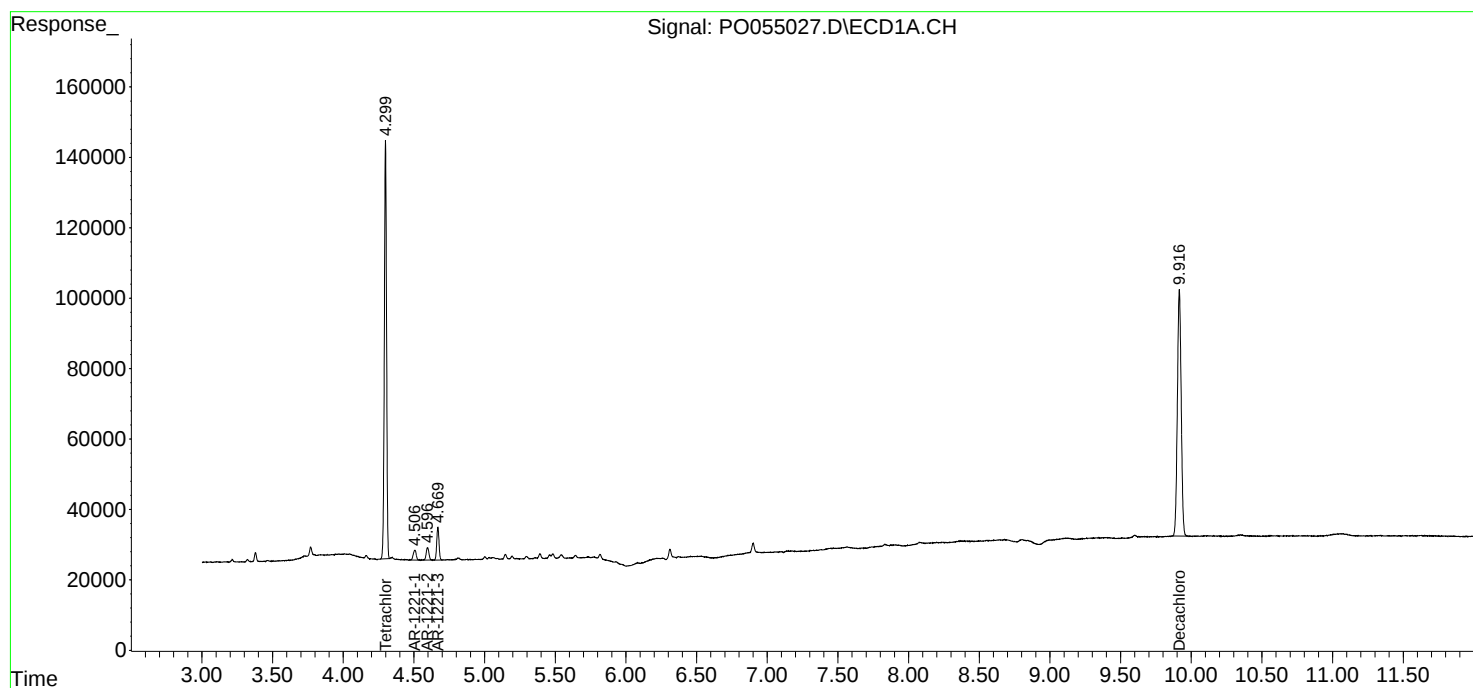


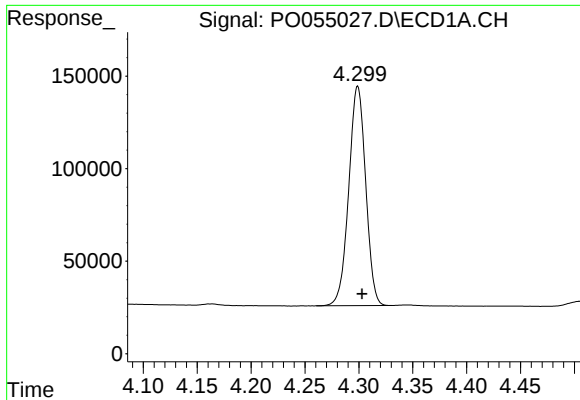

#1 Tetrachloro-m-xylene


R.T.: 4.299 min
Delta R.T.: -0.004 min
Response: 1295477
Conc: 37.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

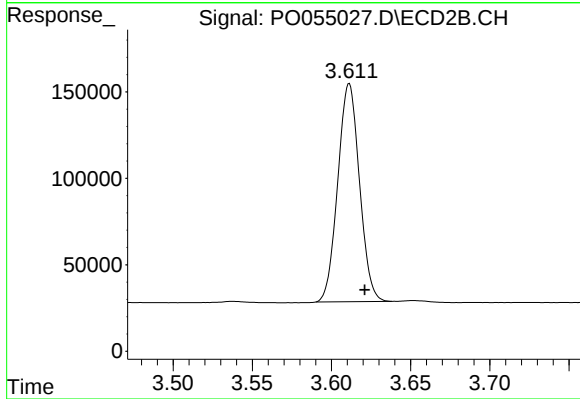


#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: -0.010 min
Response: 1202855
Conc: 37.69 ng/ml

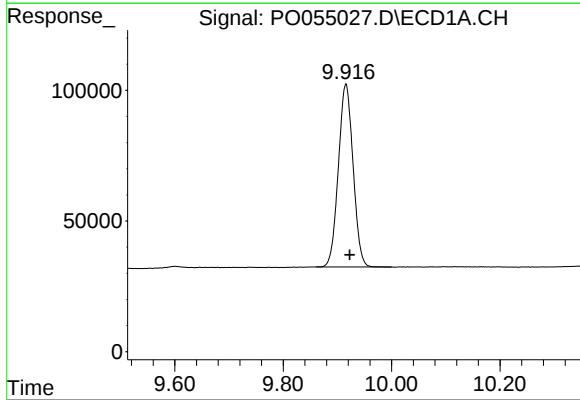


#2 Decachlorobiphenyl

R.T.: 9.916 min
Delta R.T.: -0.008 min
Response: 1314684
Conc: 26.67 ng/ml

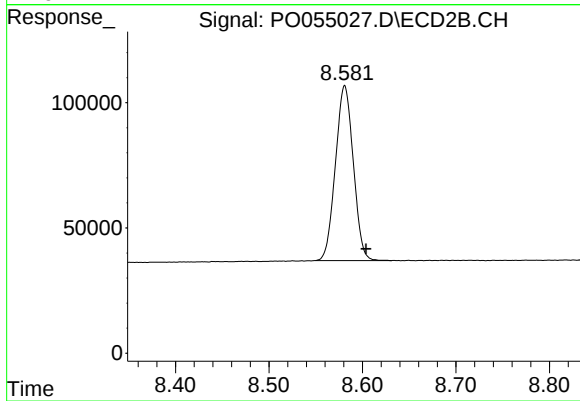

#2 Decachlorobiphenyl


R.T.: 8.581 min
Delta R.T.: -0.023 min
Response: 928713
Conc: 29.16 ng/ml

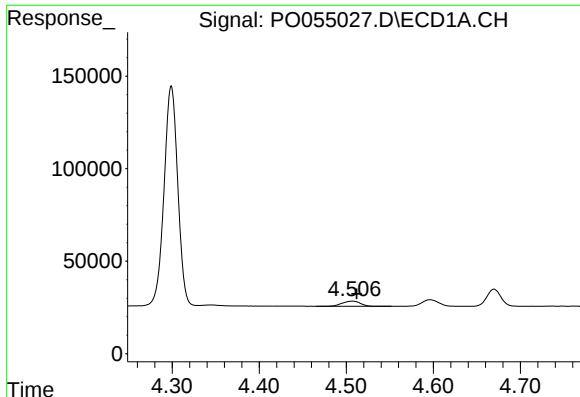

#8 AR-1221-1


R.T.: 4.507 min
Delta R.T.: -0.005 min
Response: 41724
Conc: 95.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

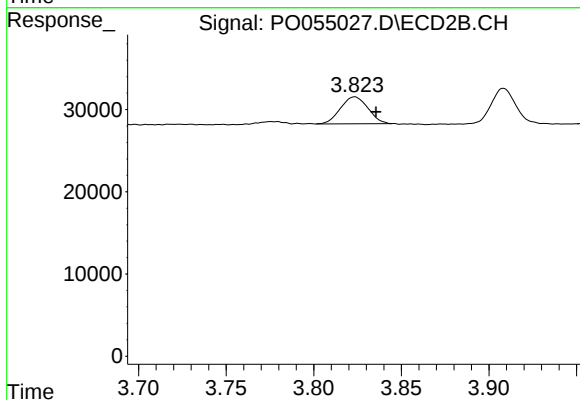


#8 AR-1221-1

R.T.: 3.824 min
Delta R.T.: -0.012 min
Response: 35785
Conc: 92.04 ng/ml

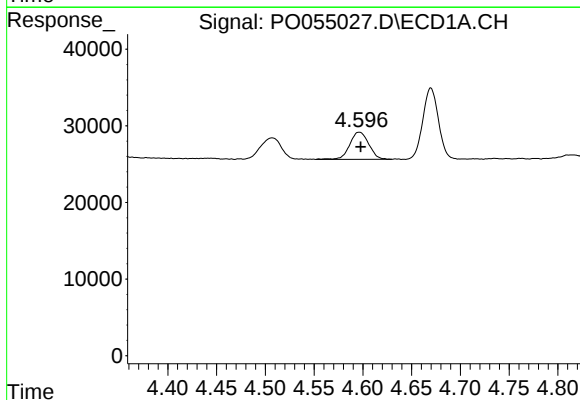


#9 AR-1221-2

R.T.: 4.596 min
Delta R.T.: -0.002 min
Response: 48143
Conc: 141.96 ng/ml

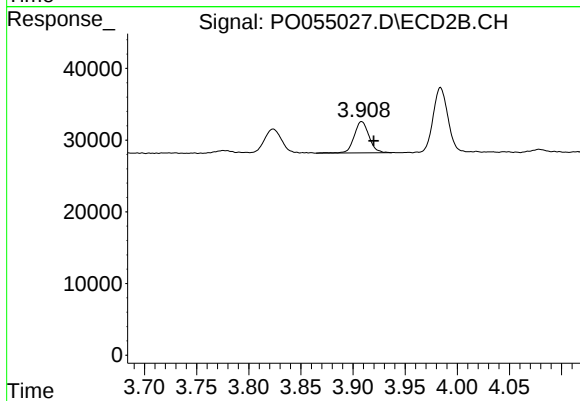

#9 AR-1221-2


R.T.: 3.908 min
Delta R.T.: -0.012 min
Response: 43414
Conc: 144.81 ng/ml

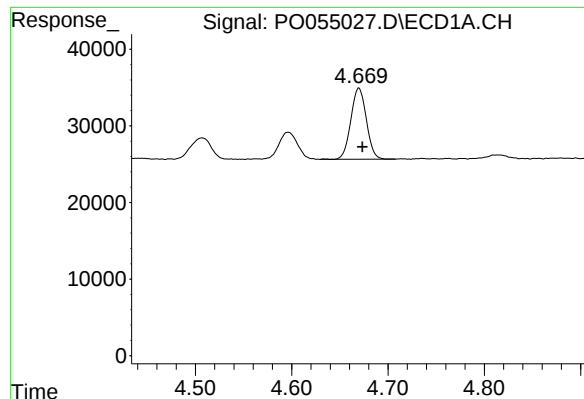

#10 AR-1221-3

R.T.: 4.670 min
Delta R.T.: -0.004 min
Response: 103365
Conc: 99.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

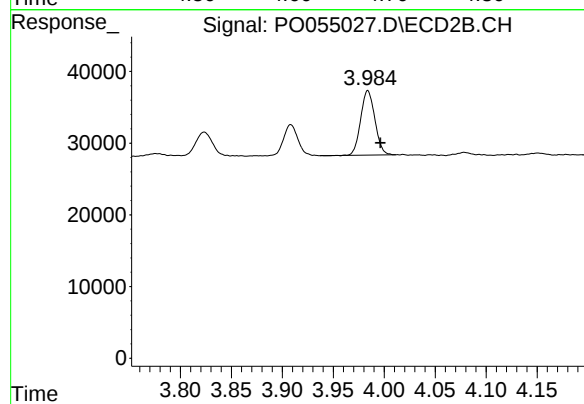

#10 AR-1221-3

R.T.: 3.984 min
Delta R.T.: -0.012 min
Response: 87459
Conc: 94.88 ng/ml