

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040819\
 Data File : P0055031.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Apr 2019 12:07
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1232 LOD 40PPB
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Manual Integrations
 APPROVED

mohammad
 4/10/2019 4:02:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 06:50:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.299	3.612	1260463	1178350	36.319	36.925
2) SA Decachlor...	9.918	8.581	1292391	910812	26.216	28.599
Target Compounds						
11) L3 AR-1232-1	4.670	3.985	82199	70872	95.473	94.510
12) L3 AR-1232-2	5.195	4.708	44368	75881	90.707	88.121
13) L3 AR-1232-3	5.484	4.883	86757	40174	88.772	82.907
14) L3 AR-1232-4	5.642	4.964	43569	36530	85.119	83.136
15) L3 AR-1232-5	5.732	5.135	35666	43478	85.735	89.395m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040819\
Data File : PO055031.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Apr 2019 12:07
Operator : SM/SJ
Sample : K1560-07
Misc : AR1232 LOD 40PPB
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:02:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 06:50:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

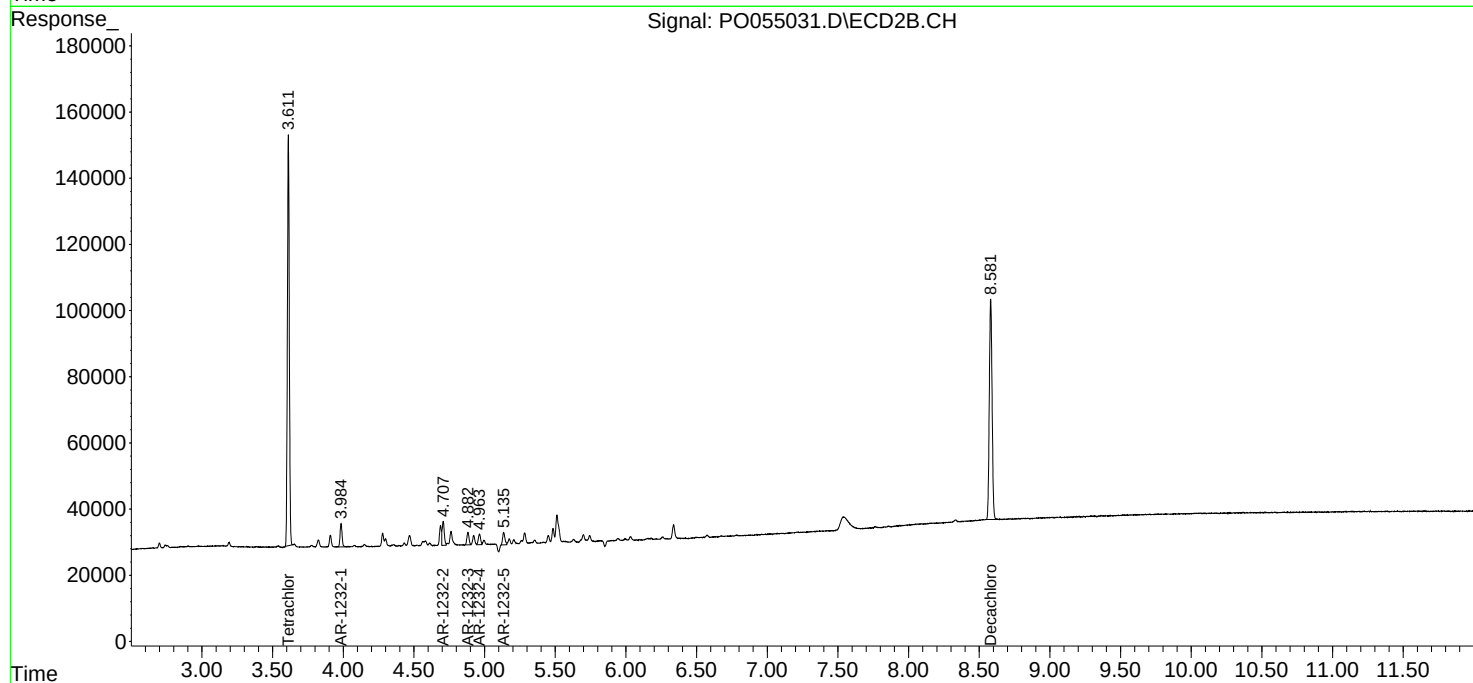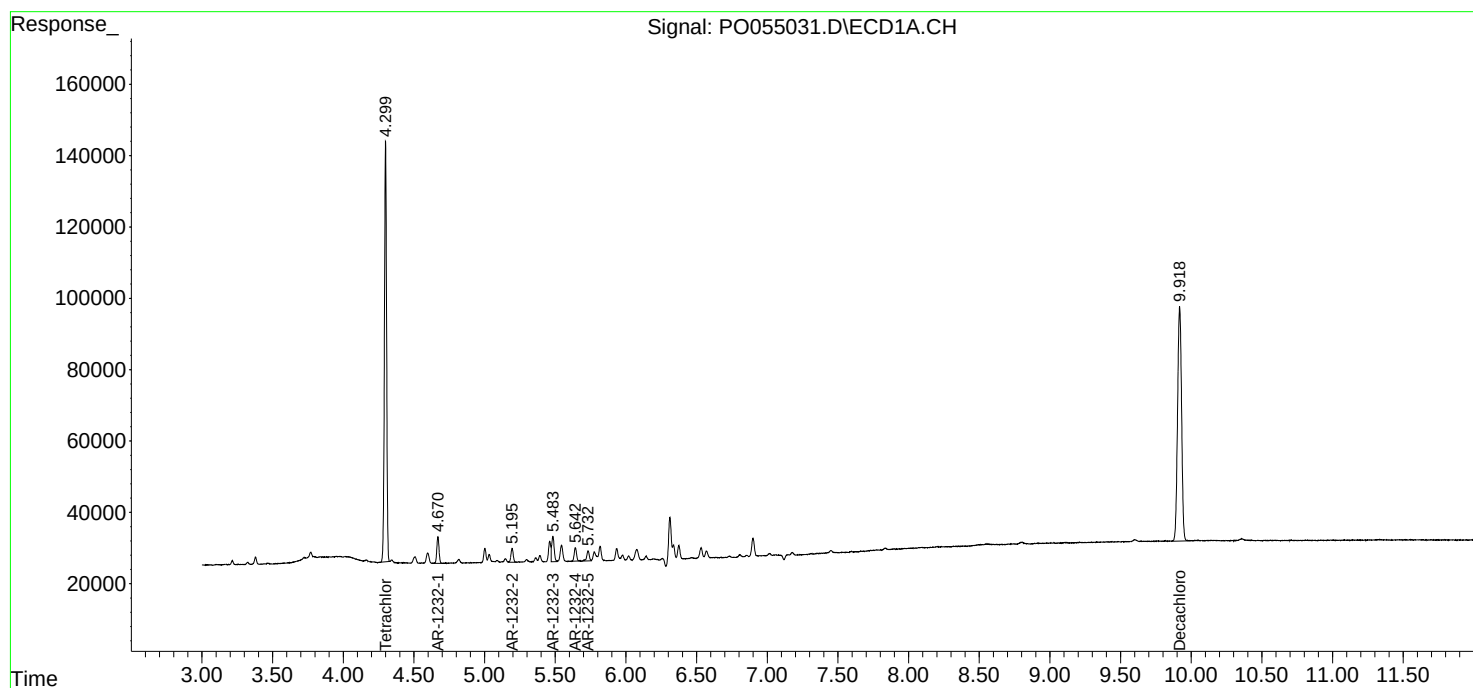

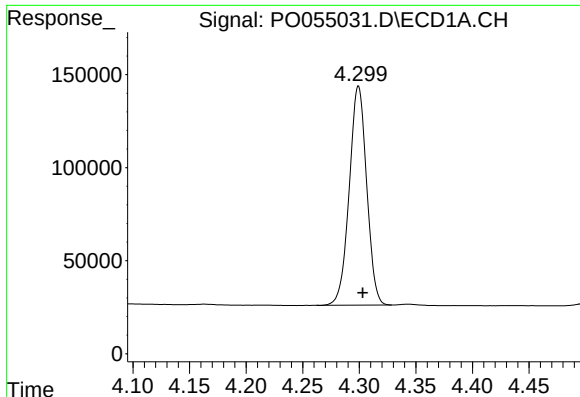


#1 Tetrachloro-m-xylene

R.T.: 4.299 min
Delta R.T.: -0.004 min
Response: 1260463
Conc: 36.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:02:41 PM

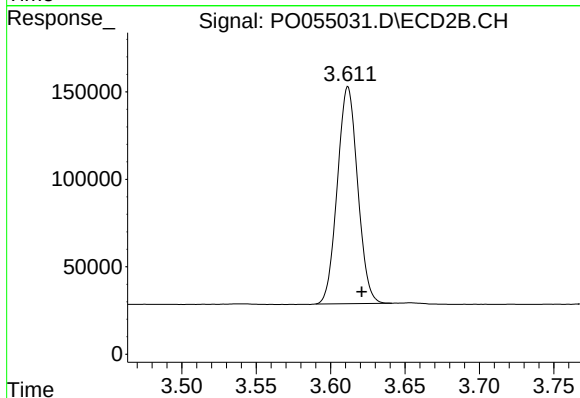


#1 Tetrachloro-m-xylene

R.T.: 3.612 min
Delta R.T.: -0.009 min
Response: 1178350
Conc: 36.92 ng/ml

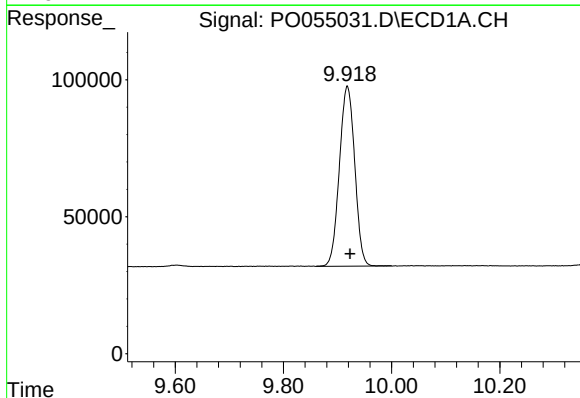


#2 Decachlorobiphenyl

R.T.: 9.918 min
Delta R.T.: -0.005 min
Response: 1292391
Conc: 26.22 ng/ml

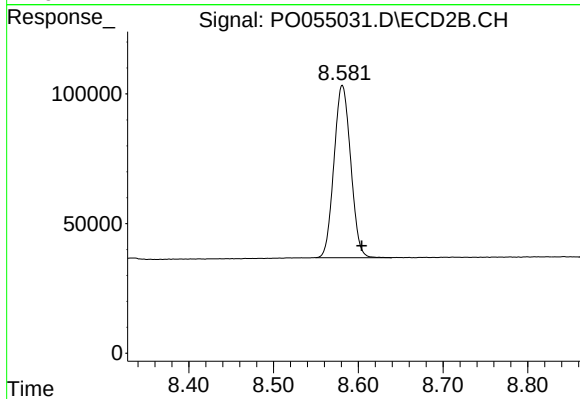

#2 Decachlorobiphenyl

R.T.: 8.581 min
Delta R.T.: -0.023 min
Response: 910812
Conc: 28.60 ng/ml

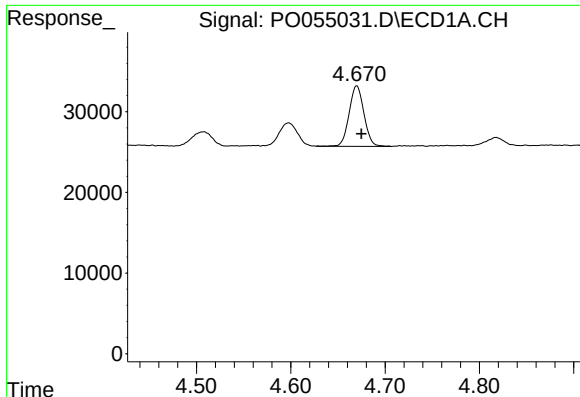


#11 AR-1232-1

R.T.: 4.670 min
Delta R.T.: -0.005 min
Response: 82199
Conc: 95.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:02:41 PM

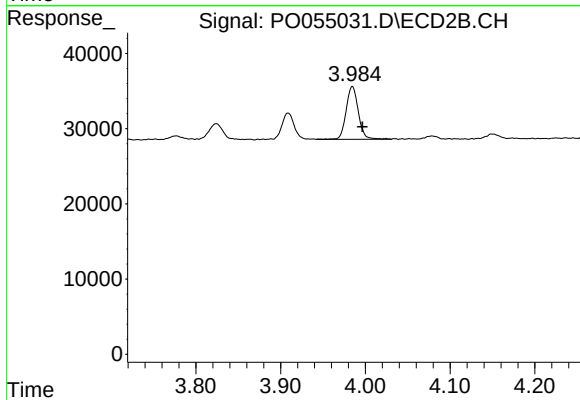


#11 AR-1232-1

R.T.: 3.985 min
Delta R.T.: -0.012 min
Response: 70872
Conc: 94.51 ng/ml

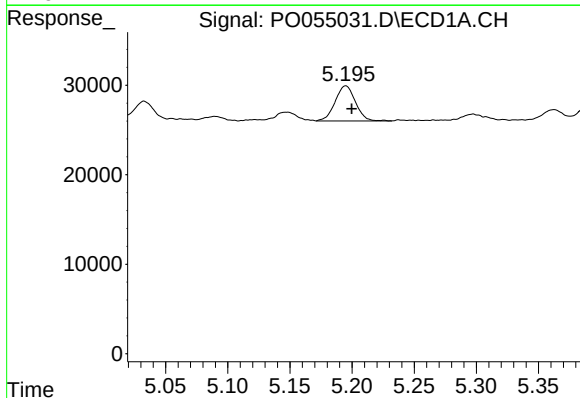


#12 AR-1232-2

R.T.: 5.195 min
Delta R.T.: -0.005 min
Response: 44368
Conc: 90.71 ng/ml

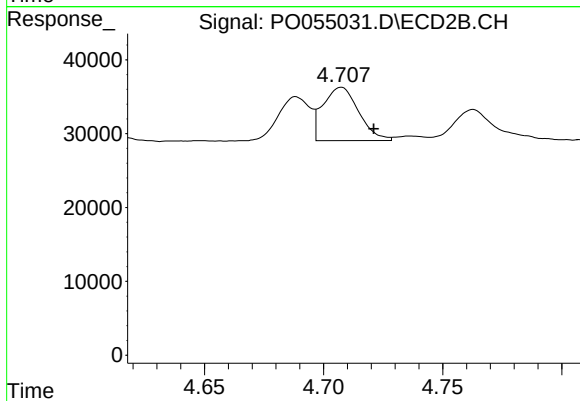

#12 AR-1232-2

R.T.: 4.708 min
Delta R.T.: -0.013 min
Response: 75881
Conc: 88.12 ng/ml

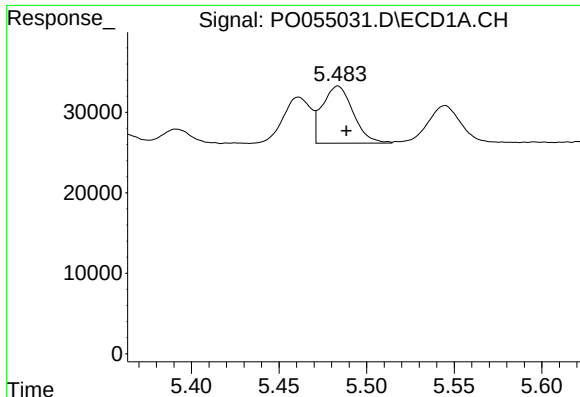


#13 AR-1232-3

R.T.: 5.484 min
Delta R.T.: -0.005 min
Response: 86757
Conc: 88.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:02:41 PM

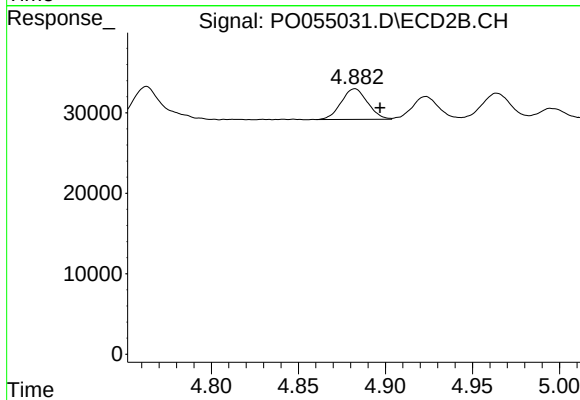


#13 AR-1232-3

R.T.: 4.883 min
Delta R.T.: -0.014 min
Response: 40174
Conc: 82.91 ng/ml

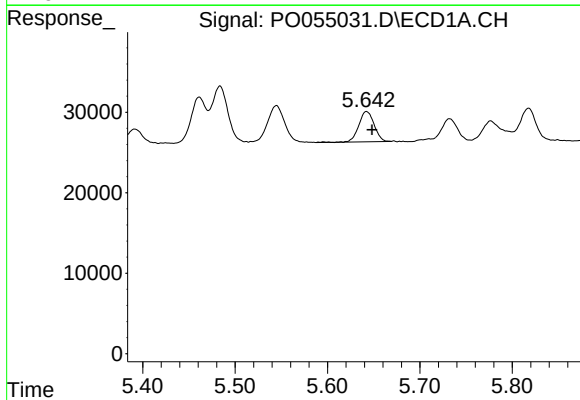


#14 AR-1232-4

R.T.: 5.642 min
Delta R.T.: -0.006 min
Response: 43569
Conc: 85.12 ng/ml

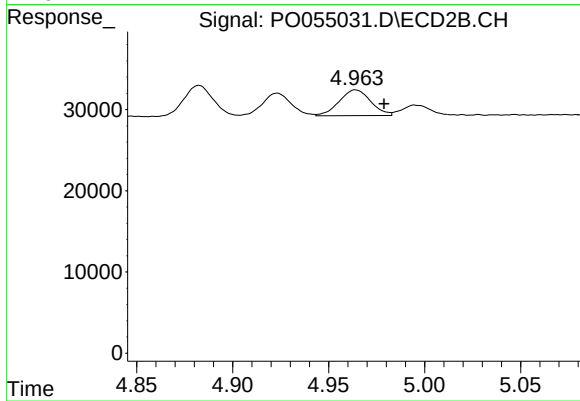

#14 AR-1232-4

R.T.: 4.964 min
Delta R.T.: -0.015 min
Response: 36530
Conc: 83.14 ng/ml

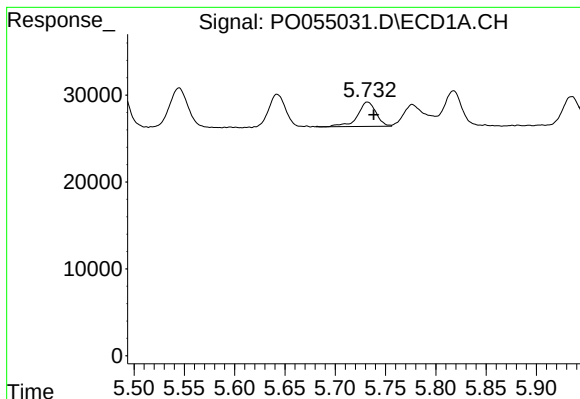


#15 AR-1232-5

R.T.: 5.732 min
Delta R.T.: -0.006 min
Response: 35666
Conc: 85.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Manual Integrations
APPROVED

mohammad
4/10/2019 4:02:41 PM

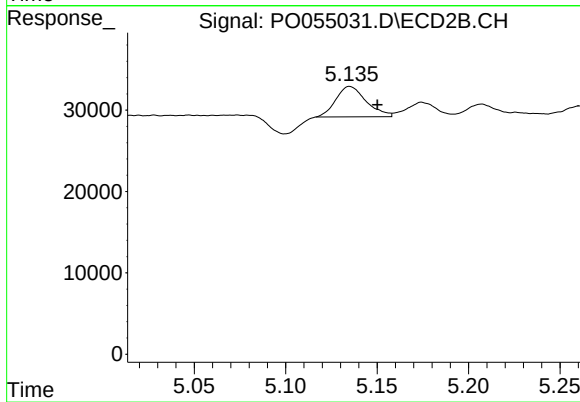

#15 AR-1232-5

R.T.: 5.135 min
Delta R.T.: -0.015 min
Response: 43478
Conc: 89.40 ng/ml m