

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040819\
 Data File : P0055033.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Apr 2019 12:41
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1242 LOD 25PPB
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Manual Integrations
 APPROVED

mohammad
 4/10/2019 4:02:47 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 06:51:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.299	3.611	1367854	1277249	39.414	40.024
2) SA Decachlor...	9.916	8.581	1423672	1011479	28.879	31.759
Target Compounds						
16) L4 AR-1242-1	5.461	4.687	75564	62992	54.391	51.309m
17) L4 AR-1242-2	5.482	4.706	102544	88232	53.591	53.241m
18) L4 AR-1242-3	5.544	4.882	70317	45623	56.733	48.159
19) L4 AR-1242-4	5.642	4.962	54251	47518	53.211	49.717
20) L4 AR-1242-5	6.373	5.483	70520	67960	58.418	55.257m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040819\
Data File : PO055033.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Apr 2019 12:41
Operator : SM/SJ
Sample : K1560-07
Misc : AR1242 LOD 25PPB
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:02:47 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 06:51:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

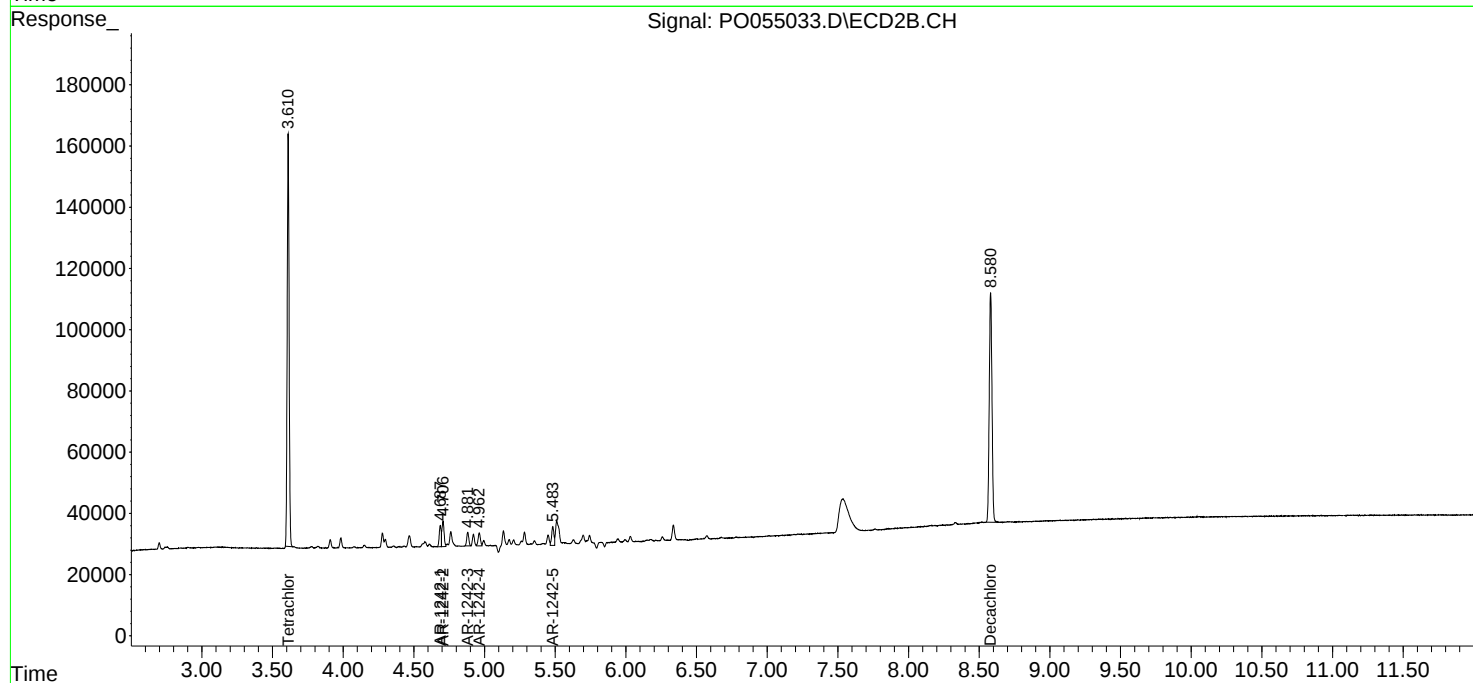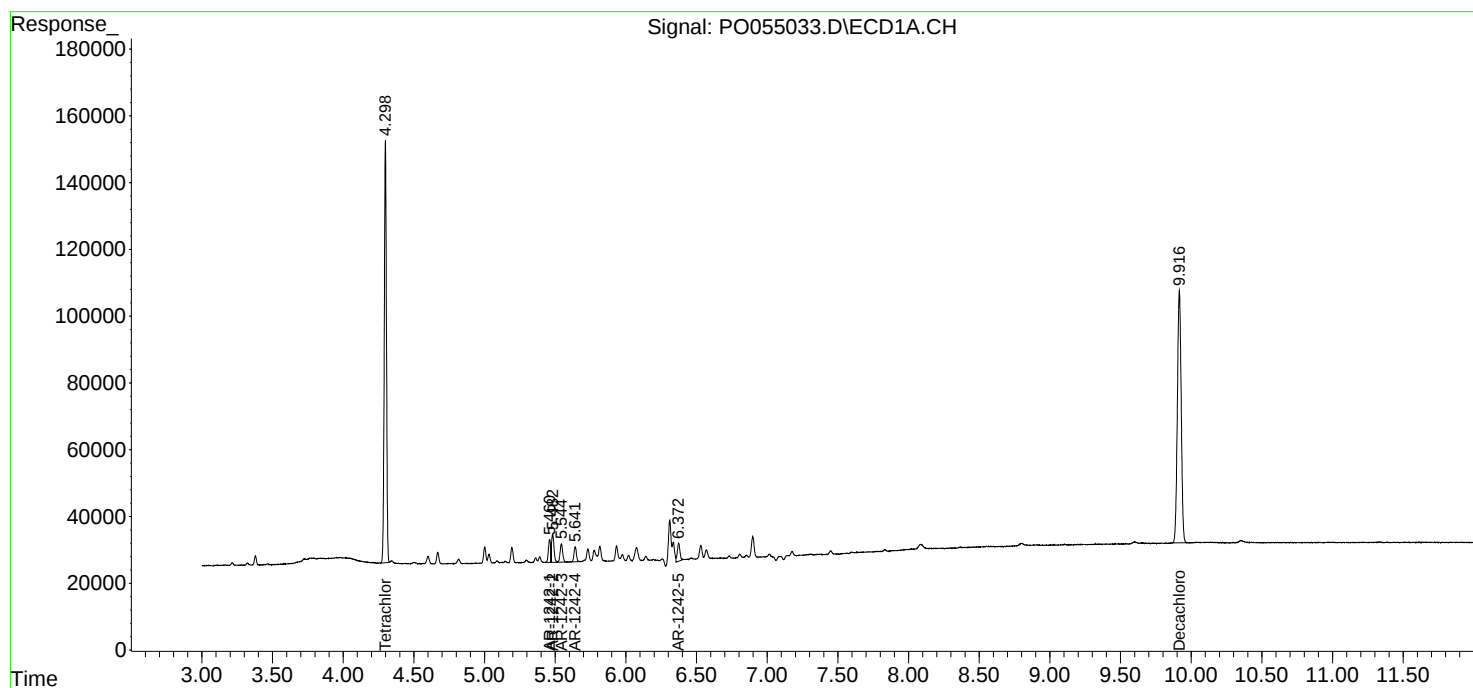

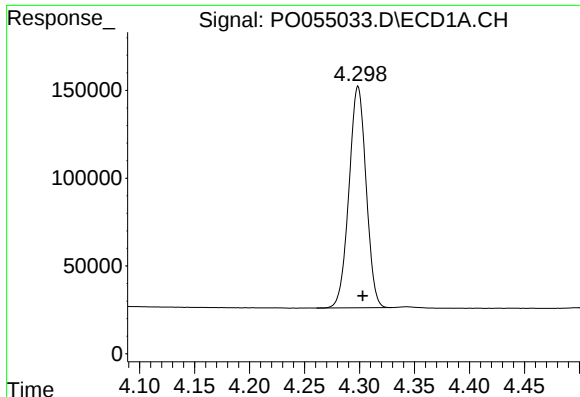


#1 Tetrachloro-m-xylene

R.T.: 4.299 min
Delta R.T.: -0.004 min
Response: 1367854
Conc: 39.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:02:47 PM

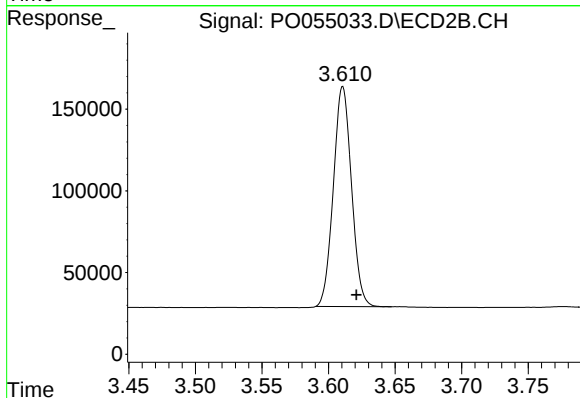


#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: -0.010 min
Response: 1277249
Conc: 40.02 ng/ml

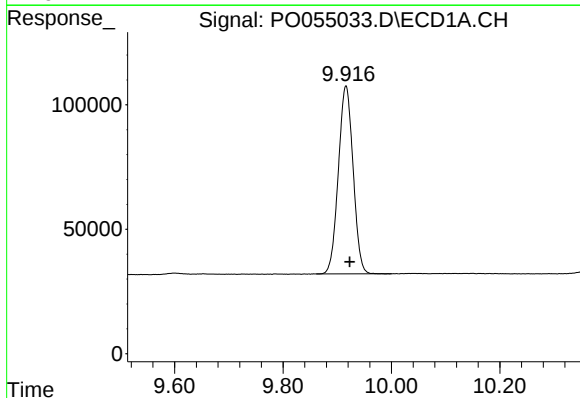


#2 Decachlorobiphenyl

R.T.: 9.916 min
Delta R.T.: -0.007 min
Response: 1423672
Conc: 28.88 ng/ml

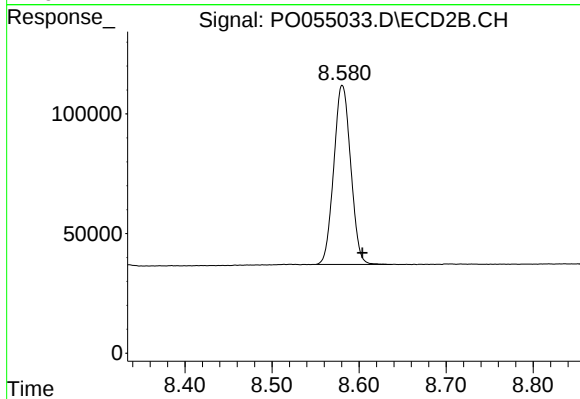

#2 Decachlorobiphenyl

R.T.: 8.581 min
Delta R.T.: -0.023 min
Response: 1011479
Conc: 31.76 ng/ml

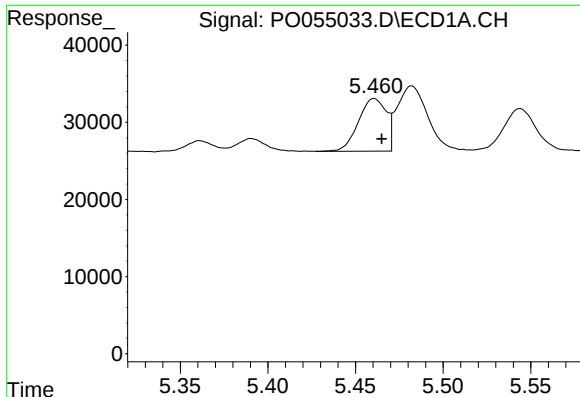


#16 AR-1242-1

R.T.: 5.461 min
Delta R.T.: -0.004 min
Response: 75564
Conc: 54.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:02:47 PM

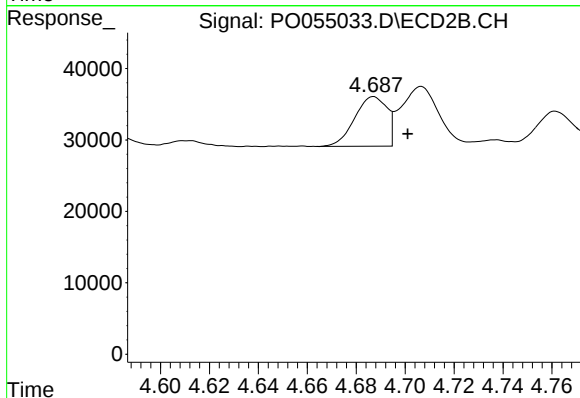


#16 AR-1242-1

R.T.: 4.687 min
Delta R.T.: -0.014 min
Response: 62992
Conc: 51.31 ng/ml m

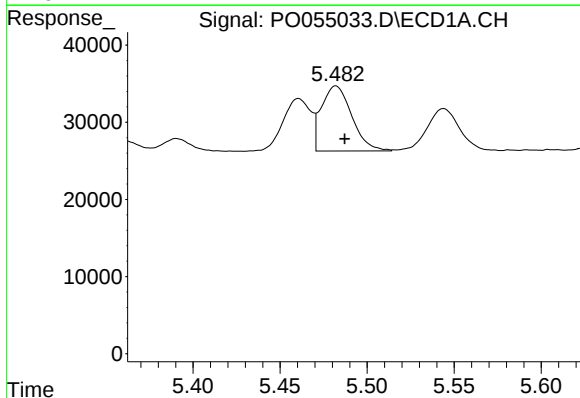


#17 AR-1242-2

R.T.: 5.482 min
Delta R.T.: -0.005 min
Response: 102544
Conc: 53.59 ng/ml

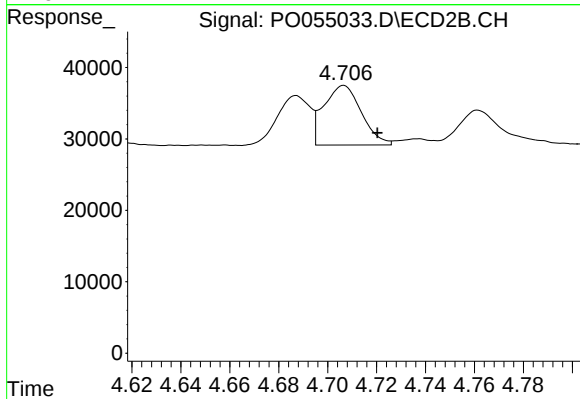

#17 AR-1242-2

R.T.: 4.706 min
Delta R.T.: -0.014 min
Response: 88232
Conc: 53.24 ng/ml m

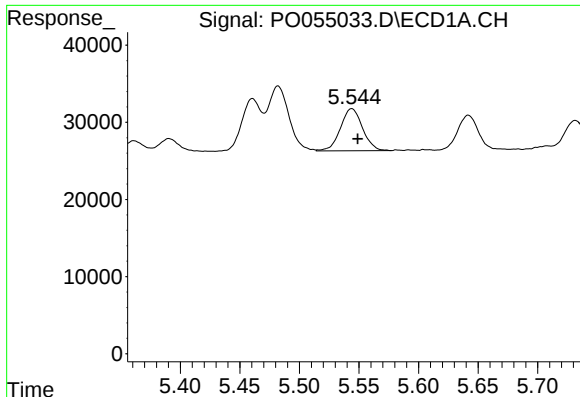


#18 AR-1242-3

R.T.: 5.544 min
Delta R.T.: -0.005 min
Response: 70317
Conc: 56.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:02:47 PM

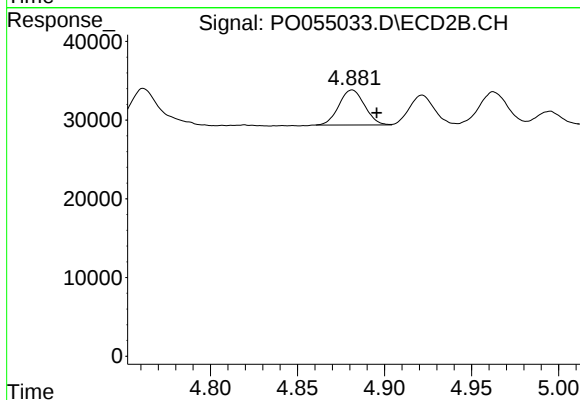


#18 AR-1242-3

R.T.: 4.882 min
Delta R.T.: -0.014 min
Response: 45623
Conc: 48.16 ng/ml

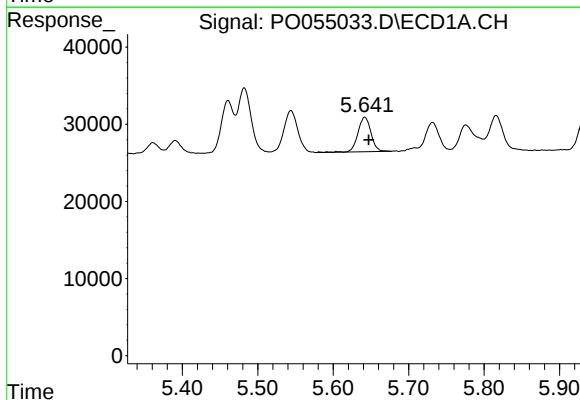


#19 AR-1242-4

R.T.: 5.642 min
Delta R.T.: -0.005 min
Response: 54251
Conc: 53.21 ng/ml

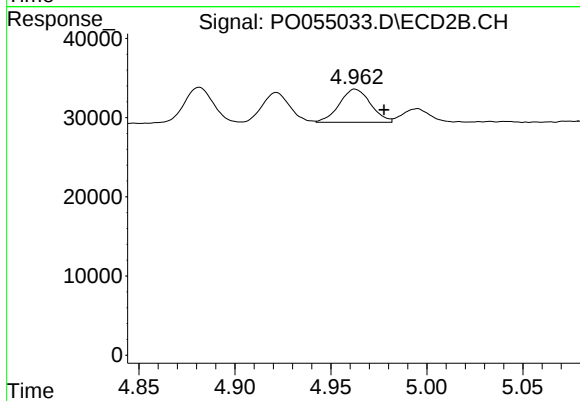

#19 AR-1242-4

R.T.: 4.962 min
Delta R.T.: -0.015 min
Response: 47518
Conc: 49.72 ng/ml

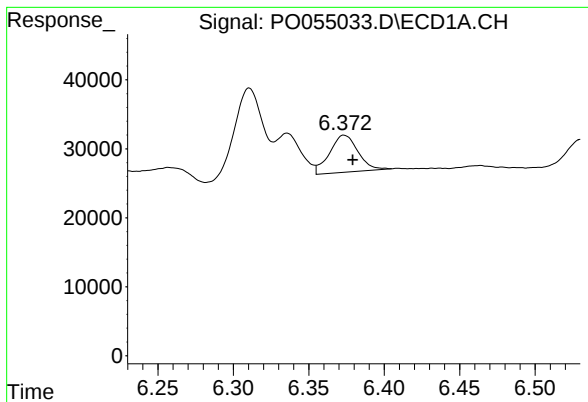


#20 AR-1242-5

R.T.: 6.373 min
Delta R.T.: -0.006 min
Response: 70520
Conc: 58.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Manual Integrations
APPROVED

mohammad
4/10/2019 4:02:47 PM

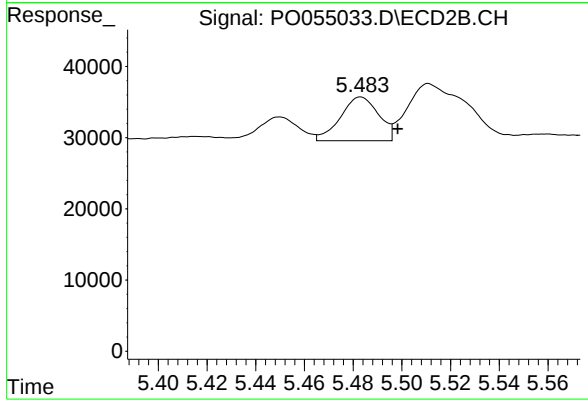

#20 AR-1242-5

R.T.: 5.483 min
Delta R.T.: -0.016 min
Response: 67960
Conc: 55.26 ng/ml m