

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040819\
 Data File : P0055036.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Apr 2019 13:32
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1248 LOD 25PPB
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Manual Integrations
 APPROVED

mohammad
 4/10/2019 4:02:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 06:53:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.299	3.611	1566221	1475136	45.129	46.225
2) SA Decachlor...	9.918	8.581	1632425	1157986	33.114	36.360
Target Compounds						
21) L5 AR-1248-1	5.461	4.688	60610	54770	60.629	62.396m
22) L5 AR-1248-2	5.733	4.923	92215	67706	63.496	56.023
23) L5 AR-1248-3	5.935	4.964	94442	73137	59.131	58.613
24) L5 AR-1248-4	6.338	5.134	109078	89671	58.065	58.879m
25) L5 AR-1248-5	6.375	5.524	103690	79501	57.837	53.325m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040819\
Data File : PO055036.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Apr 2019 13:32
Operator : SM/SJ
Sample : K1560-07
Misc : AR1248 LOD 25PPB
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:02:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 06:53:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

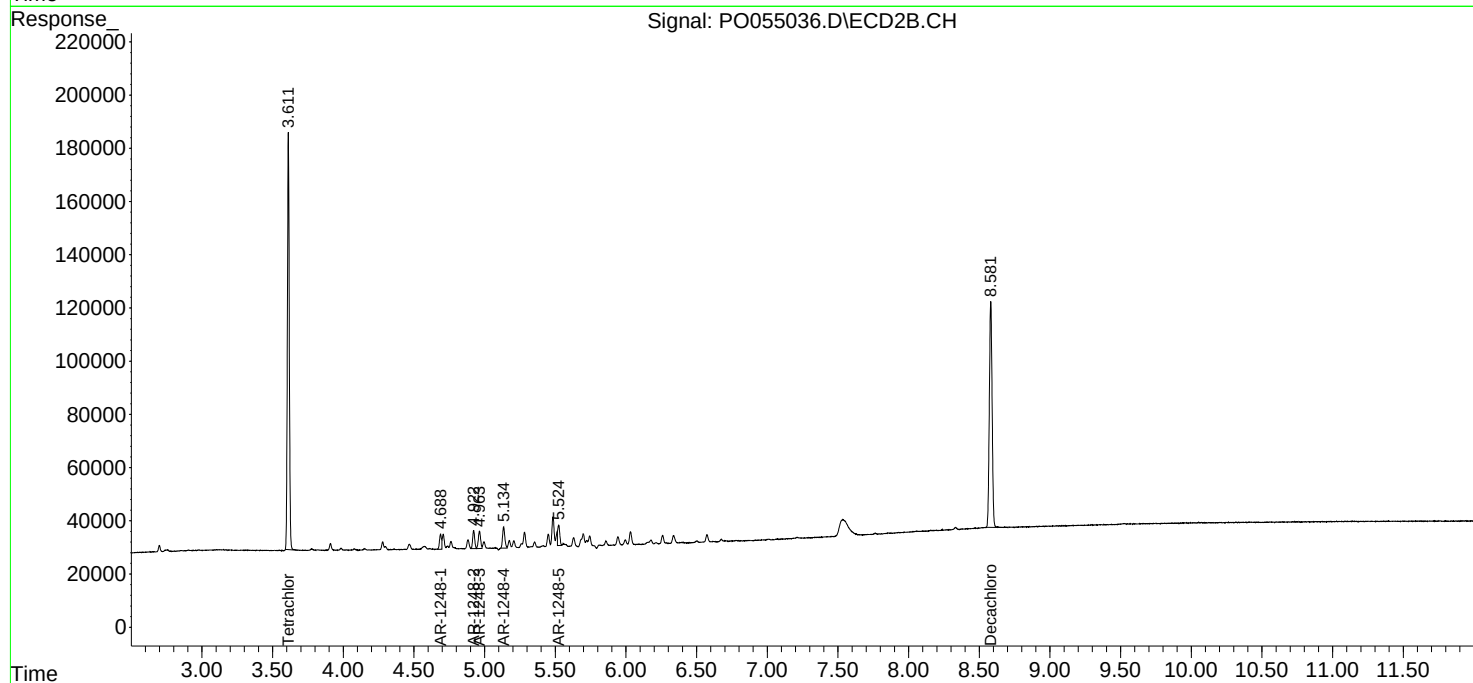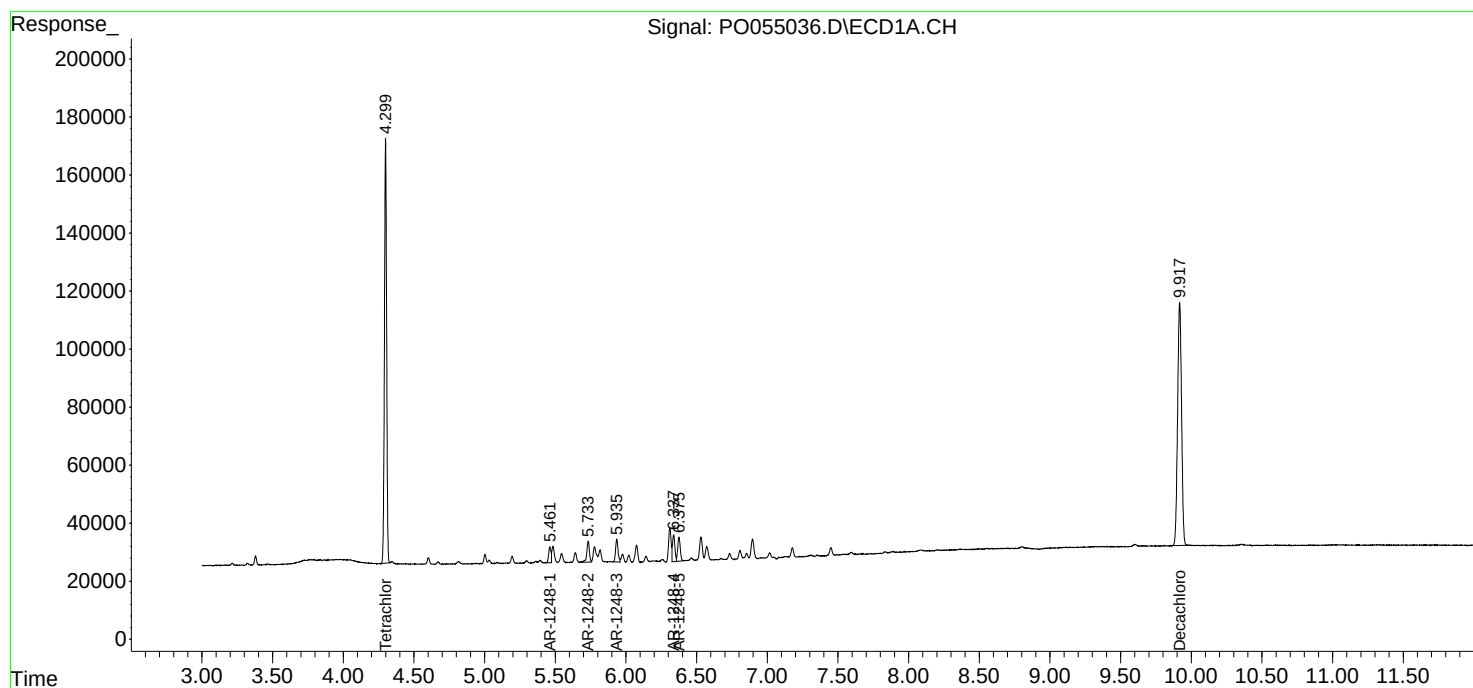

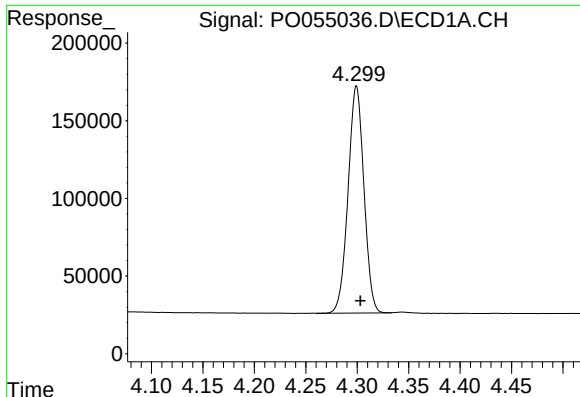


#1 Tetrachloro-m-xylene

R.T.: 4.299 min
Delta R.T.: -0.004 min
Response: 1566221
Conc: 45.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:02:50 PM

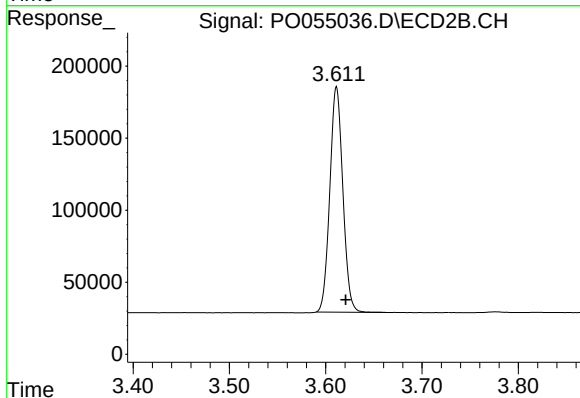


#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: -0.010 min
Response: 1475136
Conc: 46.22 ng/ml

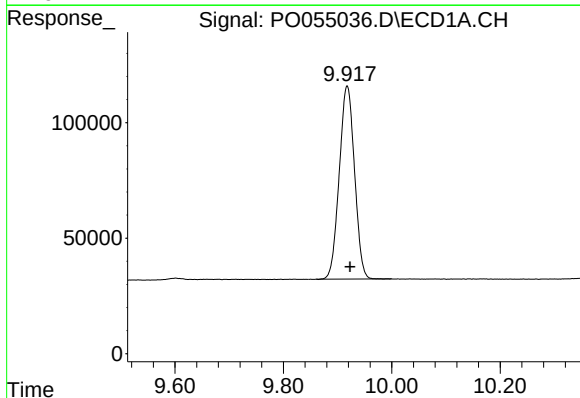


#2 Decachlorobiphenyl

R.T.: 9.918 min
Delta R.T.: -0.005 min
Response: 1632425
Conc: 33.11 ng/ml

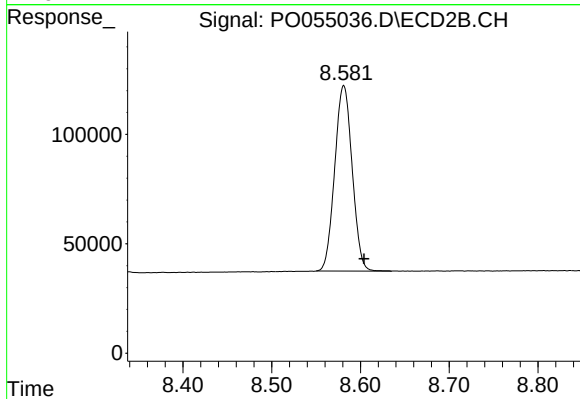

#2 Decachlorobiphenyl

R.T.: 8.581 min
Delta R.T.: -0.023 min
Response: 1157986
Conc: 36.36 ng/ml

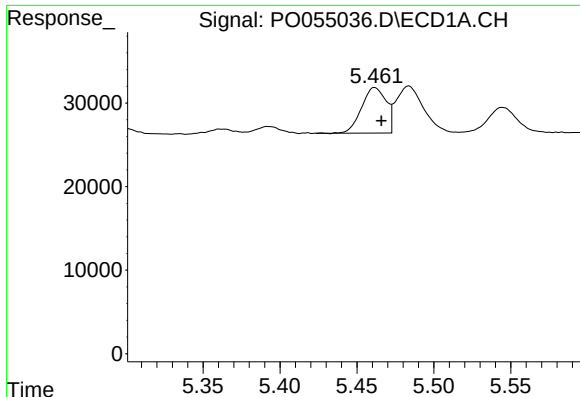


#21 AR-1248-1

R.T.: 5.461 min
Delta R.T.: -0.005 min
Response: 60610
Conc: 60.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:02:50 PM

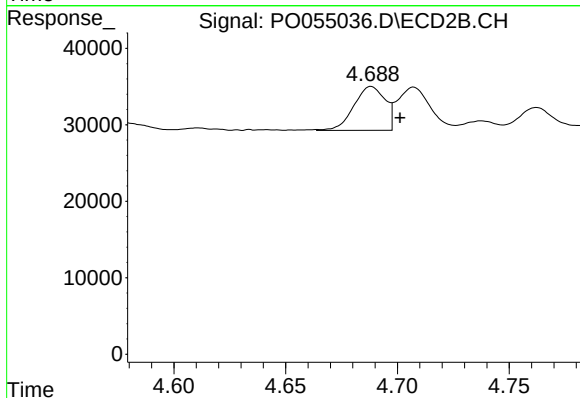


#21 AR-1248-1

R.T.: 4.688 min
Delta R.T.: -0.013 min
Response: 54770
Conc: 62.40 ng/ml m

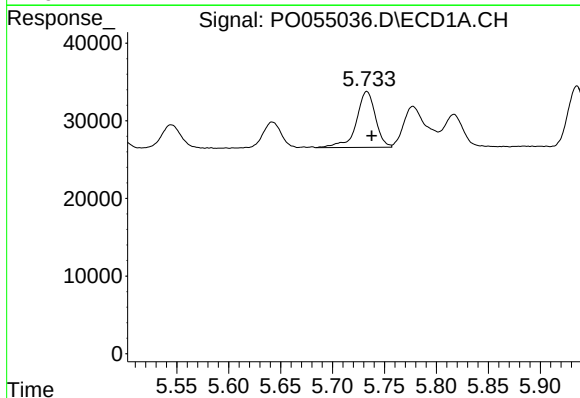


#22 AR-1248-2

R.T.: 5.733 min
Delta R.T.: -0.005 min
Response: 92215
Conc: 63.50 ng/ml

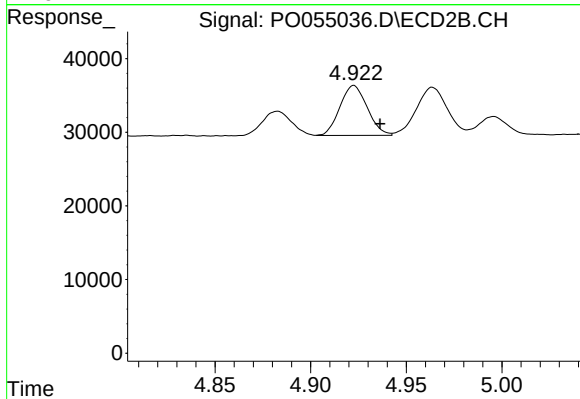

#22 AR-1248-2

R.T.: 4.923 min
Delta R.T.: -0.014 min
Response: 67706
Conc: 56.02 ng/ml

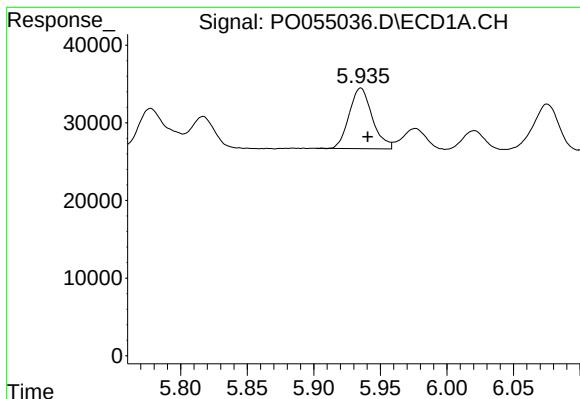


#23 AR-1248-3

R.T.: 5.935 min
Delta R.T.: -0.005 min
Response: 94442
Conc: 59.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:02:50 PM

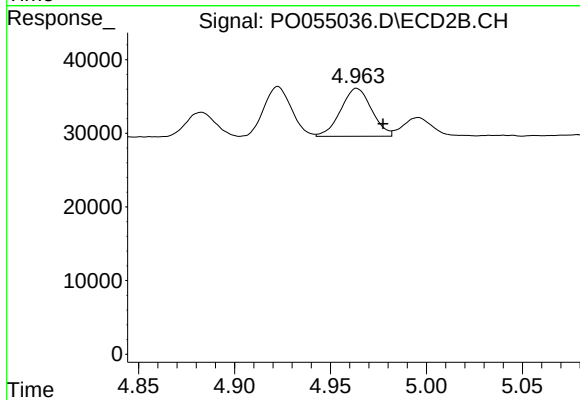


#23 AR-1248-3

R.T.: 4.964 min
Delta R.T.: -0.014 min
Response: 73137
Conc: 58.61 ng/ml

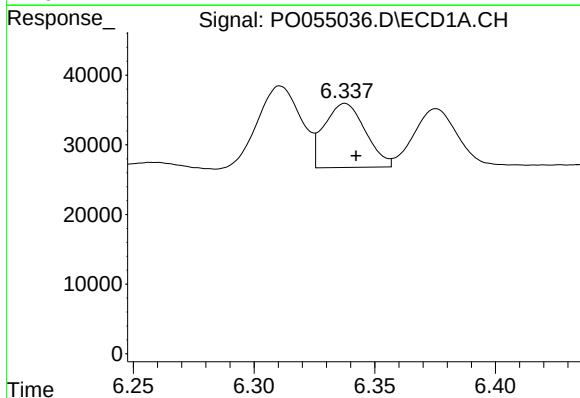


#24 AR-1248-4

R.T.: 6.338 min
Delta R.T.: -0.005 min
Response: 109078
Conc: 58.07 ng/ml

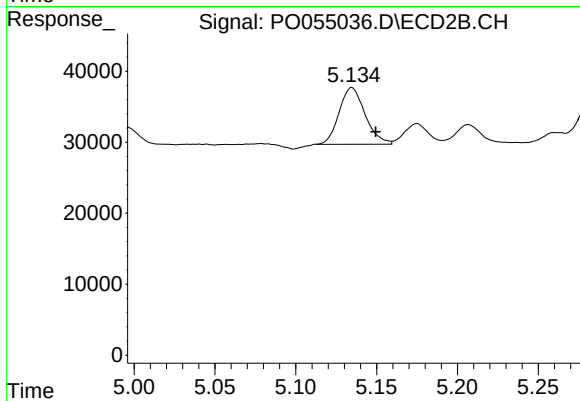

#24 AR-1248-4

R.T.: 5.134 min
Delta R.T.: -0.015 min
Response: 89671
Conc: 58.88 ng/ml m

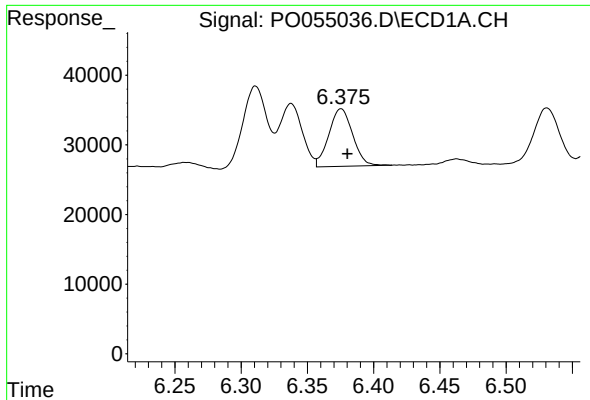


#25 AR-1248-5

R.T.: 6.375 min
Delta R.T.: -0.005 min
Response: 103690
Conc: 57.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Manual Integrations
APPROVED

mohammad
4/10/2019 4:02:50 PM

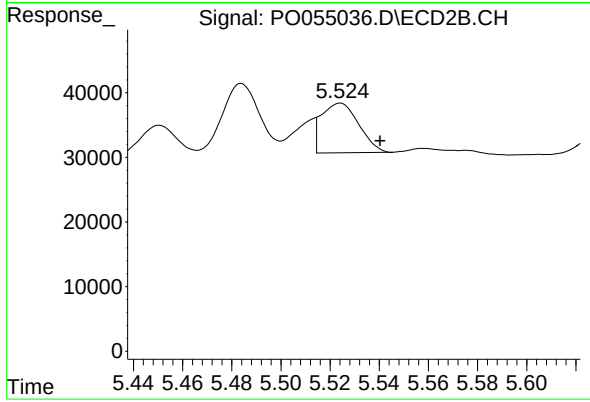

#25 AR-1248-5

R.T.: 5.524 min
Delta R.T.: -0.016 min
Response: 79501
Conc: 53.33 ng/ml m