

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040819\
 Data File : P0055037.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Apr 2019 13:49
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1248 LOD 40PPB
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Manual Integrations
 APPROVED

mohammad
 4/10/2019 4:02:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 06:53:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.298	3.610	1334918	1228235	38.465	38.488
2) SA Decachlor...	9.917	8.581	1493635	1050273	30.298	32.977
Target Compounds						
21) L5 AR-1248-1	5.460	4.687	87989	76934	88.018	87.647m
22) L5 AR-1248-2	5.731	4.922	132048	101897	90.923	84.313
23) L5 AR-1248-3	5.935	4.963	142726	104677	89.362	83.890
24) L5 AR-1248-4	6.336	5.134	150412	125092	80.068m	82.136m
25) L5 AR-1248-5	6.374	5.522	149669	120391	83.484m	80.752m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040819\
Data File : PO055037.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Apr 2019 13:49
Operator : SM/SJ
Sample : K1560-07
Misc : AR1248 LOD 40PPB
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:02:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 06:53:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

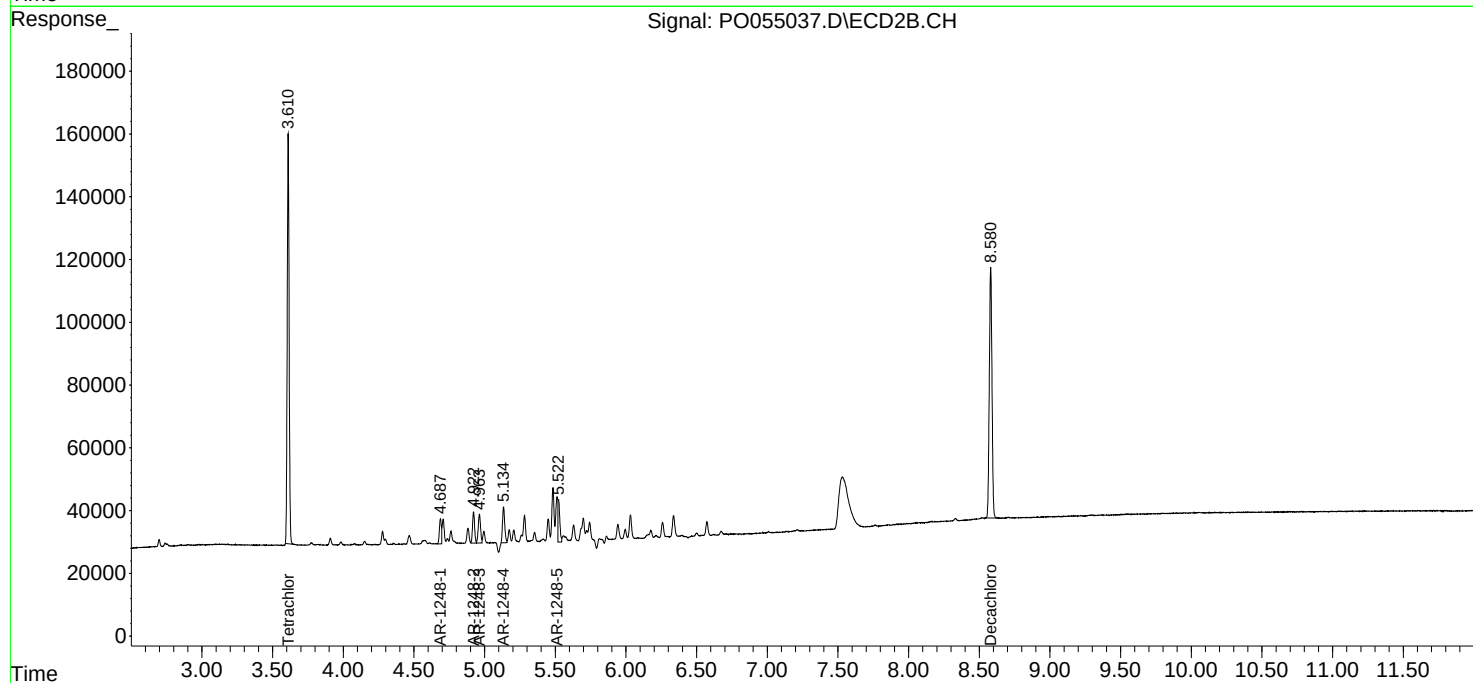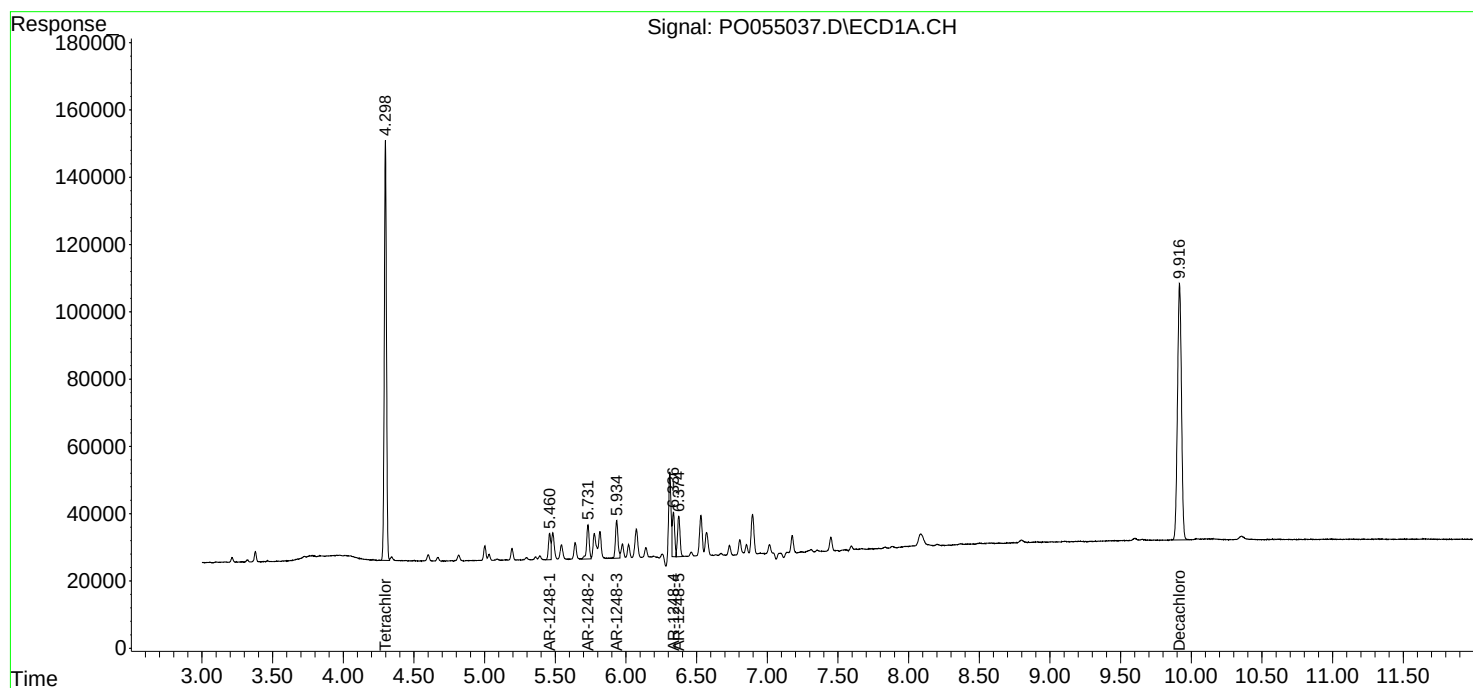

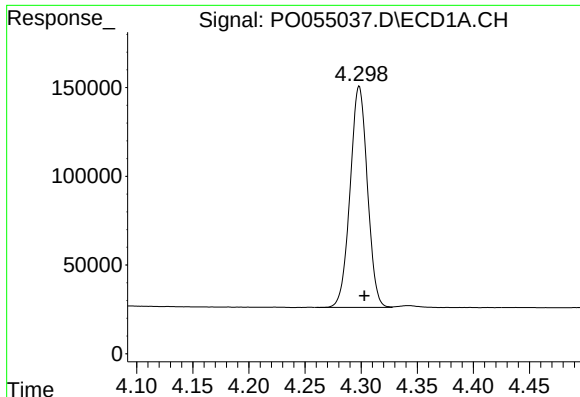


#1 Tetrachloro-m-xylene

R.T.: 4.298 min
Delta R.T.: -0.005 min
Response: 1334918
Conc: 38.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:02:53 PM

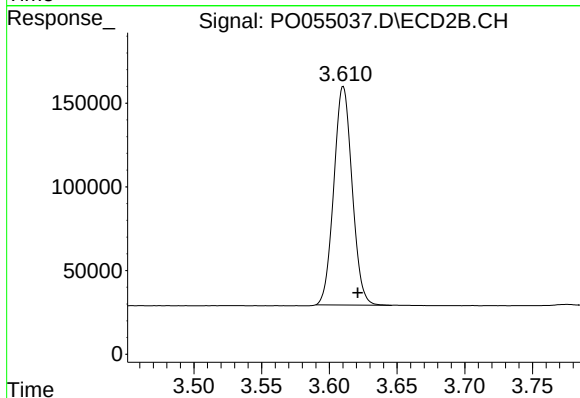


#1 Tetrachloro-m-xylene

R.T.: 3.610 min
Delta R.T.: -0.011 min
Response: 1228235
Conc: 38.49 ng/ml

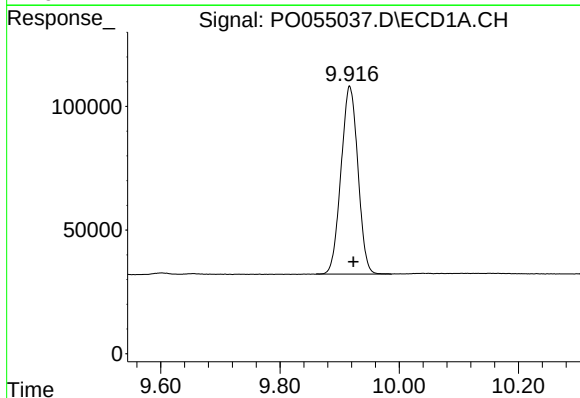


#2 Decachlorobiphenyl

R.T.: 9.917 min
Delta R.T.: -0.006 min
Response: 1493635
Conc: 30.30 ng/ml

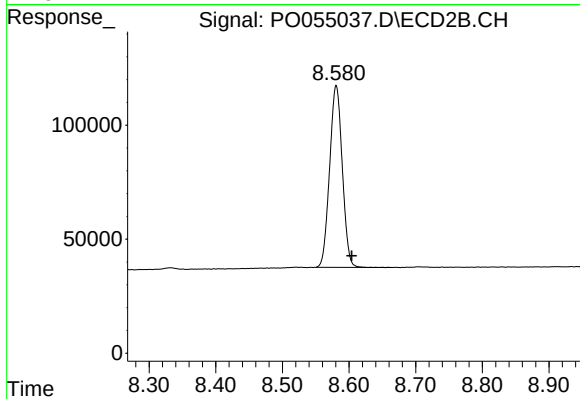

#2 Decachlorobiphenyl

R.T.: 8.581 min
Delta R.T.: -0.023 min
Response: 1050273
Conc: 32.98 ng/ml

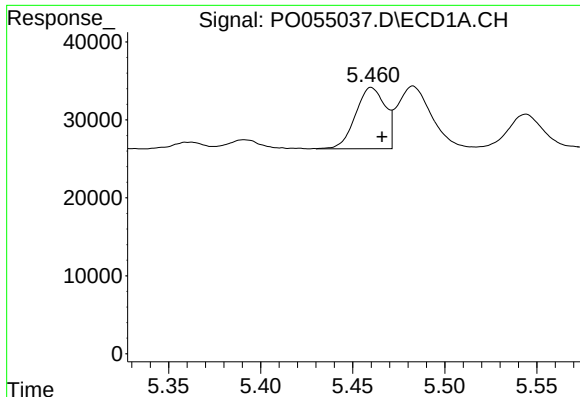


#21 AR-1248-1

R.T.: 5.460 min
Delta R.T.: -0.006 min
Response: 87989
Conc: 88.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:02:53 PM

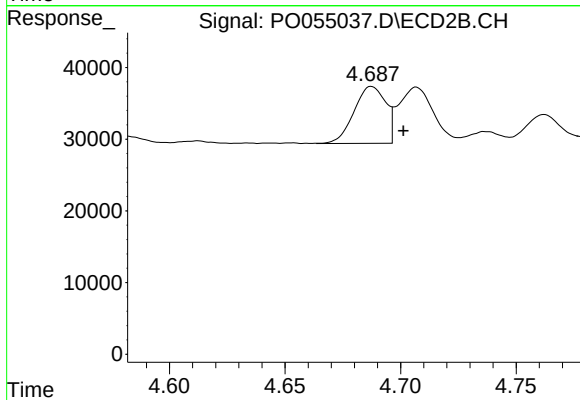


#21 AR-1248-1

R.T.: 4.687 min
Delta R.T.: -0.014 min
Response: 76934
Conc: 87.65 ng/ml m

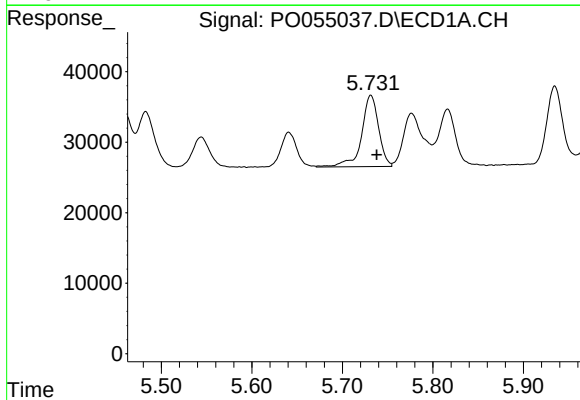


#22 AR-1248-2

R.T.: 5.731 min
Delta R.T.: -0.006 min
Response: 132048
Conc: 90.92 ng/ml

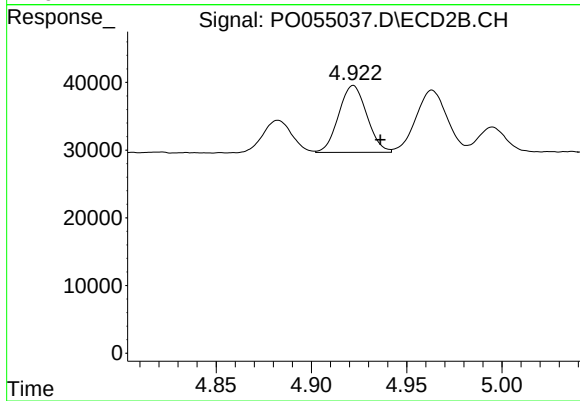

#22 AR-1248-2

R.T.: 4.922 min
Delta R.T.: -0.014 min
Response: 101897
Conc: 84.31 ng/ml

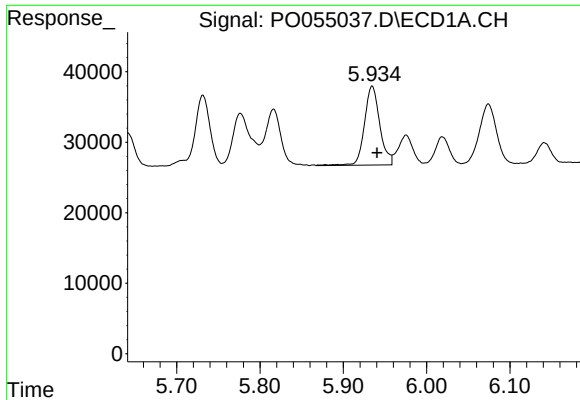


#23 AR-1248-3

R.T.: 5.935 min
Delta R.T.: -0.006 min
Response: 142726
Conc: 89.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:02:53 PM

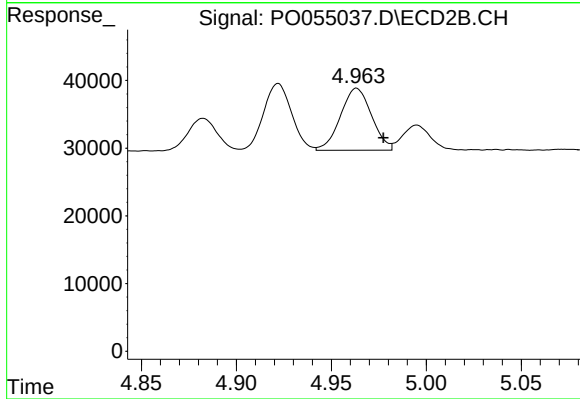


#23 AR-1248-3

R.T.: 4.963 min
Delta R.T.: -0.014 min
Response: 104677
Conc: 83.89 ng/ml

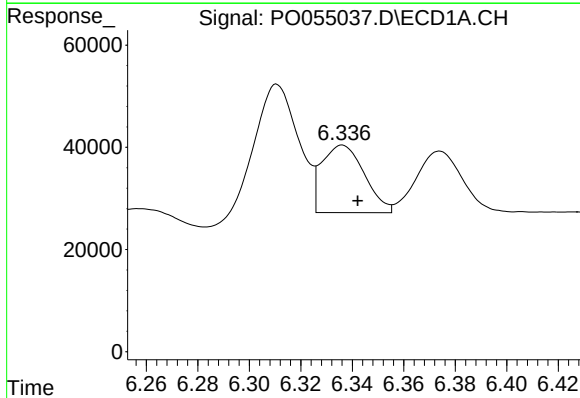


#24 AR-1248-4

R.T.: 6.336 min
Delta R.T.: -0.006 min
Response: 150412
Conc: 80.07 ng/ml m

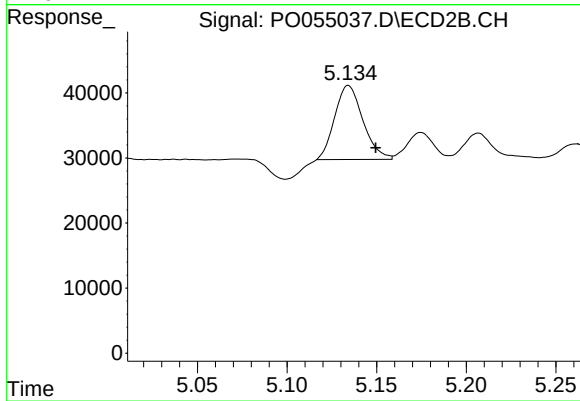

#24 AR-1248-4

R.T.: 5.134 min
Delta R.T.: -0.016 min
Response: 125092
Conc: 82.14 ng/ml m

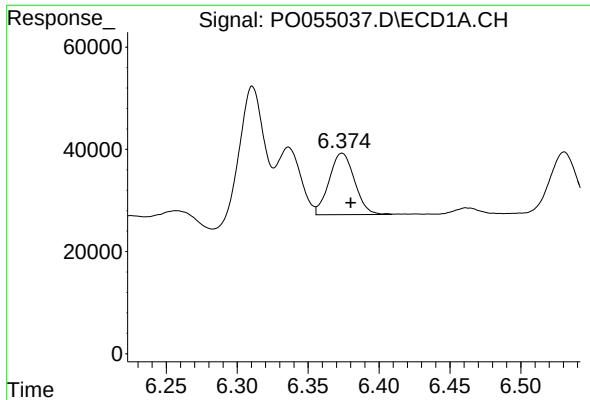


#25 AR-1248-5

R.T.: 6.374 min
Delta R.T.: -0.007 min
Response: 149669
Conc: 83.48 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Manual Integrations
APPROVED

mohammad
4/10/2019 4:02:53 PM

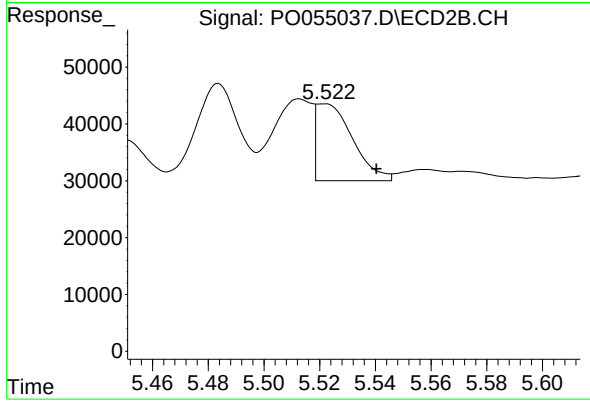

#25 AR-1248-5

R.T.: 5.522 min
Delta R.T.: -0.018 min
Response: 120391
Conc: 80.75 ng/ml m