

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040819\
 Data File : P0055040.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Apr 2019 14:40
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1254 LOD 40PPB
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Manual Integrations
 APPROVED

mohammad
 4/10/2019 4:03:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 06:55:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.299	3.611	1210106	1136712	34.868	35.620
2)	SA Decachlor...	9.917	8.581	1346450	953600	27.313	29.942
Target Compounds							
26)	L6 AR-1254-1	6.311	5.485	186131	180800	102.654m	82.728m
27)	L6 AR-1254-2	6.528	5.630	228732	171250	80.124	88.321m
28)	L6 AR-1254-3	6.894	6.033	267363	268415	85.020	83.731m
29)	L6 AR-1254-4	7.177	6.259	169329	174355	69.217	89.050m#
30)	L6 AR-1254-5	7.595	6.675	174416	197627	65.073	68.747

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040819\
Data File : PO055040.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Apr 2019 14:40
Operator : SM/SJ
Sample : K1560-07
Misc : AR1254 LOD 40PPB
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:03:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 06:55:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

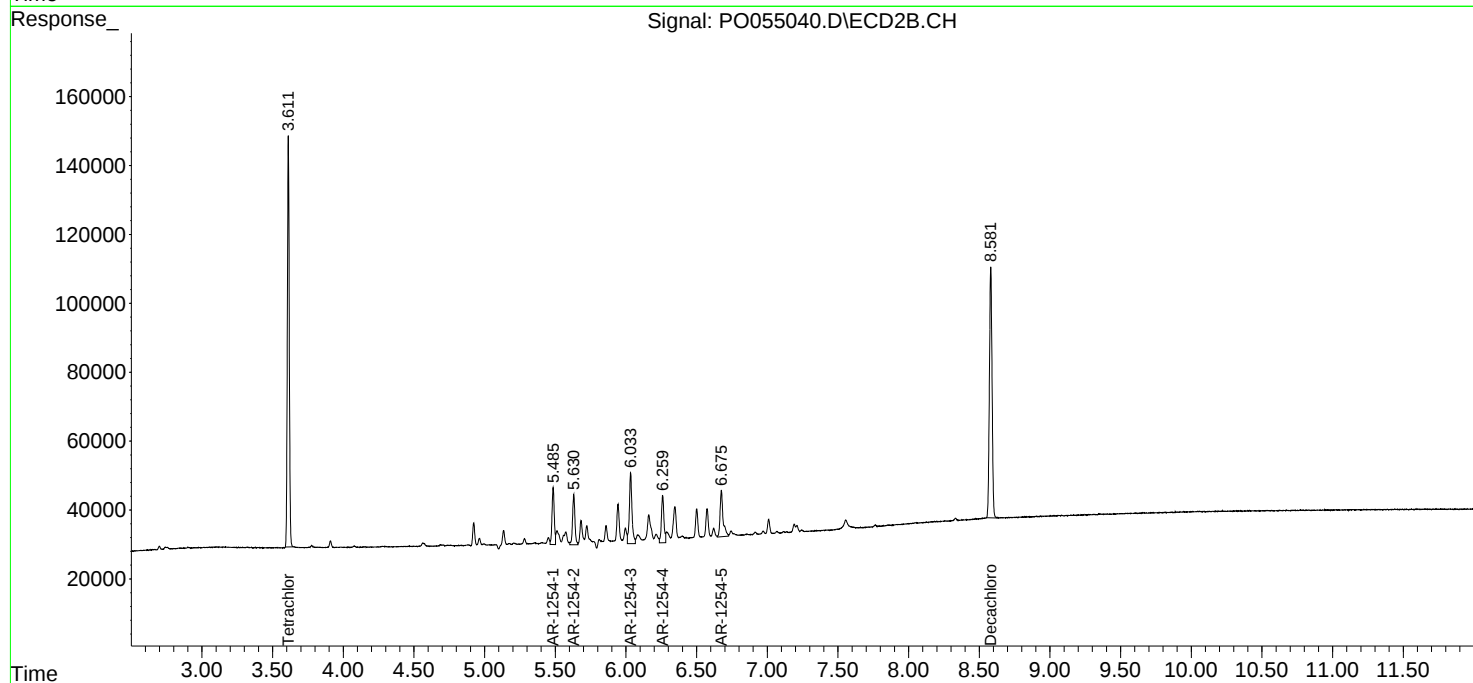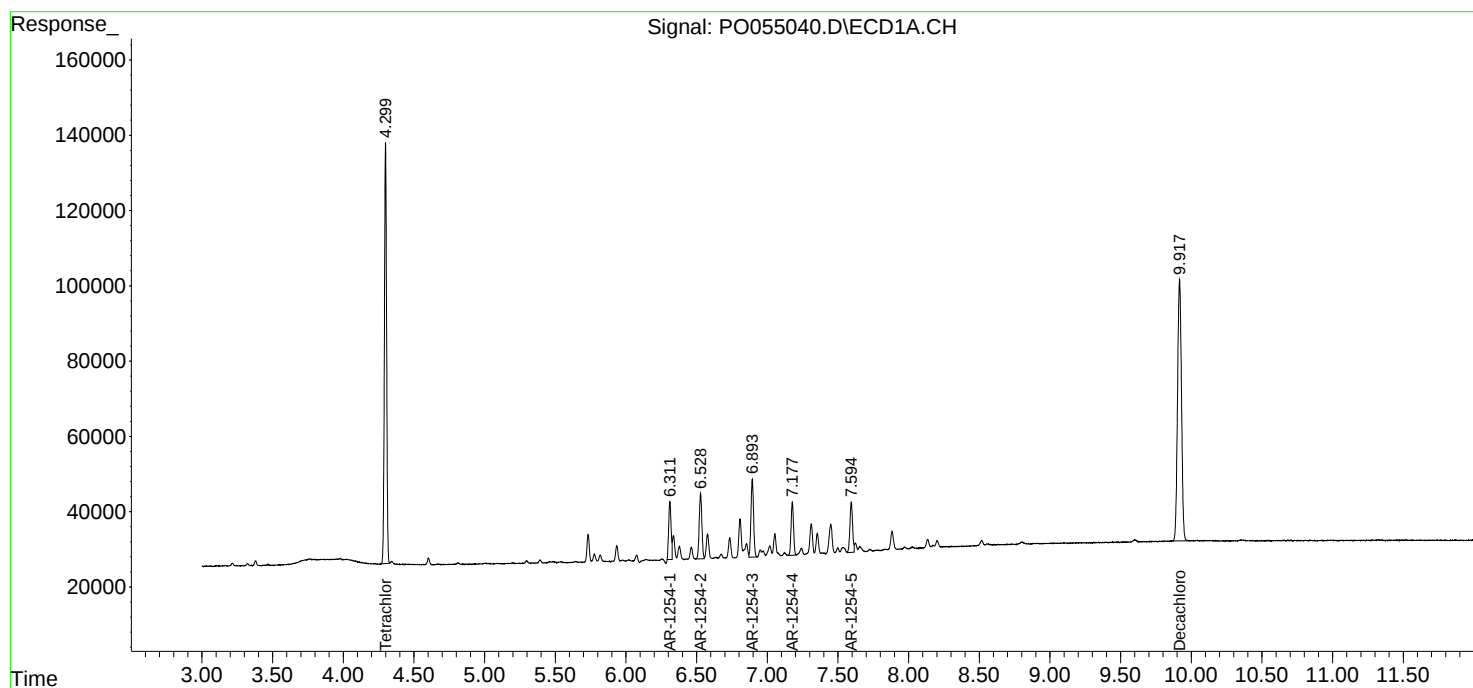

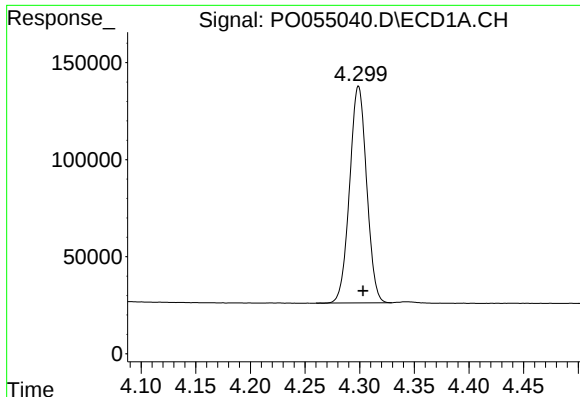


#1 Tetrachloro-m-xylene

R.T.: 4.299 min
Delta R.T.: -0.004 min
Response: 1210106
Conc: 34.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:03:05 PM

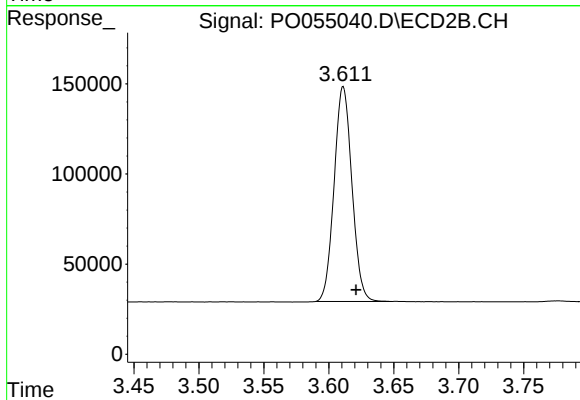


#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: -0.010 min
Response: 1136712
Conc: 35.62 ng/ml

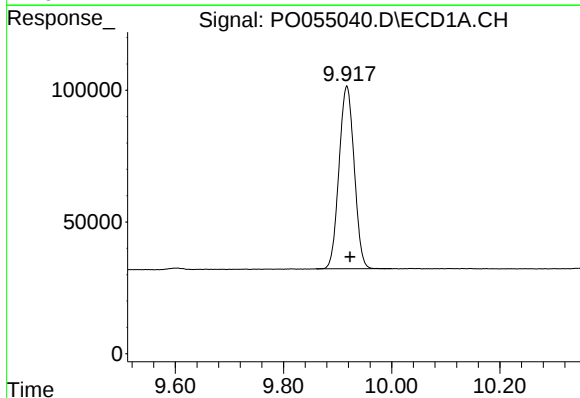


#2 Decachlorobiphenyl

R.T.: 9.917 min
Delta R.T.: -0.006 min
Response: 1346450
Conc: 27.31 ng/ml

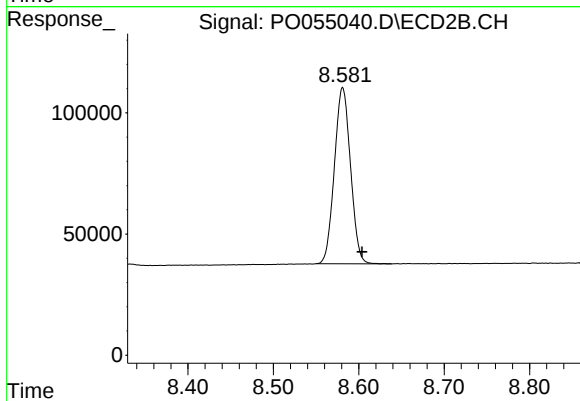

#2 Decachlorobiphenyl

R.T.: 8.581 min
Delta R.T.: -0.023 min
Response: 953600
Conc: 29.94 ng/ml

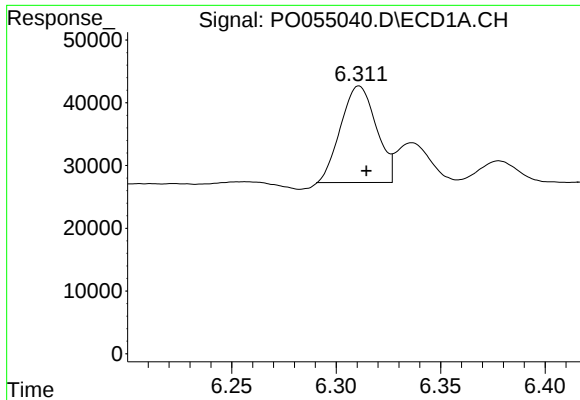


#26 AR-1254-1

R.T.: 6.311 min
Delta R.T.: -0.004 min
Response: 186131
Conc: 102.65 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:03:05 PM

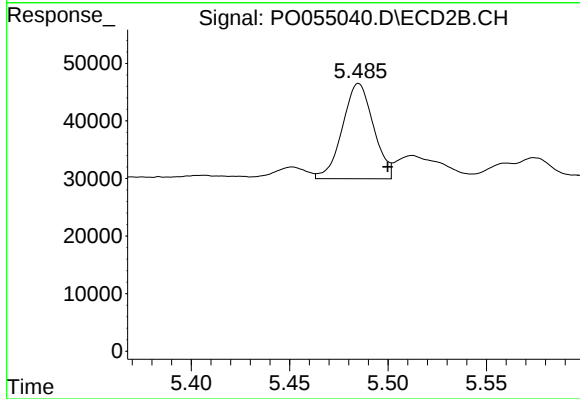


#26 AR-1254-1

R.T.: 5.485 min
Delta R.T.: -0.015 min
Response: 180800
Conc: 82.73 ng/ml m

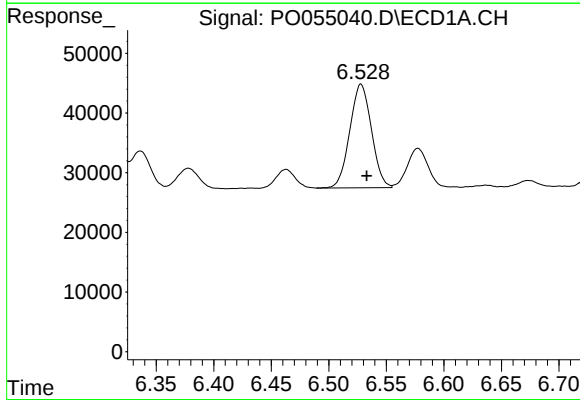


#27 AR-1254-2

R.T.: 6.528 min
Delta R.T.: -0.005 min
Response: 228732
Conc: 80.12 ng/ml

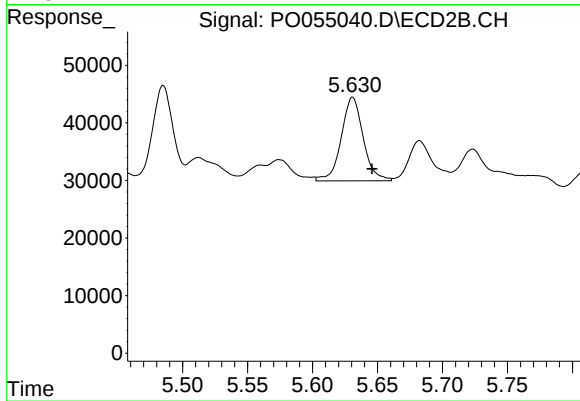

#27 AR-1254-2

R.T.: 5.630 min
Delta R.T.: -0.015 min
Response: 171250
Conc: 88.32 ng/ml m

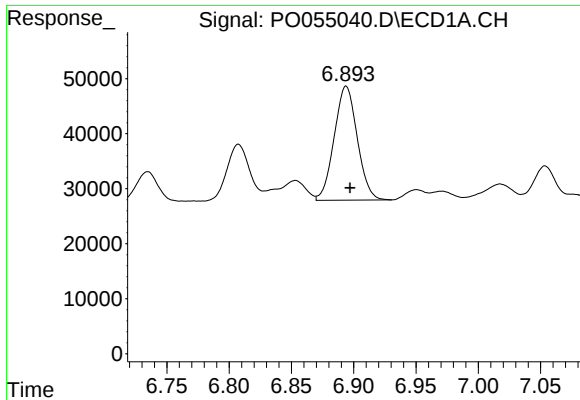


#28 AR-1254-3

R.T.: 6.894 min
Delta R.T.: -0.003 min
Response: 267363
Conc: 85.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:03:05 PM

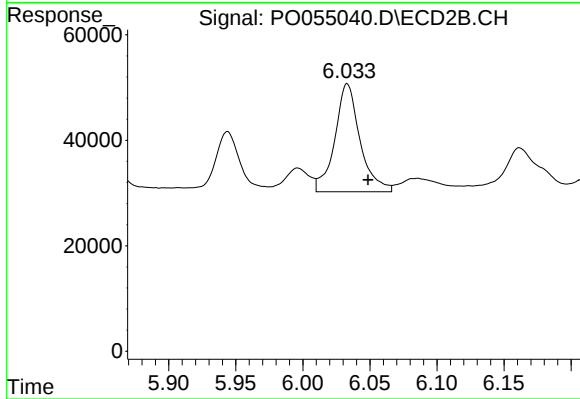


#28 AR-1254-3

R.T.: 6.033 min
Delta R.T.: -0.016 min
Response: 268415
Conc: 83.73 ng/ml m

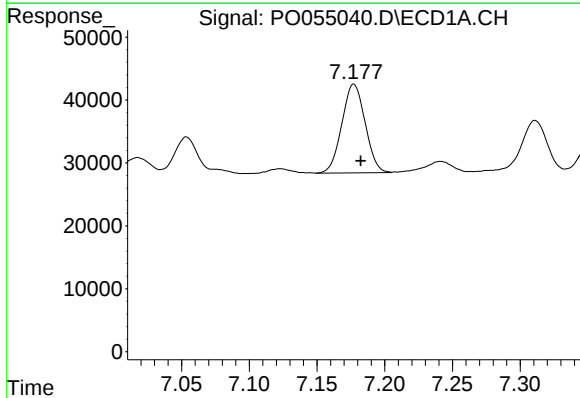


#29 AR-1254-4

R.T.: 7.177 min
Delta R.T.: -0.005 min
Response: 169329
Conc: 69.22 ng/ml

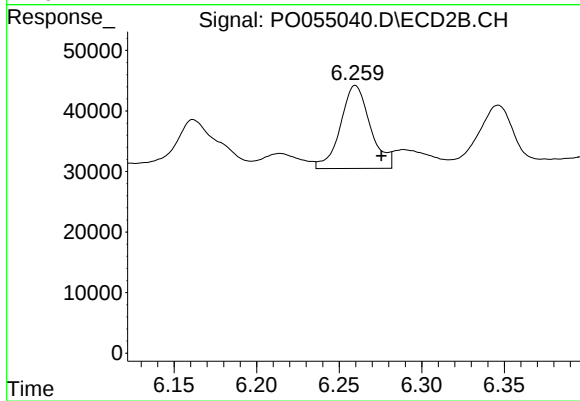

#29 AR-1254-4

R.T.: 6.259 min
Delta R.T.: -0.016 min
Response: 174355
Conc: 89.05 ng/ml m

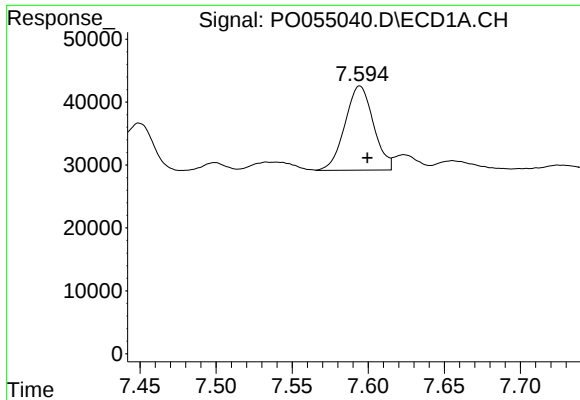


#30 AR-1254-5

R.T.: 7.595 min
Delta R.T.: -0.005 min
Response: 174416
Conc: 65.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Manual Integrations
APPROVED

mohammad
4/10/2019 4:03:05 PM

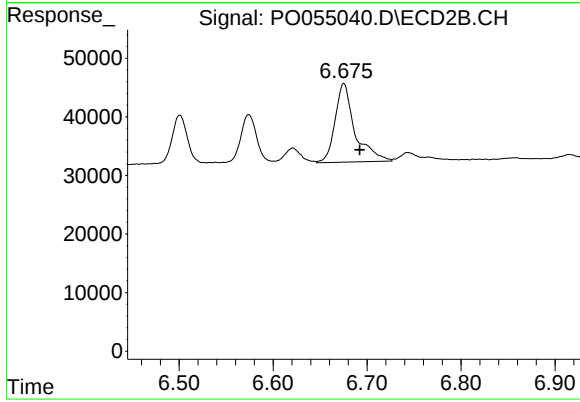

#30 AR-1254-5

R.T.: 6.675 min
Delta R.T.: -0.017 min
Response: 197627
Conc: 68.75 ng/ml