

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040819\
 Data File : P0055042.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Apr 2019 15:14
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1262 LOD 25PPB
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Manual Integrations
 APPROVED

mohammad
 4/10/2019 4:03:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 06:56:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.299	3.611	1576976	1475145	45.439	46.225
2) SA Decachlor...	9.917	8.581	1657941	1178025	33.631	36.989
Target Compounds						
36) L8 AR-1262-1	7.668	6.712	191594	170214	57.500	57.216
37) L8 AR-1262-2	8.202	7.211	291112	258142	49.138	52.670
38) L8 AR-1262-3	8.499	7.534	197618	1291030	47.702	628.711m#
39) L8 AR-1262-4	8.586	7.554	76054	1581800	23.605	436.705m#
40) L8 AR-1262-5	9.211	8.048	102015	89311	46.662	55.339

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040819\
Data File : PO055042.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Apr 2019 15:14
Operator : SM/SJ
Sample : K1560-07
Misc : AR1262 LOD 25PPB
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:03:28 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 06:56:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

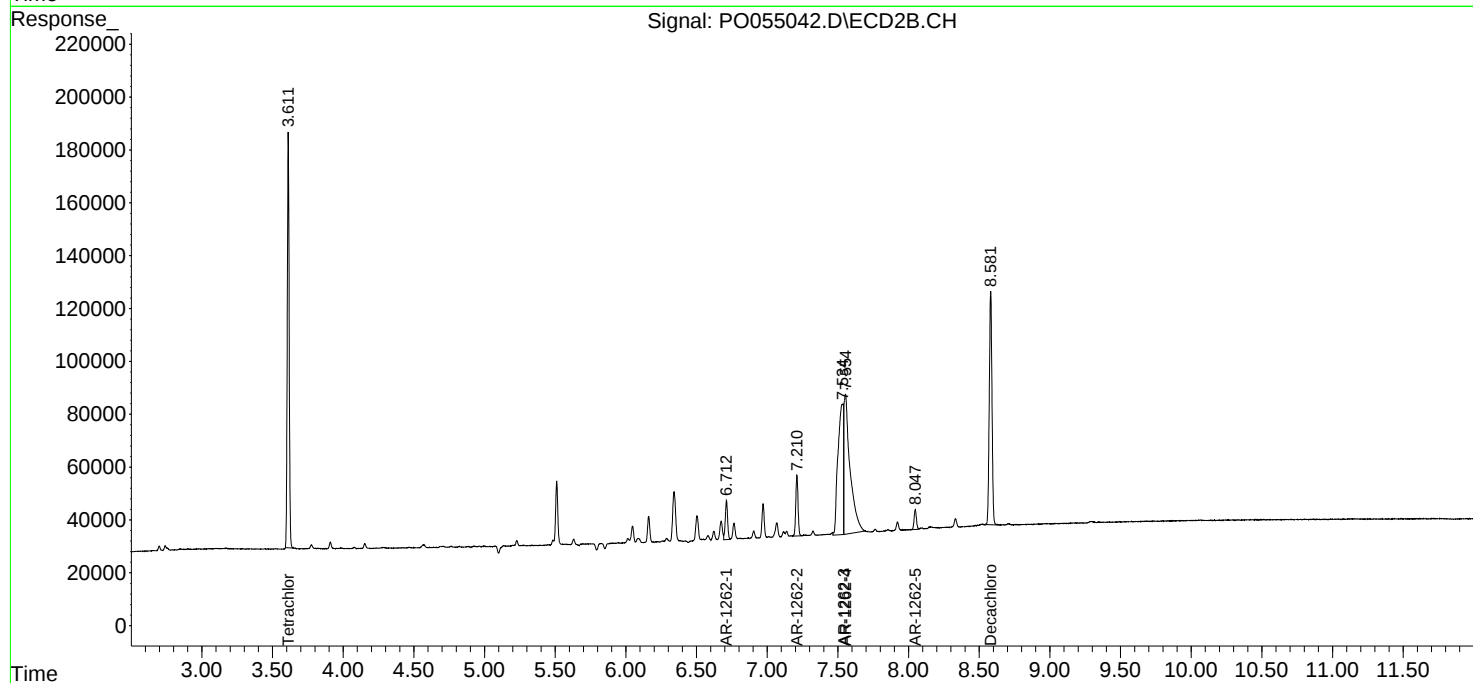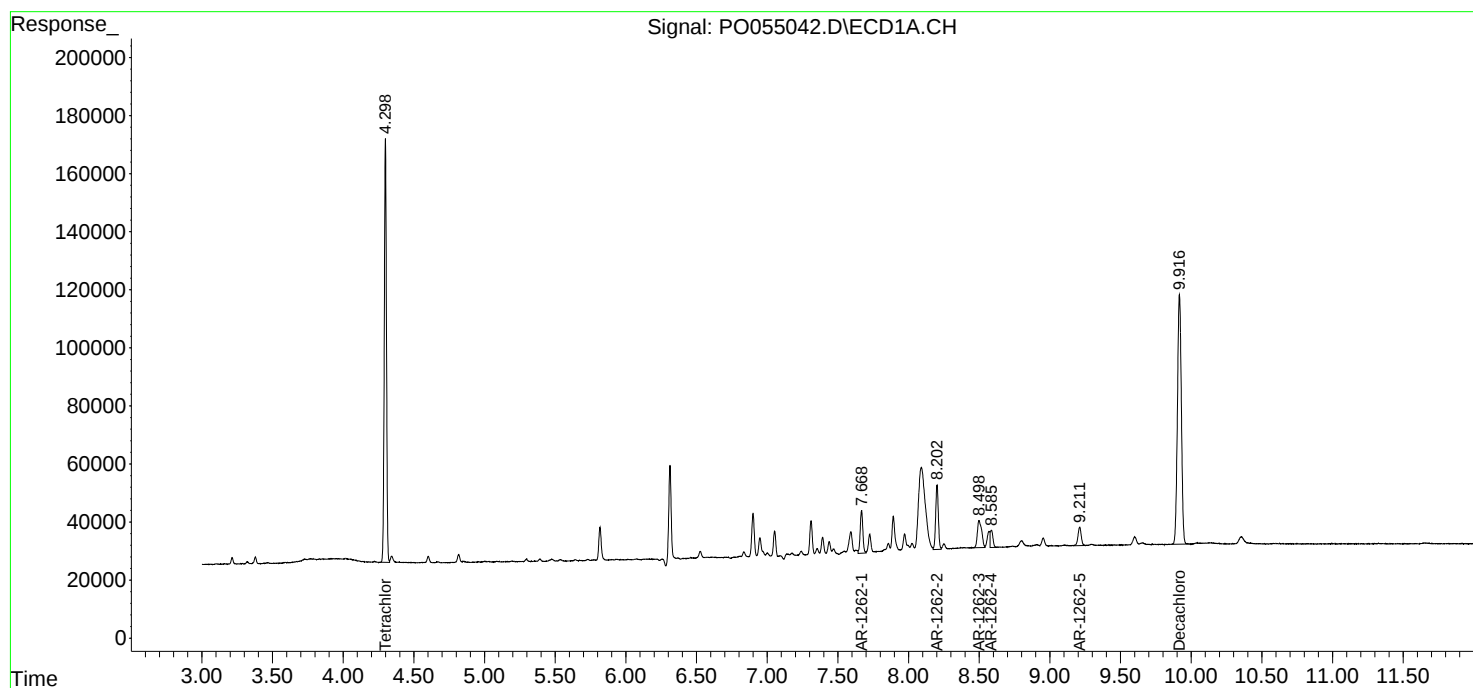

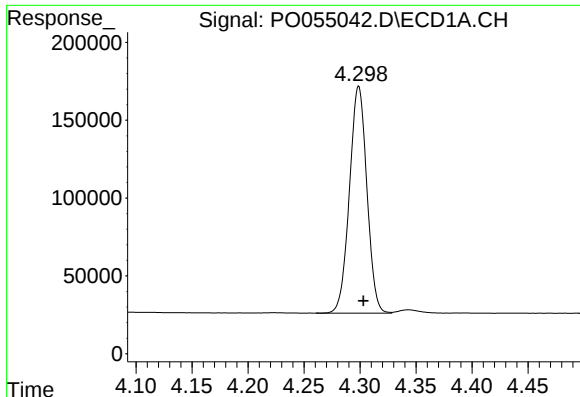


#1 Tetrachloro-m-xylene

R.T.: 4.299 min
Delta R.T.: -0.004 min
Response: 1576976
Conc: 45.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:03:28 PM

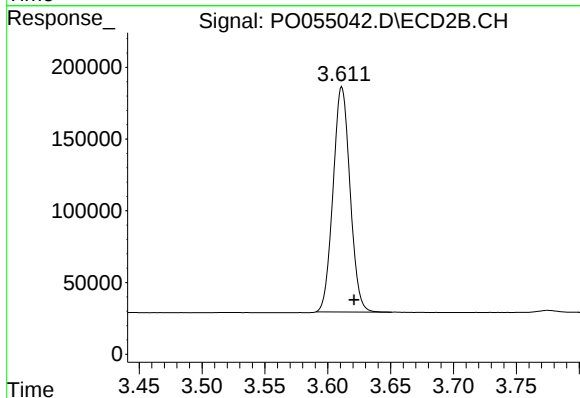


#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: -0.010 min
Response: 1475145
Conc: 46.22 ng/ml

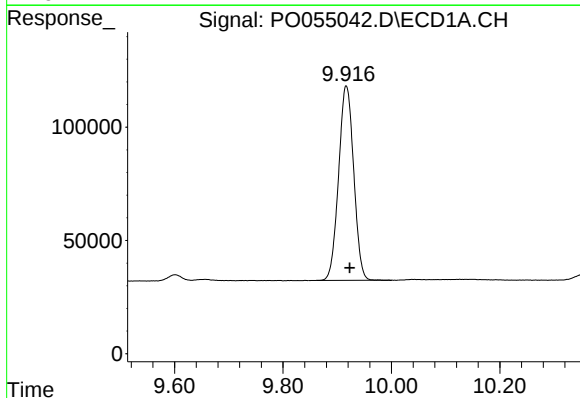


#2 Decachlorobiphenyl

R.T.: 9.917 min
Delta R.T.: -0.006 min
Response: 1657941
Conc: 33.63 ng/ml

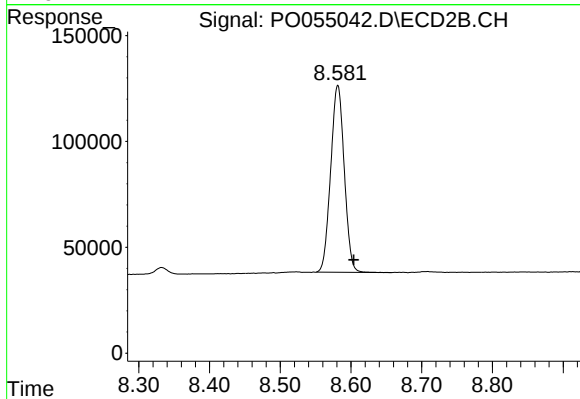

#2 Decachlorobiphenyl

R.T.: 8.581 min
Delta R.T.: -0.023 min
Response: 1178025
Conc: 36.99 ng/ml

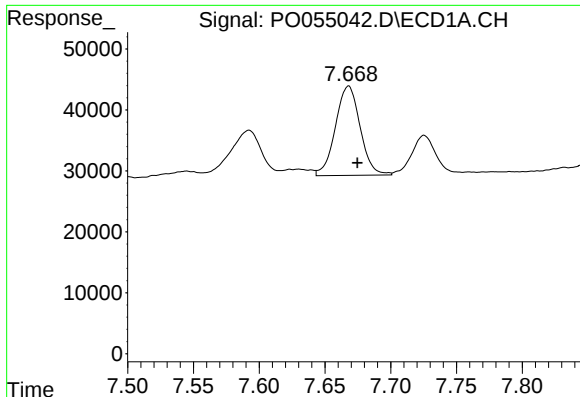


#36 AR-1262-1

R.T.: 7.668 min
Delta R.T.: -0.007 min
Response: 191594
Conc: 57.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:03:28 PM

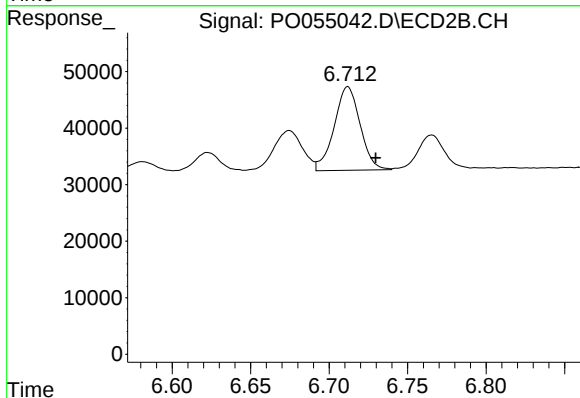


#36 AR-1262-1

R.T.: 6.712 min
Delta R.T.: -0.018 min
Response: 170214
Conc: 57.22 ng/ml

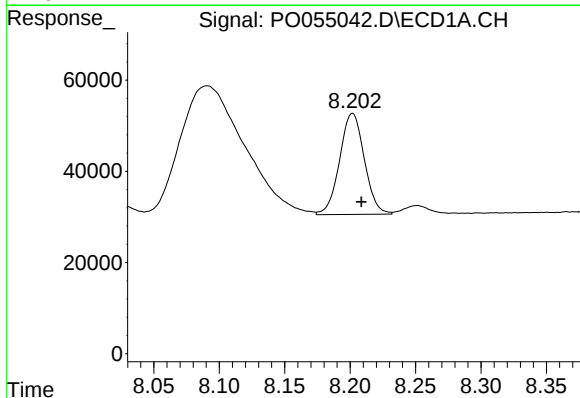


#37 AR-1262-2

R.T.: 8.202 min
Delta R.T.: -0.007 min
Response: 291112
Conc: 49.14 ng/ml

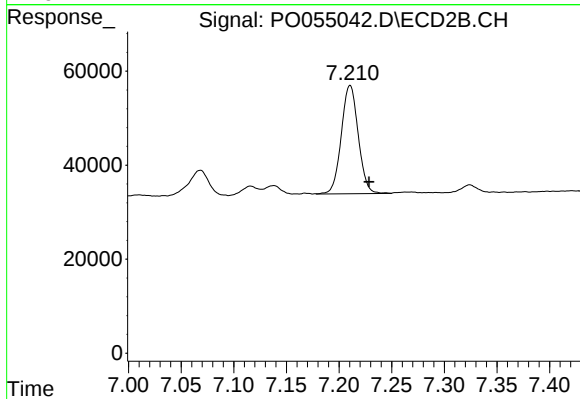

#37 AR-1262-2

R.T.: 7.211 min
Delta R.T.: -0.018 min
Response: 258142
Conc: 52.67 ng/ml

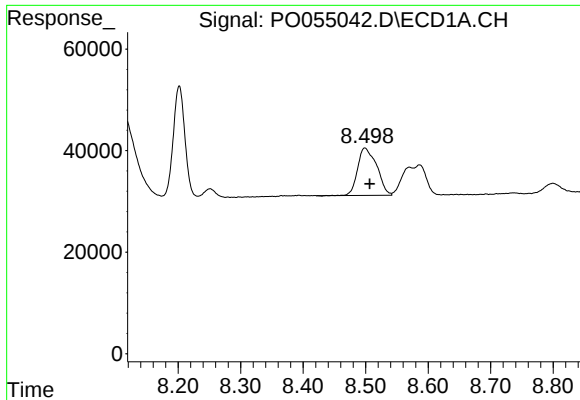


#38 AR-1262-3

R.T.: 8.499 min
Delta R.T.: -0.008 min
Response: 197618
Conc: 47.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:03:28 PM

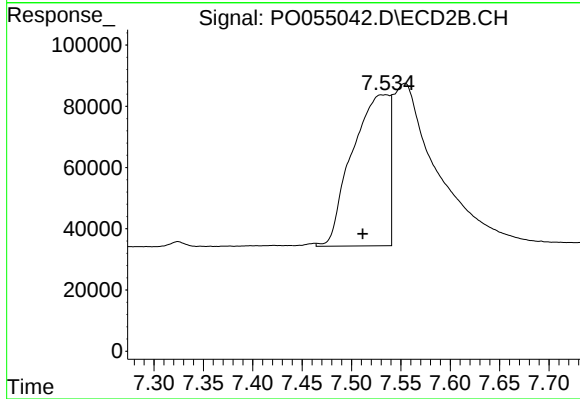


#38 AR-1262-3

R.T.: 7.534 min
Delta R.T.: 0.023 min
Response: 1291030
Conc: 628.71 ng/ml m

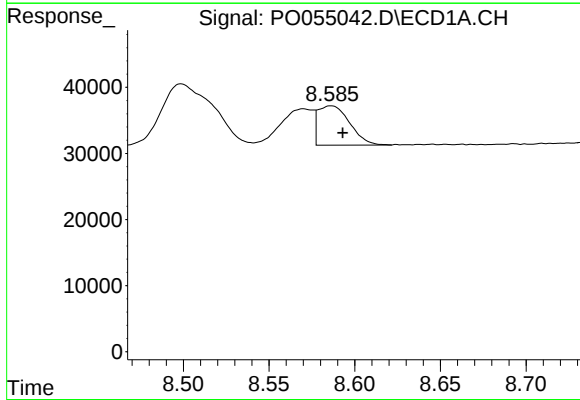


#39 AR-1262-4

R.T.: 8.586 min
Delta R.T.: -0.007 min
Response: 76054
Conc: 23.60 ng/ml

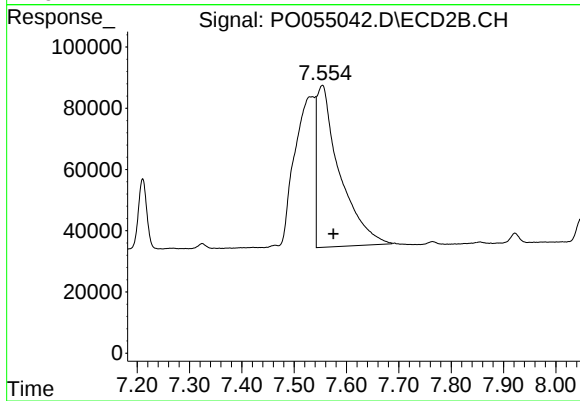

#39 AR-1262-4

R.T.: 7.554 min
Delta R.T.: -0.021 min
Response: 1581800
Conc: 436.70 ng/ml m

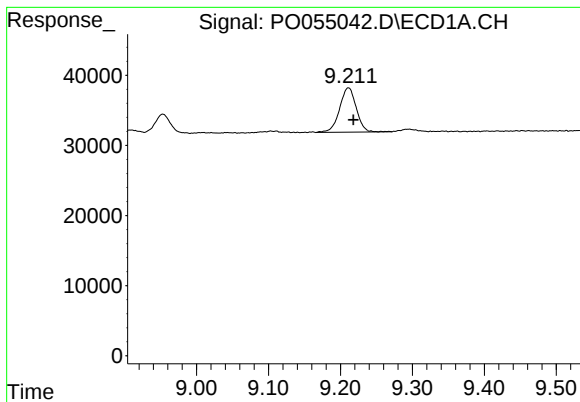


#40 AR-1262-5

R.T.: 9.211 min
Delta R.T.: -0.007 min
Response: 102015
Conc: 46.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Manual Integrations
APPROVED

mohammad
4/10/2019 4:03:28 PM

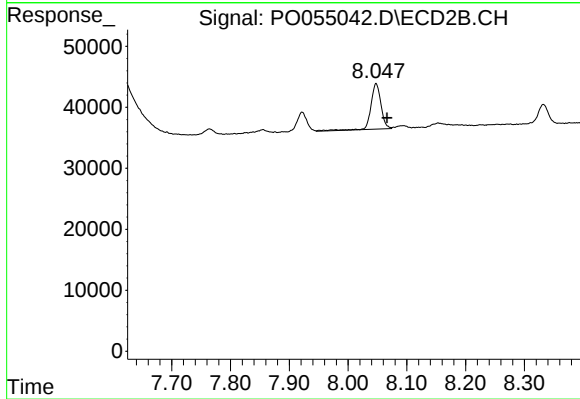

#40 AR-1262-5

R.T.: 8.048 min
Delta R.T.: -0.019 min
Response: 89311
Conc: 55.34 ng/ml