

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040819\
 Data File : P0055045.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Apr 2019 16:05
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1268 LOD 25PPB
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Manual Integrations
 APPROVED

mohammad
 4/10/2019 4:03:14 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 06:57:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.299	3.611	1315402	1234047	37.902	38.670
2) SA Decachlor...	9.918	8.582	1616041	1148475	32.781	36.061
Target Compounds						
41) L9 AR-1268-1	8.499	7.493	306469	256265	43.059	45.323
42) L9 AR-1268-2	8.589	7.558	275146	242928	41.994	46.974
43) L9 AR-1268-3	8.805	7.764	231703	198423	42.534	46.108
44) L9 AR-1268-4	9.212	8.048	99270	84529	41.609	45.596
45) L9 AR-1268-5	9.602	8.332	694398	538771	42.148	47.333m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040819\
Data File : PO055045.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Apr 2019 16:05
Operator : SM/SJ
Sample : K1560-07
Misc : AR1268 LOD 25PPB
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:03:14 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 06:57:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

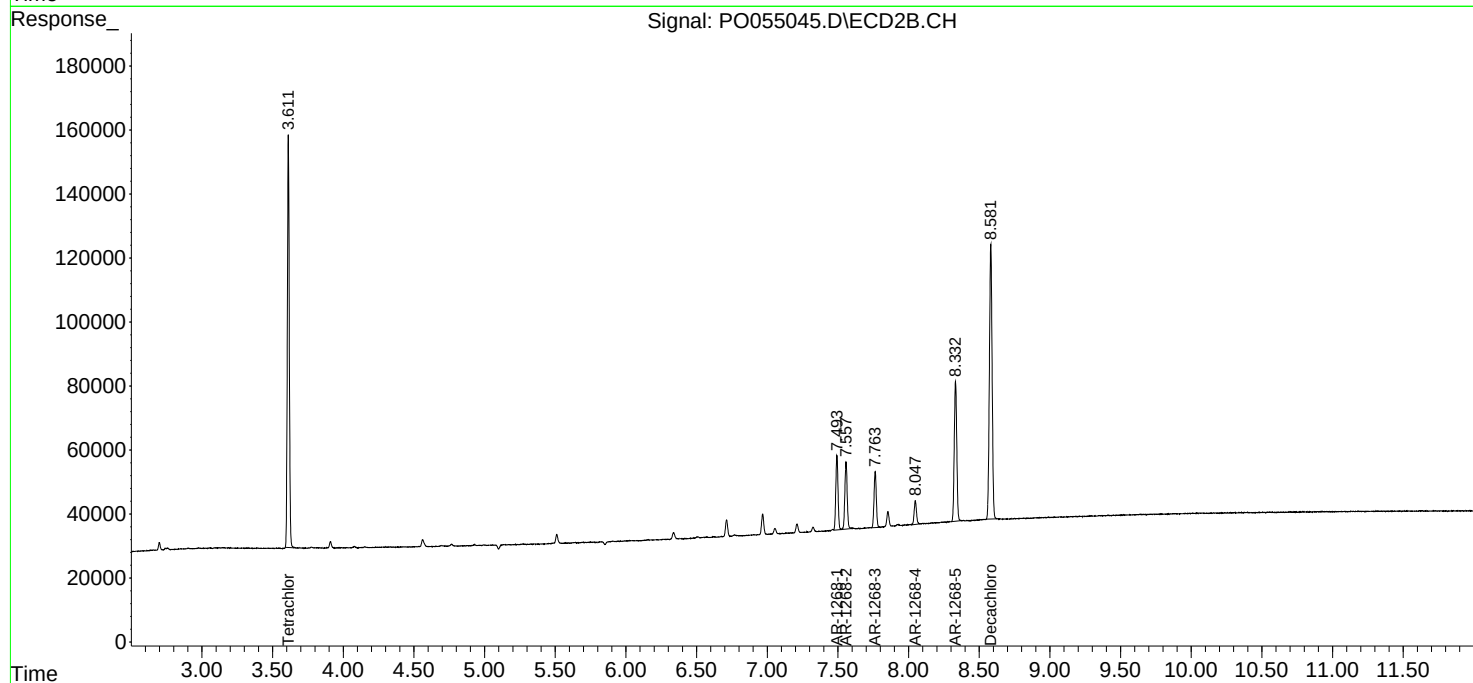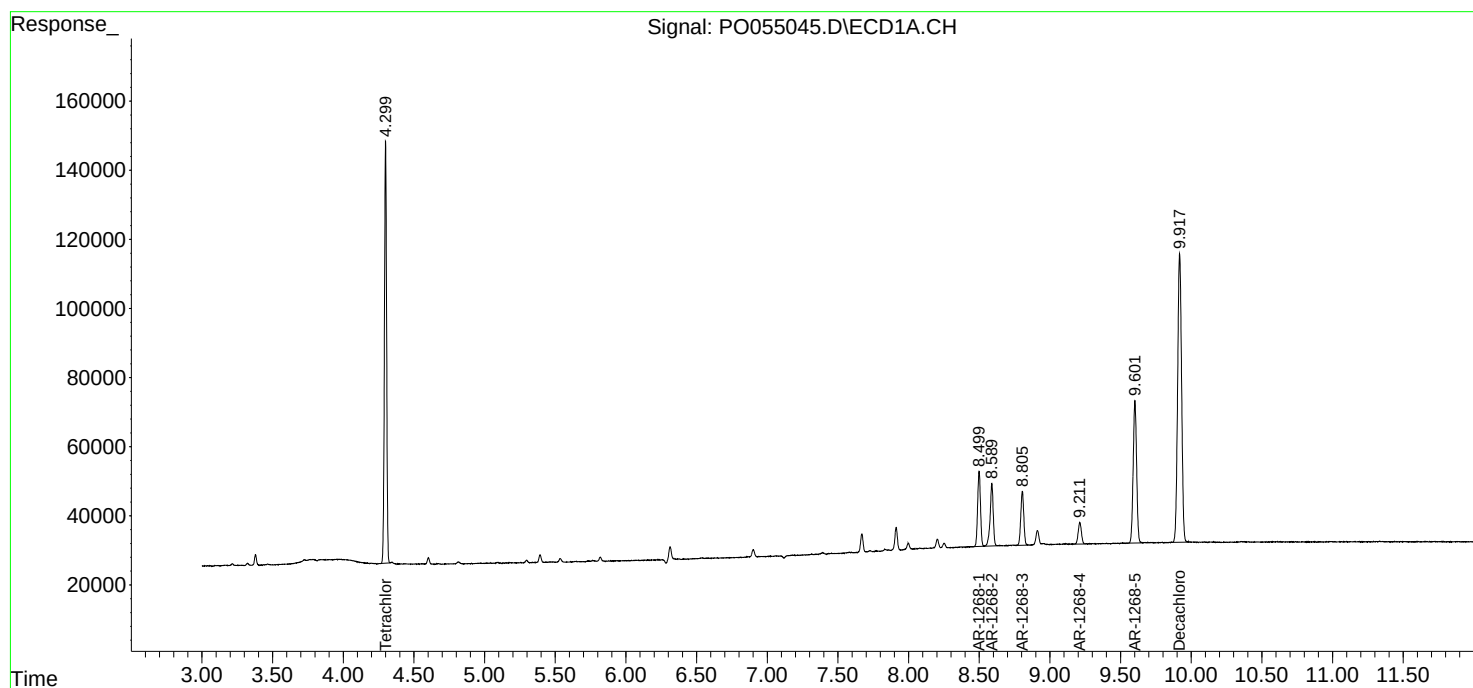

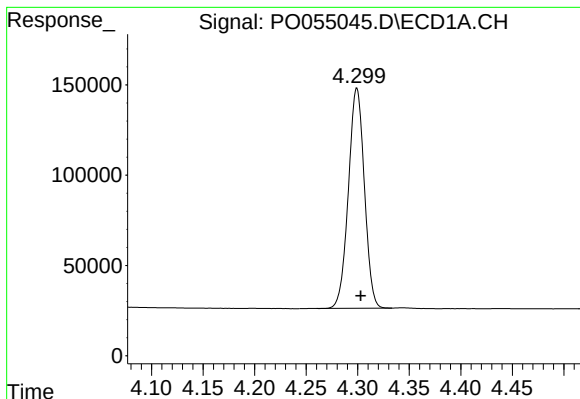


#1 Tetrachloro-m-xylene

R.T.: 4.299 min
Delta R.T.: -0.004 min
Response: 1315402
Conc: 37.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:03:14 PM

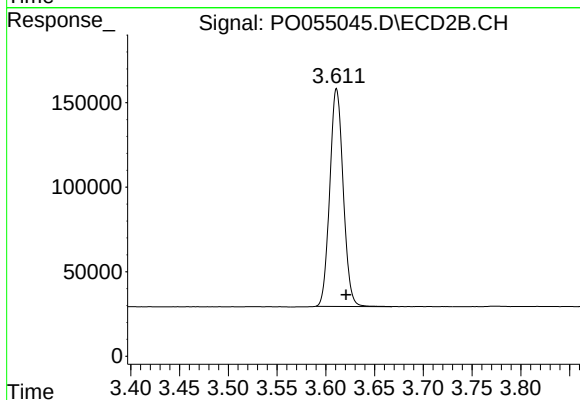


#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: -0.010 min
Response: 1234047
Conc: 38.67 ng/ml

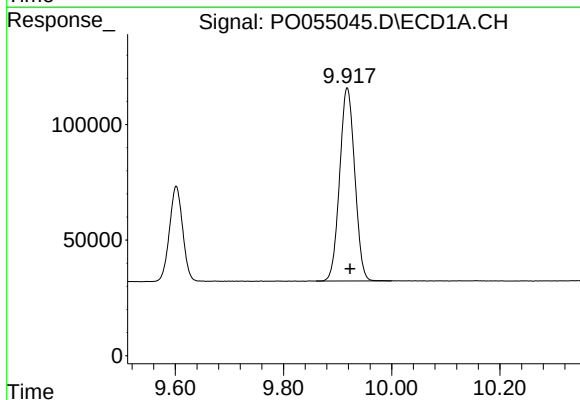


#2 Decachlorobiphenyl

R.T.: 9.918 min
Delta R.T.: -0.005 min
Response: 1616041
Conc: 32.78 ng/ml

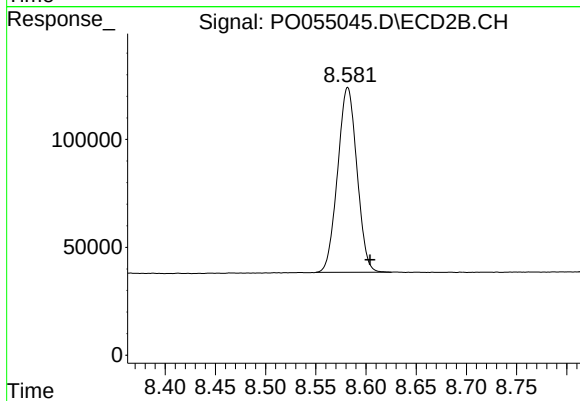

#2 Decachlorobiphenyl

R.T.: 8.582 min
Delta R.T.: -0.022 min
Response: 1148475
Conc: 36.06 ng/ml

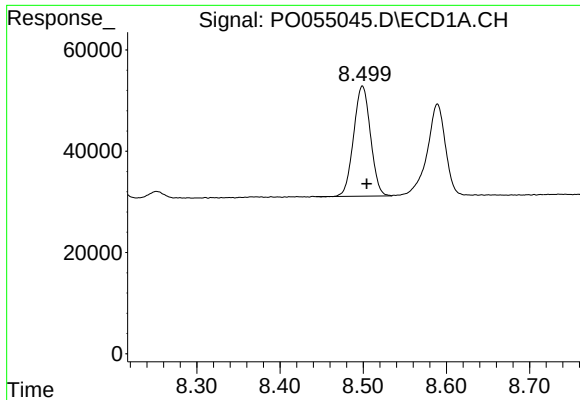


#41 AR-1268-1

R.T.: 8.499 min
Delta R.T.: -0.005 min
Response: 306469
Conc: 43.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:03:14 PM

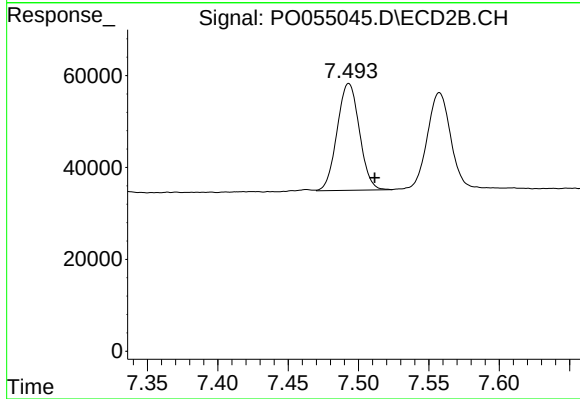


#41 AR-1268-1

R.T.: 7.493 min
Delta R.T.: -0.018 min
Response: 256265
Conc: 45.32 ng/ml

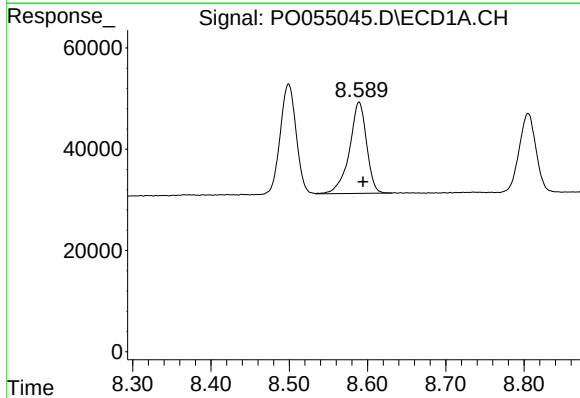


#42 AR-1268-2

R.T.: 8.589 min
Delta R.T.: -0.005 min
Response: 275146
Conc: 41.99 ng/ml

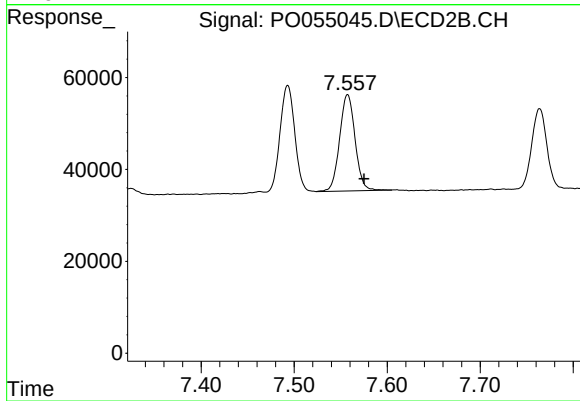

#42 AR-1268-2

R.T.: 7.558 min
Delta R.T.: -0.018 min
Response: 242928
Conc: 46.97 ng/ml

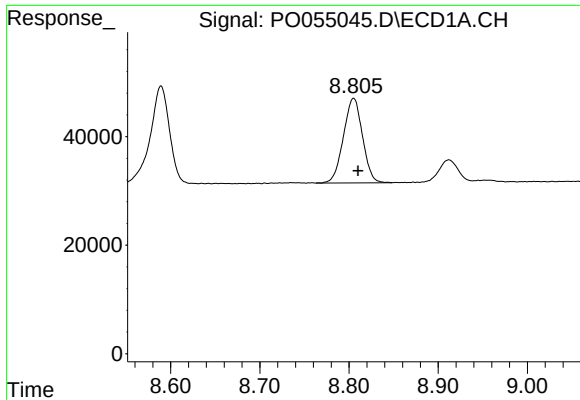


#43 AR-1268-3

R.T.: 8.805 min
Delta R.T.: -0.005 min
Response: 231703
Conc: 42.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:03:14 PM

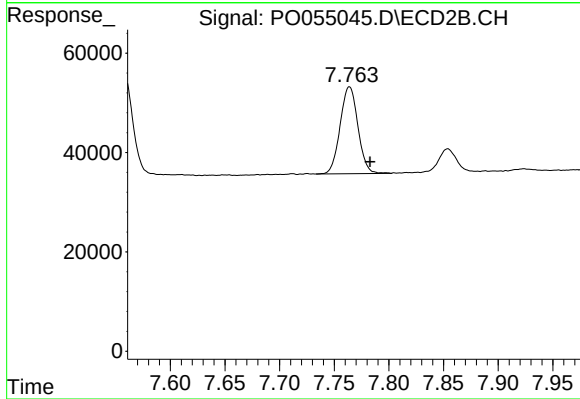


#43 AR-1268-3

R.T.: 7.764 min
Delta R.T.: -0.019 min
Response: 198423
Conc: 46.11 ng/ml

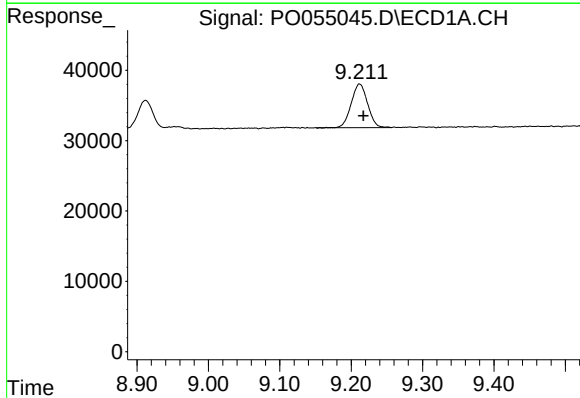


#44 AR-1268-4

R.T.: 9.212 min
Delta R.T.: -0.005 min
Response: 99270
Conc: 41.61 ng/ml

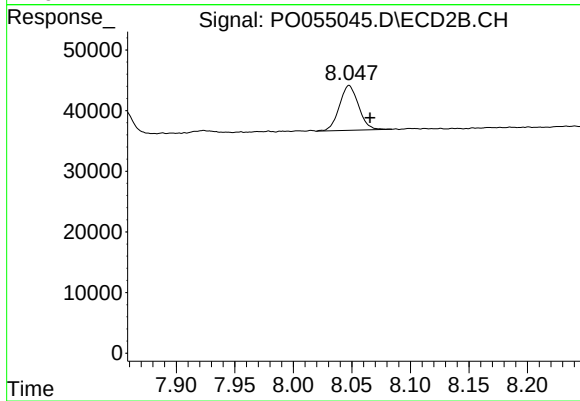

#44 AR-1268-4

R.T.: 8.048 min
Delta R.T.: -0.018 min
Response: 84529
Conc: 45.60 ng/ml

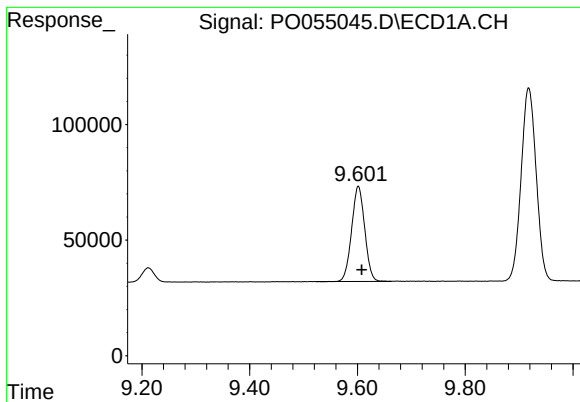


#45 AR-1268-5

R.T.: 9.602 min
Delta R.T.: -0.006 min
Response: 694398
Conc: 42.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Manual Integrations
APPROVED

mohammad
4/10/2019 4:03:14 PM

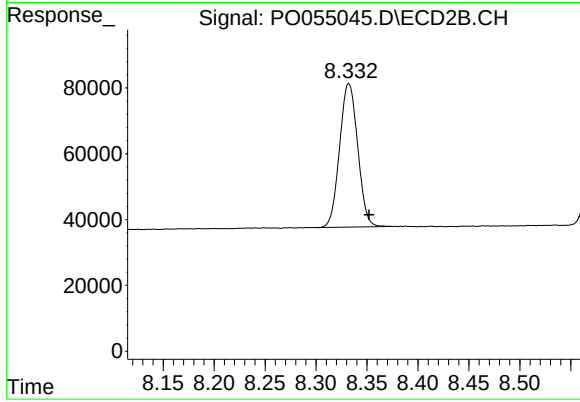

#45 AR-1268-5

R.T.: 8.332 min
Delta R.T.: -0.020 min
Response: 538771
Conc: 47.33 ng/ml m