

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040820\
 Data File : P0067747.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Apr 2020 15:23
 Operator : DD\AJ
 Sample : PB128087BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB128087BL

Manual Integrations
 APPROVED

Sohil
 4/10/2020 12:25:18 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 14:44:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.933	3.943	605024	889978	25.406	26.553
2) SA Decachlor...	10.914	9.229	1029415	918713	30.238	22.220m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040820\
Data File : P0067747.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Apr 2020 15:23
Operator : DD\AJ
Sample : PB128087BL
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB128087BL


Manual Integrations
APPROVED

Sohil
4/10/2020 12:25:18 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 14:44:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

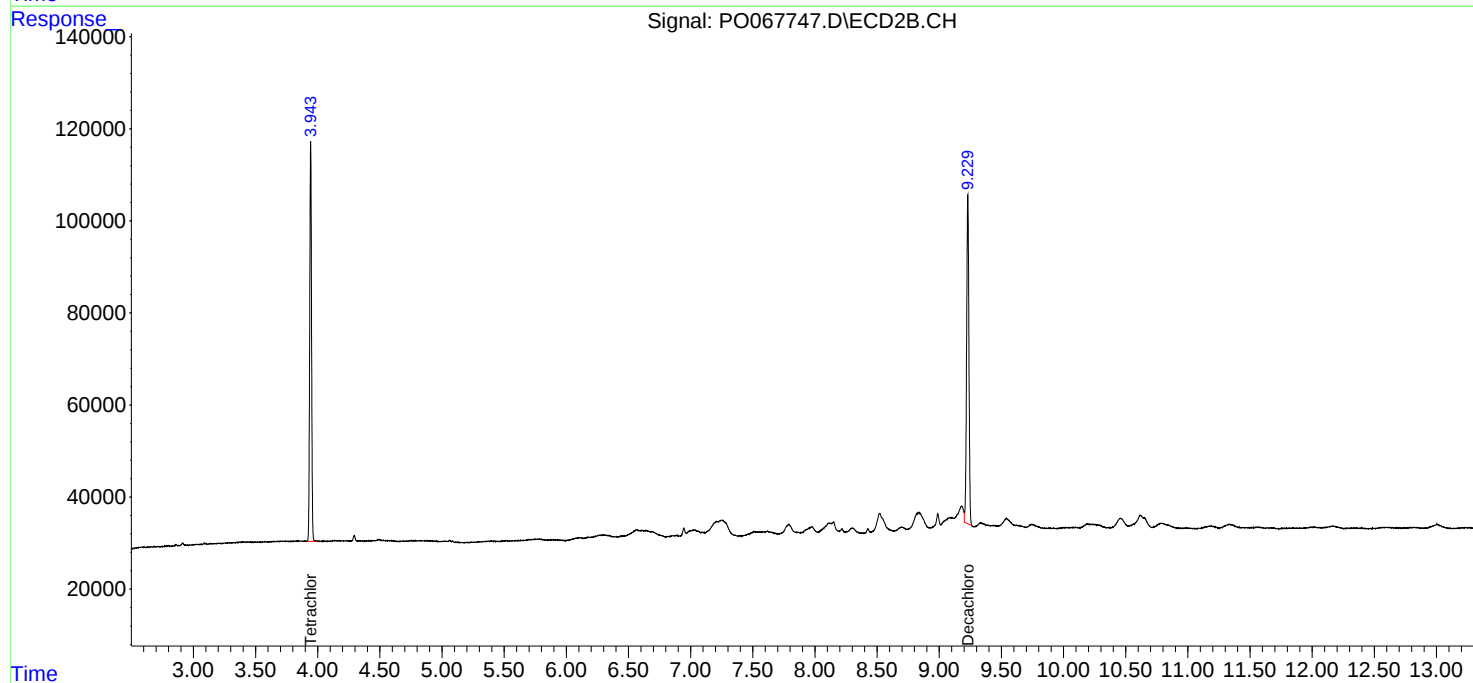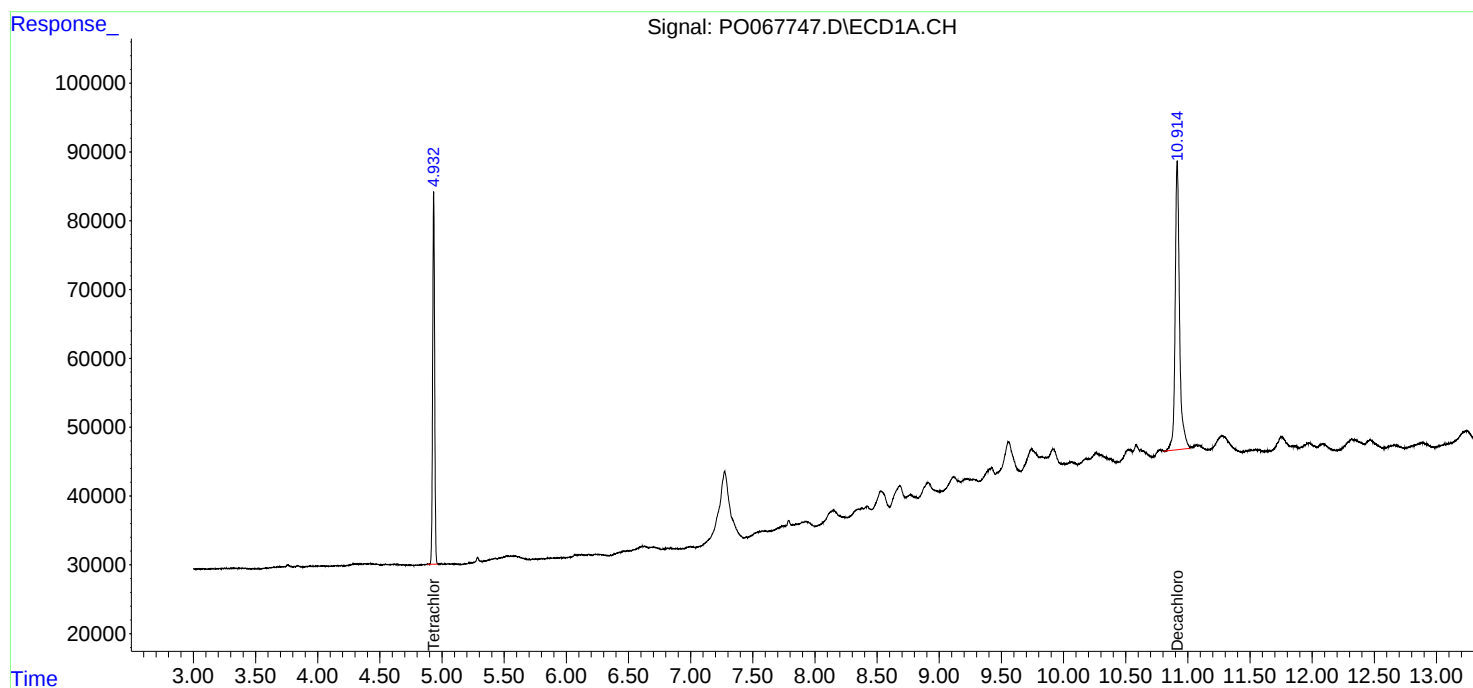

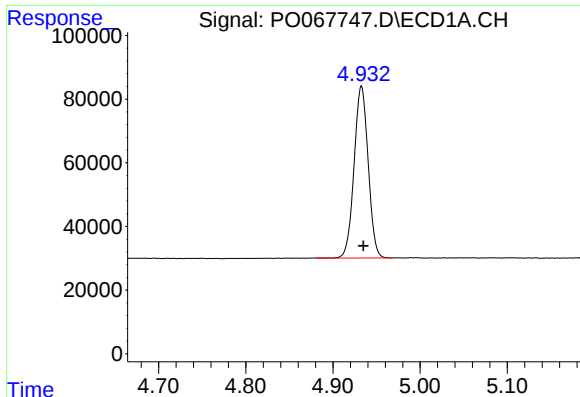


#1 Tetrachloro-m-xylene

R.T.: 4.933 min
Delta R.T.: -0.002 min
Response: 605024
Conc: 25.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB128087BL


Manual Integrations
APPROVED

Sohil
4/10/2020 12:25:18 PM

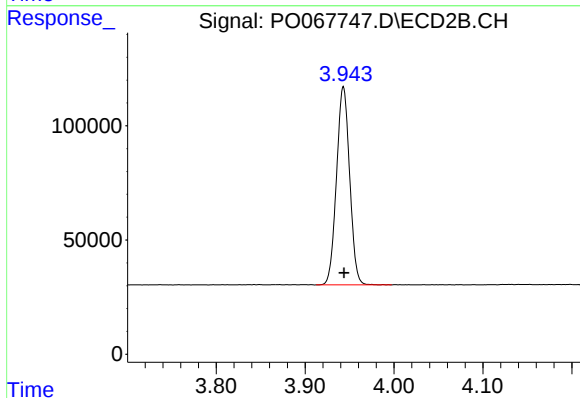


#1 Tetrachloro-m-xylene

R.T.: 3.943 min
Delta R.T.: 0.000 min
Response: 889978
Conc: 26.55 ng/ml

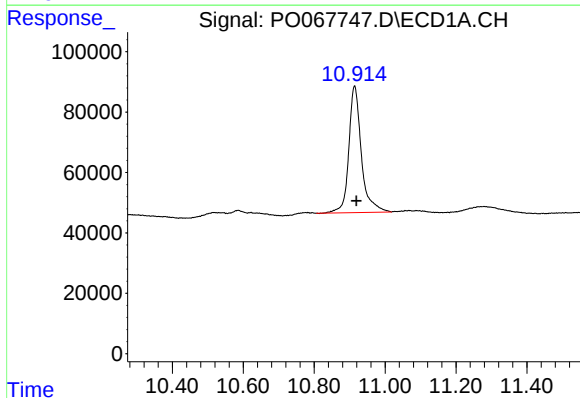

#2 Decachlorobiphenyl

R.T.: 10.914 min
Delta R.T.: -0.005 min
Response: 1029415
Conc: 30.24 ng/ml

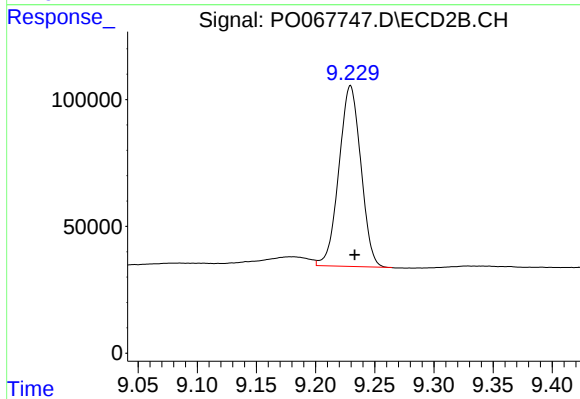

#2 Decachlorobiphenyl

R.T.: 9.229 min
Delta R.T.: -0.004 min
Response: 918713
Conc: 22.22 ng/ml m