

Data Path : \\74.0.250.170\pestpcbsrv\HPCHEM1\ECD_0\Data\P0040918\
 Data File : P0043692.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Apr 2018 13:28
 Operator : SM/UA
 Sample : J2203-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-01-D02-D02A-E02-E02A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 01:06:16 2018
 Quant Method : P:\HPCHEM1\ECD_0\methods\P0040418.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 04 15:17:57 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.063	3.323	4112739	5285335	23.134	19.671
2) SA Decachlor...	9.396	8.080	3007033	4893160	16.686	20.871 #
Target Compounds						
33) L7 AR-1260-3	0.000	6.262	0	131837	N.D.	5.987 #
34) L7 AR-1260-4	0.000	6.790	0	275713	N.D.	7.464 #
35) L7 AR-1260-5	0.000	7.123	0	247989	N.D.	9.643 #
38) L8 AR-1262-3	0.000	6.262	0	131837	N.D.	3.785 #
40) L8 AR-1262-5	0.000	6.790	0	275713	N.D.	4.728 #
41) L9 AR-1268-1	0.000	7.123	0	247989	N.D.	4.258 #
42) L9 AR-1268-2	0.000	7.123	0	247989	N.D.	4.752 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\pestpcbsrv\HPCHEM1\ECD_0\Data\P0040918\
Data File : P0043692.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Apr 2018 13:28
Operator : SM/UA
Sample : J2203-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-D02-D02A-E02-E02A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 01:06:16 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0040418.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 04 15:17:57 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

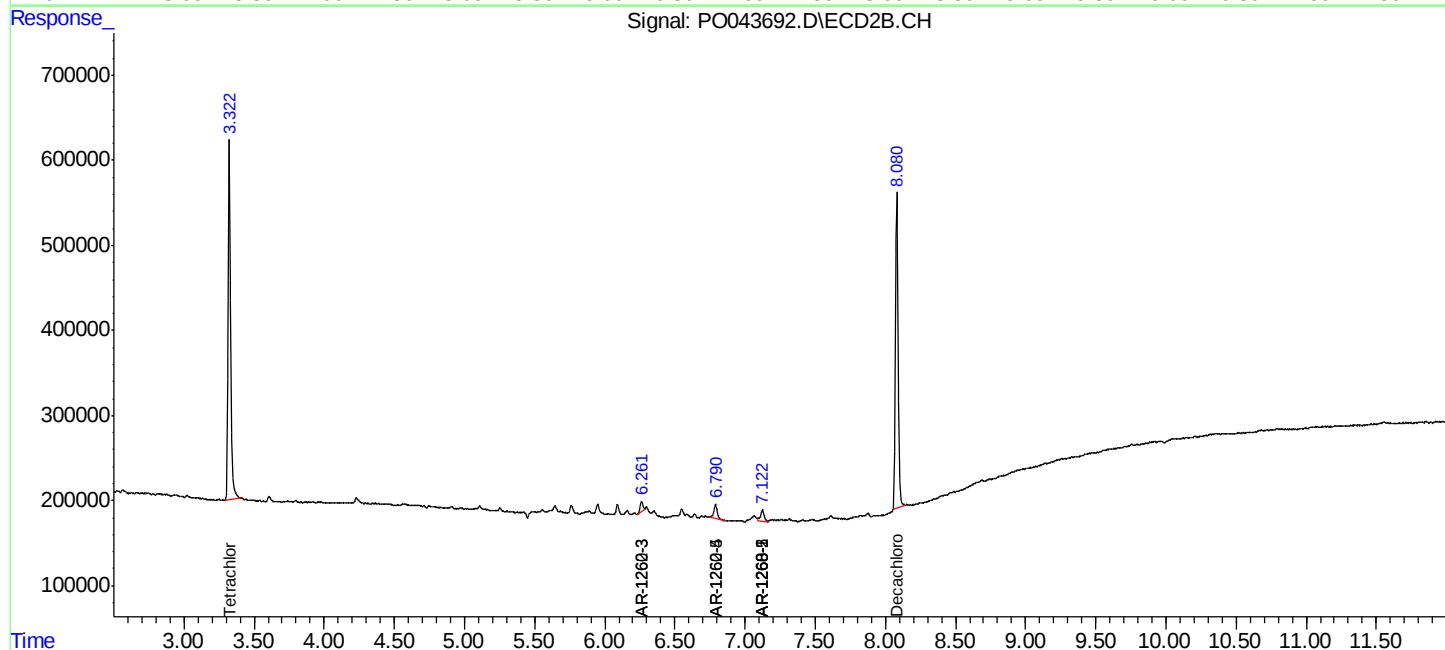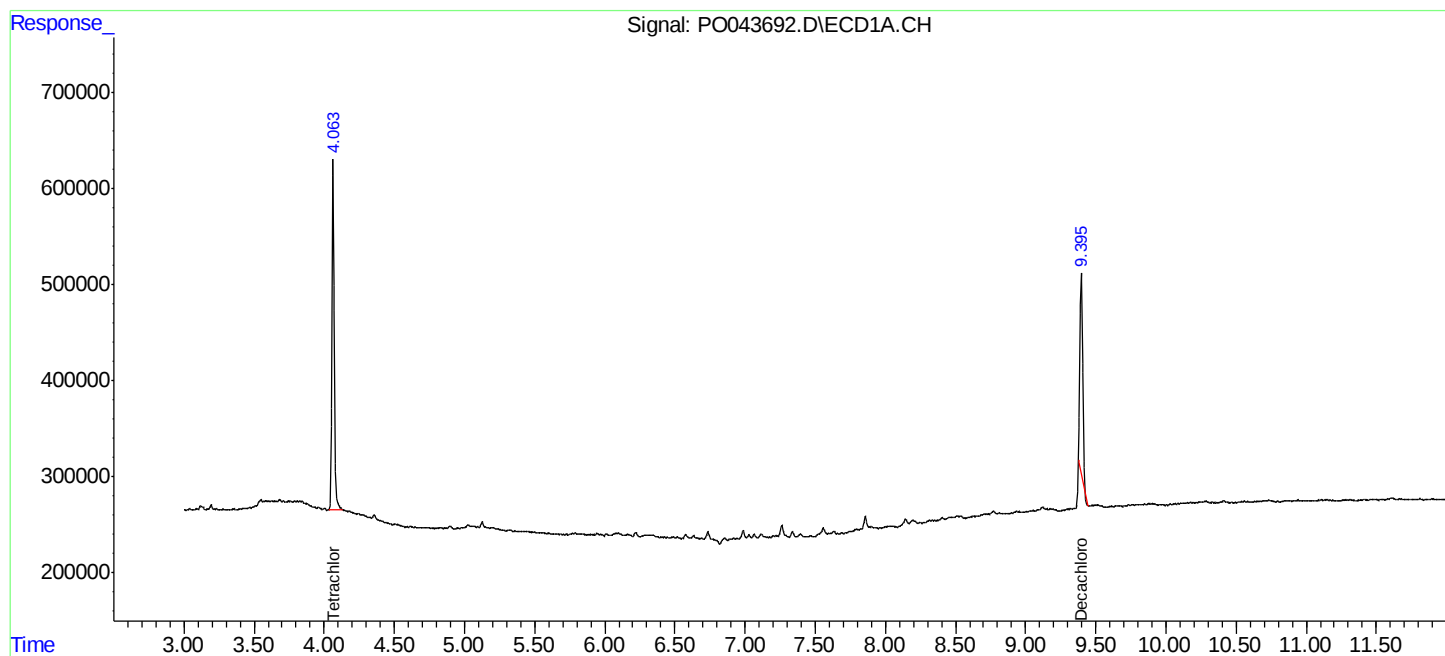


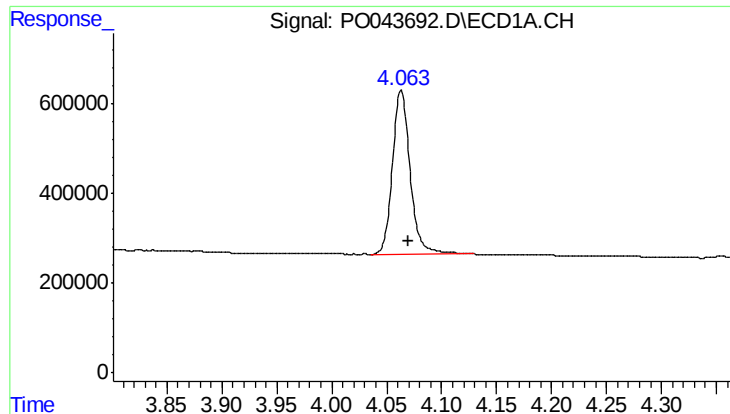

#1 Tetrachloro-m-xylene


R.T.: 4.063 min
Delta R.T.: -0.006 min
Response: 4112739
Conc: 23.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-D02-D02A-E02-E02A

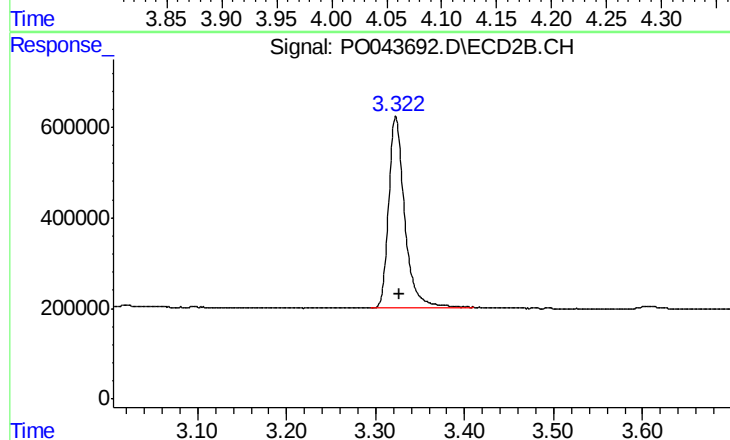


#1 Tetrachloro-m-xylene

R.T.: 3.323 min
Delta R.T.: -0.003 min
Response: 5285335
Conc: 19.67 ng/ml

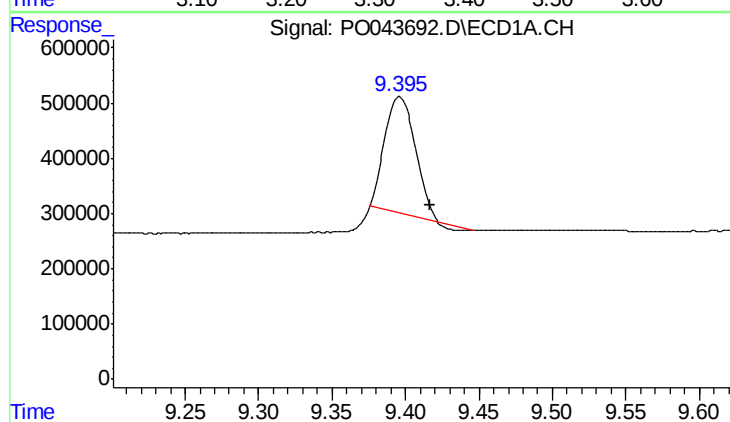


#2 Decachlorobiphenyl

R.T.: 9.396 min
Delta R.T.: -0.021 min
Response: 3007033
Conc: 16.69 ng/ml

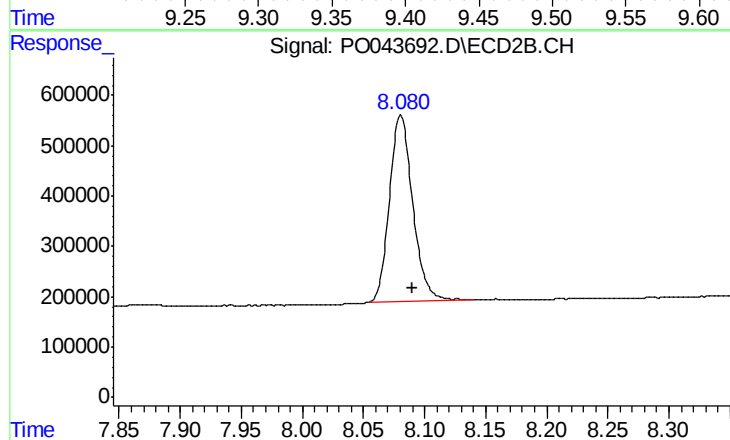

#2 Decachlorobiphenyl


R.T.: 8.080 min
Delta R.T.: -0.010 min
Response: 4893160
Conc: 20.87 ng/ml

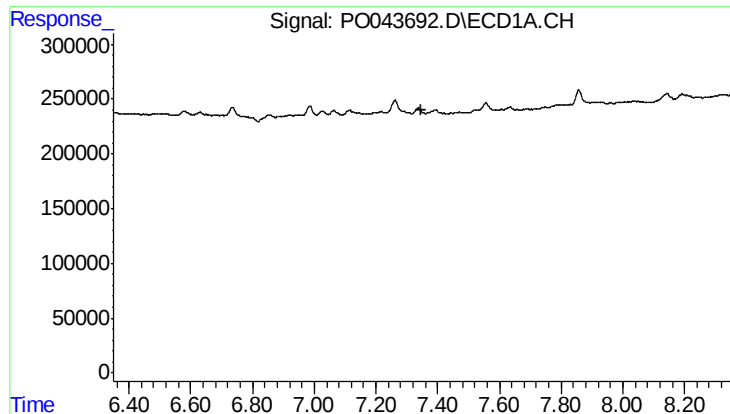

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.349 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-D02-D02A-E02-E02A

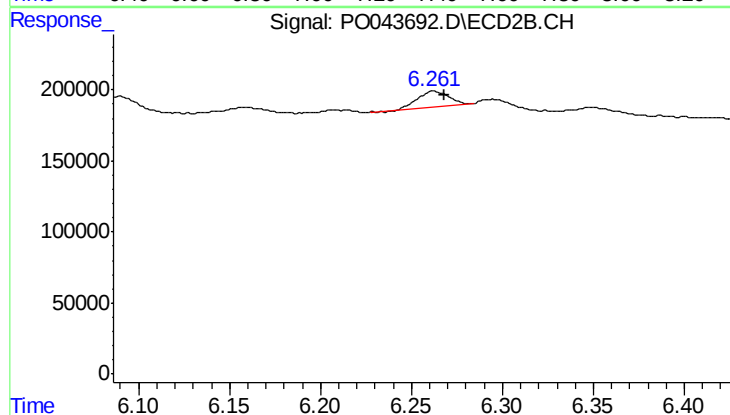


#33 AR-1260-3

R.T.: 6.262 min
Delta R.T.: -0.006 min
Response: 131837
Conc: 5.99 ng/ml

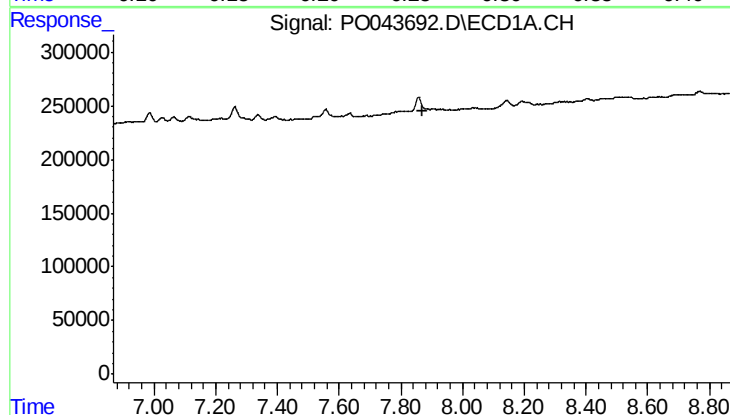


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.869 min
Response: 0
Conc: N.D.

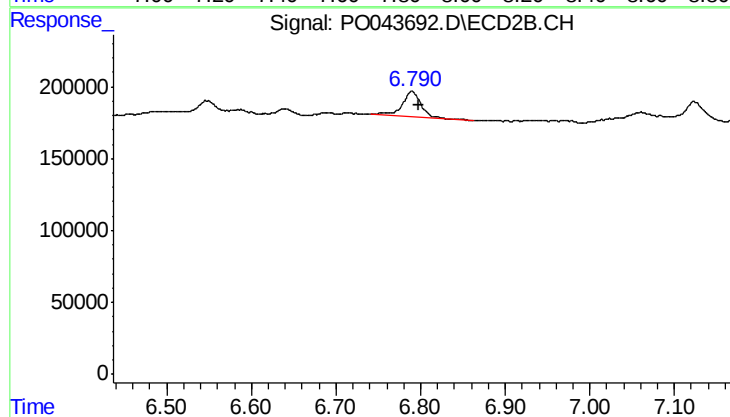

#34 AR-1260-4


R.T.: 6.790 min
Delta R.T.: -0.007 min
Response: 275713
Conc: 7.46 ng/ml

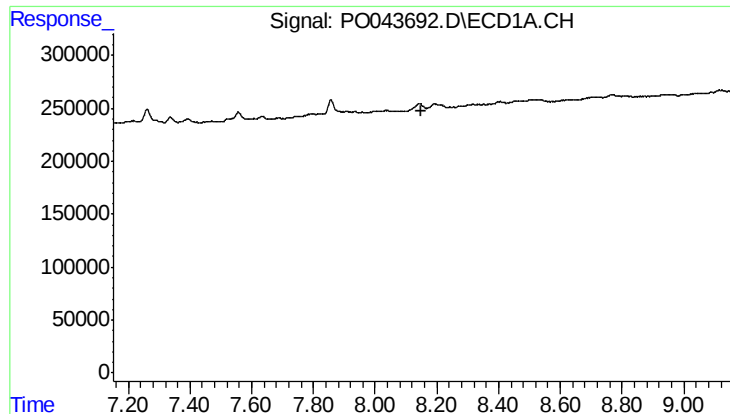

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-D02-D02A-E02-E02A

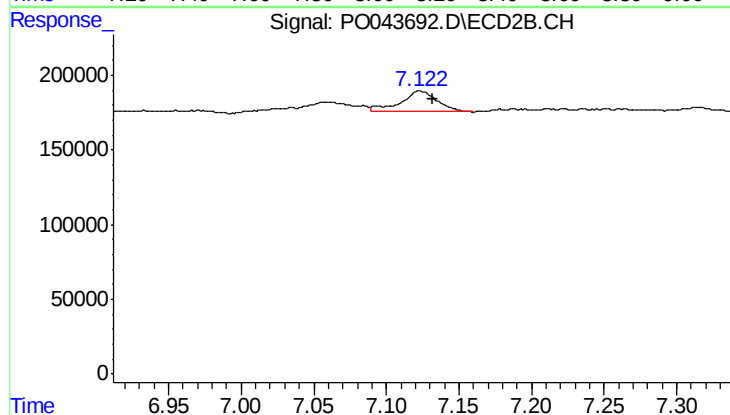


#35 AR-1260-5

R.T.: 7.123 min
Delta R.T.: -0.009 min
Response: 247989
Conc: 9.64 ng/ml

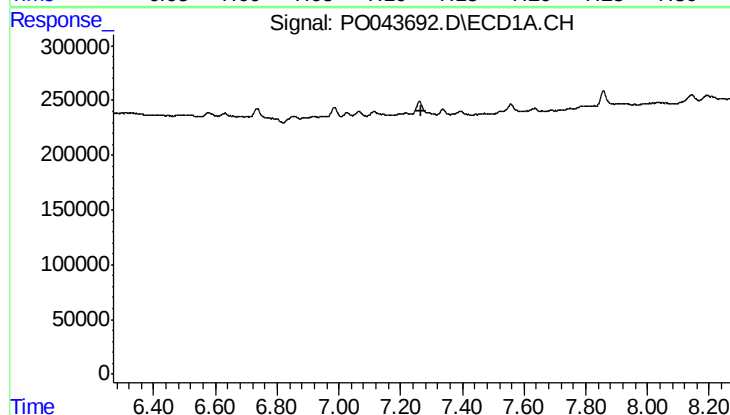


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

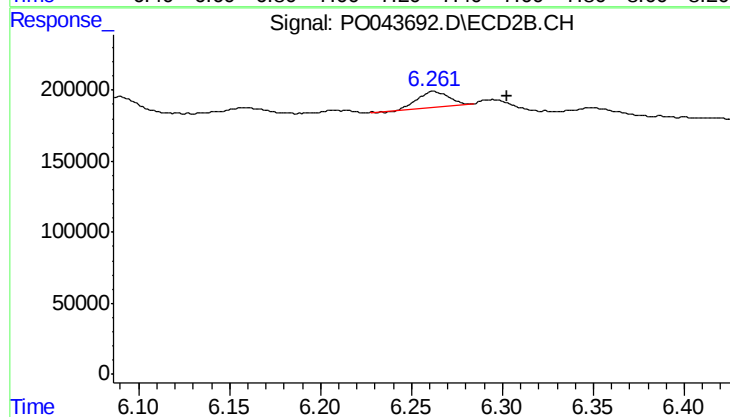

#38 AR-1262-3


R.T.: 6.262 min
Delta R.T.: -0.040 min
Response: 131837
Conc: 3.78 ng/ml

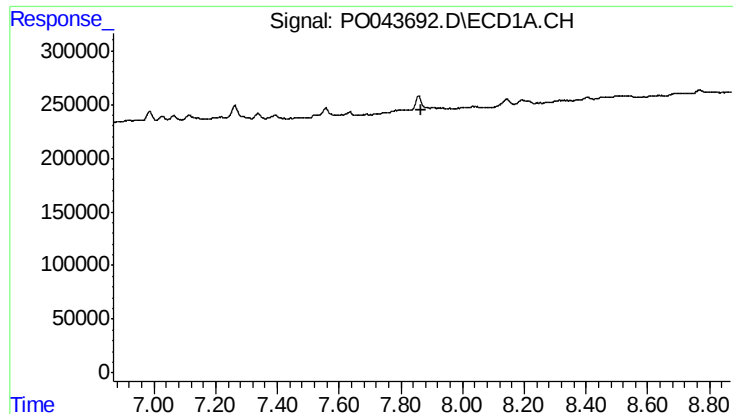

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 7.868 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-D02-D02A-E02-E02A

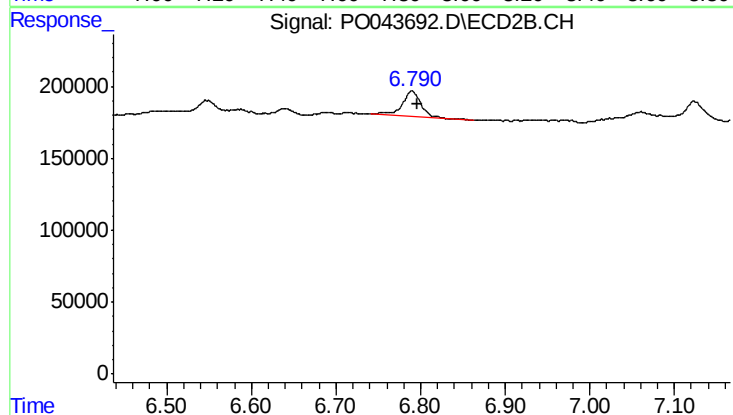


#40 AR-1262-5

R.T.: 6.790 min
Delta R.T.: -0.007 min
Response: 275713
Conc: 4.73 ng/ml

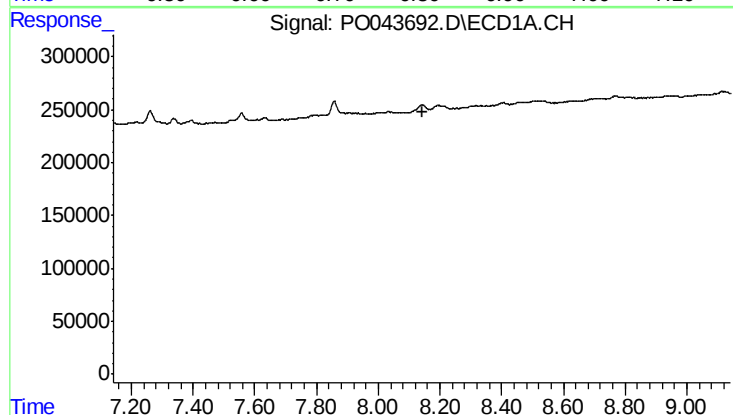


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 8.142 min
Response: 0
Conc: N.D.

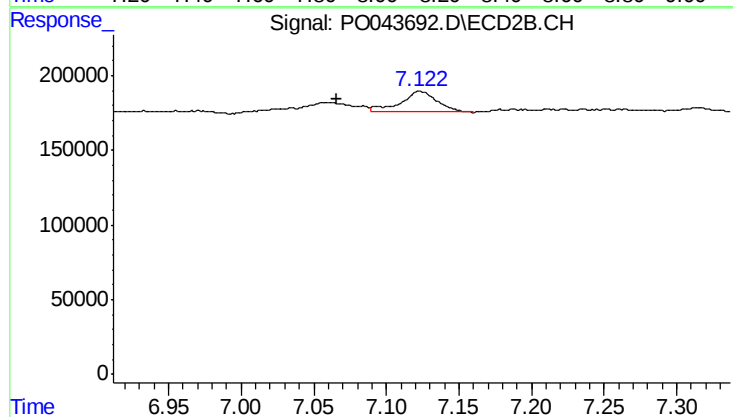

#41 AR-1268-1


R.T.: 7.123 min
Delta R.T.: 0.057 min
Response: 247989
Conc: 4.26 ng/ml

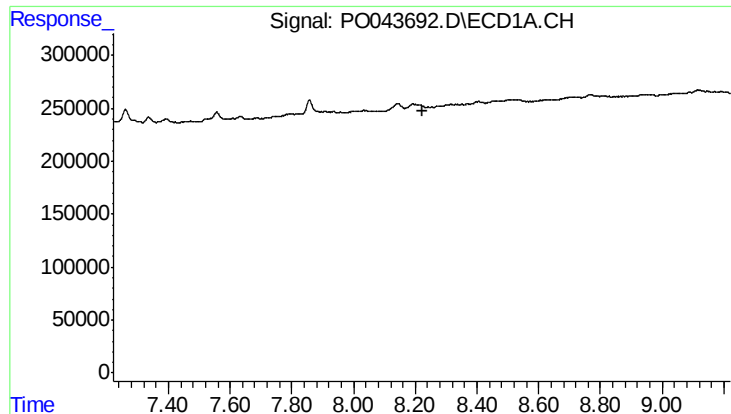

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.222 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-D02-D02A-E02-E02A

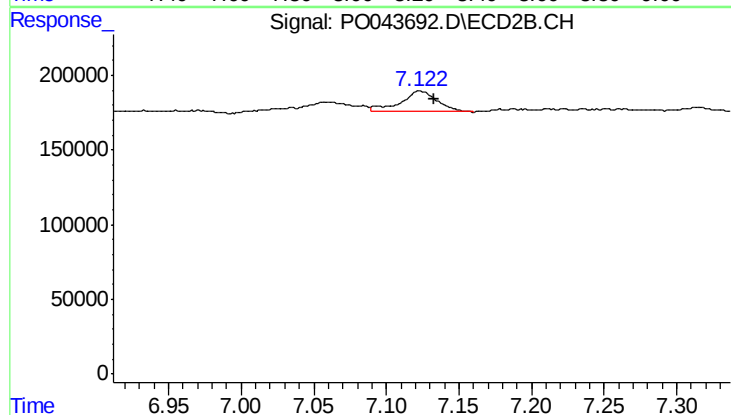

#42 AR-1268-2

R.T.: 7.123 min
Delta R.T.: -0.009 min
Response: 247989
Conc: 4.75 ng/ml