

Data Path : P:\HPCHEM1\ECD_0\Data\P0040918\
Data File : P0043687.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Apr 2018 12:13
Operator : SM/UA
Sample : J2204-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-F02-F02A-G02-G02A

Manual Integrations
APPROVED

UGO
4/11/2018 7:54:38 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 01:41:34 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0040418.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 04 15:17:57 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.069	3.320	4585100	5678541	25.791	21.135
2) SA Decachlor...	9.407	8.084	4540779	5643560	25.197m	24.072

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_0\Data\P0040918\
Data File : P0043687.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Apr 2018 12:13
Operator : SM/UA
Sample : J2204-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-F02-F02A-G02-G02A


Manual Integrations
APPROVED

UGO
4/11/2018 7:54:38 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 01:41:34 2018
Quant Method : P:\HPCHEM1\ECD_0\methods\P0040418.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 04 15:17:57 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

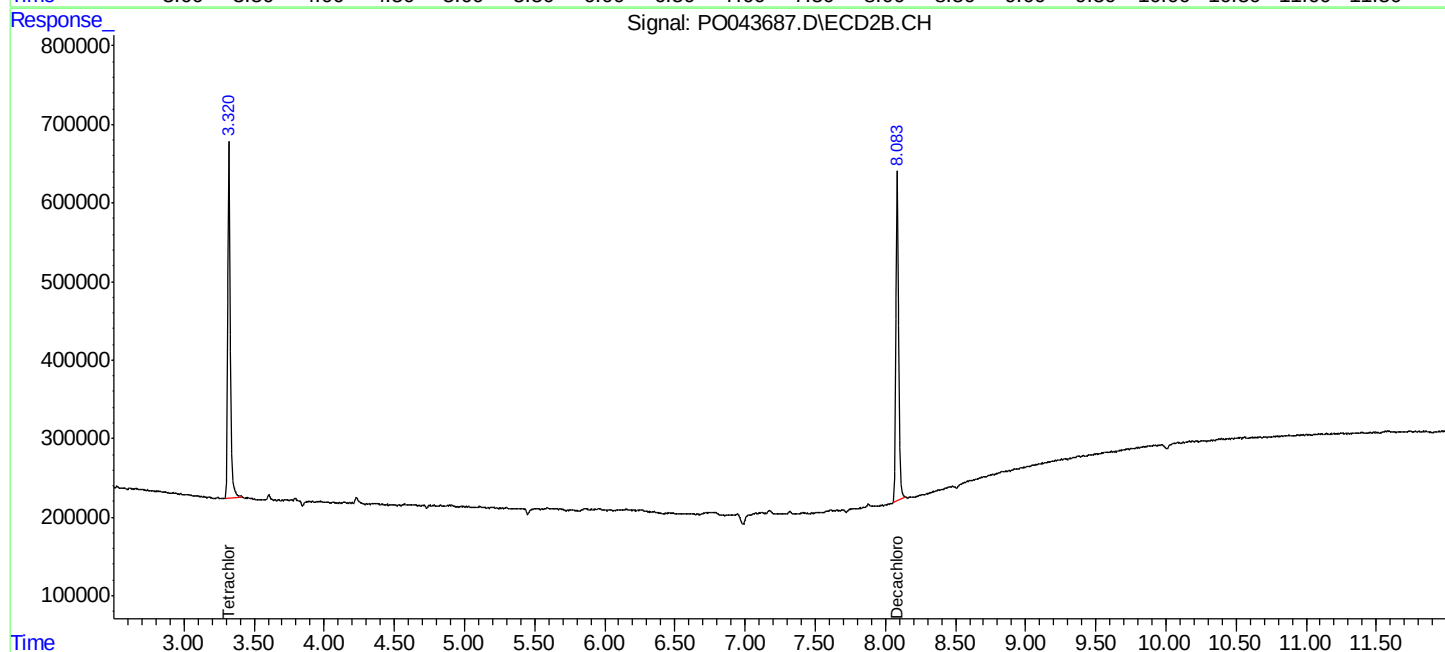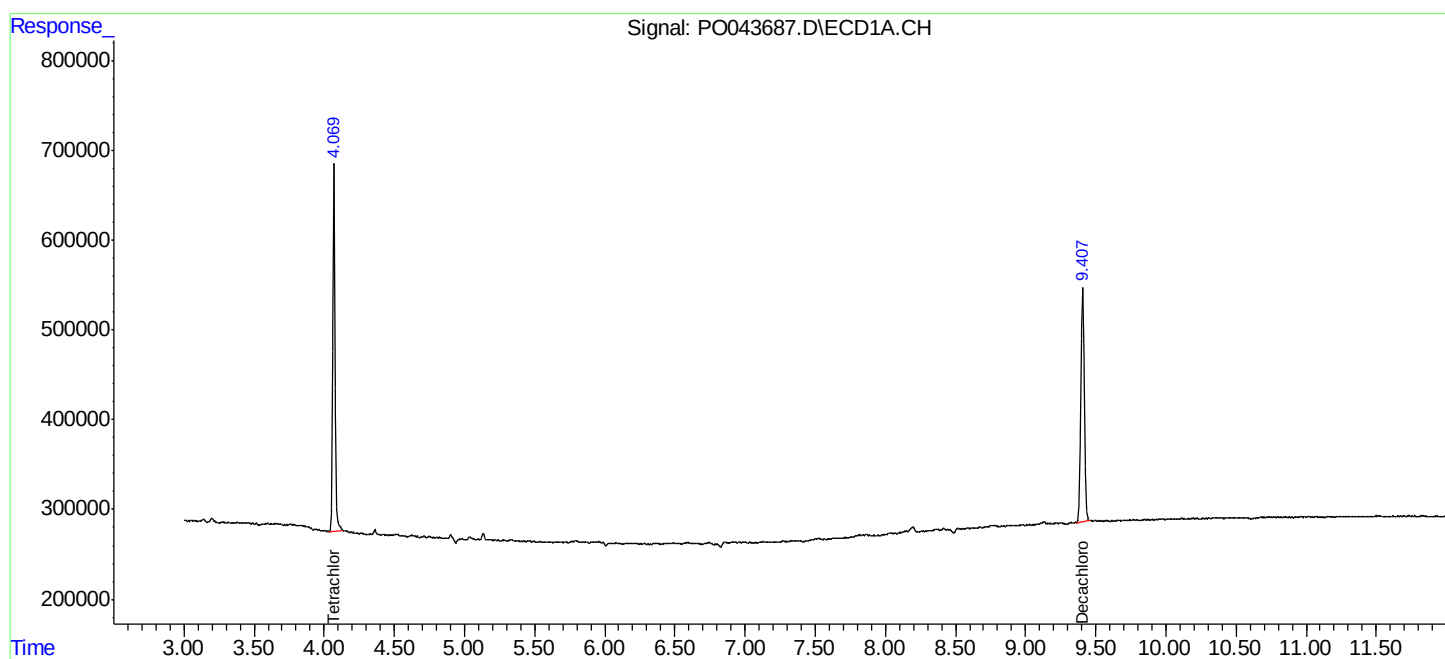

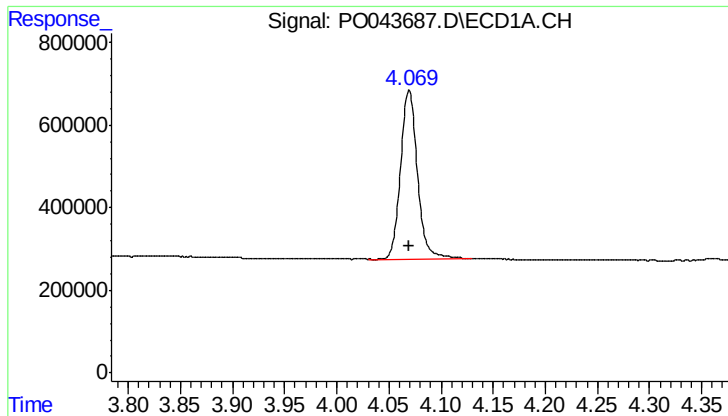


#1 Tetrachloro-m-xylene

R.T.: 4.069 min
Delta R.T.: 0.000 min
Response: 4585100
Conc: 25.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-F02-F02A-G02-G02A


Manual Integrations
APPROVED

UGO
4/11/2018 7:54:38 AM

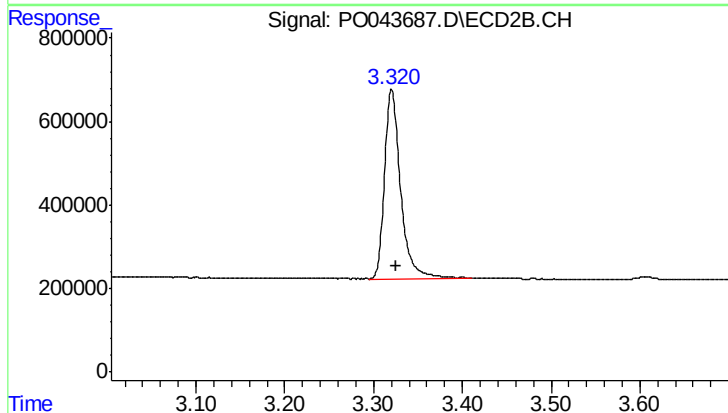


#1 Tetrachloro-m-xylene

R.T.: 3.320 min
Delta R.T.: -0.006 min
Response: 5678541
Conc: 21.13 ng/ml

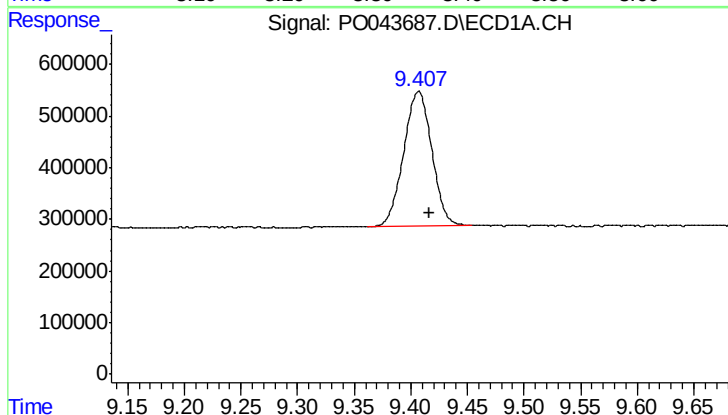

#2 Decachlorobiphenyl

R.T.: 9.407 min
Delta R.T.: -0.010 min
Response: 4540779
Conc: 25.20 ng/ml m

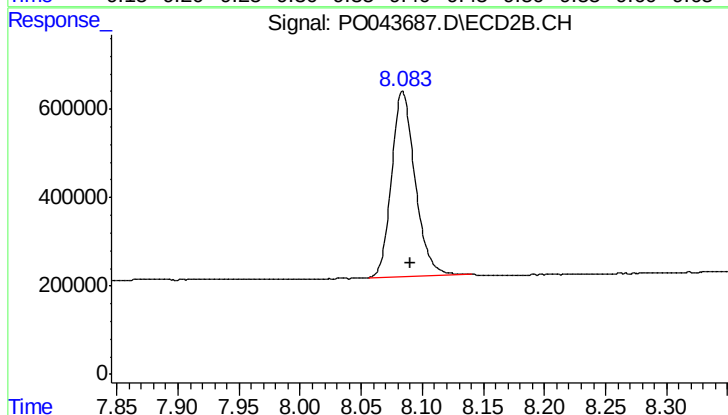

#2 Decachlorobiphenyl

R.T.: 8.084 min
Delta R.T.: -0.006 min
Response: 5643560
Conc: 24.07 ng/ml