

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040919\
 Data File : P0055064.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Apr 2019 11:42
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 05:47:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.312	3.611	727911	689900	20.974	21.619
2)	SA Decachlor...	9.938	8.586	926935	665986	18.803	20.911
Target Compounds							
9)	L2 AR-1221-2	4.617	3.910	11883	10795	35.040	36.009
10)	L2 AR-1221-3	4.617	0.000	11883	0	11.439	N.D. #
11)	L3 AR-1232-1	4.617	0.000	11883	0	13.802	N.D. #
20)	L4 AR-1242-5	6.328	0.000	14293	0	11.840	N.D. #
24)	L5 AR-1248-4	6.328	0.000	14293	0	7.609	N.D. #
25)	L5 AR-1248-5	6.328	0.000	14293	0	7.973	N.D. #
26)	L6 AR-1254-1	6.328	0.000	14293	0	7.883	N.D. #
27)	L6 AR-1254-2	6.496	0.000	13941	0	4.884	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040919\
Data File : P0055064.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Apr 2019 11:42
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 05:47:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

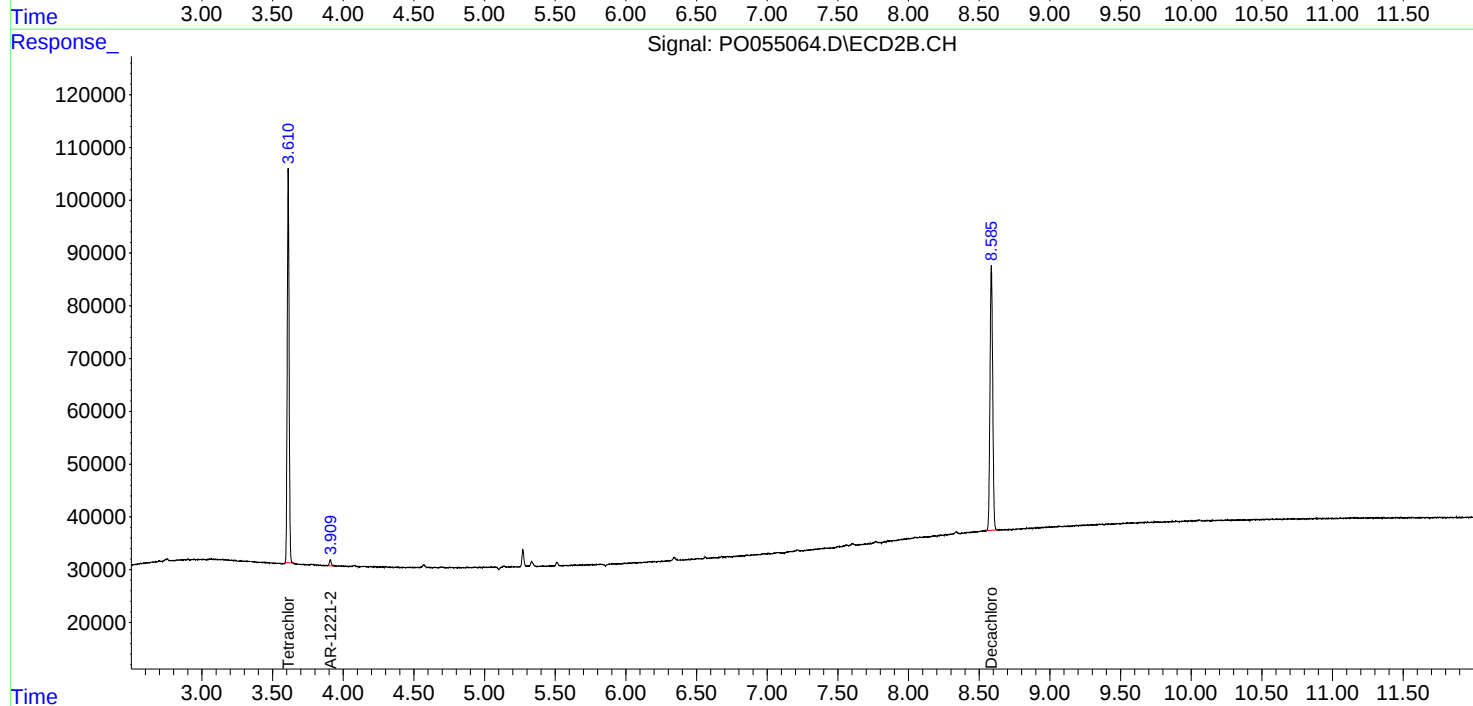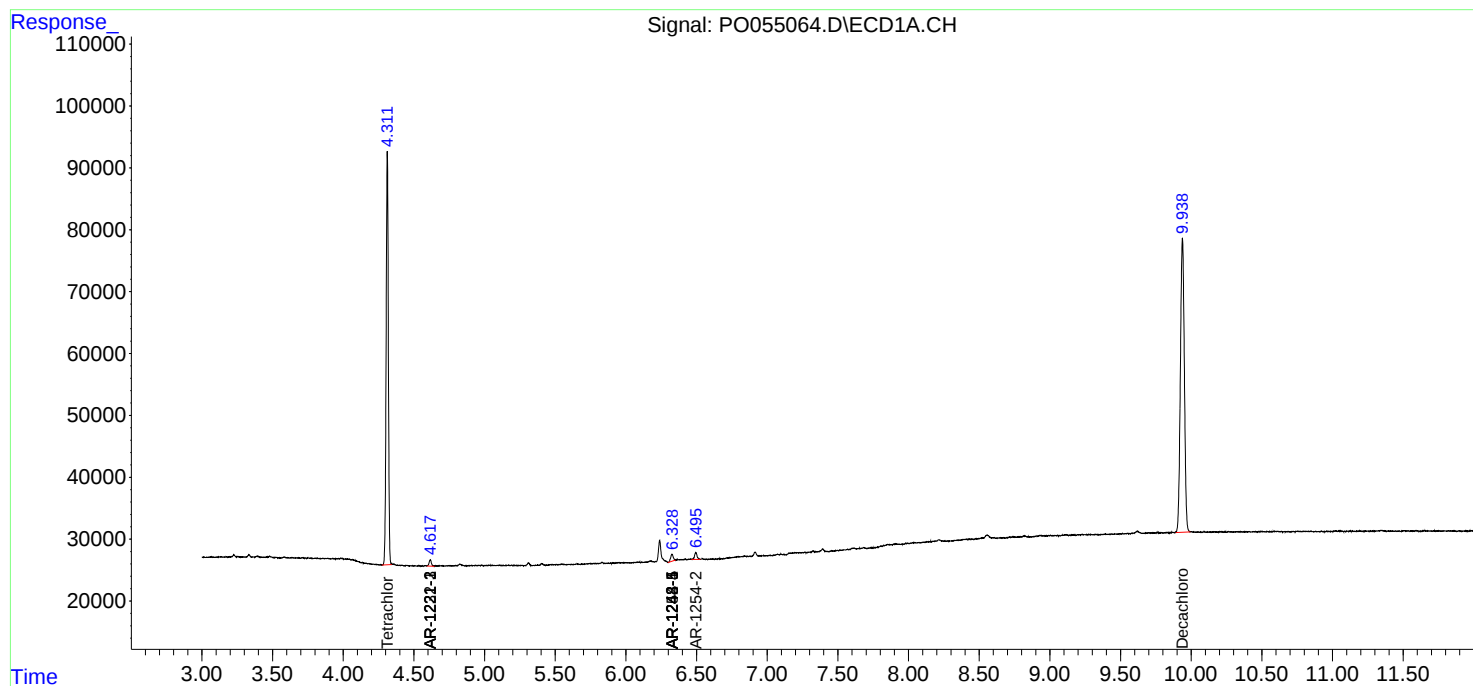


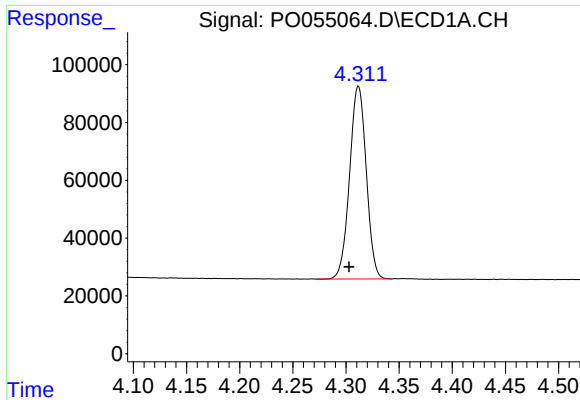

#1 Tetrachloro-m-xylene


R.T.: 4.312 min
Delta R.T.: 0.009 min
Response: 727911
Conc: 20.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

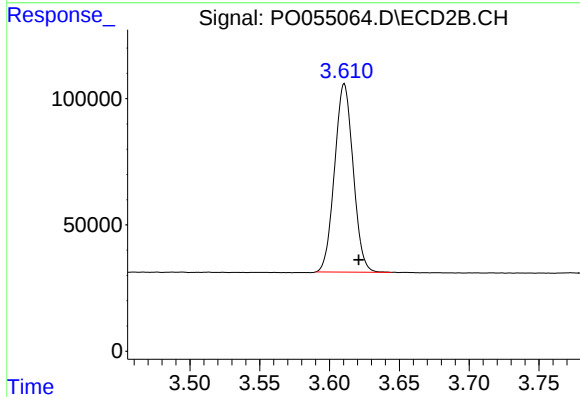


#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: -0.010 min
Response: 689900
Conc: 21.62 ng/ml

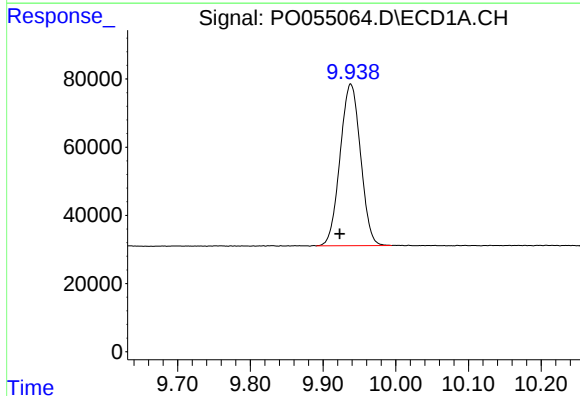


#2 Decachlorobiphenyl

R.T.: 9.938 min
Delta R.T.: 0.015 min
Response: 926935
Conc: 18.80 ng/ml

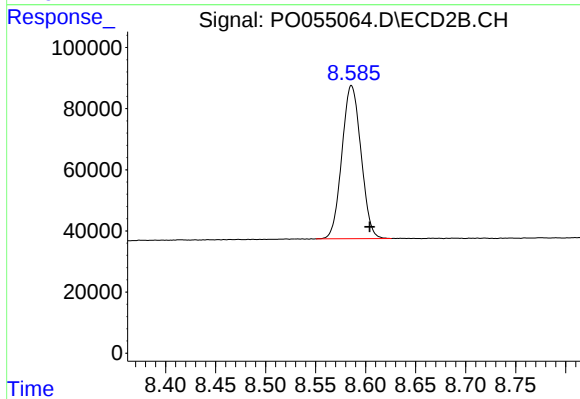

#2 Decachlorobiphenyl


R.T.: 8.586 min
Delta R.T.: -0.018 min
Response: 665986
Conc: 20.91 ng/ml

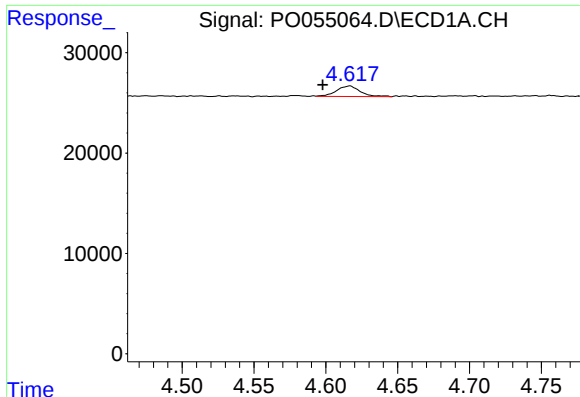

#9 AR-1221-2


R.T.: 4.617 min
Delta R.T.: 0.019 min
Response: 11883
Conc: 35.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

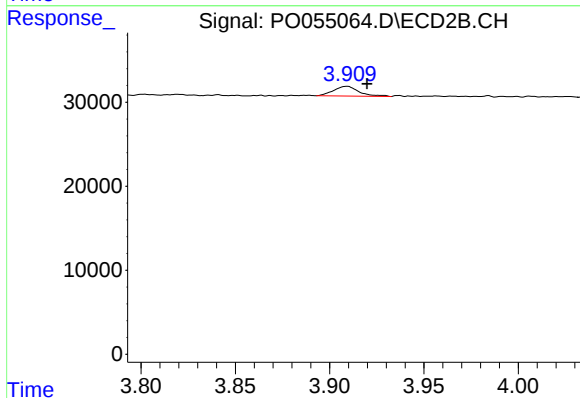


#9 AR-1221-2

R.T.: 3.910 min
Delta R.T.: -0.010 min
Response: 10795
Conc: 36.01 ng/ml

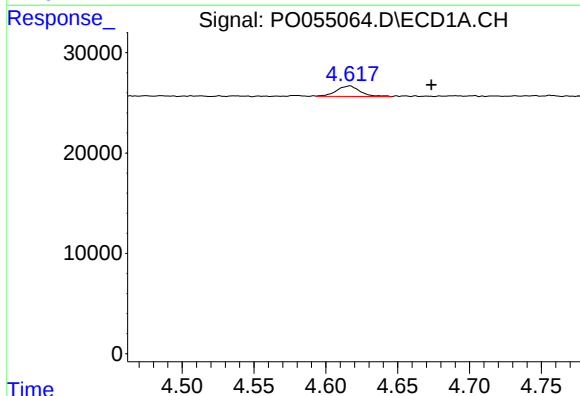


#10 AR-1221-3

R.T.: 4.617 min
Delta R.T.: -0.057 min
Response: 11883
Conc: 11.44 ng/ml

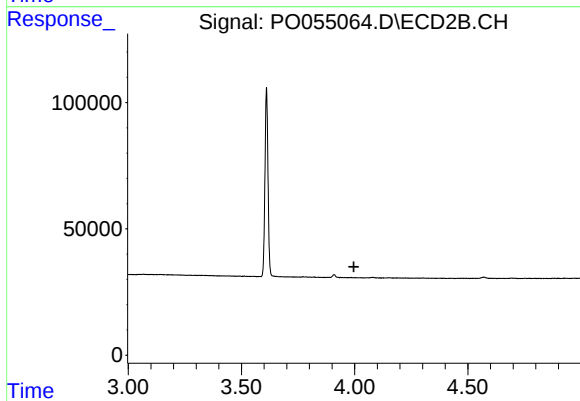

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 3.996 min
Response: 0
Conc: N.D.

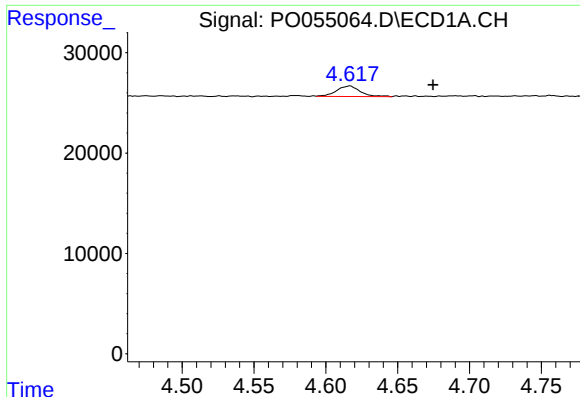

#11 AR-1232-1


R.T.: 4.617 min
Delta R.T.: -0.058 min
Response: 11883
Conc: 13.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

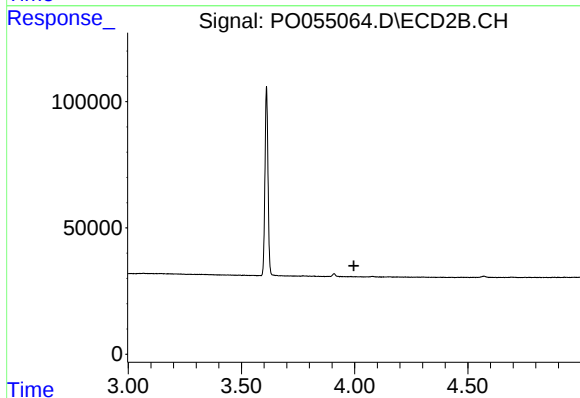


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 3.997 min
Response: 0
Conc: N.D.

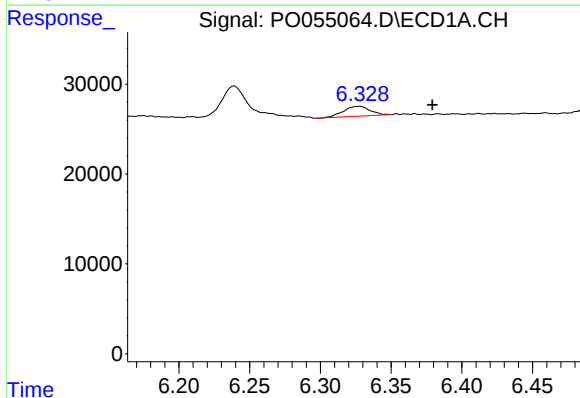


#20 AR-1242-5

R.T.: 6.328 min
Delta R.T.: -0.051 min
Response: 14293
Conc: 11.84 ng/ml

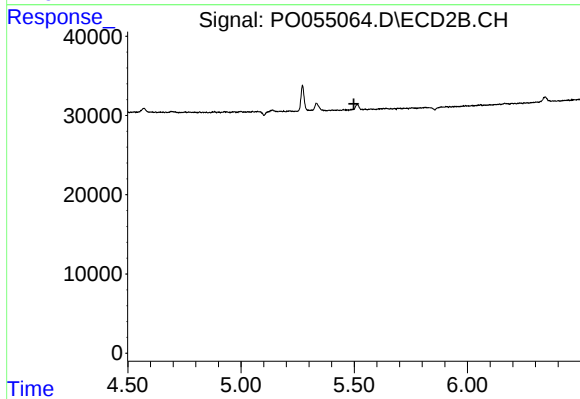

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 5.498 min
Response: 0
Conc: N.D.

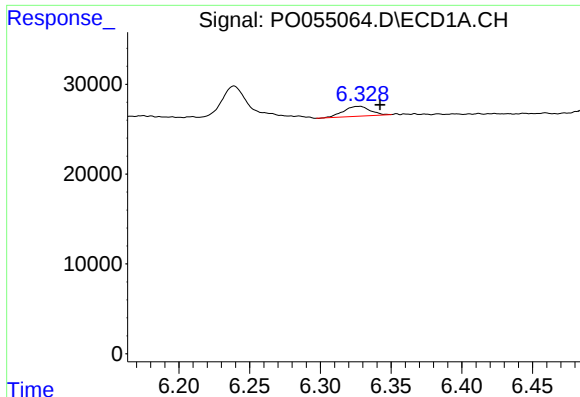

#24 AR-1248-4


R.T.: 6.328 min
Delta R.T.: -0.014 min
Response: 14293
Conc: 7.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

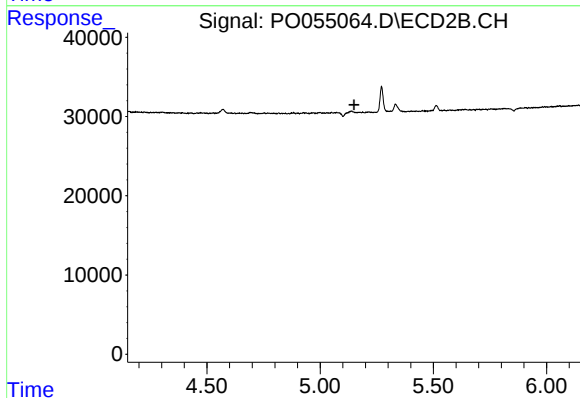


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.149 min
Response: 0
Conc: N.D.

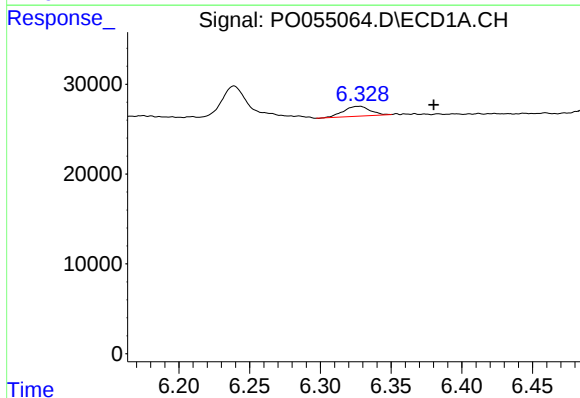


#25 AR-1248-5

R.T.: 6.328 min
Delta R.T.: -0.052 min
Response: 14293
Conc: 7.97 ng/ml

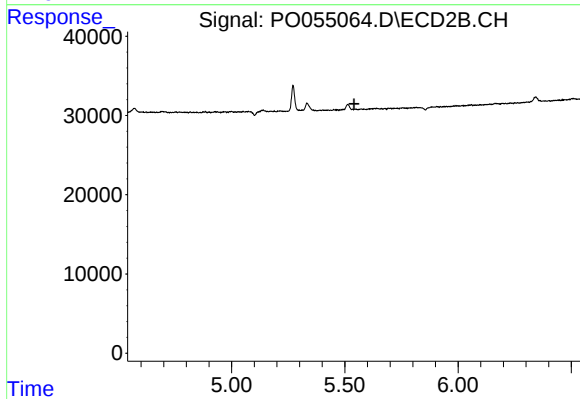

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 5.540 min
Response: 0
Conc: N.D.

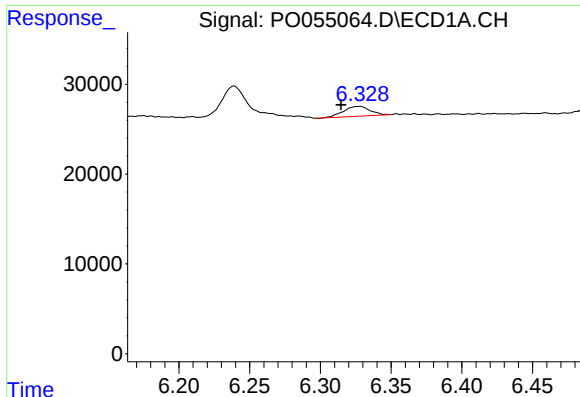

#26 AR-1254-1


R.T.: 6.328 min
Delta R.T.: 0.014 min
Response: 14293
Conc: 7.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

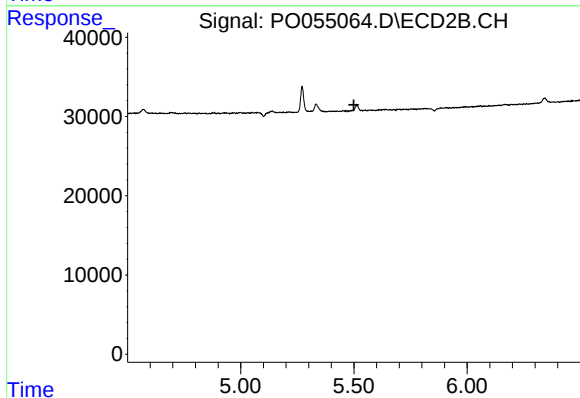


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.500 min
Response: 0
Conc: N.D.

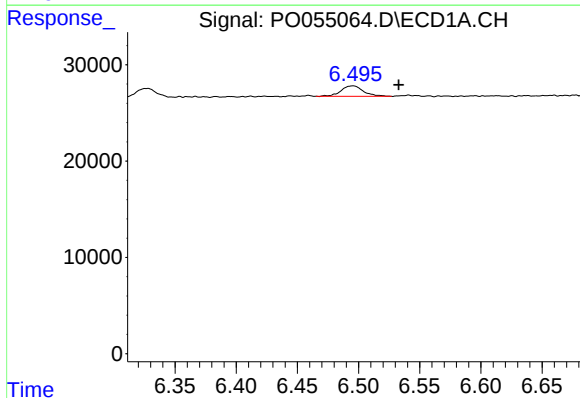

#27 AR-1254-2

R.T.: 6.496 min
Delta R.T.: -0.037 min
Response: 13941
Conc: 4.88 ng/ml

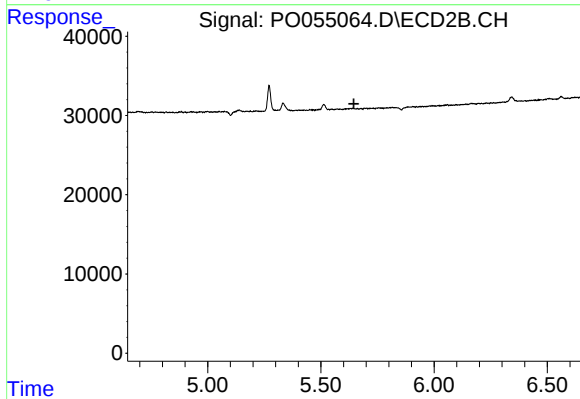

#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.646 min
Response: 0
Conc: N.D.