

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040919\
 Data File : P0055078.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Apr 2019 16:25
 Operator : SM/SJ
 Sample : K1560-09
 Misc : AR1660 MDL 100PPB
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 05:55:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.298	3.611	865472	794556	24.938	24.898
2)	SA Decachlor...	9.919	8.583	1050175	749453	21.303	23.532
Target Compounds							
3)	L1 AR-1016-1	5.461	4.707	71536	82032	39.755	51.873 #
4)	L1 AR-1016-2	5.484	4.707	96264	82032	38.759	38.284
5)	L1 AR-1016-3	5.545	4.883	64093	45393	40.739	37.570
6)	L1 AR-1016-4	5.643	4.923	50943	37321	39.095	36.931
7)	L1 AR-1016-5	5.936	5.135	54804	42349	41.074	32.491
9)	L2 AR-1221-2	4.598	3.909	10349	17911	30.518	59.743 #
10)	L2 AR-1221-3	4.669	3.984	33905	26751	32.639	29.022
11)	L3 AR-1232-1	4.669	3.984	33905	26751	39.380	35.674
12)	L3 AR-1232-2	5.195	4.707	47972	82032	98.075	95.264
13)	L3 AR-1232-3	5.484	4.883	96264	45393	98.499	93.677
14)	L3 AR-1232-4	5.643	4.964	50943	45133	99.527	102.715
15)	L3 AR-1232-5	5.733	5.135	49687	42349	119.441	87.073 #
16)	L4 AR-1242-1	5.461	4.707	71536	82032	51.491	66.817 #
17)	L4 AR-1242-2	5.484	4.707	96264	82032	50.308	49.500
18)	L4 AR-1242-3	5.545	4.883	64093	45393	51.711	47.917
19)	L4 AR-1242-4	5.643	4.964	50943	45133	49.967	47.222
20)	L4 AR-1242-5	6.375	5.486	14244	49852	11.800	40.533 #
21)	L5 AR-1248-1	5.461	4.707	71536	82032	71.559	93.454 #
22)	L5 AR-1248-2	5.733	4.923	49687	37321	34.213	30.881
23)	L5 AR-1248-3	5.936	4.964	54804	45133	34.313	36.170
24)	L5 AR-1248-4	6.338	5.135	18034	42349	9.600	27.806 #
25)	L5 AR-1248-5	6.375	5.527	14244	10852	7.945	7.279
26)	L6 AR-1254-1	6.311	5.486	49388	49852	27.238	22.811
27)	L6 AR-1254-2	6.528	5.631	48325	37952	16.928	19.573
28)	L6 AR-1254-3	6.895	6.049	29346	68360	9.332	21.325 #
29)	L6 AR-1254-4	7.178	6.289	14774	21739	6.039	11.103 #
30)	L6 AR-1254-5	7.595	6.676	147036	120017	54.858	41.749
31)	L7 AR-1260-1	7.056	6.162	113569	99436	45.199	43.269
32)	L7 AR-1260-2	7.313	6.349	134693	121238	43.400	44.042
33)	L7 AR-1260-3	7.670	6.503	96067	107116	39.141	41.551
34)	L7 AR-1260-4	7.895	6.972	105597	81915	38.177	38.491
35)	L7 AR-1260-5	8.205	7.212	182467	174654	32.885	36.468
36)	L8 AR-1262-1	7.670	6.714	96067	91653	28.831	30.808
37)	L8 AR-1262-2	8.205	7.212	182467	174654	30.799	35.635
38)	L8 AR-1262-3	8.517	7.495	119164	41487	28.764	20.203 #
39)	L8 AR-1262-4	8.570	7.558	74179	120249	23.023	33.198 #
40)	L8 AR-1262-5	9.213	8.050	46676	38519	21.349	23.867
41)	L9 AR-1268-1	8.517	7.495	119164	41487	16.742	7.337 #
42)	L9 AR-1268-2	8.570	7.558	74179	120249	11.322	23.252 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040919\
 Data File : P0055078.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Apr 2019 16:25
 Operator : SM/SJ
 Sample : K1560-09
 Misc : AR1660 MDL 100PPB
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 05:55:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43) L9	AR-1268-3	0.000	7.765	0	9064	N.D.	2.106 #
44) L9	AR-1268-4	9.213	8.050	46676	38519	19.564	20.778
45) L9	AR-1268-5	9.604	8.335	19429	11924	1.179	1.048



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040919\
Data File : P0055078.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Apr 2019 16:25
Operator : SM/SJ
Sample : K1560-09
Misc : AR1660 MDL 100PPB
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 05:55:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

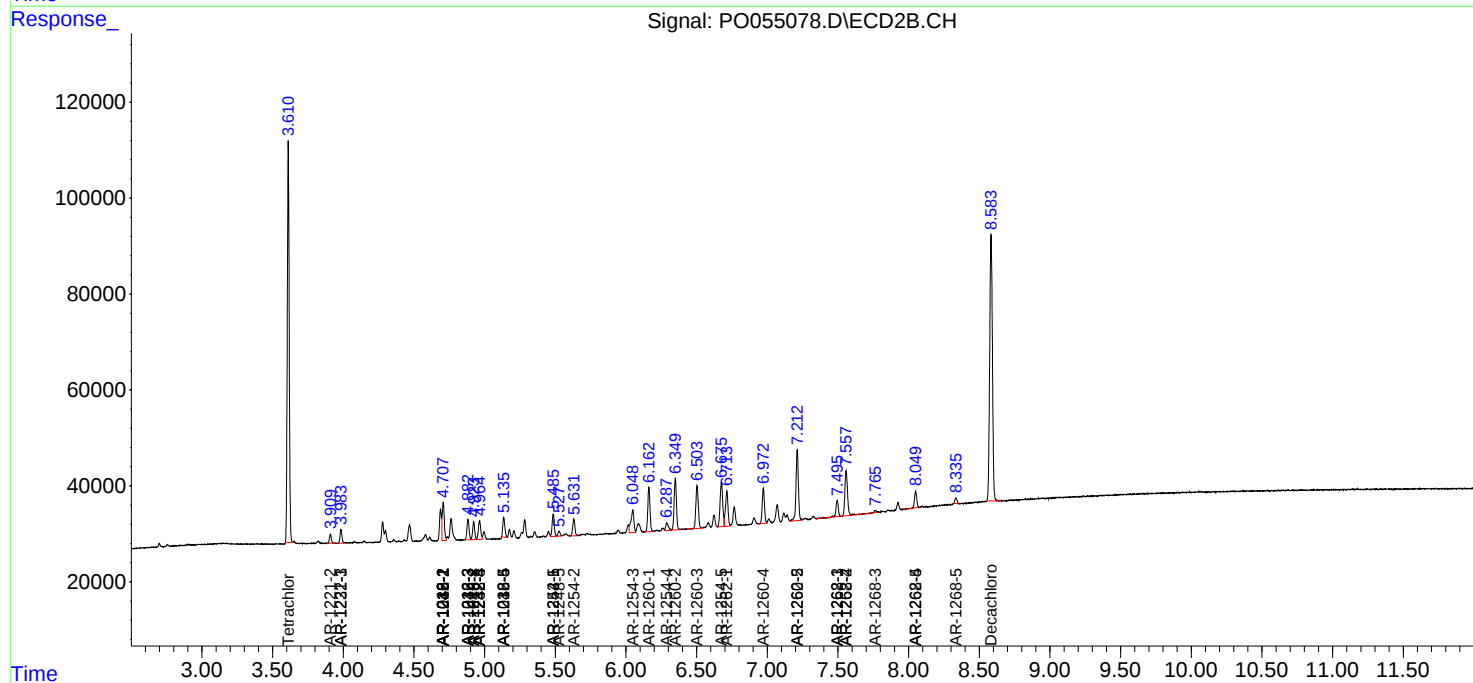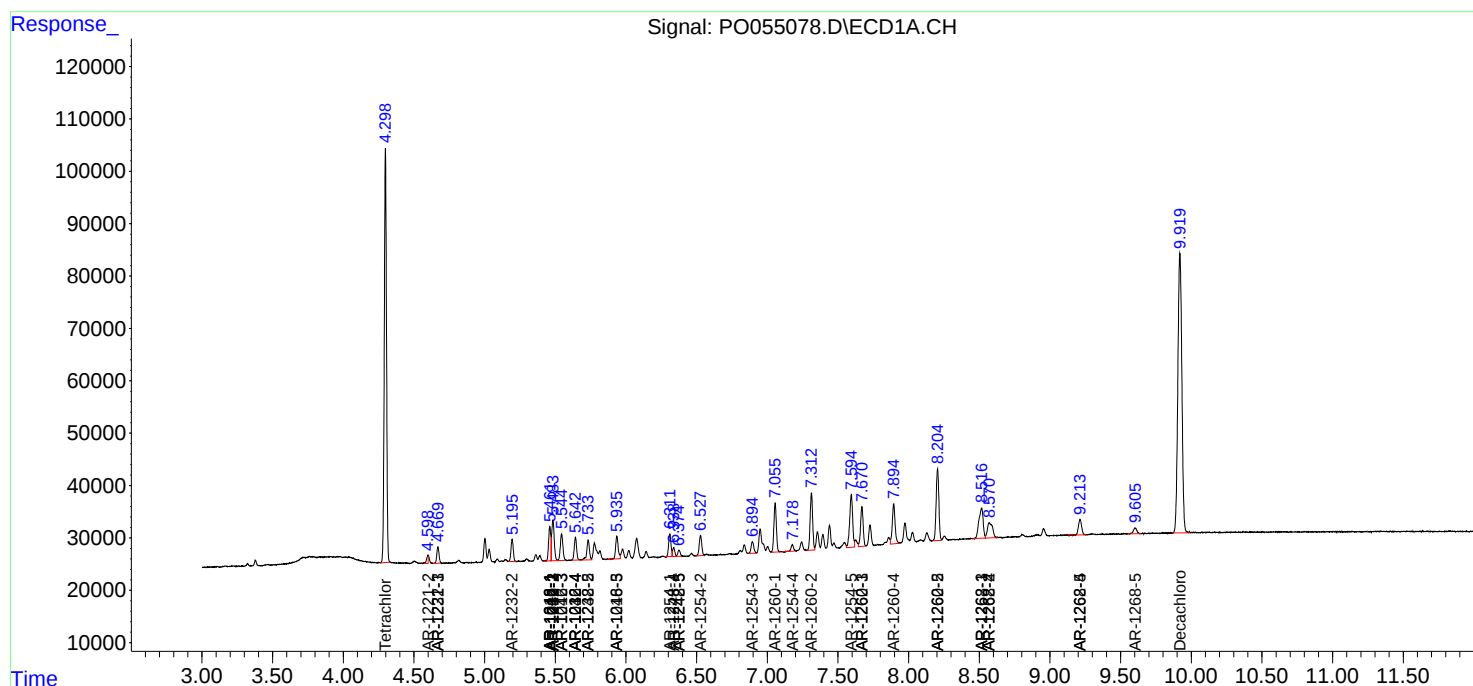


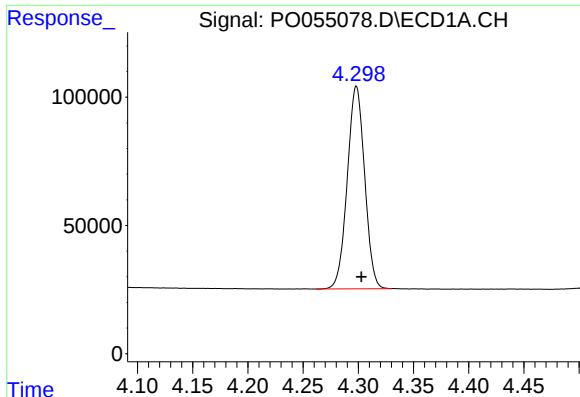

#1 Tetrachloro-m-xylene


R.T.: 4.298 min
Delta R.T.: -0.005 min
Response: 865472
Conc: 24.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

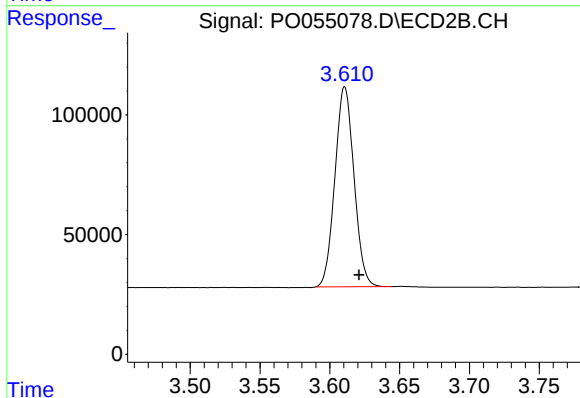


#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: -0.010 min
Response: 794556
Conc: 24.90 ng/ml

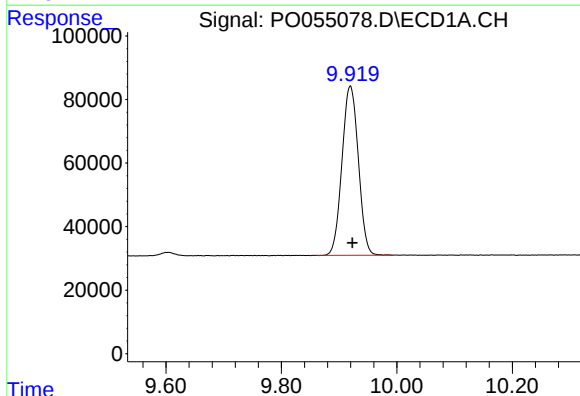


#2 Decachlorobiphenyl

R.T.: 9.919 min
Delta R.T.: -0.004 min
Response: 1050175
Conc: 21.30 ng/ml

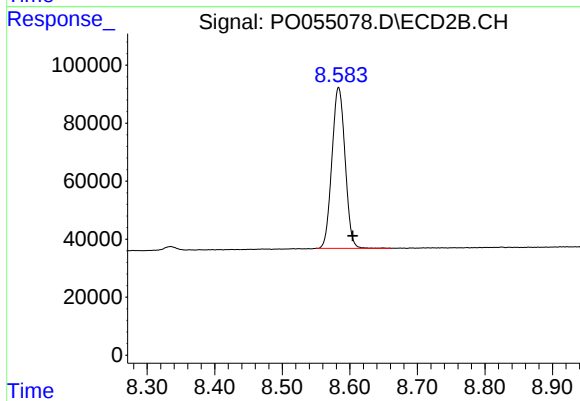

#2 Decachlorobiphenyl


R.T.: 8.583 min
Delta R.T.: -0.021 min
Response: 749453
Conc: 23.53 ng/ml

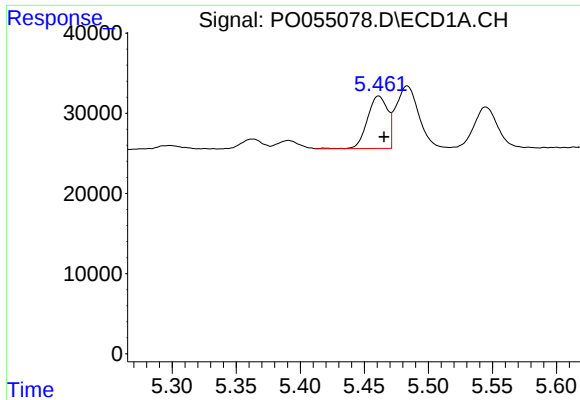

#3 AR-1016-1


R.T.: 5.461 min
Delta R.T.: -0.004 min
Response: 71536
Conc: 39.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

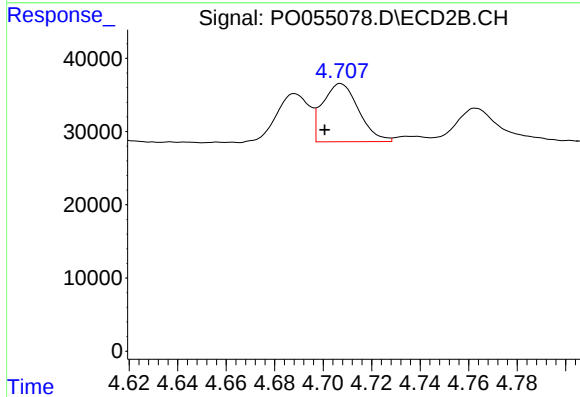


#3 AR-1016-1

R.T.: 4.707 min
Delta R.T.: 0.007 min
Response: 82032
Conc: 51.87 ng/ml

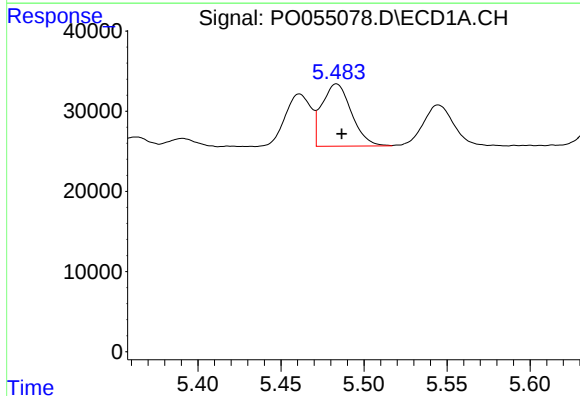


#4 AR-1016-2

R.T.: 5.484 min
Delta R.T.: -0.003 min
Response: 96264
Conc: 38.76 ng/ml

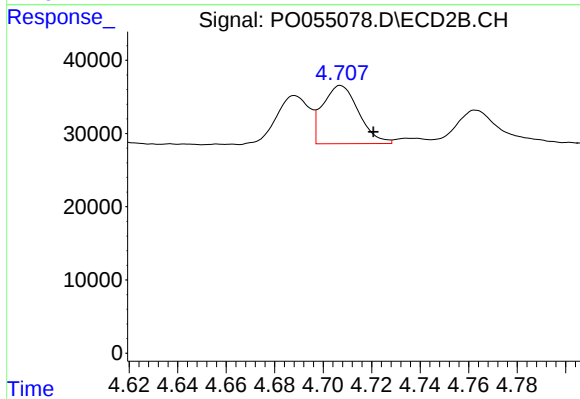

#4 AR-1016-2


R.T.: 4.707 min
Delta R.T.: -0.014 min
Response: 82032
Conc: 38.28 ng/ml

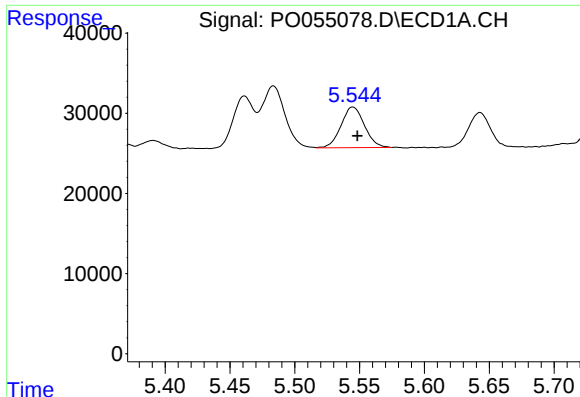

#5 AR-1016-3


R.T.: 5.545 min
Delta R.T.: -0.004 min
Response: 64093
Conc: 40.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

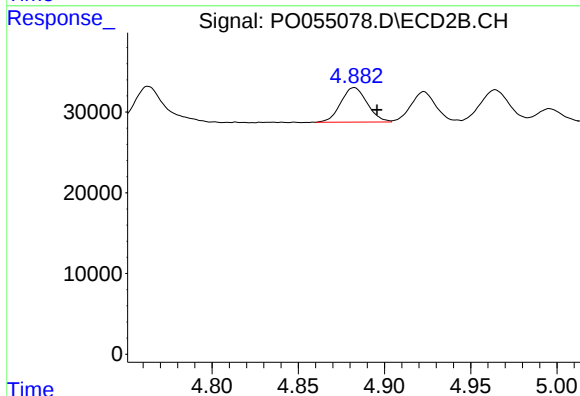


#5 AR-1016-3

R.T.: 4.883 min
Delta R.T.: -0.013 min
Response: 45393
Conc: 37.57 ng/ml

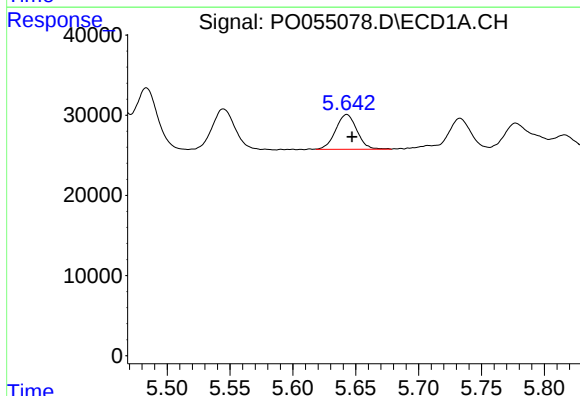


#6 AR-1016-4

R.T.: 5.643 min
Delta R.T.: -0.004 min
Response: 50943
Conc: 39.09 ng/ml

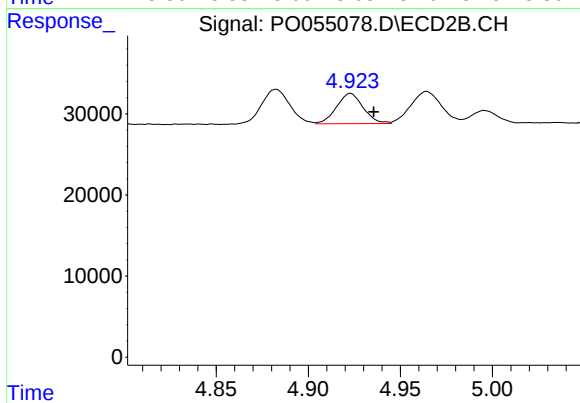

#6 AR-1016-4


R.T.: 4.923 min
Delta R.T.: -0.013 min
Response: 37321
Conc: 36.93 ng/ml

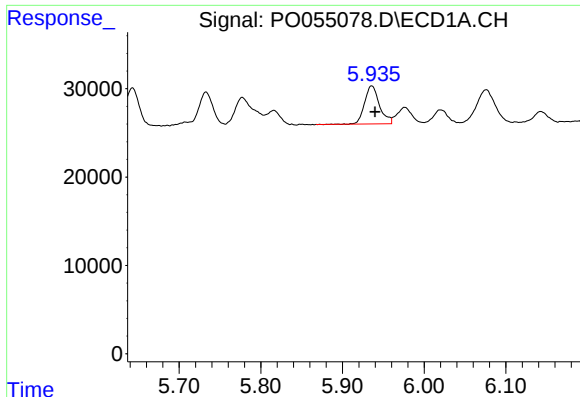

#7 AR-1016-5


R.T.: 5.936 min
Delta R.T.: -0.004 min
Response: 54804
Conc: 41.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

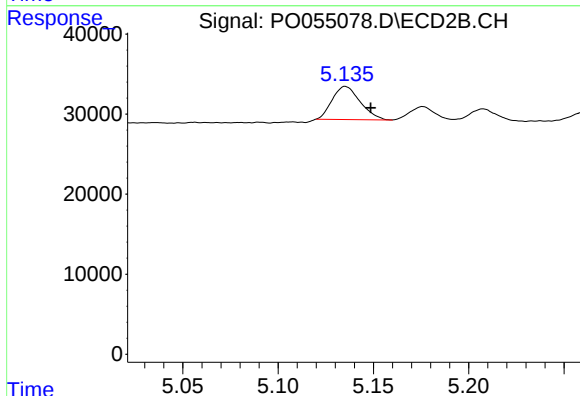


#7 AR-1016-5

R.T.: 5.135 min
Delta R.T.: -0.013 min
Response: 42349
Conc: 32.49 ng/ml

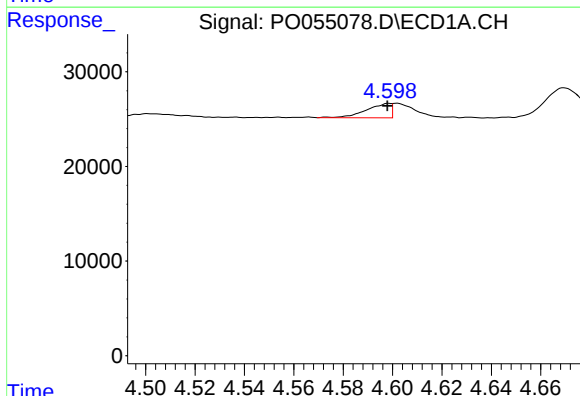


#9 AR-1221-2

R.T.: 4.598 min
Delta R.T.: 0.000 min
Response: 10349
Conc: 30.52 ng/ml

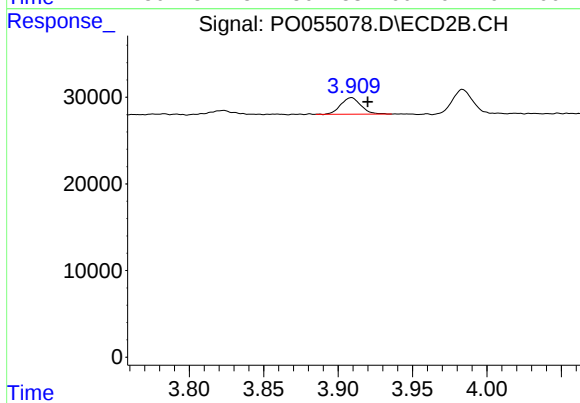

#9 AR-1221-2


R.T.: 3.909 min
Delta R.T.: -0.011 min
Response: 17911
Conc: 59.74 ng/ml

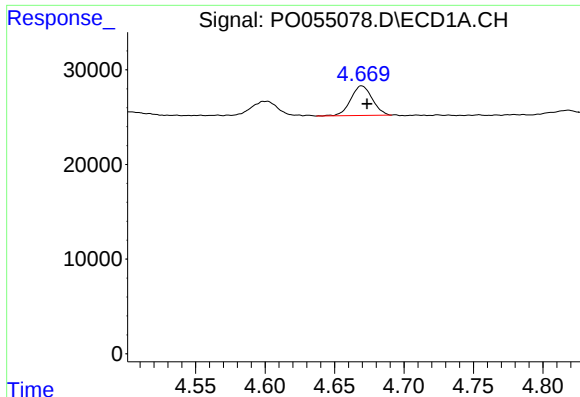

#10 AR-1221-3


R.T.: 4.669 min
Delta R.T.: -0.004 min
Response: 33905
Conc: 32.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

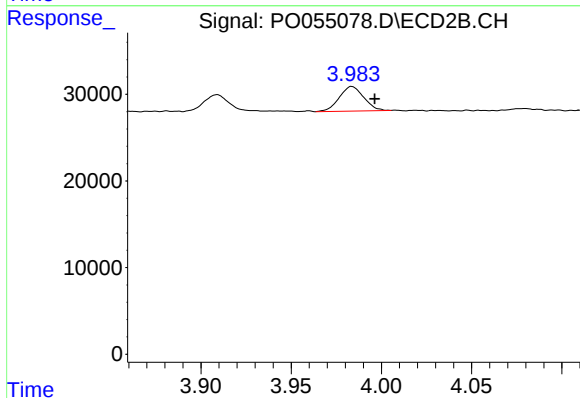


#10 AR-1221-3

R.T.: 3.984 min
Delta R.T.: -0.013 min
Response: 26751
Conc: 29.02 ng/ml

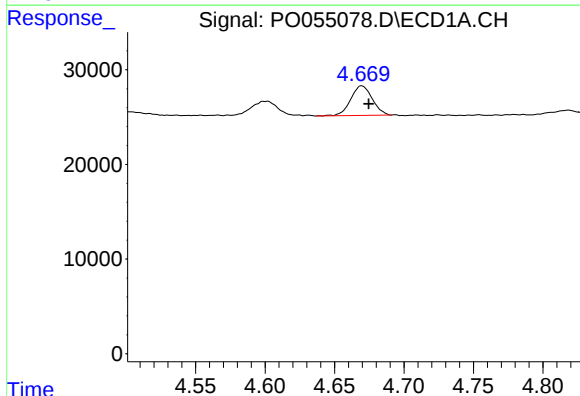


#11 AR-1232-1

R.T.: 4.669 min
Delta R.T.: -0.005 min
Response: 33905
Conc: 39.38 ng/ml

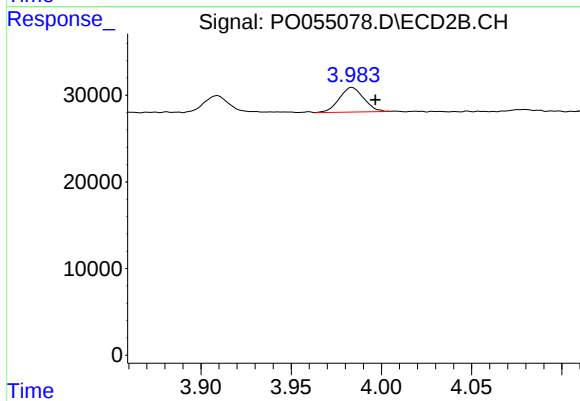

#11 AR-1232-1


R.T.: 3.984 min
Delta R.T.: -0.013 min
Response: 26751
Conc: 35.67 ng/ml

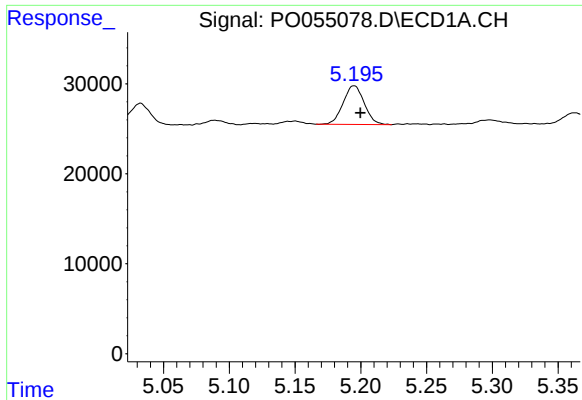

#12 AR-1232-2


R.T.: 5.195 min
Delta R.T.: -0.005 min
Response: 47972
Conc: 98.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

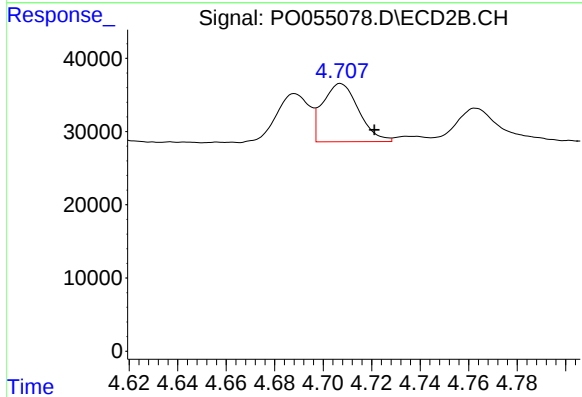


#12 AR-1232-2

R.T.: 4.707 min
Delta R.T.: -0.014 min
Response: 82032
Conc: 95.26 ng/ml

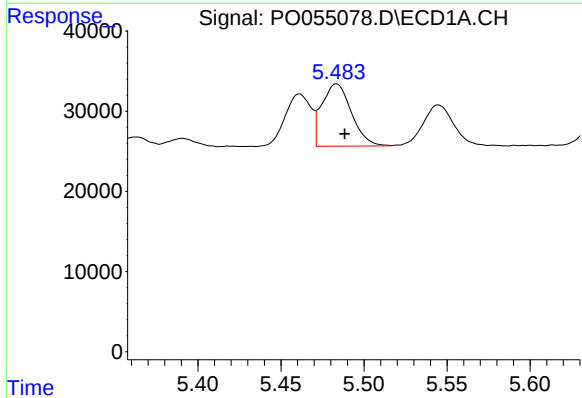


#13 AR-1232-3

R.T.: 5.484 min
Delta R.T.: -0.005 min
Response: 96264
Conc: 98.50 ng/ml

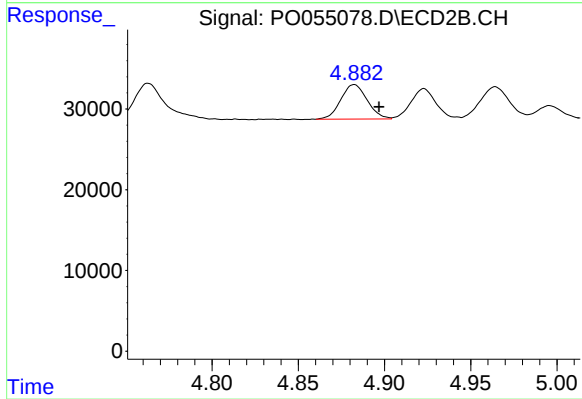

#13 AR-1232-3


R.T.: 4.883 min
Delta R.T.: -0.014 min
Response: 45393
Conc: 93.68 ng/ml

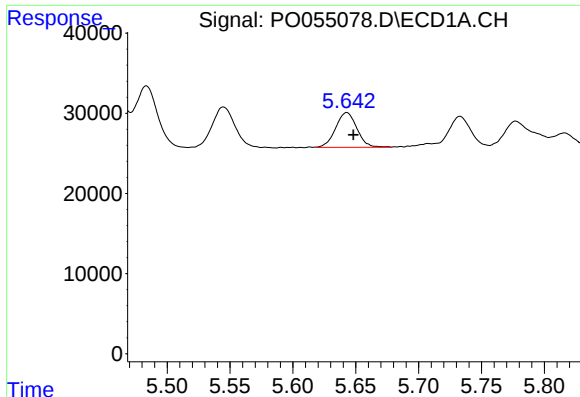

#14 AR-1232-4


R.T.: 5.643 min
Delta R.T.: -0.005 min
Response: 50943
Conc: 99.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

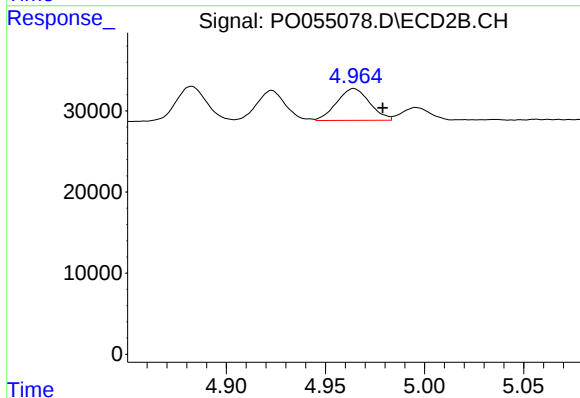


#14 AR-1232-4

R.T.: 4.964 min
Delta R.T.: -0.015 min
Response: 45133
Conc: 102.71 ng/ml

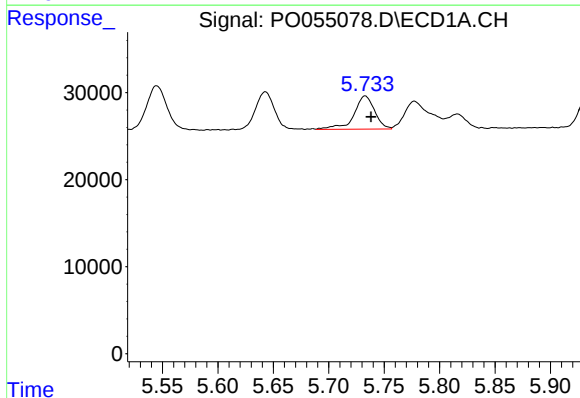


#15 AR-1232-5

R.T.: 5.733 min
Delta R.T.: -0.005 min
Response: 49687
Conc: 119.44 ng/ml

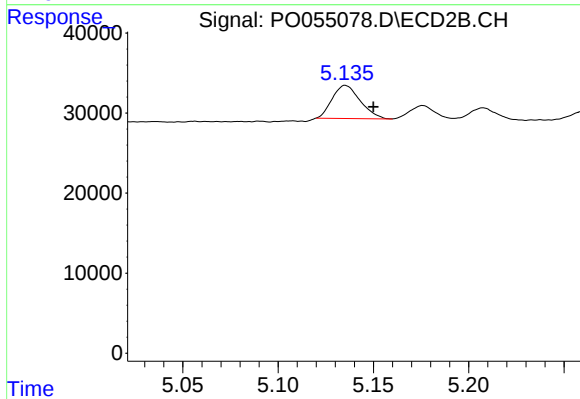

#15 AR-1232-5


R.T.: 5.135 min
Delta R.T.: -0.015 min
Response: 42349
Conc: 87.07 ng/ml

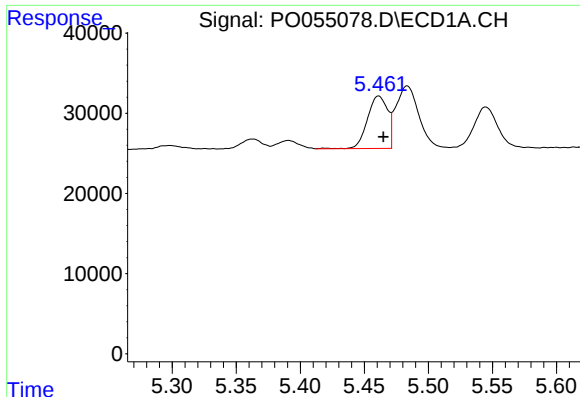

#16 AR-1242-1


R.T.: 5.461 min
Delta R.T.: -0.004 min
Response: 71536
Conc: 51.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

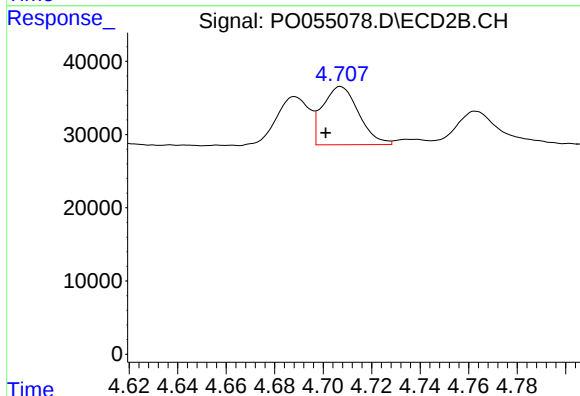


#16 AR-1242-1

R.T.: 4.707 min
Delta R.T.: 0.006 min
Response: 82032
Conc: 66.82 ng/ml

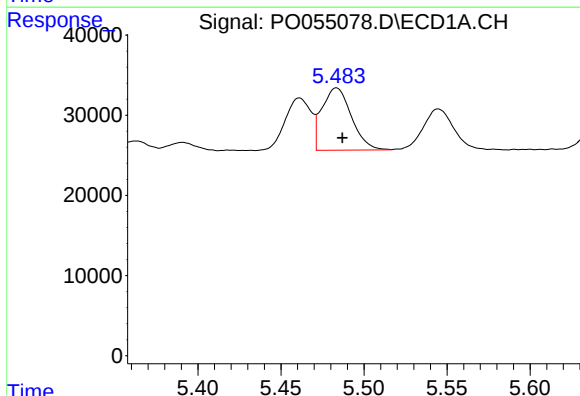


#17 AR-1242-2

R.T.: 5.484 min
Delta R.T.: -0.004 min
Response: 96264
Conc: 50.31 ng/ml

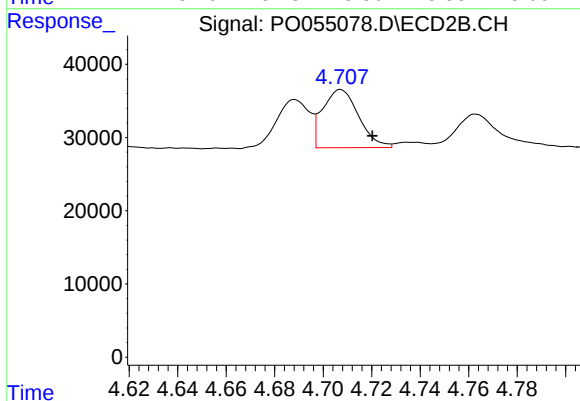

#17 AR-1242-2


R.T.: 4.707 min
Delta R.T.: -0.013 min
Response: 82032
Conc: 49.50 ng/ml

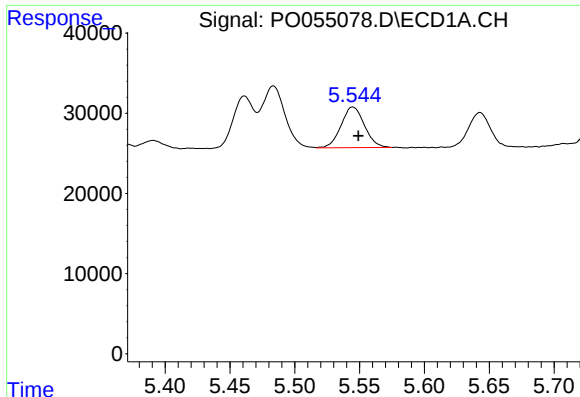

#18 AR-1242-3


R.T.: 5.545 min
Delta R.T.: -0.004 min
Response: 64093
Conc: 51.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

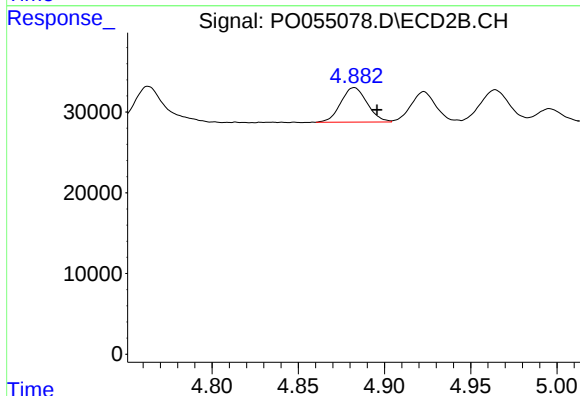


#18 AR-1242-3

R.T.: 4.883 min
Delta R.T.: -0.013 min
Response: 45393
Conc: 47.92 ng/ml

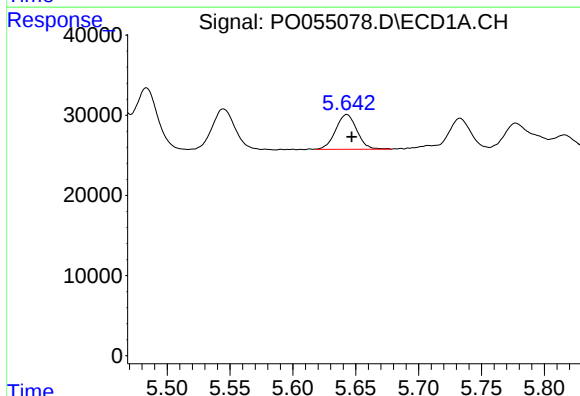


#19 AR-1242-4

R.T.: 5.643 min
Delta R.T.: -0.004 min
Response: 50943
Conc: 49.97 ng/ml

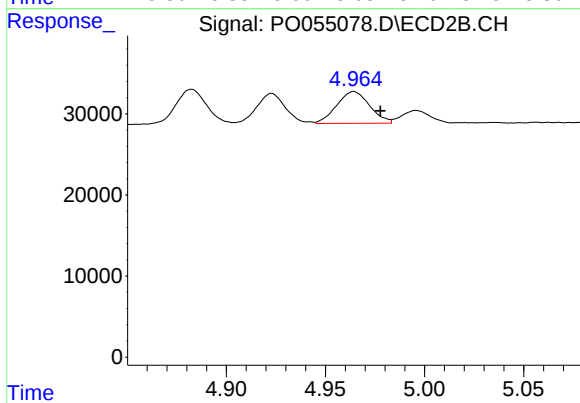

#19 AR-1242-4


R.T.: 4.964 min
Delta R.T.: -0.013 min
Response: 45133
Conc: 47.22 ng/ml

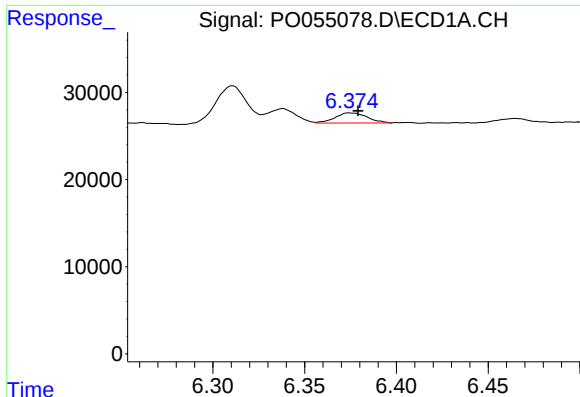

#20 AR-1242-5


R.T.: 6.375 min
Delta R.T.: -0.004 min
Response: 14244
Conc: 11.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

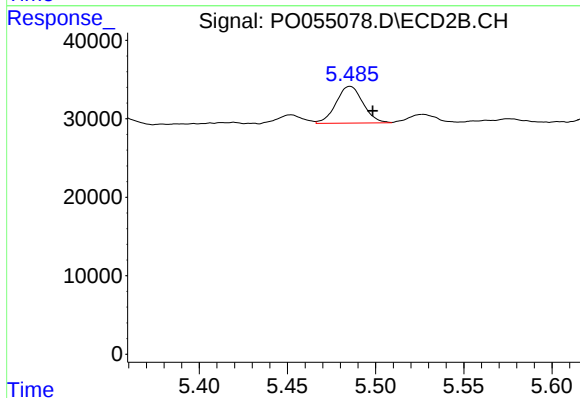


#20 AR-1242-5

R.T.: 5.486 min
Delta R.T.: -0.013 min
Response: 49852
Conc: 40.53 ng/ml

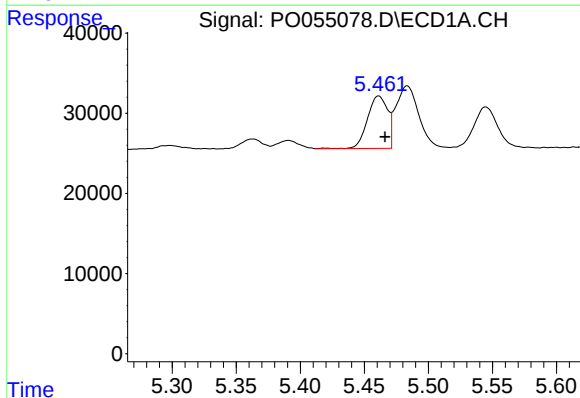


#21 AR-1248-1

R.T.: 5.461 min
Delta R.T.: -0.005 min
Response: 71536
Conc: 71.56 ng/ml

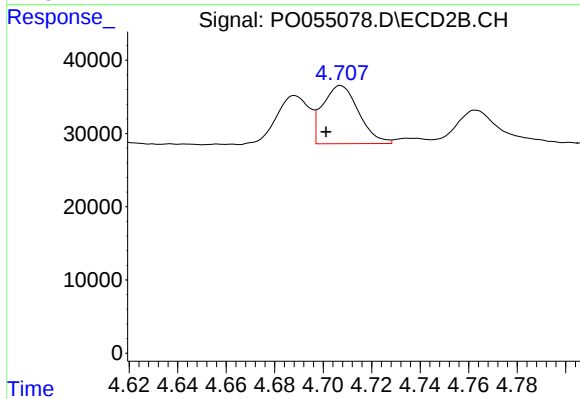

#21 AR-1248-1


R.T.: 4.707 min
Delta R.T.: 0.006 min
Response: 82032
Conc: 93.45 ng/ml

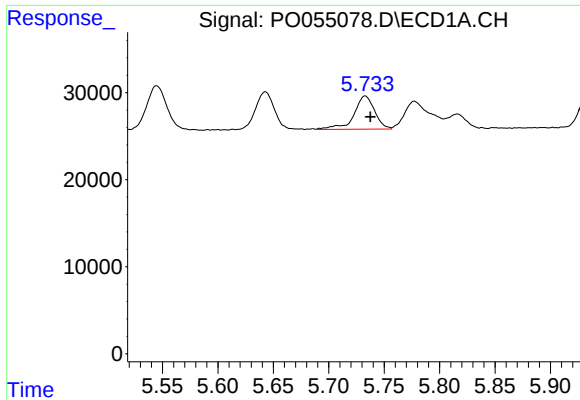

#22 AR-1248-2


R.T.: 5.733 min
Delta R.T.: -0.005 min
Response: 49687
Conc: 34.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

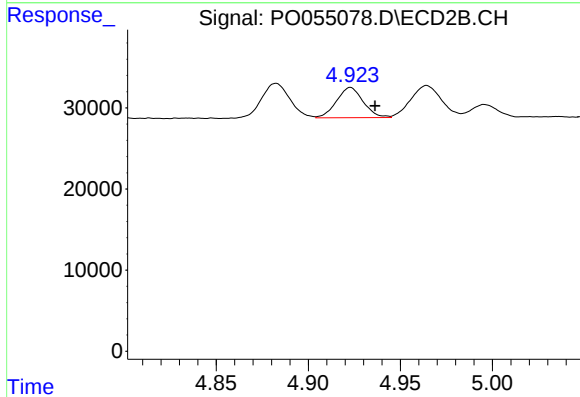


#22 AR-1248-2

R.T.: 4.923 min
Delta R.T.: -0.013 min
Response: 37321
Conc: 30.88 ng/ml

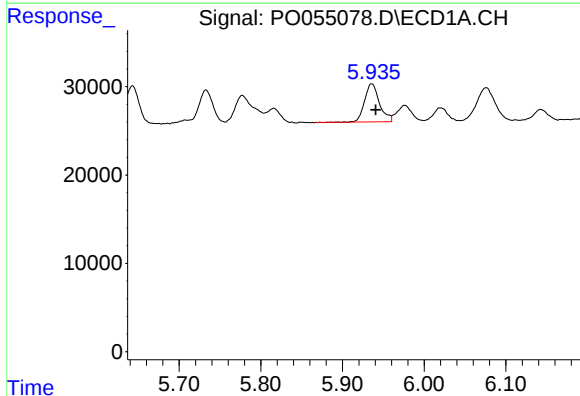


#23 AR-1248-3

R.T.: 5.936 min
Delta R.T.: -0.005 min
Response: 54804
Conc: 34.31 ng/ml

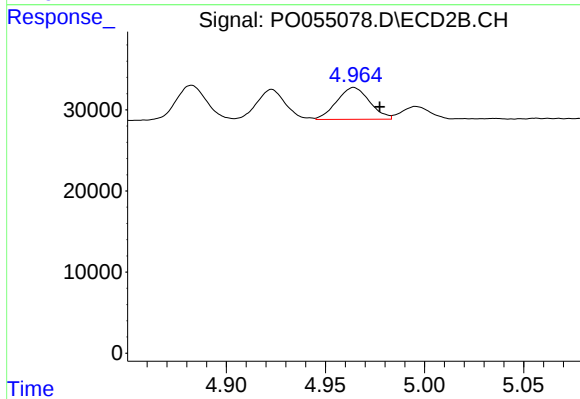

#23 AR-1248-3


R.T.: 4.964 min
Delta R.T.: -0.013 min
Response: 45133
Conc: 36.17 ng/ml

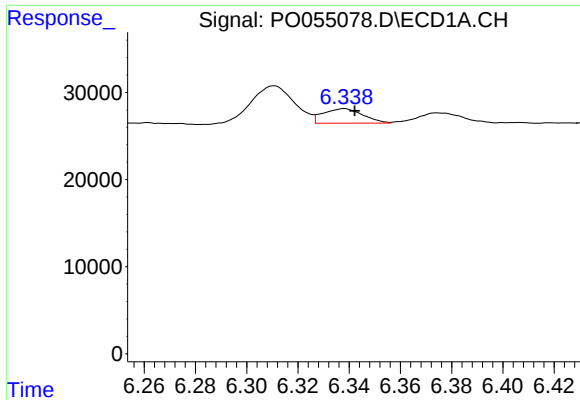

#24 AR-1248-4


R.T.: 6.338 min
Delta R.T.: -0.004 min
Response: 18034
Conc: 9.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

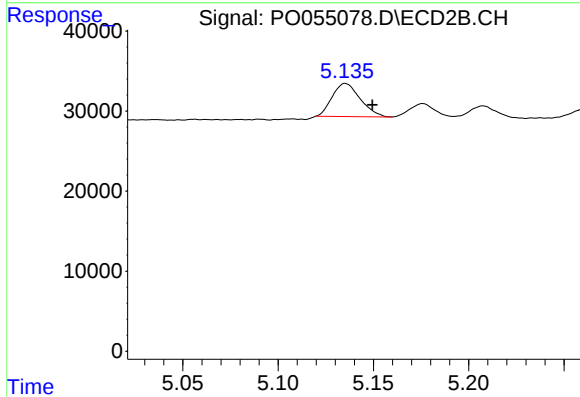


#24 AR-1248-4

R.T.: 5.135 min
Delta R.T.: -0.014 min
Response: 42349
Conc: 27.81 ng/ml

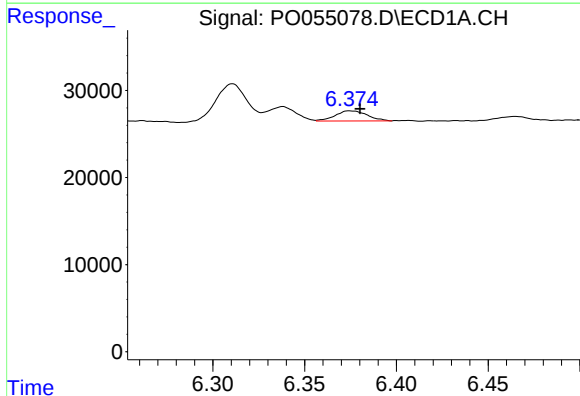


#25 AR-1248-5

R.T.: 6.375 min
Delta R.T.: -0.005 min
Response: 14244
Conc: 7.95 ng/ml

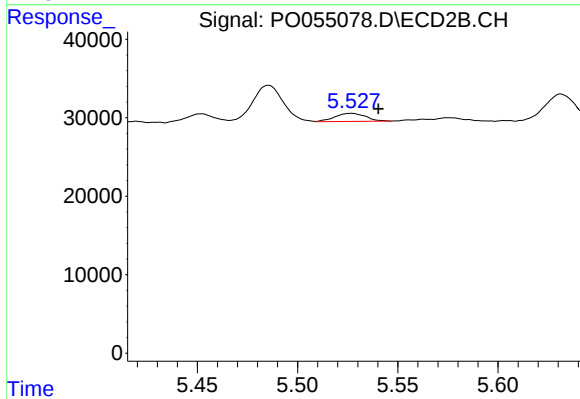

#25 AR-1248-5


R.T.: 5.527 min
Delta R.T.: -0.014 min
Response: 10852
Conc: 7.28 ng/ml

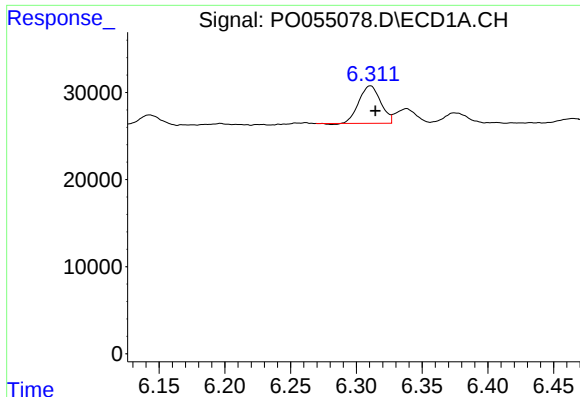

#26 AR-1254-1


R.T.: 6.311 min
Delta R.T.: -0.004 min
Response: 49388
Conc: 27.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

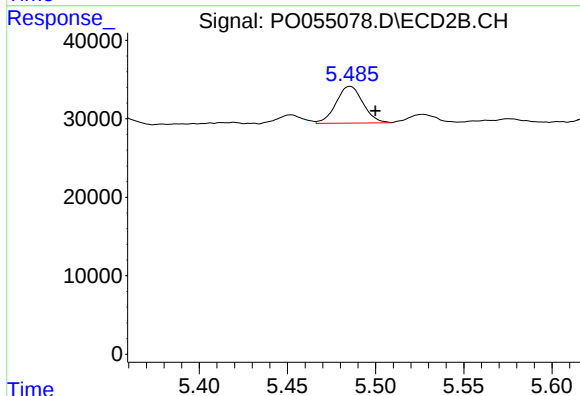


#26 AR-1254-1

R.T.: 5.486 min
Delta R.T.: -0.014 min
Response: 49852
Conc: 22.81 ng/ml

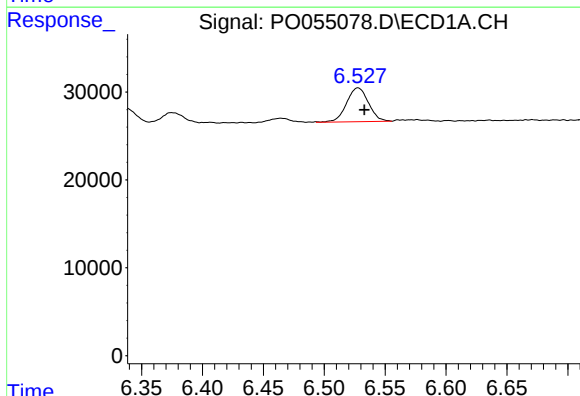


#27 AR-1254-2

R.T.: 6.528 min
Delta R.T.: -0.005 min
Response: 48325
Conc: 16.93 ng/ml

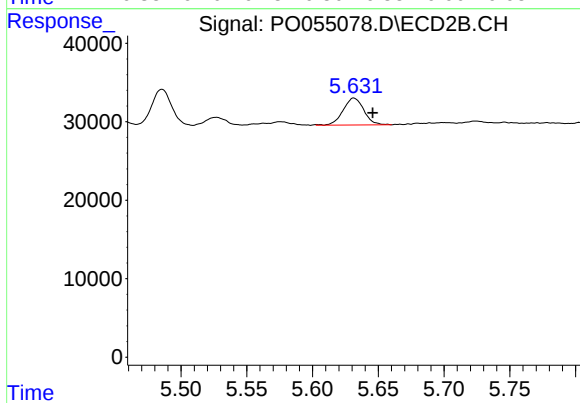

#27 AR-1254-2


R.T.: 5.631 min
Delta R.T.: -0.014 min
Response: 37952
Conc: 19.57 ng/ml

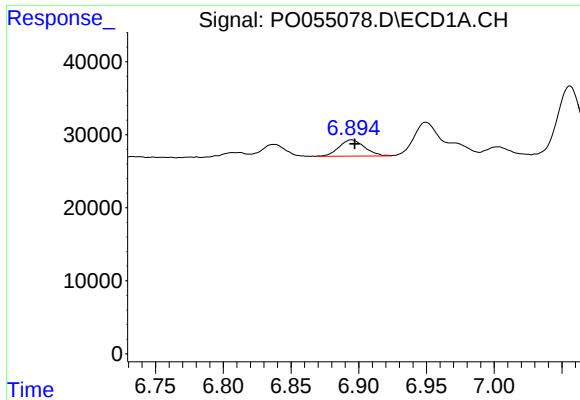

#28 AR-1254-3


R.T.: 6.895 min
Delta R.T.: -0.003 min
Response: 29346
Conc: 9.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

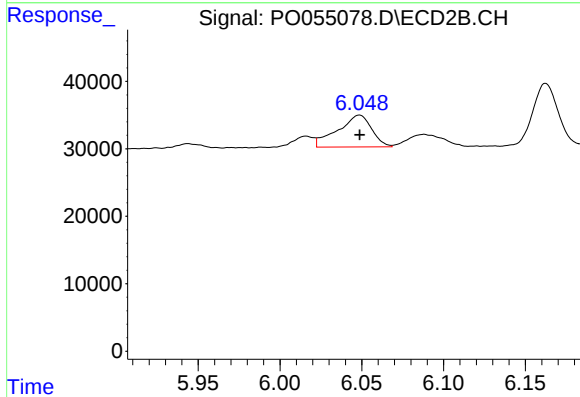


#28 AR-1254-3

R.T.: 6.049 min
Delta R.T.: 0.000 min
Response: 68360
Conc: 21.32 ng/ml

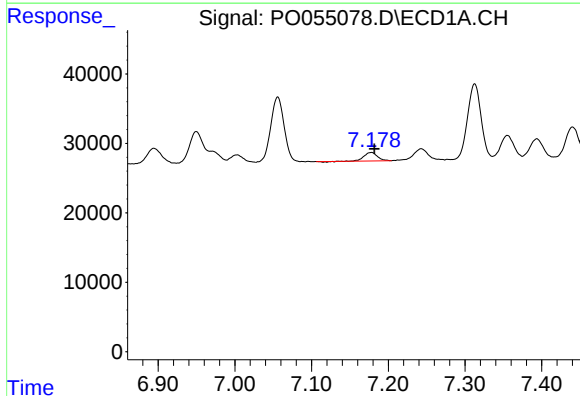


#29 AR-1254-4

R.T.: 7.178 min
Delta R.T.: -0.004 min
Response: 14774
Conc: 6.04 ng/ml

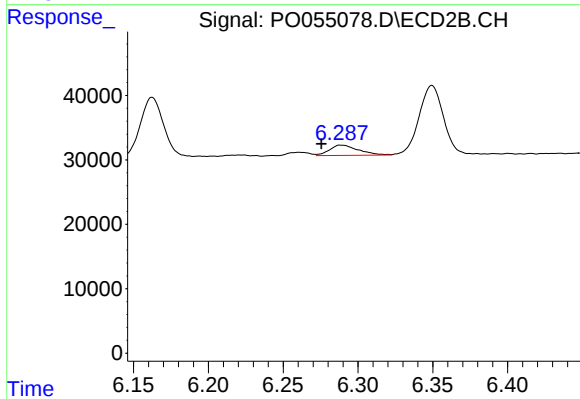

#29 AR-1254-4


R.T.: 6.289 min
Delta R.T.: 0.013 min
Response: 21739
Conc: 11.10 ng/ml

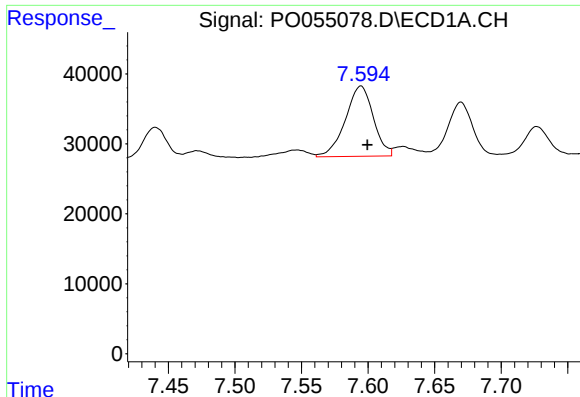

#30 AR-1254-5


R.T.: 7.595 min
Delta R.T.: -0.005 min
Response: 147036
Conc: 54.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

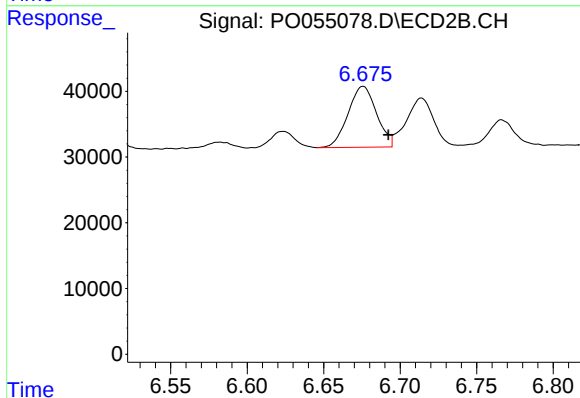


#30 AR-1254-5

R.T.: 6.676 min
Delta R.T.: -0.016 min
Response: 120017
Conc: 41.75 ng/ml

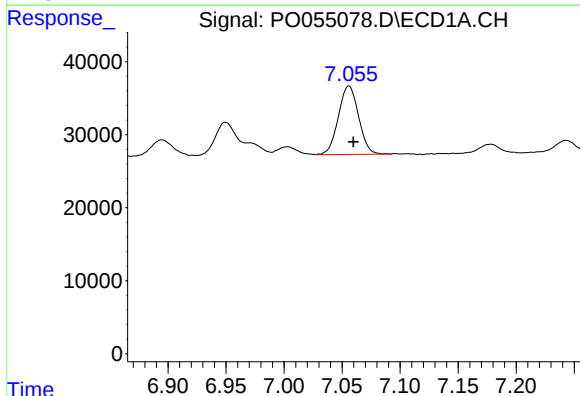


#31 AR-1260-1

R.T.: 7.056 min
Delta R.T.: -0.004 min
Response: 113569
Conc: 45.20 ng/ml

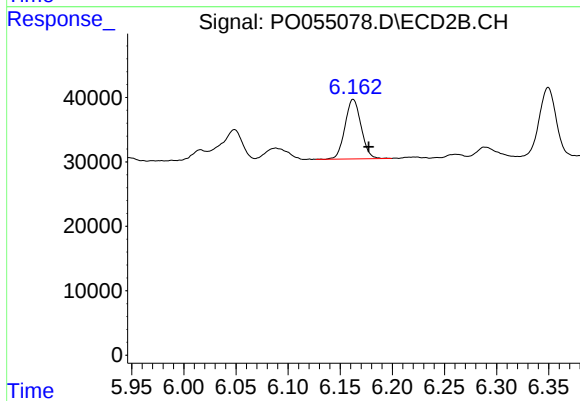

#31 AR-1260-1


R.T.: 6.162 min
Delta R.T.: -0.015 min
Response: 99436
Conc: 43.27 ng/ml

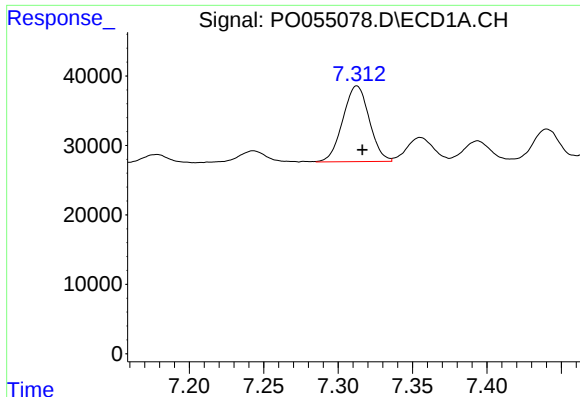

#32 AR-1260-2


R.T.: 7.313 min
Delta R.T.: -0.004 min
Response: 134693
Conc: 43.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

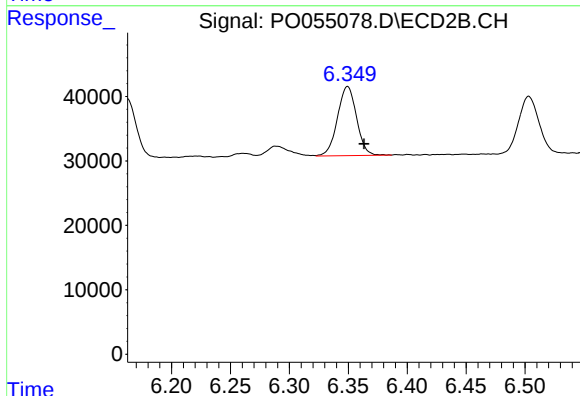


#32 AR-1260-2

R.T.: 6.349 min
Delta R.T.: -0.014 min
Response: 121238
Conc: 44.04 ng/ml

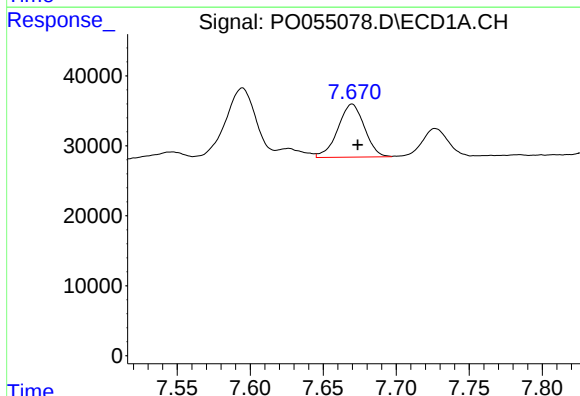


#33 AR-1260-3

R.T.: 7.670 min
Delta R.T.: -0.004 min
Response: 96067
Conc: 39.14 ng/ml

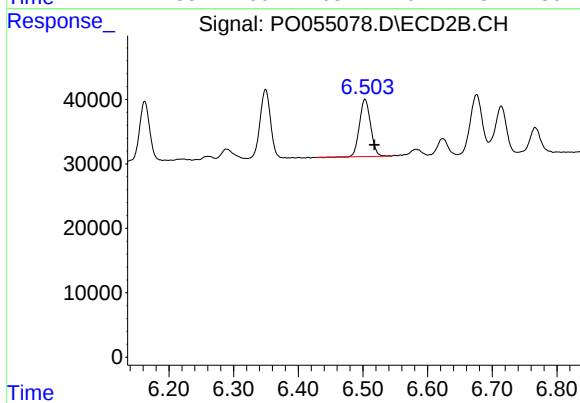

#33 AR-1260-3


R.T.: 6.503 min
Delta R.T.: -0.015 min
Response: 107116
Conc: 41.55 ng/ml

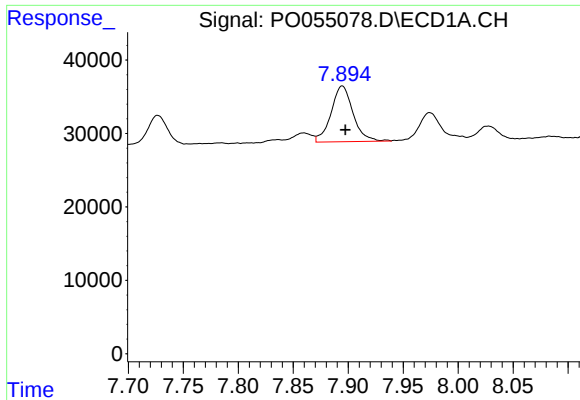

#34 AR-1260-4


R.T.: 7.895 min
Delta R.T.: -0.003 min
Response: 105597
Conc: 38.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

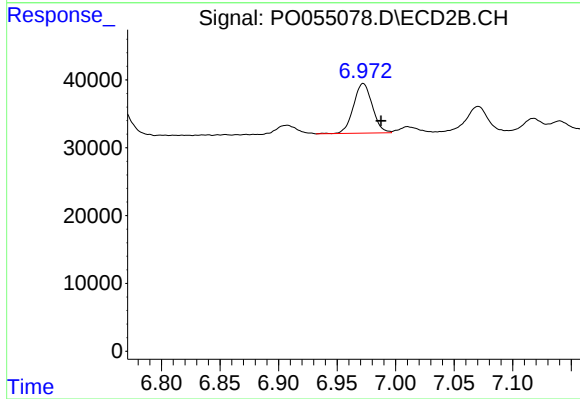


#34 AR-1260-4

R.T.: 6.972 min
Delta R.T.: -0.015 min
Response: 81915
Conc: 38.49 ng/ml

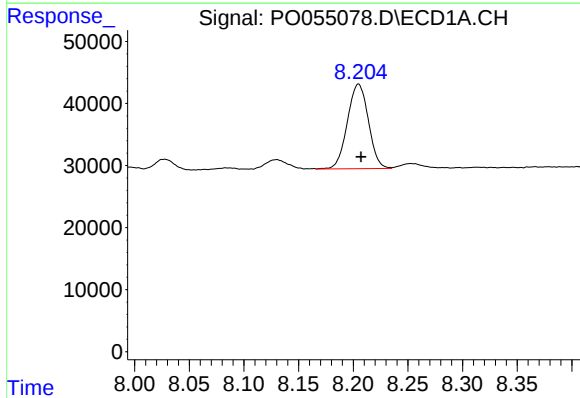


#35 AR-1260-5

R.T.: 8.205 min
Delta R.T.: -0.002 min
Response: 182467
Conc: 32.89 ng/ml

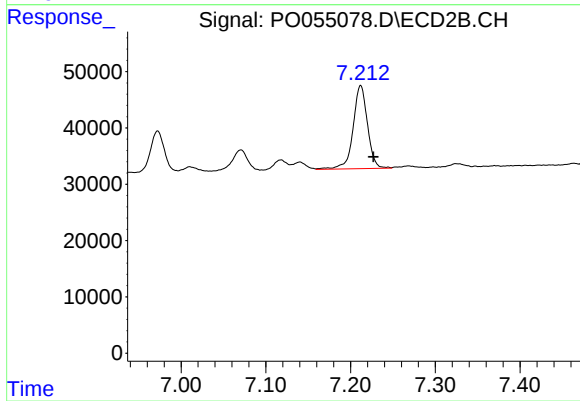

#35 AR-1260-5


R.T.: 7.212 min
Delta R.T.: -0.015 min
Response: 174654
Conc: 36.47 ng/ml

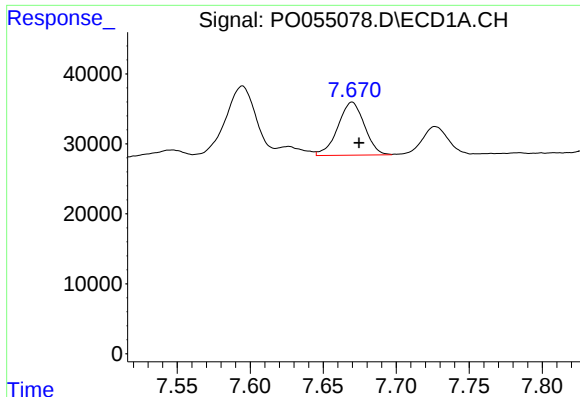

#36 AR-1262-1


R.T.: 7.670 min
Delta R.T.: -0.005 min
Response: 96067
Conc: 28.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

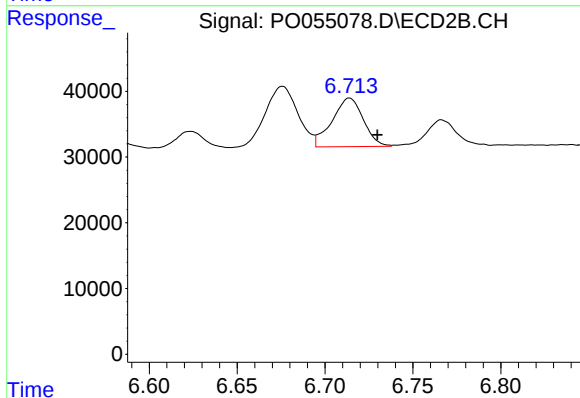


#36 AR-1262-1

R.T.: 6.714 min
Delta R.T.: -0.016 min
Response: 91653
Conc: 30.81 ng/ml

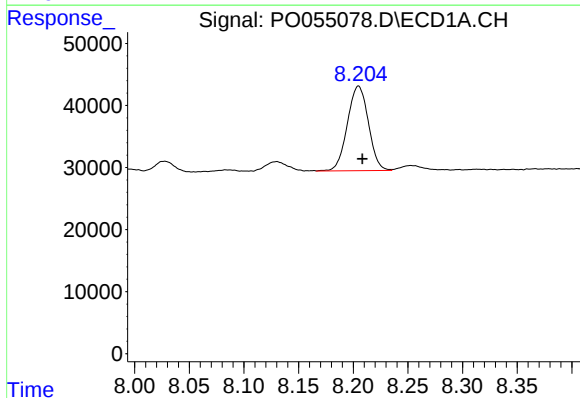


#37 AR-1262-2

R.T.: 8.205 min
Delta R.T.: -0.004 min
Response: 182467
Conc: 30.80 ng/ml

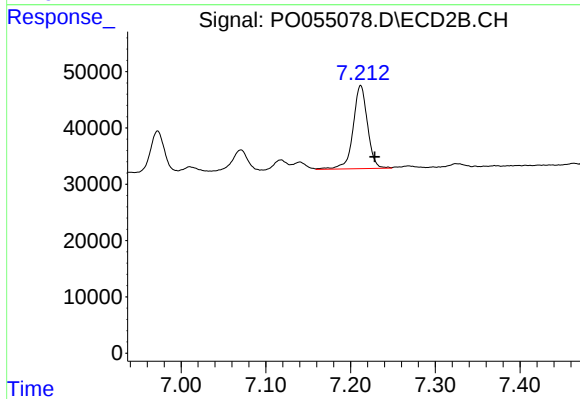

#37 AR-1262-2


R.T.: 7.212 min
Delta R.T.: -0.017 min
Response: 174654
Conc: 35.64 ng/ml

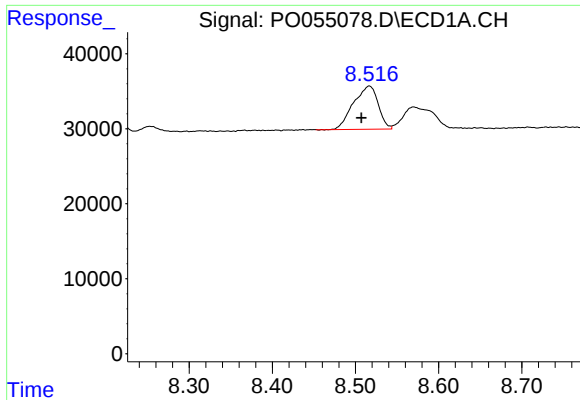

#38 AR-1262-3


R.T.: 8.517 min
Delta R.T.: 0.010 min
Response: 119164
Conc: 28.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

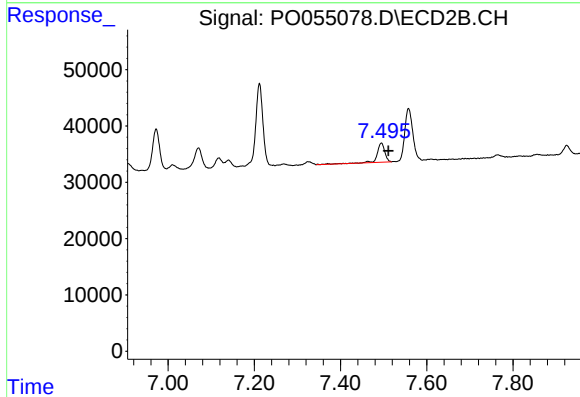


#38 AR-1262-3

R.T.: 7.495 min
Delta R.T.: -0.016 min
Response: 41487
Conc: 20.20 ng/ml

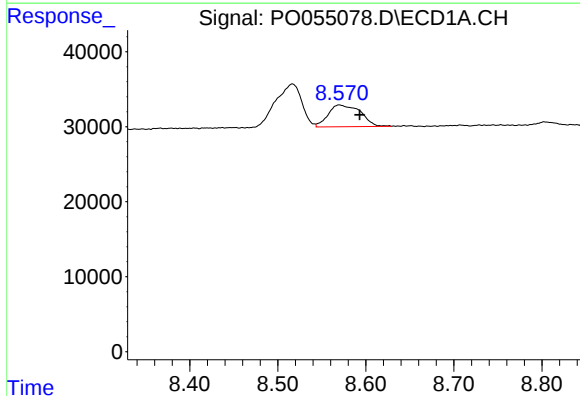


#39 AR-1262-4

R.T.: 8.570 min
Delta R.T.: -0.023 min
Response: 74179
Conc: 23.02 ng/ml

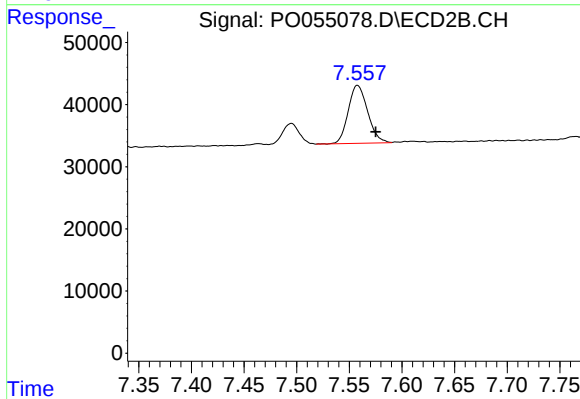

#39 AR-1262-4


R.T.: 7.558 min
Delta R.T.: -0.017 min
Response: 120249
Conc: 33.20 ng/ml

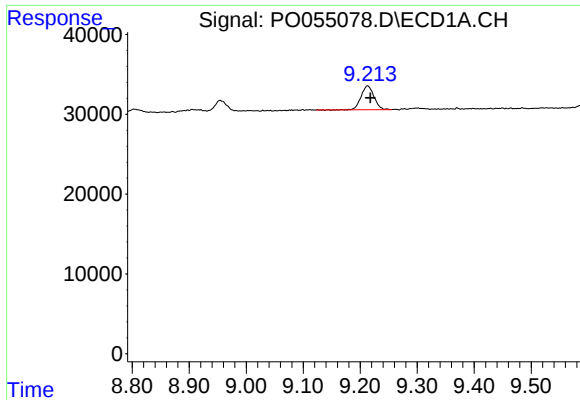

#40 AR-1262-5


R.T.: 9.213 min
Delta R.T.: -0.005 min
Response: 46676
Conc: 21.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

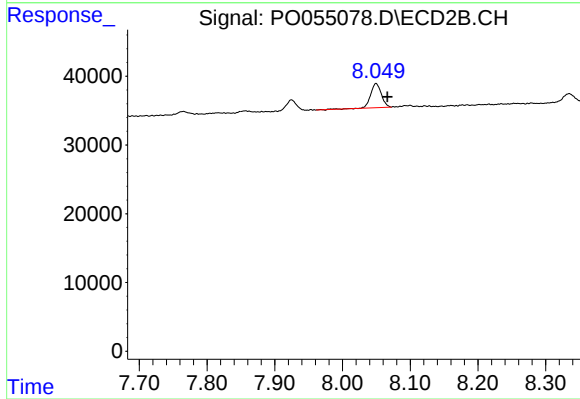


#40 AR-1262-5

R.T.: 8.050 min
Delta R.T.: -0.017 min
Response: 38519
Conc: 23.87 ng/ml

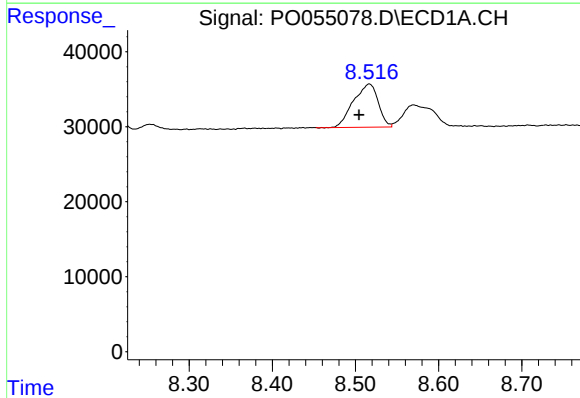


#41 AR-1268-1

R.T.: 8.517 min
Delta R.T.: 0.012 min
Response: 119164
Conc: 16.74 ng/ml

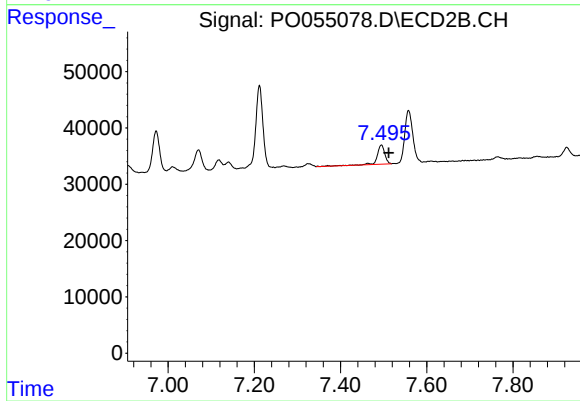

#41 AR-1268-1


R.T.: 7.495 min
Delta R.T.: -0.016 min
Response: 41487
Conc: 7.34 ng/ml

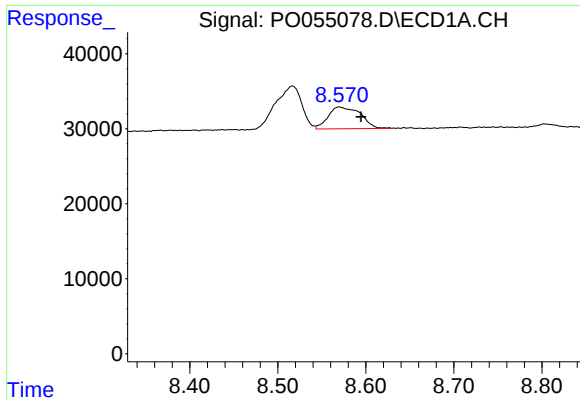

#42 AR-1268-2


R.T.: 8.570 min
Delta R.T.: -0.024 min
Response: 74179
Conc: 11.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

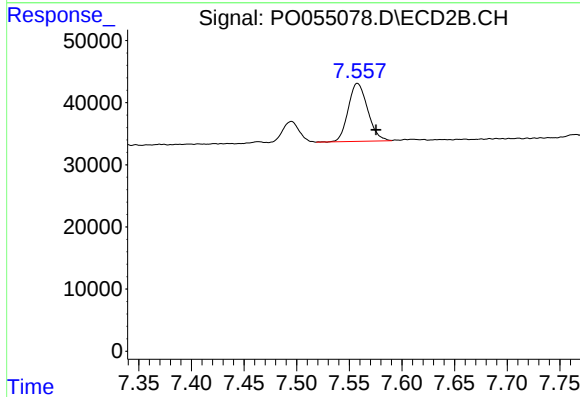


#42 AR-1268-2

R.T.: 7.558 min
Delta R.T.: -0.017 min
Response: 120249
Conc: 23.25 ng/ml

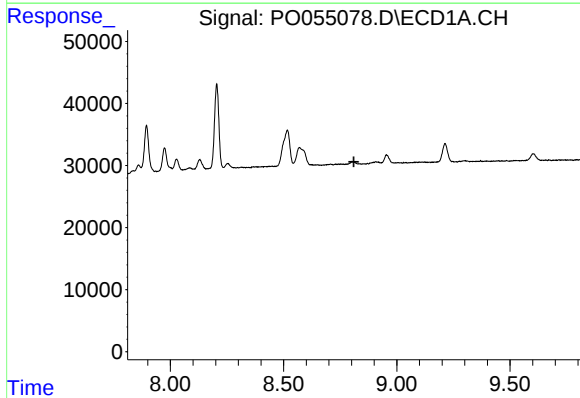


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.810 min
Response: 0
Conc: N.D.

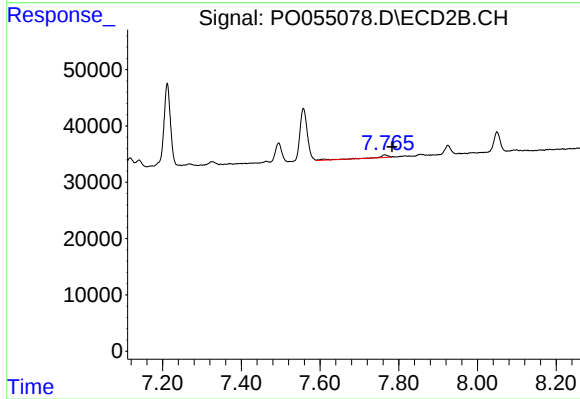

#43 AR-1268-3


R.T.: 7.765 min
Delta R.T.: -0.018 min
Response: 9064
Conc: 2.11 ng/ml

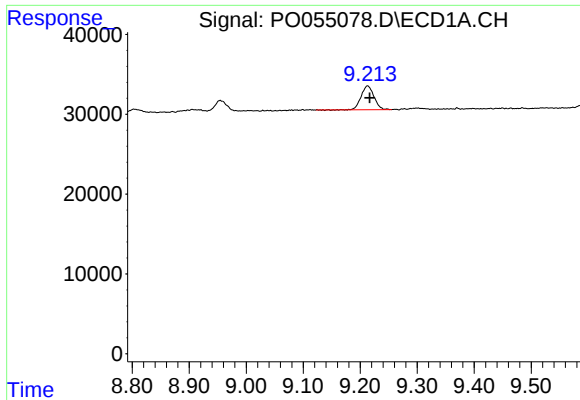

#44 AR-1268-4


R.T.: 9.213 min
Delta R.T.: -0.004 min
Response: 46676
Conc: 19.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

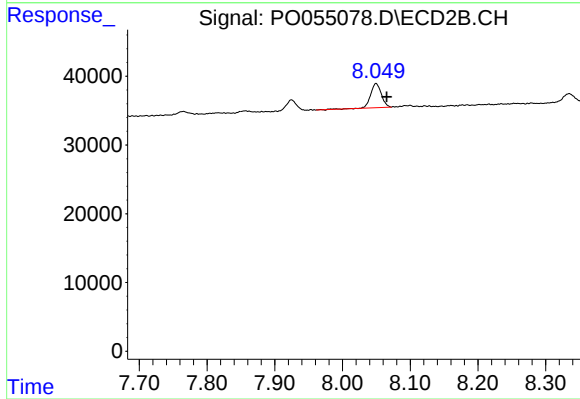


#44 AR-1268-4

R.T.: 8.050 min
Delta R.T.: -0.016 min
Response: 38519
Conc: 20.78 ng/ml

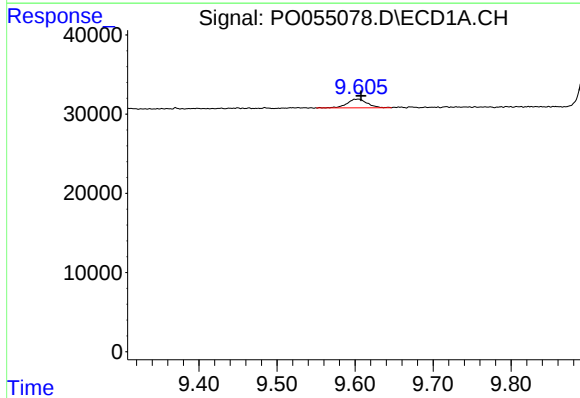

#45 AR-1268-5

R.T.: 9.604 min
Delta R.T.: -0.004 min
Response: 19429
Conc: 1.18 ng/ml

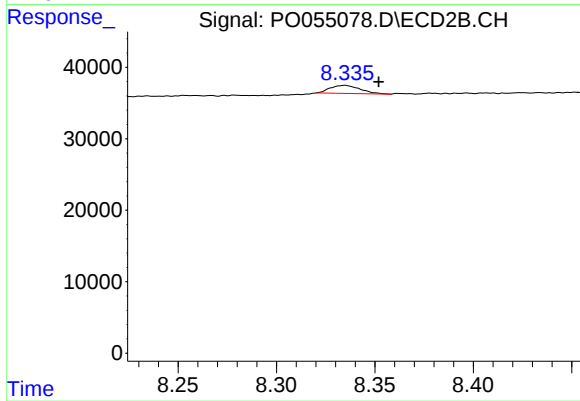

#45 AR-1268-5

R.T.: 8.335 min
Delta R.T.: -0.017 min
Response: 11924
Conc: 1.05 ng/ml