

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040919\
 Data File : P0055079.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Apr 2019 16:42
 Operator : SM/SJ
 Sample : K1560-09
 Misc : AR1221 MDL 100PPB
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: 01 Apr 10 07:00:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.299	3.611	860597	786634	24.797	24.650
2) SA Decachlor...	9.919	8.584	1016751	724276	20.625	22.741
Target Compounds						
8) L2 AR-1221-1	4.509	3.824	30958	25584	70.912	65.805
9) L2 AR-1221-2	4.597	3.909	34034	28600	100.361	95.400
10) L2 AR-1221-3	4.670	3.984	76089	61461	73.249	66.676



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040919\
Data File : P0055079.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Apr 2019 16:42
Operator : SM/SJ
Sample : K1560-09
Misc : AR1221 MDL 100PPB
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 07:00:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

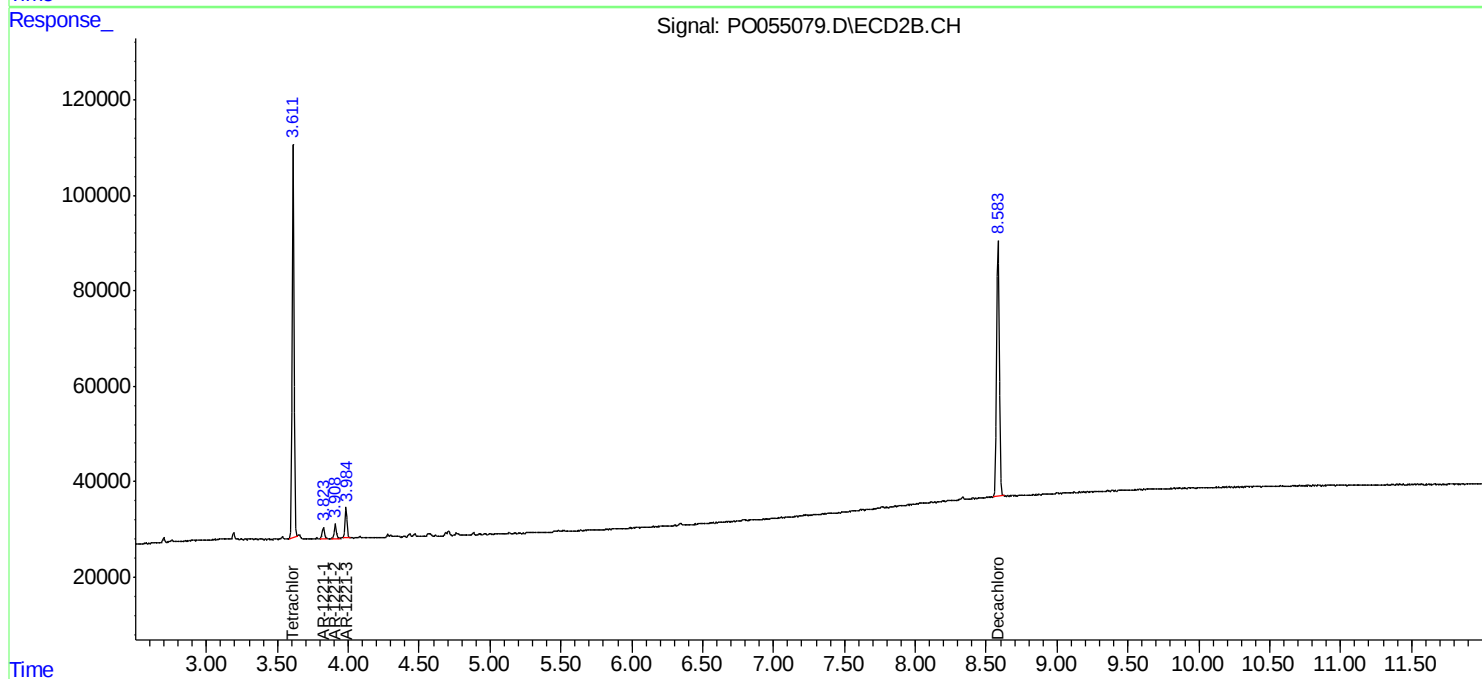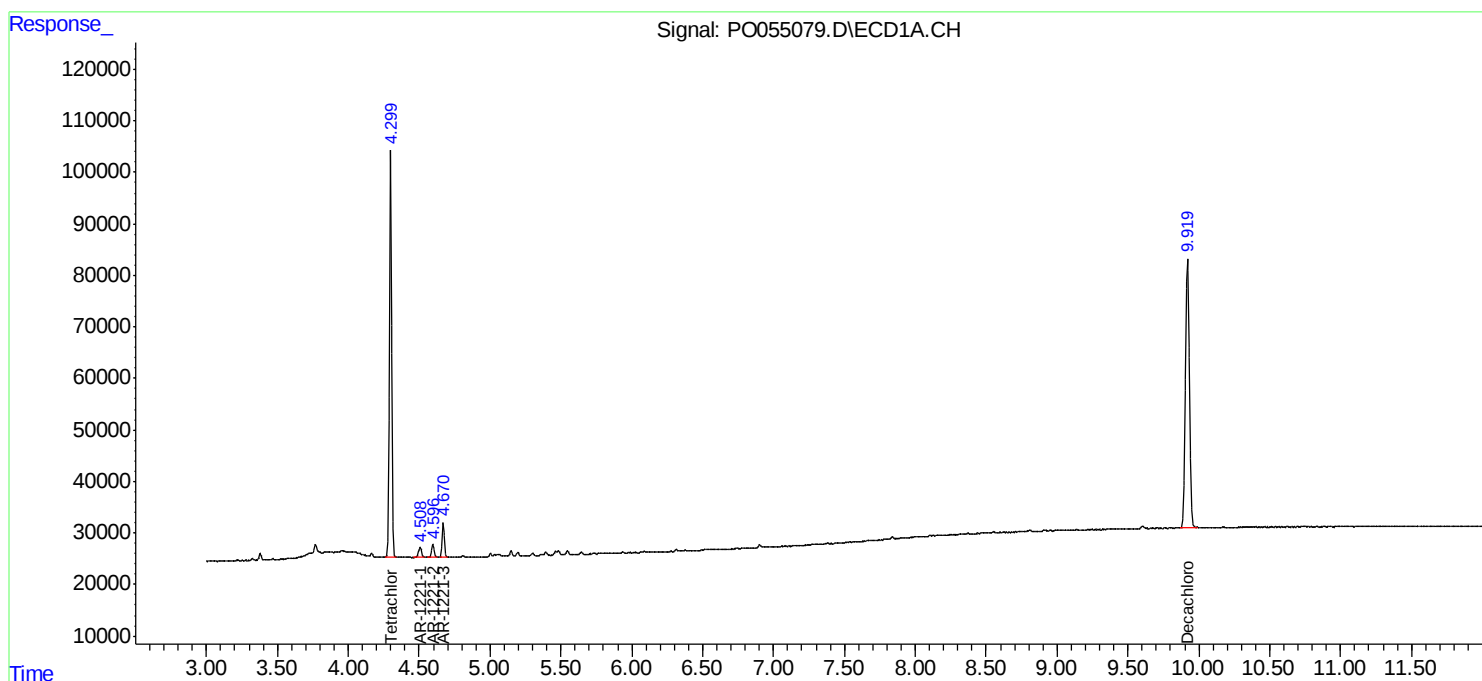


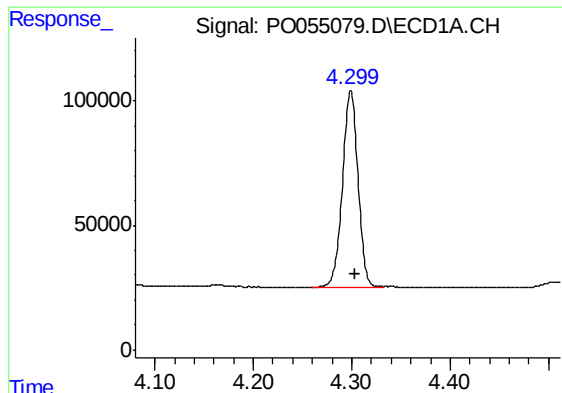

#1 Tetrachloro-m-xylene


R.T.: 4.299 min
Delta R.T.: -0.004 min
Response: 860597
Conc: 24.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

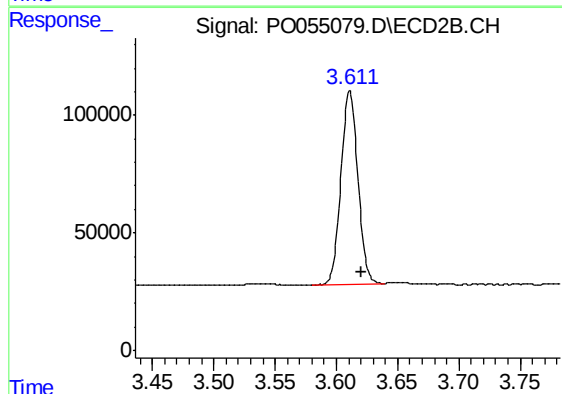


#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: -0.010 min
Response: 786634
Conc: 24.65 ng/ml

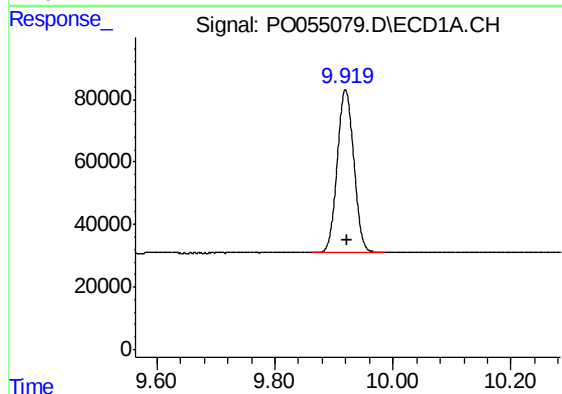


#2 Decachlorobiphenyl

R.T.: 9.919 min
Delta R.T.: -0.004 min
Response: 1016751
Conc: 20.62 ng/ml

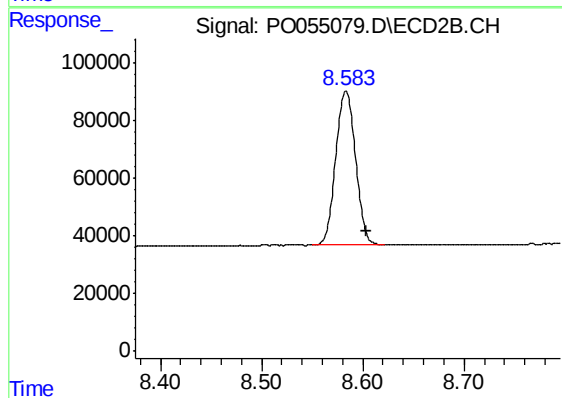

#2 Decachlorobiphenyl


R.T.: 8.584 min
Delta R.T.: -0.021 min
Response: 724276
Conc: 22.74 ng/ml

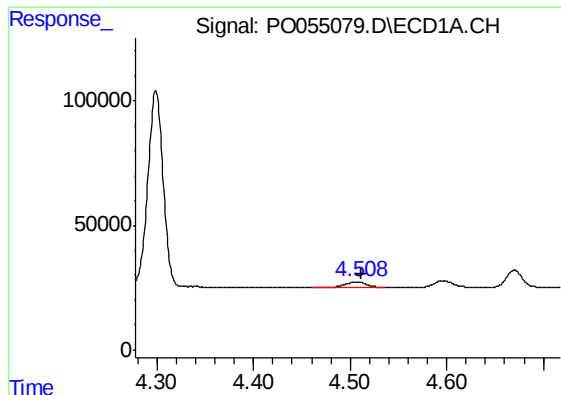

#8 AR-1221-1


R.T.: 4.509 min
Delta R.T.: -0.003 min
Response: 30958
Conc: 70.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

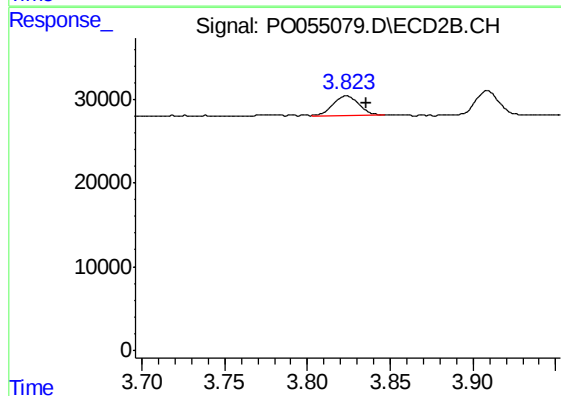


#8 AR-1221-1

R.T.: 3.824 min
Delta R.T.: -0.012 min
Response: 25584
Conc: 65.80 ng/ml

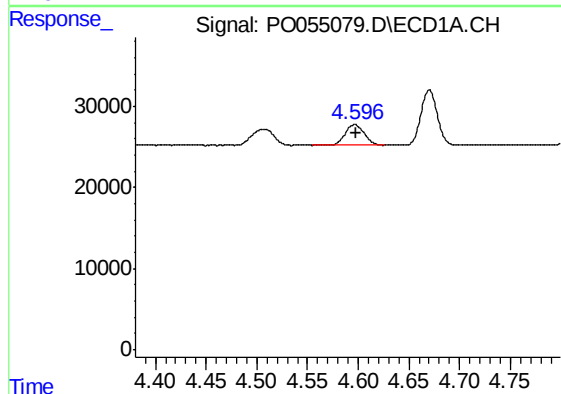


#9 AR-1221-2

R.T.: 4.597 min
Delta R.T.: -0.001 min
Response: 34034
Conc: 100.36 ng/ml

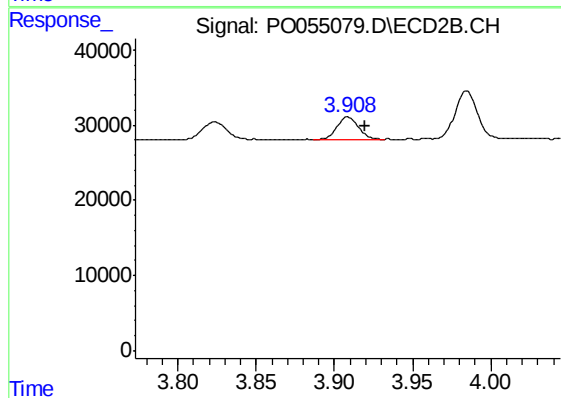

#9 AR-1221-2


R.T.: 3.909 min
Delta R.T.: -0.011 min
Response: 28600
Conc: 95.40 ng/ml

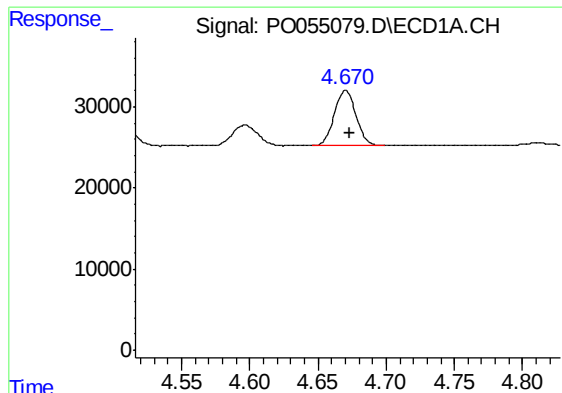

#10 AR-1221-3

R.T.: 4.670 min
Delta R.T.: -0.003 min
Response: 76089
Conc: 73.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

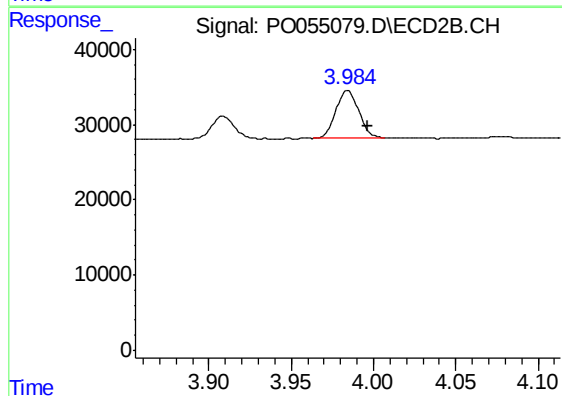

#10 AR-1221-3

R.T.: 3.984 min
Delta R.T.: -0.012 min
Response: 61461
Conc: 66.68 ng/ml