

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040919\
 Data File : P0055081.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Apr 2019 17:16
 Operator : SM/SJ
 Sample : K1560-09
 Misc : AR1242 MDL 100PPB
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Manual Integrations
 APPROVED

mohammad
 4/10/2019 4:01:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 07:04:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.299	3.611	899582	840840	25.921	26.348
2)	SA Decachlor...	9.919	8.583	1054648	757615	21.394	23.788
Target Compounds							
16)	L4 AR-1242-1	5.461	4.687	51615	45132	37.152	36.761m
17)	L4 AR-1242-2	5.484	4.706	70415	58685	36.800	35.412m
18)	L4 AR-1242-3	5.545	4.881	49849	33777	40.219	35.655
19)	L4 AR-1242-4	5.643	4.964	36080	33402	35.388	34.949
20)	L4 AR-1242-5	6.375	5.484	45248	42351	37.483	34.434

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040919\
Data File : PO055081.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Apr 2019 17:16
Operator : SM/SJ
Sample : K1560-09
Misc : AR1242 MDL 100PPB
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:01:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 07:04:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

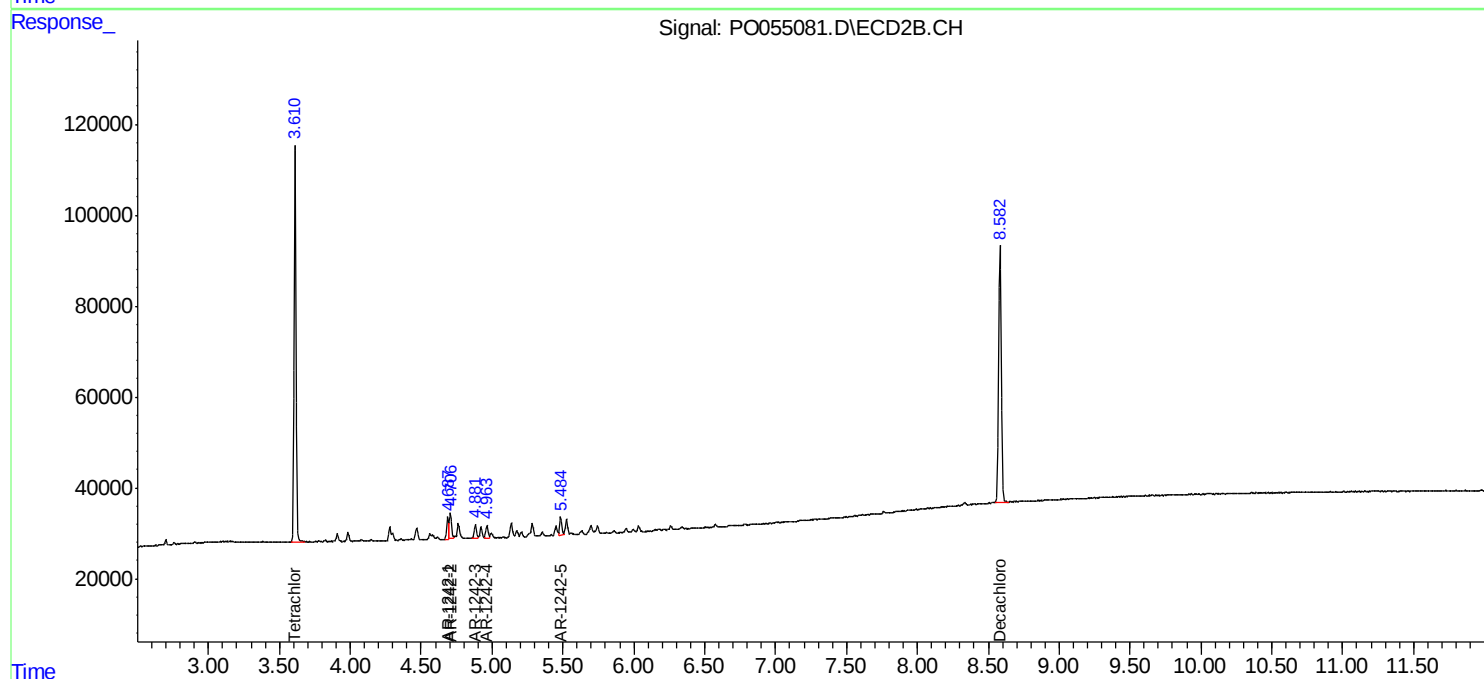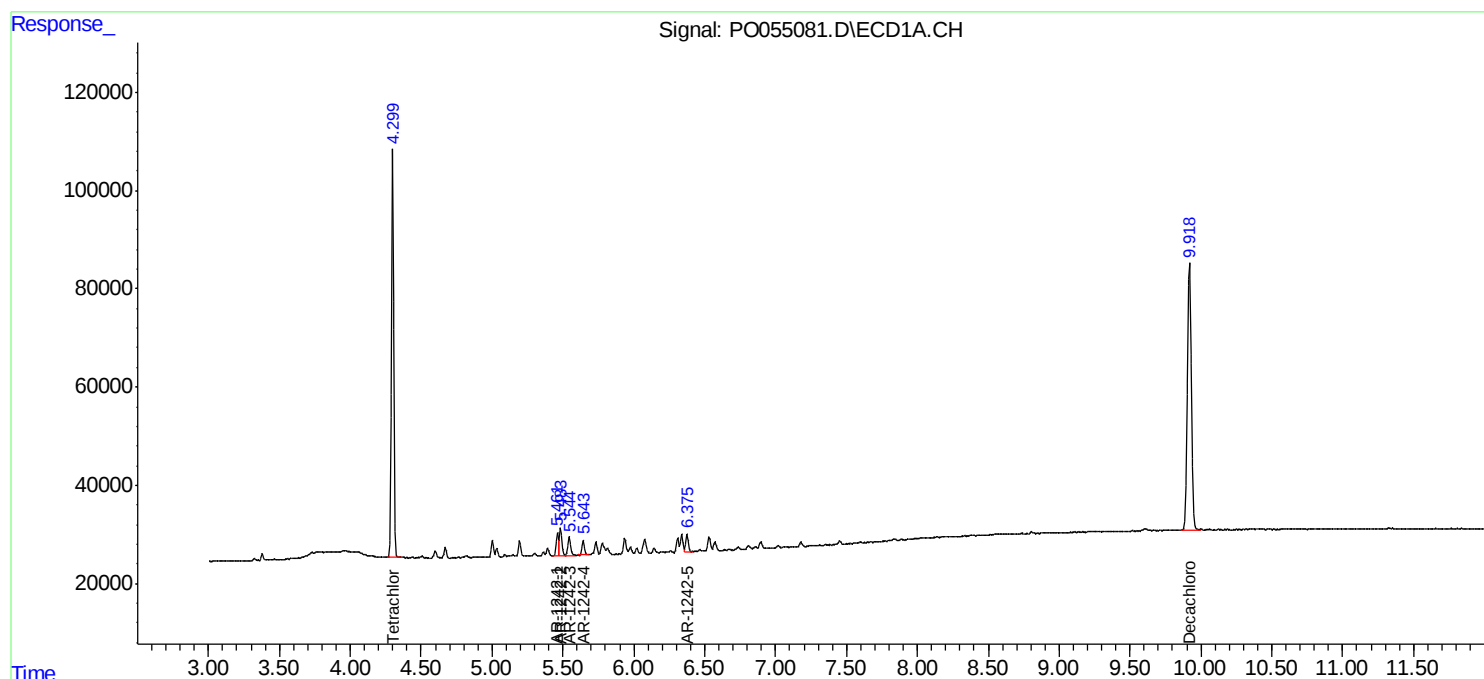

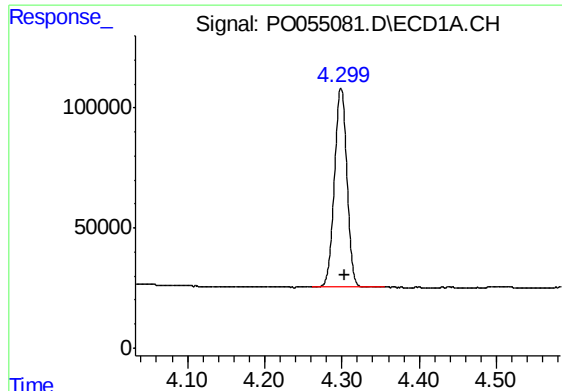


#1 Tetrachloro-m-xylene

R.T.: 4.299 min
Delta R.T.: -0.004 min
Response: 899582
Conc: 25.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:01:51 PM

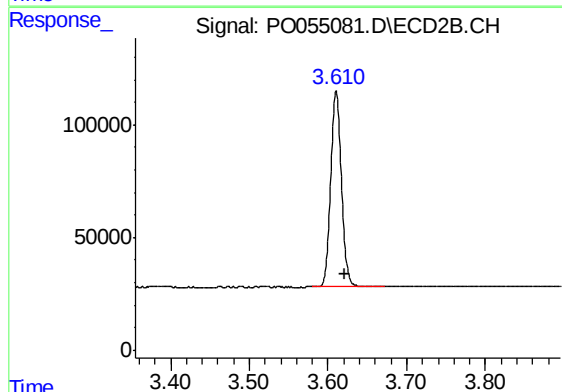


#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: -0.010 min
Response: 840840
Conc: 26.35 ng/ml

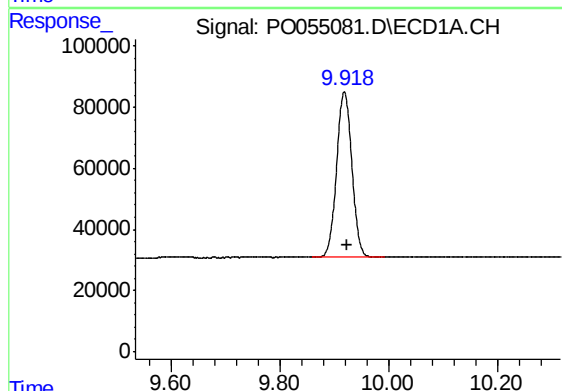


#2 Decachlorobiphenyl

R.T.: 9.919 min
Delta R.T.: -0.004 min
Response: 1054648
Conc: 21.39 ng/ml

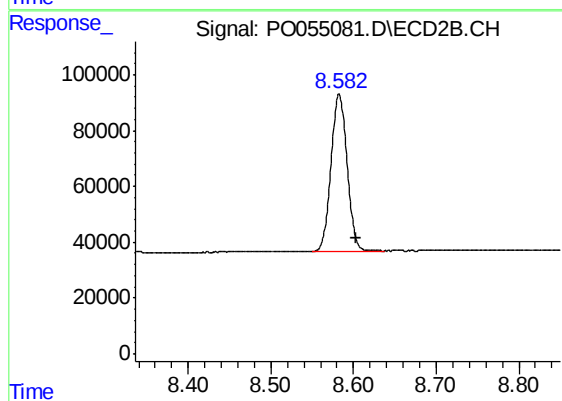

#2 Decachlorobiphenyl

R.T.: 8.583 min
Delta R.T.: -0.022 min
Response: 757615
Conc: 23.79 ng/ml

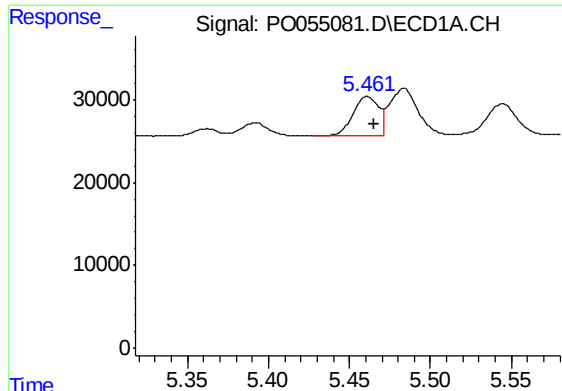


#16 AR-1242-1

R.T.: 5.461 min
Delta R.T.: -0.004 min
Response: 51615
Conc: 37.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:01:51 PM

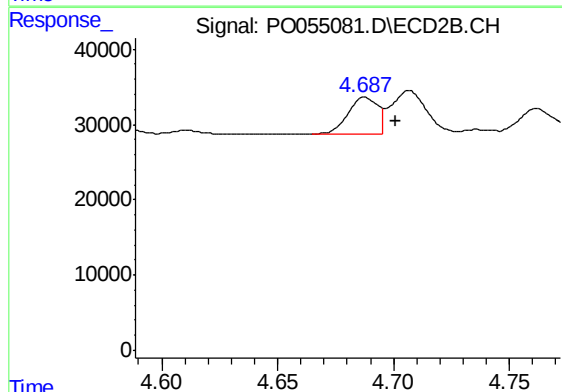


#16 AR-1242-1

R.T.: 4.687 min
Delta R.T.: -0.014 min
Response: 45132
Conc: 36.76 ng/ml m

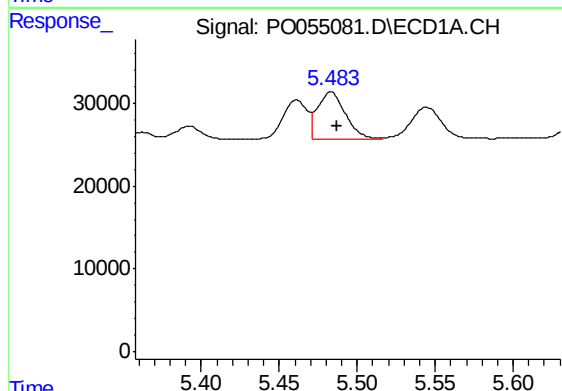


#17 AR-1242-2

R.T.: 5.484 min
Delta R.T.: -0.003 min
Response: 70415
Conc: 36.80 ng/ml

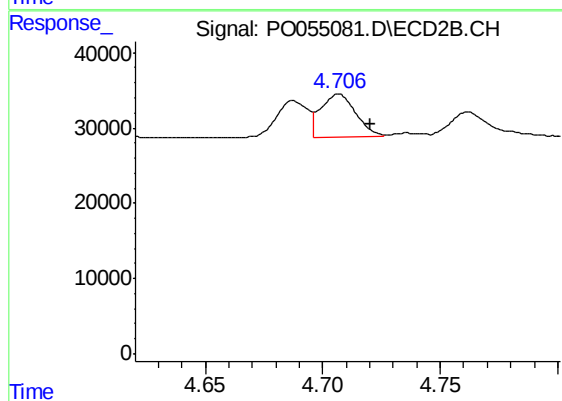

#17 AR-1242-2

R.T.: 4.706 min
Delta R.T.: -0.014 min
Response: 58685
Conc: 35.41 ng/ml m

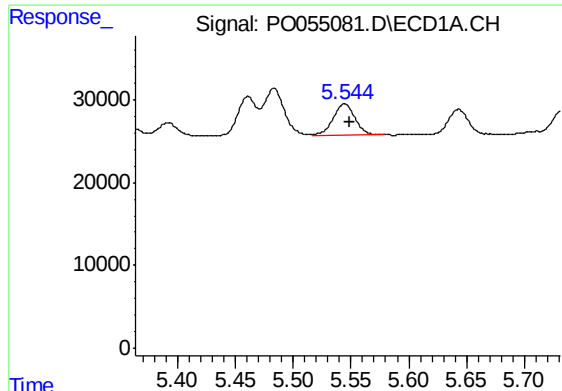


#18 AR-1242-3

R.T.: 5.545 min
Delta R.T.: -0.004 min
Response: 49849
Conc: 40.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:01:51 PM

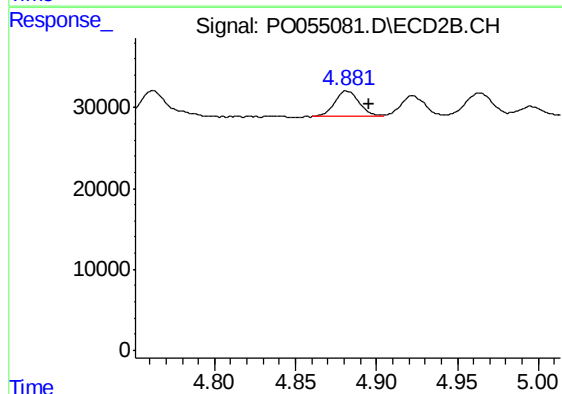


#18 AR-1242-3

R.T.: 4.881 min
Delta R.T.: -0.014 min
Response: 33777
Conc: 35.65 ng/ml

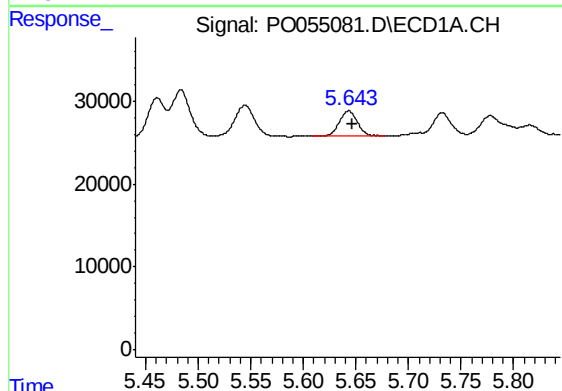


#19 AR-1242-4

R.T.: 5.643 min
Delta R.T.: -0.004 min
Response: 36080
Conc: 35.39 ng/ml

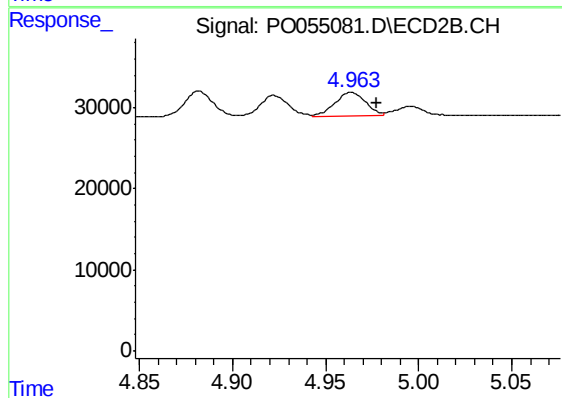

#19 AR-1242-4

R.T.: 4.964 min
Delta R.T.: -0.014 min
Response: 33402
Conc: 34.95 ng/ml

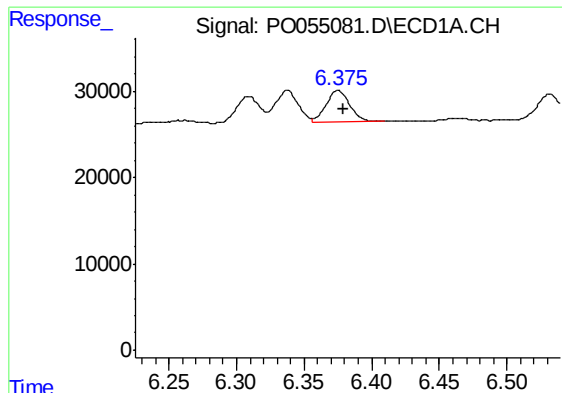


#20 AR-1242-5

R.T.: 6.375 min
Delta R.T.: -0.004 min
Response: 45248
Conc: 37.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Manual Integrations
APPROVED

mohammad
4/10/2019 4:01:51 PM

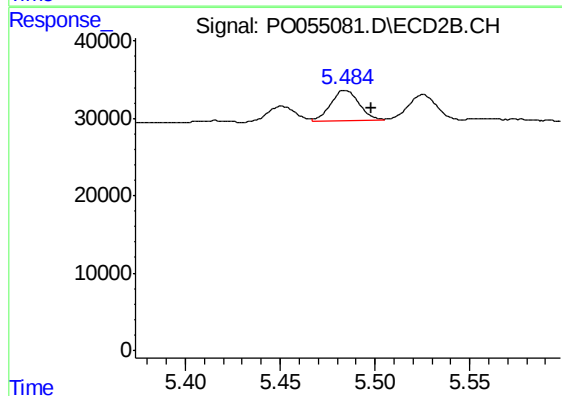

#20 AR-1242-5

R.T.: 5.484 min
Delta R.T.: -0.014 min
Response: 42351
Conc: 34.43 ng/ml