

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040919\
 Data File : P0055082.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Apr 2019 17:33
 Operator : SM/SJ
 Sample : K1560-09
 Misc : AR1248 MDL 100PPB
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Manual Integrations
 APPROVED

mohammad
 4/10/2019 4:01:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 07:06:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.300	3.611	916352	853269	26.404	26.738
2)	SA Decachlor...	9.921	8.583	1077855	773929	21.864	24.301
Target Compounds							
21)	L5 AR-1248-1	5.462	4.689	38132	34550	38.144	39.360m
22)	L5 AR-1248-2	5.733	4.922	56479	46893	38.890m	38.801
23)	L5 AR-1248-3	5.936	4.964	64720	46818	40.522	37.521
24)	L5 AR-1248-4	6.339	5.135	73478	55477	39.114	36.427m
25)	L5 AR-1248-5	6.376	5.526	68572	47900	38.249	32.129

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040919\
Data File : PO055082.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Apr 2019 17:33
Operator : SM/SJ
Sample : K1560-09
Misc : AR1248 MDL 100PPB
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:01:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 07:06:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

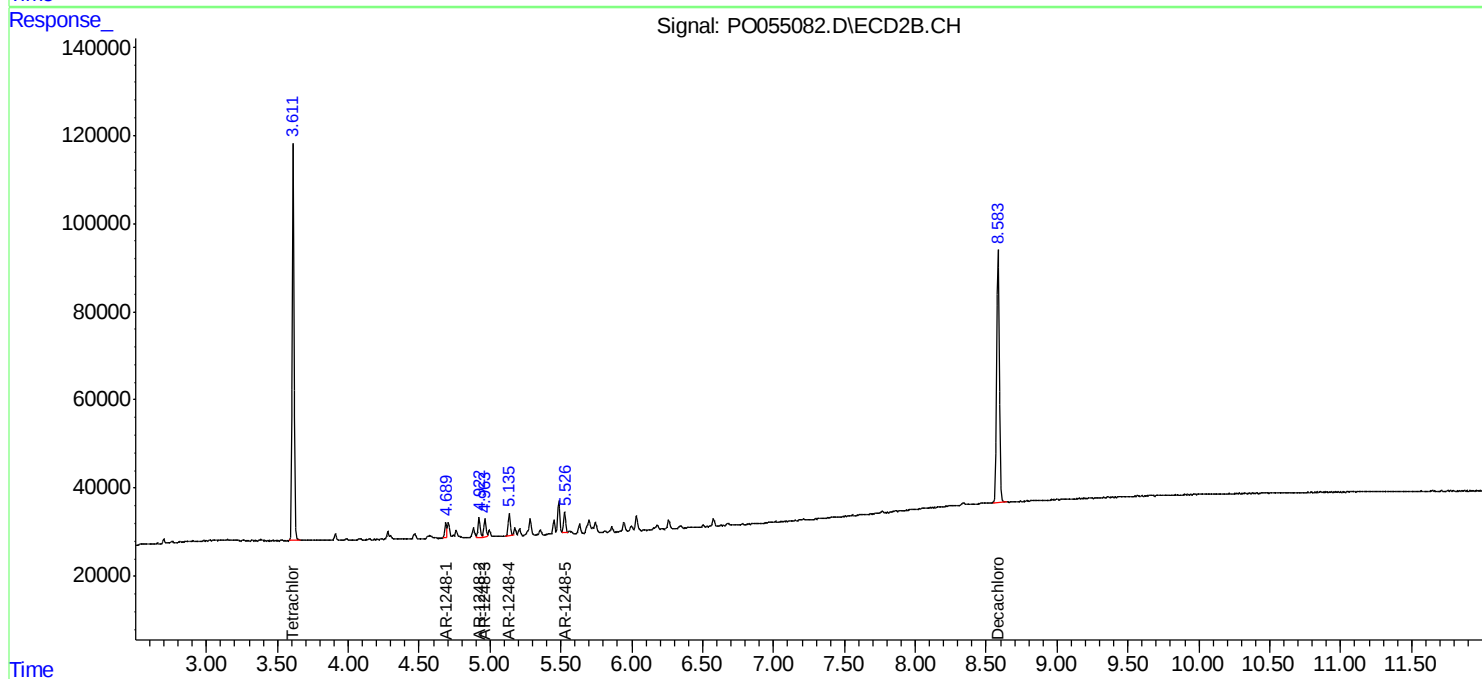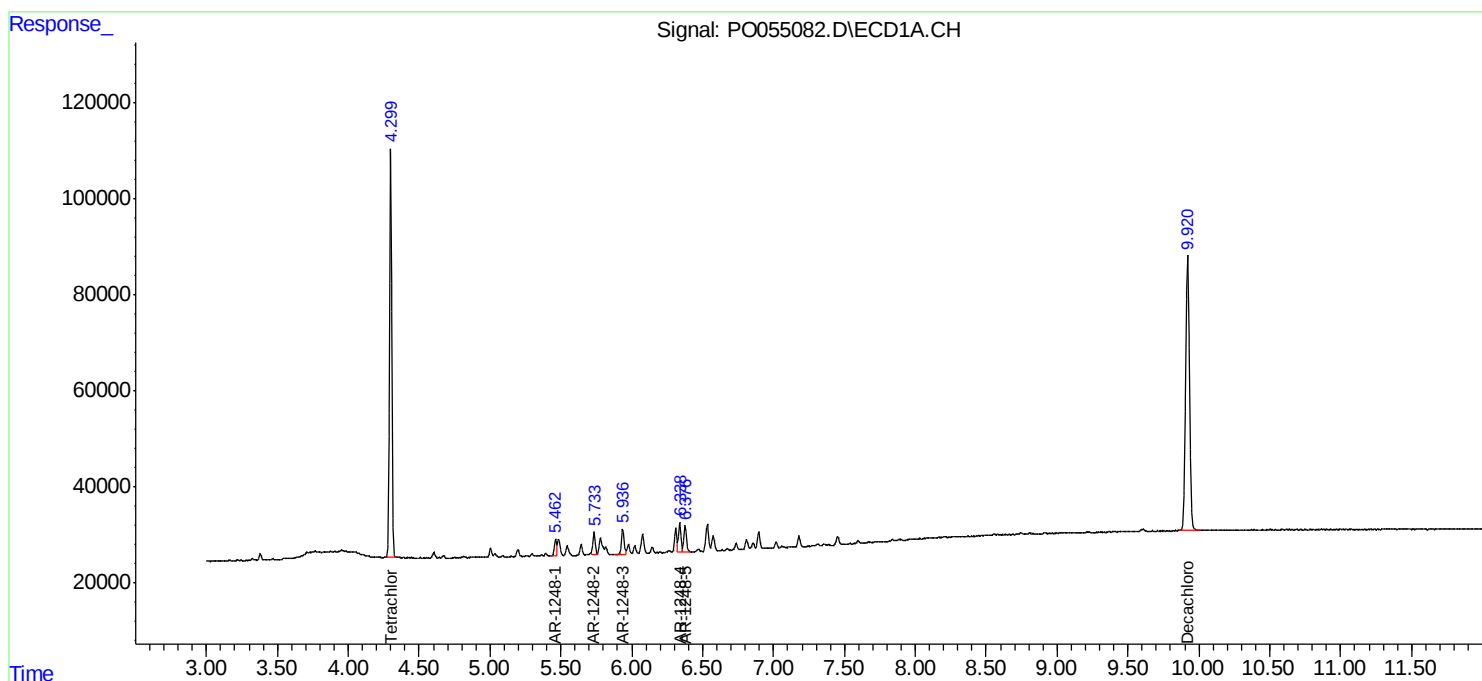

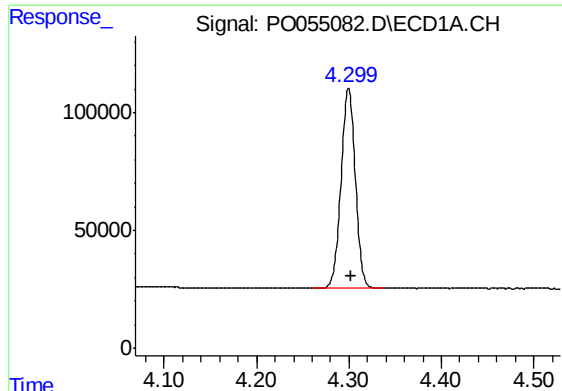


#1 Tetrachloro-m-xylene

R.T.: 4.300 min
Delta R.T.: -0.003 min
Response: 916352
Conc: 26.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:01:54 PM

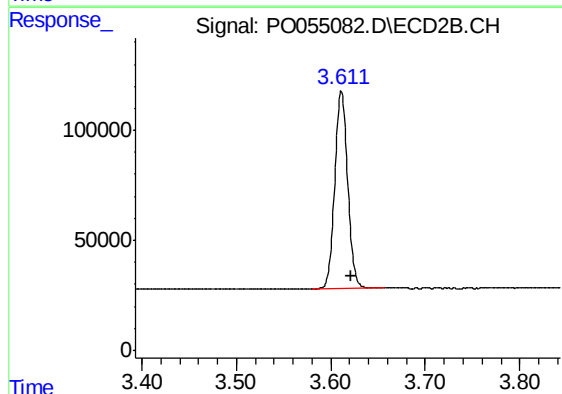


#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: -0.010 min
Response: 853269
Conc: 26.74 ng/ml

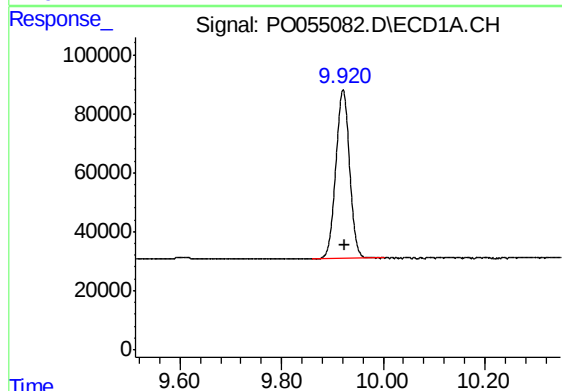


#2 Decachlorobiphenyl

R.T.: 9.921 min
Delta R.T.: -0.002 min
Response: 1077855
Conc: 21.86 ng/ml

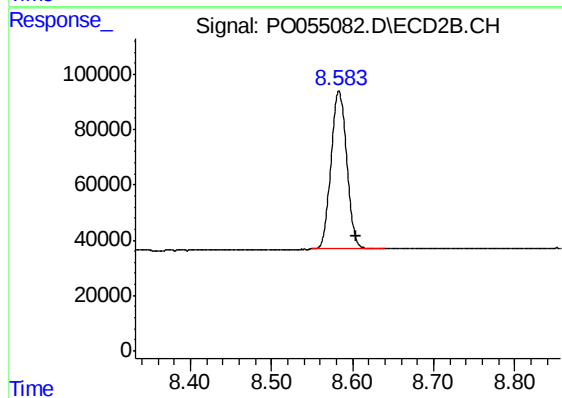

#2 Decachlorobiphenyl

R.T.: 8.583 min
Delta R.T.: -0.021 min
Response: 773929
Conc: 24.30 ng/ml

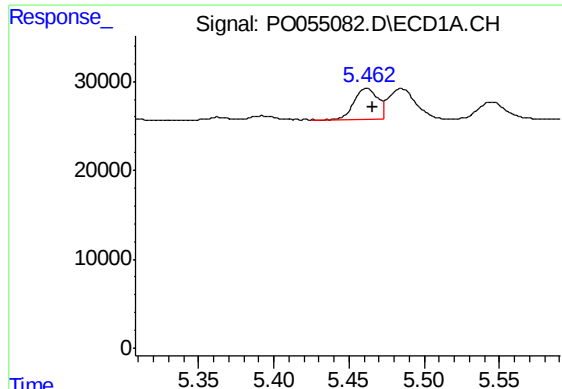


#21 AR-1248-1

R.T.: 5.462 min
Delta R.T.: -0.004 min
Response: 38132
Conc: 38.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:01:54 PM

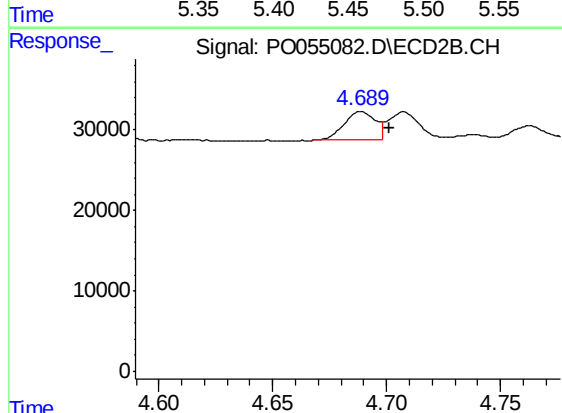


#21 AR-1248-1

R.T.: 4.689 min
Delta R.T.: -0.013 min
Response: 34550
Conc: 39.36 ng/ml m

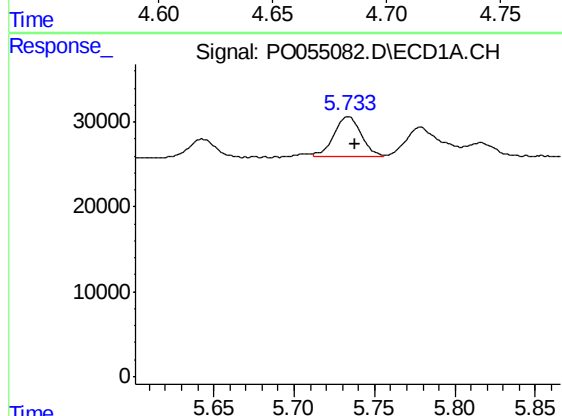


#22 AR-1248-2

R.T.: 5.733 min
Delta R.T.: -0.004 min
Response: 56479
Conc: 38.89 ng/ml m

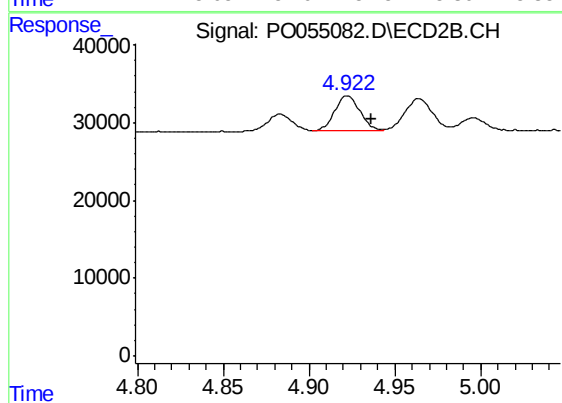

#22 AR-1248-2

R.T.: 4.922 min
Delta R.T.: -0.014 min
Response: 46893
Conc: 38.80 ng/ml

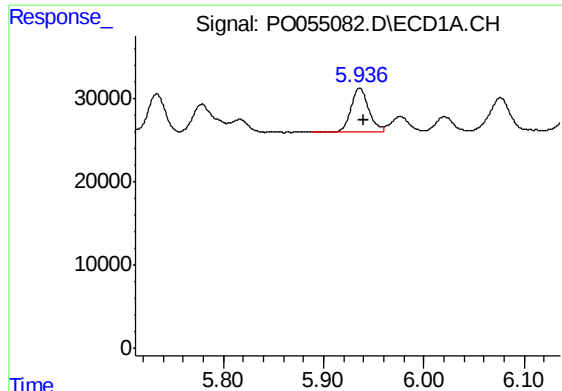


#23 AR-1248-3

R.T.: 5.936 min
Delta R.T.: -0.005 min
Response: 64720
Conc: 40.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:01:54 PM

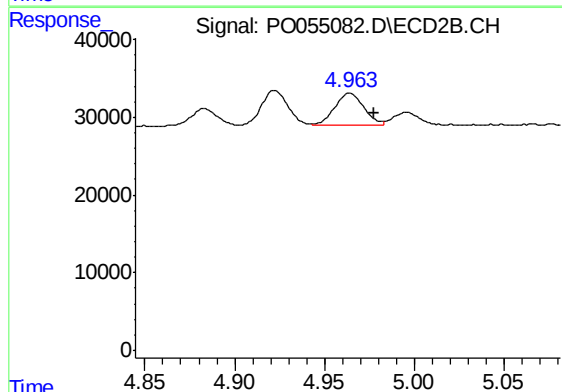


#23 AR-1248-3

R.T.: 4.964 min
Delta R.T.: -0.014 min
Response: 46818
Conc: 37.52 ng/ml

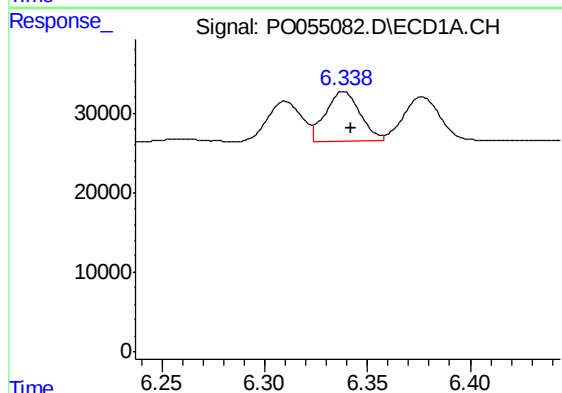


#24 AR-1248-4

R.T.: 6.339 min
Delta R.T.: -0.004 min
Response: 73478
Conc: 39.11 ng/ml

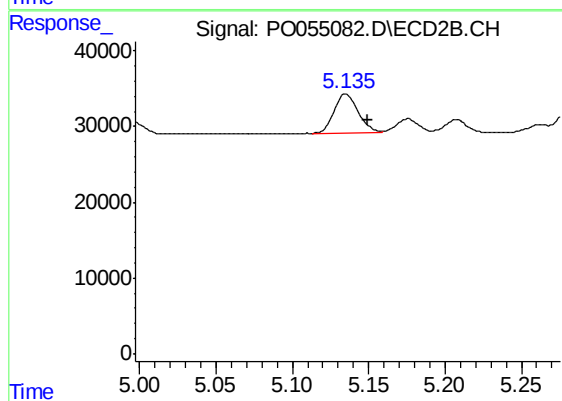

#24 AR-1248-4

R.T.: 5.135 min
Delta R.T.: -0.015 min
Response: 55477
Conc: 36.43 ng/ml m

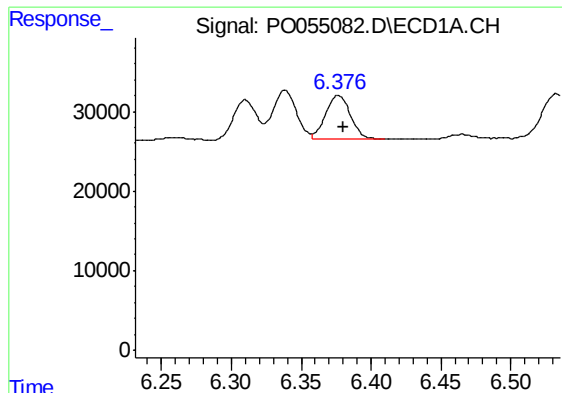


#25 AR-1248-5

R.T.: 6.376 min
Delta R.T.: -0.004 min
Response: 68572
Conc: 38.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Manual Integrations
APPROVED

mohammad
4/10/2019 4:01:54 PM

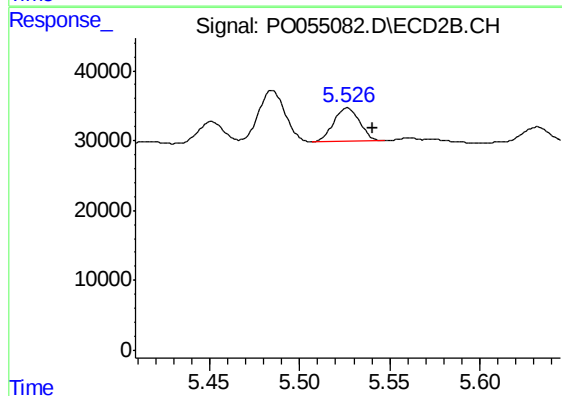

#25 AR-1248-5

R.T.: 5.526 min
Delta R.T.: -0.014 min
Response: 47900
Conc: 32.13 ng/ml