

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040919\
 Data File : P0055083.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Apr 2019 17:50
 Operator : SM/SJ
 Sample : K1560-09
 Misc : AR1254 MDL 100PPB
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-MDL-WATER-03-QT1-2019

Manual Integrations
 APPROVED

mohammad
 4/10/2019 4:01:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 07:07:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.299	3.611	911394	844132	26.261	26.452
2)	SA Decachlor...	9.920	8.583	1102132	784127	22.357	24.621
Target Compounds							
26)	L6 AR-1254-1	6.310	5.484	74587	85202	41.136	38.986
27)	L6 AR-1254-2	6.529	5.631	118385	76286	41.470	39.344
28)	L6 AR-1254-3	6.893	6.033	123053	121798	39.130	37.994
29)	L6 AR-1254-4	7.178	6.260	88353	65888	36.116	33.652m
30)	L6 AR-1254-5	7.595	6.676	89134	82588	33.255	28.729m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040919\
Data File : PO055083.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Apr 2019 17:50
Operator : SM/SJ
Sample : K1560-09
Misc : AR1254 MDL 100PPB
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:01:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 07:07:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

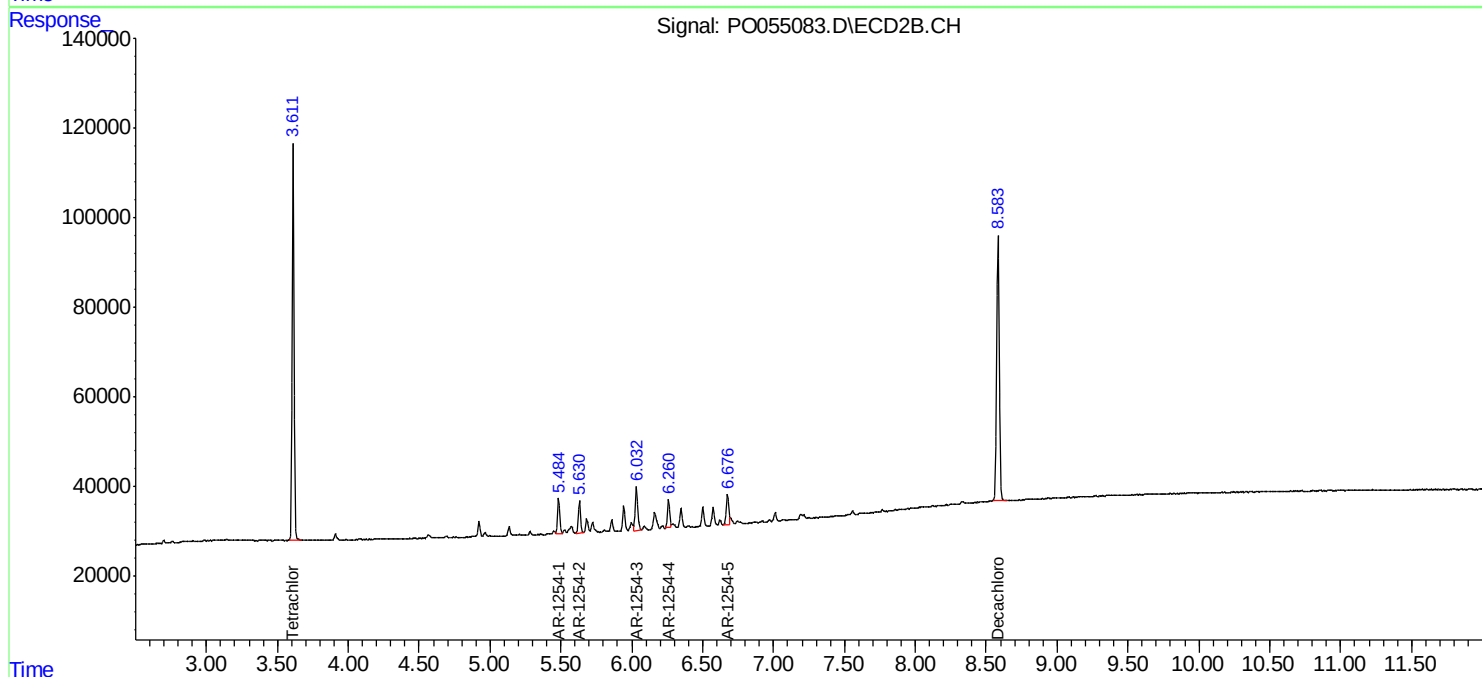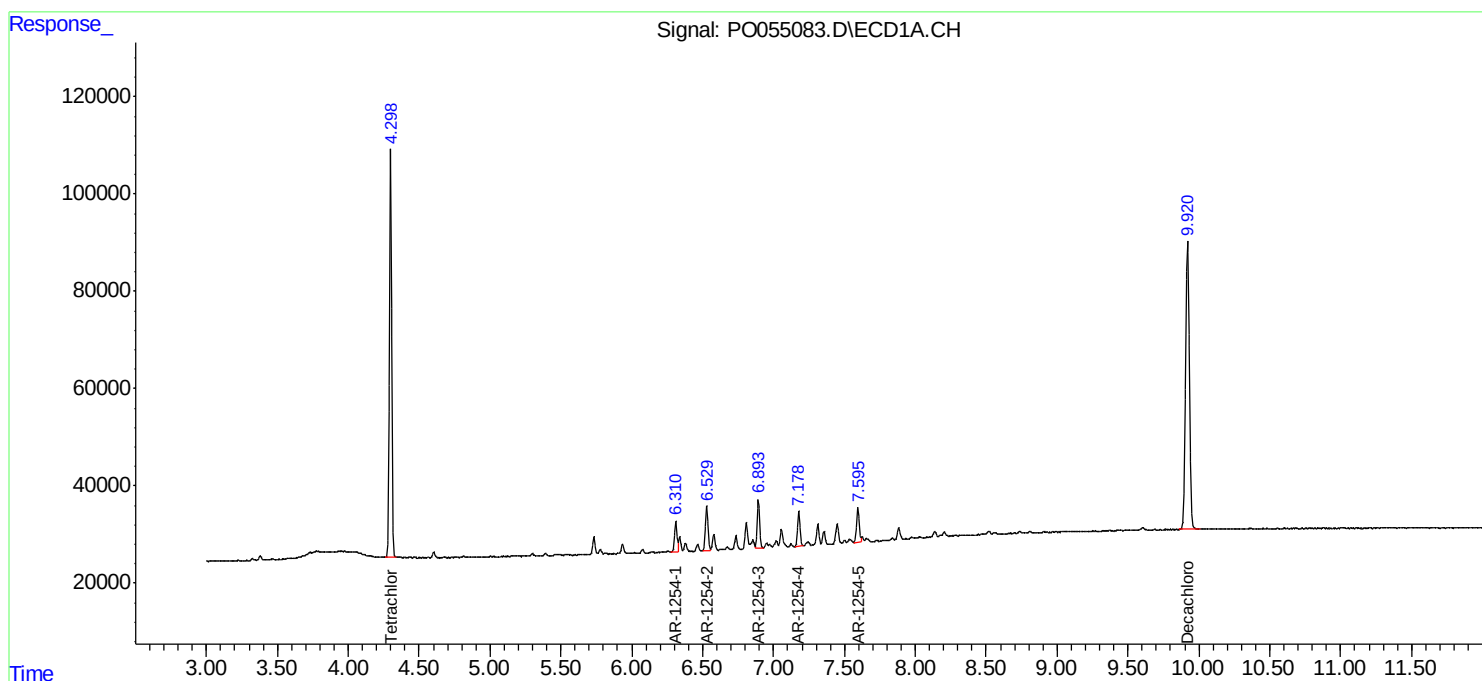

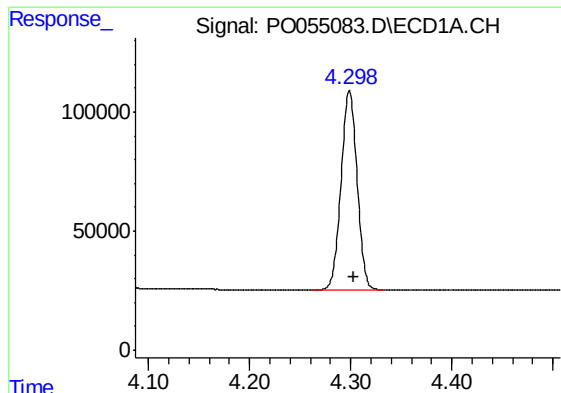


#1 Tetrachloro-m-xylene

R.T.: 4.299 min
Delta R.T.: -0.004 min
Response: 911394
Conc: 26.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:01:57 PM

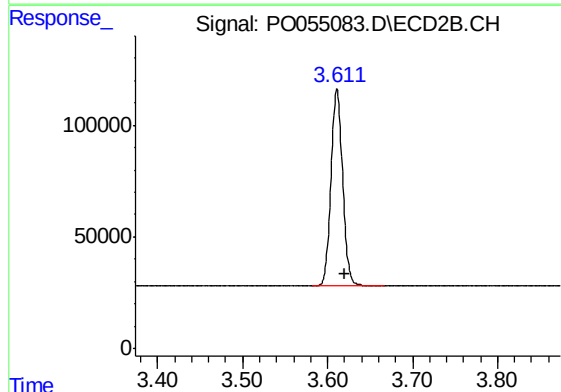


#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: -0.010 min
Response: 844132
Conc: 26.45 ng/ml

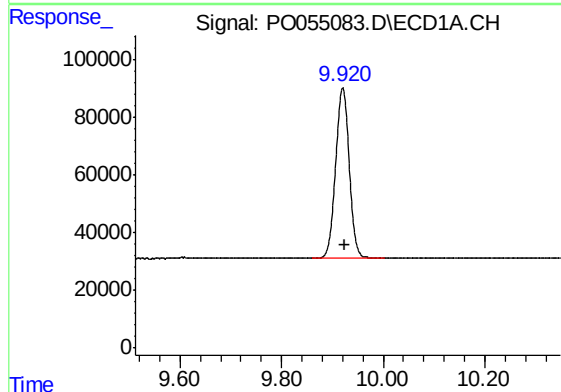


#2 Decachlorobiphenyl

R.T.: 9.920 min
Delta R.T.: -0.003 min
Response: 1102132
Conc: 22.36 ng/ml

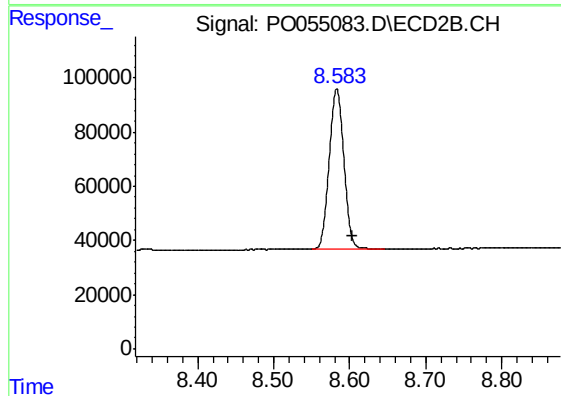

#2 Decachlorobiphenyl

R.T.: 8.583 min
Delta R.T.: -0.021 min
Response: 784127
Conc: 24.62 ng/ml

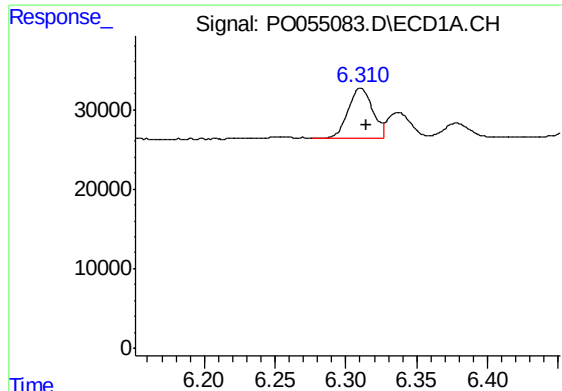


#26 AR-1254-1

R.T.: 6.310 min
Delta R.T.: -0.004 min
Response: 74587
Conc: 41.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:01:57 PM

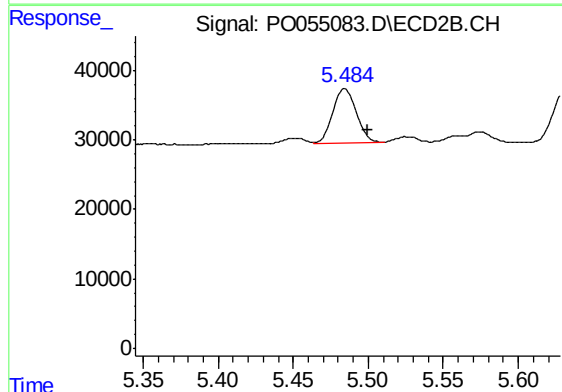


#26 AR-1254-1

R.T.: 5.484 min
Delta R.T.: -0.015 min
Response: 85202
Conc: 38.99 ng/ml

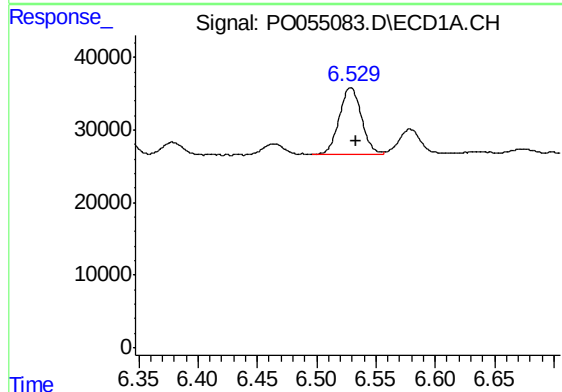


#27 AR-1254-2

R.T.: 6.529 min
Delta R.T.: -0.004 min
Response: 118385
Conc: 41.47 ng/ml

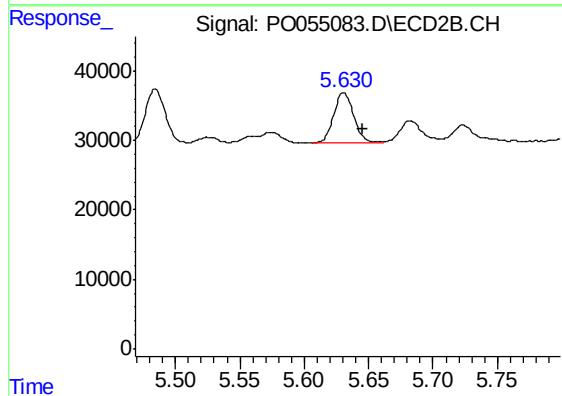

#27 AR-1254-2

R.T.: 5.631 min
Delta R.T.: -0.015 min
Response: 76286
Conc: 39.34 ng/ml

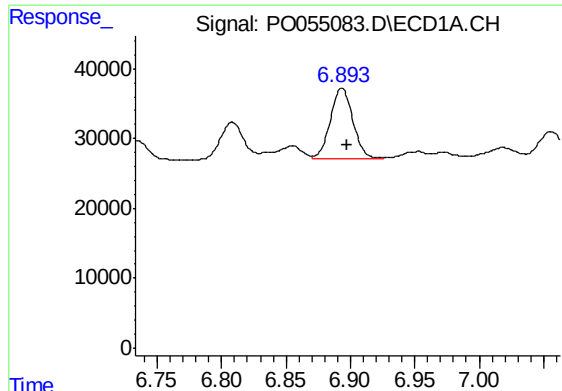


#28 AR-1254-3

R.T.: 6.893 min
Delta R.T.: -0.004 min
Response: 123053
Conc: 39.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019


Manual Integrations
APPROVED

mohammad
4/10/2019 4:01:57 PM

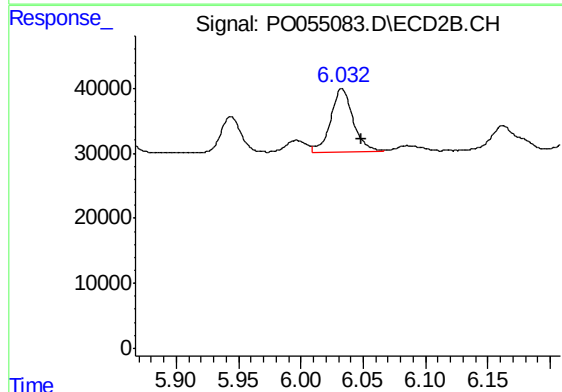


#28 AR-1254-3

R.T.: 6.033 min
Delta R.T.: -0.016 min
Response: 121798
Conc: 37.99 ng/ml

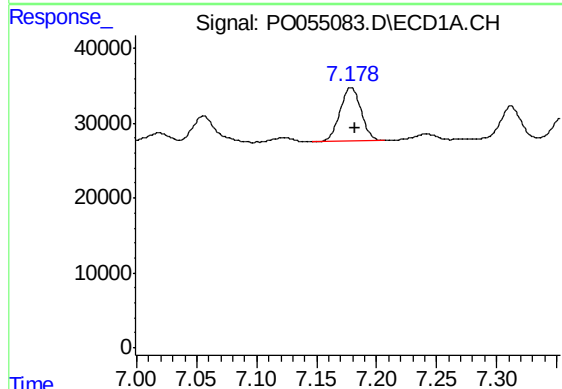


#29 AR-1254-4

R.T.: 7.178 min
Delta R.T.: -0.004 min
Response: 88353
Conc: 36.12 ng/ml

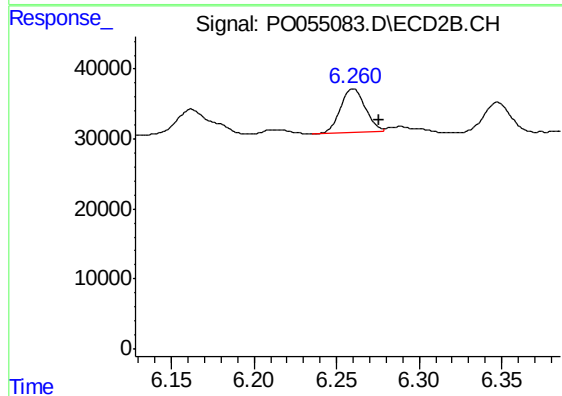

#29 AR-1254-4

R.T.: 6.260 min
Delta R.T.: -0.016 min
Response: 65888
Conc: 33.65 ng/ml m

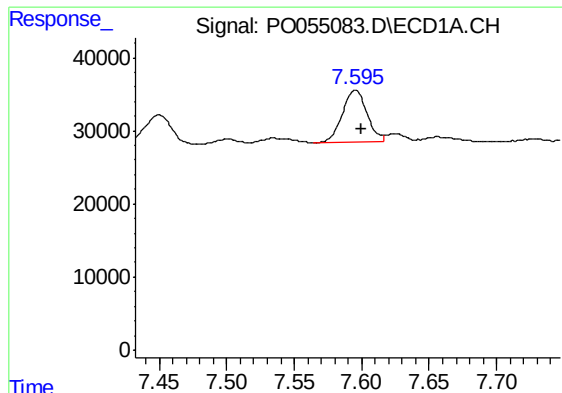


#30 AR-1254-5

R.T.: 7.595 min
Delta R.T.: -0.004 min
Response: 89134
Conc: 33.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-MDL-WATER-03-QT1-2019

Manual Integrations
APPROVED

mohammad
4/10/2019 4:01:57 PM

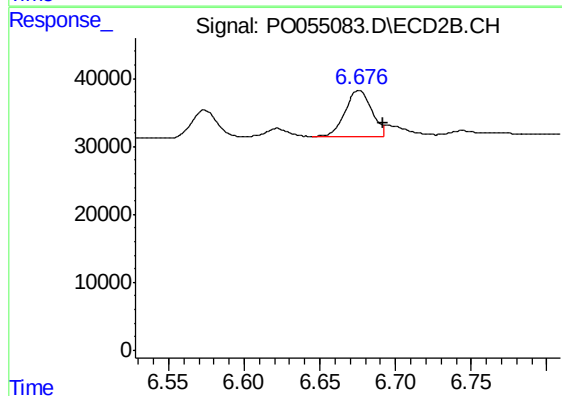

#30 AR-1254-5

R.T.: 6.676 min
Delta R.T.: -0.016 min
Response: 82588
Conc: 28.73 ng/ml m