

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041020\
 Data File : P0067790.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Apr 2020 10:12
 Operator : DD\AJ
 Sample : L2186-01 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-8:1-SOLIDS

Manual Integrations
 APPROVED

Sohil
 4/13/2020 10:17:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 13:27:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.929	3.941	125436	177450	5.267	5.294m
2) SA Decachlor...	10.916	9.232	161569	205456	4.746	4.969

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041020\
Data File : P0067790.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Apr 2020 10:12
Operator : DD\AJ
Sample : L2186-01 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-8:1-SOLIDS


Manual Integrations
APPROVED

Sohil
4/13/2020 10:17:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 13:27:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

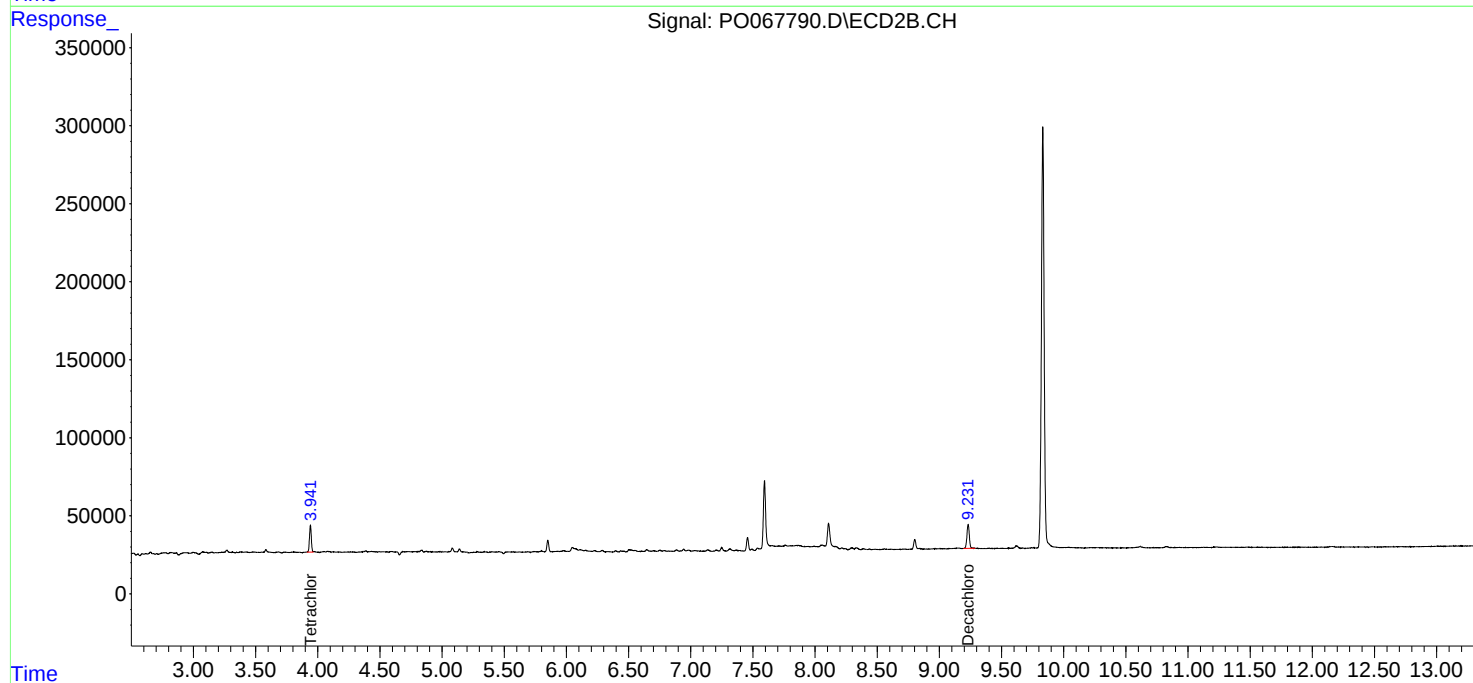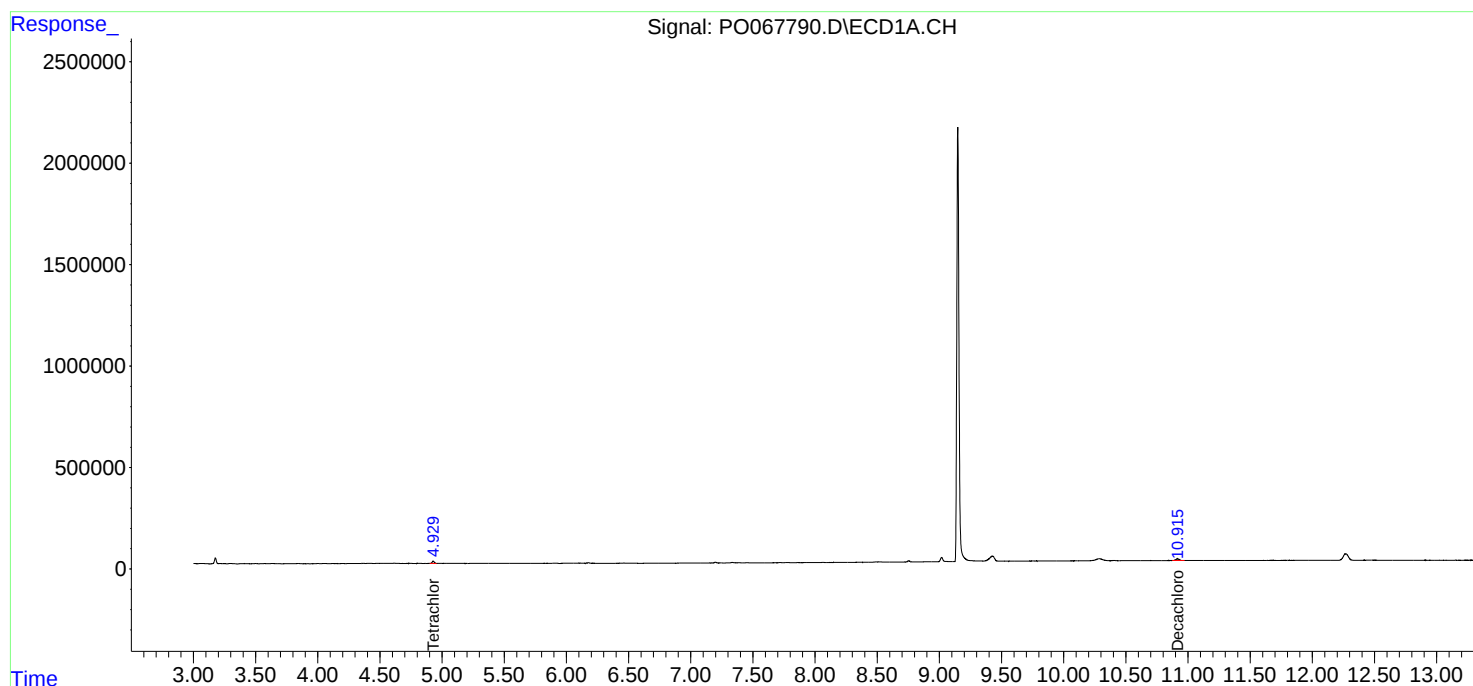

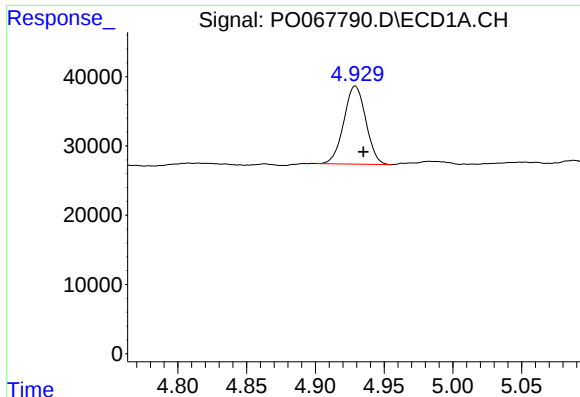


#1 Tetrachloro-m-xylene

R.T.: 4.929 min
Delta R.T.: -0.006 min
Response: 125436
Conc: 5.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-8:1-SOLIDS


Manual Integrations
APPROVED

Sohil
4/13/2020 10:17:46 AM

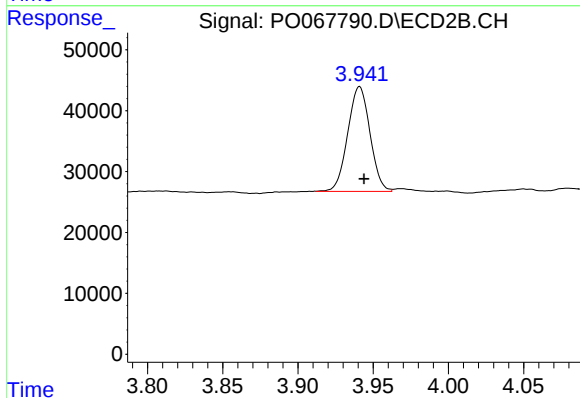


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: -0.003 min
Response: 177450
Conc: 5.29 ng/ml m

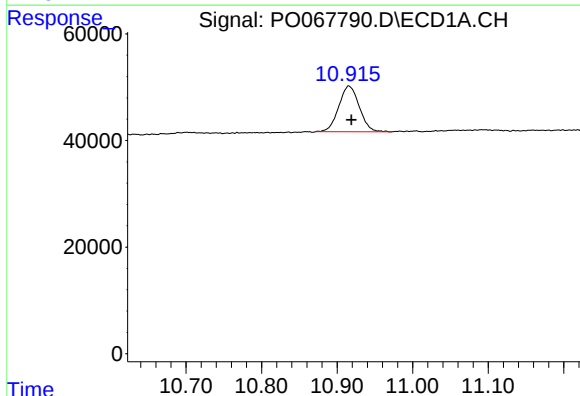

#2 Decachlorobiphenyl

R.T.: 10.916 min
Delta R.T.: -0.003 min
Response: 161569
Conc: 4.75 ng/ml

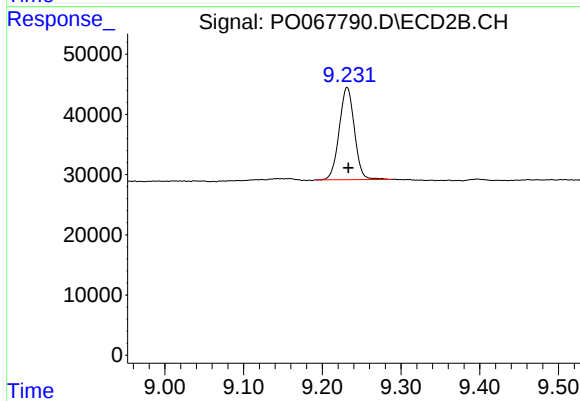

#2 Decachlorobiphenyl

R.T.: 9.232 min
Delta R.T.: -0.002 min
Response: 205456
Conc: 4.97 ng/ml