

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041020\
 Data File : P0067800.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Apr 2020 13:03
 Operator : DD\AJ
 Sample : L2199-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-39-38-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 14:21:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.930	3.942	597417	810906	25.087	24.194
2) SA Decachlor...	10.915	9.230	621727	693218	18.263	16.766

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041020\
Data File : P0067800.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Apr 2020 13:03
Operator : DD\AJ
Sample : L2199-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-39-38-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 14:21:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

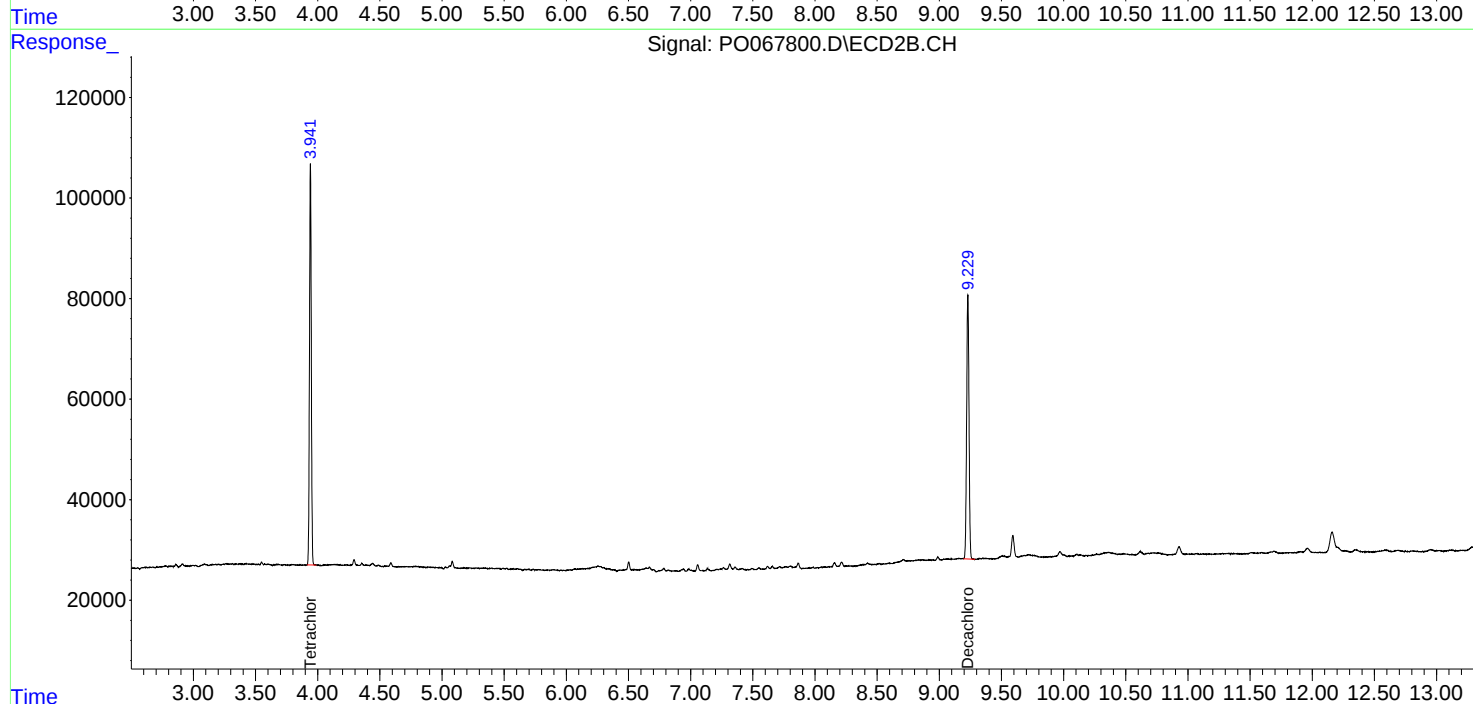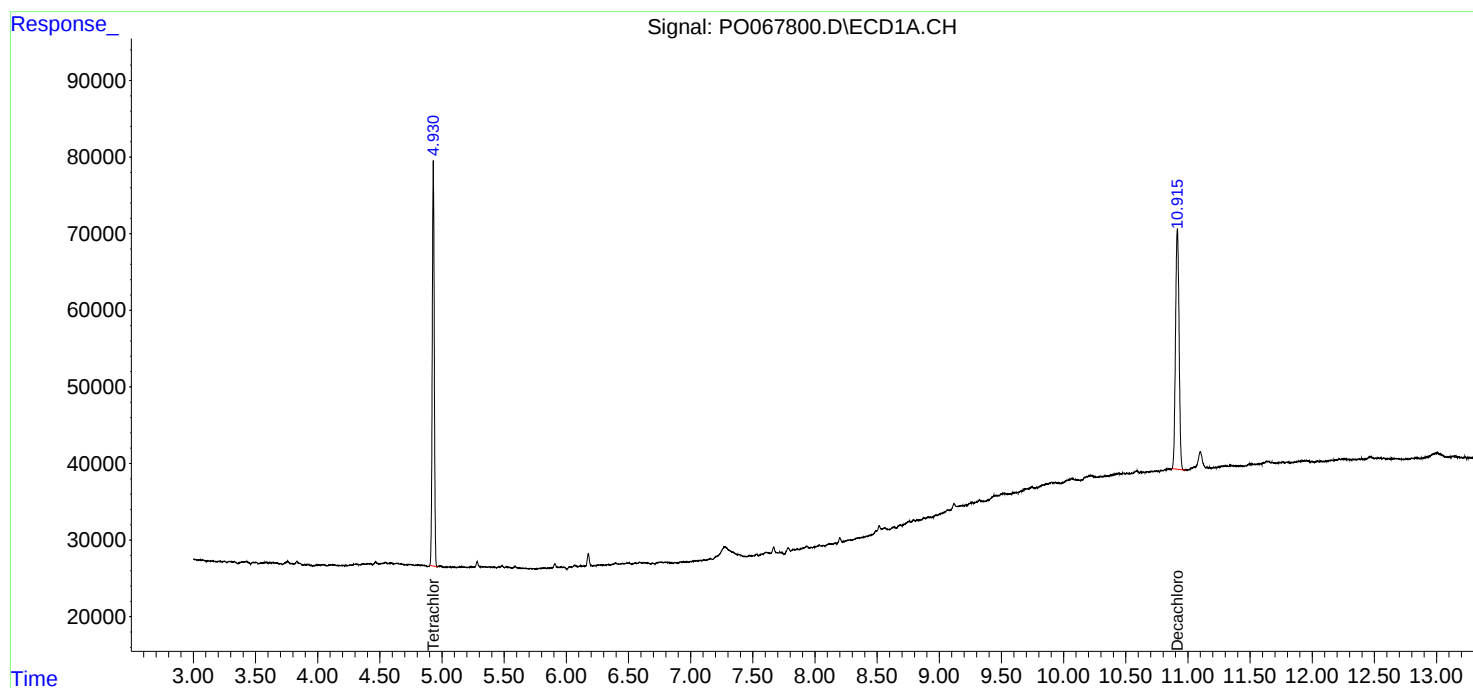


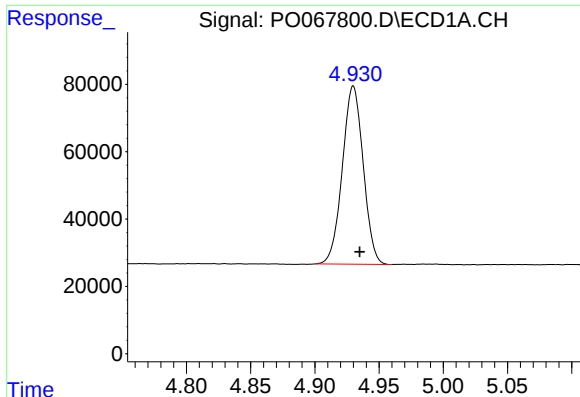

#1 Tetrachloro-m-xylene


R.T.: 4.930 min
Delta R.T.: -0.005 min
Response: 597417
Conc: 25.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-39-38-COMP

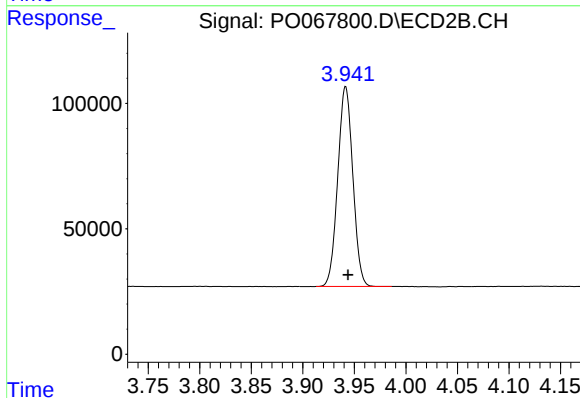


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: -0.002 min
Response: 810906
Conc: 24.19 ng/ml

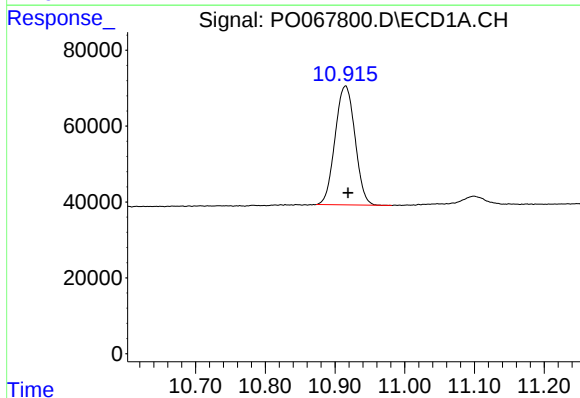

#2 Decachlorobiphenyl

R.T.: 10.915 min
Delta R.T.: -0.004 min
Response: 621727
Conc: 18.26 ng/ml

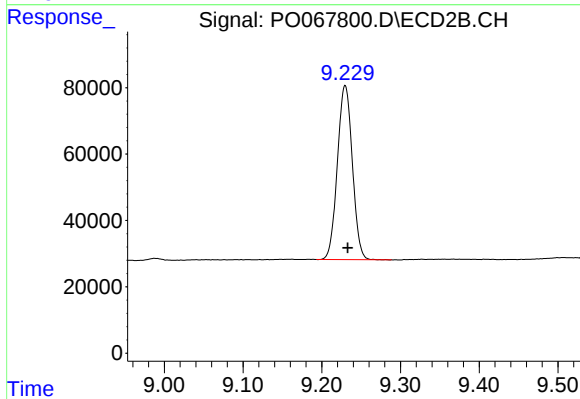

#2 Decachlorobiphenyl

R.T.: 9.230 min
Delta R.T.: -0.003 min
Response: 693218
Conc: 16.77 ng/ml