

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041119\
 Data File : P0055166.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Apr 2019 19:54
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1660 LOD 25PPB
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 02:41:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.293	3.606	659039	585192	18.990	18.337
2)	SA Decachlor...	9.903	8.572	1022064	719411	20.733	22.589
Target Compounds							
3)	L1 AR-1016-1	5.454	4.701	55525	61689	30.857	39.009 #
4)	L1 AR-1016-2	5.476	4.701	73316	61689	29.519	28.790
5)	L1 AR-1016-3	5.538	4.916	49396	26378	31.397	21.832 #
6)	L1 AR-1016-4	5.636	4.916	39391	26378	30.229	26.103
7)	L1 AR-1016-5	5.929	5.168	40951	12492	30.692	9.584 #
8)	L2 AR-1221-1	0.000	3.903	0	13333	N.D.	34.294 #
9)	L2 AR-1221-2	4.594	3.903	14938	13333	44.049	44.475
10)	L2 AR-1221-3	4.664	3.978	25850	20202	24.885	21.917
11)	L3 AR-1232-1	4.664	3.978	25850	20202	30.025	26.940
12)	L3 AR-1232-2	5.188	4.701	36179	61689	73.964	71.639
13)	L3 AR-1232-3	5.476	4.916	73316	26378	75.019	54.437 #
14)	L3 AR-1232-4	5.636	4.989	39391	11008	76.957	25.053 #
15)	L3 AR-1232-5	5.726	5.168	38773	12492	93.206	25.684 #
16)	L4 AR-1242-1	5.454	4.701	55525	61689	39.967	50.247 #
17)	L4 AR-1242-2	5.476	4.701	73316	61689	38.316	37.224
18)	L4 AR-1242-3	5.538	4.916	49396	26378	39.853	27.845 #
19)	L4 AR-1242-4	5.636	4.989	39391	11008	38.636	11.518 #
20)	L4 AR-1242-5	6.370	5.518	13206	9758	10.940	7.934 #
21)	L5 AR-1248-1	5.476	4.701	73316	61689	73.340	70.278
22)	L5 AR-1248-2	5.726	4.916	38773	26378	26.698	21.827
23)	L5 AR-1248-3	5.929	4.989	40951	11008	25.640	8.822 #
24)	L5 AR-1248-4	6.330	5.168	14983	12492	7.976	8.202
25)	L5 AR-1248-5	6.370	5.518	13206	9758	7.366	6.545
26)	L6 AR-1254-1	6.303	5.518	43670	9758	24.085	4.465 #
27)	L6 AR-1254-2	6.520	5.623	38430	30834	13.462	15.902
28)	L6 AR-1254-3	6.886	6.039	24338	58569	7.739	18.270 #
29)	L6 AR-1254-4	7.169	6.280	11328	19108	4.630	9.759 #
30)	L6 AR-1254-5	7.585	6.704	131349	86850	49.005	30.212 #
31)	L7 AR-1260-1	7.047	6.153	95333	85504	37.941	37.207
32)	L7 AR-1260-2	7.304	6.340	116633	110842	37.581	40.266
33)	L7 AR-1260-3	7.661	6.493	85938	96294	35.014	37.354
34)	L7 AR-1260-4	7.886	7.001	95619	8194	34.569	3.850 #
35)	L7 AR-1260-5	8.194	7.202	172411	168455	31.073	35.173
36)	L8 AR-1262-1	7.661	6.704	85938	86850	25.791	29.194
37)	L8 AR-1262-2	8.194	7.202	172411	168455	29.102	34.371
38)	L8 AR-1262-3	8.507	7.485	111486	40550	26.911	19.747 #
39)	L8 AR-1262-4	8.558	7.548	68059	121303	21.123	33.489 #
40)	L8 AR-1262-5	9.200	8.040	45736	38187	20.920	23.662
41)	L9 AR-1268-1	8.507	7.485	111486	40550	15.664	7.172 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041119\
 Data File : P0055166.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Apr 2019 19:54
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1660 LOD 25PPB
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 02:41:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.558	7.548	68059	121303	10.387	23.456 #
43) L9	AR-1268-3	0.000	7.756	0	8701	N.D.	2.022 #
44) L9	AR-1268-4	9.200	8.040	45736	38187	19.170	20.599
45) L9	AR-1268-5	9.588	0.000	20270	0	1.230	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041119\
Data File : PO055166.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Apr 2019 19:54
Operator : SM/SJ
Sample : K1560-07
Misc : AR1660 LOD 25PPB
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 02:41:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

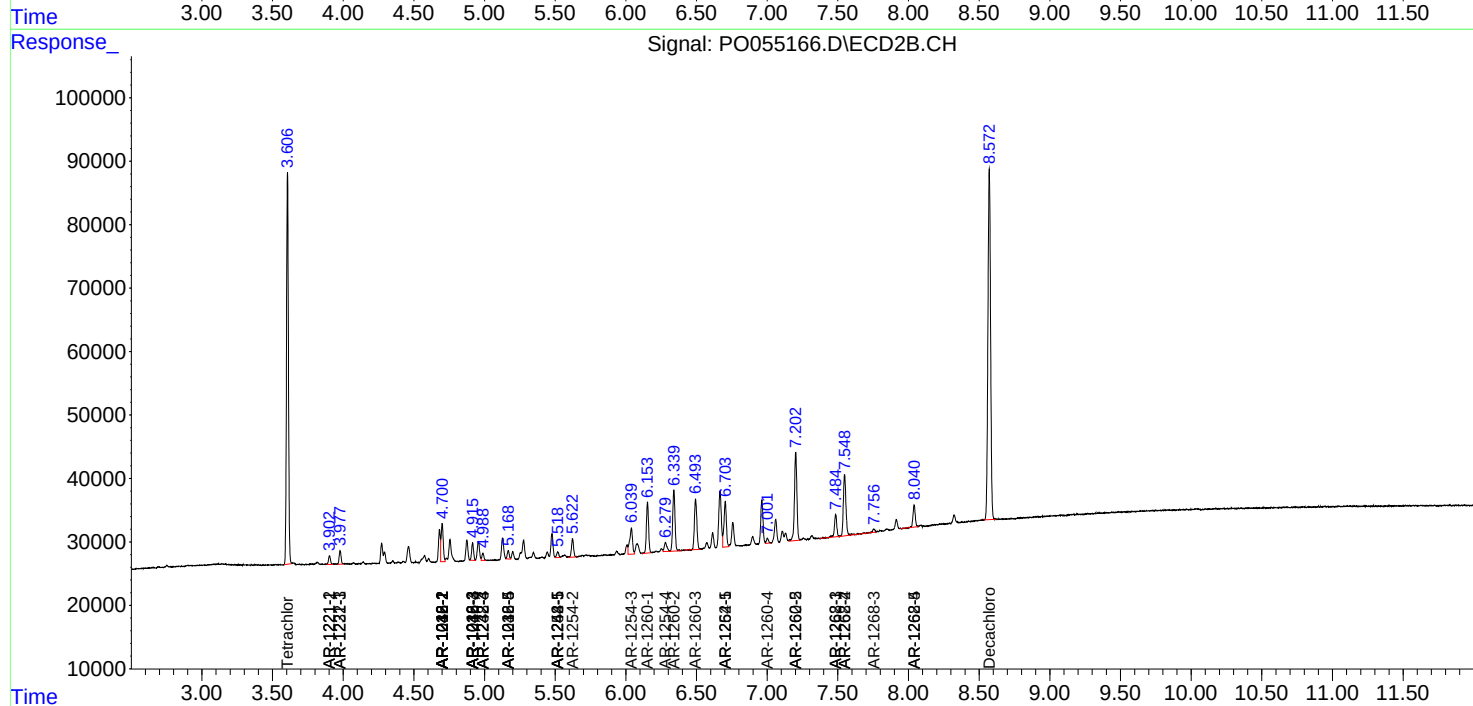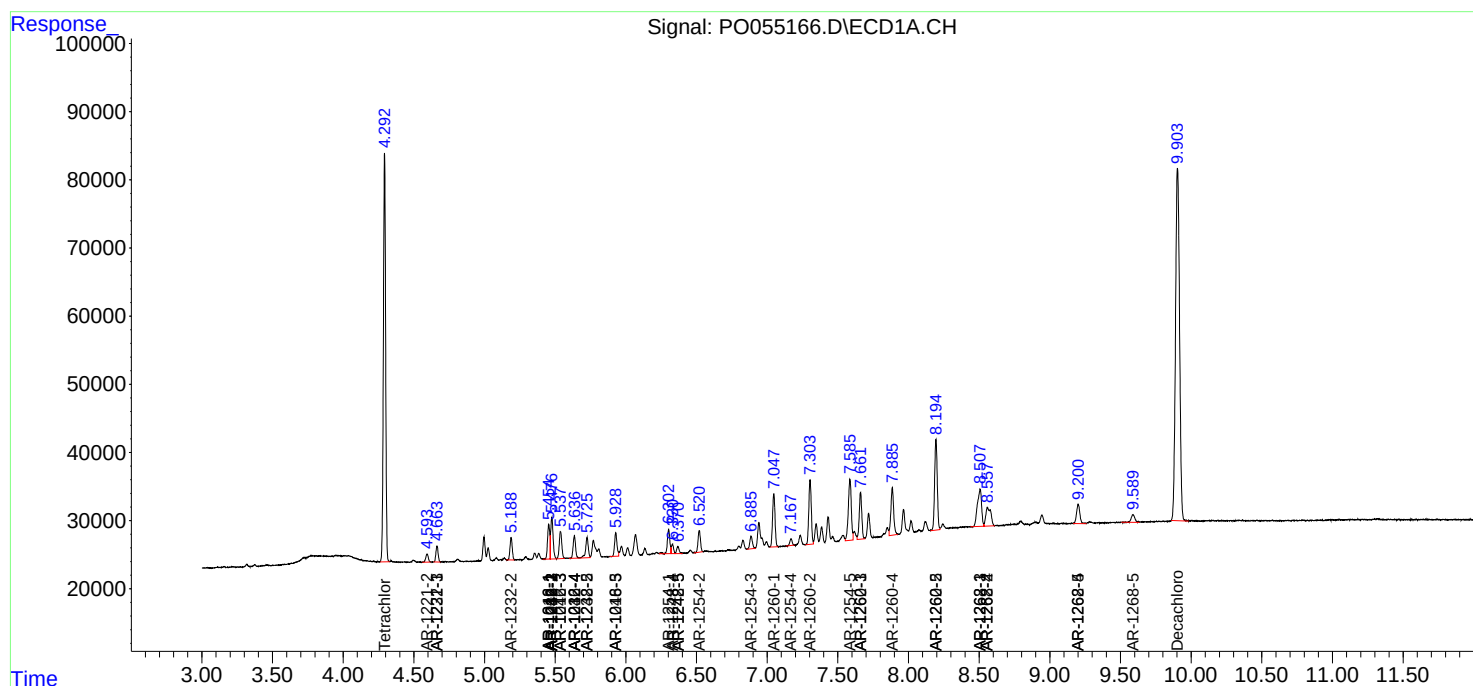


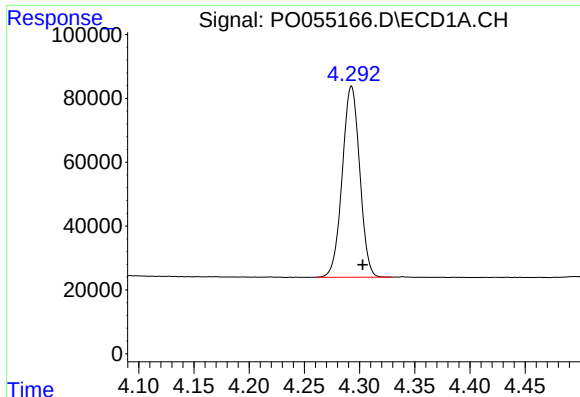

#1 Tetrachloro-m-xylene


R.T.: 4.293 min
Delta R.T.: -0.010 min
Response: 659039
Conc: 18.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

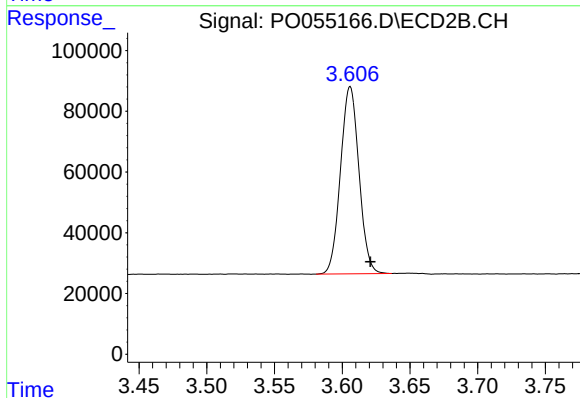


#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: -0.015 min
Response: 585192
Conc: 18.34 ng/ml

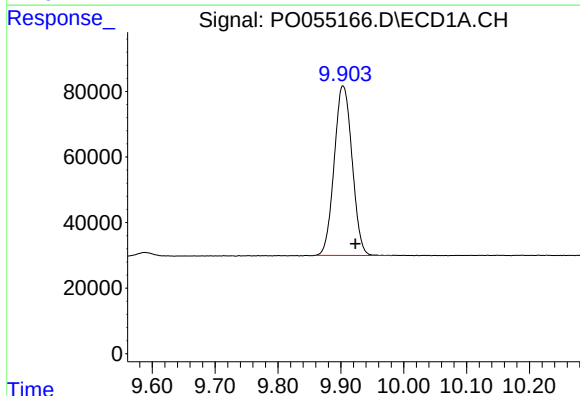


#2 Decachlorobiphenyl

R.T.: 9.903 min
Delta R.T.: -0.020 min
Response: 1022064
Conc: 20.73 ng/ml

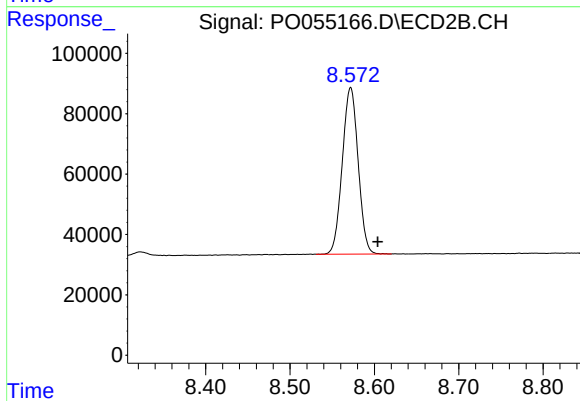

#2 Decachlorobiphenyl


R.T.: 8.572 min
Delta R.T.: -0.032 min
Response: 719411
Conc: 22.59 ng/ml

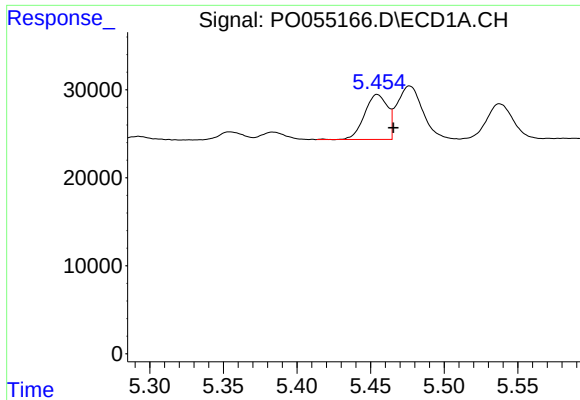

#3 AR-1016-1


R.T.: 5.454 min
Delta R.T.: -0.011 min
Response: 55525
Conc: 30.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

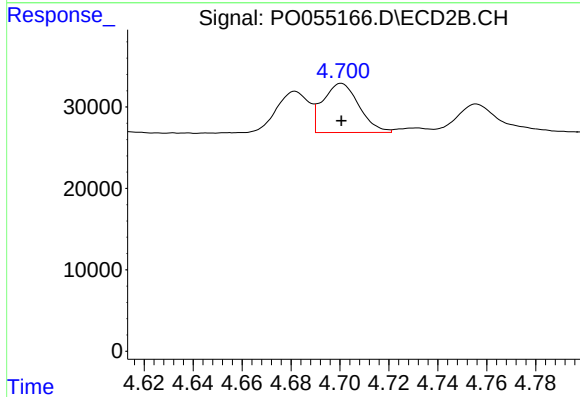


#3 AR-1016-1

R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 61689
Conc: 39.01 ng/ml

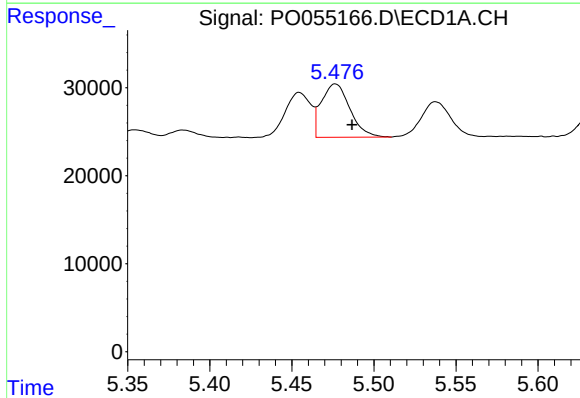


#4 AR-1016-2

R.T.: 5.476 min
Delta R.T.: -0.010 min
Response: 73316
Conc: 29.52 ng/ml

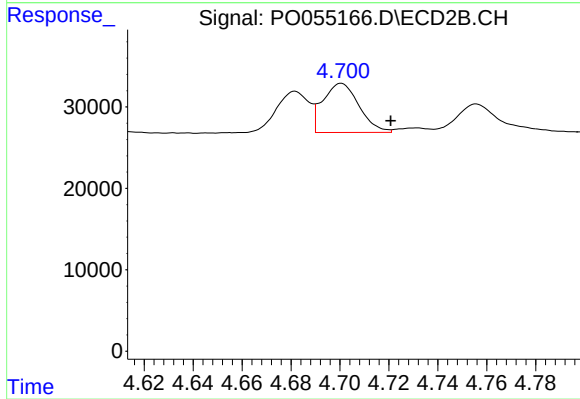

#4 AR-1016-2


R.T.: 4.701 min
Delta R.T.: -0.020 min
Response: 61689
Conc: 28.79 ng/ml

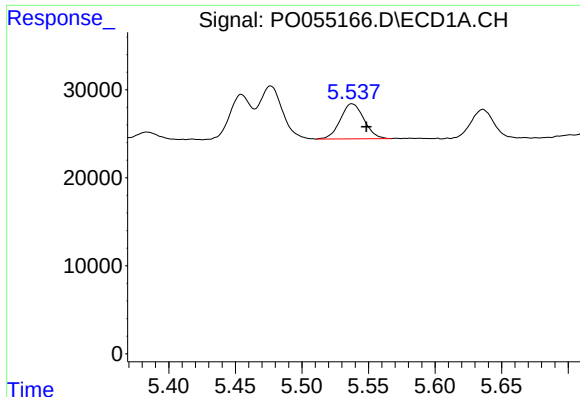

#5 AR-1016-3


R.T.: 5.538 min
Delta R.T.: -0.011 min
Response: 49396
Conc: 31.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

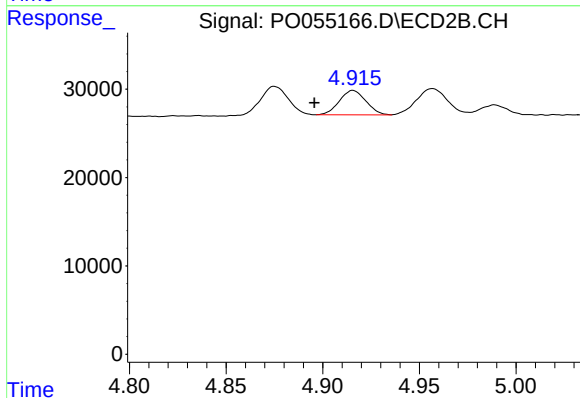


#5 AR-1016-3

R.T.: 4.916 min
Delta R.T.: 0.020 min
Response: 26378
Conc: 21.83 ng/ml

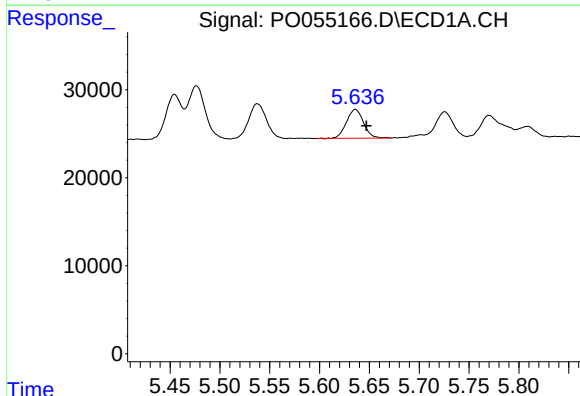


#6 AR-1016-4

R.T.: 5.636 min
Delta R.T.: -0.011 min
Response: 39391
Conc: 30.23 ng/ml

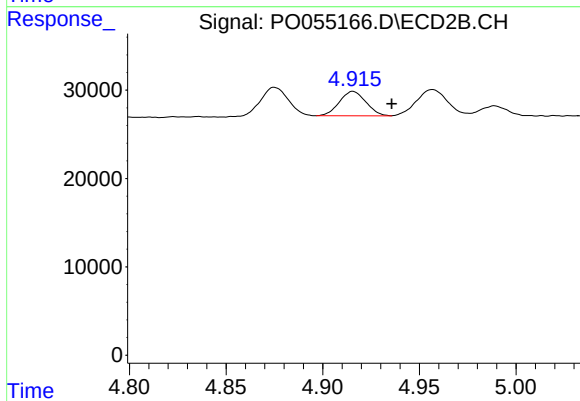

#6 AR-1016-4


R.T.: 4.916 min
Delta R.T.: -0.020 min
Response: 26378
Conc: 26.10 ng/ml

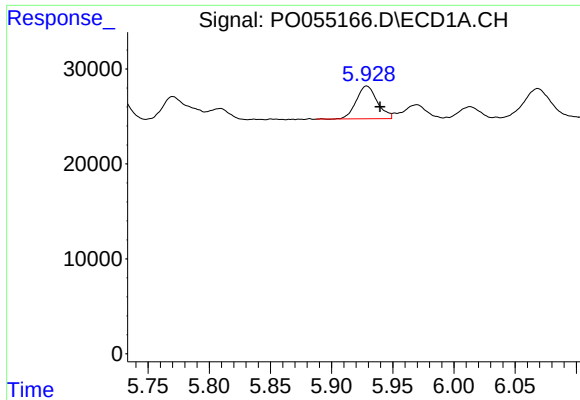

#7 AR-1016-5


R.T.: 5.929 min
Delta R.T.: -0.011 min
Response: 40951
Conc: 30.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

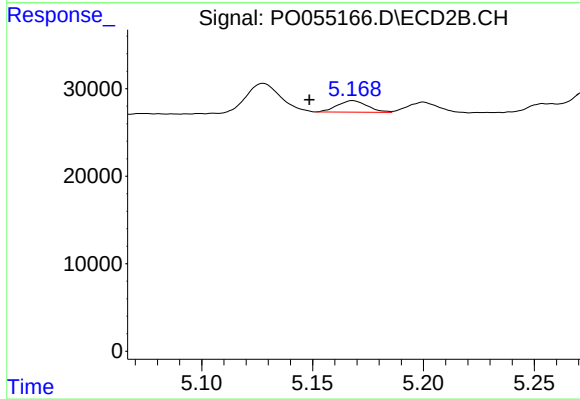


#7 AR-1016-5

R.T.: 5.168 min
Delta R.T.: 0.020 min
Response: 12492
Conc: 9.58 ng/ml

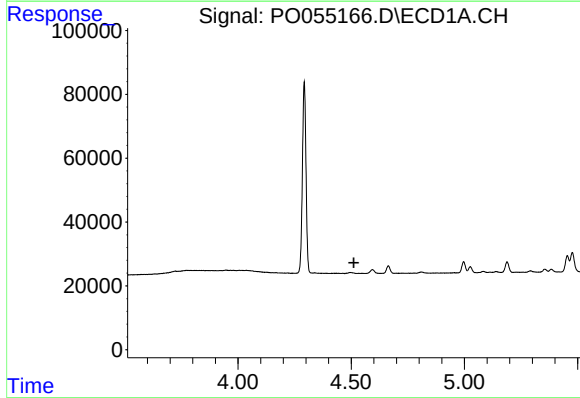


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.512 min
Response: 0
Conc: N.D.

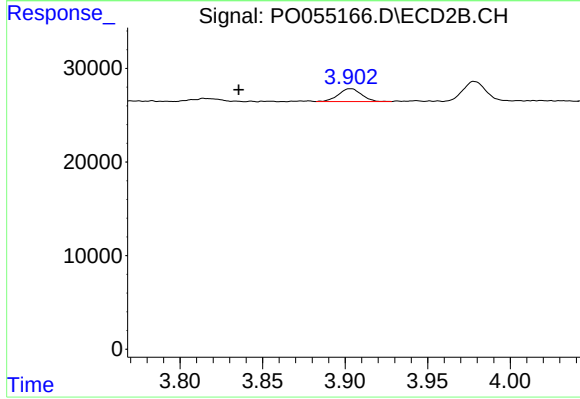

#8 AR-1221-1


R.T.: 3.903 min
Delta R.T.: 0.067 min
Response: 13333
Conc: 34.29 ng/ml

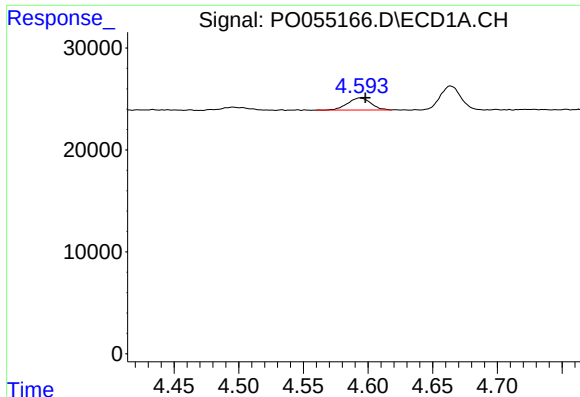

#9 AR-1221-2


R.T.: 4.594 min
Delta R.T.: -0.004 min
Response: 14938
Conc: 44.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

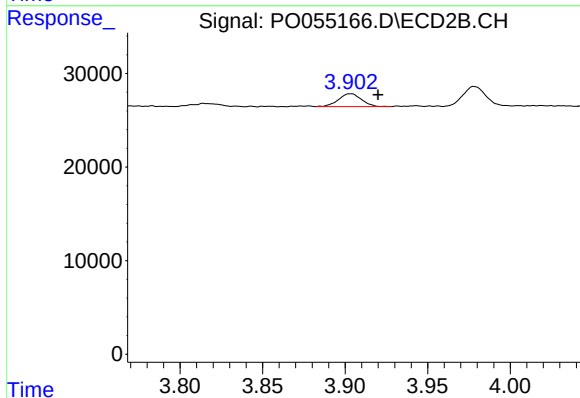


#9 AR-1221-2

R.T.: 3.903 min
Delta R.T.: -0.017 min
Response: 13333
Conc: 44.48 ng/ml

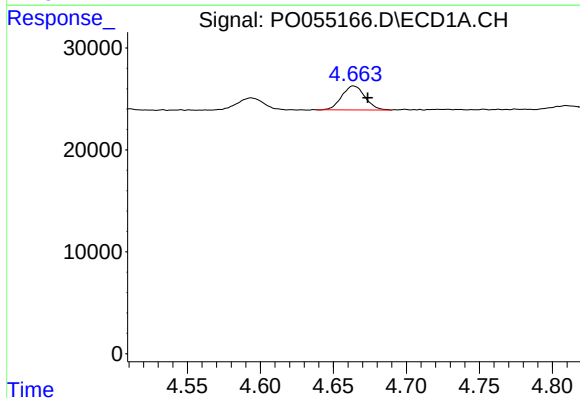


#10 AR-1221-3

R.T.: 4.664 min
Delta R.T.: -0.010 min
Response: 25850
Conc: 24.89 ng/ml

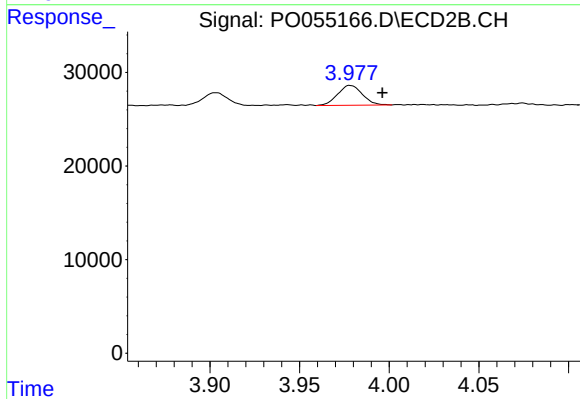

#10 AR-1221-3


R.T.: 3.978 min
Delta R.T.: -0.018 min
Response: 20202
Conc: 21.92 ng/ml

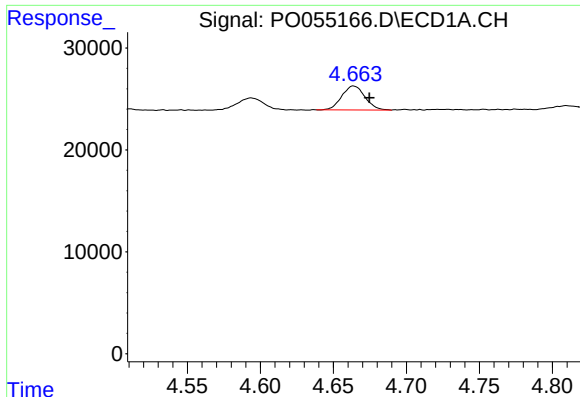

#11 AR-1232-1


R.T.: 4.664 min
Delta R.T.: -0.011 min
Response: 25850
Conc: 30.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

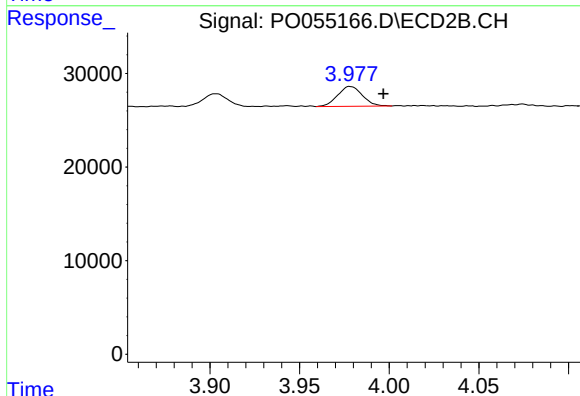


#11 AR-1232-1

R.T.: 3.978 min
Delta R.T.: -0.019 min
Response: 20202
Conc: 26.94 ng/ml

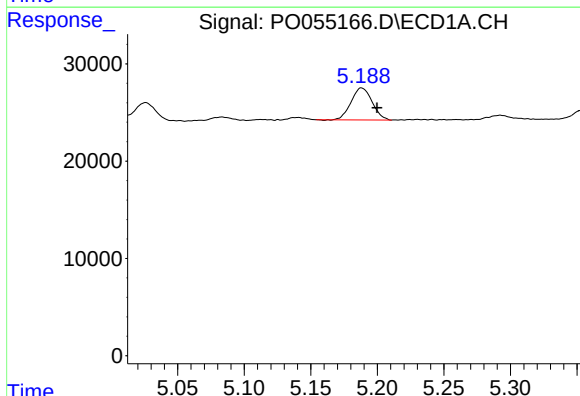


#12 AR-1232-2

R.T.: 5.188 min
Delta R.T.: -0.012 min
Response: 36179
Conc: 73.96 ng/ml

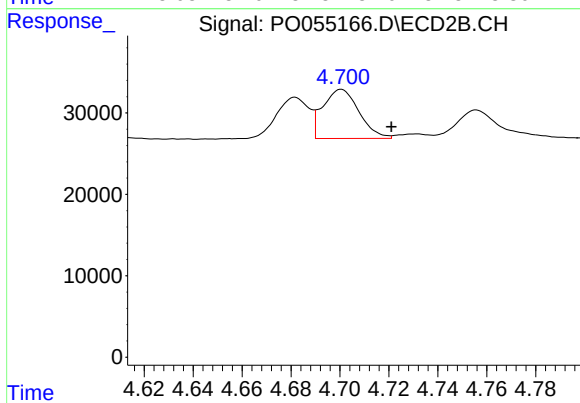

#12 AR-1232-2


R.T.: 4.701 min
Delta R.T.: -0.021 min
Response: 61689
Conc: 71.64 ng/ml

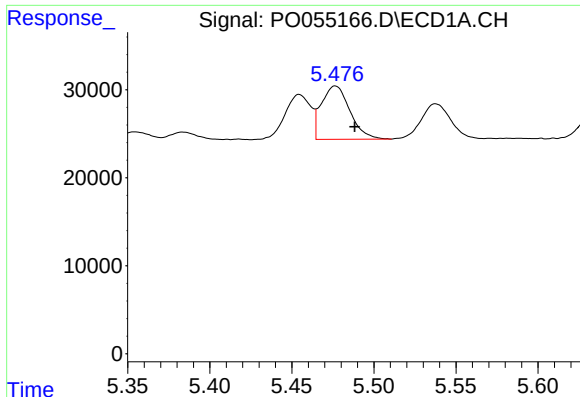

#13 AR-1232-3


R.T.: 5.476 min
Delta R.T.: -0.012 min
Response: 73316
Conc: 75.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

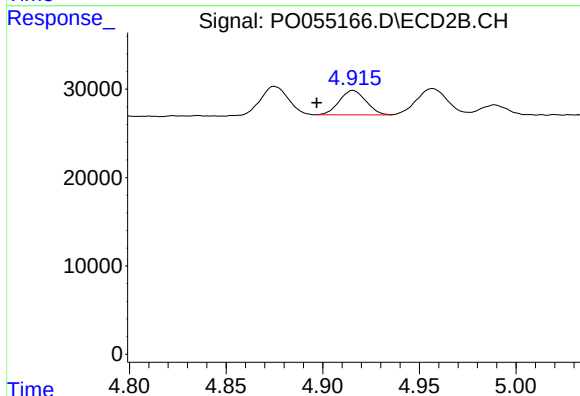


#13 AR-1232-3

R.T.: 4.916 min
Delta R.T.: 0.019 min
Response: 26378
Conc: 54.44 ng/ml

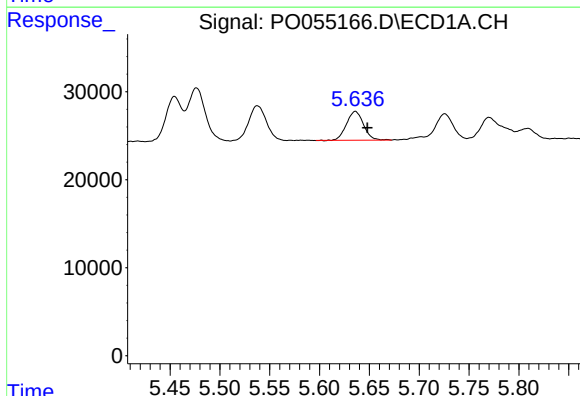


#14 AR-1232-4

R.T.: 5.636 min
Delta R.T.: -0.012 min
Response: 39391
Conc: 76.96 ng/ml

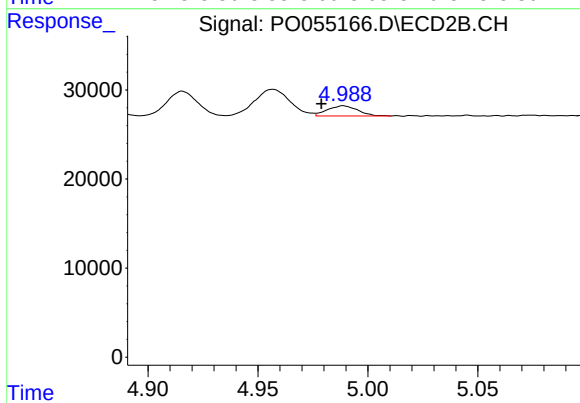

#14 AR-1232-4


R.T.: 4.989 min
Delta R.T.: 0.010 min
Response: 11008
Conc: 25.05 ng/ml

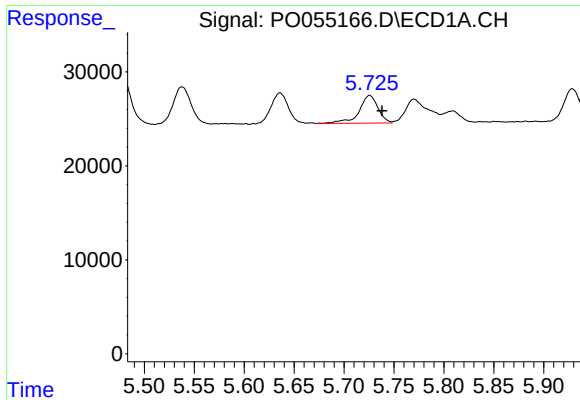

#15 AR-1232-5


R.T.: 5.726 min
Delta R.T.: -0.013 min
Response: 38773
Conc: 93.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

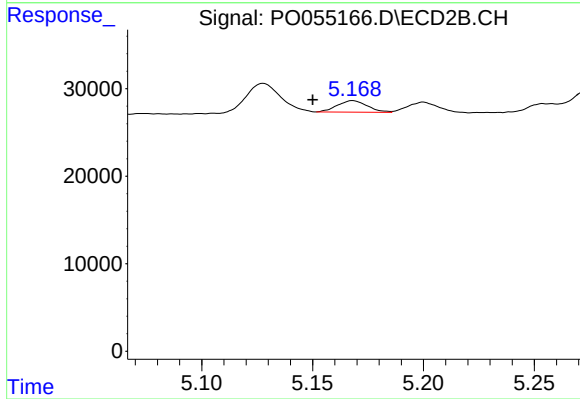


#15 AR-1232-5

R.T.: 5.168 min
Delta R.T.: 0.018 min
Response: 12492
Conc: 25.68 ng/ml

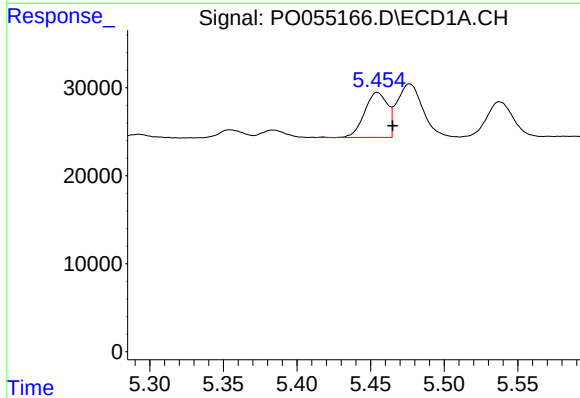


#16 AR-1242-1

R.T.: 5.454 min
Delta R.T.: -0.011 min
Response: 55525
Conc: 39.97 ng/ml

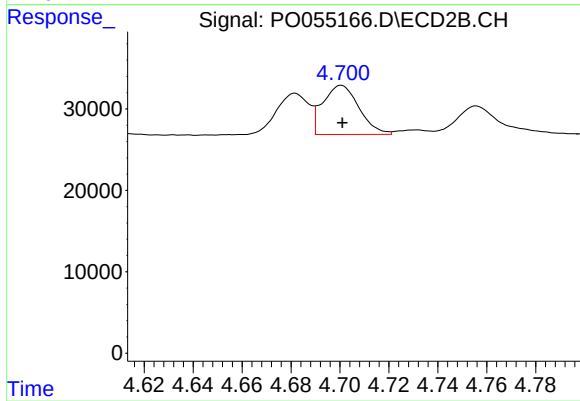

#16 AR-1242-1


R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 61689
Conc: 50.25 ng/ml

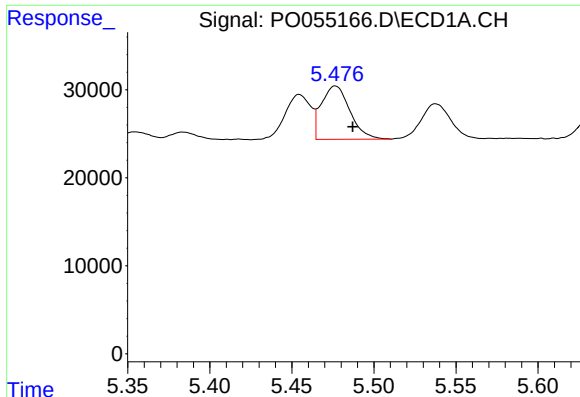

#17 AR-1242-2


R.T.: 5.476 min
Delta R.T.: -0.011 min
Response: 73316
Conc: 38.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

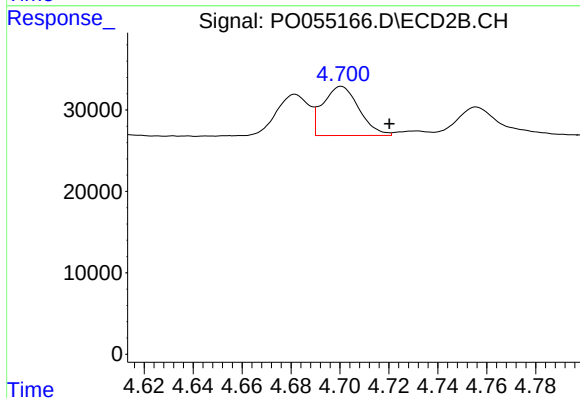


#17 AR-1242-2

R.T.: 4.701 min
Delta R.T.: -0.020 min
Response: 61689
Conc: 37.22 ng/ml

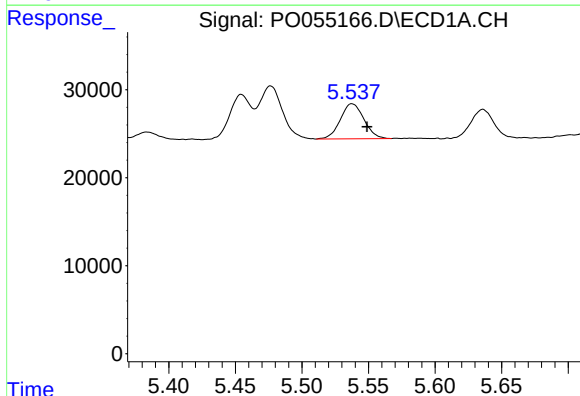


#18 AR-1242-3

R.T.: 5.538 min
Delta R.T.: -0.011 min
Response: 49396
Conc: 39.85 ng/ml

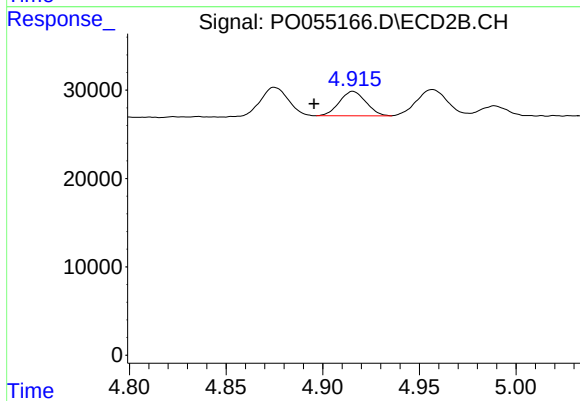

#18 AR-1242-3


R.T.: 4.916 min
Delta R.T.: 0.020 min
Response: 26378
Conc: 27.85 ng/ml

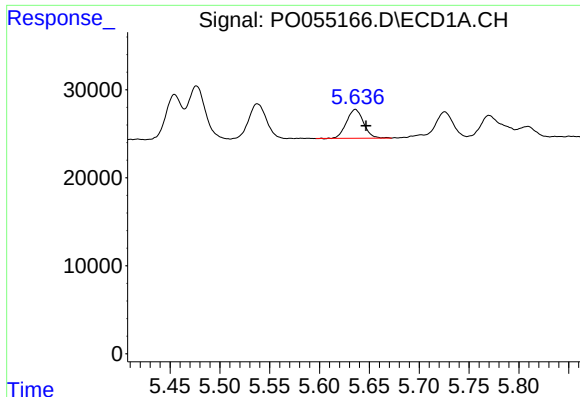

#19 AR-1242-4


R.T.: 5.636 min
Delta R.T.: -0.011 min
Response: 39391
Conc: 38.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

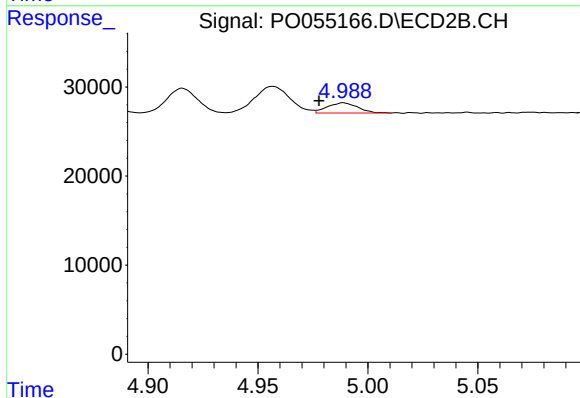


#19 AR-1242-4

R.T.: 4.989 min
Delta R.T.: 0.011 min
Response: 11008
Conc: 11.52 ng/ml

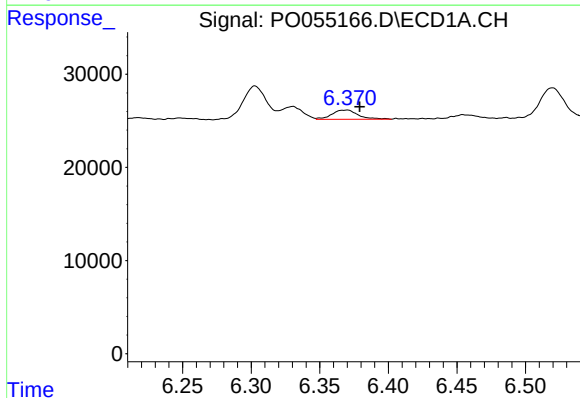


#20 AR-1242-5

R.T.: 6.370 min
Delta R.T.: -0.010 min
Response: 13206
Conc: 10.94 ng/ml

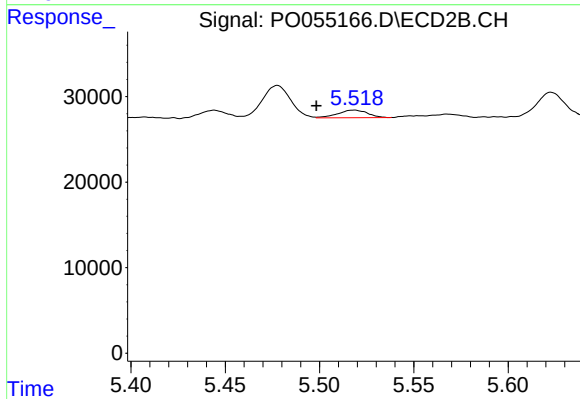

#20 AR-1242-5


R.T.: 5.518 min
Delta R.T.: 0.020 min
Response: 9758
Conc: 7.93 ng/ml

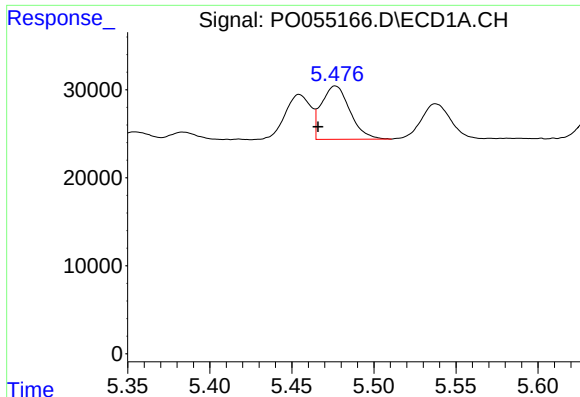

#21 AR-1248-1


R.T.: 5.476 min
Delta R.T.: 0.010 min
Response: 73316
Conc: 73.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

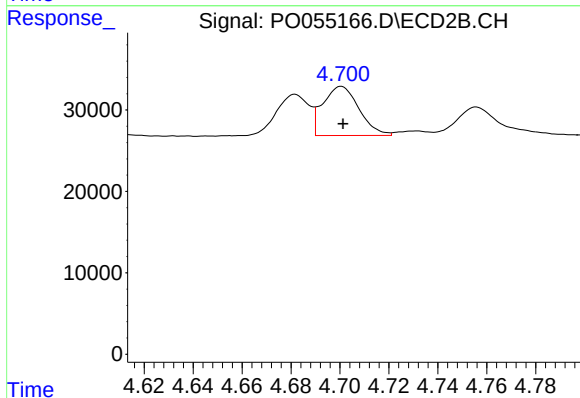


#21 AR-1248-1

R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 61689
Conc: 70.28 ng/ml

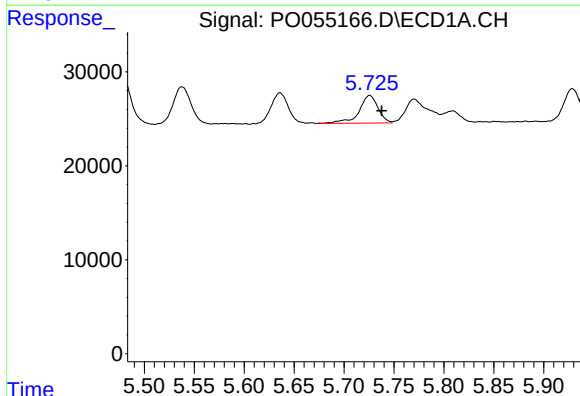


#22 AR-1248-2

R.T.: 5.726 min
Delta R.T.: -0.012 min
Response: 38773
Conc: 26.70 ng/ml

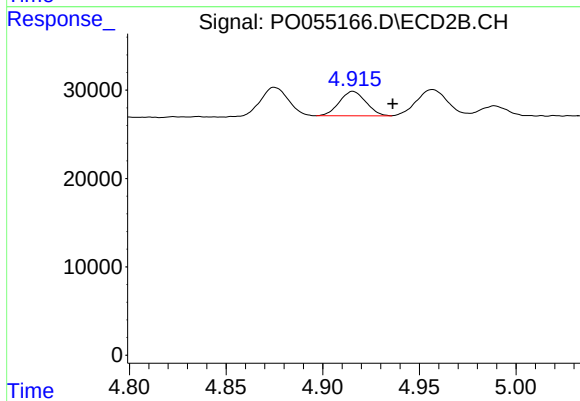

#22 AR-1248-2


R.T.: 4.916 min
Delta R.T.: -0.021 min
Response: 26378
Conc: 21.83 ng/ml

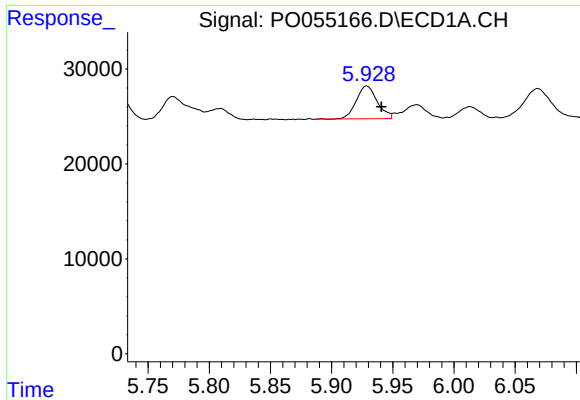

#23 AR-1248-3


R.T.: 5.929 min
Delta R.T.: -0.012 min
Response: 40951
Conc: 25.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

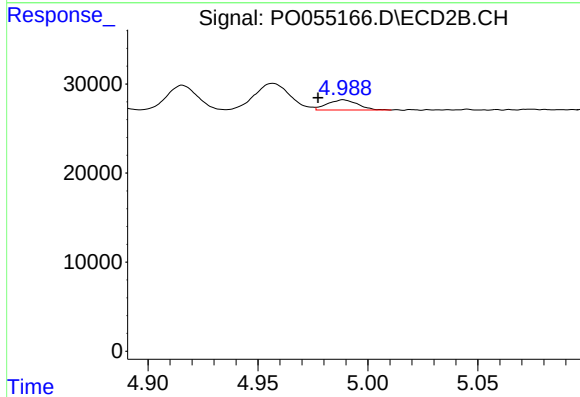


#23 AR-1248-3

R.T.: 4.989 min
Delta R.T.: 0.012 min
Response: 11008
Conc: 8.82 ng/ml

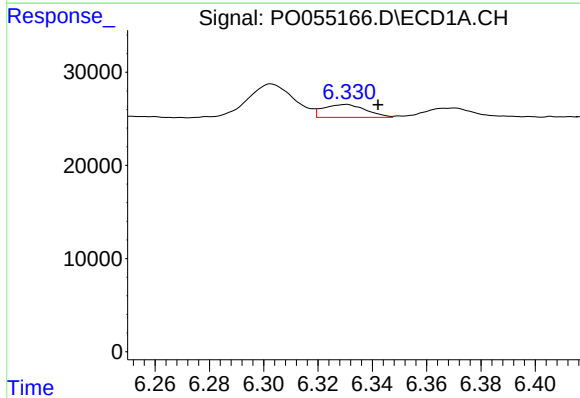


#24 AR-1248-4

R.T.: 6.330 min
Delta R.T.: -0.012 min
Response: 14983
Conc: 7.98 ng/ml

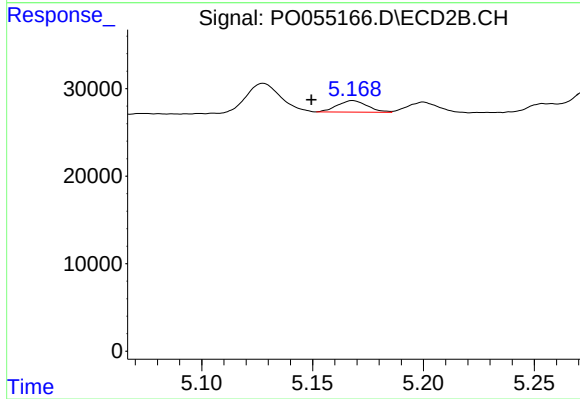

#24 AR-1248-4


R.T.: 5.168 min
Delta R.T.: 0.019 min
Response: 12492
Conc: 8.20 ng/ml

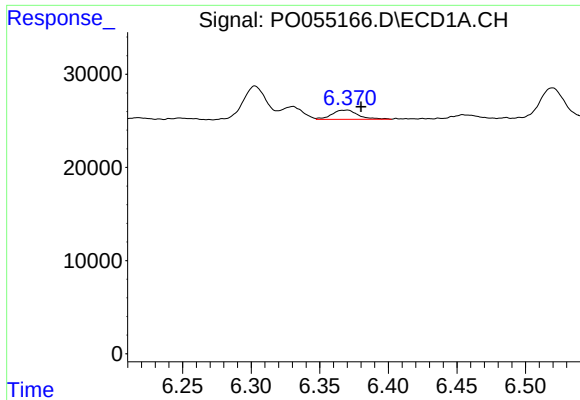

#25 AR-1248-5


R.T.: 6.370 min
Delta R.T.: -0.010 min
Response: 13206
Conc: 7.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

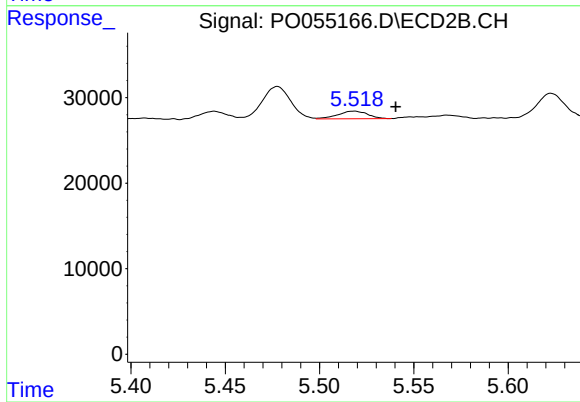


#25 AR-1248-5

R.T.: 5.518 min
Delta R.T.: -0.022 min
Response: 9758
Conc: 6.55 ng/ml

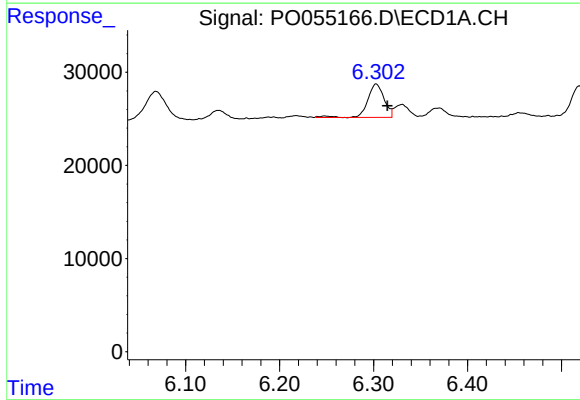


#26 AR-1254-1

R.T.: 6.303 min
Delta R.T.: -0.012 min
Response: 43670
Conc: 24.08 ng/ml

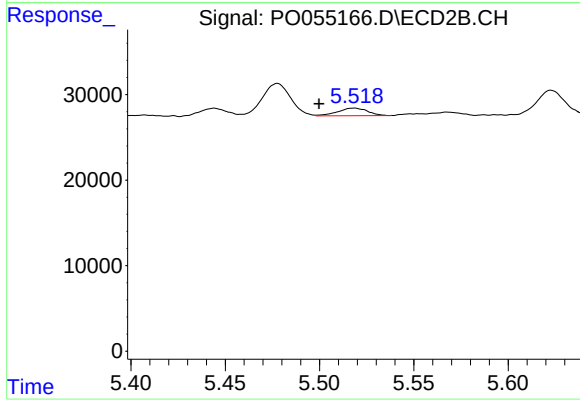

#26 AR-1254-1


R.T.: 5.518 min
Delta R.T.: 0.018 min
Response: 9758
Conc: 4.47 ng/ml

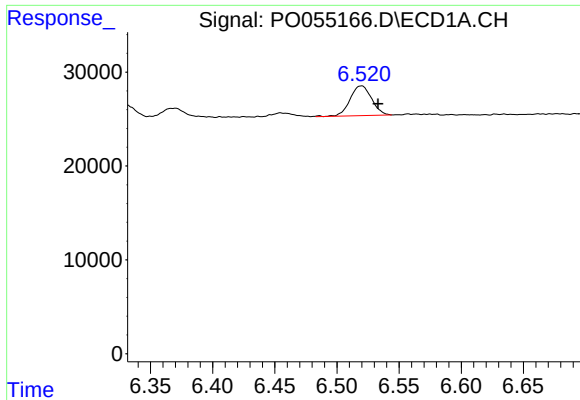

#27 AR-1254-2


R.T.: 6.520 min
Delta R.T.: -0.013 min
Response: 38430
Conc: 13.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

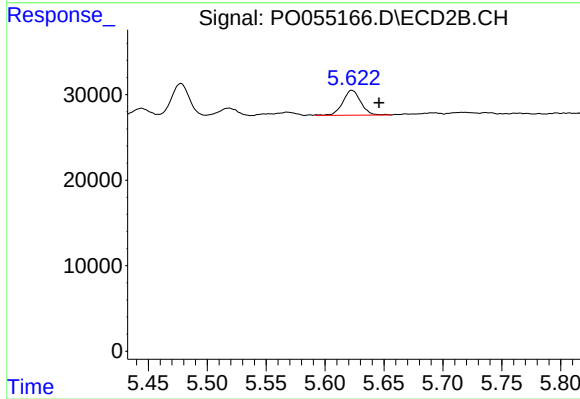


#27 AR-1254-2

R.T.: 5.623 min
Delta R.T.: -0.023 min
Response: 30834
Conc: 15.90 ng/ml

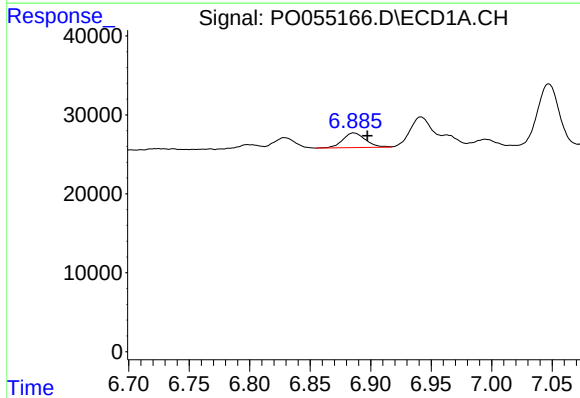


#28 AR-1254-3

R.T.: 6.886 min
Delta R.T.: -0.011 min
Response: 24338
Conc: 7.74 ng/ml

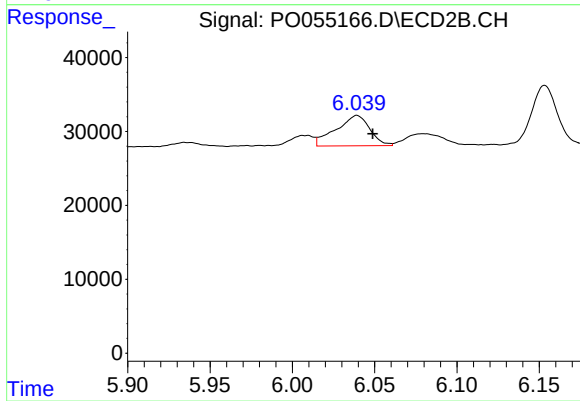

#28 AR-1254-3


R.T.: 6.039 min
Delta R.T.: -0.009 min
Response: 58569
Conc: 18.27 ng/ml

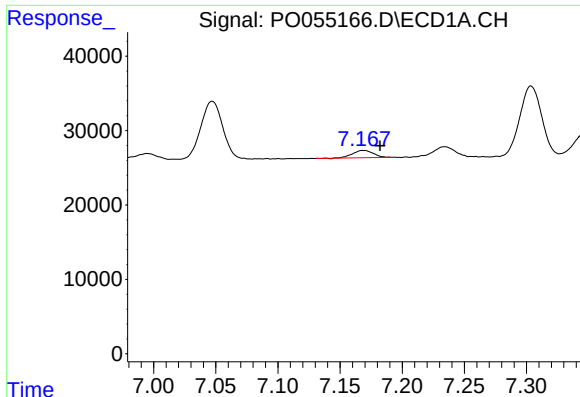

#29 AR-1254-4


R.T.: 7.169 min
Delta R.T.: -0.013 min
Response: 11328
Conc: 4.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

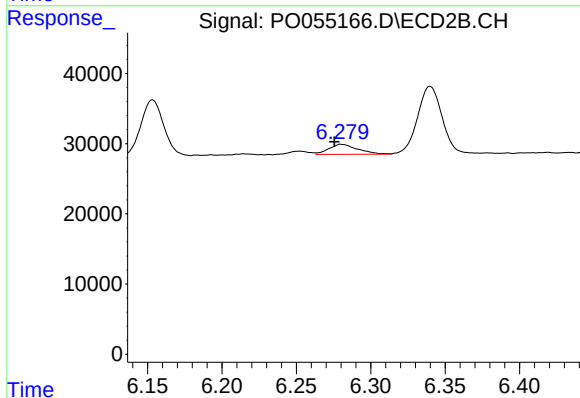


#29 AR-1254-4

R.T.: 6.280 min
Delta R.T.: 0.005 min
Response: 19108
Conc: 9.76 ng/ml

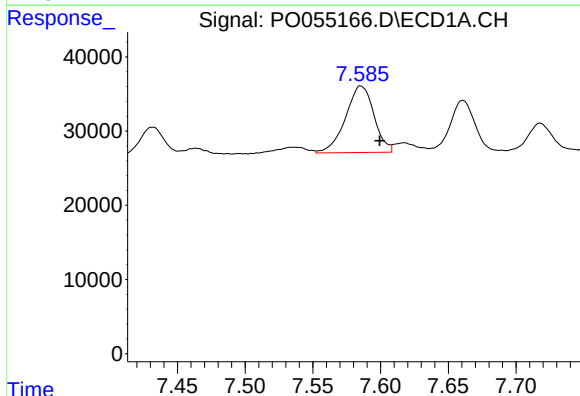


#30 AR-1254-5

R.T.: 7.585 min
Delta R.T.: -0.014 min
Response: 131349
Conc: 49.01 ng/ml

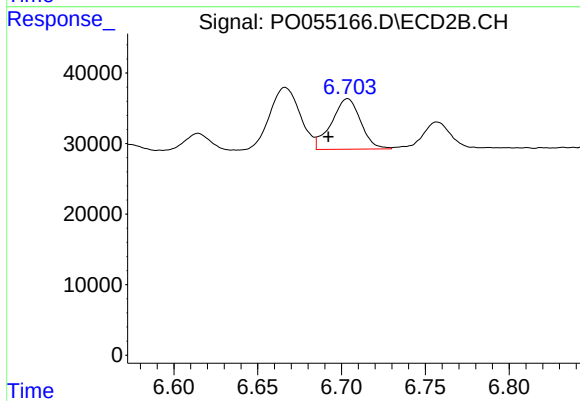

#30 AR-1254-5


R.T.: 6.704 min
Delta R.T.: 0.011 min
Response: 86850
Conc: 30.21 ng/ml

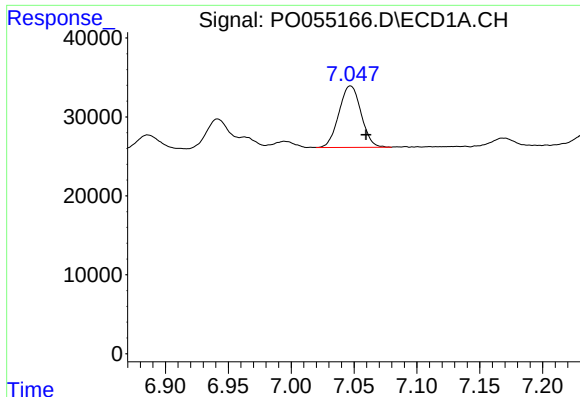

#31 AR-1260-1


R.T.: 7.047 min
Delta R.T.: -0.012 min
Response: 95333
Conc: 37.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

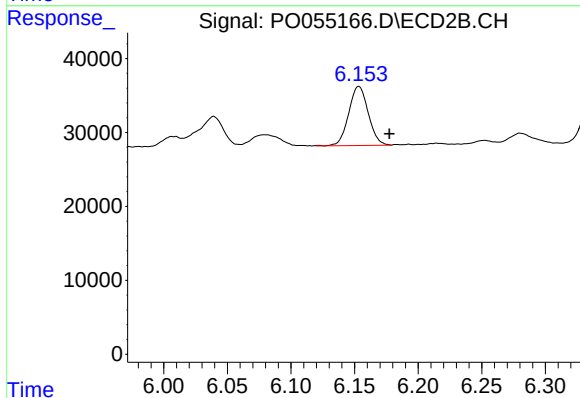


#31 AR-1260-1

R.T.: 6.153 min
Delta R.T.: -0.024 min
Response: 85504
Conc: 37.21 ng/ml

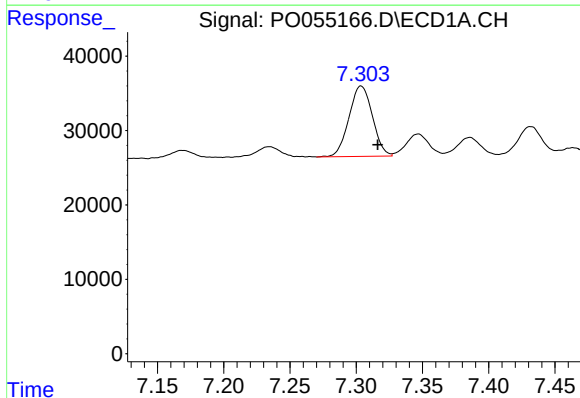


#32 AR-1260-2

R.T.: 7.304 min
Delta R.T.: -0.013 min
Response: 116633
Conc: 37.58 ng/ml

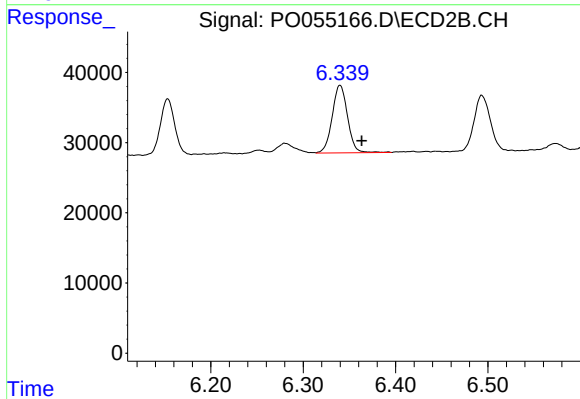

#32 AR-1260-2


R.T.: 6.340 min
Delta R.T.: -0.024 min
Response: 110842
Conc: 40.27 ng/ml

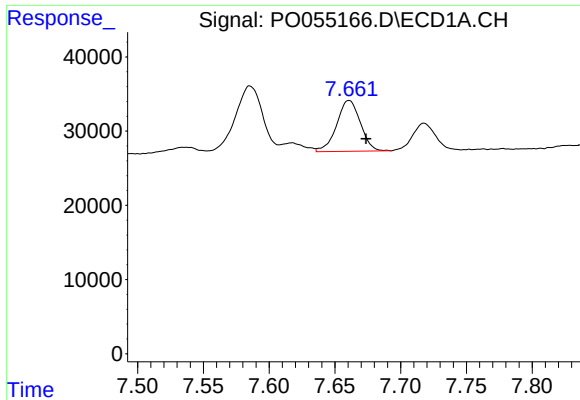

#33 AR-1260-3


R.T.: 7.661 min
Delta R.T.: -0.013 min
Response: 85938
Conc: 35.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

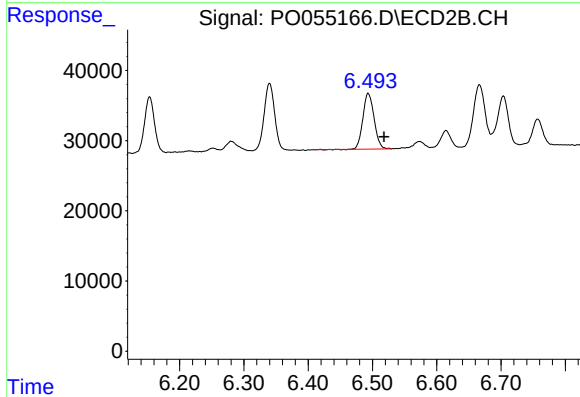


#33 AR-1260-3

R.T.: 6.493 min
Delta R.T.: -0.025 min
Response: 96294
Conc: 37.35 ng/ml

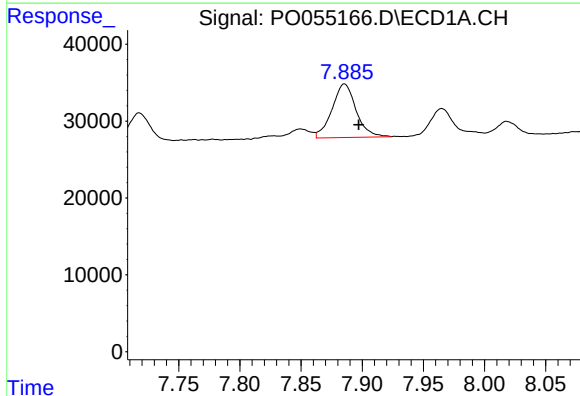


#34 AR-1260-4

R.T.: 7.886 min
Delta R.T.: -0.012 min
Response: 95619
Conc: 34.57 ng/ml

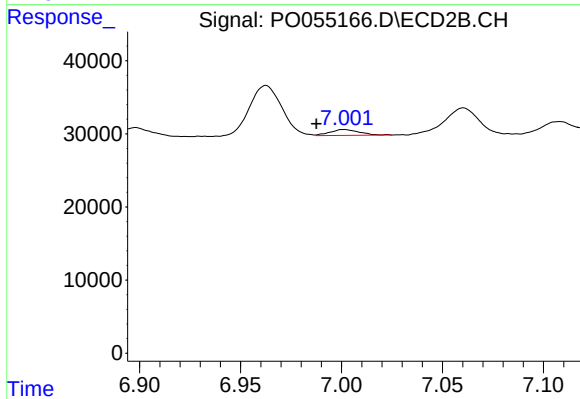

#34 AR-1260-4


R.T.: 7.001 min
Delta R.T.: 0.014 min
Response: 8194
Conc: 3.85 ng/ml

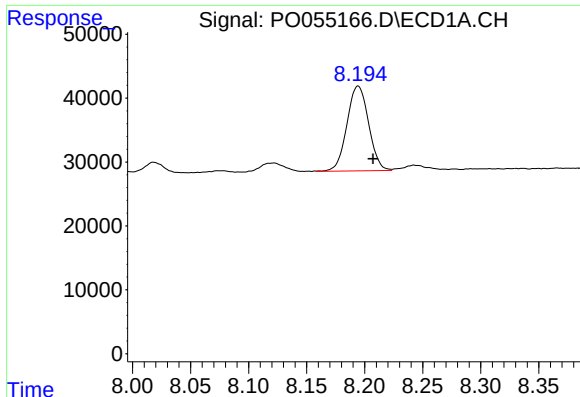

#35 AR-1260-5


R.T.: 8.194 min
Delta R.T.: -0.013 min
Response: 172411
Conc: 31.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

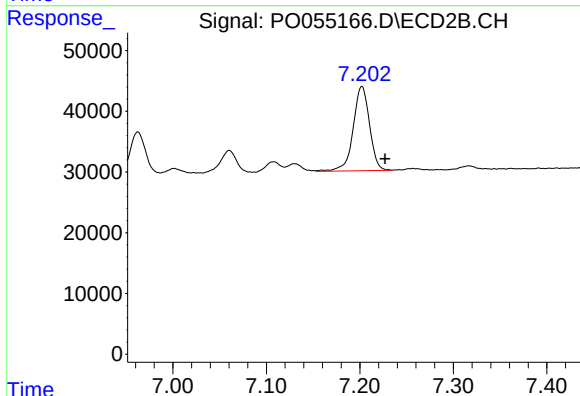


#35 AR-1260-5

R.T.: 7.202 min
Delta R.T.: -0.025 min
Response: 168455
Conc: 35.17 ng/ml

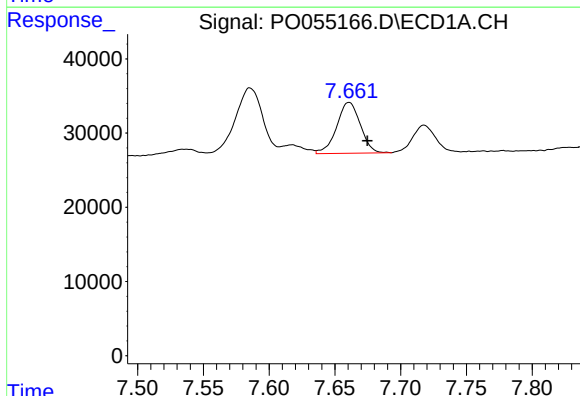


#36 AR-1262-1

R.T.: 7.661 min
Delta R.T.: -0.014 min
Response: 85938
Conc: 25.79 ng/ml

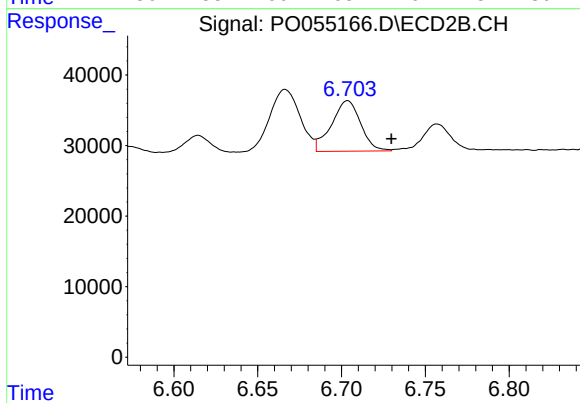

#36 AR-1262-1


R.T.: 6.704 min
Delta R.T.: -0.026 min
Response: 86850
Conc: 29.19 ng/ml

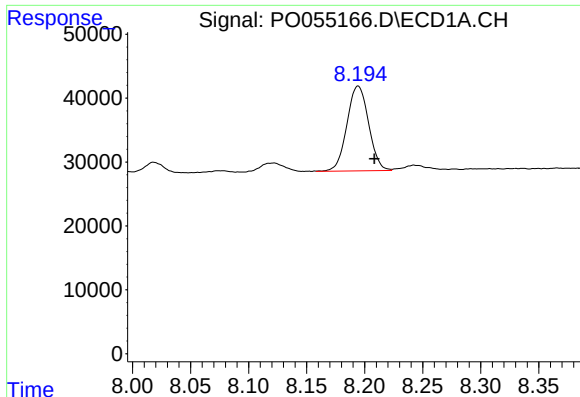

#37 AR-1262-2


R.T.: 8.194 min
Delta R.T.: -0.014 min
Response: 172411
Conc: 29.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

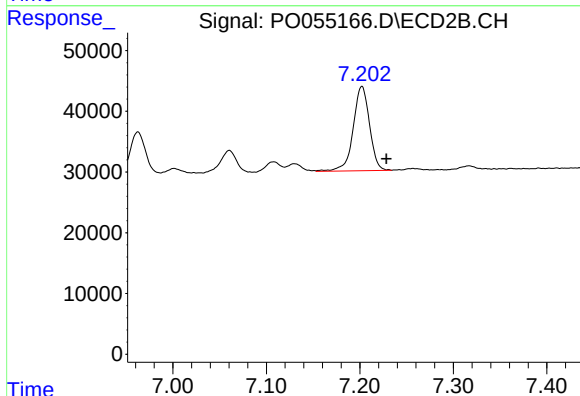


#37 AR-1262-2

R.T.: 7.202 min
Delta R.T.: -0.026 min
Response: 168455
Conc: 34.37 ng/ml

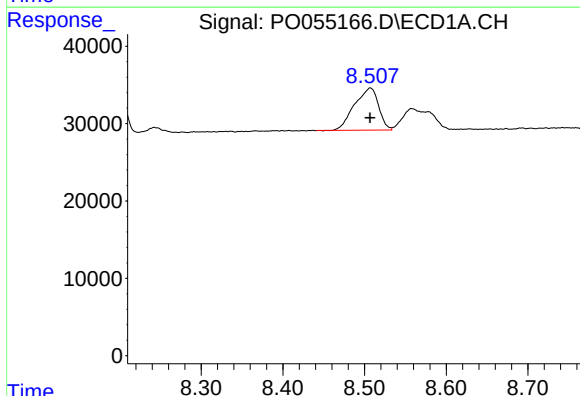


#38 AR-1262-3

R.T.: 8.507 min
Delta R.T.: 0.000 min
Response: 111486
Conc: 26.91 ng/ml

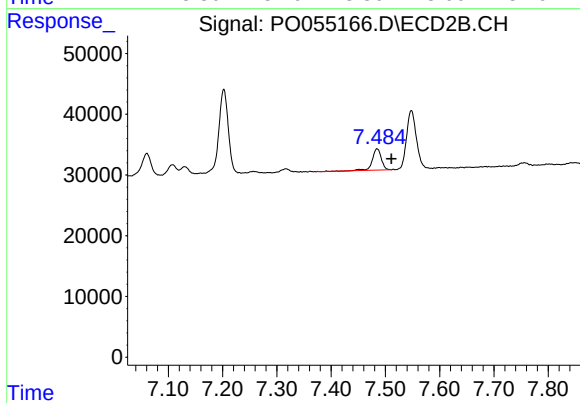

#38 AR-1262-3


R.T.: 7.485 min
Delta R.T.: -0.026 min
Response: 40550
Conc: 19.75 ng/ml

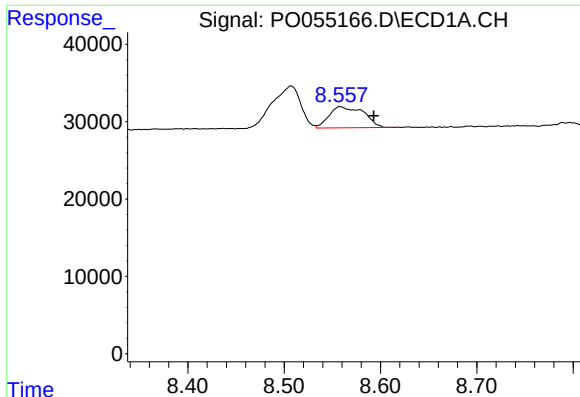

#39 AR-1262-4


R.T.: 8.558 min
Delta R.T.: -0.035 min
Response: 68059
Conc: 21.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

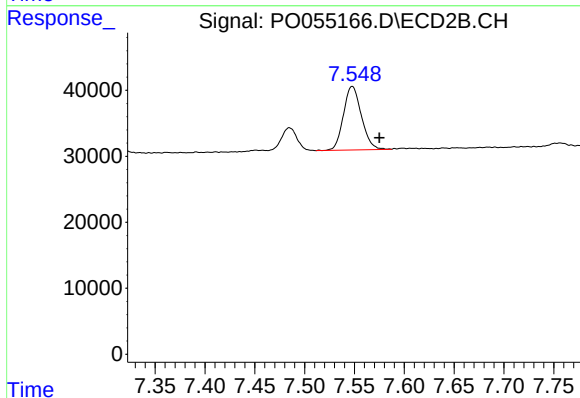


#39 AR-1262-4

R.T.: 7.548 min
Delta R.T.: -0.027 min
Response: 121303
Conc: 33.49 ng/ml

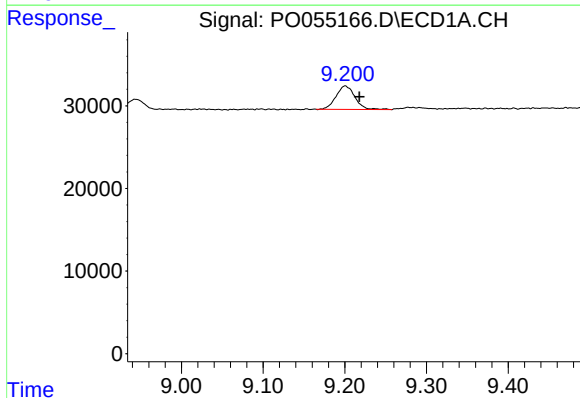


#40 AR-1262-5

R.T.: 9.200 min
Delta R.T.: -0.018 min
Response: 45736
Conc: 20.92 ng/ml

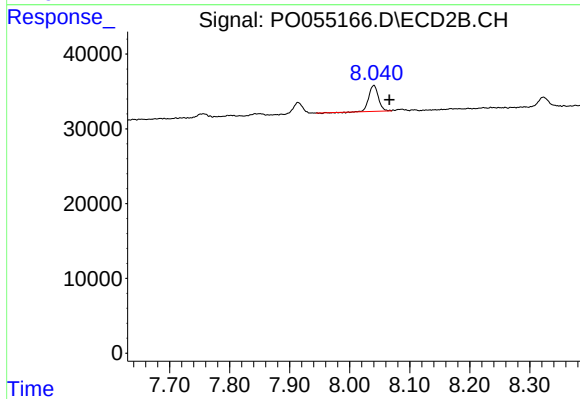

#40 AR-1262-5


R.T.: 8.040 min
Delta R.T.: -0.026 min
Response: 38187
Conc: 23.66 ng/ml

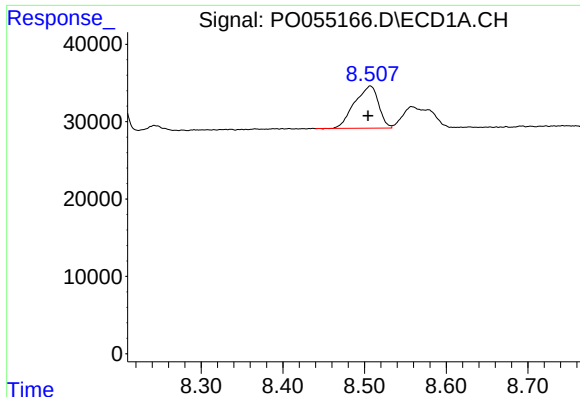

#41 AR-1268-1


R.T.: 8.507 min
Delta R.T.: 0.003 min
Response: 111486
Conc: 15.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

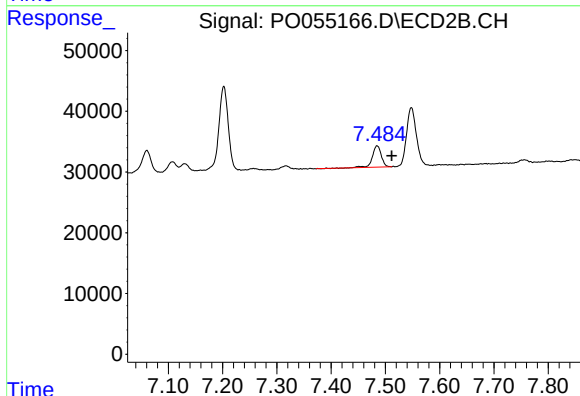


#41 AR-1268-1

R.T.: 7.485 min
Delta R.T.: -0.027 min
Response: 40550
Conc: 7.17 ng/ml

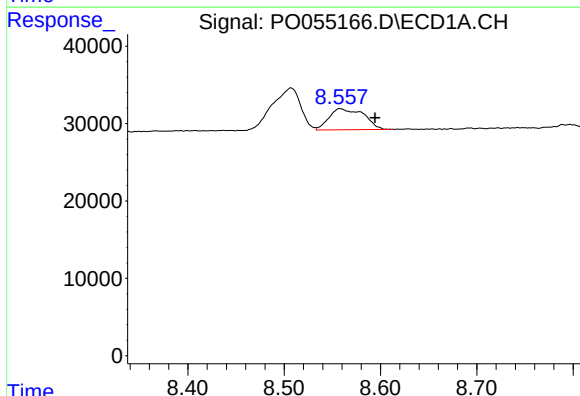


#42 AR-1268-2

R.T.: 8.558 min
Delta R.T.: -0.036 min
Response: 68059
Conc: 10.39 ng/ml

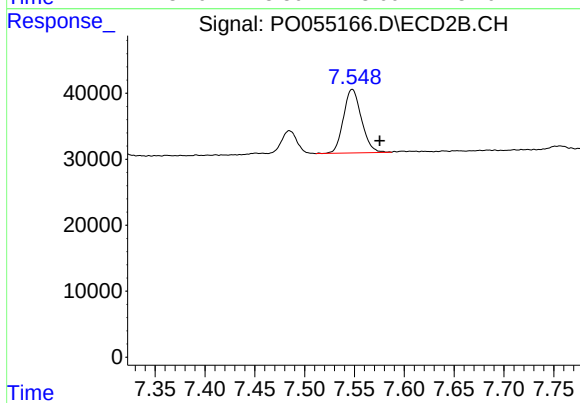

#42 AR-1268-2


R.T.: 7.548 min
Delta R.T.: -0.027 min
Response: 121303
Conc: 23.46 ng/ml

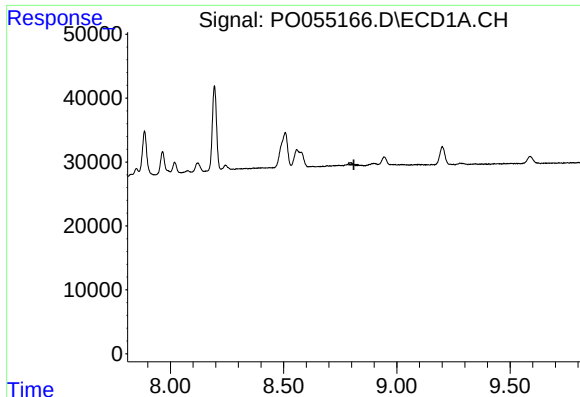

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.810 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

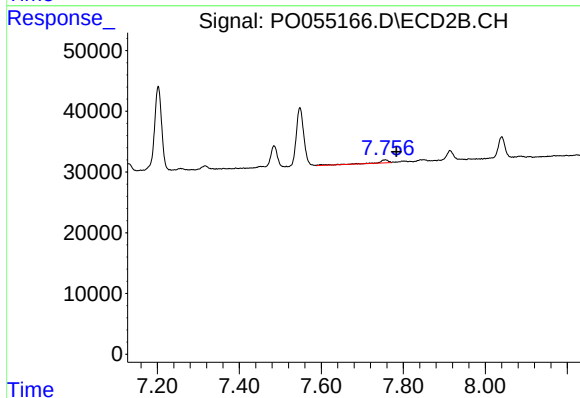


#43 AR-1268-3

R.T.: 7.756 min
Delta R.T.: -0.026 min
Response: 8701
Conc: 2.02 ng/ml

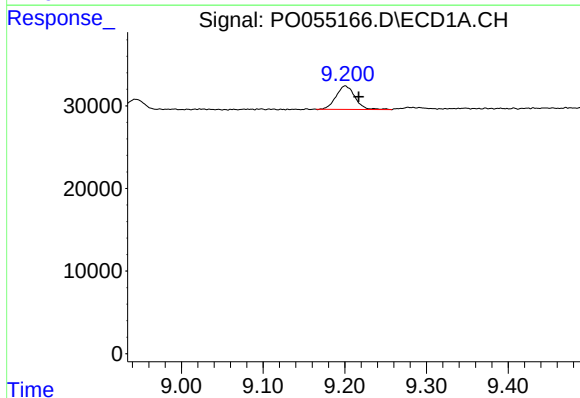


#44 AR-1268-4

R.T.: 9.200 min
Delta R.T.: -0.017 min
Response: 45736
Conc: 19.17 ng/ml

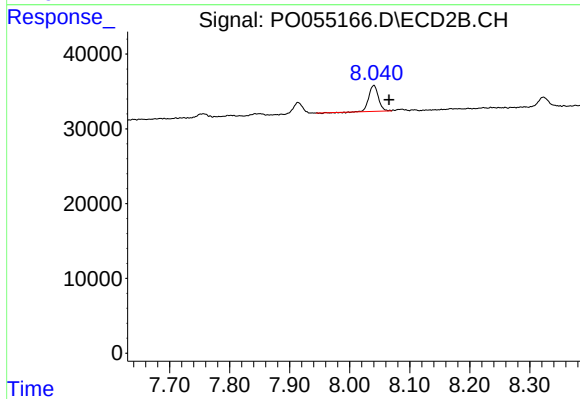

#44 AR-1268-4


R.T.: 8.040 min
Delta R.T.: -0.025 min
Response: 38187
Conc: 20.60 ng/ml

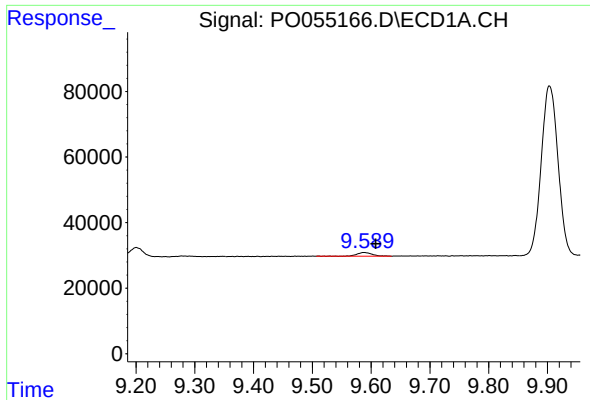

#45 AR-1268-5

R.T.: 9.588 min
Delta R.T.: -0.020 min
Response: 20270
Conc: 1.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

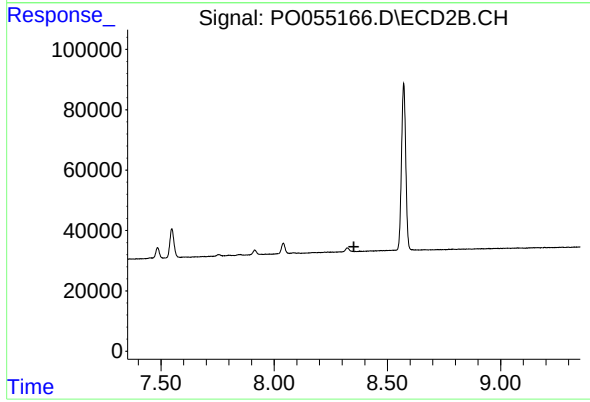

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.352 min
Response: 0
Conc: N.D.