

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041119\
 Data File : P0055167.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Apr 2019 20:11
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1660 LOD 40PPB
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 02:42:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.293	3.606	715015	641337	20.603	20.097
2)	SA Decachlor...	9.904	8.572	1053368	747720	21.368	23.478
Target Compounds							
3)	L1 AR-1016-1	5.476	4.701	121943	103392	67.768	65.380
4)	L1 AR-1016-2	5.476	4.701	121943	103392	49.098	48.252
5)	L1 AR-1016-3	5.537	4.875	84647	51305	53.804	42.463
6)	L1 AR-1016-4	5.636	4.916	67119	45179	51.508	44.708
7)	L1 AR-1016-5	5.928	5.168	71238	20659	53.391	15.850 #
8)	L2 AR-1221-1	0.000	3.903	0	17472	N.D.	44.938 #
9)	L2 AR-1221-2	4.592	3.903	19266	17472	56.812	58.279
10)	L2 AR-1221-3	4.664	3.978	43624	36200	41.996	39.272
11)	L3 AR-1232-1	4.664	3.978	43624	36200	50.669	48.274
12)	L3 AR-1232-2	5.188	4.701	62522	103392	127.820	120.069
13)	L3 AR-1232-3	5.476	4.916	121943	45179	124.775	93.236 #
14)	L3 AR-1232-4	5.636	4.989	67119	19933	131.130	45.363 #
15)	L3 AR-1232-5	5.725	5.168	65111	20659	156.519	42.476 #
16)	L4 AR-1242-1	5.454	4.701	93502	103392	67.302	84.215 #
17)	L4 AR-1242-2	5.476	4.701	121943	103392	63.729	62.389
18)	L4 AR-1242-3	5.537	4.875	84647	51305	68.293	54.158
19)	L4 AR-1242-4	5.636	4.989	67119	19933	65.832	20.855 #
20)	L4 AR-1242-5	6.368	5.478	20835	66014	17.259	53.675 #
21)	L5 AR-1248-1	5.476	4.701	121943	103392	121.982	117.789
22)	L5 AR-1248-2	5.725	4.916	65111	45179	44.833	37.383
23)	L5 AR-1248-3	5.928	4.989	71238	19933	44.603	15.974 #
24)	L5 AR-1248-4	6.329	5.168	25487	20659	13.568	13.565
25)	L5 AR-1248-5	6.368	5.519	20835	14989	11.621	10.054
26)	L6 AR-1254-1	6.302	5.519	70296	14989	38.769	6.858 #
27)	L6 AR-1254-2	6.520	5.623	64235	50363	22.501	25.974
28)	L6 AR-1254-3	6.886	6.040	35816	95145	11.389	29.680 #
29)	L6 AR-1254-4	7.169	6.281	22001	31976	8.994	16.331 #
30)	L6 AR-1254-5	7.586	6.705	208138	134941	77.655	46.941 #
31)	L7 AR-1260-1	7.047	6.154	155347	139081	61.826	60.521
32)	L7 AR-1260-2	7.304	6.340	183766	169371	59.212	61.528
33)	L7 AR-1260-3	7.660	6.494	137630	152918	56.076	59.319
34)	L7 AR-1260-4	7.886	7.002	159074	14442	57.510	6.786 #
35)	L7 AR-1260-5	8.195	7.203	283853	267125	51.157	55.775
36)	L8 AR-1262-1	7.660	6.705	137630	134941	41.305	45.359
37)	L8 AR-1262-2	8.195	7.203	283853	267125	47.912	54.503
38)	L8 AR-1262-3	8.505	7.484	189642	62570	45.776	30.471 #
39)	L8 AR-1262-4	8.577	7.548	45112	188967	14.001	52.170 #
40)	L8 AR-1262-5	9.201	8.040	75680	61521	34.616	38.120
41)	L9 AR-1268-1	8.505	7.484	189642	62570	26.645	11.066 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041119\
 Data File : P0055167.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Apr 2019 20:11
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1660 LOD 40PPB
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 02:42:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.577	7.548	45112	188967	6.885	36.540 #
43) L9	AR-1268-3	0.000	7.757	0	9370	N.D.	2.177 #
44) L9	AR-1268-4	9.201	8.040	75680	61521	31.721	33.185
45) L9	AR-1268-5	9.589	0.000	31619	0	1.919	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041119\
Data File : P0055167.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Apr 2019 20:11
Operator : SM/SJ
Sample : K1560-07
Misc : AR1660 LOD 40PPB
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 02:42:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

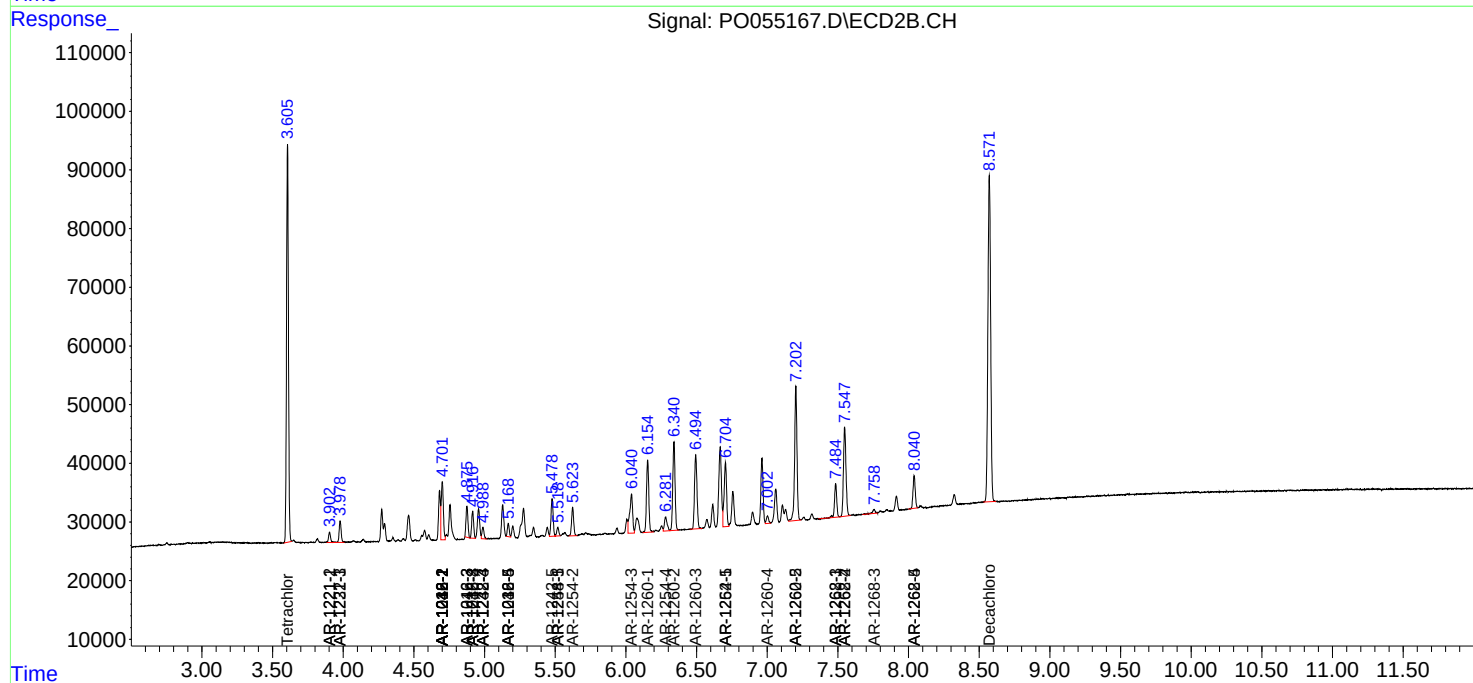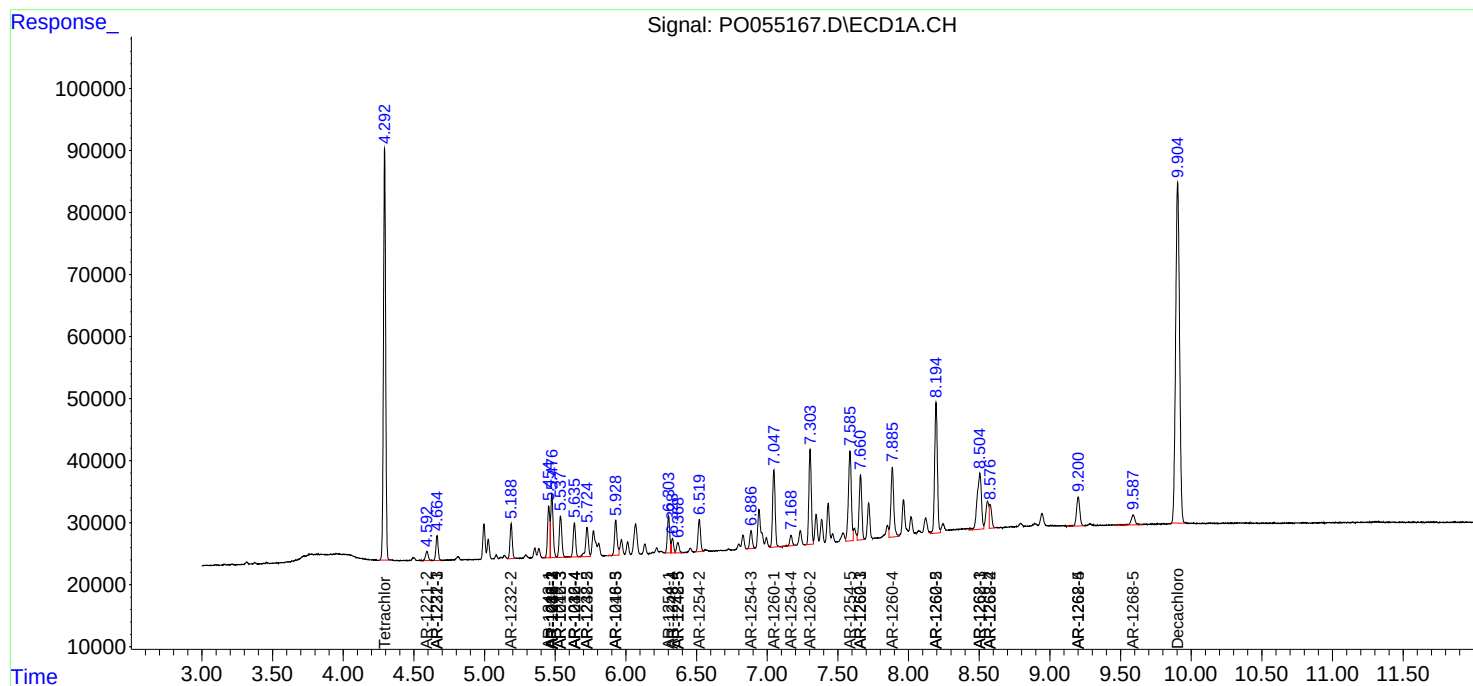


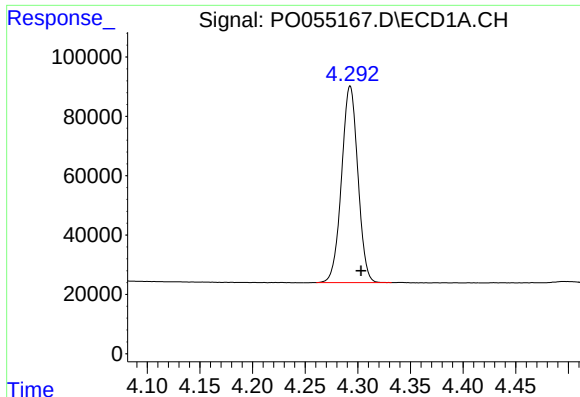

#1 Tetrachloro-m-xylene


R.T.: 4.293 min
Delta R.T.: -0.010 min
Response: 715015
Conc: 20.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

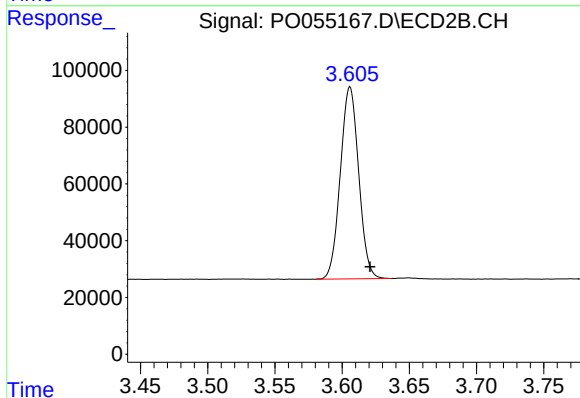


#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: -0.015 min
Response: 641337
Conc: 20.10 ng/ml

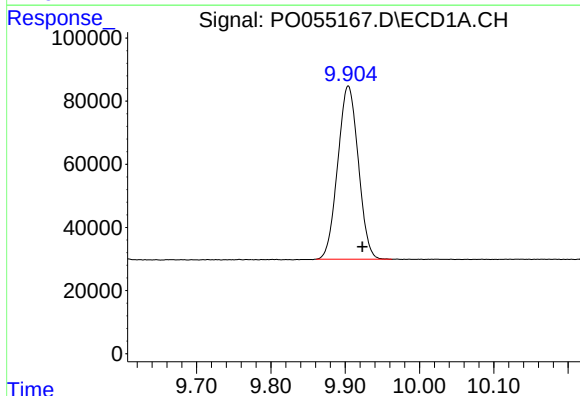


#2 Decachlorobiphenyl

R.T.: 9.904 min
Delta R.T.: -0.019 min
Response: 1053368
Conc: 21.37 ng/ml

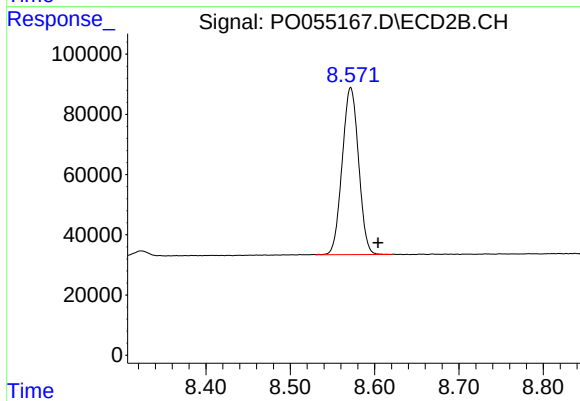

#2 Decachlorobiphenyl


R.T.: 8.572 min
Delta R.T.: -0.032 min
Response: 747720
Conc: 23.48 ng/ml

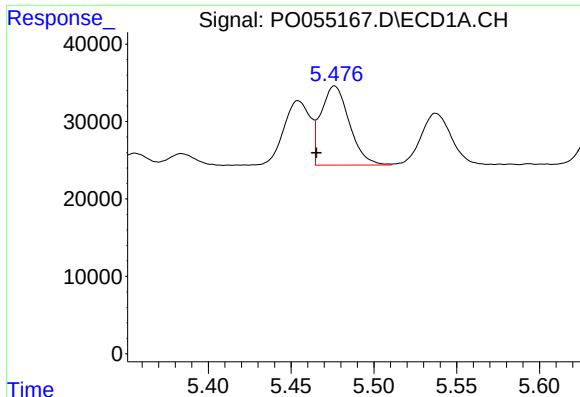

#3 AR-1016-1


R.T.: 5.476 min
Delta R.T.: 0.011 min
Response: 121943
Conc: 67.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

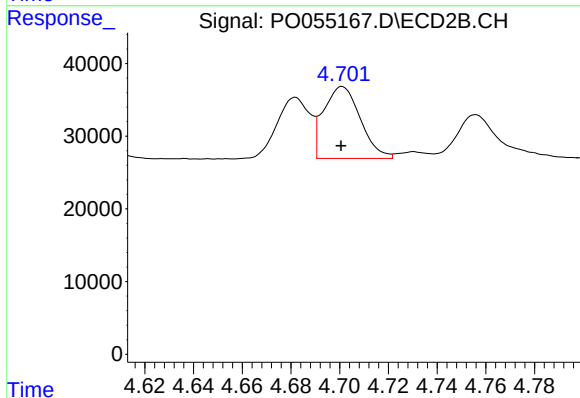


#3 AR-1016-1

R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 103392
Conc: 65.38 ng/ml

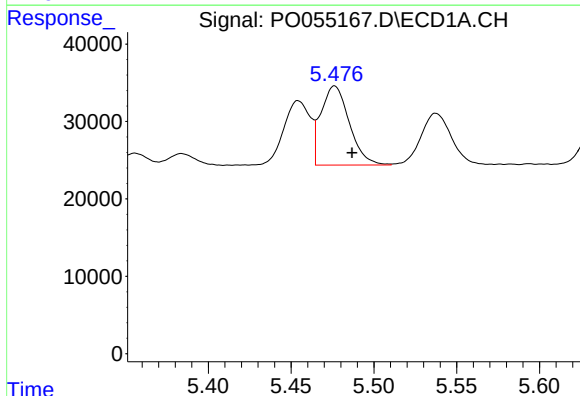


#4 AR-1016-2

R.T.: 5.476 min
Delta R.T.: -0.010 min
Response: 121943
Conc: 49.10 ng/ml

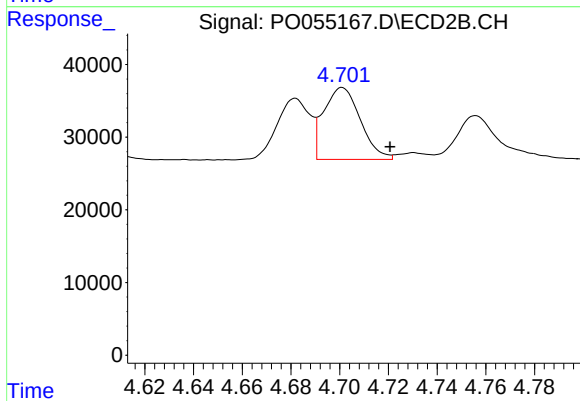

#4 AR-1016-2


R.T.: 4.701 min
Delta R.T.: -0.020 min
Response: 103392
Conc: 48.25 ng/ml

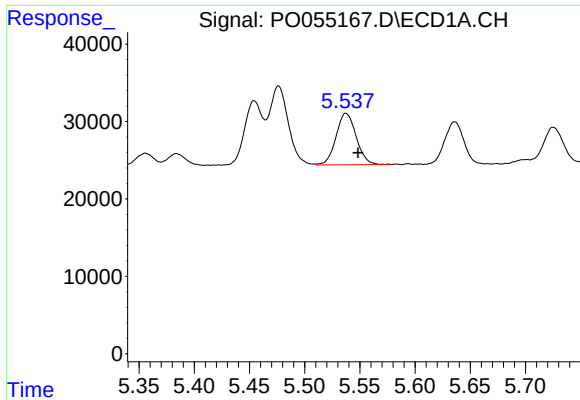

#5 AR-1016-3


R.T.: 5.537 min
Delta R.T.: -0.011 min
Response: 84647
Conc: 53.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

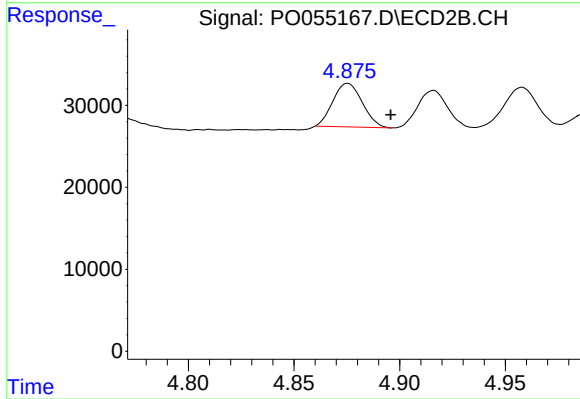


#5 AR-1016-3

R.T.: 4.875 min
Delta R.T.: -0.020 min
Response: 51305
Conc: 42.46 ng/ml

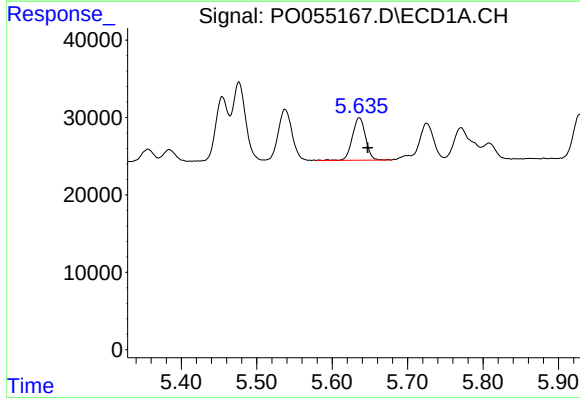


#6 AR-1016-4

R.T.: 5.636 min
Delta R.T.: -0.011 min
Response: 67119
Conc: 51.51 ng/ml

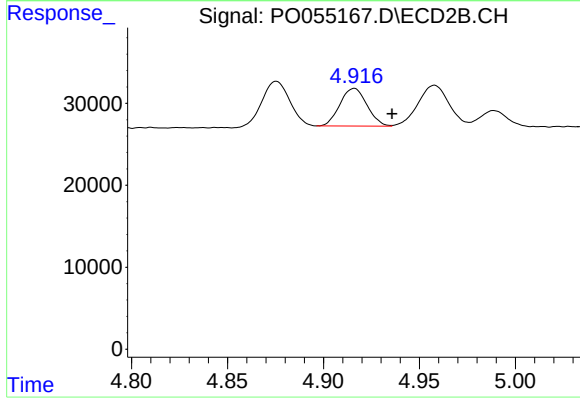

#6 AR-1016-4


R.T.: 4.916 min
Delta R.T.: -0.019 min
Response: 45179
Conc: 44.71 ng/ml

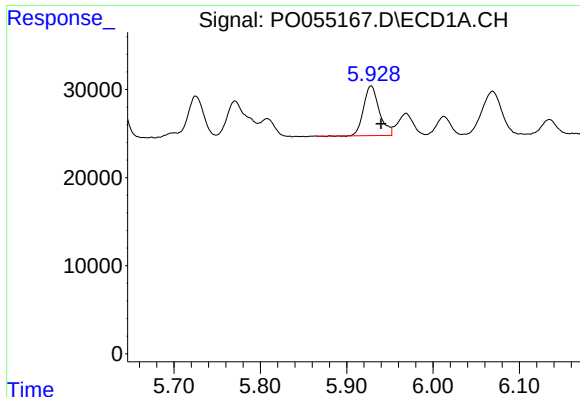

#7 AR-1016-5


R.T.: 5.928 min
Delta R.T.: -0.011 min
Response: 71238
Conc: 53.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

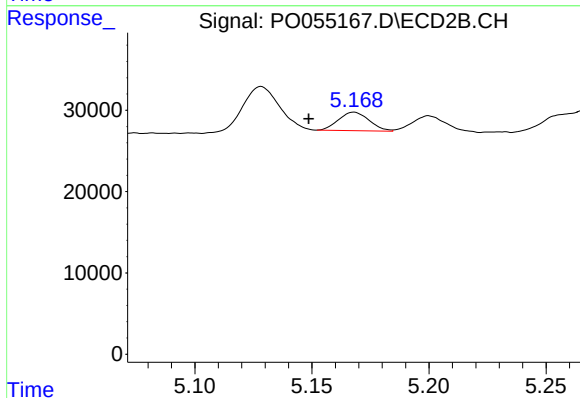


#7 AR-1016-5

R.T.: 5.168 min
Delta R.T.: 0.019 min
Response: 20659
Conc: 15.85 ng/ml

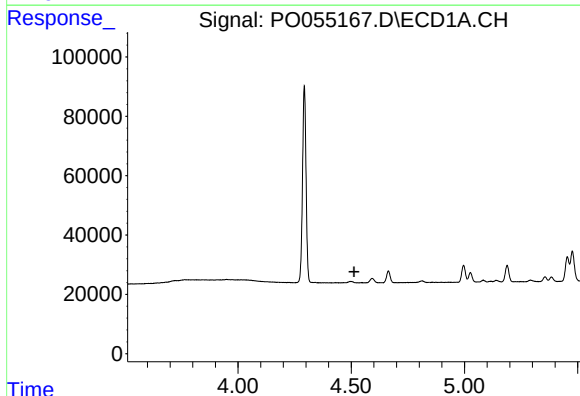


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.512 min
Response: 0
Conc: N.D.

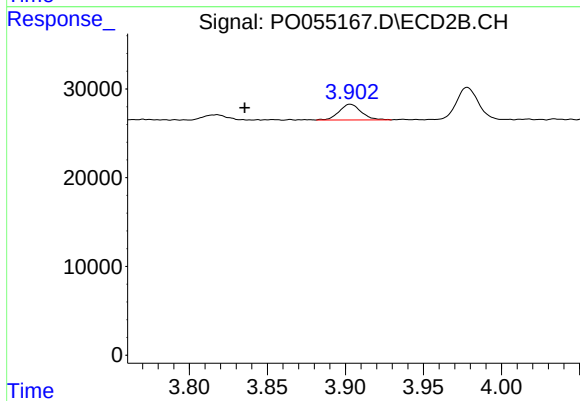

#8 AR-1221-1


R.T.: 3.903 min
Delta R.T.: 0.067 min
Response: 17472
Conc: 44.94 ng/ml

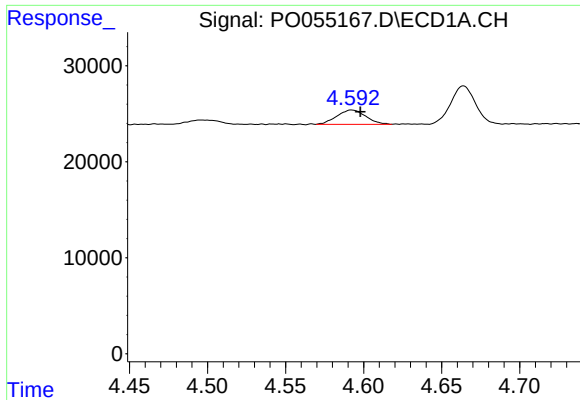

#9 AR-1221-2


R.T.: 4.592 min
Delta R.T.: -0.006 min
Response: 19266
Conc: 56.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

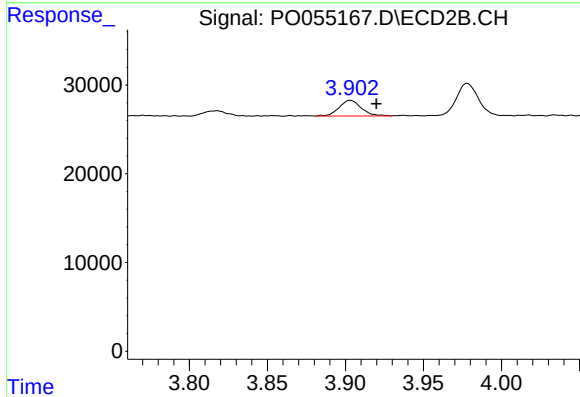


#9 AR-1221-2

R.T.: 3.903 min
Delta R.T.: -0.017 min
Response: 17472
Conc: 58.28 ng/ml

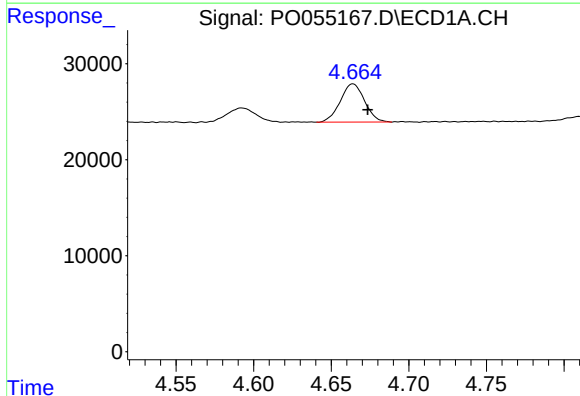


#10 AR-1221-3

R.T.: 4.664 min
Delta R.T.: -0.009 min
Response: 43624
Conc: 42.00 ng/ml

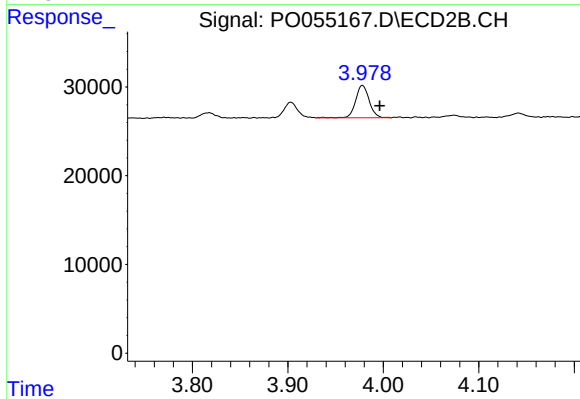

#10 AR-1221-3


R.T.: 3.978 min
Delta R.T.: -0.018 min
Response: 36200
Conc: 39.27 ng/ml

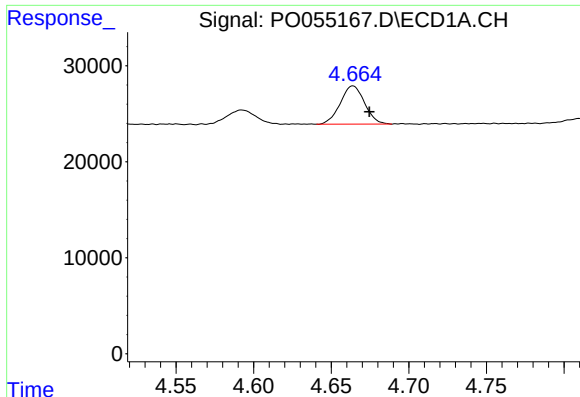

#11 AR-1232-1


R.T.: 4.664 min
Delta R.T.: -0.011 min
Response: 43624
Conc: 50.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

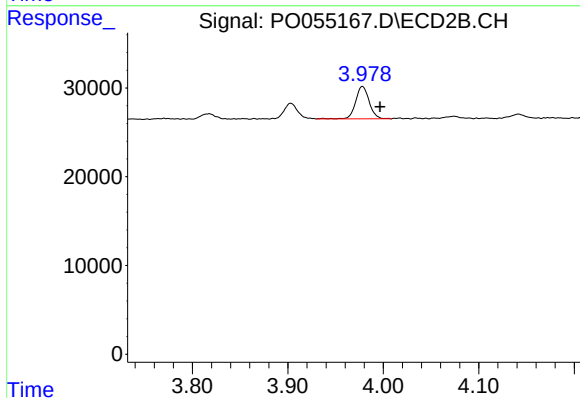


#11 AR-1232-1

R.T.: 3.978 min
Delta R.T.: -0.019 min
Response: 36200
Conc: 48.27 ng/ml

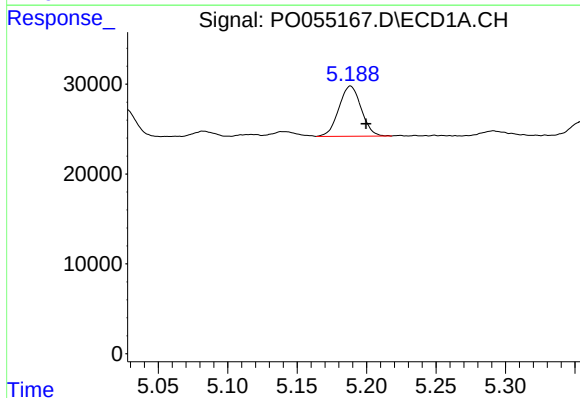


#12 AR-1232-2

R.T.: 5.188 min
Delta R.T.: -0.011 min
Response: 62522
Conc: 127.82 ng/ml

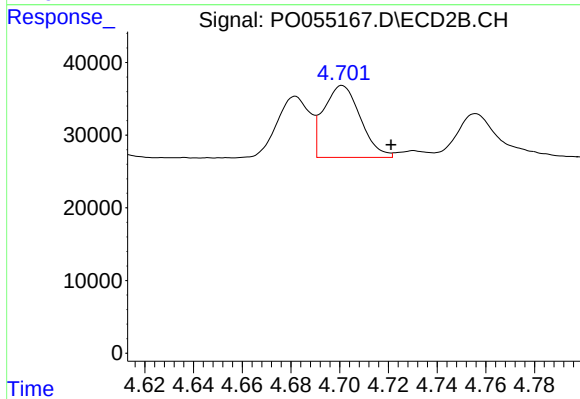

#12 AR-1232-2


R.T.: 4.701 min
Delta R.T.: -0.020 min
Response: 103392
Conc: 120.07 ng/ml

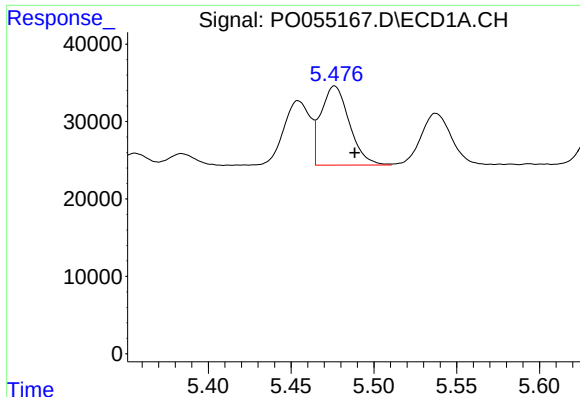

#13 AR-1232-3


R.T.: 5.476 min
Delta R.T.: -0.012 min
Response: 121943
Conc: 124.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

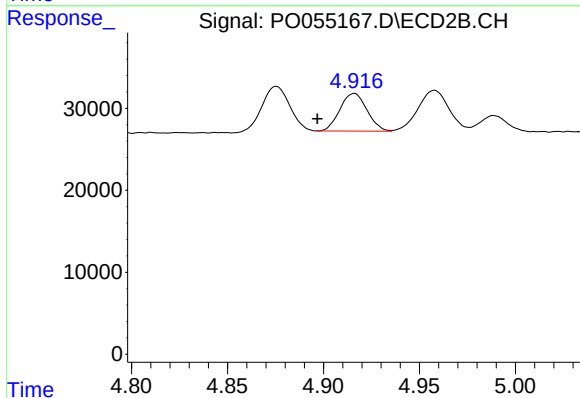


#13 AR-1232-3

R.T.: 4.916 min
Delta R.T.: 0.019 min
Response: 45179
Conc: 93.24 ng/ml

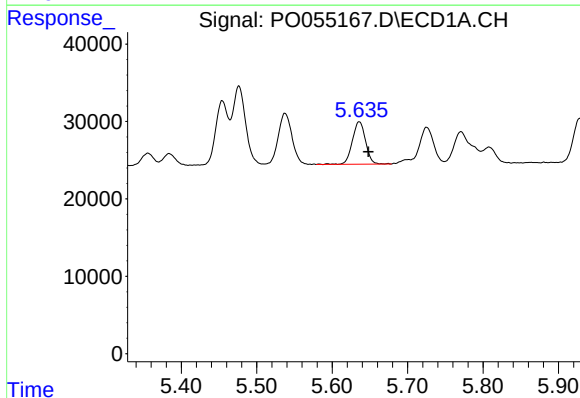


#14 AR-1232-4

R.T.: 5.636 min
Delta R.T.: -0.012 min
Response: 67119
Conc: 131.13 ng/ml

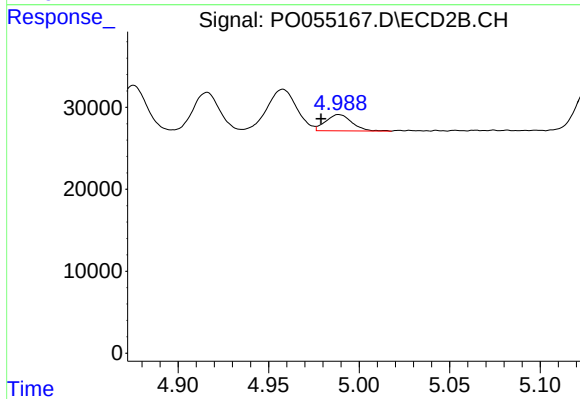

#14 AR-1232-4


R.T.: 4.989 min
Delta R.T.: 0.010 min
Response: 19933
Conc: 45.36 ng/ml

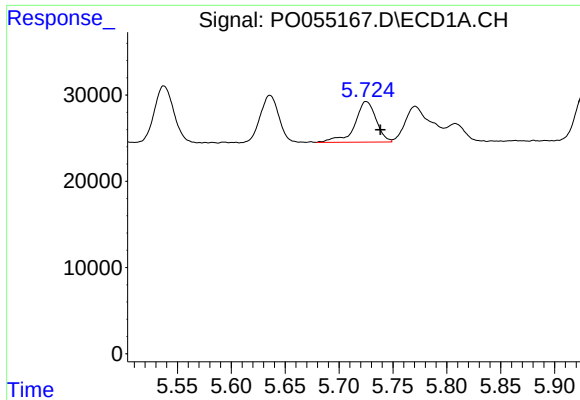

#15 AR-1232-5


R.T.: 5.725 min
Delta R.T.: -0.013 min
Response: 65111
Conc: 156.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

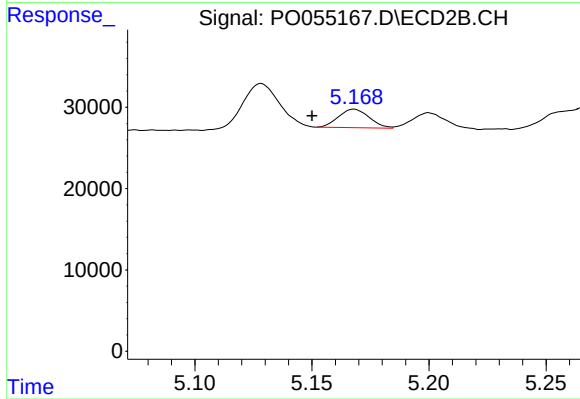


#15 AR-1232-5

R.T.: 5.168 min
Delta R.T.: 0.018 min
Response: 20659
Conc: 42.48 ng/ml

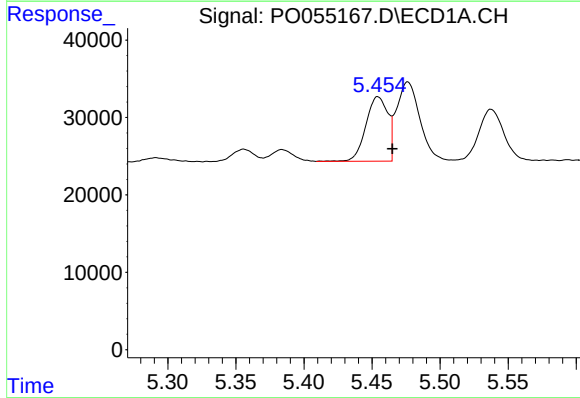


#16 AR-1242-1

R.T.: 5.454 min
Delta R.T.: -0.011 min
Response: 93502
Conc: 67.30 ng/ml

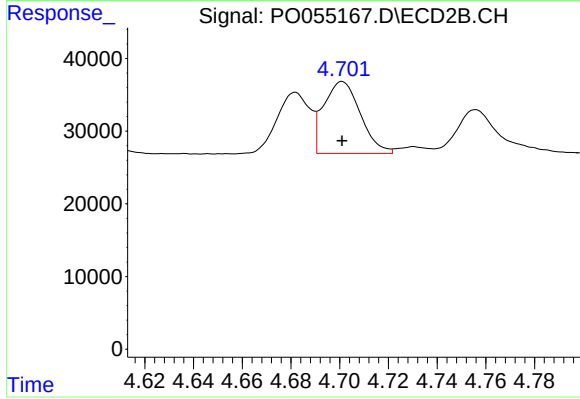

#16 AR-1242-1


R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 103392
Conc: 84.22 ng/ml

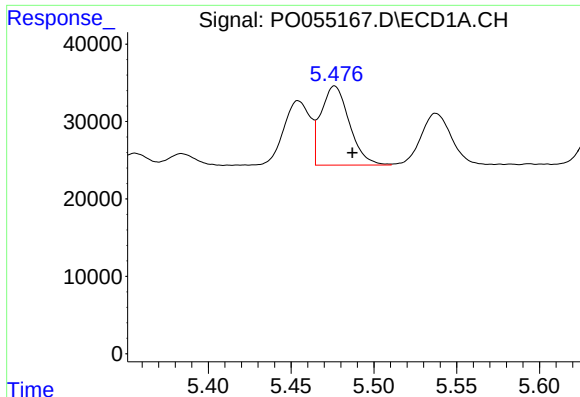

#17 AR-1242-2


R.T.: 5.476 min
Delta R.T.: -0.011 min
Response: 121943
Conc: 63.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

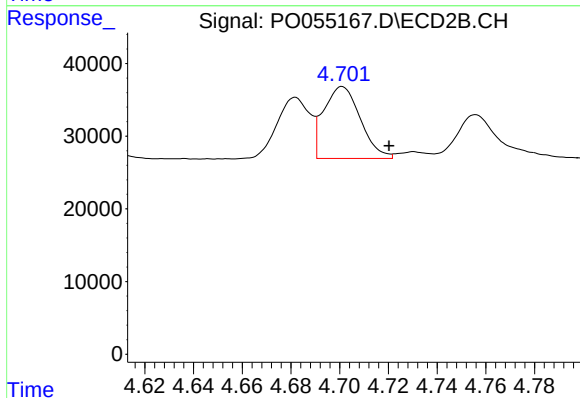


#17 AR-1242-2

R.T.: 4.701 min
Delta R.T.: -0.019 min
Response: 103392
Conc: 62.39 ng/ml

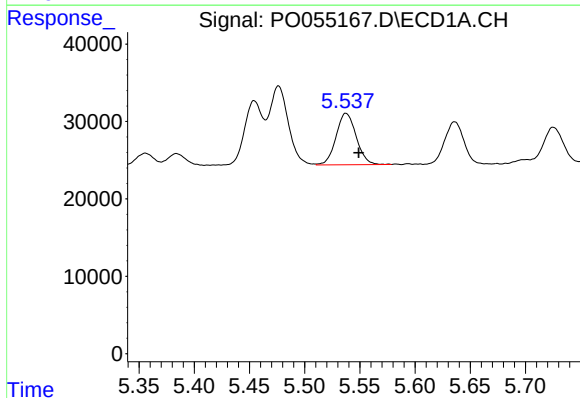


#18 AR-1242-3

R.T.: 5.537 min
Delta R.T.: -0.012 min
Response: 84647
Conc: 68.29 ng/ml

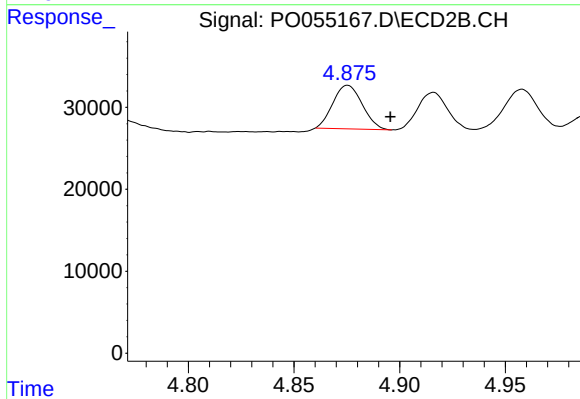

#18 AR-1242-3


R.T.: 4.875 min
Delta R.T.: -0.020 min
Response: 51305
Conc: 54.16 ng/ml

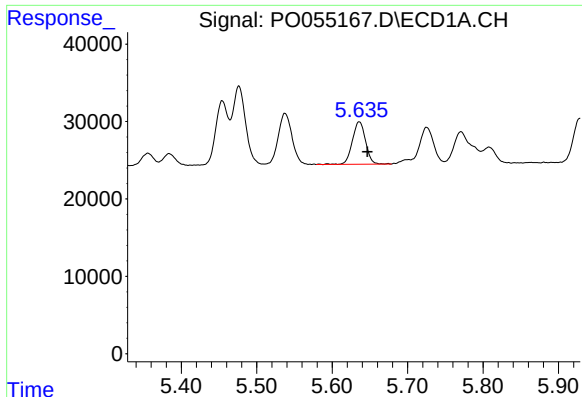

#19 AR-1242-4


R.T.: 5.636 min
Delta R.T.: -0.011 min
Response: 67119
Conc: 65.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

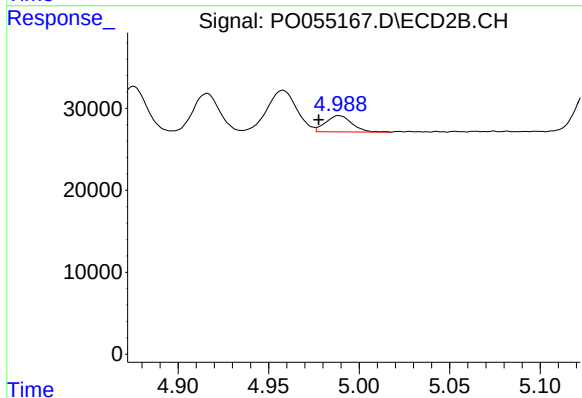


#19 AR-1242-4

R.T.: 4.989 min
Delta R.T.: 0.011 min
Response: 19933
Conc: 20.86 ng/ml

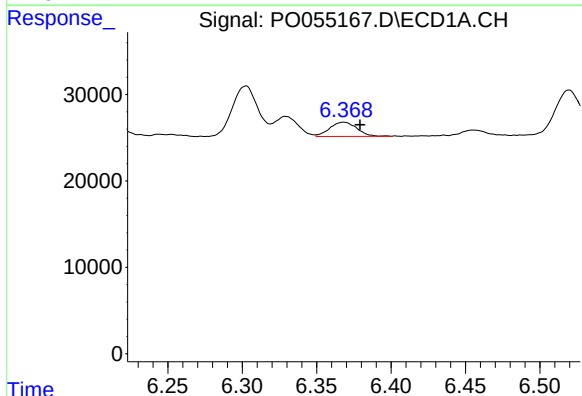


#20 AR-1242-5

R.T.: 6.368 min
Delta R.T.: -0.011 min
Response: 20835
Conc: 17.26 ng/ml

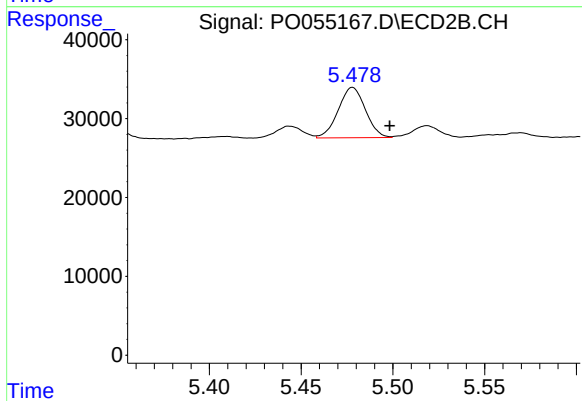

#20 AR-1242-5


R.T.: 5.478 min
Delta R.T.: -0.020 min
Response: 66014
Conc: 53.67 ng/ml

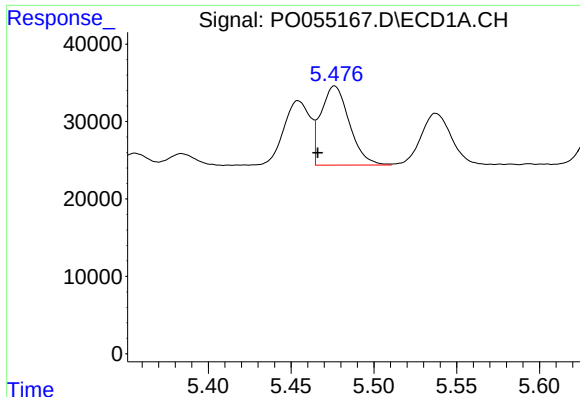

#21 AR-1248-1


R.T.: 5.476 min
Delta R.T.: 0.010 min
Response: 121943
Conc: 121.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

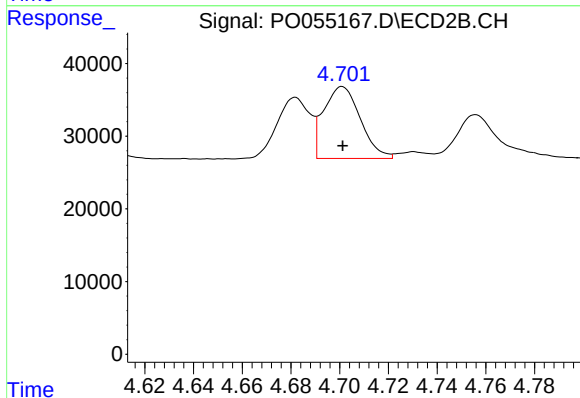


#21 AR-1248-1

R.T.: 4.701 min
Delta R.T.: 0.000 min
Response: 103392
Conc: 117.79 ng/ml

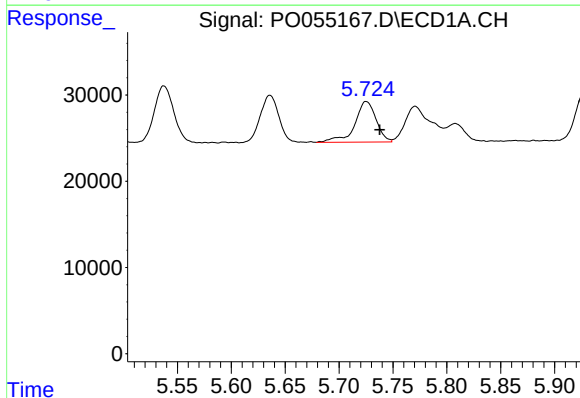


#22 AR-1248-2

R.T.: 5.725 min
Delta R.T.: -0.012 min
Response: 65111
Conc: 44.83 ng/ml

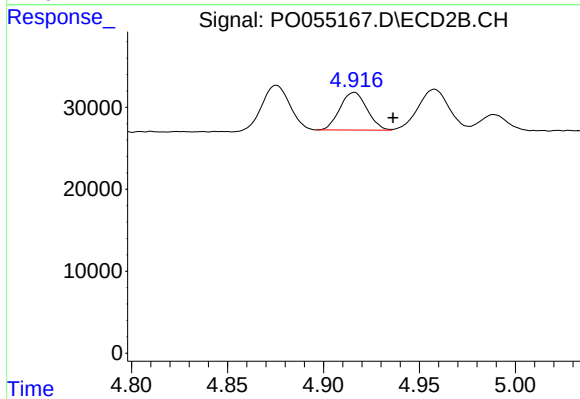

#22 AR-1248-2


R.T.: 4.916 min
Delta R.T.: -0.020 min
Response: 45179
Conc: 37.38 ng/ml

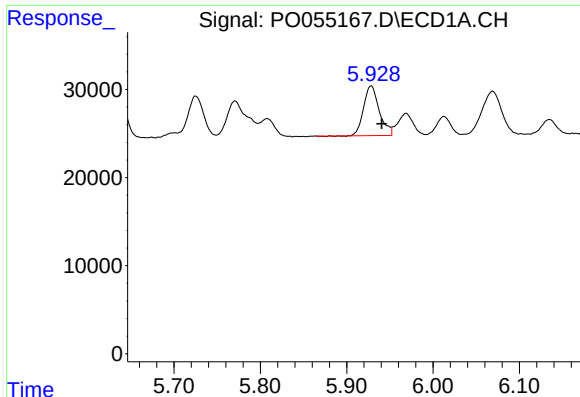

#23 AR-1248-3


R.T.: 5.928 min
Delta R.T.: -0.012 min
Response: 71238
Conc: 44.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

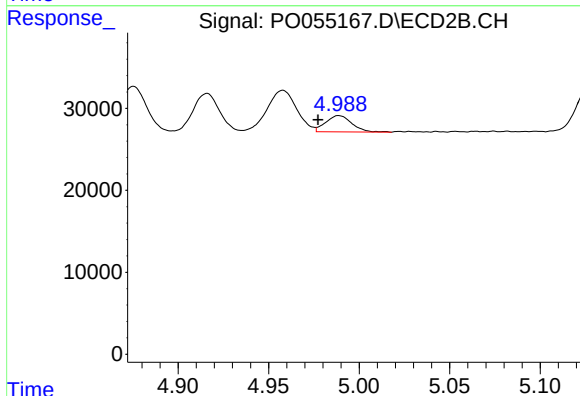


#23 AR-1248-3

R.T.: 4.989 min
Delta R.T.: 0.011 min
Response: 19933
Conc: 15.97 ng/ml

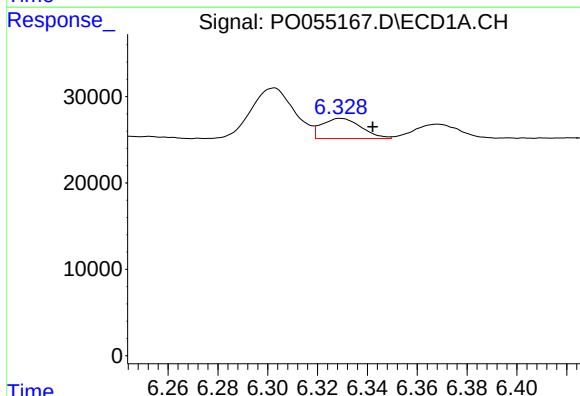


#24 AR-1248-4

R.T.: 6.329 min
Delta R.T.: -0.013 min
Response: 25487
Conc: 13.57 ng/ml

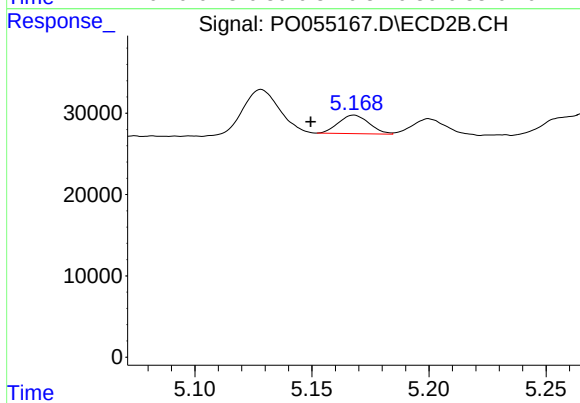

#24 AR-1248-4


R.T.: 5.168 min
Delta R.T.: 0.019 min
Response: 20659
Conc: 13.56 ng/ml

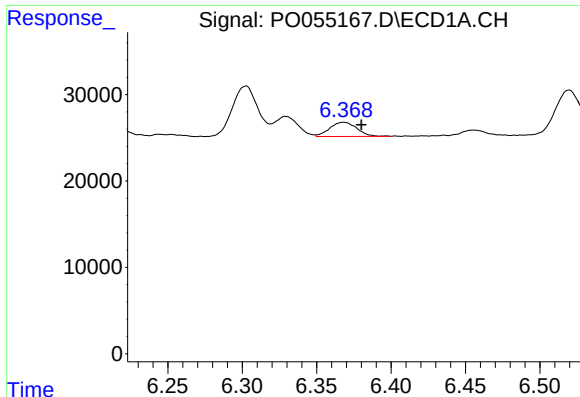

#25 AR-1248-5


R.T.: 6.368 min
Delta R.T.: -0.012 min
Response: 20835
Conc: 11.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

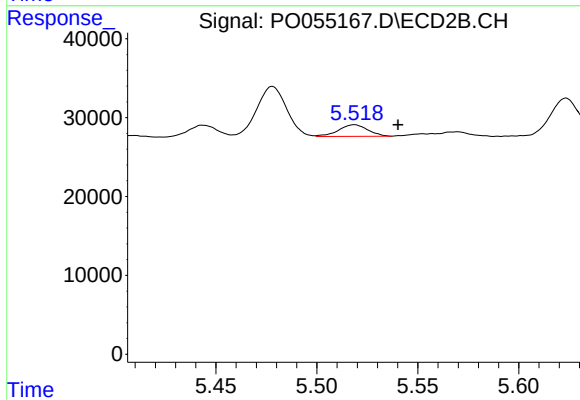


#25 AR-1248-5

R.T.: 5.519 min
Delta R.T.: -0.022 min
Response: 14989
Conc: 10.05 ng/ml

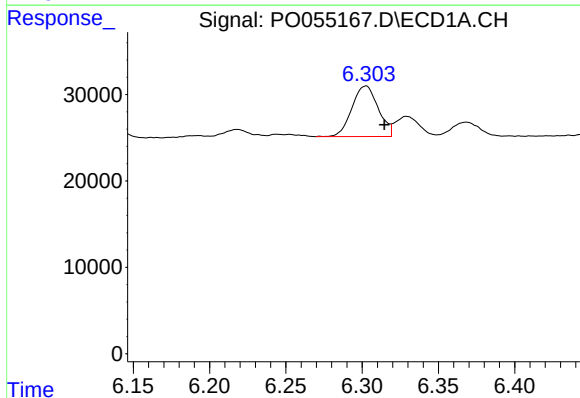


#26 AR-1254-1

R.T.: 6.302 min
Delta R.T.: -0.012 min
Response: 70296
Conc: 38.77 ng/ml

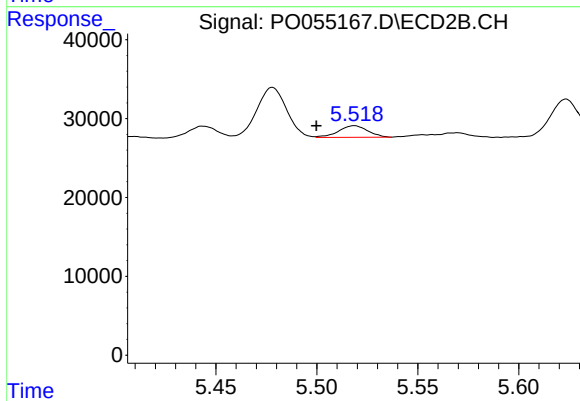

#26 AR-1254-1


R.T.: 5.519 min
Delta R.T.: 0.019 min
Response: 14989
Conc: 6.86 ng/ml

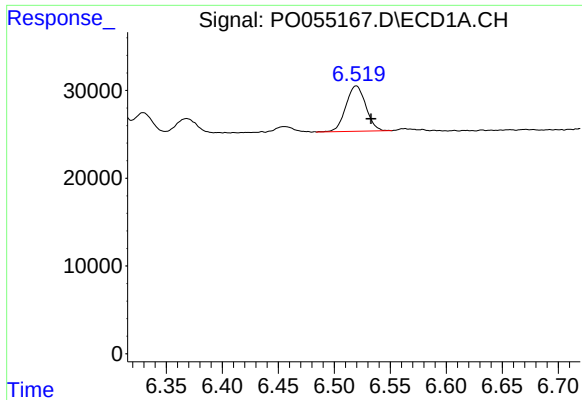

#27 AR-1254-2


R.T.: 6.520 min
Delta R.T.: -0.013 min
Response: 64235
Conc: 22.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

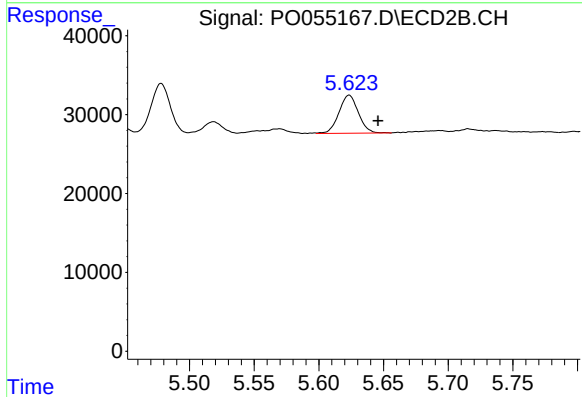


#27 AR-1254-2

R.T.: 5.623 min
Delta R.T.: -0.022 min
Response: 50363
Conc: 25.97 ng/ml

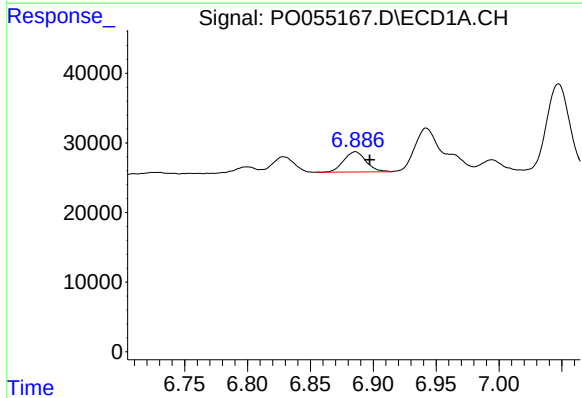


#28 AR-1254-3

R.T.: 6.886 min
Delta R.T.: -0.011 min
Response: 35816
Conc: 11.39 ng/ml

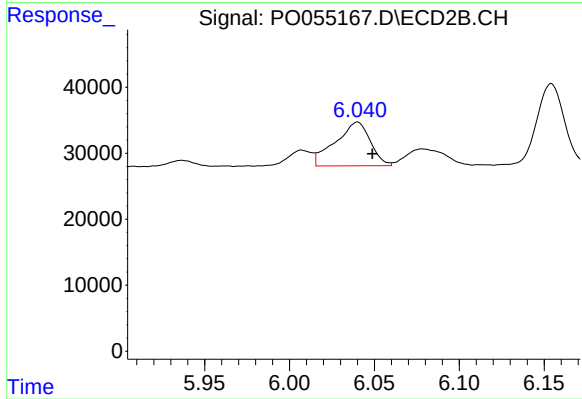

#28 AR-1254-3


R.T.: 6.040 min
Delta R.T.: -0.009 min
Response: 95145
Conc: 29.68 ng/ml

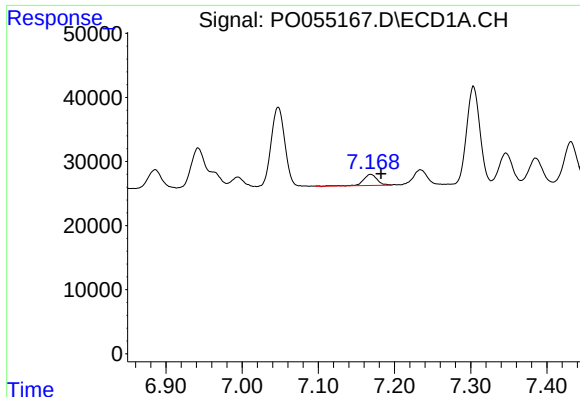

#29 AR-1254-4


R.T.: 7.169 min
Delta R.T.: -0.014 min
Response: 22001
Conc: 8.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

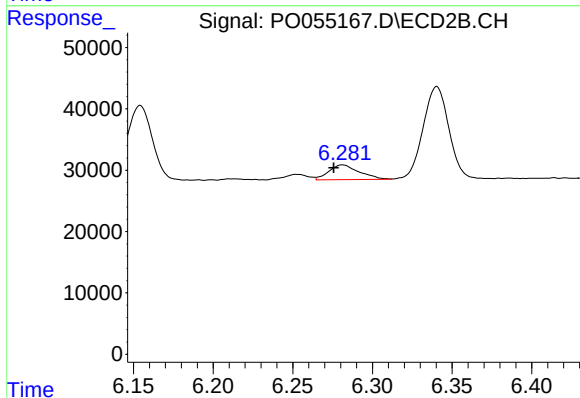


#29 AR-1254-4

R.T.: 6.281 min
Delta R.T.: 0.006 min
Response: 31976
Conc: 16.33 ng/ml

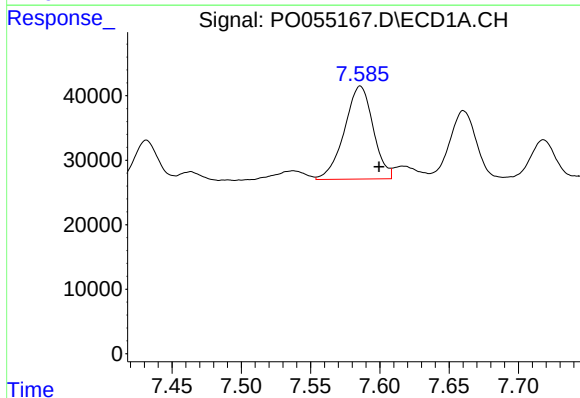


#30 AR-1254-5

R.T.: 7.586 min
Delta R.T.: -0.014 min
Response: 208138
Conc: 77.65 ng/ml

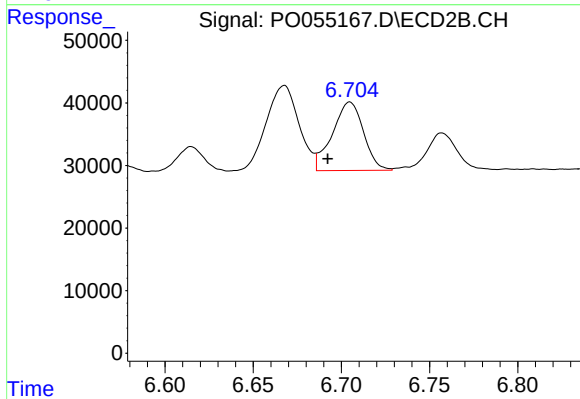

#30 AR-1254-5


R.T.: 6.705 min
Delta R.T.: 0.013 min
Response: 134941
Conc: 46.94 ng/ml

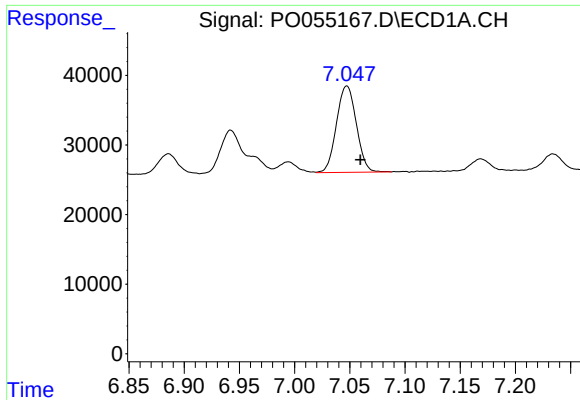

#31 AR-1260-1


R.T.: 7.047 min
Delta R.T.: -0.012 min
Response: 155347
Conc: 61.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

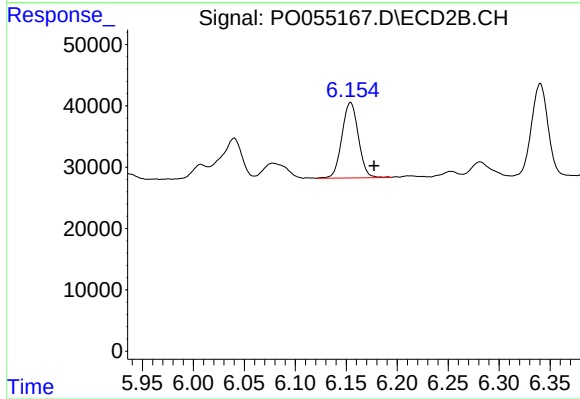


#31 AR-1260-1

R.T.: 6.154 min
Delta R.T.: -0.023 min
Response: 139081
Conc: 60.52 ng/ml

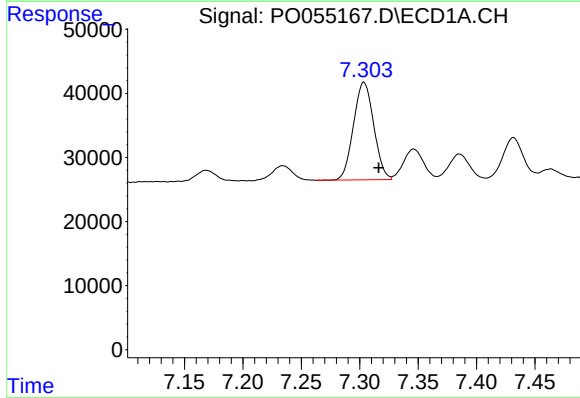


#32 AR-1260-2

R.T.: 7.304 min
Delta R.T.: -0.013 min
Response: 183766
Conc: 59.21 ng/ml

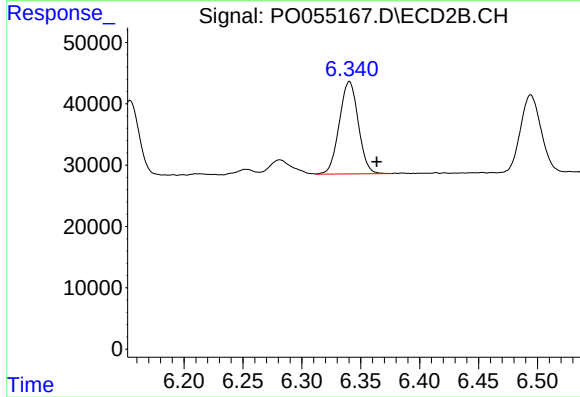

#32 AR-1260-2


R.T.: 6.340 min
Delta R.T.: -0.023 min
Response: 169371
Conc: 61.53 ng/ml

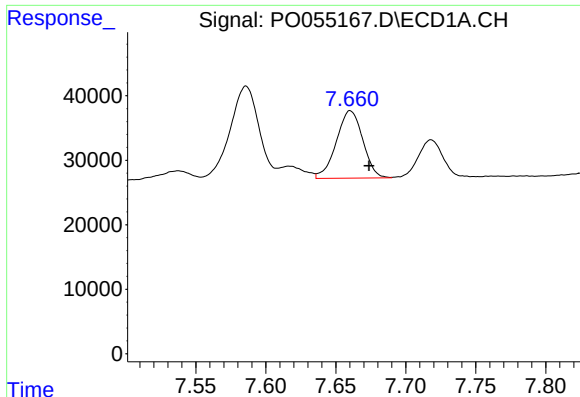

#33 AR-1260-3


R.T.: 7.660 min
Delta R.T.: -0.013 min
Response: 137630
Conc: 56.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

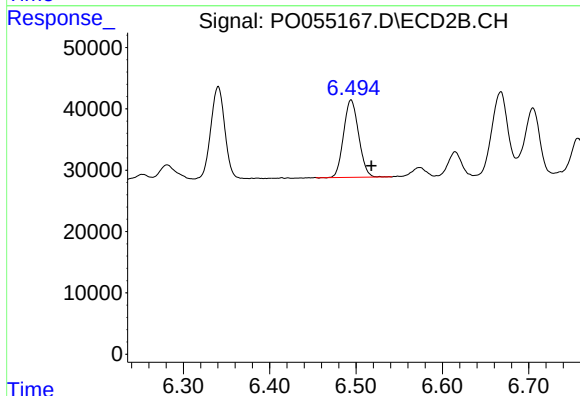


#33 AR-1260-3

R.T.: 6.494 min
Delta R.T.: -0.024 min
Response: 152918
Conc: 59.32 ng/ml

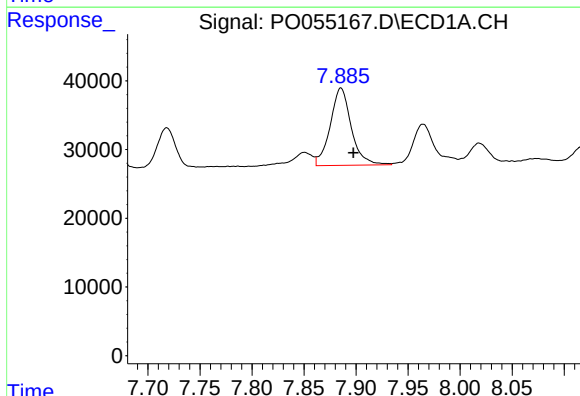


#34 AR-1260-4

R.T.: 7.886 min
Delta R.T.: -0.012 min
Response: 159074
Conc: 57.51 ng/ml

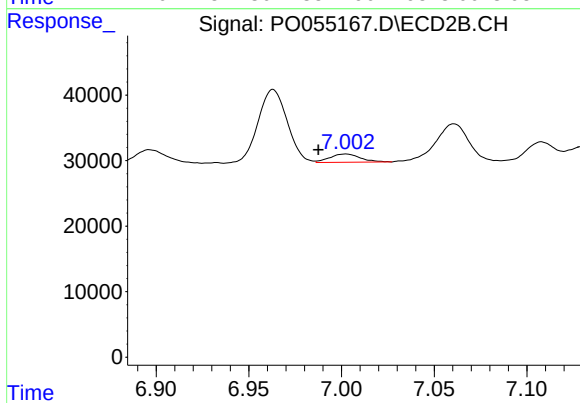

#34 AR-1260-4


R.T.: 7.002 min
Delta R.T.: 0.015 min
Response: 14442
Conc: 6.79 ng/ml

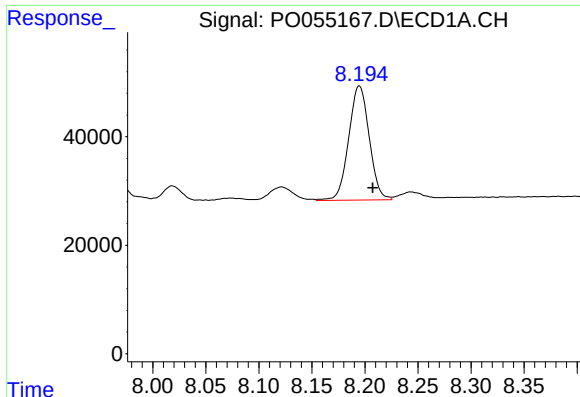

#35 AR-1260-5


R.T.: 8.195 min
Delta R.T.: -0.012 min
Response: 283853
Conc: 51.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

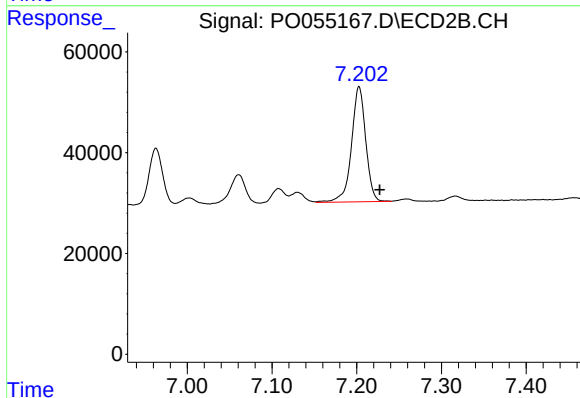


#35 AR-1260-5

R.T.: 7.203 min
Delta R.T.: -0.024 min
Response: 267125
Conc: 55.78 ng/ml

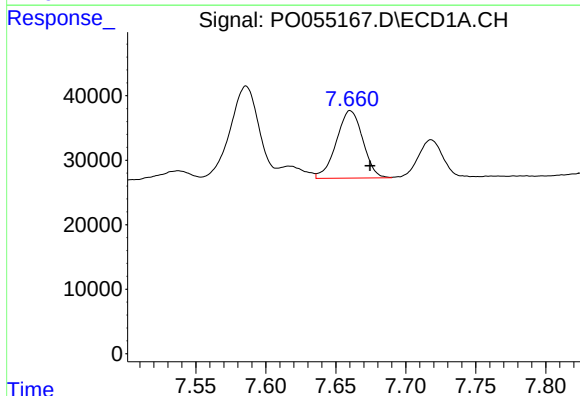


#36 AR-1262-1

R.T.: 7.660 min
Delta R.T.: -0.014 min
Response: 137630
Conc: 41.30 ng/ml

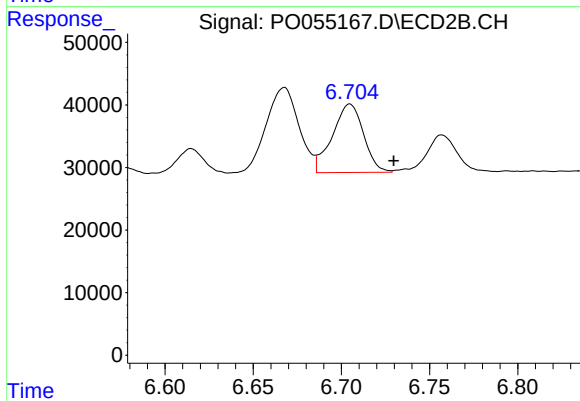

#36 AR-1262-1


R.T.: 6.705 min
Delta R.T.: -0.025 min
Response: 134941
Conc: 45.36 ng/ml

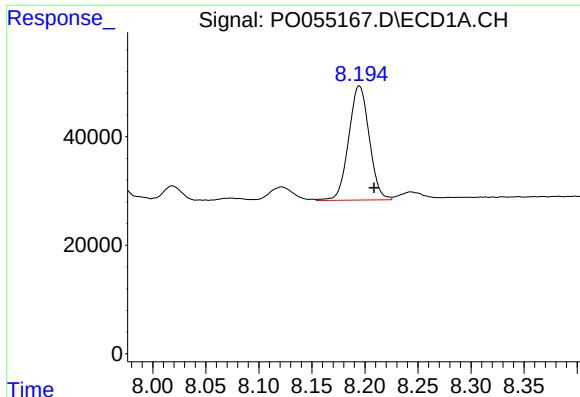

#37 AR-1262-2


R.T.: 8.195 min
Delta R.T.: -0.014 min
Response: 283853
Conc: 47.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

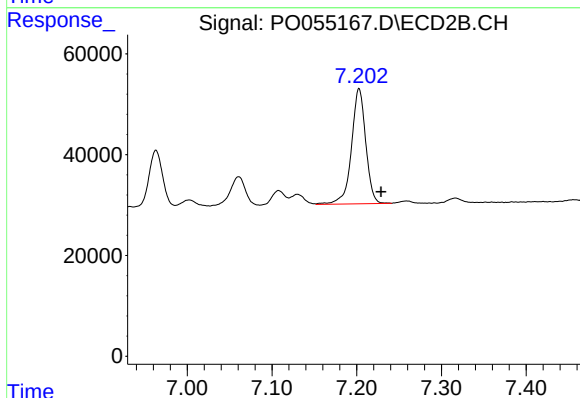


#37 AR-1262-2

R.T.: 7.203 min
Delta R.T.: -0.026 min
Response: 267125
Conc: 54.50 ng/ml

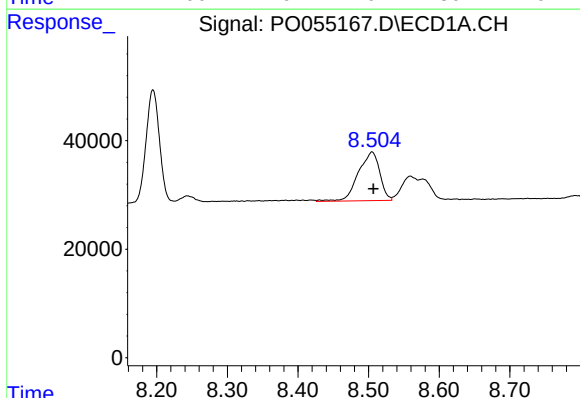


#38 AR-1262-3

R.T.: 8.505 min
Delta R.T.: -0.002 min
Response: 189642
Conc: 45.78 ng/ml

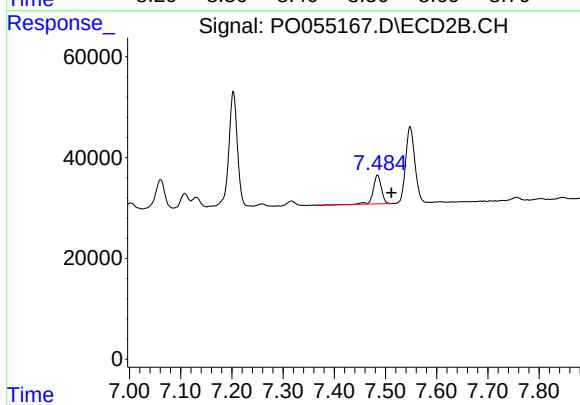

#38 AR-1262-3


R.T.: 7.484 min
Delta R.T.: -0.027 min
Response: 62570
Conc: 30.47 ng/ml

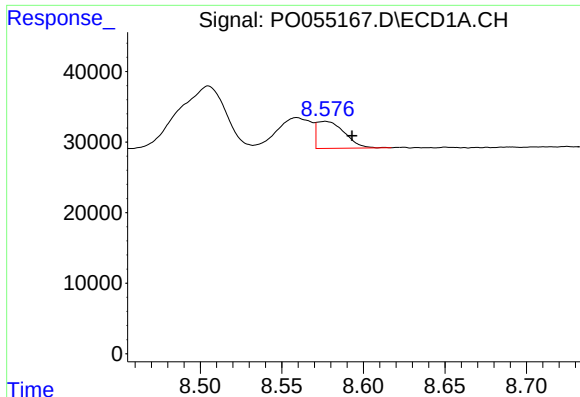

#39 AR-1262-4


R.T.: 8.577 min
Delta R.T.: -0.016 min
Response: 45112
Conc: 14.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

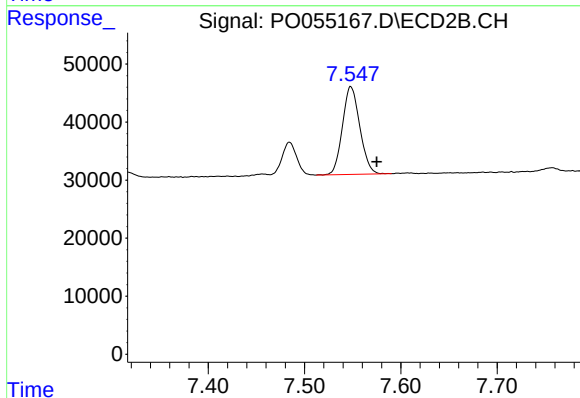


#39 AR-1262-4

R.T.: 7.548 min
Delta R.T.: -0.027 min
Response: 188967
Conc: 52.17 ng/ml

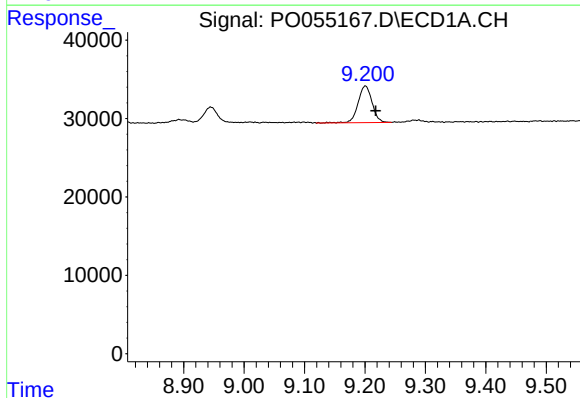


#40 AR-1262-5

R.T.: 9.201 min
Delta R.T.: -0.017 min
Response: 75680
Conc: 34.62 ng/ml

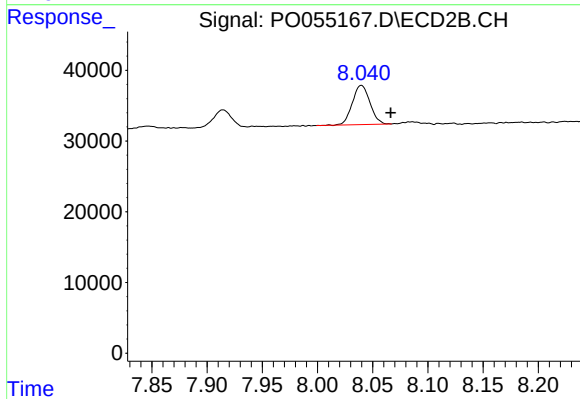

#40 AR-1262-5


R.T.: 8.040 min
Delta R.T.: -0.027 min
Response: 61521
Conc: 38.12 ng/ml

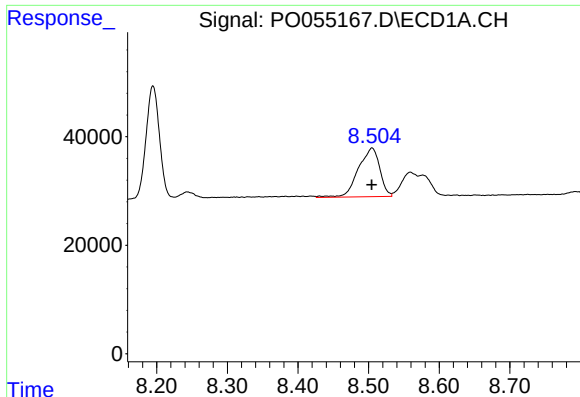

#41 AR-1268-1


R.T.: 8.505 min
Delta R.T.: 0.000 min
Response: 189642
Conc: 26.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

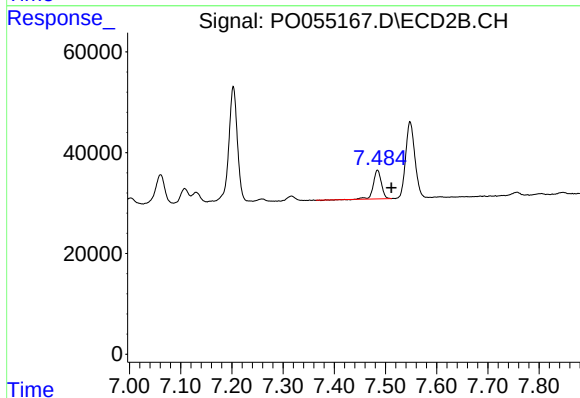


#41 AR-1268-1

R.T.: 7.484 min
Delta R.T.: -0.027 min
Response: 62570
Conc: 11.07 ng/ml

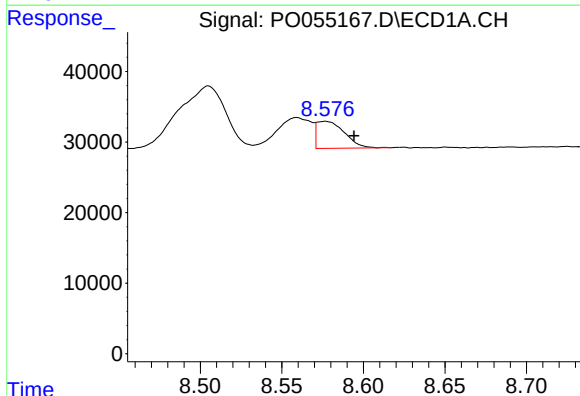


#42 AR-1268-2

R.T.: 8.577 min
Delta R.T.: -0.018 min
Response: 45112
Conc: 6.89 ng/ml

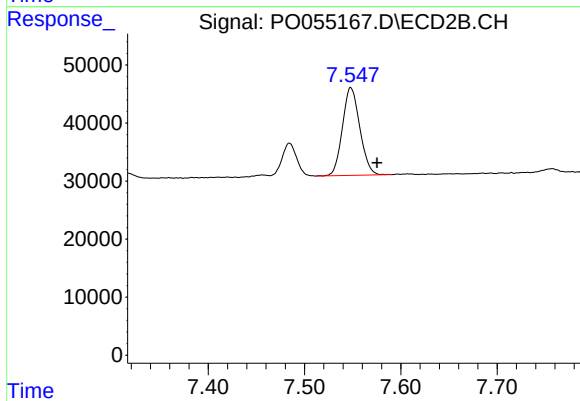

#42 AR-1268-2


R.T.: 7.548 min
Delta R.T.: -0.027 min
Response: 188967
Conc: 36.54 ng/ml

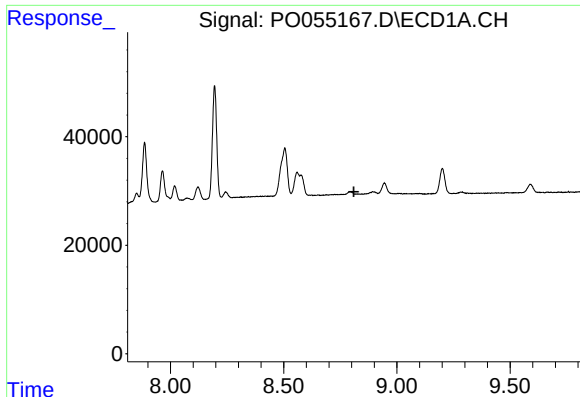

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 8.810 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

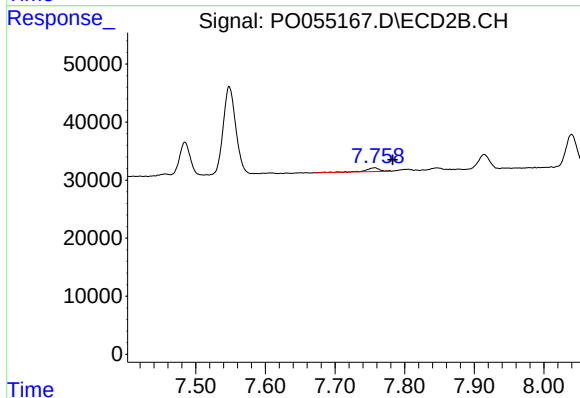


#43 AR-1268-3

R.T.: 7.757 min
Delta R.T.: -0.026 min
Response: 9370
Conc: 2.18 ng/ml

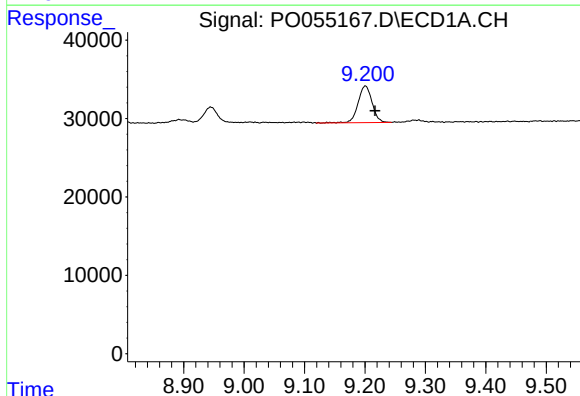


#44 AR-1268-4

R.T.: 9.201 min
Delta R.T.: -0.016 min
Response: 75680
Conc: 31.72 ng/ml

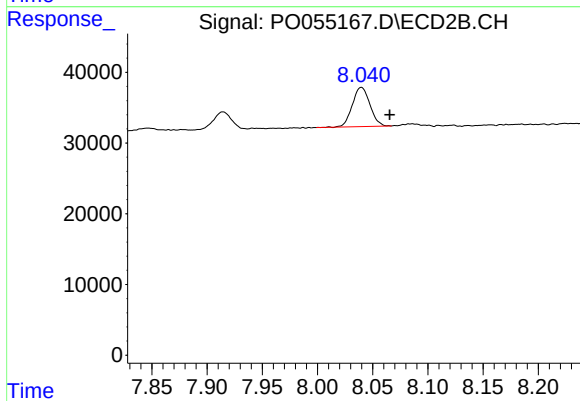

#44 AR-1268-4


R.T.: 8.040 min
Delta R.T.: -0.026 min
Response: 61521
Conc: 33.19 ng/ml

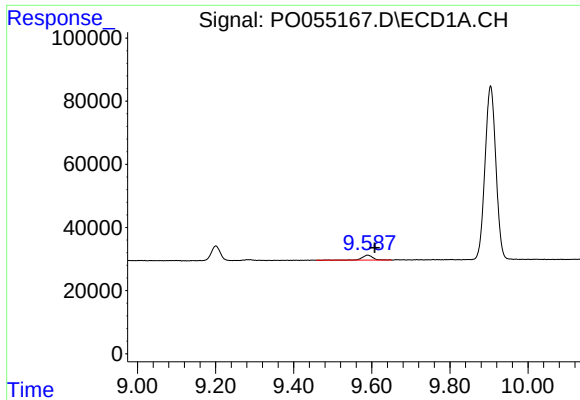

#45 AR-1268-5

R.T.: 9.589 min
Delta R.T.: -0.019 min
Response: 31619
Conc: 1.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

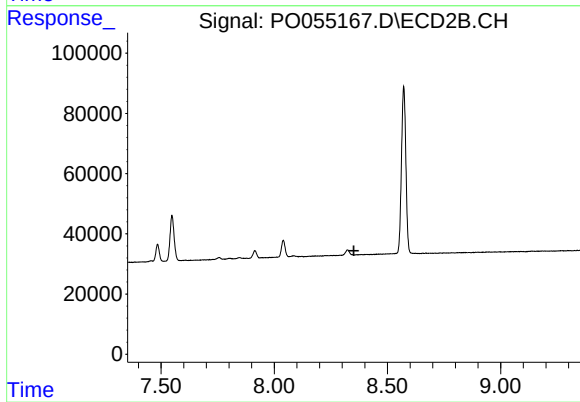

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.352 min
Response: 0
Conc: N.D.