

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041119\
 Data File : P0055188.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Apr 2019 2:07
 Operator : SM/SJ
 Sample : K2311-11
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 0236-COMP-CS-1-ELTRT-DISS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 10:01:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.294	3.606	591540	542329	17.045	16.994
2) SA Decachlor...	9.903	8.571	902934	647098	18.316	20.318
Target Compounds						
8) L2 AR-1221-1	4.472	3.904	18986	8952	43.488	23.025 #
9) L2 AR-1221-2	0.000	3.904	0	8952	N.D.	29.860 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041119\
Data File : P0055188.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Apr 2019 2:07
Operator : SM/SJ
Sample : K2311-11
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
0236-COMP-CS-1-ELTRT-DISS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 10:01:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

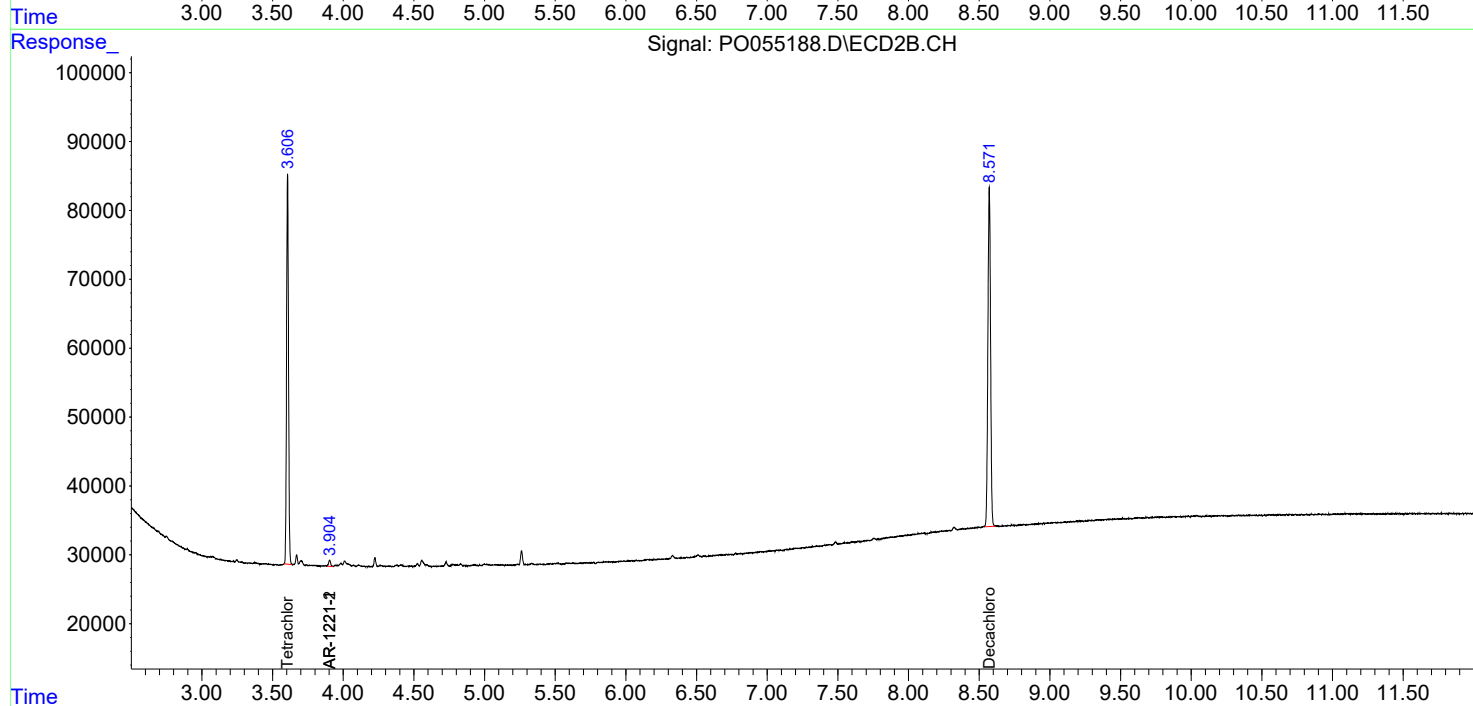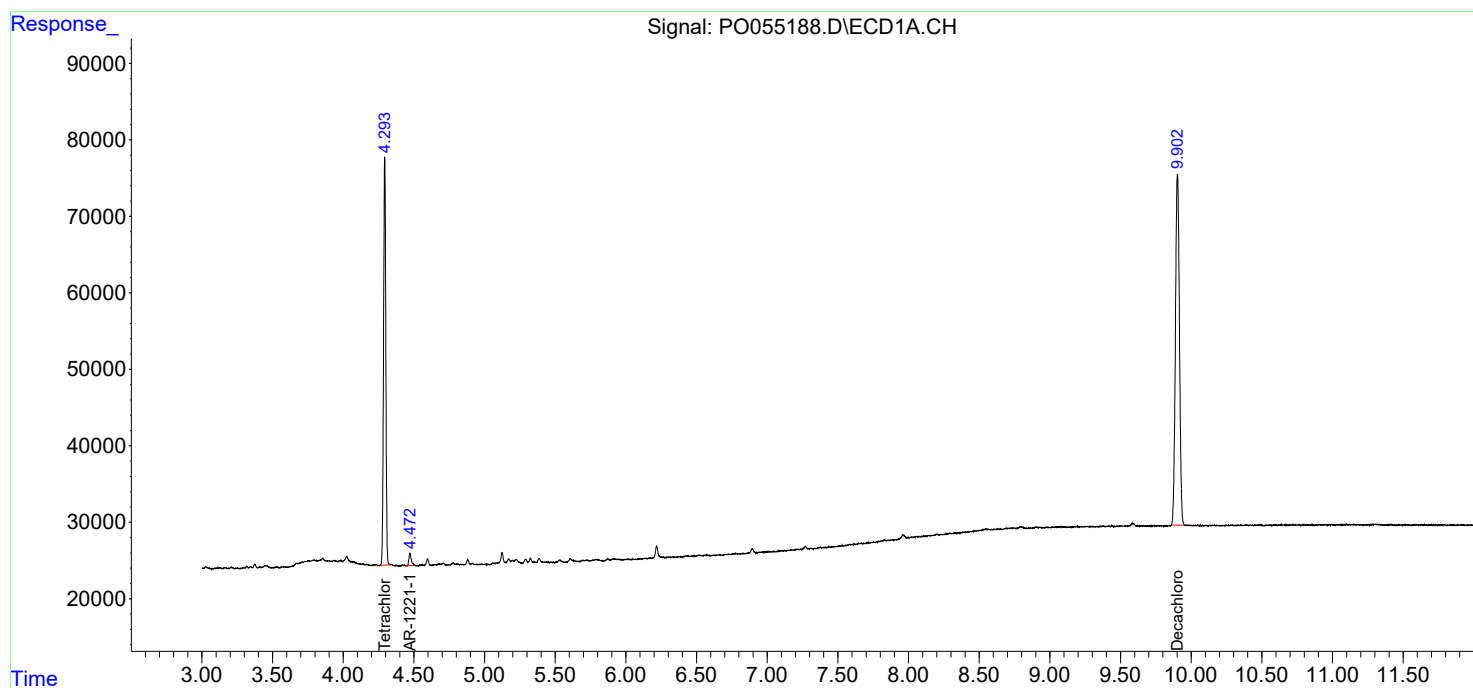


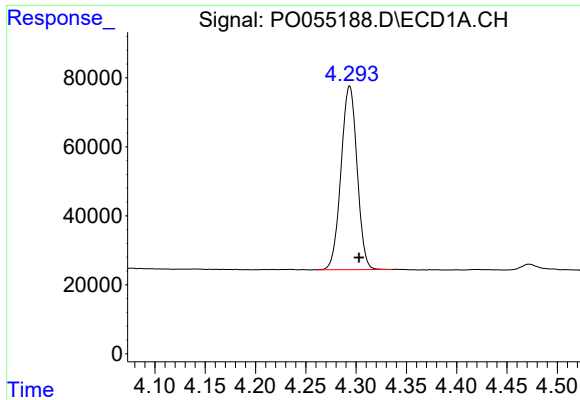

#1 Tetrachloro-m-xylene


R.T.: 4.294 min
Delta R.T.: -0.009 min
Response: 591540
Conc: 17.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
0236-COMP-CS-1-ELTRT-DISS

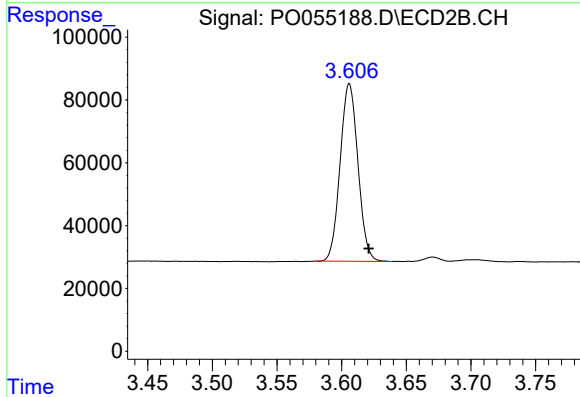


#1 Tetrachloro-m-xylene

R.T.: 3.606 min
Delta R.T.: -0.015 min
Response: 542329
Conc: 16.99 ng/ml

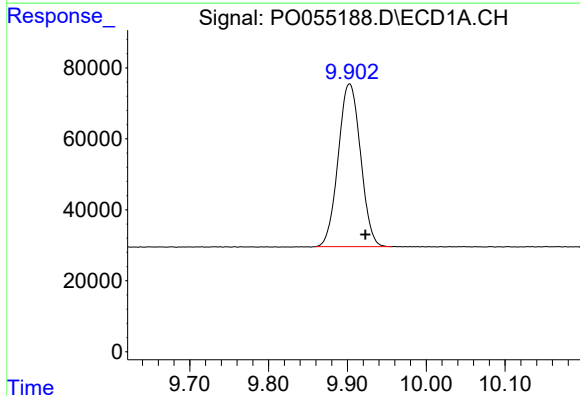


#2 Decachlorobiphenyl

R.T.: 9.903 min
Delta R.T.: -0.020 min
Response: 902934
Conc: 18.32 ng/ml

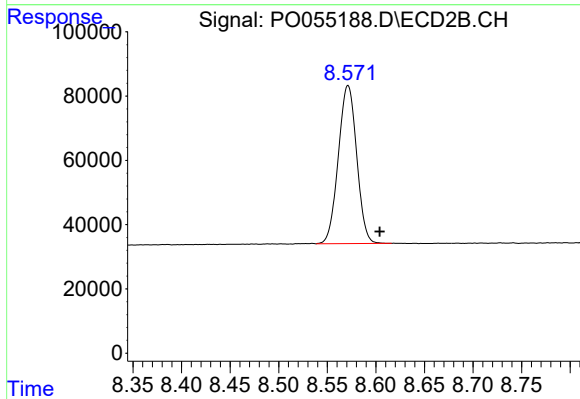

#2 Decachlorobiphenyl


R.T.: 8.571 min
Delta R.T.: -0.033 min
Response: 647098
Conc: 20.32 ng/ml

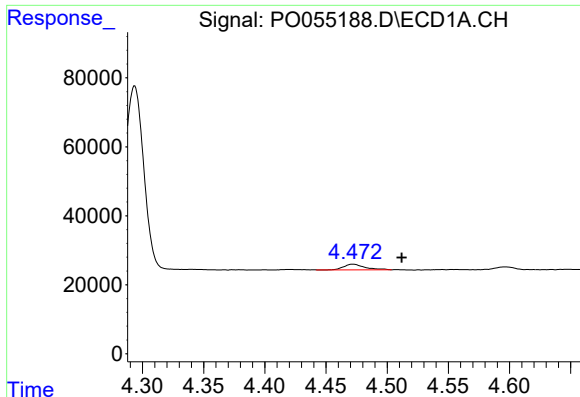

#8 AR-1221-1


R.T.: 4.472 min
Delta R.T.: -0.040 min
Response: 18986
Conc: 43.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
0236-COMP-CS-1-ELTRT-DISS

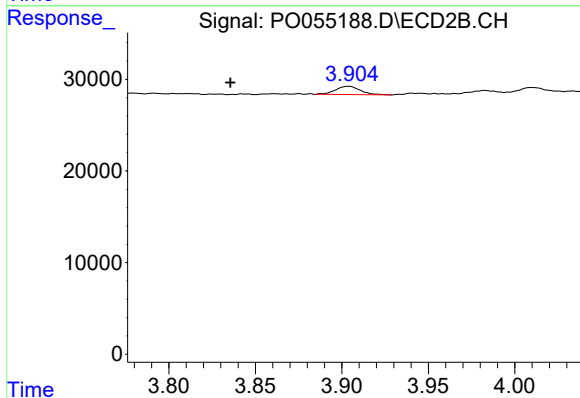


#8 AR-1221-1

R.T.: 3.904 min
Delta R.T.: 0.069 min
Response: 8952
Conc: 23.02 ng/ml

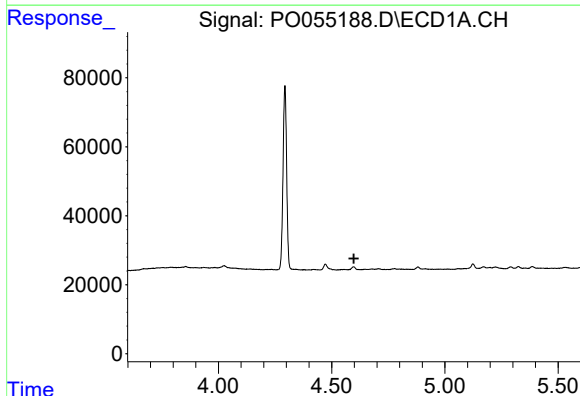

#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.598 min
Response: 0
Conc: N.D.

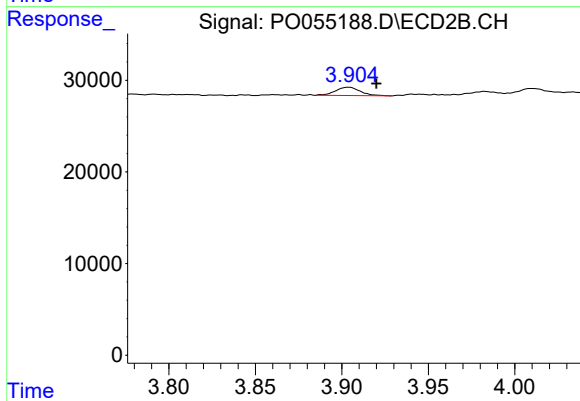

#9 AR-1221-2

R.T.: 3.904 min
Delta R.T.: -0.016 min
Response: 8952
Conc: 29.86 ng/ml