

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041119\
 Data File : P0055143.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Apr 2019 11:28
 Operator : SM/SJ
 Sample : K2200-05RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EO-01-040919-CRE

Manual Integrations
 APPROVED

mohammad
 4/15/2019 4:41:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 02:28:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.295	3.608	37731	35014	1.087	1.097
2) SA Decachlor...	9.908	8.571	54140	41055	1.098	1.289m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041119\
Data File : P0055143.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Apr 2019 11:28
Operator : SM/SJ
Sample : K2200-05RE
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
EO-01-040919-CRE


Manual Integrations
APPROVED

mohammad
4/15/2019 4:41:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 02:28:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

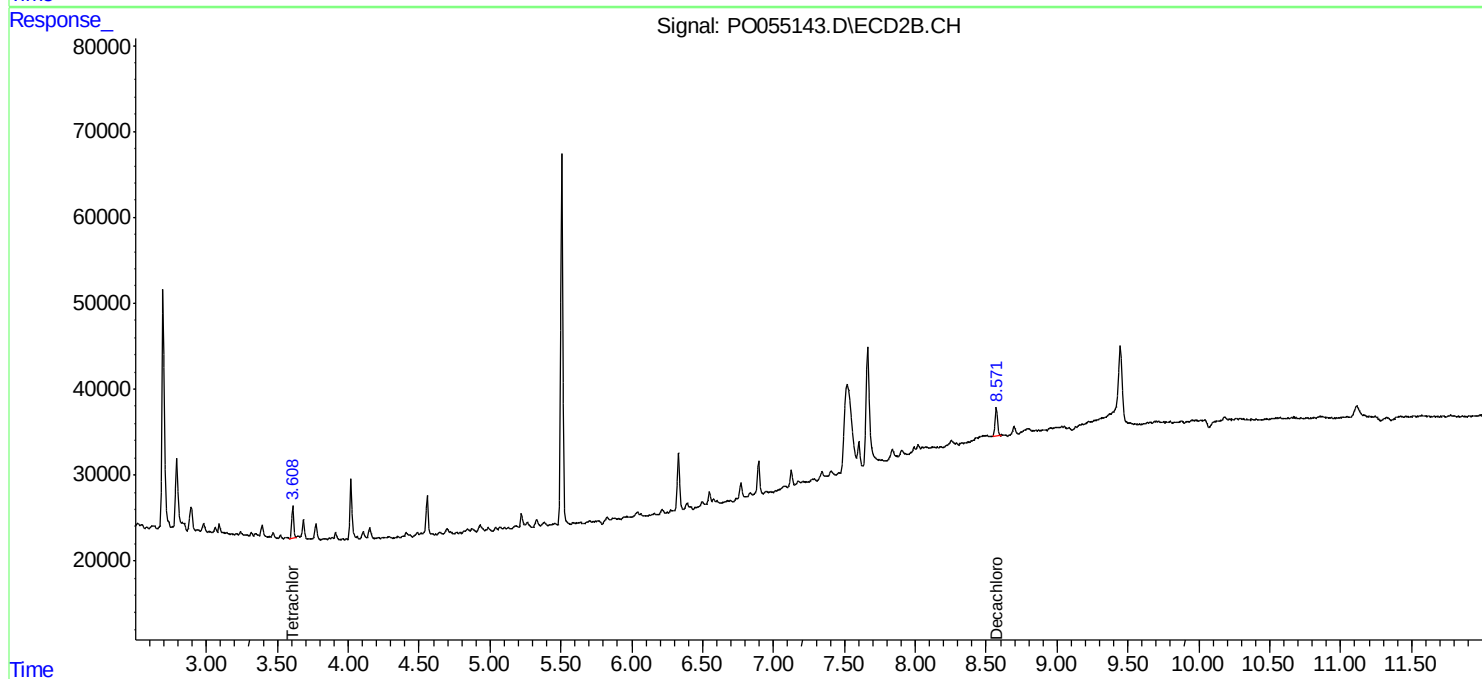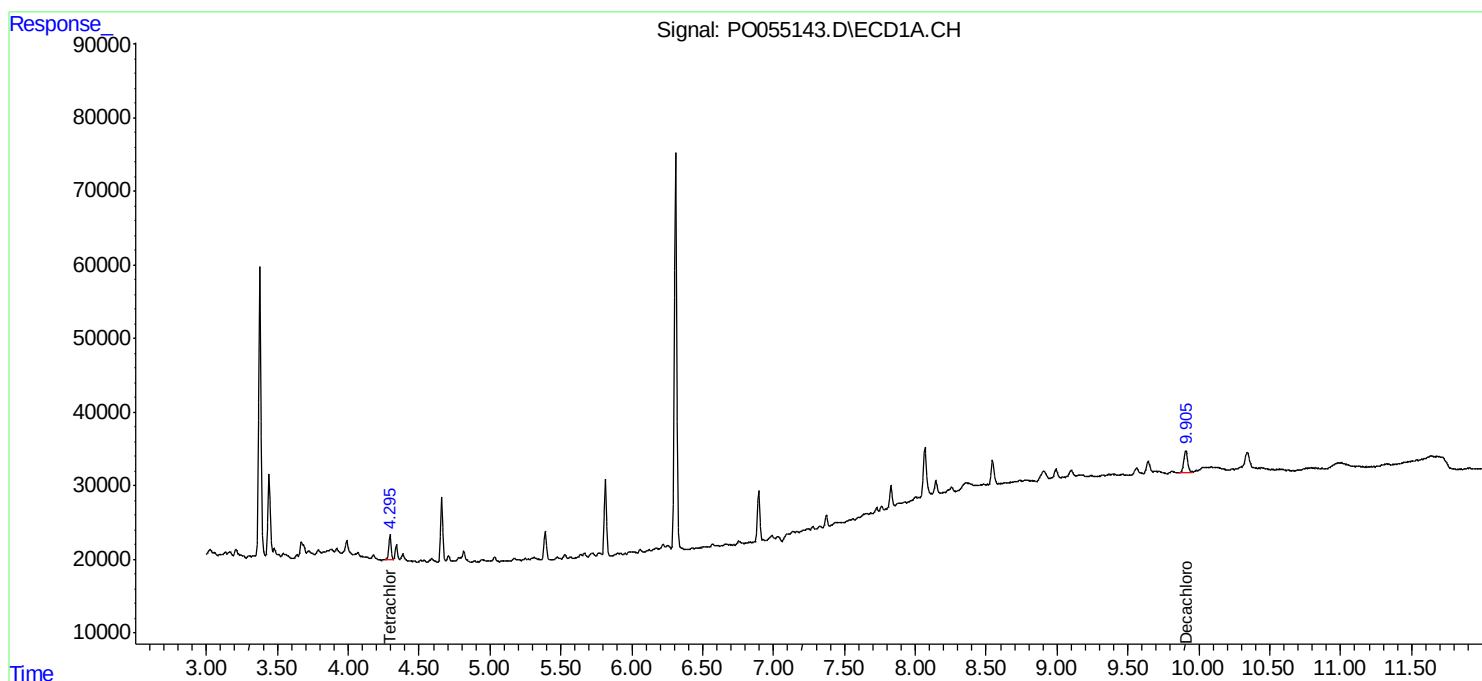

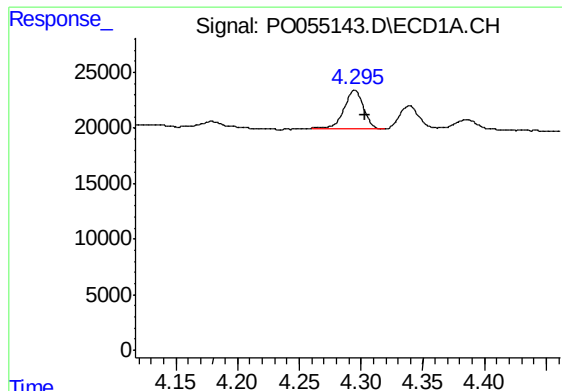


#1 Tetrachloro-m-xylene

R.T.: 4.295 min
Delta R.T.: -0.008 min
Response: 37731
Conc: 1.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
EO-01-040919-CRE


Manual Integrations
APPROVED

mohammad
4/15/2019 4:41:17 PM

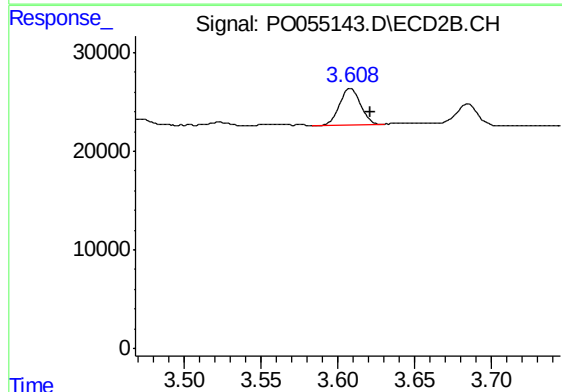


#1 Tetrachloro-m-xylene

R.T.: 3.608 min
Delta R.T.: -0.013 min
Response: 35014
Conc: 1.10 ng/ml

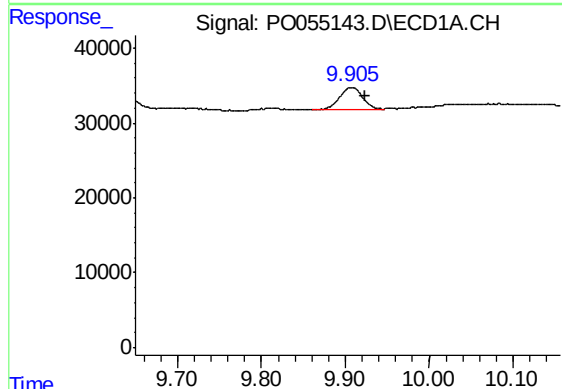

#2 Decachlorobiphenyl

R.T.: 9.908 min
Delta R.T.: -0.015 min
Response: 54140
Conc: 1.10 ng/ml

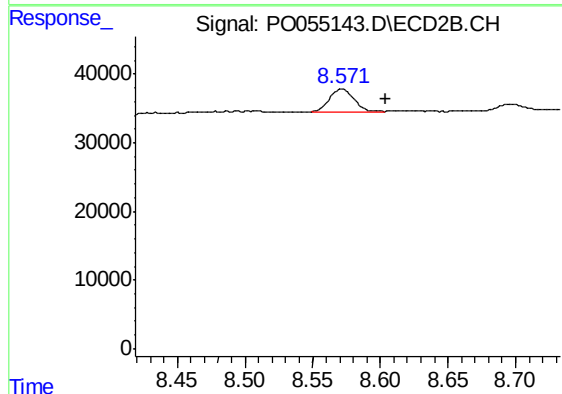

#2 Decachlorobiphenyl

R.T.: 8.571 min
Delta R.T.: -0.033 min
Response: 41055
Conc: 1.29 ng/ml m