

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041119\
 Data File : P0055163.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Apr 2019 19:03
 Operator : SM/SJ
 Sample : K1560-07
 Misc : AR1262 LOD 40PPB
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2019

Manual Integrations
 APPROVED

mohammad
 4/15/2019 4:42:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 04:01:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.293	3.605	677672	613297	19.527	19.218
2)	SA Decachlor...	9.905	8.573	1039522	734889	21.087	23.075
Target Compounds							
36)	L8 AR-1262-1	7.661	6.705	186450	172528	55.956	57.993
37)	L8 AR-1262-2	8.196	7.202	299543	277356	50.561	56.590m
38)	L8 AR-1262-3	8.492	7.486	215909	114936	52.117	55.972
39)	L8 AR-1262-4	8.579	7.549	165985	203121	51.517	56.078
40)	L8 AR-1262-5	9.202	8.040	108078	92790	49.435	57.495m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041119\
Data File : PO055163.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Apr 2019 19:03
Operator : SM/SJ
Sample : K1560-07
Misc : AR1262 LOD 40PPB
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/15/2019 4:42:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 04:01:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

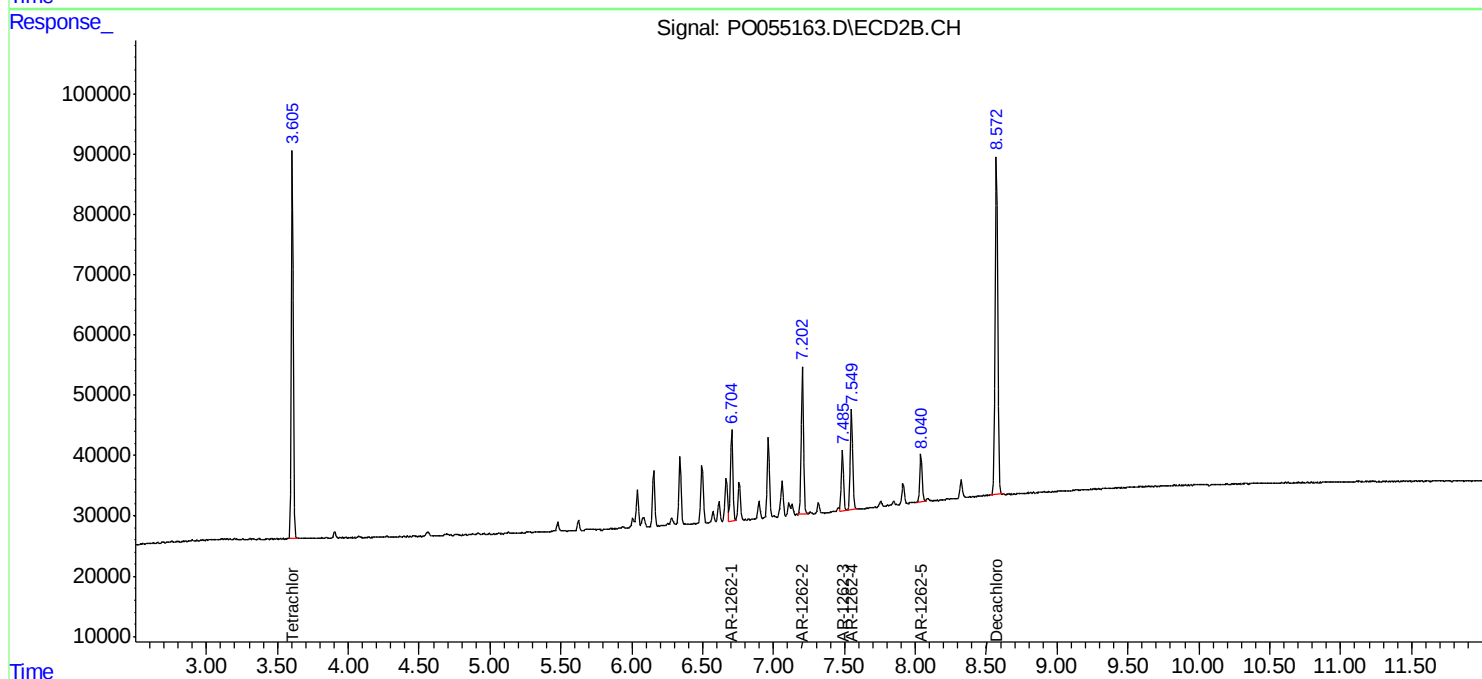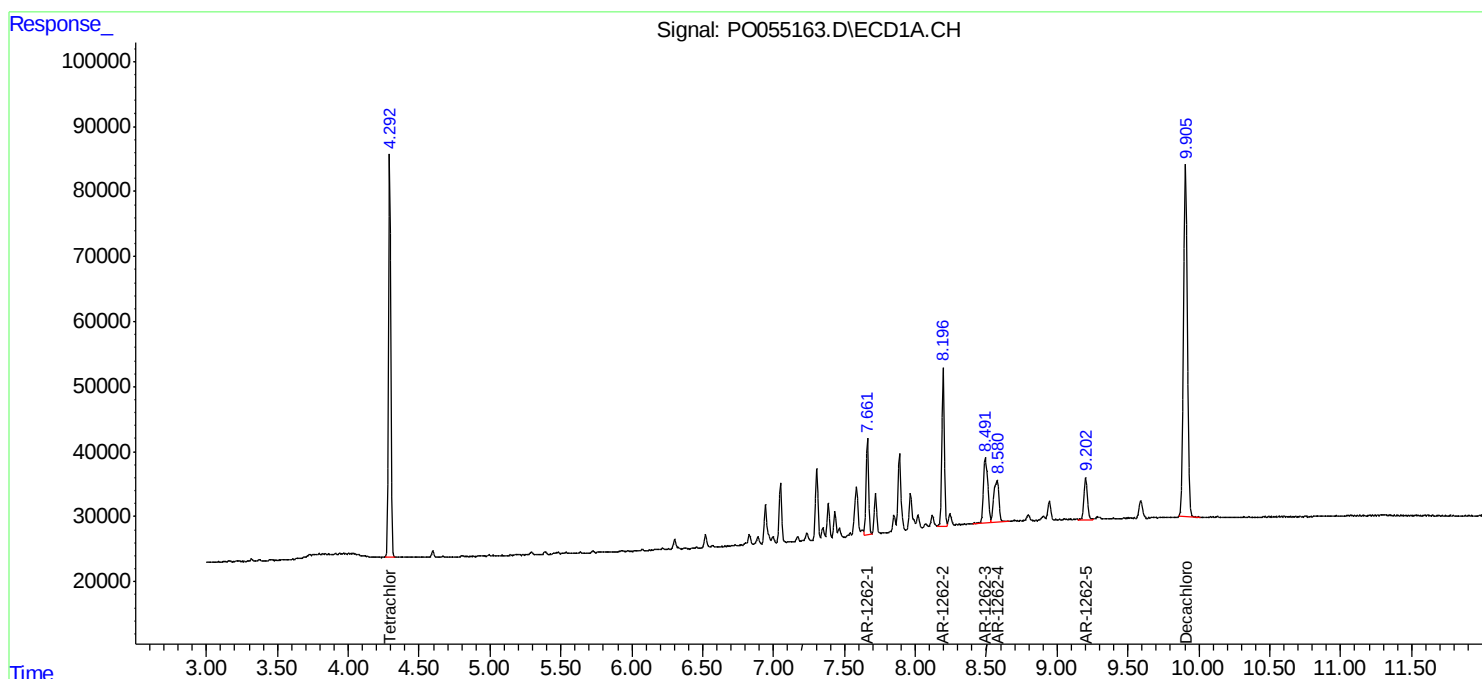

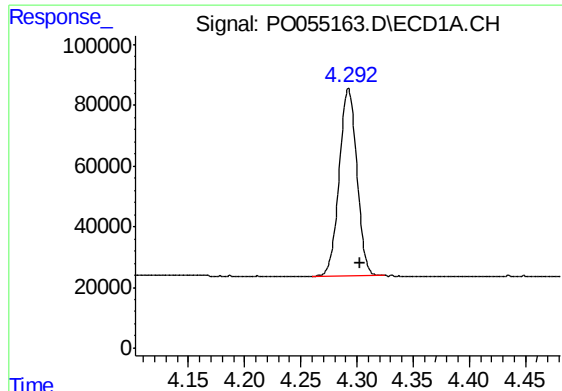


#1 Tetrachloro-m-xylene

R.T.: 4.293 min
Delta R.T.: -0.010 min
Response: 677672
Conc: 19.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/15/2019 4:42:06 PM

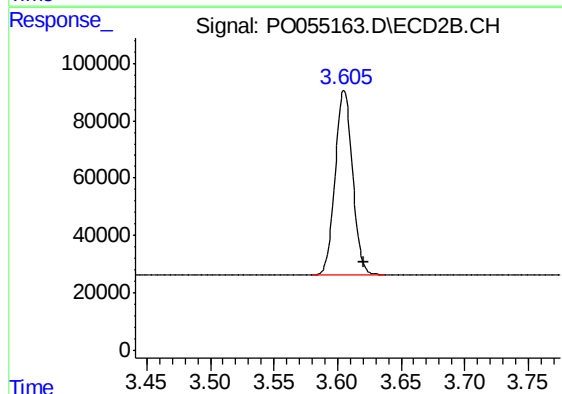


#1 Tetrachloro-m-xylene

R.T.: 3.605 min
Delta R.T.: -0.016 min
Response: 613297
Conc: 19.22 ng/ml

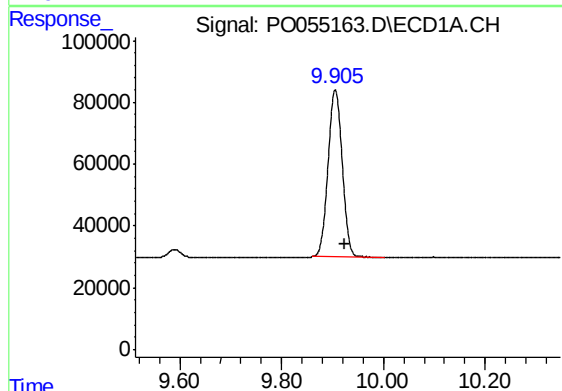


#2 Decachlorobiphenyl

R.T.: 9.905 min
Delta R.T.: -0.018 min
Response: 1039522
Conc: 21.09 ng/ml

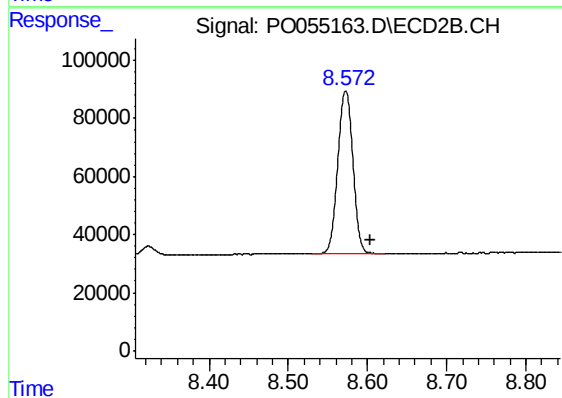

#2 Decachlorobiphenyl

R.T.: 8.573 min
Delta R.T.: -0.032 min
Response: 734889
Conc: 23.07 ng/ml

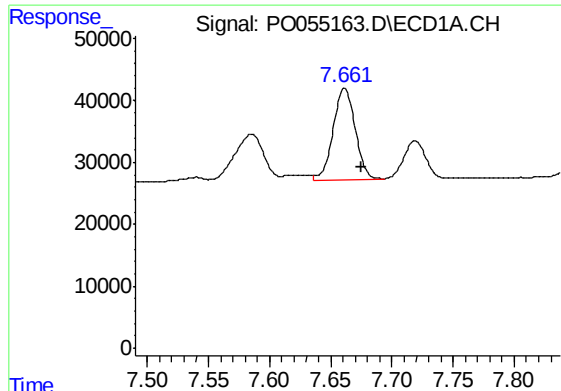


#36 AR-1262-1

R.T.: 7.661 min
Delta R.T.: -0.013 min
Response: 186450
Conc: 55.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/15/2019 4:42:06 PM

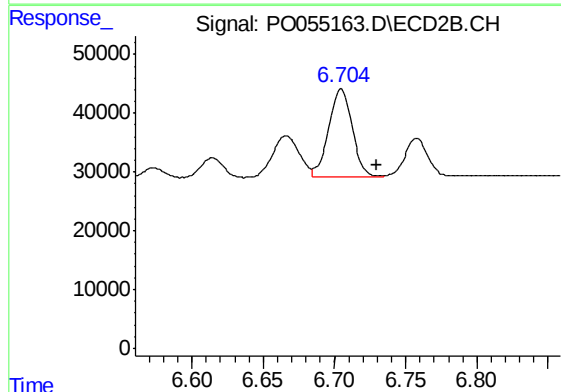


#36 AR-1262-1

R.T.: 6.705 min
Delta R.T.: -0.025 min
Response: 172528
Conc: 57.99 ng/ml

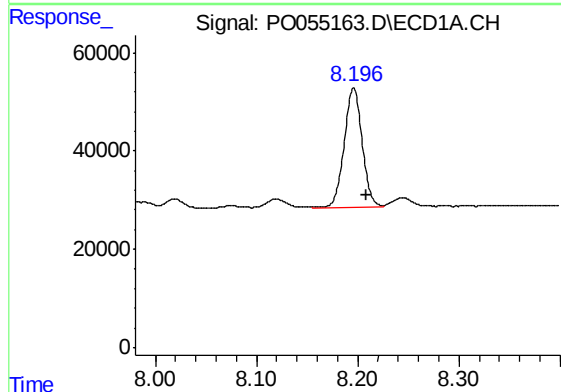


#37 AR-1262-2

R.T.: 8.196 min
Delta R.T.: -0.013 min
Response: 299543
Conc: 50.56 ng/ml

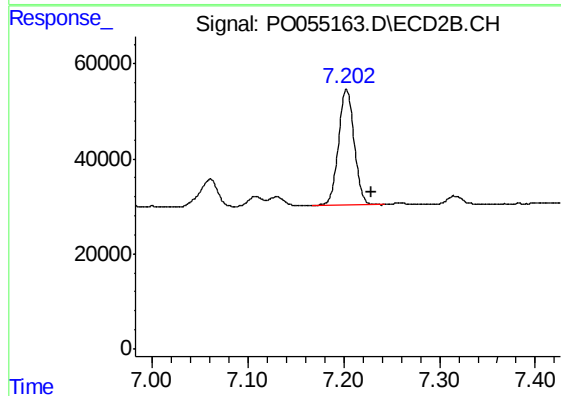

#37 AR-1262-2

R.T.: 7.202 min
Delta R.T.: -0.026 min
Response: 277356
Conc: 56.59 ng/ml m

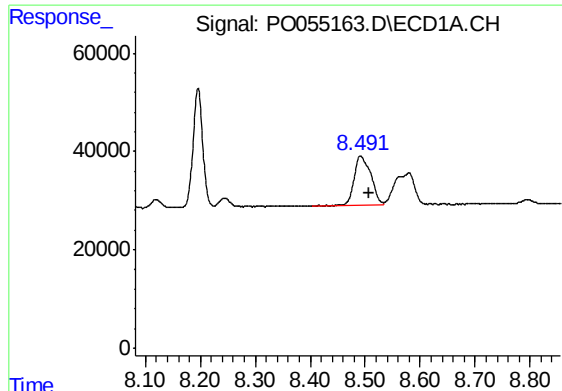


#38 AR-1262-3

R.T.: 8.492 min
Delta R.T.: -0.015 min
Response: 215909
Conc: 52.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019


Manual Integrations
APPROVED

mohammad
4/15/2019 4:42:06 PM

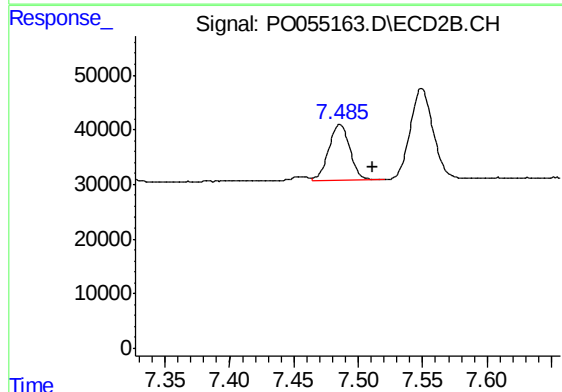


#38 AR-1262-3

R.T.: 7.486 min
Delta R.T.: -0.026 min
Response: 114936
Conc: 55.97 ng/ml

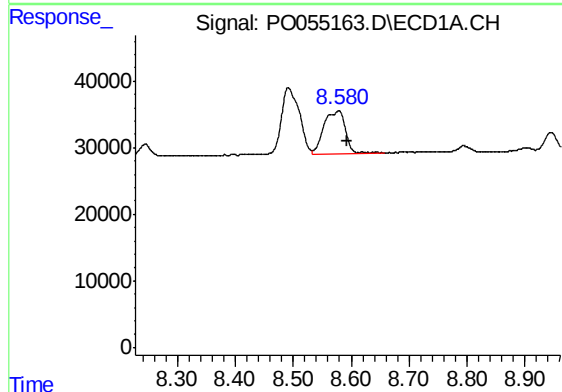


#39 AR-1262-4

R.T.: 8.579 min
Delta R.T.: -0.014 min
Response: 165985
Conc: 51.52 ng/ml

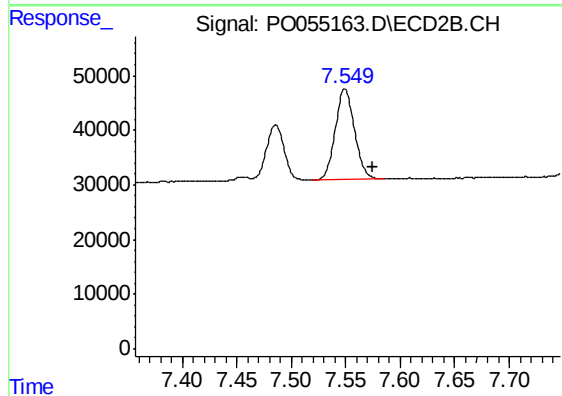

#39 AR-1262-4

R.T.: 7.549 min
Delta R.T.: -0.026 min
Response: 203121
Conc: 56.08 ng/ml

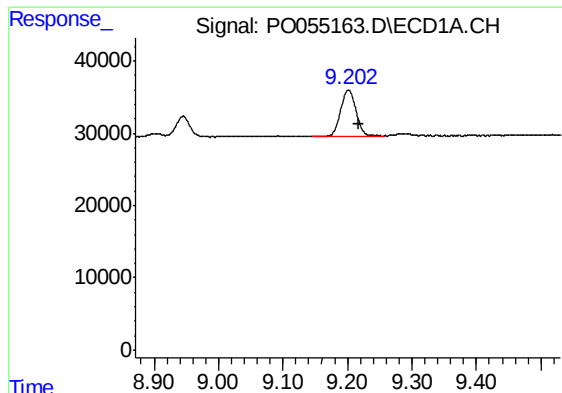


#40 AR-1262-5

R.T.: 9.202 min
Delta R.T.: -0.016 min
Response: 108078
Conc: 49.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOD-MDL-WATER-01-QT1-2019

Manual Integrations
APPROVED

mohammad
4/15/2019 4:42:06 PM

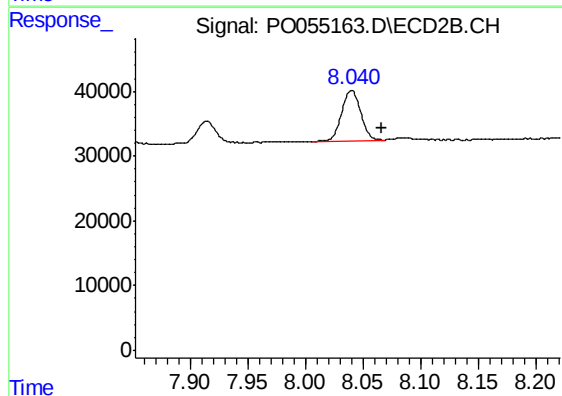

#40 AR-1262-5

R.T.: 8.040 min
Delta R.T.: -0.027 min
Response: 92790
Conc: 57.49 ng/ml m