

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041119\
 Data File : P0055194.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Apr 2019 3:48
 Operator : SM/SJ
 Sample : K2311-15
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 0238-COMP-CS-3-ELTRT-DISS

Manual Integrations
 APPROVED

mohammad
 4/15/2019 4:42:51 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 10:14:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.292	3.605	547757	545865	15.783m	17.105
2) SA Decachlor...	9.902	8.570	749725	531164	15.208	16.678

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041119\
Data File : P0055194.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Apr 2019 3:48
Operator : SM/SJ
Sample : K2311-15
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
0238-COMP-CS-3-ELTRT-DISS


Manual Integrations
APPROVED

mohammad
4/15/2019 4:42:51 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 10:14:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

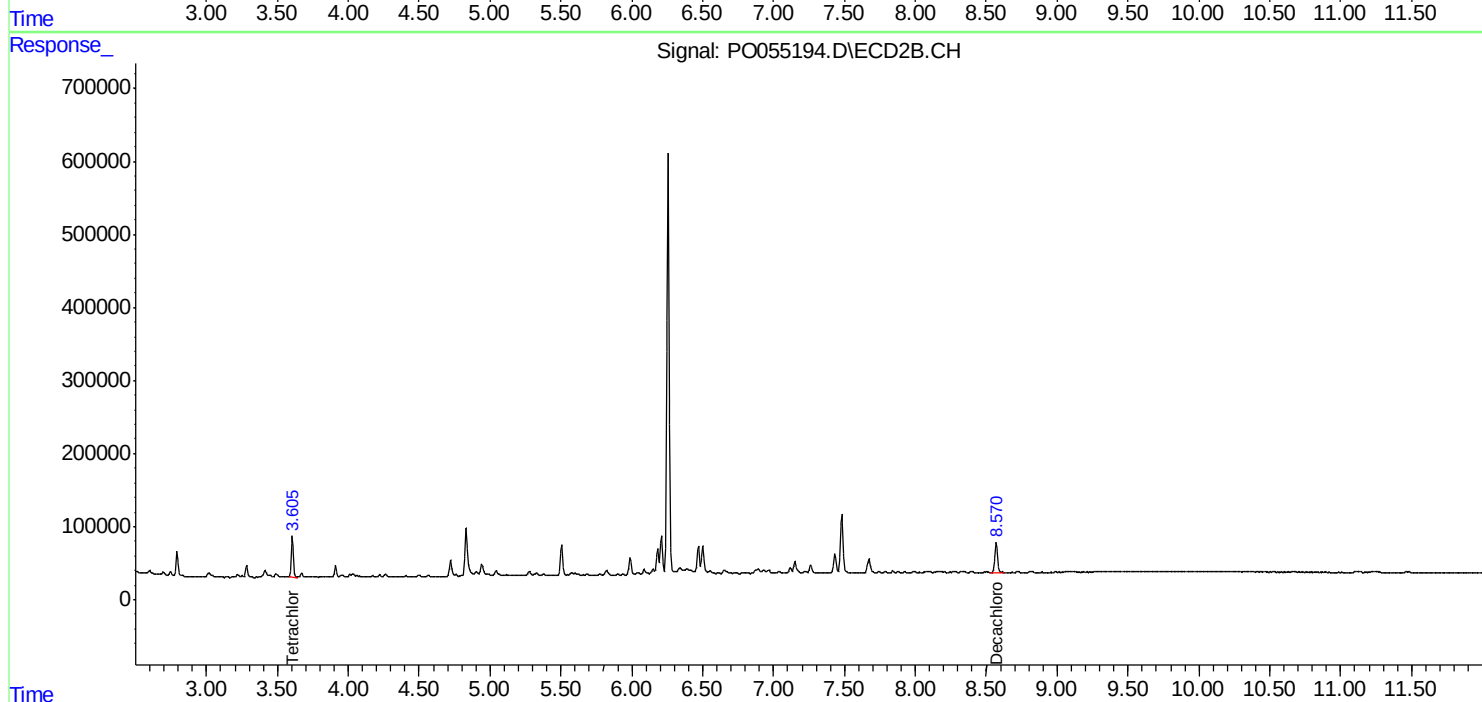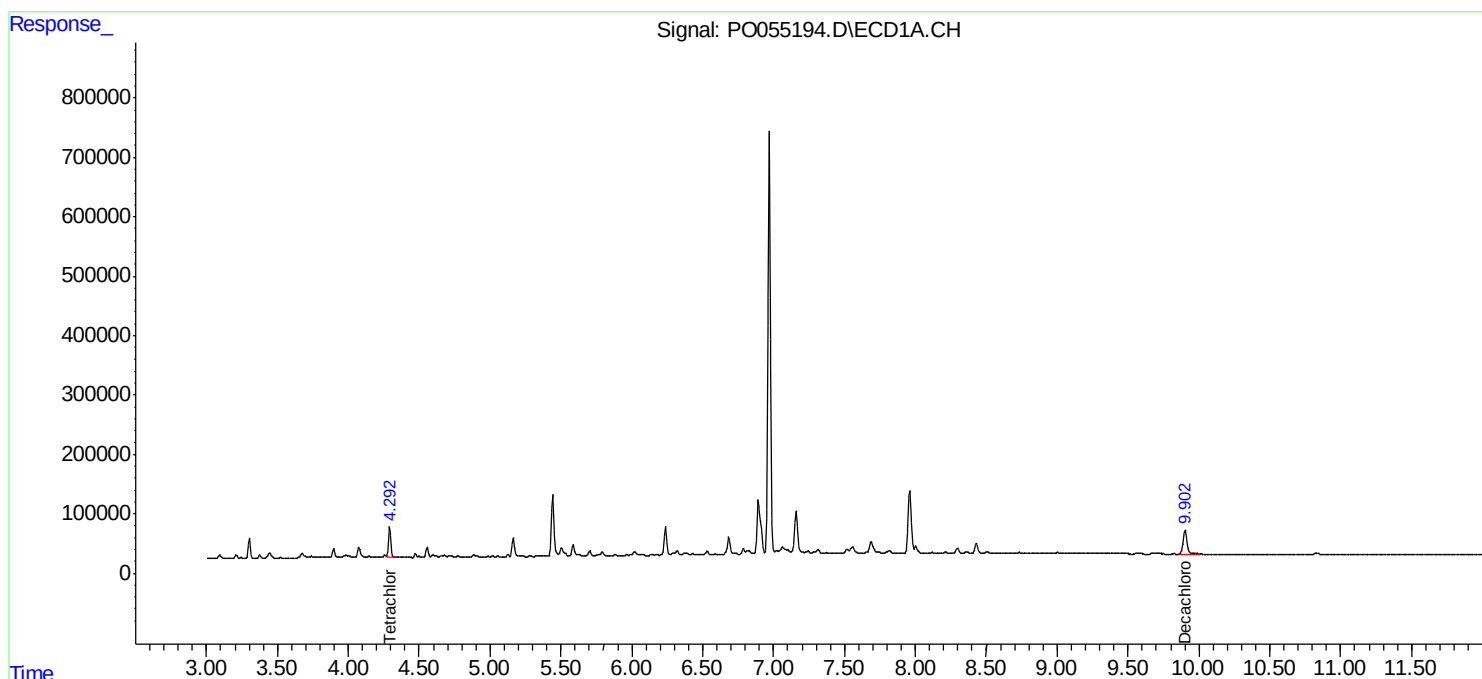

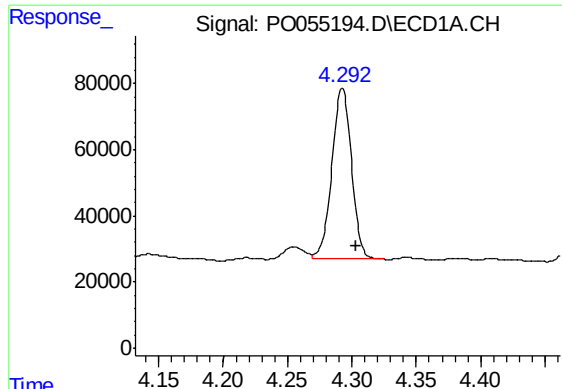


#1 Tetrachloro-m-xylene

R.T.: 4.292 min
Delta R.T.: -0.011 min
Response: 547757
Conc: 15.78 ng/ml m

Instrument :
ECD_O
ClientSampleId :
0238-COMP-CS-3-ELTRT-DISS


Manual Integrations
APPROVED

mohammad
4/15/2019 4:42:51 PM

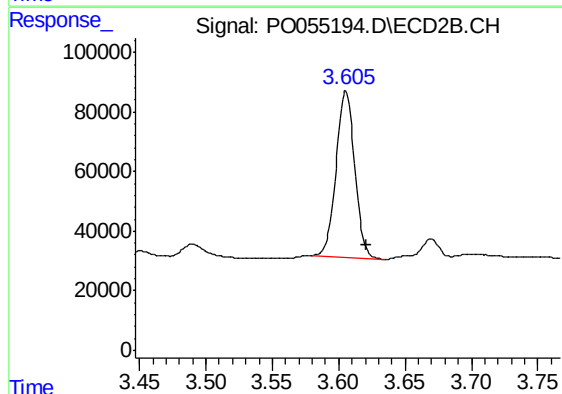


#1 Tetrachloro-m-xylene

R.T.: 3.605 min
Delta R.T.: -0.015 min
Response: 545865
Conc: 17.11 ng/ml

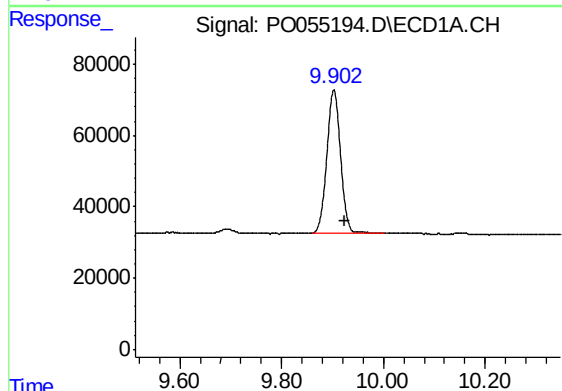

#2 Decachlorobiphenyl

R.T.: 9.902 min
Delta R.T.: -0.021 min
Response: 749725
Conc: 15.21 ng/ml

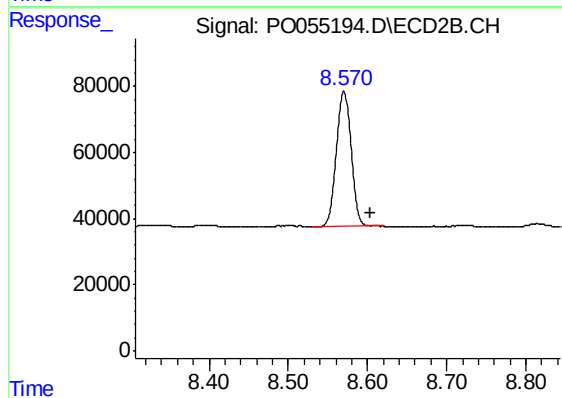

#2 Decachlorobiphenyl

R.T.: 8.570 min
Delta R.T.: -0.034 min
Response: 531164
Conc: 16.68 ng/ml