

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041219\
 Data File : P0055207.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Apr 2019 8:57
 Operator : SM/SJ
 Sample : K2361-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-01-E1-E1A-F1-F1A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 11:18:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.304	3.605	609379	564096	17.559	17.676
2)	SA Decachlor...	9.919	8.573	828810	588967	16.812	18.493
Target Compounds							
8)	L2 AR-1221-1	0.000	3.904	0	10944	N.D.	28.149 #
9)	L2 AR-1221-2	4.608	3.904	9321	10944	27.487	36.506 #
10)	L2 AR-1221-3	4.608	0.000	9321	0	8.973	N.D. #
11)	L3 AR-1232-1	4.608	0.000	9321	0	10.827	N.D. #
12)	L3 AR-1232-2	5.157	0.000	9978	0	20.399	N.D. #
32)	L7 AR-1260-2	7.382	0.000	17098	0	5.509	N.D. #
33)	L7 AR-1260-3	0.000	6.550	0	7943	N.D.	3.081 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041219\
Data File : P0055207.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Apr 2019 8:57
Operator : SM/SJ
Sample : K2361-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 11:18:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

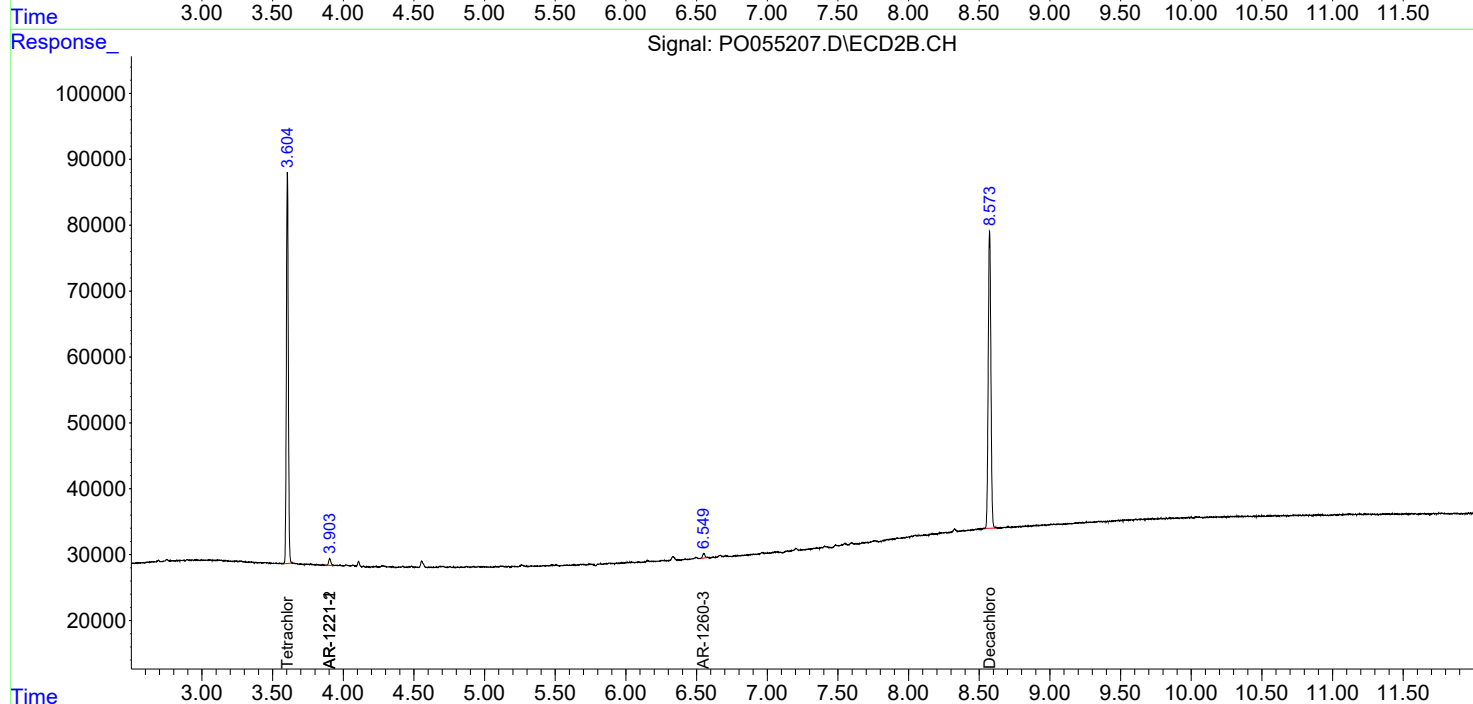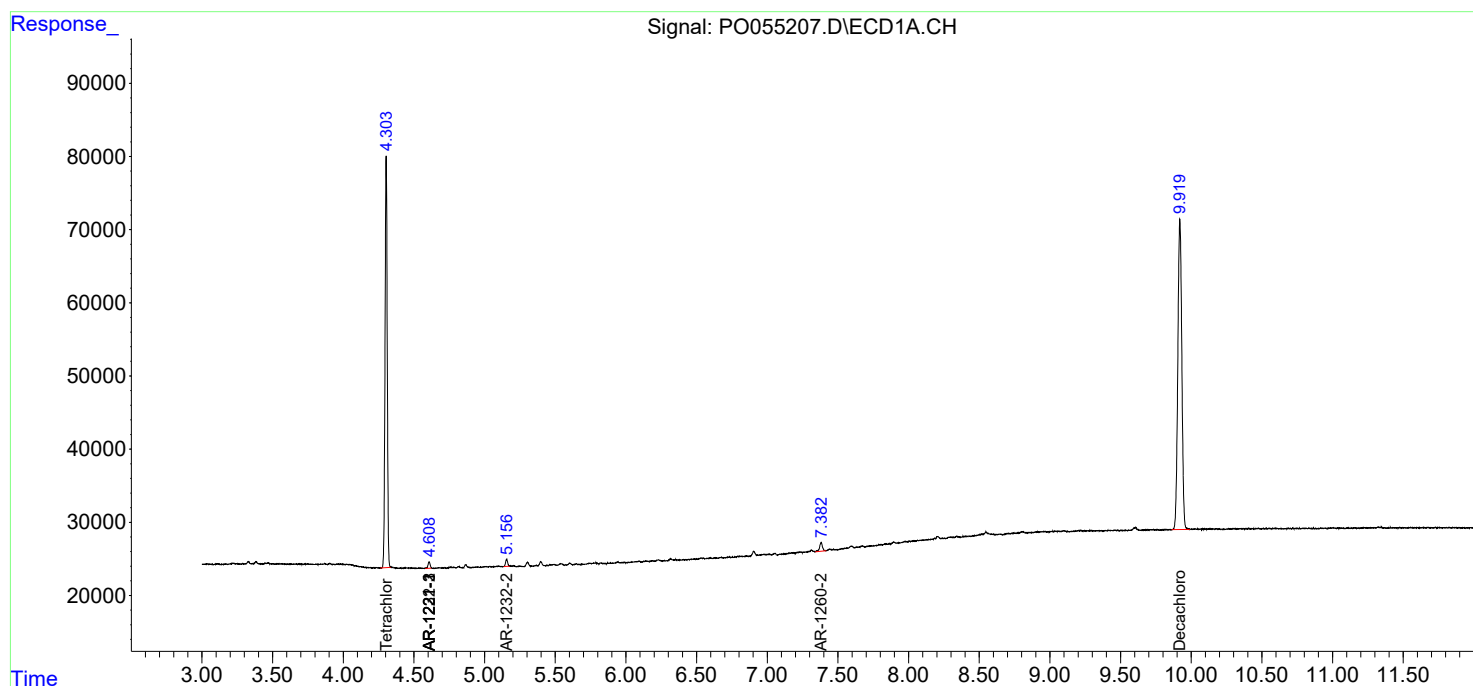


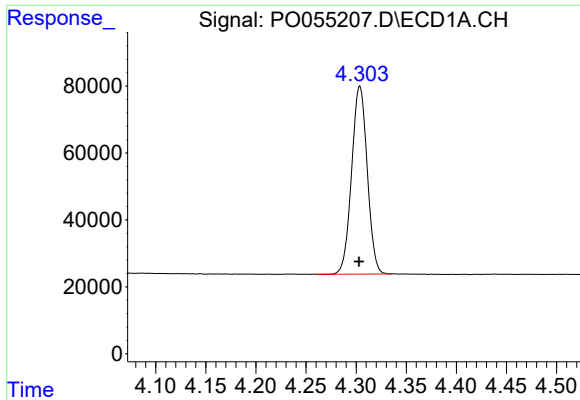

#1 Tetrachloro-m-xylene


R.T.: 4.304 min
Delta R.T.: 0.000 min
Response: 609379
Conc: 17.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1A

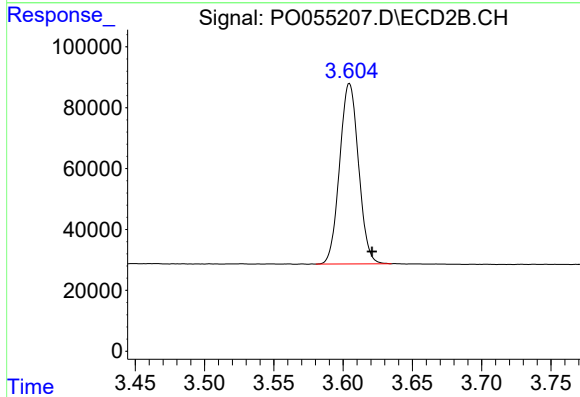


#1 Tetrachloro-m-xylene

R.T.: 3.605 min
Delta R.T.: -0.016 min
Response: 564096
Conc: 17.68 ng/ml

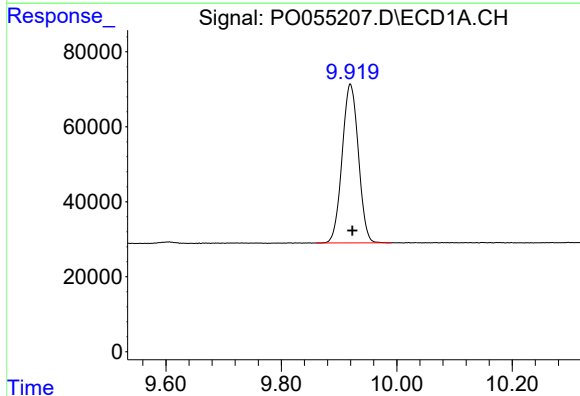


#2 Decachlorobiphenyl

R.T.: 9.919 min
Delta R.T.: -0.004 min
Response: 828810
Conc: 16.81 ng/ml

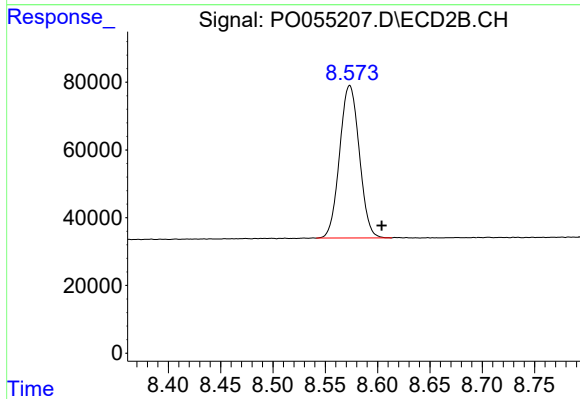

#2 Decachlorobiphenyl


R.T.: 8.573 min
Delta R.T.: -0.031 min
Response: 588967
Conc: 18.49 ng/ml

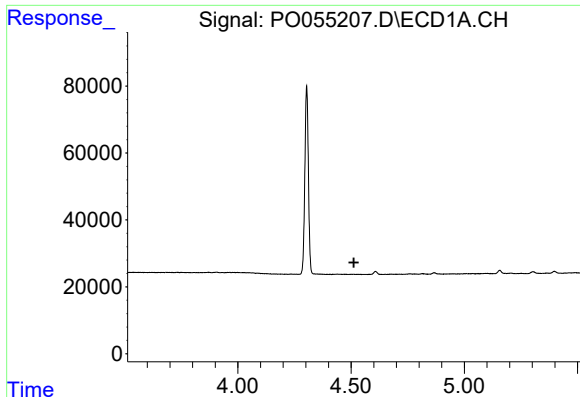

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 4.512 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1A

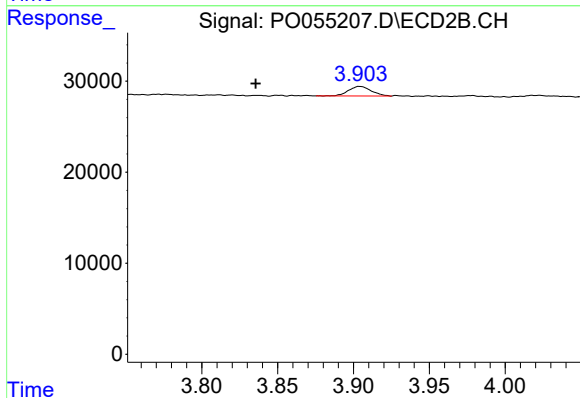


#8 AR-1221-1

R.T.: 3.904 min
Delta R.T.: 0.068 min
Response: 10944
Conc: 28.15 ng/ml

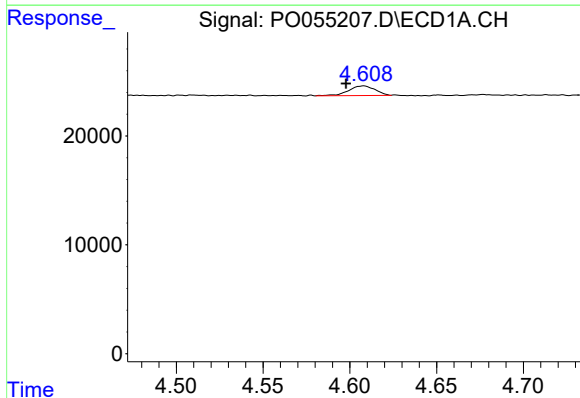


#9 AR-1221-2

R.T.: 4.608 min
Delta R.T.: 0.010 min
Response: 9321
Conc: 27.49 ng/ml

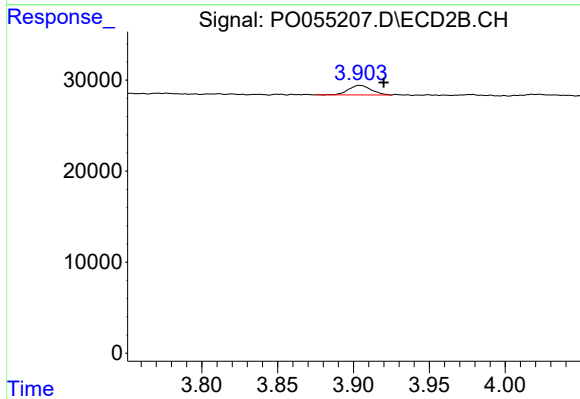

#9 AR-1221-2


R.T.: 3.904 min
Delta R.T.: -0.016 min
Response: 10944
Conc: 36.51 ng/ml

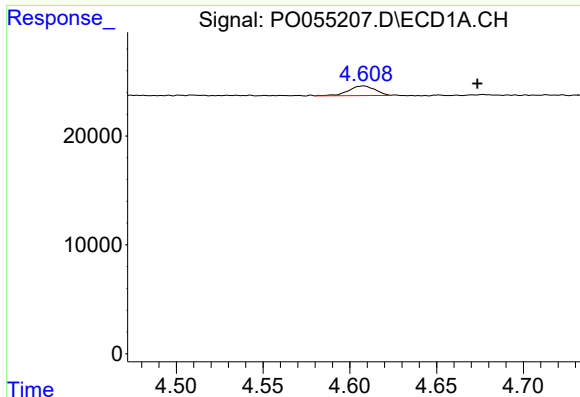

#10 AR-1221-3


R.T.: 4.608 min
Delta R.T.: -0.065 min
Response: 9321
Conc: 8.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1A

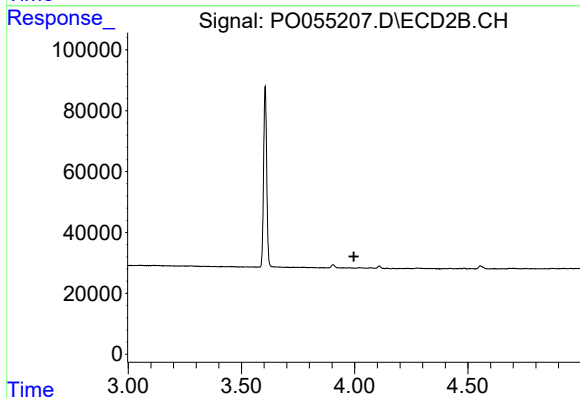


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 3.996 min
Response: 0
Conc: N.D.

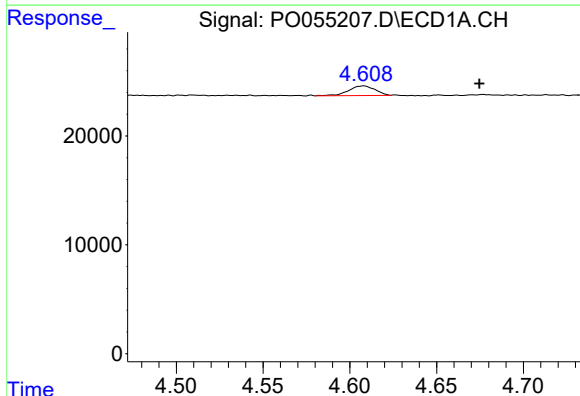


#11 AR-1232-1

R.T.: 4.608 min
Delta R.T.: -0.066 min
Response: 9321
Conc: 10.83 ng/ml

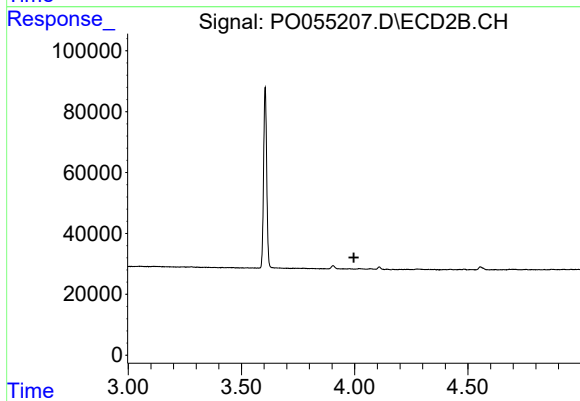

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T. : 3.997 min
Response: 0
Conc: N.D.

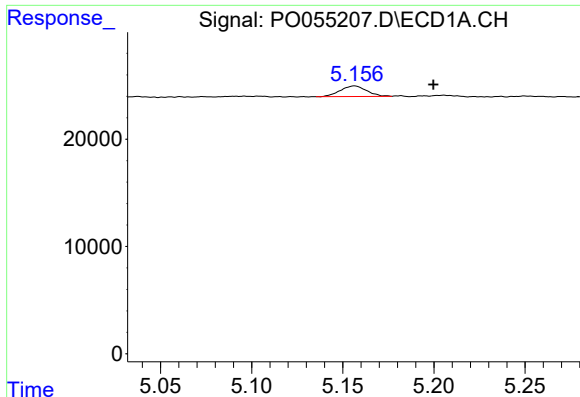

#12 AR-1232-2


R.T.: 5.157 min
Delta R.T.: -0.043 min
Response: 9978
Conc: 20.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1A

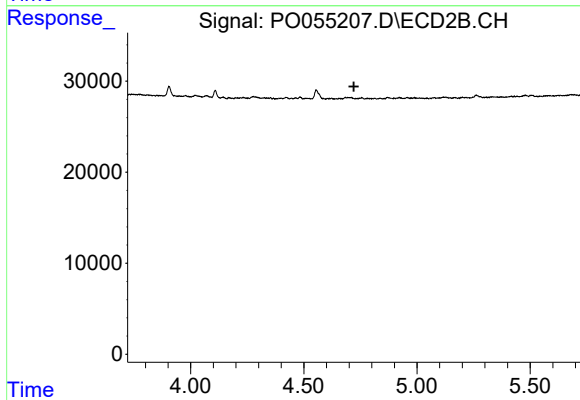


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 4.721 min
Response: 0
Conc: N.D.

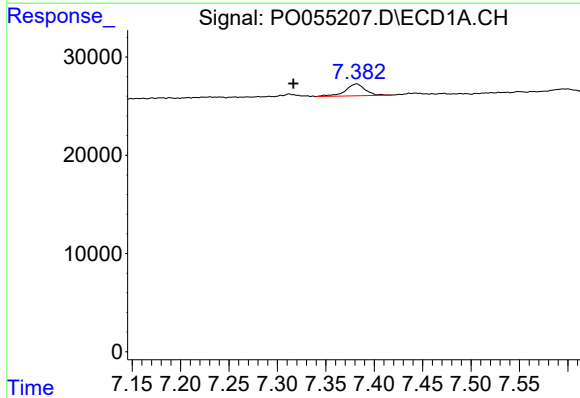


#32 AR-1260-2

R.T.: 7.382 min
Delta R.T.: 0.066 min
Response: 17098
Conc: 5.51 ng/ml

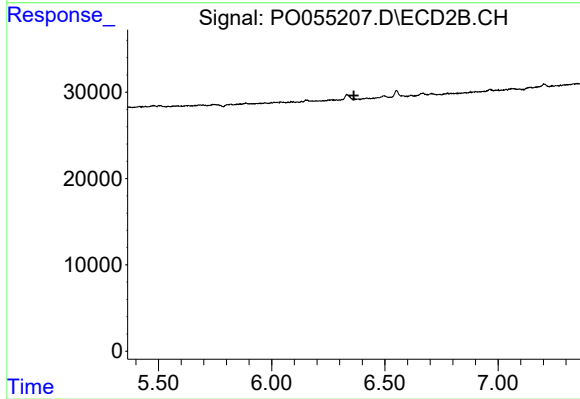

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.363 min
Response: 0
Conc: N.D.

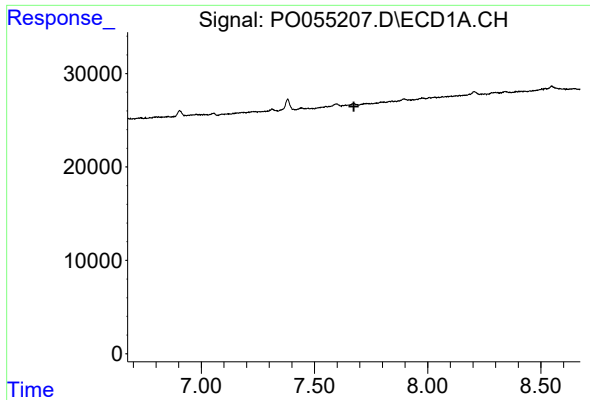

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 7.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1A

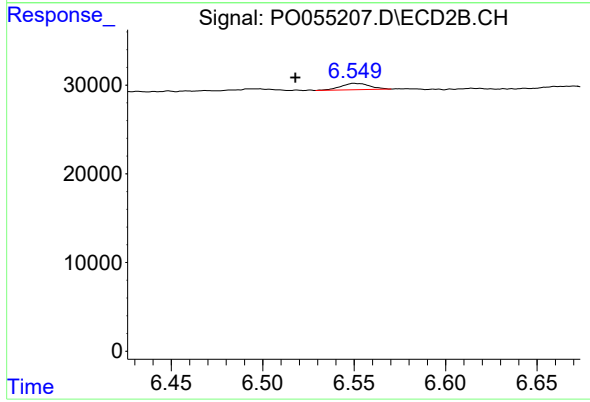

#33 AR-1260-3

R.T.: 6.550 min
Delta R.T.: 0.032 min
Response: 7943
Conc: 3.08 ng/ml