

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0041219\
 Data File : P0055208.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Apr 2019 9:14
 Operator : SM/SJ
 Sample : K2361-01MS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 FK-BPM-01-E1-E1A-F1-F1AMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 11:18:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.294	3.604	616469	583178	17.763	18.274
2)	SA Decachlor...	9.905	8.569	937483	675533	19.017	21.211
Target Compounds							
3)	L1 AR-1016-1	5.455	4.699	330245	399790	183.528	252.808 #
4)	L1 AR-1016-2	5.477	4.729	457918	33591	184.371	15.677 #
5)	L1 AR-1016-3	5.538	4.914	302246	170219	192.116	140.883 #
6)	L1 AR-1016-4	5.637	4.956	245698	219918	188.552	217.626
7)	L1 AR-1016-5	5.929	5.167	264383	-1328	198.150	N.D. #
8)	L2 AR-1221-1	4.495	3.815	25087	24525	57.463	63.081
9)	L2 AR-1221-2	4.590	3.901	39993	36276	117.933	121.004
10)	L2 AR-1221-3	4.665	3.977	147331	125873	141.831	136.554
11)	L3 AR-1232-1	4.665	3.977	147331	125873	171.123	167.855
12)	L3 AR-1232-2	5.189	4.729	224656	33591	459.290	39.009 #
13)	L3 AR-1232-3	5.477	4.914	457918	170219	468.552	351.282 #
14)	L3 AR-1232-4	5.637	4.987	245698	77554	480.017	176.499 #
15)	L3 AR-1232-5	5.726	5.167	240069	-1328	577.094	N.D. #
16)	L4 AR-1242-1	5.455	4.699	330245	399790	237.707	325.639 #
17)	L4 AR-1242-2	5.477	4.729	457918	33591	239.313	20.269 #
18)	L4 AR-1242-3	5.538	4.914	302246	170219	243.854	179.683 #
19)	L4 AR-1242-4	5.637	4.987	245698	77554	240.988	81.144 #
20)	L4 AR-1242-5	6.368	5.517	43800	35979	36.283	29.254
21)	L5 AR-1248-1	5.455	4.699	330245	399790	330.352	455.458 #
22)	L5 AR-1248-2	5.726	4.956	240069	219918	165.303	181.969
23)	L5 AR-1248-3	5.929	4.987	264383	77554	165.533	62.153 #
24)	L5 AR-1248-4	6.331	5.167	47113	-1328	25.079	N.D. #
25)	L5 AR-1248-5	6.368	5.517	43800	35979	24.431	24.133
26)	L6 AR-1254-1	6.304	5.517	218067	35979	120.268	16.463 #
27)	L6 AR-1254-2	6.520	5.621	248173	204665	86.934	105.554
28)	L6 AR-1254-3	6.886	6.038	145675	368372	46.324	114.912 #
29)	L6 AR-1254-4	7.170	6.278	98016	134186	40.066	68.534 #
30)	L6 AR-1254-5	7.587	6.702	828367	454296	309.057	158.032 #
31)	L7 AR-1260-1	7.048	6.152	567931	511329	226.029	222.504
32)	L7 AR-1260-2	7.304	6.339	682784	612426	220.003	222.477
33)	L7 AR-1260-3	7.661	6.492	454561	577274	185.205	223.931
34)	L7 AR-1260-4	7.886	7.000	553679	64927	200.173	30.509 #
35)	L7 AR-1260-5	8.196	7.201	967666	919210	174.398	191.930
36)	L8 AR-1262-1	7.661	6.755	454561	240553	136.420	80.860 #
37)	L8 AR-1262-2	8.196	7.256	967666	25092	163.335	5.120 #
38)	L8 AR-1262-3	8.508	7.483	649977	189168	156.893	92.122 #
39)	L8 AR-1262-4	8.559	7.546	357378	654256	110.919	180.628 #
40)	L8 AR-1262-5	9.202	8.082	236866	11874	108.342	7.357 #
41)	L9 AR-1268-1	8.508	7.483	649977	189168	91.321	33.456 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041219\
 Data File : P0055208.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Apr 2019 9:14
 Operator : SM/SJ
 Sample : K2361-01MS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-01-E1-E1A-F1-F1AMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 11:18:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.559	7.546	357378	654256	54.545	126.510 #
43) L9	AR-1268-3	8.794	7.799	21041	13091	3.862	3.042
44) L9	AR-1268-4	9.202	8.082	236866	11874	99.282	6.405 #
45) L9	AR-1268-5	9.590	0.000	85656	0	5.199	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041219\
Data File : P0055208.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Apr 2019 9:14
Operator : SM/SJ
Sample : K2361-01MS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 11:18:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

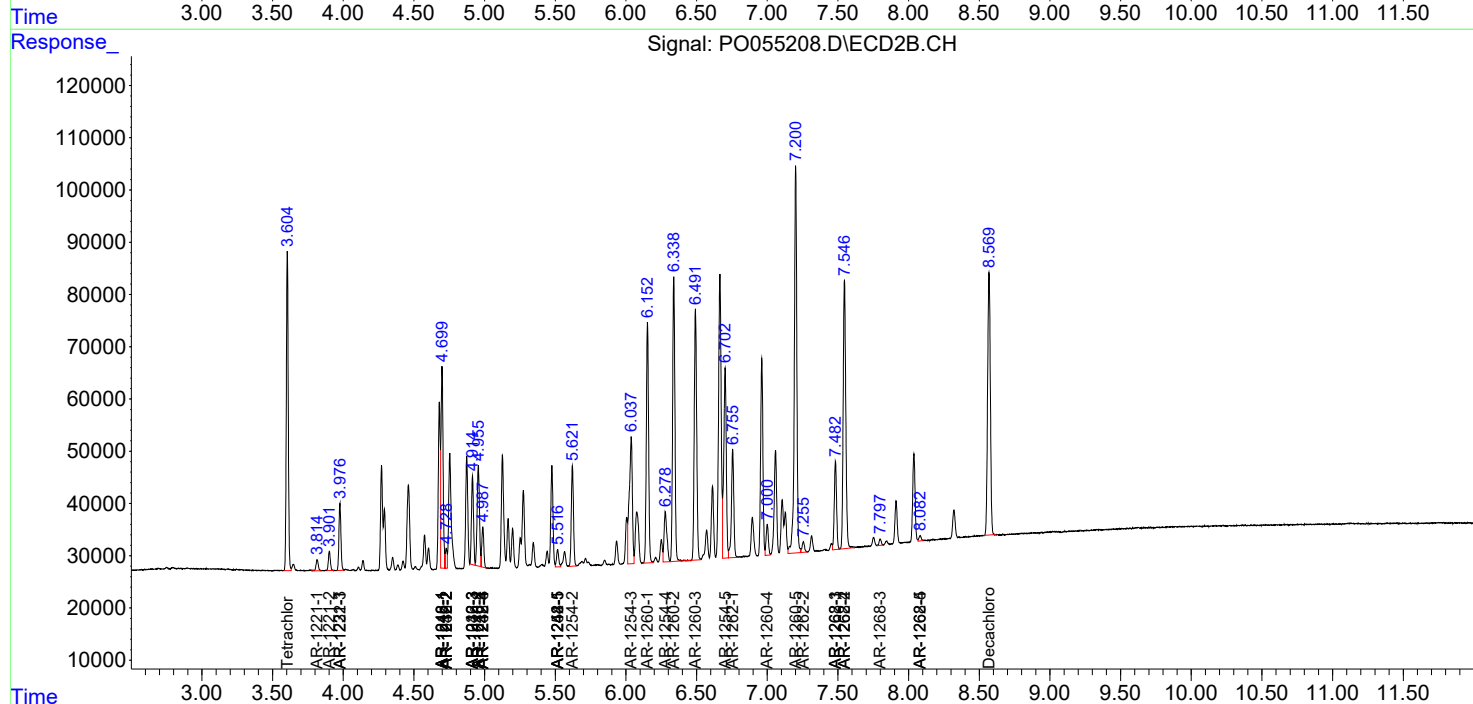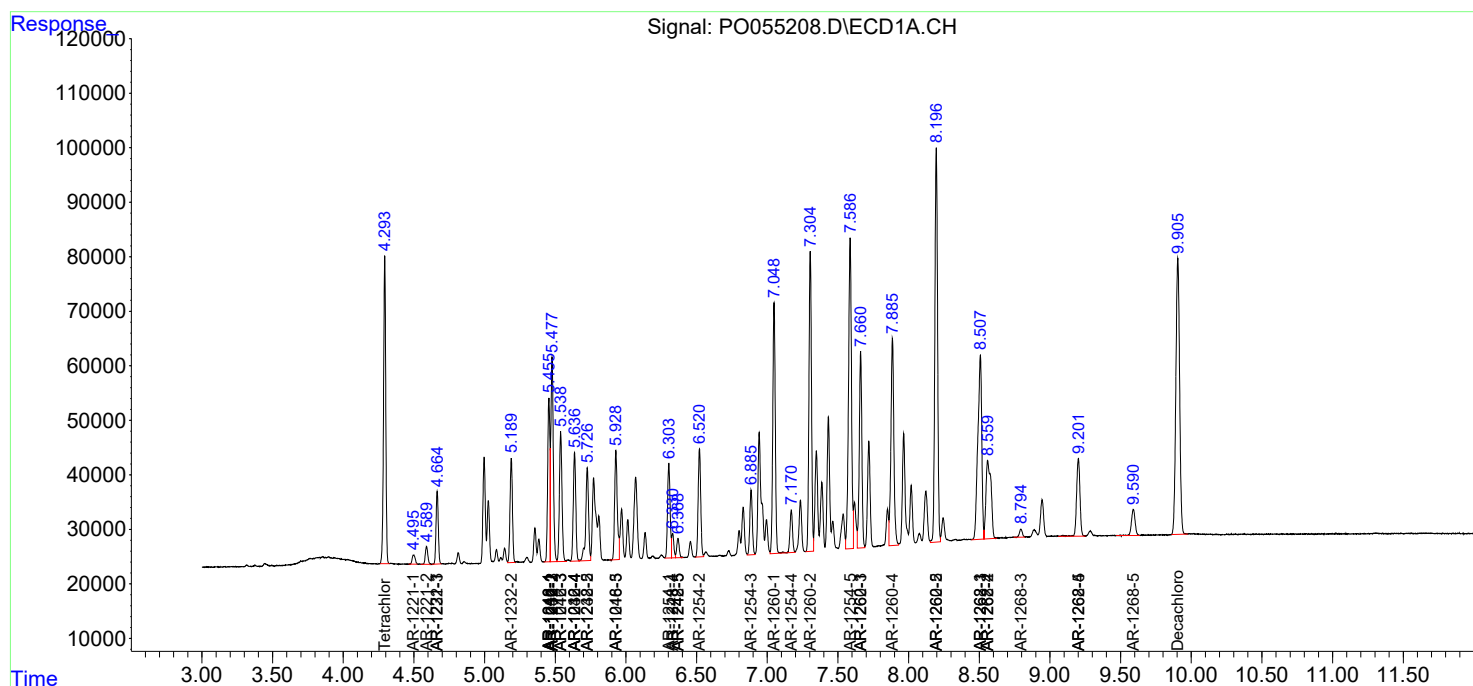


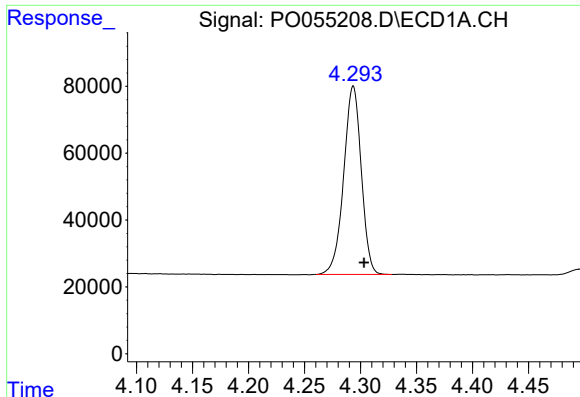

#1 Tetrachloro-m-xylene


R.T.: 4.294 min
Delta R.T.: -0.009 min
Response: 616469
Conc: 17.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

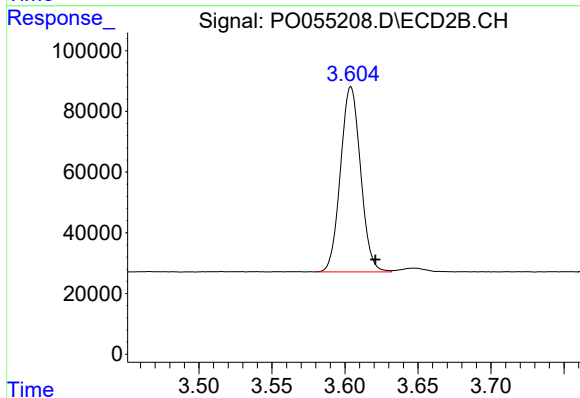


#1 Tetrachloro-m-xylene

R.T.: 3.604 min
Delta R.T.: -0.017 min
Response: 583178
Conc: 18.27 ng/ml

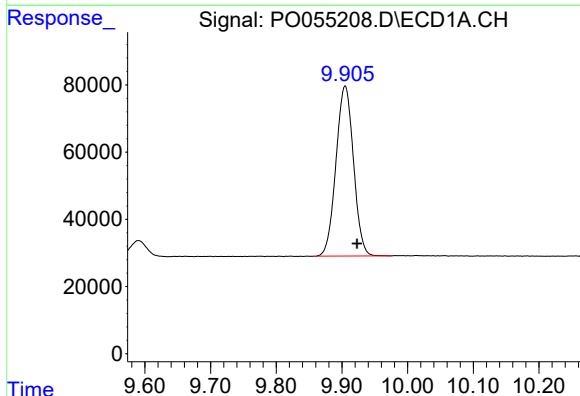


#2 Decachlorobiphenyl

R.T.: 9.905 min
Delta R.T.: -0.018 min
Response: 937483
Conc: 19.02 ng/ml

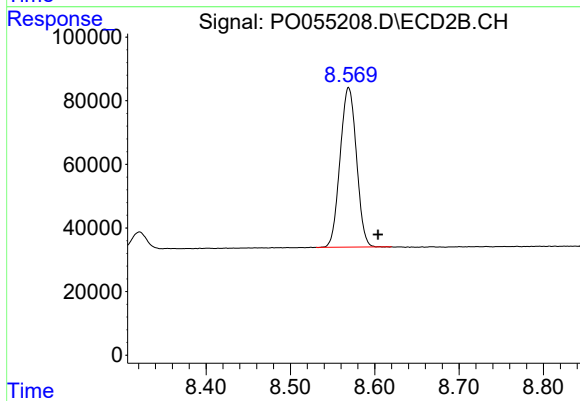

#2 Decachlorobiphenyl


R.T.: 8.569 min
Delta R.T.: -0.035 min
Response: 675533
Conc: 21.21 ng/ml

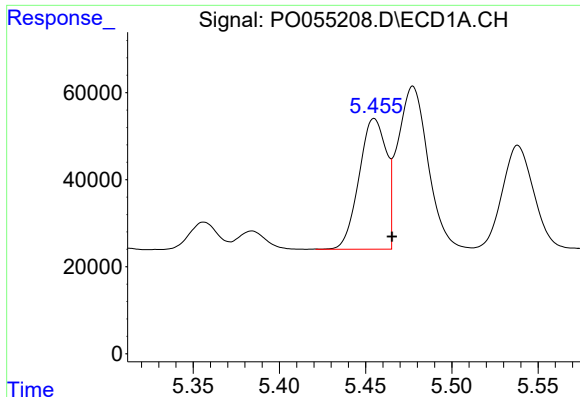

#3 AR-1016-1


R.T.: 5.455 min
Delta R.T.: -0.010 min
Response: 330245
Conc: 183.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

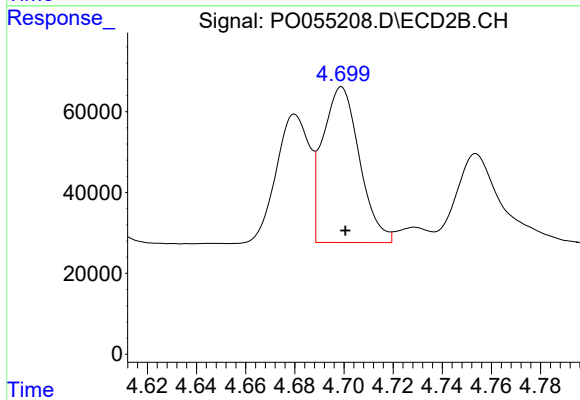


#3 AR-1016-1

R.T.: 4.699 min
Delta R.T.: -0.002 min
Response: 399790
Conc: 252.81 ng/ml

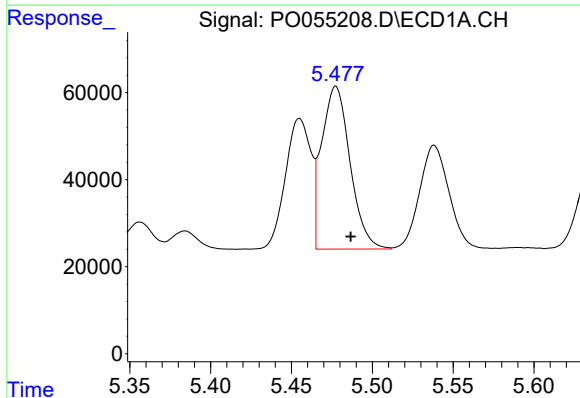


#4 AR-1016-2

R.T.: 5.477 min
Delta R.T.: -0.009 min
Response: 457918
Conc: 184.37 ng/ml

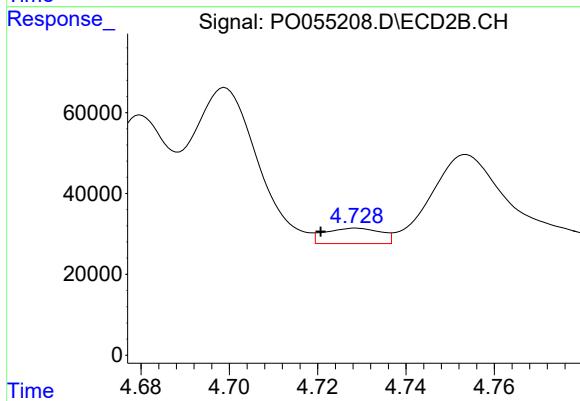

#4 AR-1016-2


R.T.: 4.729 min
Delta R.T.: 0.008 min
Response: 33591
Conc: 15.68 ng/ml

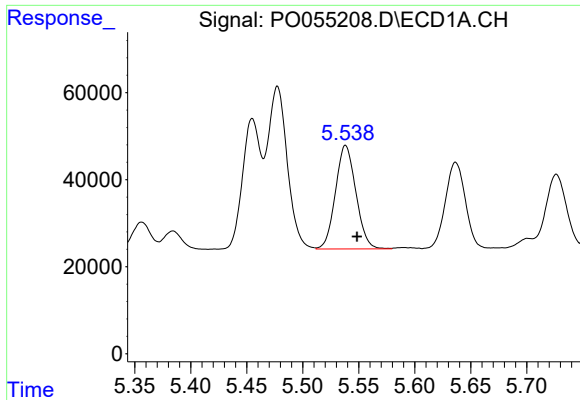

#5 AR-1016-3


R.T.: 5.538 min
Delta R.T.: -0.010 min
Response: 302246
Conc: 192.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

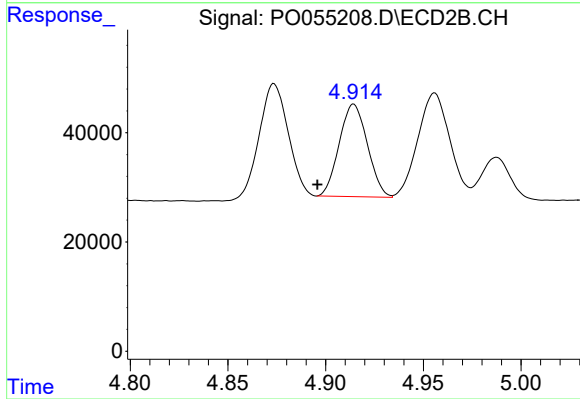


#5 AR-1016-3

R.T.: 4.914 min
Delta R.T.: 0.019 min
Response: 170219
Conc: 140.88 ng/ml

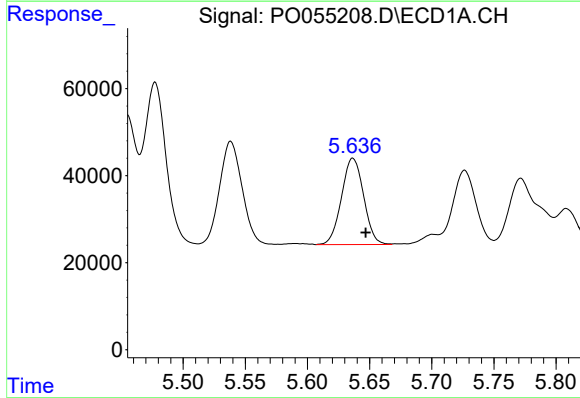


#6 AR-1016-4

R.T.: 5.637 min
Delta R.T.: -0.010 min
Response: 245698
Conc: 188.55 ng/ml

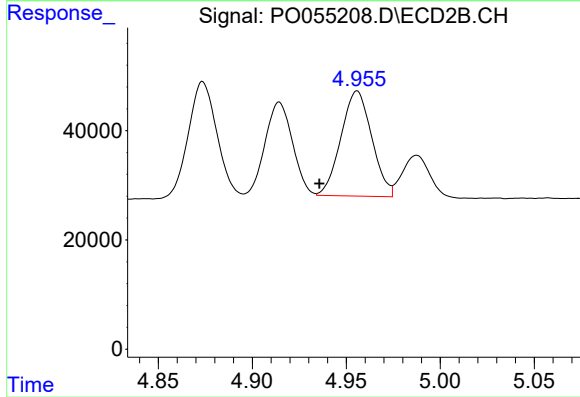

#6 AR-1016-4


R.T.: 4.956 min
Delta R.T.: 0.020 min
Response: 219918
Conc: 217.63 ng/ml

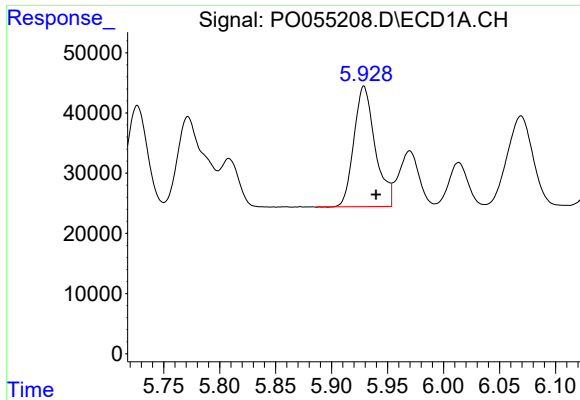

#7 AR-1016-5


R.T.: 5.929 min
Delta R.T.: -0.011 min
Response: 264383
Conc: 198.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

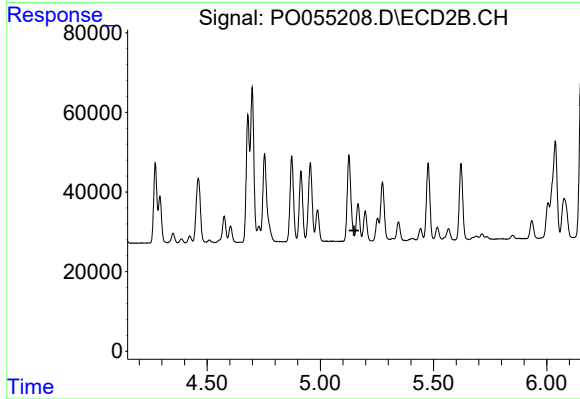


#7 AR-1016-5

R.T.: 5.167 min
Delta R.T.: 0.018 min
Response: -1328
Conc: N.D.

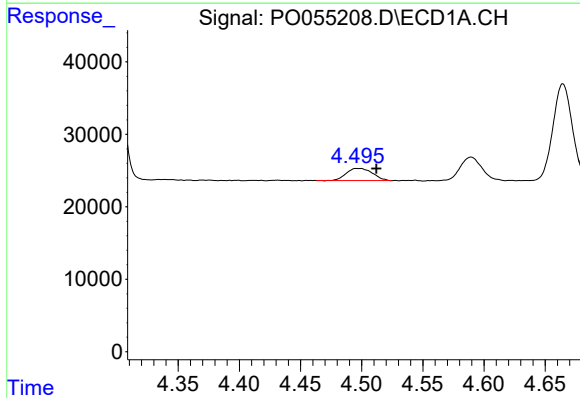


#8 AR-1221-1

R.T.: 4.495 min
Delta R.T.: -0.017 min
Response: 25087
Conc: 57.46 ng/ml

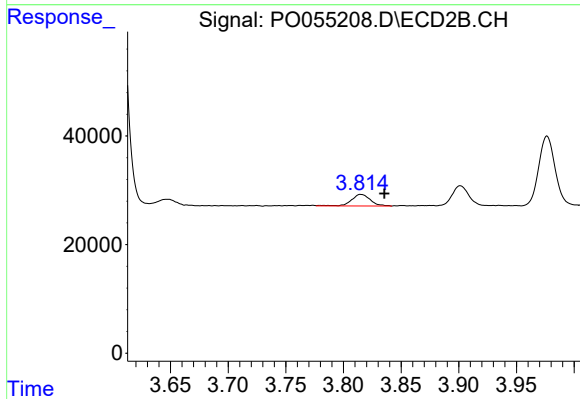

#8 AR-1221-1


R.T.: 3.815 min
Delta R.T.: -0.021 min
Response: 24525
Conc: 63.08 ng/ml

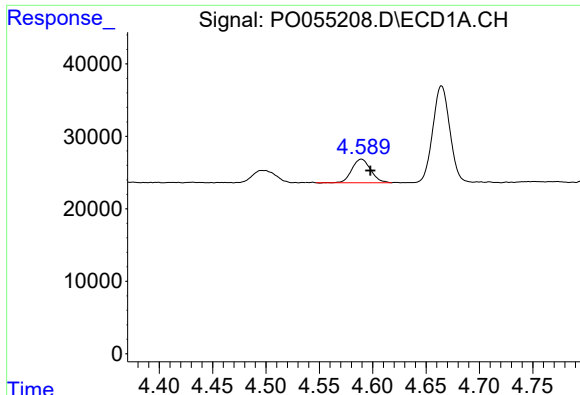

#9 AR-1221-2


R.T.: 4.590 min
Delta R.T.: -0.008 min
Response: 39993
Conc: 117.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

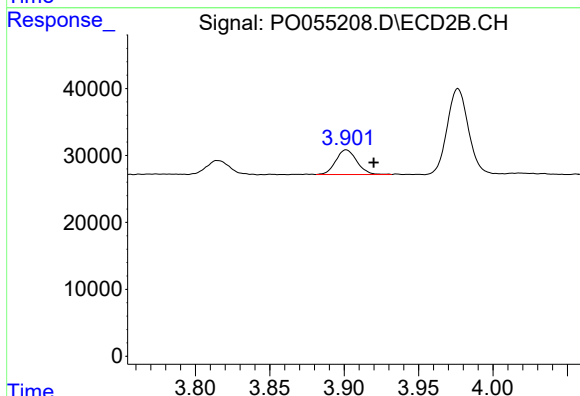


#9 AR-1221-2

R.T.: 3.901 min
Delta R.T.: -0.018 min
Response: 36276
Conc: 121.00 ng/ml

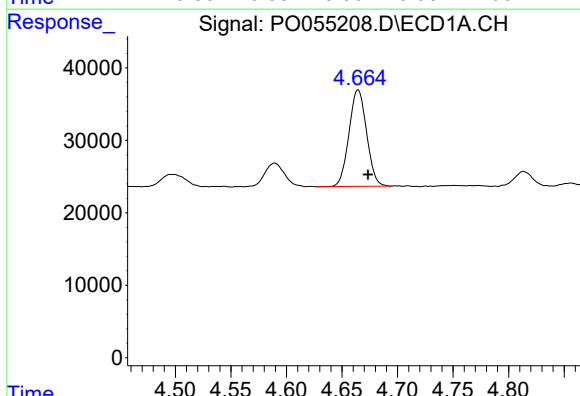


#10 AR-1221-3

R.T.: 4.665 min
Delta R.T.: -0.009 min
Response: 147331
Conc: 141.83 ng/ml

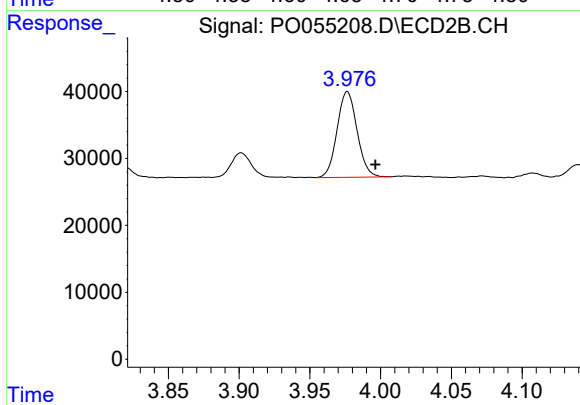

#10 AR-1221-3


R.T.: 3.977 min
Delta R.T.: -0.020 min
Response: 125873
Conc: 136.55 ng/ml

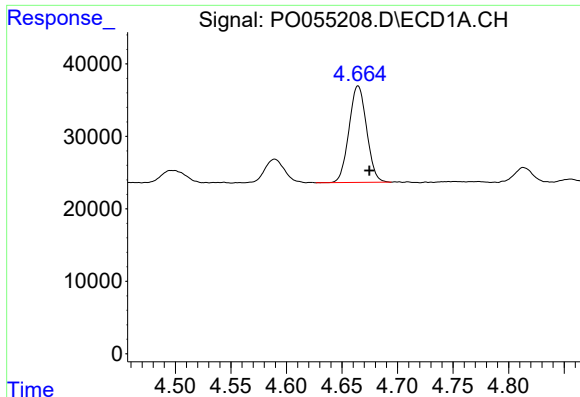

#11 AR-1232-1


R.T.: 4.665 min
Delta R.T.: -0.010 min
Response: 147331
Conc: 171.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

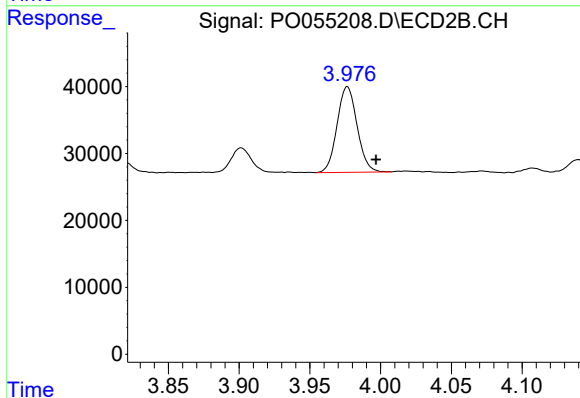


#11 AR-1232-1

R.T.: 3.977 min
Delta R.T.: -0.020 min
Response: 125873
Conc: 167.85 ng/ml

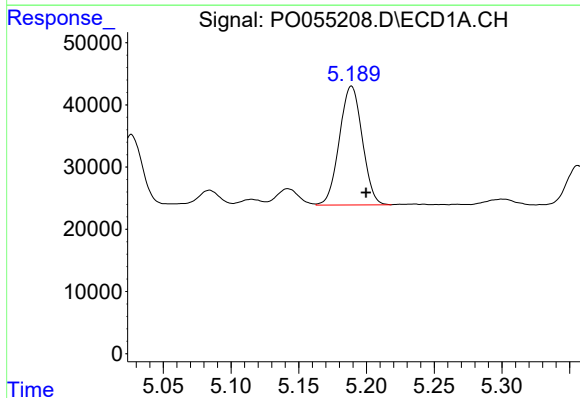


#12 AR-1232-2

R.T.: 5.189 min
Delta R.T.: -0.011 min
Response: 224656
Conc: 459.29 ng/ml

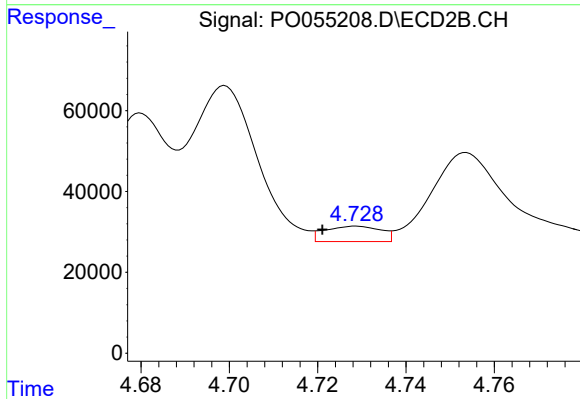

#12 AR-1232-2


R.T.: 4.729 min
Delta R.T.: 0.008 min
Response: 33591
Conc: 39.01 ng/ml

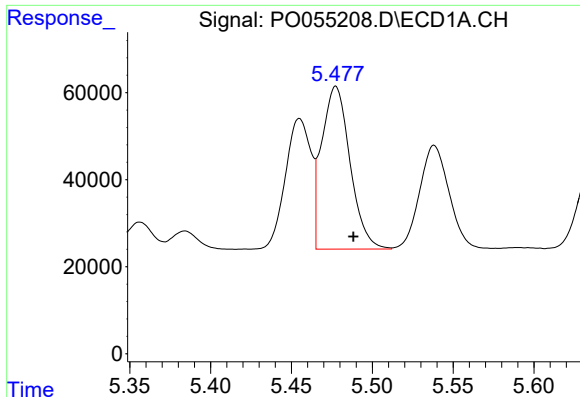

#13 AR-1232-3


R.T.: 5.477 min
Delta R.T.: -0.011 min
Response: 457918
Conc: 468.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

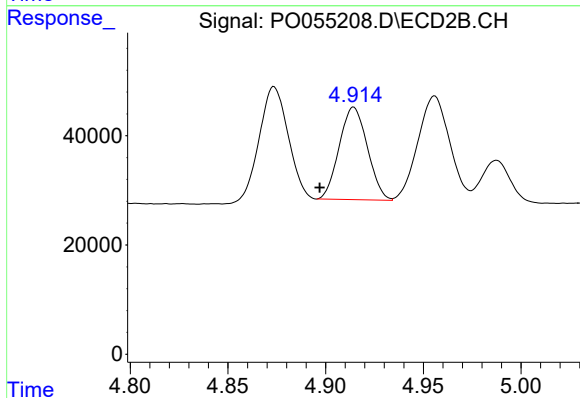


#13 AR-1232-3

R.T.: 4.914 min
Delta R.T.: 0.017 min
Response: 170219
Conc: 351.28 ng/ml

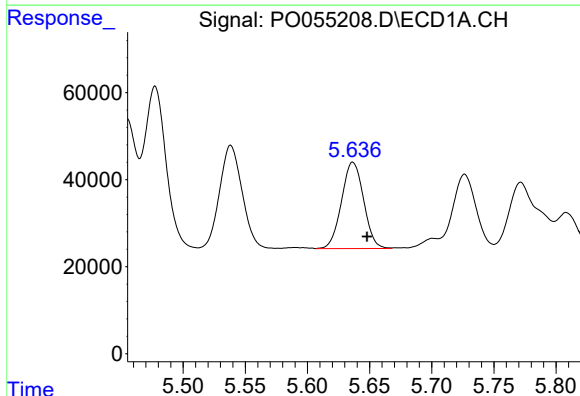


#14 AR-1232-4

R.T.: 5.637 min
Delta R.T.: -0.012 min
Response: 245698
Conc: 480.02 ng/ml

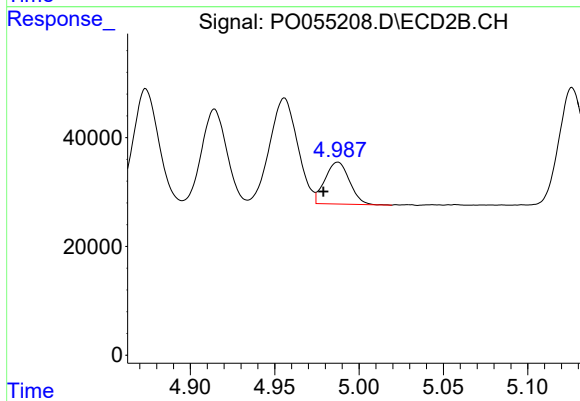

#14 AR-1232-4


R.T.: 4.987 min
Delta R.T.: 0.009 min
Response: 77554
Conc: 176.50 ng/ml

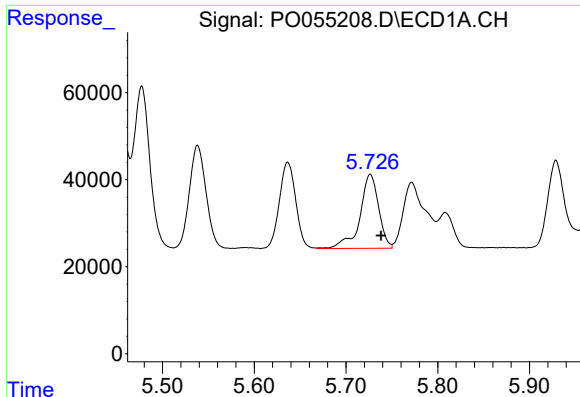

#15 AR-1232-5


R.T.: 5.726 min
Delta R.T.: -0.012 min
Response: 240069
Conc: 577.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

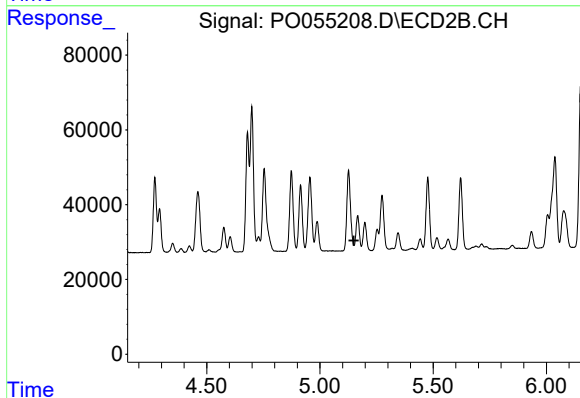


#15 AR-1232-5

R.T.: 5.167 min
Delta R.T.: 0.017 min
Response: -1328
Conc: N.D.

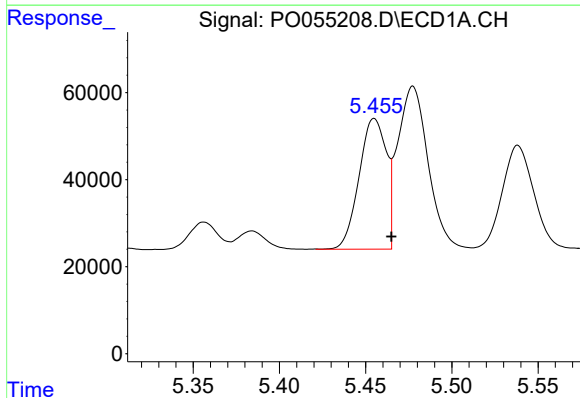


#16 AR-1242-1

R.T.: 5.455 min
Delta R.T.: -0.010 min
Response: 330245
Conc: 237.71 ng/ml

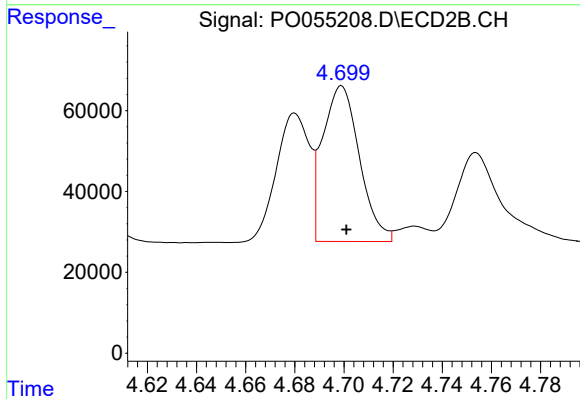

#16 AR-1242-1


R.T.: 4.699 min
Delta R.T.: -0.002 min
Response: 399790
Conc: 325.64 ng/ml

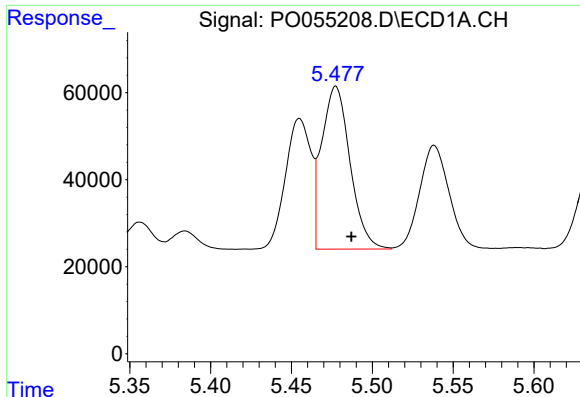

#17 AR-1242-2


R.T.: 5.477 min
Delta R.T.: -0.010 min
Response: 457918
Conc: 239.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

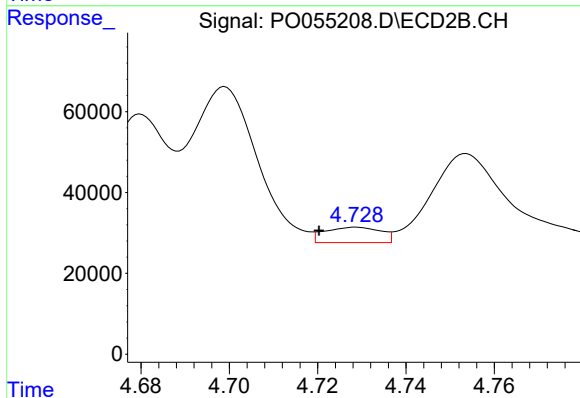


#17 AR-1242-2

R.T.: 4.729 min
Delta R.T.: 0.008 min
Response: 33591
Conc: 20.27 ng/ml

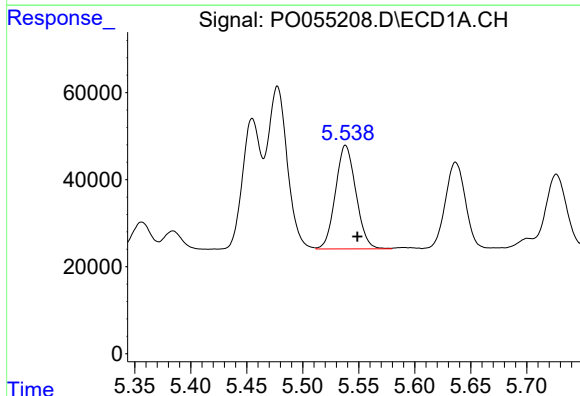


#18 AR-1242-3

R.T.: 5.538 min
Delta R.T.: -0.011 min
Response: 302246
Conc: 243.85 ng/ml

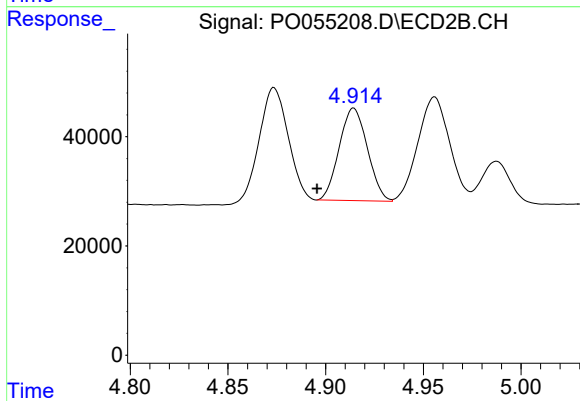

#18 AR-1242-3


R.T.: 4.914 min
Delta R.T.: 0.019 min
Response: 170219
Conc: 179.68 ng/ml

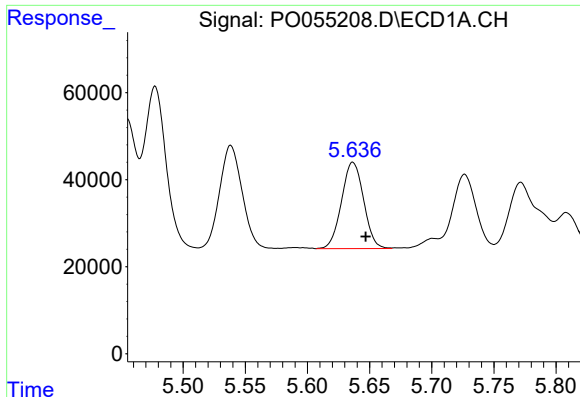

#19 AR-1242-4


R.T.: 5.637 min
Delta R.T.: -0.010 min
Response: 245698
Conc: 240.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

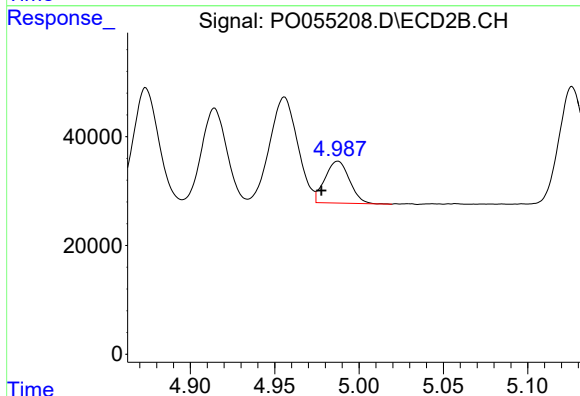


#19 AR-1242-4

R.T.: 4.987 min
Delta R.T.: 0.010 min
Response: 77554
Conc: 81.14 ng/ml

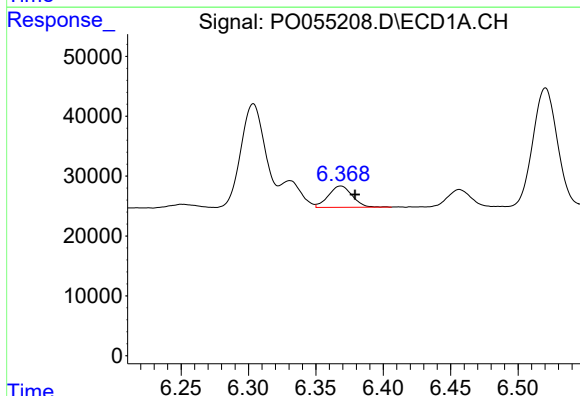


#20 AR-1242-5

R.T.: 6.368 min
Delta R.T.: -0.011 min
Response: 43800
Conc: 36.28 ng/ml

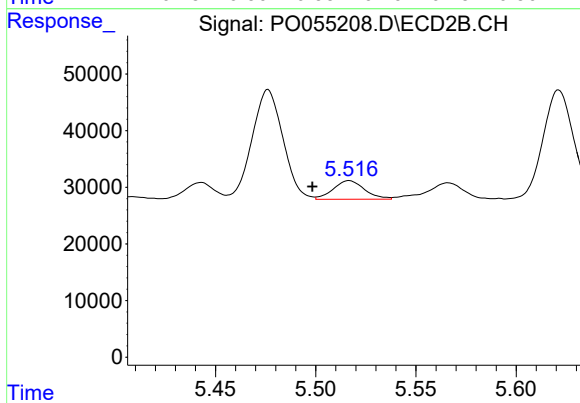

#20 AR-1242-5


R.T.: 5.517 min
Delta R.T.: 0.018 min
Response: 35979
Conc: 29.25 ng/ml

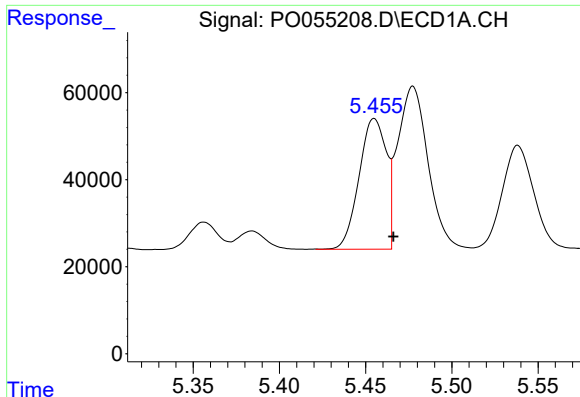

#21 AR-1248-1


R.T.: 5.455 min
Delta R.T.: -0.011 min
Response: 330245
Conc: 330.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

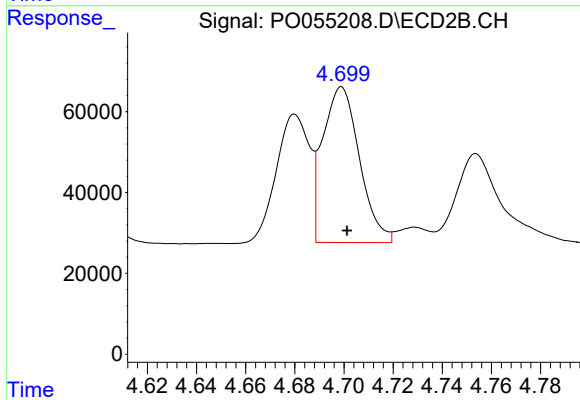


#21 AR-1248-1

R.T.: 4.699 min
Delta R.T.: -0.002 min
Response: 399790
Conc: 455.46 ng/ml

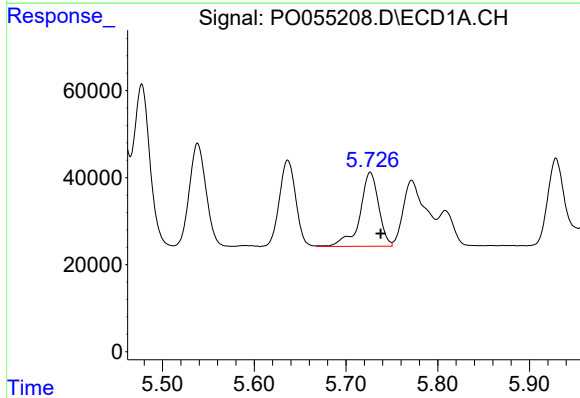


#22 AR-1248-2

R.T.: 5.726 min
Delta R.T.: -0.011 min
Response: 240069
Conc: 165.30 ng/ml

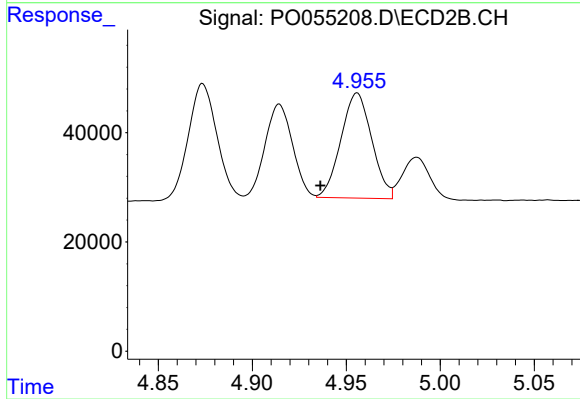

#22 AR-1248-2


R.T.: 4.956 min
Delta R.T.: 0.020 min
Response: 219918
Conc: 181.97 ng/ml

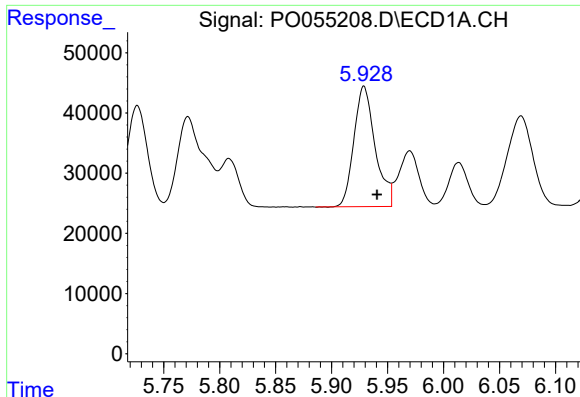

#23 AR-1248-3


R.T.: 5.929 min
Delta R.T.: -0.012 min
Response: 264383
Conc: 165.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

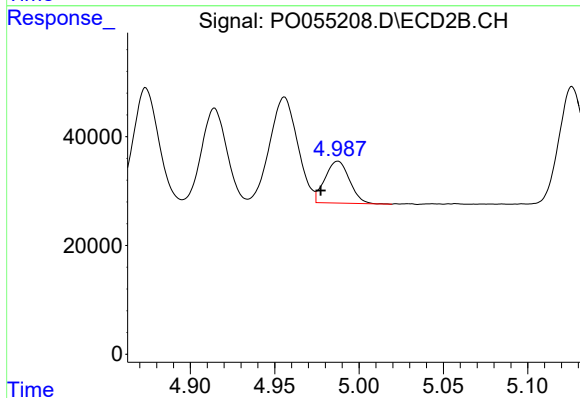


#23 AR-1248-3

R.T.: 4.987 min
Delta R.T.: 0.010 min
Response: 77554
Conc: 62.15 ng/ml

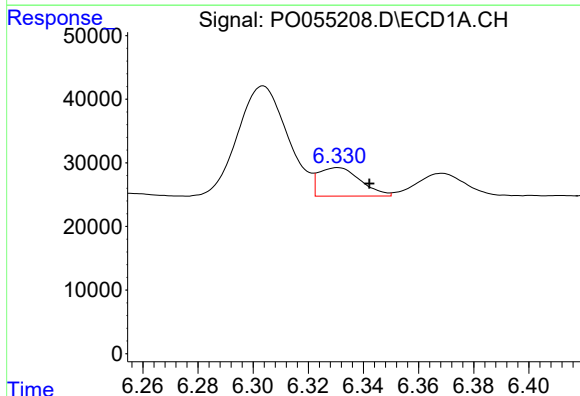


#24 AR-1248-4

R.T.: 6.331 min
Delta R.T.: -0.011 min
Response: 47113
Conc: 25.08 ng/ml

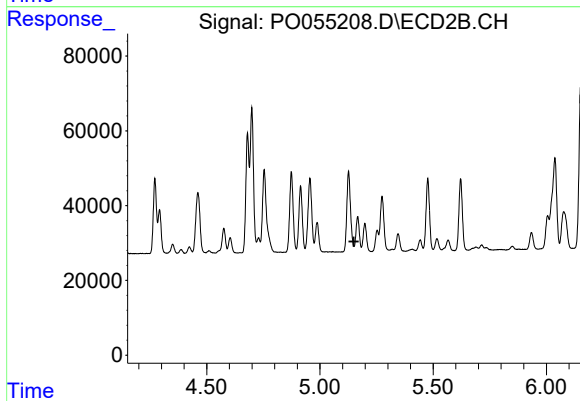

#24 AR-1248-4


R.T.: 5.167 min
Delta R.T.: 0.017 min
Response: -1328
Conc: N.D.

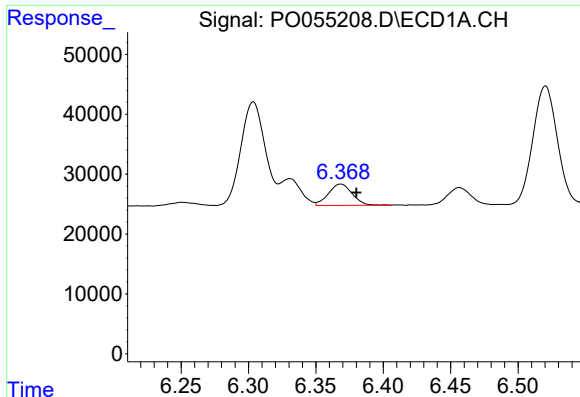

#25 AR-1248-5


R.T.: 6.368 min
Delta R.T.: -0.012 min
Response: 43800
Conc: 24.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

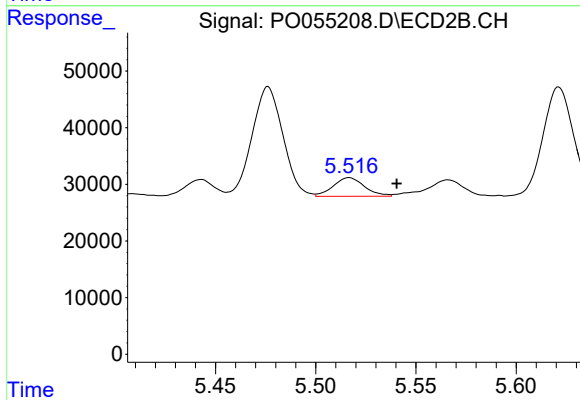


#25 AR-1248-5

R.T.: 5.517 min
Delta R.T.: -0.024 min
Response: 35979
Conc: 24.13 ng/ml

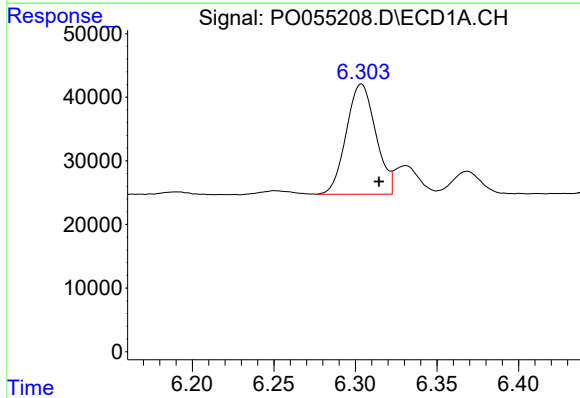


#26 AR-1254-1

R.T.: 6.304 min
Delta R.T.: -0.011 min
Response: 218067
Conc: 120.27 ng/ml

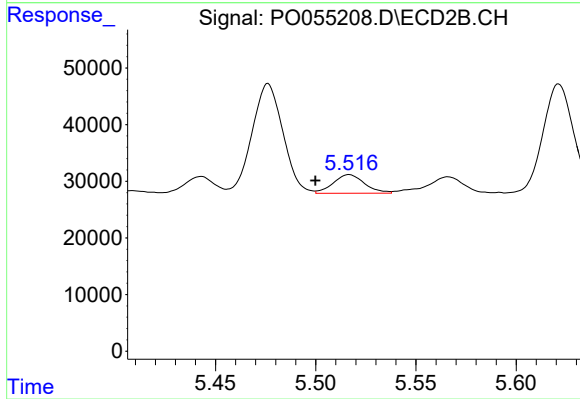

#26 AR-1254-1


R.T.: 5.517 min
Delta R.T.: 0.017 min
Response: 35979
Conc: 16.46 ng/ml

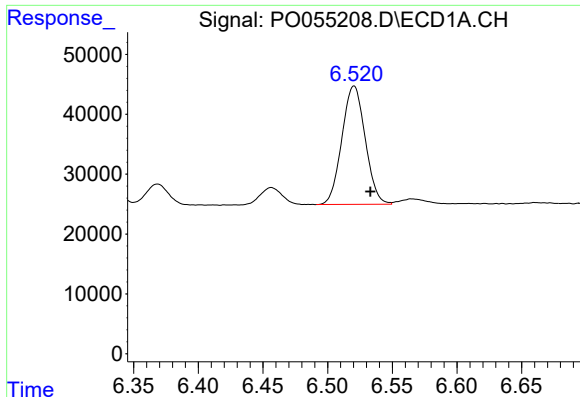

#27 AR-1254-2


R.T.: 6.520 min
Delta R.T.: -0.013 min
Response: 248173
Conc: 86.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

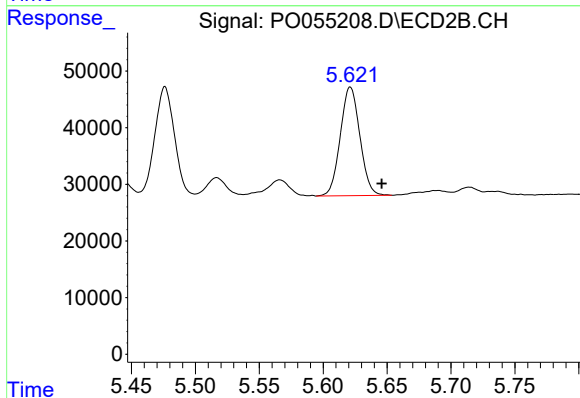


#27 AR-1254-2

R.T.: 5.621 min
Delta R.T.: -0.025 min
Response: 204665
Conc: 105.55 ng/ml

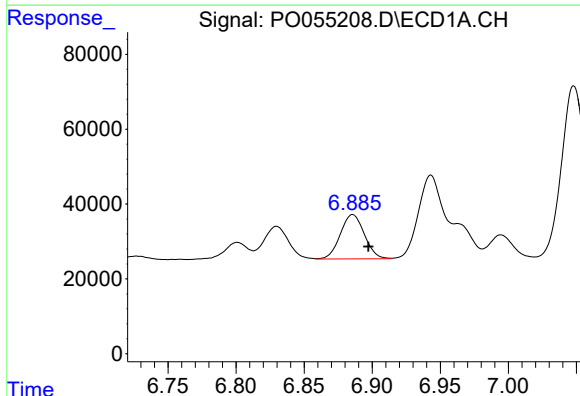


#28 AR-1254-3

R.T.: 6.886 min
Delta R.T.: -0.011 min
Response: 145675
Conc: 46.32 ng/ml

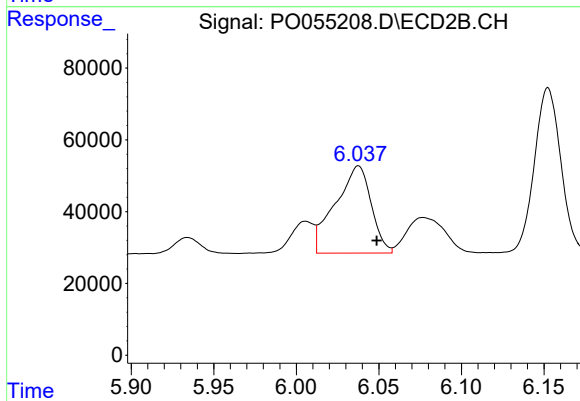

#28 AR-1254-3


R.T.: 6.038 min
Delta R.T.: -0.011 min
Response: 368372
Conc: 114.91 ng/ml

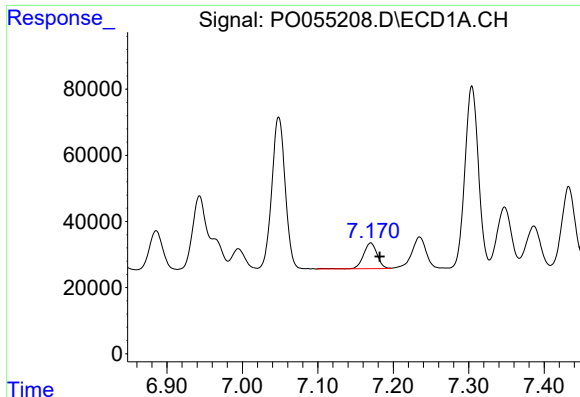

#29 AR-1254-4


R.T.: 7.170 min
Delta R.T.: -0.012 min
Response: 98016
Conc: 40.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

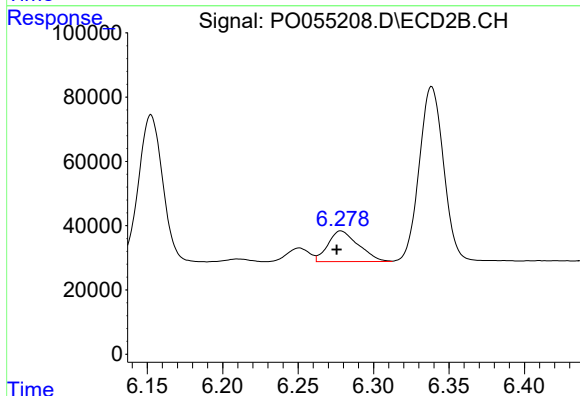


#29 AR-1254-4

R.T.: 6.278 min
Delta R.T.: 0.003 min
Response: 134186
Conc: 68.53 ng/ml

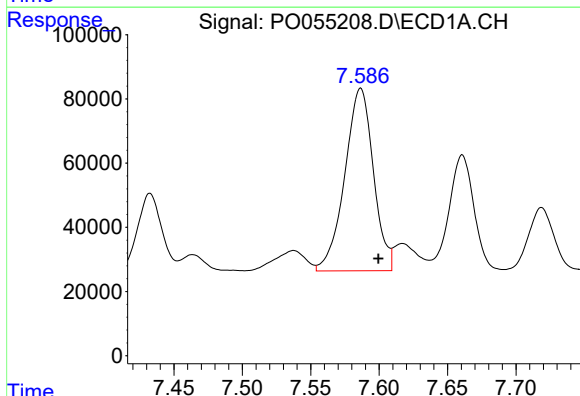


#30 AR-1254-5

R.T.: 7.587 min
Delta R.T.: -0.013 min
Response: 828367
Conc: 309.06 ng/ml

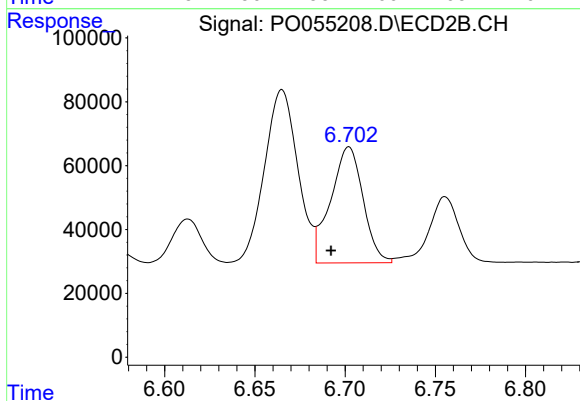

#30 AR-1254-5


R.T.: 6.702 min
Delta R.T.: 0.010 min
Response: 454296
Conc: 158.03 ng/ml

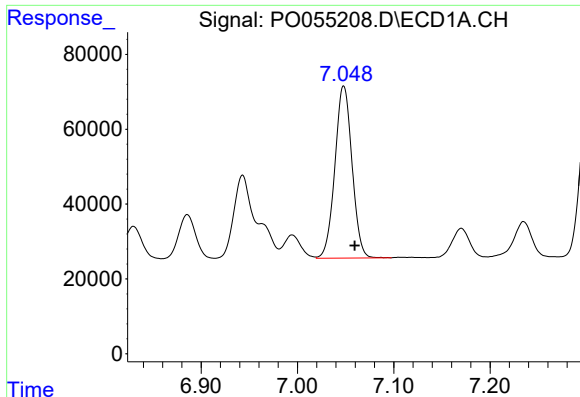

#31 AR-1260-1


R.T.: 7.048 min
Delta R.T.: -0.011 min
Response: 567931
Conc: 226.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

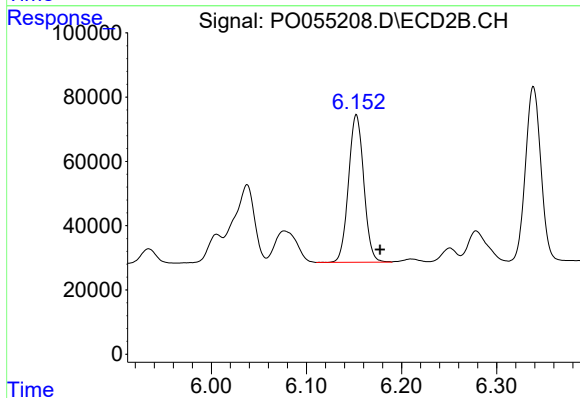


#31 AR-1260-1

R.T.: 6.152 min
Delta R.T.: -0.025 min
Response: 511329
Conc: 222.50 ng/ml

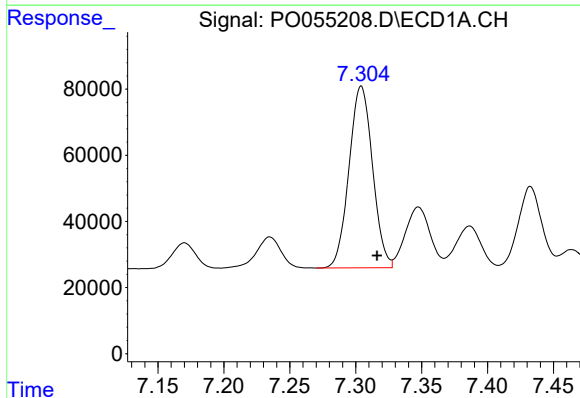


#32 AR-1260-2

R.T.: 7.304 min
Delta R.T.: -0.012 min
Response: 682784
Conc: 220.00 ng/ml

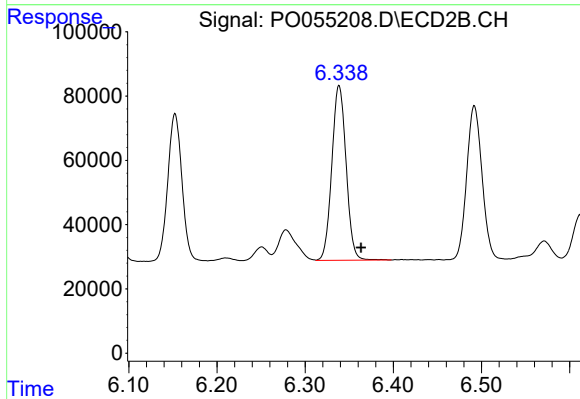

#32 AR-1260-2


R.T.: 6.339 min
Delta R.T.: -0.025 min
Response: 612426
Conc: 222.48 ng/ml

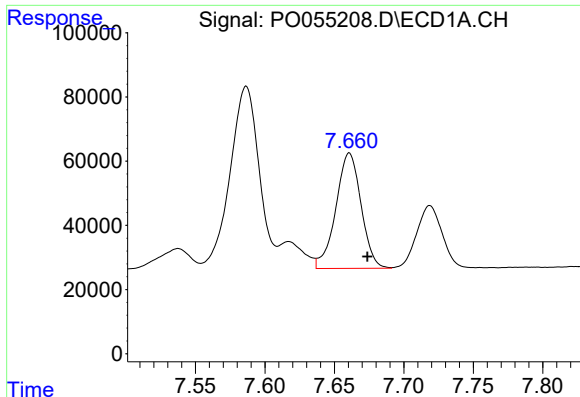

#33 AR-1260-3


R.T.: 7.661 min
Delta R.T.: -0.013 min
Response: 454561
Conc: 185.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

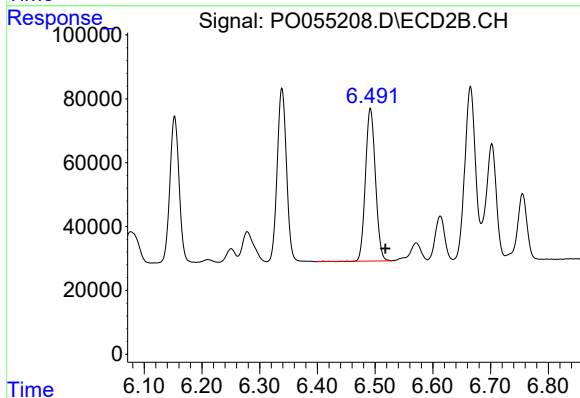


#33 AR-1260-3

R.T.: 6.492 min
Delta R.T.: -0.026 min
Response: 577274
Conc: 223.93 ng/ml

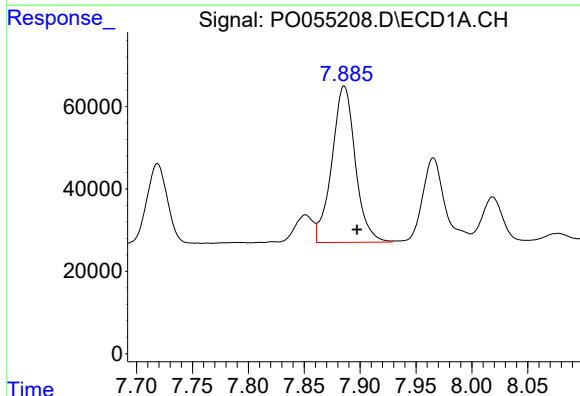


#34 AR-1260-4

R.T.: 7.886 min
Delta R.T.: -0.011 min
Response: 553679
Conc: 200.17 ng/ml

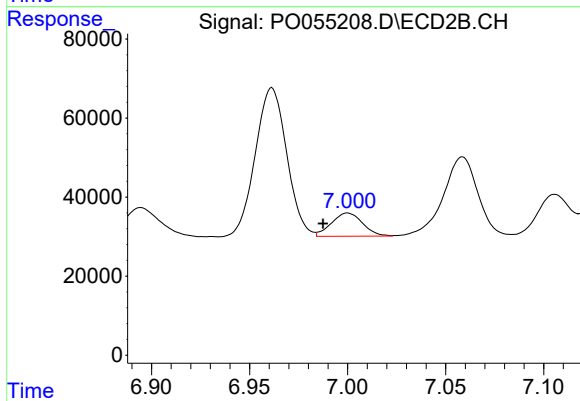

#34 AR-1260-4


R.T.: 7.000 min
Delta R.T.: 0.013 min
Response: 64927
Conc: 30.51 ng/ml

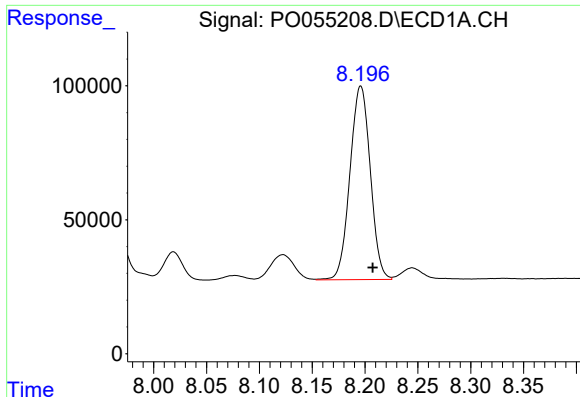

#35 AR-1260-5


R.T.: 8.196 min
Delta R.T.: -0.011 min
Response: 967666
Conc: 174.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

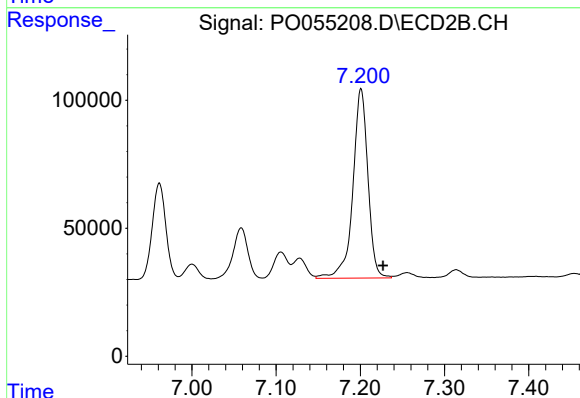


#35 AR-1260-5

R.T.: 7.201 min
Delta R.T.: -0.026 min
Response: 919210
Conc: 191.93 ng/ml

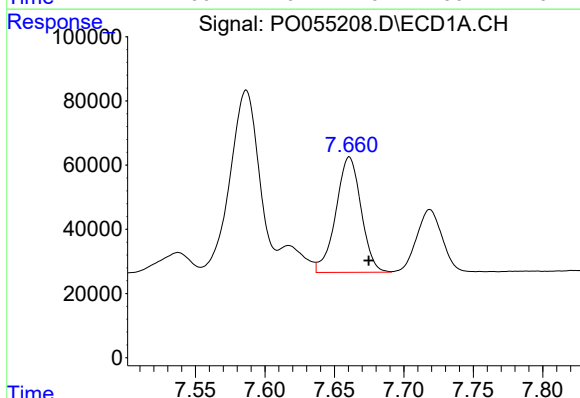


#36 AR-1262-1

R.T.: 7.661 min
Delta R.T.: -0.014 min
Response: 454561
Conc: 136.42 ng/ml

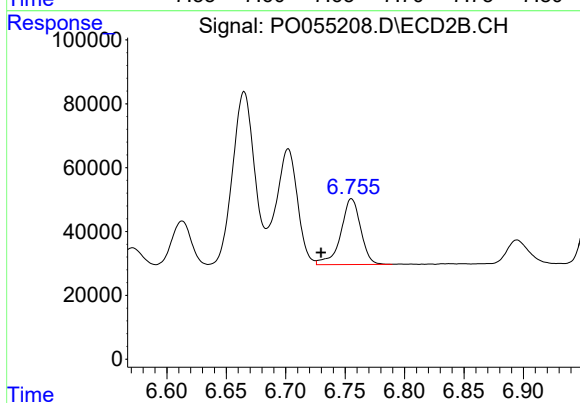

#36 AR-1262-1


R.T.: 6.755 min
Delta R.T.: 0.026 min
Response: 240553
Conc: 80.86 ng/ml

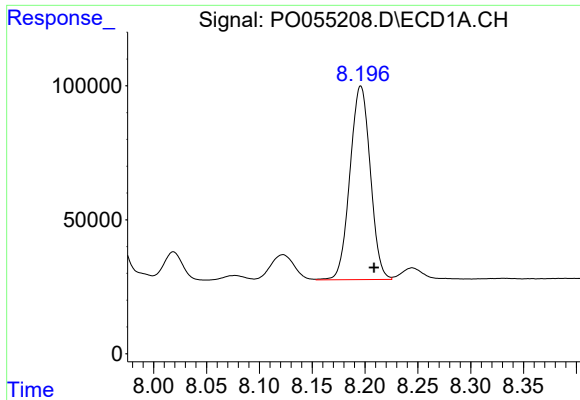

#37 AR-1262-2


R.T.: 8.196 min
Delta R.T.: -0.013 min
Response: 967666
Conc: 163.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

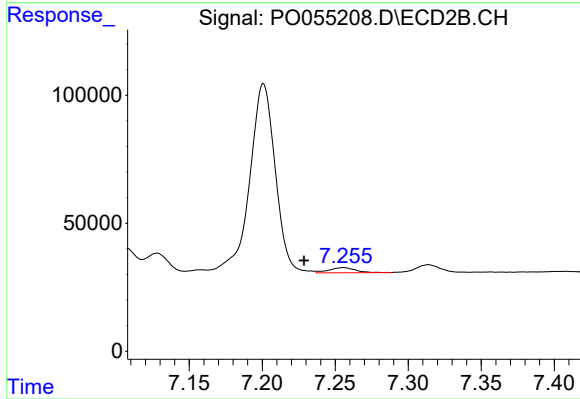


#37 AR-1262-2

R.T.: 7.256 min
Delta R.T.: 0.027 min
Response: 25092
Conc: 5.12 ng/ml

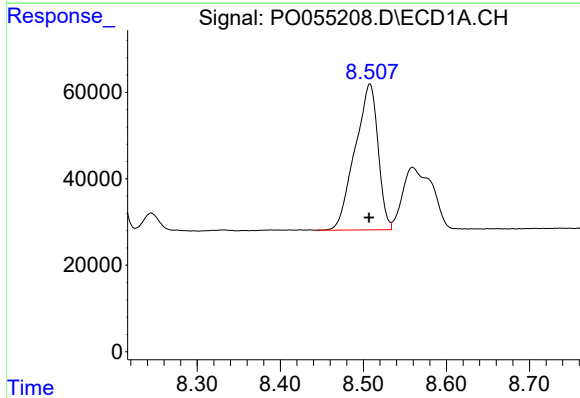


#38 AR-1262-3

R.T.: 8.508 min
Delta R.T.: 0.001 min
Response: 649977
Conc: 156.89 ng/ml

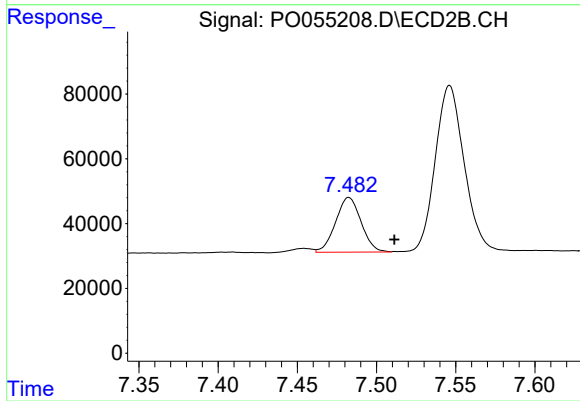

#38 AR-1262-3


R.T.: 7.483 min
Delta R.T.: -0.029 min
Response: 189168
Conc: 92.12 ng/ml

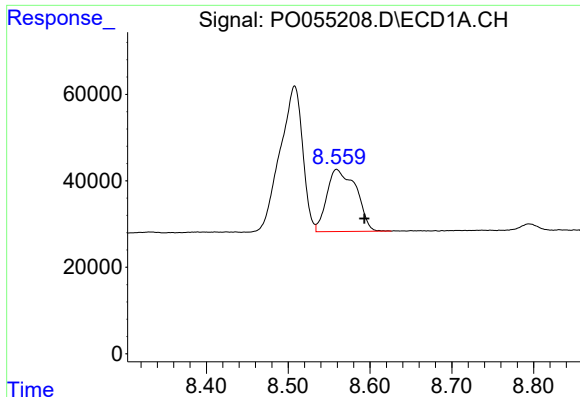

#39 AR-1262-4


R.T.: 8.559 min
Delta R.T.: -0.034 min
Response: 357378
Conc: 110.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

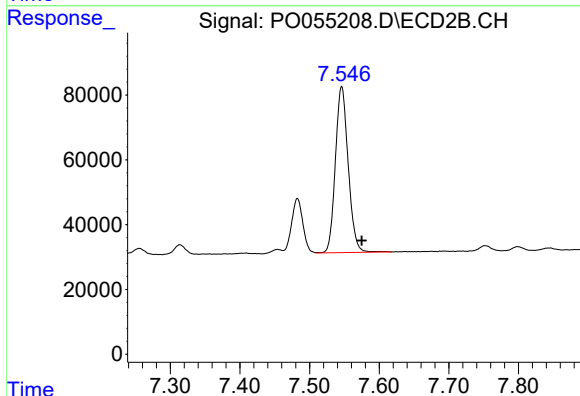


#39 AR-1262-4

R.T.: 7.546 min
Delta R.T.: -0.029 min
Response: 654256
Conc: 180.63 ng/ml

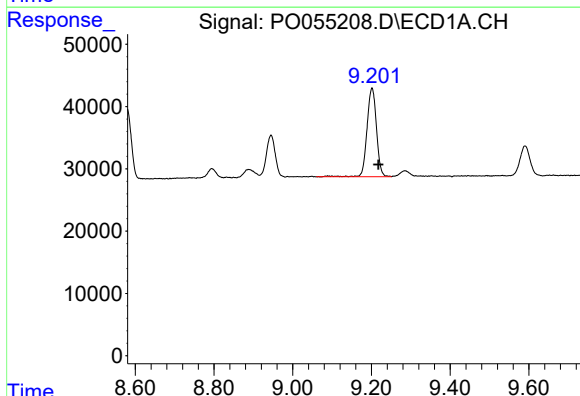


#40 AR-1262-5

R.T.: 9.202 min
Delta R.T.: -0.017 min
Response: 236866
Conc: 108.34 ng/ml

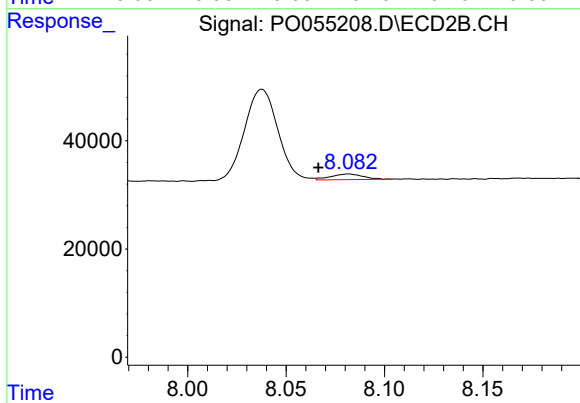

#40 AR-1262-5


R.T.: 8.082 min
Delta R.T.: 0.015 min
Response: 11874
Conc: 7.36 ng/ml

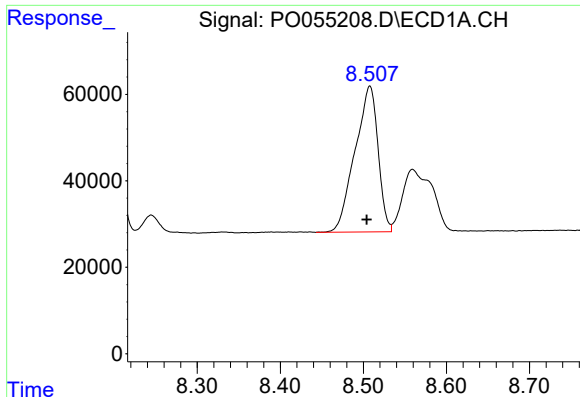

#41 AR-1268-1


R.T.: 8.508 min
Delta R.T.: 0.004 min
Response: 649977
Conc: 91.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

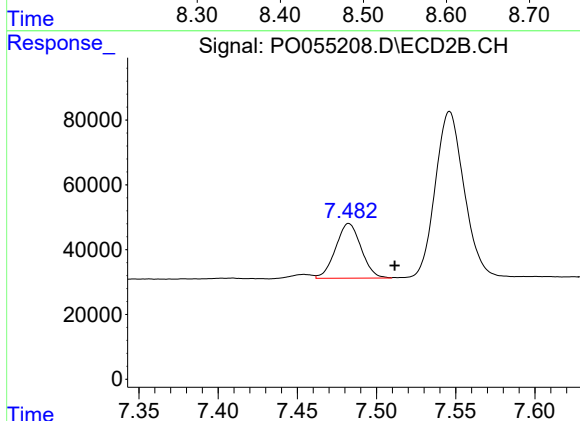


#41 AR-1268-1

R.T.: 7.483 min
Delta R.T.: -0.029 min
Response: 189168
Conc: 33.46 ng/ml

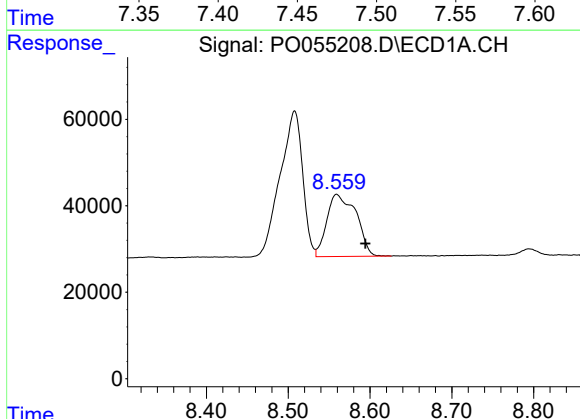


#42 AR-1268-2

R.T.: 8.559 min
Delta R.T.: -0.035 min
Response: 357378
Conc: 54.54 ng/ml

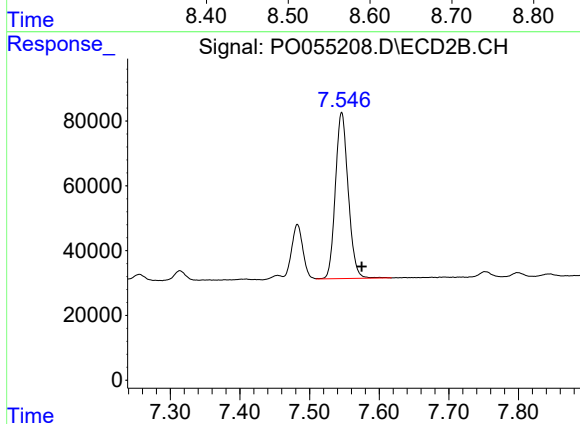

#42 AR-1268-2


R.T.: 7.546 min
Delta R.T.: -0.029 min
Response: 654256
Conc: 126.51 ng/ml

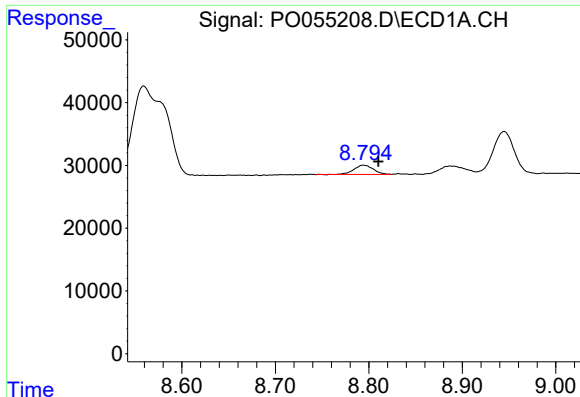

#43 AR-1268-3


R.T.: 8.794 min
Delta R.T.: -0.016 min
Response: 21041
Conc: 3.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

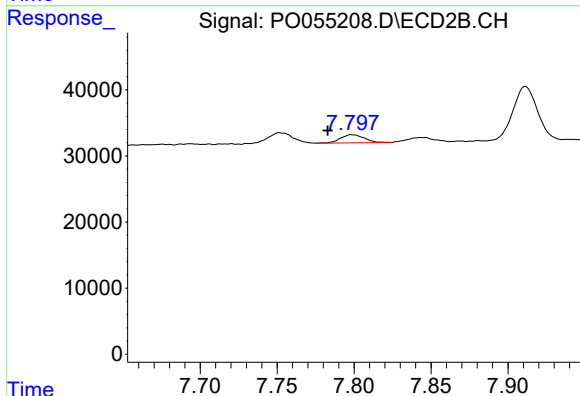


#43 AR-1268-3

R.T.: 7.799 min
Delta R.T.: 0.016 min
Response: 13091
Conc: 3.04 ng/ml

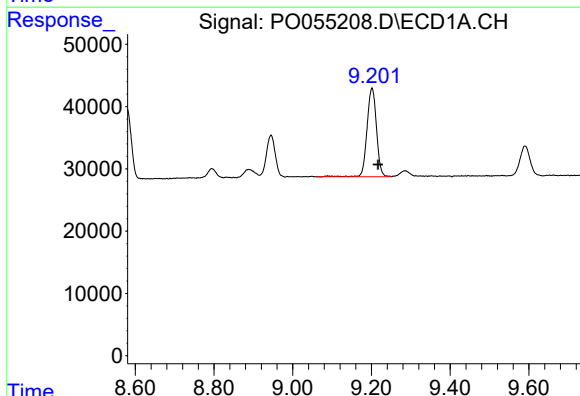


#44 AR-1268-4

R.T.: 9.202 min
Delta R.T.: -0.015 min
Response: 236866
Conc: 99.28 ng/ml

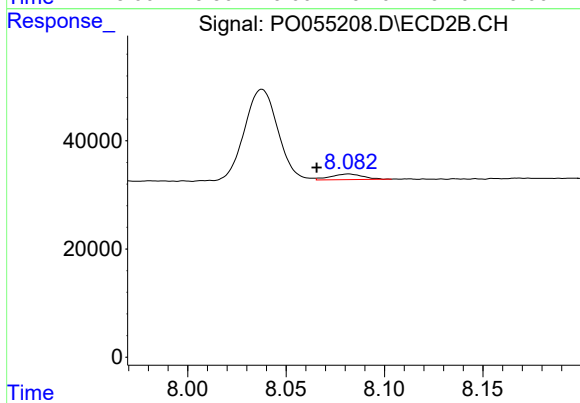

#44 AR-1268-4


R.T.: 8.082 min
Delta R.T.: 0.016 min
Response: 11874
Conc: 6.41 ng/ml

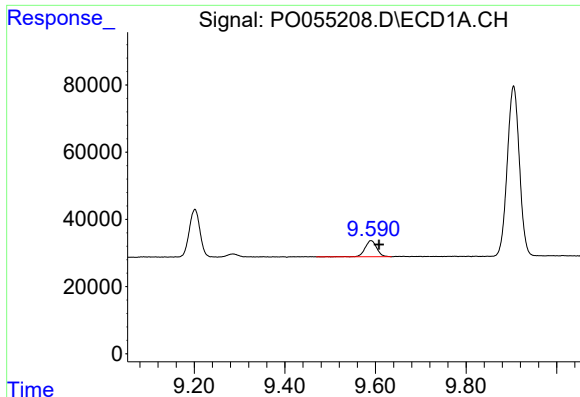

#45 AR-1268-5

R.T.: 9.590 min
Delta R.T.: -0.018 min
Response: 85656
Conc: 5.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMS

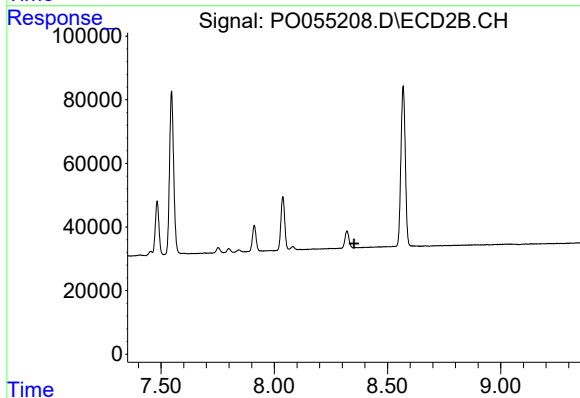

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.352 min
Response: 0
Conc: N.D.