

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0041219\
 Data File : P0055209.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Apr 2019 9:31
 Operator : SM/SJ
 Sample : K2361-01MSD
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 FK-BPM-01-E1-E1A-F1-F1AMSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 11:18:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.292	3.604	627549	574737	18.082	18.010
2)	SA Decachlor...	9.903	8.569	942653	684352	19.122	21.488
Target Compounds							
3)	L1 AR-1016-1	5.476	4.700	453285	393070	251.905	248.559
4)	L1 AR-1016-2	5.476	4.729	453285	32374	182.506	15.109 #
5)	L1 AR-1016-3	5.537	4.914	298248	167362	189.575	138.519 #
6)	L1 AR-1016-4	5.635	4.956	241475	215375	185.311	213.130
7)	L1 AR-1016-5	5.928	5.167	262481	-6358	196.724	N.D. #
8)	L2 AR-1221-1	4.497	3.815	26605	22102	60.941	56.848
9)	L2 AR-1221-2	4.587	3.902	40204	35917	118.554	119.808
10)	L2 AR-1221-3	4.663	3.977	148796	122360	143.242	132.744
11)	L3 AR-1232-1	4.663	3.977	148796	122360	172.825	163.171
12)	L3 AR-1232-2	5.188	4.729	223952	32374	457.850	37.596 #
13)	L3 AR-1232-3	5.476	4.914	453285	167362	463.812	345.387 #
14)	L3 AR-1232-4	5.635	4.987	241475	75569	471.766	171.983 #
15)	L3 AR-1232-5	5.725	5.167	233907	-6358	562.280	N.D. #
16)	L4 AR-1242-1	5.476	4.700	453285	393070	326.270	320.165
17)	L4 AR-1242-2	5.476	4.729	453285	32374	236.892	19.535 #
18)	L4 AR-1242-3	5.537	4.914	298248	167362	240.629	176.667 #
19)	L4 AR-1242-4	5.635	4.987	241475	75569	236.845	79.068 #
20)	L4 AR-1242-5	6.367	5.517	43347	34556	35.908	28.097
21)	L5 AR-1248-1	5.476	4.700	453285	393070	453.431	447.802
22)	L5 AR-1248-2	5.725	4.956	233907	215375	161.059	178.210
23)	L5 AR-1248-3	5.928	4.987	262481	75569	164.342	60.562 #
24)	L5 AR-1248-4	6.329	5.167	47242	-6358	25.148	N.D. #
25)	L5 AR-1248-5	6.367	5.517	43347	34556	24.178	23.178
26)	L6 AR-1254-1	6.302	5.517	216838	34556	119.590	15.812 #
27)	L6 AR-1254-2	6.519	5.622	248512	201614	87.052	103.981
28)	L6 AR-1254-3	6.884	6.038	144505	370478	45.952	115.569 #
29)	L6 AR-1254-4	7.168	6.279	95291	133525	38.952	68.197 #
30)	L6 AR-1254-5	7.585	6.702	829295	459065	309.403	159.691 #
31)	L7 AR-1260-1	7.047	6.152	567506	510162	225.860	221.996
32)	L7 AR-1260-2	7.303	6.339	682723	614310	219.983	223.162
33)	L7 AR-1260-3	7.659	6.492	454952	578966	185.365	224.588
34)	L7 AR-1260-4	7.884	7.000	556431	66126	201.167	31.072 #
35)	L7 AR-1260-5	8.194	7.201	972526	935724	175.274	195.378
36)	L8 AR-1262-1	7.659	6.756	454952	242469	136.538	81.504 #
37)	L8 AR-1262-2	8.194	7.256	972526	25528	164.156	5.209 #
38)	L8 AR-1262-3	8.506	7.483	656347	192336	158.431	93.665 #
39)	L8 AR-1262-4	8.558	7.546	360756	664115	111.967	183.350 #
40)	L8 AR-1262-5	9.199	8.081	236903	12925	108.359	8.009 #
41)	L9 AR-1268-1	8.506	7.483	656347	192336	92.216	34.017 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041219\
 Data File : P0055209.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Apr 2019 9:31
 Operator : SM/SJ
 Sample : K2361-01MSD
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-01-E1-E1A-F1-F1AMSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 11:18:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.558	7.546	360756	664115	55.060	128.416 #
43) L9	AR-1268-3	8.793	7.799	22634	13532	4.155	3.144
44) L9	AR-1268-4	9.199	8.081	236903	12925	99.298	6.972 #
45) L9	AR-1268-5	9.588	0.000	86622	0	5.258	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041219\
Data File : P0055209.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Apr 2019 9:31
Operator : SM/SJ
Sample : K2361-01MSD
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 11:18:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

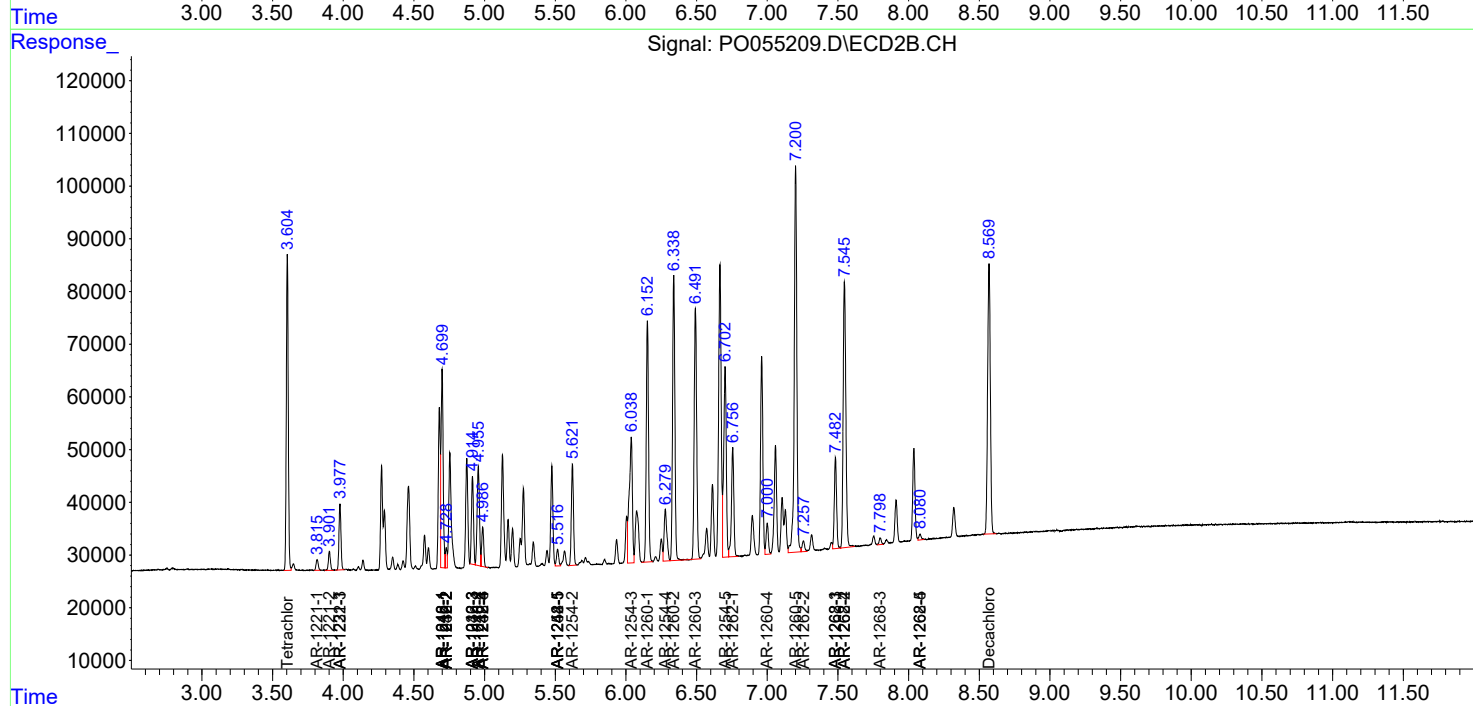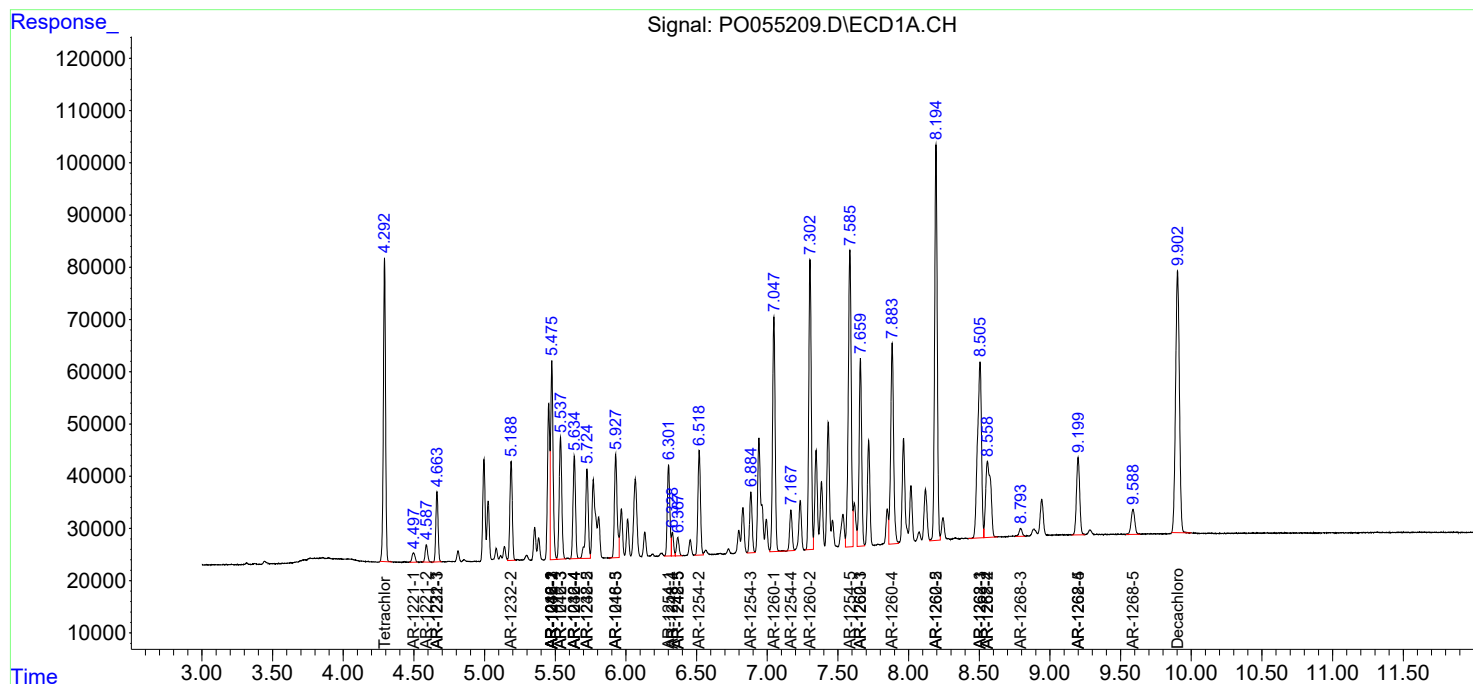


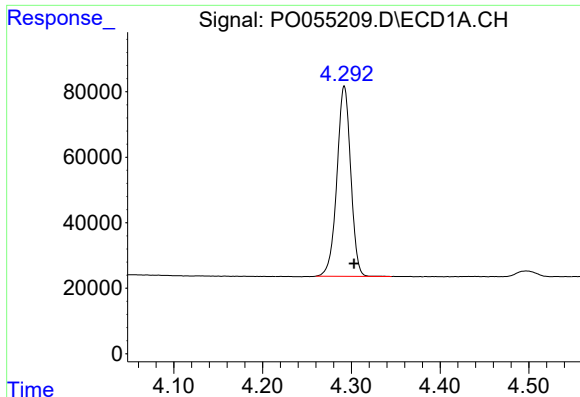

#1 Tetrachloro-m-xylene


R.T.: 4.292 min
Delta R.T.: -0.011 min
Response: 627549
Conc: 18.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

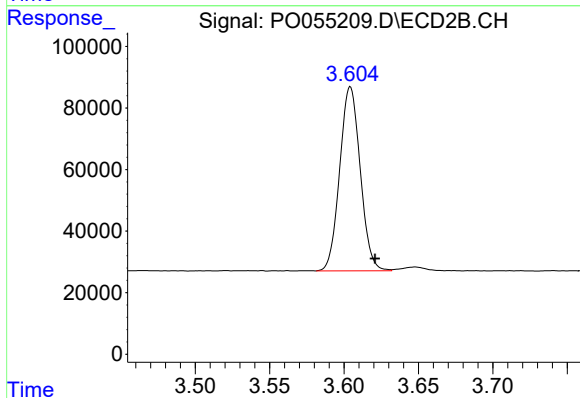


#1 Tetrachloro-m-xylene

R.T.: 3.604 min
Delta R.T.: -0.017 min
Response: 574737
Conc: 18.01 ng/ml

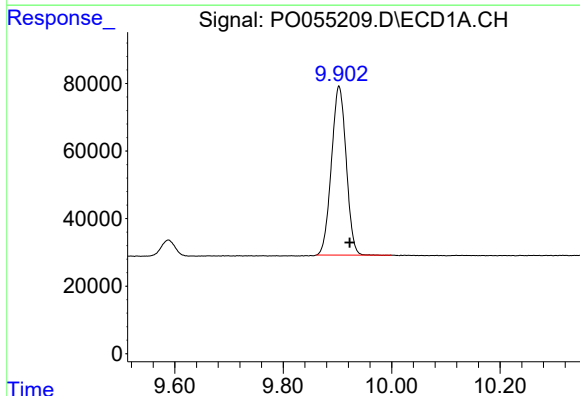


#2 Decachlorobiphenyl

R.T.: 9.903 min
Delta R.T.: -0.020 min
Response: 942653
Conc: 19.12 ng/ml

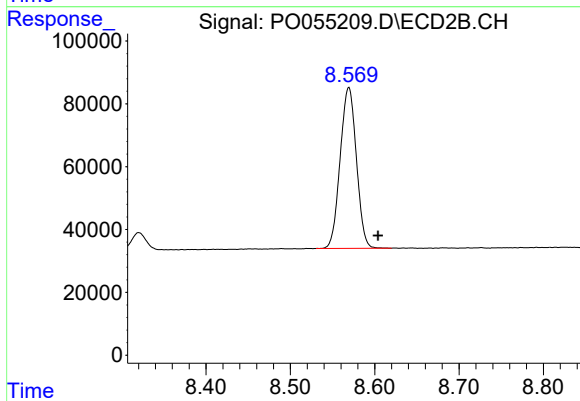

#2 Decachlorobiphenyl


R.T.: 8.569 min
Delta R.T.: -0.035 min
Response: 684352
Conc: 21.49 ng/ml

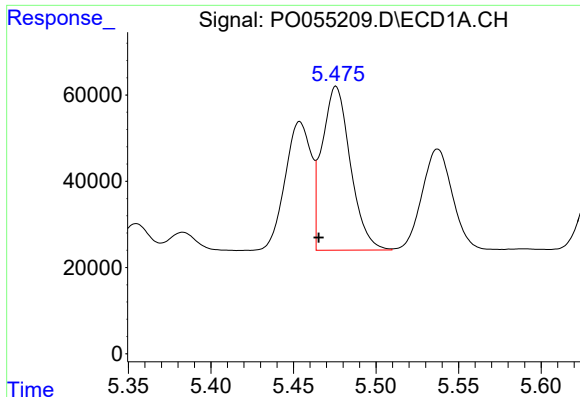

#3 AR-1016-1


R.T.: 5.476 min
Delta R.T.: 0.010 min
Response: 453285
Conc: 251.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

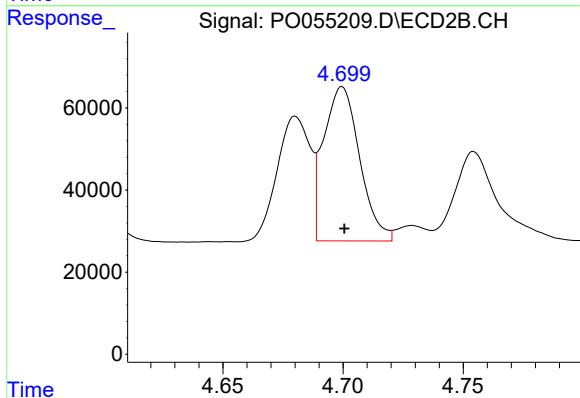


#3 AR-1016-1

R.T.: 4.700 min
Delta R.T.: 0.000 min
Response: 393070
Conc: 248.56 ng/ml

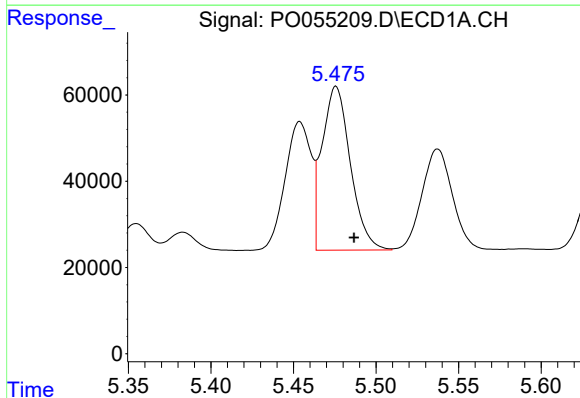


#4 AR-1016-2

R.T.: 5.476 min
Delta R.T.: -0.011 min
Response: 453285
Conc: 182.51 ng/ml

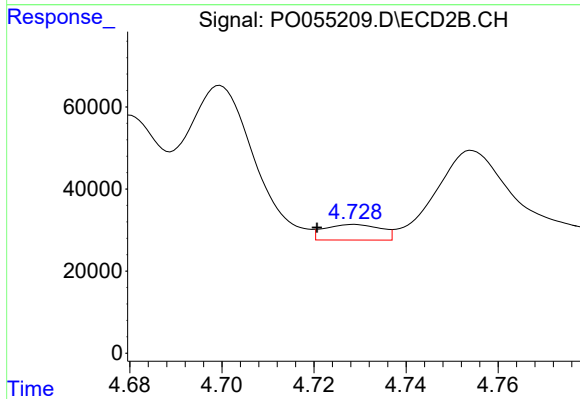

#4 AR-1016-2


R.T.: 4.729 min
Delta R.T.: 0.008 min
Response: 32374
Conc: 15.11 ng/ml

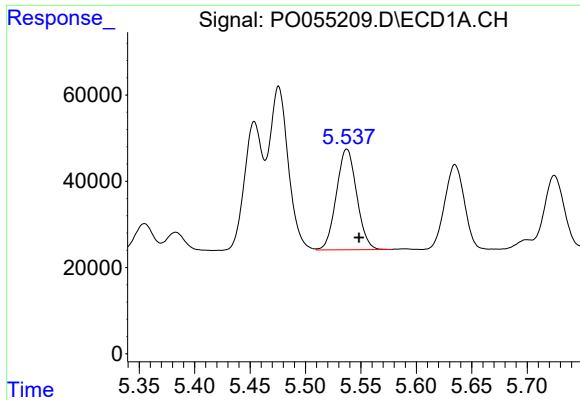

#5 AR-1016-3


R.T.: 5.537 min
Delta R.T.: -0.011 min
Response: 298248
Conc: 189.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

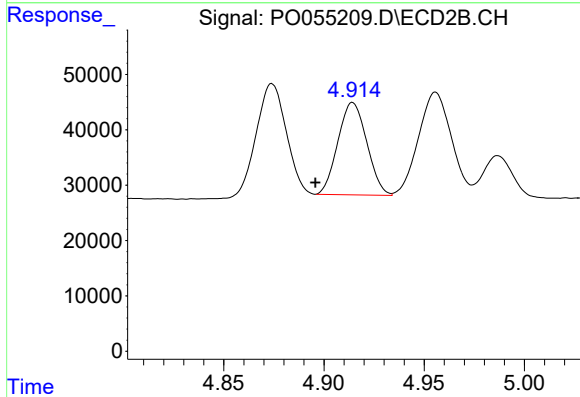


#5 AR-1016-3

R.T.: 4.914 min
Delta R.T.: 0.019 min
Response: 167362
Conc: 138.52 ng/ml

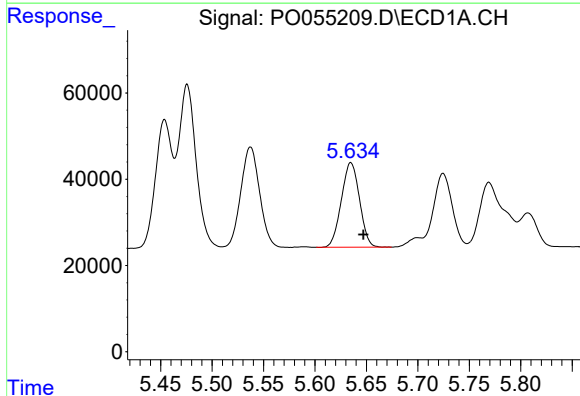


#6 AR-1016-4

R.T.: 5.635 min
Delta R.T.: -0.012 min
Response: 241475
Conc: 185.31 ng/ml

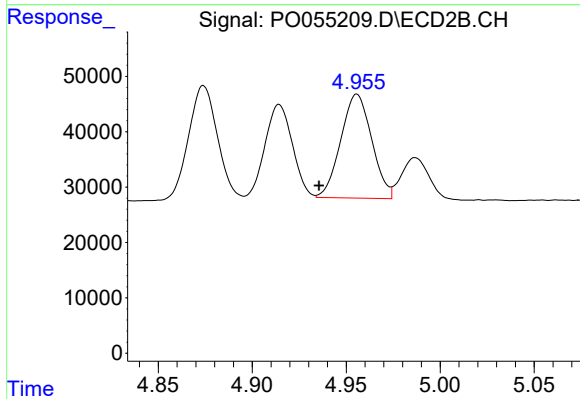

#6 AR-1016-4


R.T.: 4.956 min
Delta R.T.: 0.020 min
Response: 215375
Conc: 213.13 ng/ml

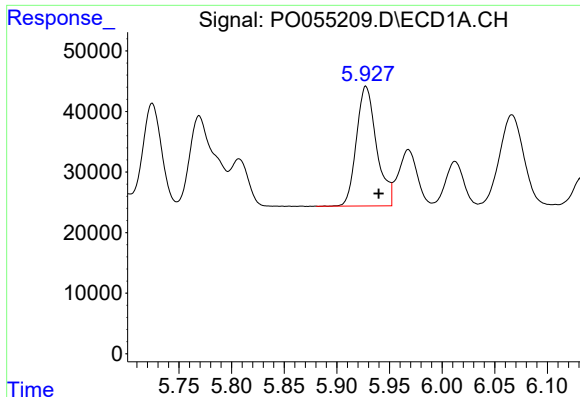

#7 AR-1016-5


R.T.: 5.928 min
Delta R.T.: -0.012 min
Response: 262481
Conc: 196.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

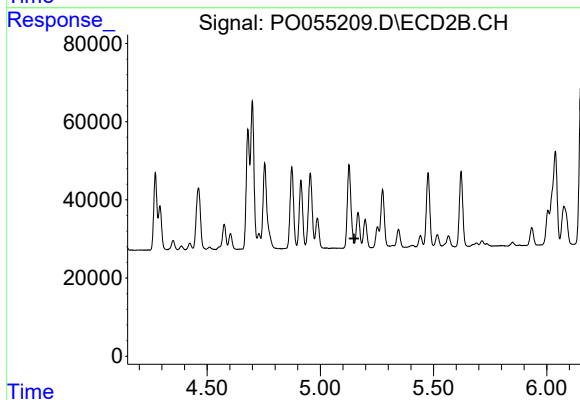


#7 AR-1016-5

R.T.: 5.167 min
Delta R.T.: 0.018 min
Response: -6358
Conc: N.D.

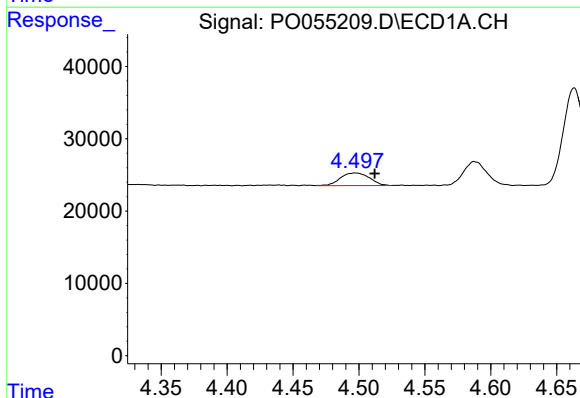


#8 AR-1221-1

R.T.: 4.497 min
Delta R.T.: -0.015 min
Response: 26605
Conc: 60.94 ng/ml

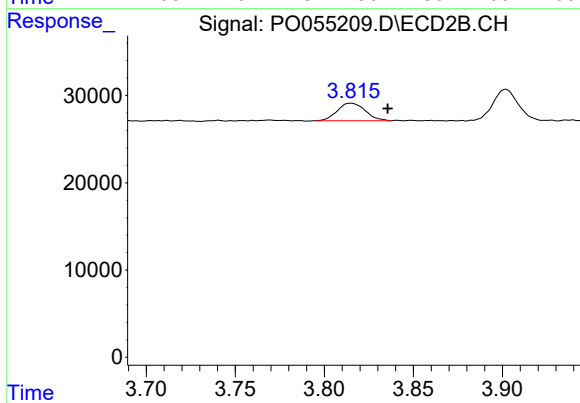

#8 AR-1221-1


R.T.: 3.815 min
Delta R.T.: -0.020 min
Response: 22102
Conc: 56.85 ng/ml

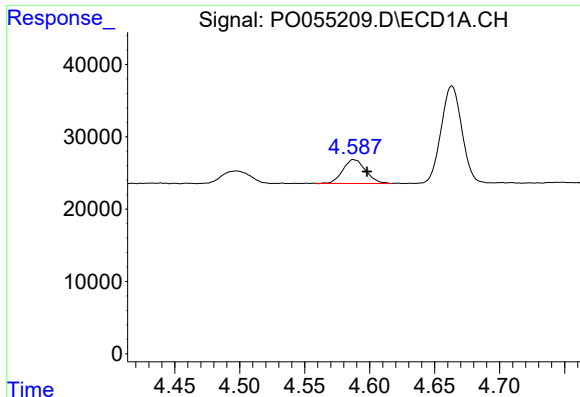

#9 AR-1221-2


R.T.: 4.587 min
Delta R.T.: -0.011 min
Response: 40204
Conc: 118.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

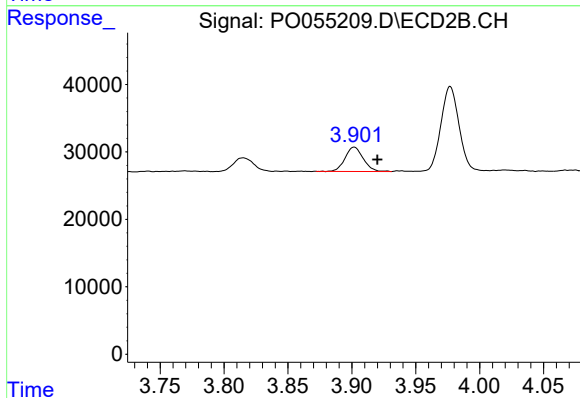


#9 AR-1221-2

R.T.: 3.902 min
Delta R.T.: -0.018 min
Response: 35917
Conc: 119.81 ng/ml

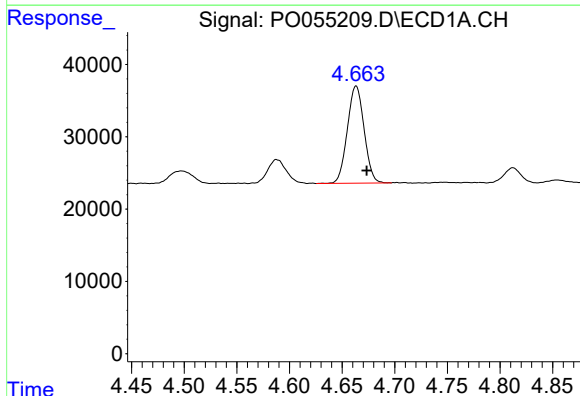


#10 AR-1221-3

R.T.: 4.663 min
Delta R.T.: -0.010 min
Response: 148796
Conc: 143.24 ng/ml

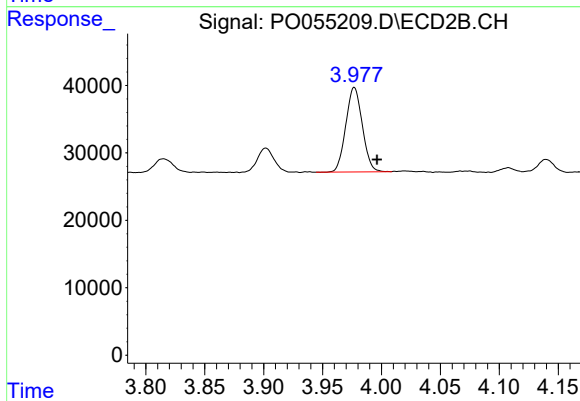

#10 AR-1221-3


R.T.: 3.977 min
Delta R.T.: -0.019 min
Response: 122360
Conc: 132.74 ng/ml

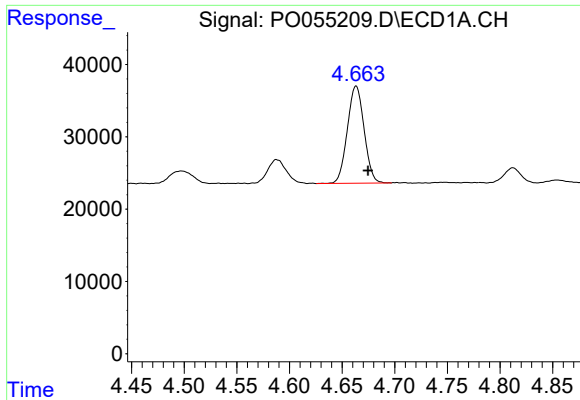

#11 AR-1232-1


R.T.: 4.663 min
Delta R.T.: -0.011 min
Response: 148796
Conc: 172.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

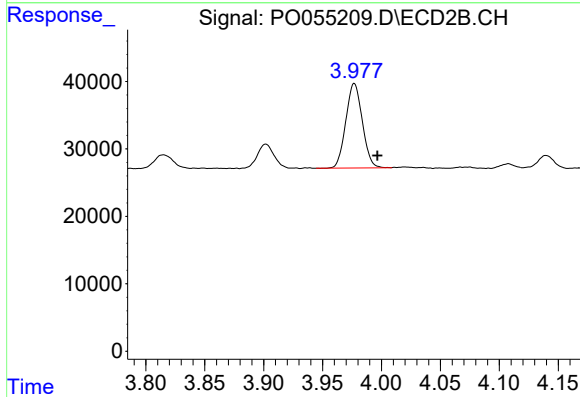


#11 AR-1232-1

R.T.: 3.977 min
Delta R.T.: -0.020 min
Response: 122360
Conc: 163.17 ng/ml

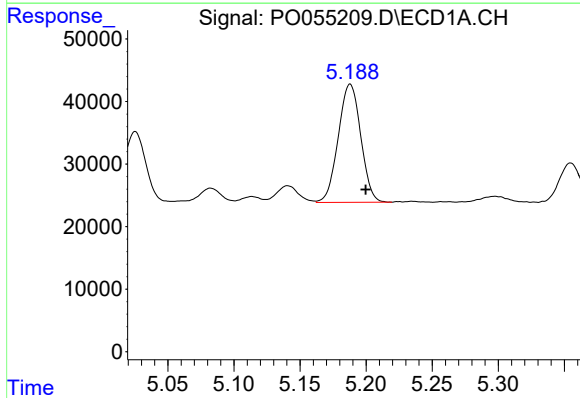


#12 AR-1232-2

R.T.: 5.188 min
Delta R.T.: -0.012 min
Response: 223952
Conc: 457.85 ng/ml

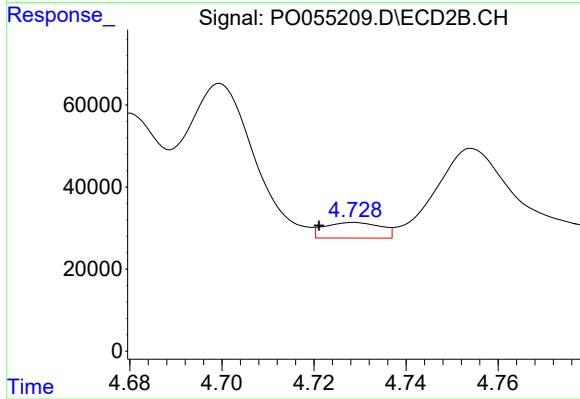

#12 AR-1232-2


R.T.: 4.729 min
Delta R.T.: 0.008 min
Response: 32374
Conc: 37.60 ng/ml

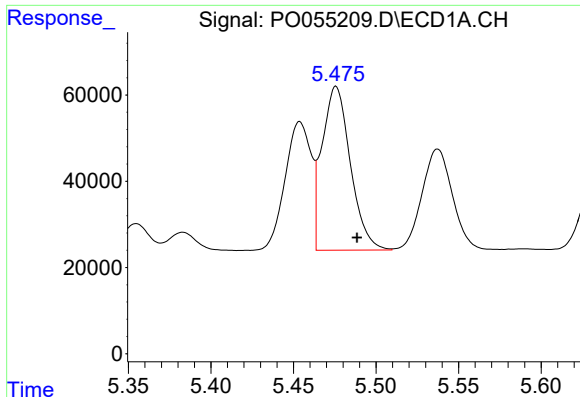

#13 AR-1232-3


R.T.: 5.476 min
Delta R.T.: -0.013 min
Response: 453285
Conc: 463.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

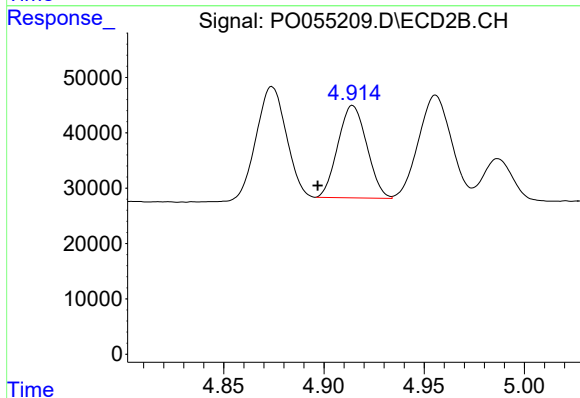


#13 AR-1232-3

R.T.: 4.914 min
Delta R.T.: 0.017 min
Response: 167362
Conc: 345.39 ng/ml

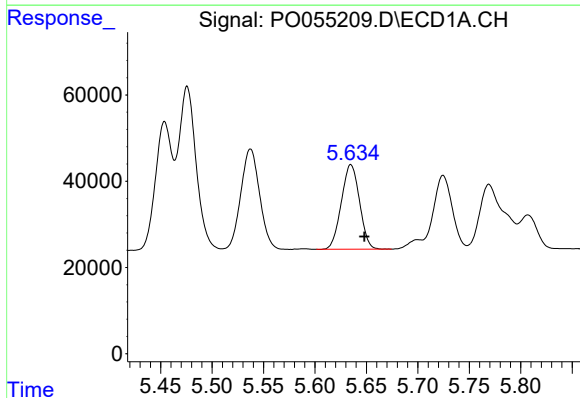


#14 AR-1232-4

R.T.: 5.635 min
Delta R.T.: -0.013 min
Response: 241475
Conc: 471.77 ng/ml

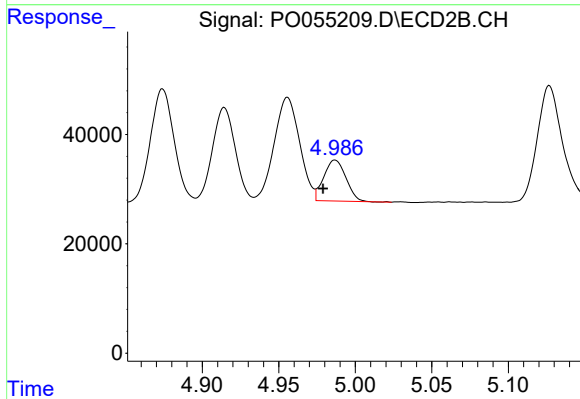

#14 AR-1232-4


R.T.: 4.987 min
Delta R.T.: 0.008 min
Response: 75569
Conc: 171.98 ng/ml

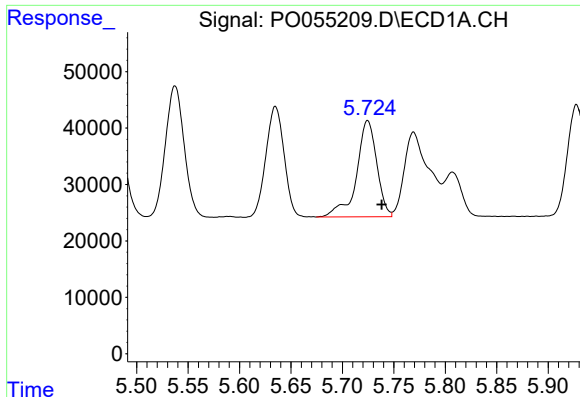

#15 AR-1232-5


R.T.: 5.725 min
Delta R.T.: -0.014 min
Response: 233907
Conc: 562.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

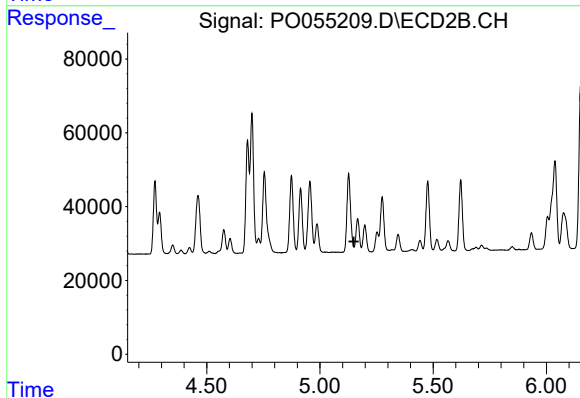


#15 AR-1232-5

R.T.: 5.167 min
Delta R.T.: 0.016 min
Response: -6358
Conc: N.D.

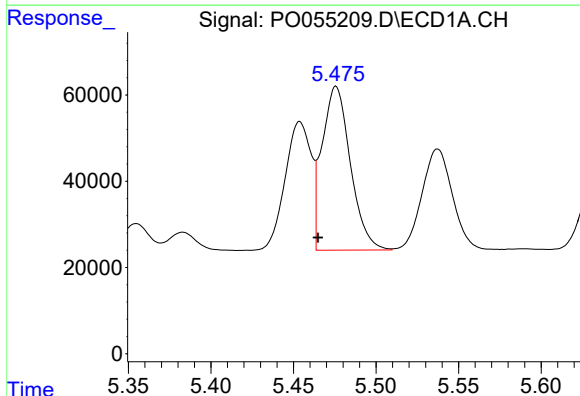


#16 AR-1242-1

R.T.: 5.476 min
Delta R.T.: 0.011 min
Response: 453285
Conc: 326.27 ng/ml

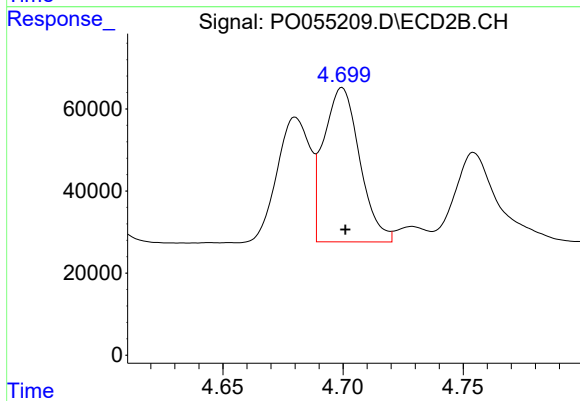

#16 AR-1242-1


R.T.: 4.700 min
Delta R.T.: -0.001 min
Response: 393070
Conc: 320.16 ng/ml

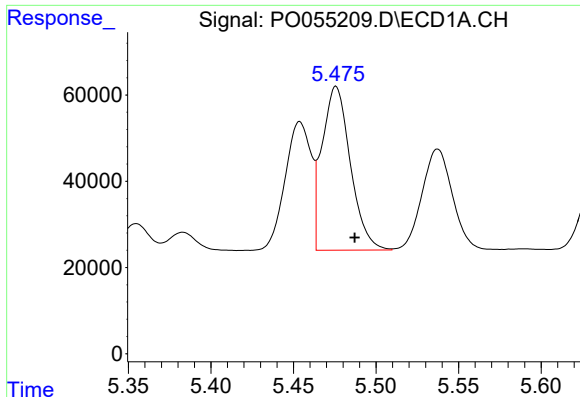

#17 AR-1242-2


R.T.: 5.476 min
Delta R.T.: -0.011 min
Response: 453285
Conc: 236.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

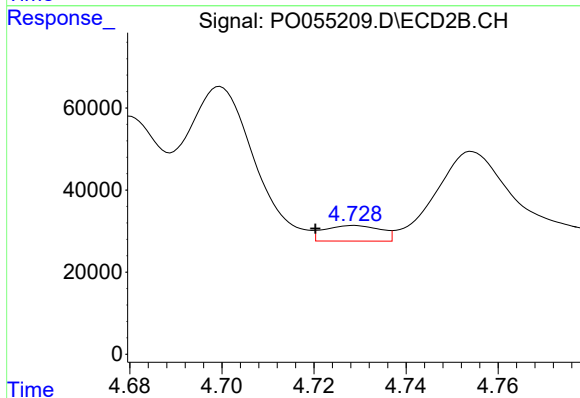


#17 AR-1242-2

R.T.: 4.729 min
Delta R.T.: 0.008 min
Response: 32374
Conc: 19.53 ng/ml

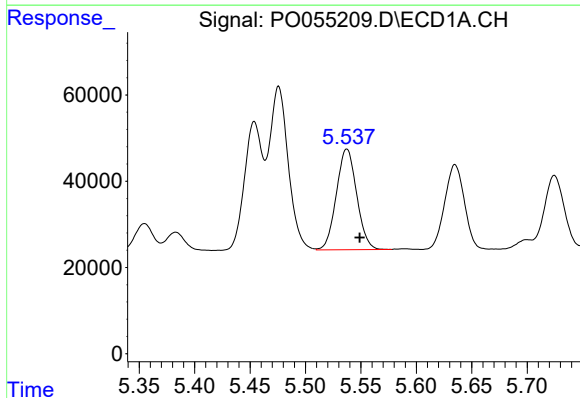


#18 AR-1242-3

R.T.: 5.537 min
Delta R.T.: -0.012 min
Response: 298248
Conc: 240.63 ng/ml

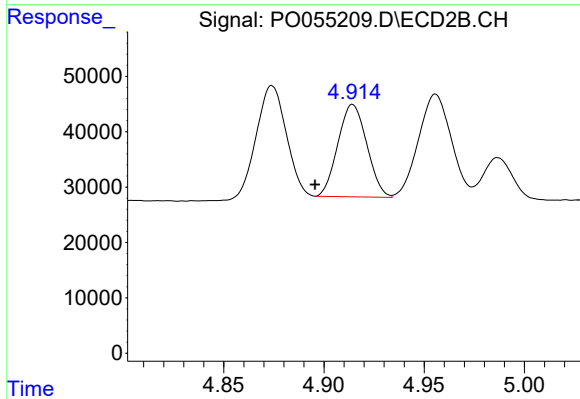

#18 AR-1242-3


R.T.: 4.914 min
Delta R.T.: 0.019 min
Response: 167362
Conc: 176.67 ng/ml

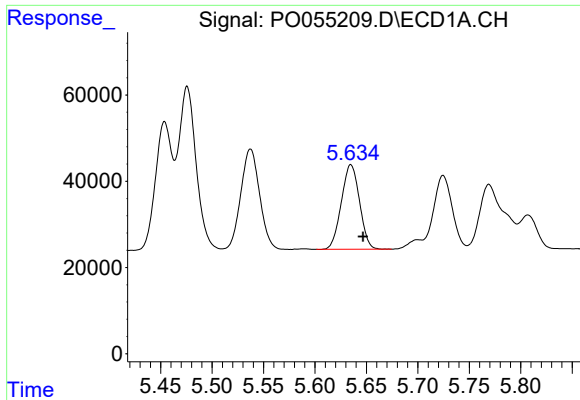

#19 AR-1242-4


R.T.: 5.635 min
Delta R.T.: -0.012 min
Response: 241475
Conc: 236.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

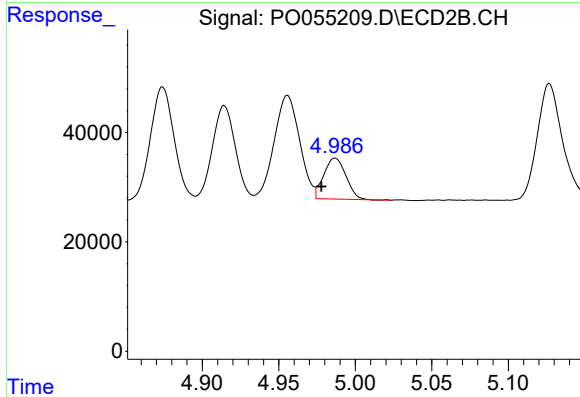


#19 AR-1242-4

R.T.: 4.987 min
Delta R.T.: 0.009 min
Response: 75569
Conc: 79.07 ng/ml

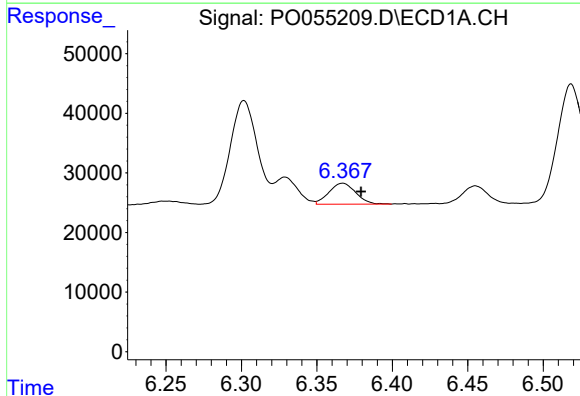


#20 AR-1242-5

R.T.: 6.367 min
Delta R.T.: -0.012 min
Response: 43347
Conc: 35.91 ng/ml

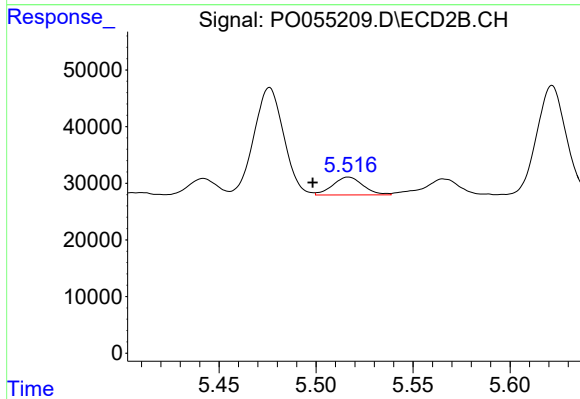

#20 AR-1242-5


R.T.: 5.517 min
Delta R.T.: 0.018 min
Response: 34556
Conc: 28.10 ng/ml

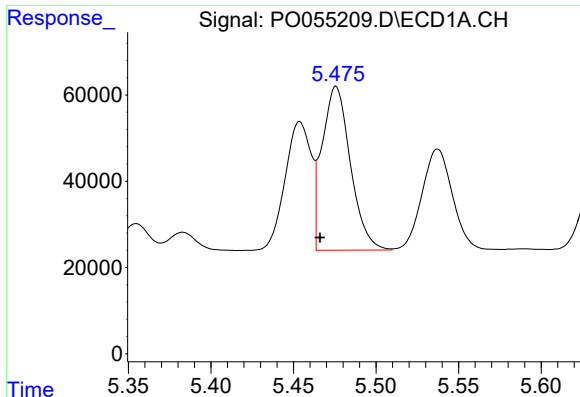

#21 AR-1248-1


R.T.: 5.476 min
Delta R.T.: 0.010 min
Response: 453285
Conc: 453.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

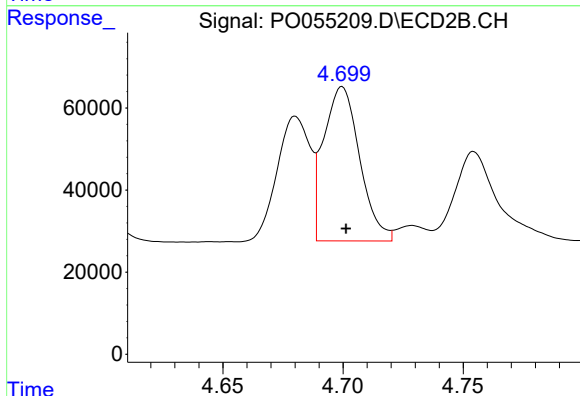


#21 AR-1248-1

R.T.: 4.700 min
Delta R.T.: -0.002 min
Response: 393070
Conc: 447.80 ng/ml

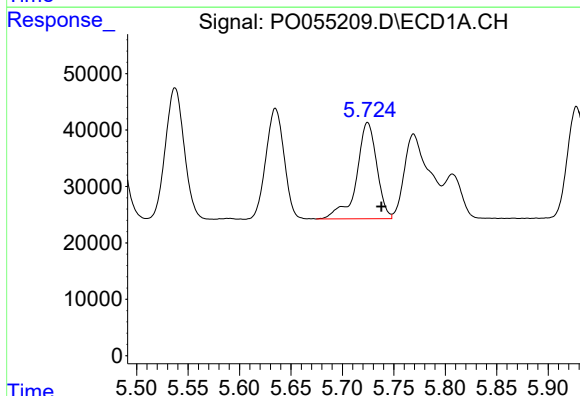


#22 AR-1248-2

R.T.: 5.725 min
Delta R.T.: -0.013 min
Response: 233907
Conc: 161.06 ng/ml

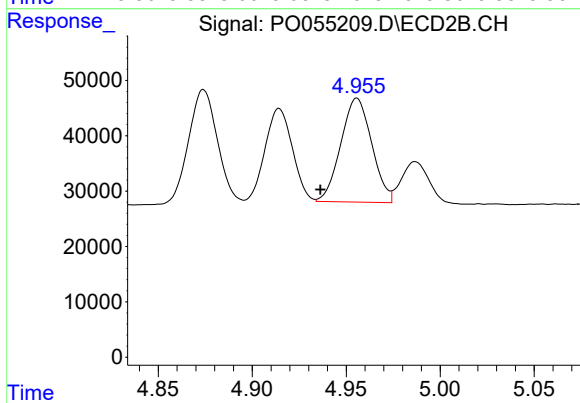

#22 AR-1248-2


R.T.: 4.956 min
Delta R.T.: 0.019 min
Response: 215375
Conc: 178.21 ng/ml

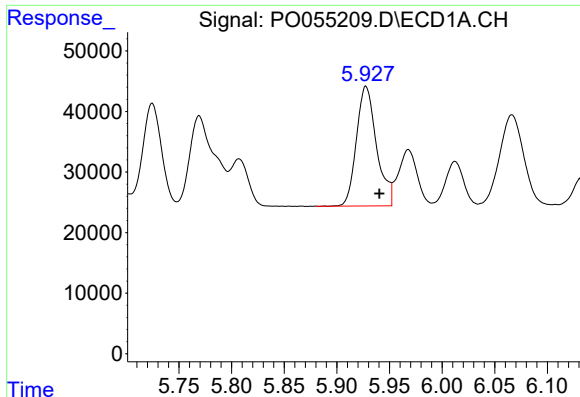

#23 AR-1248-3


R.T.: 5.928 min
Delta R.T.: -0.013 min
Response: 262481
Conc: 164.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

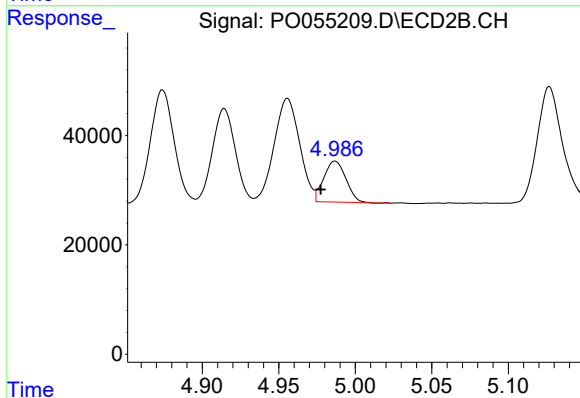


#23 AR-1248-3

R.T.: 4.987 min
Delta R.T.: 0.009 min
Response: 75569
Conc: 60.56 ng/ml

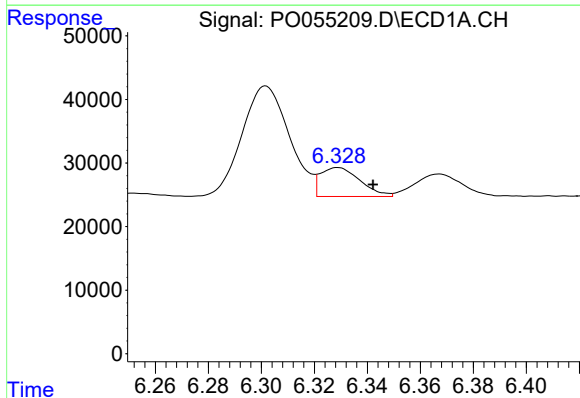


#24 AR-1248-4

R.T.: 6.329 min
Delta R.T.: -0.013 min
Response: 47242
Conc: 25.15 ng/ml

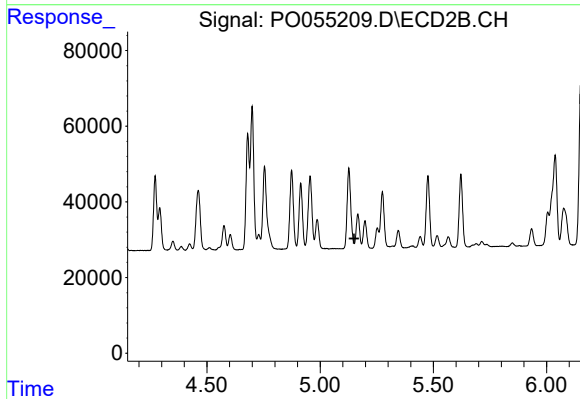

#24 AR-1248-4


R.T.: 5.167 min
Delta R.T.: 0.017 min
Response: -6358
Conc: N.D.

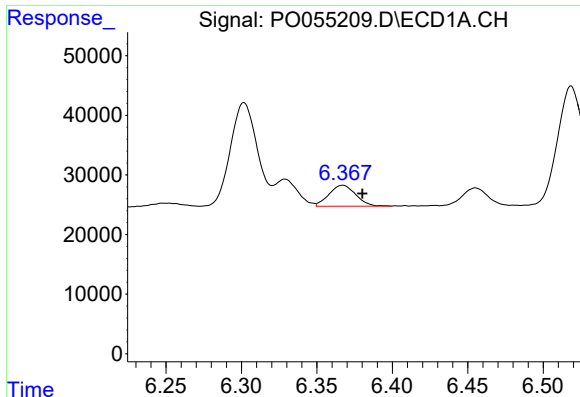

#25 AR-1248-5


R.T.: 6.367 min
Delta R.T.: -0.013 min
Response: 43347
Conc: 24.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

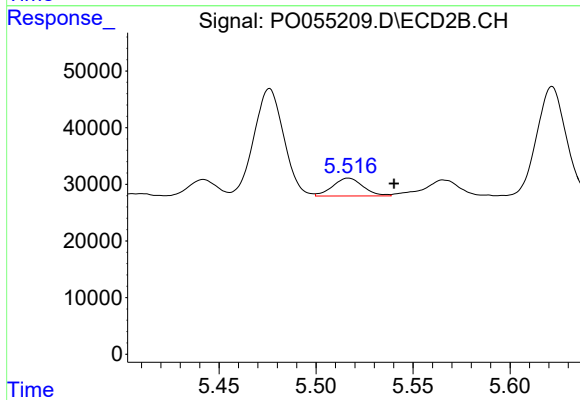


#25 AR-1248-5

R.T.: 5.517 min
Delta R.T.: -0.024 min
Response: 34556
Conc: 23.18 ng/ml

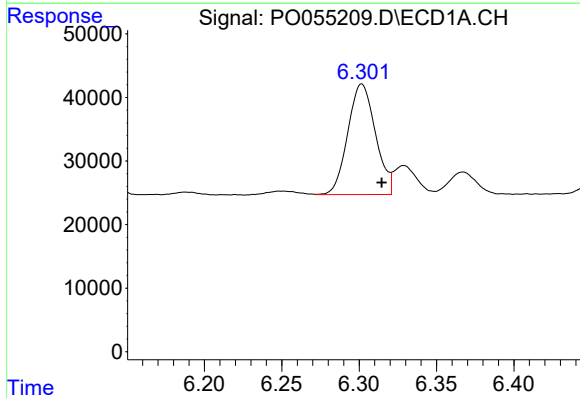


#26 AR-1254-1

R.T.: 6.302 min
Delta R.T.: -0.013 min
Response: 216838
Conc: 119.59 ng/ml

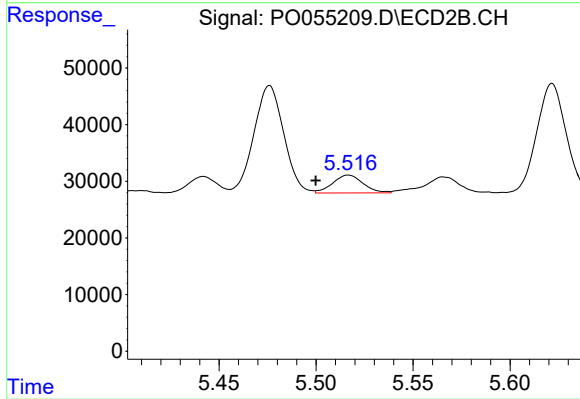

#26 AR-1254-1


R.T.: 5.517 min
Delta R.T.: 0.017 min
Response: 34556
Conc: 15.81 ng/ml

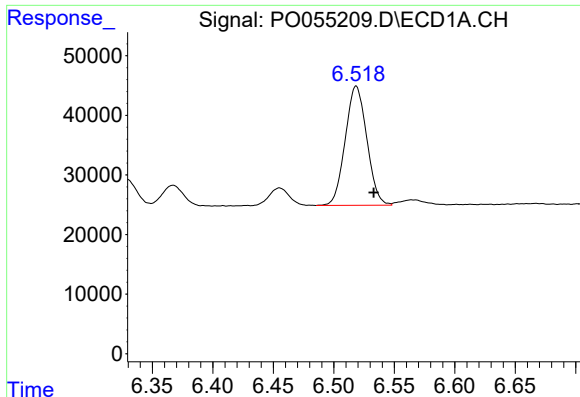

#27 AR-1254-2


R.T.: 6.519 min
Delta R.T.: -0.014 min
Response: 248512
Conc: 87.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

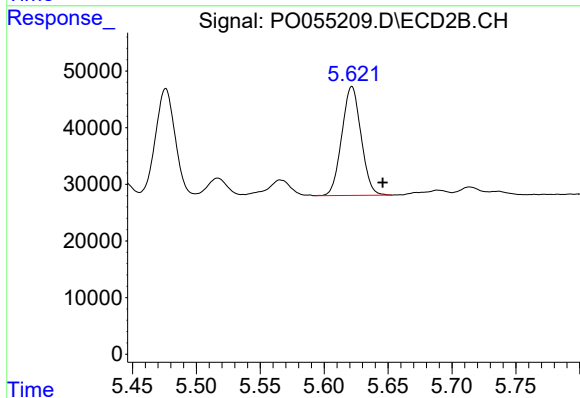


#27 AR-1254-2

R.T.: 5.622 min
Delta R.T.: -0.024 min
Response: 201614
Conc: 103.98 ng/ml

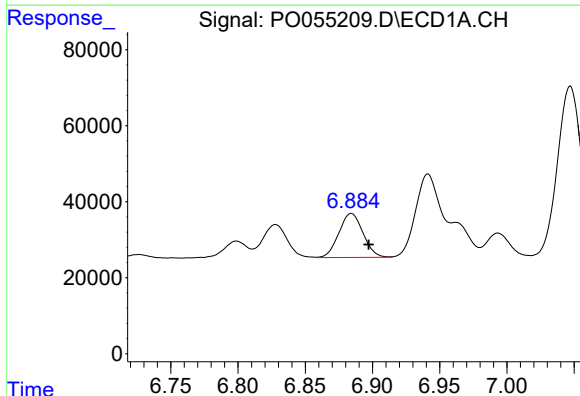


#28 AR-1254-3

R.T.: 6.884 min
Delta R.T.: -0.013 min
Response: 144505
Conc: 45.95 ng/ml

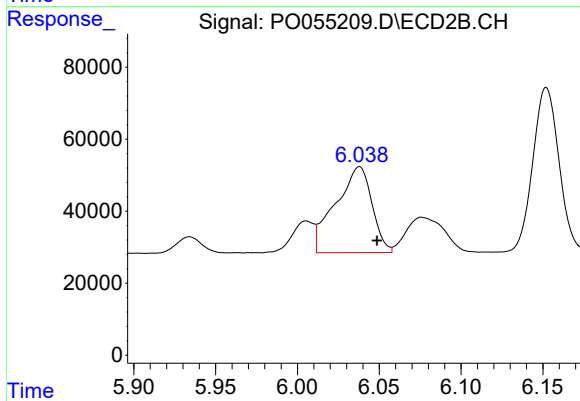

#28 AR-1254-3


R.T.: 6.038 min
Delta R.T.: -0.011 min
Response: 370478
Conc: 115.57 ng/ml

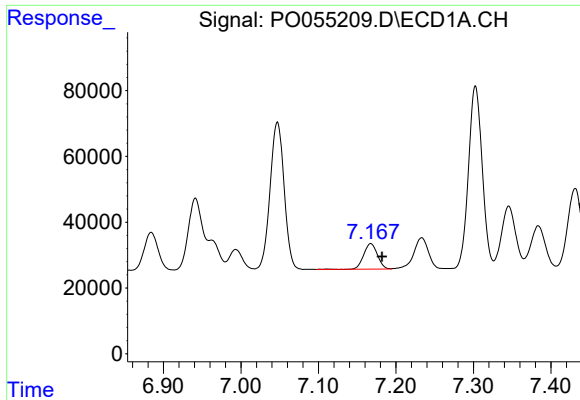

#29 AR-1254-4


R.T.: 7.168 min
Delta R.T.: -0.015 min
Response: 95291
Conc: 38.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

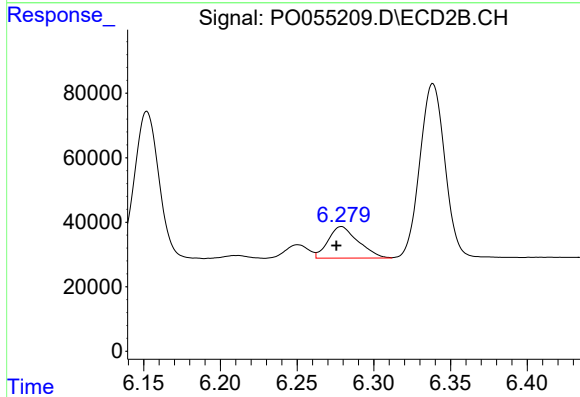


#29 AR-1254-4

R.T.: 6.279 min
Delta R.T.: 0.003 min
Response: 133525
Conc: 68.20 ng/ml

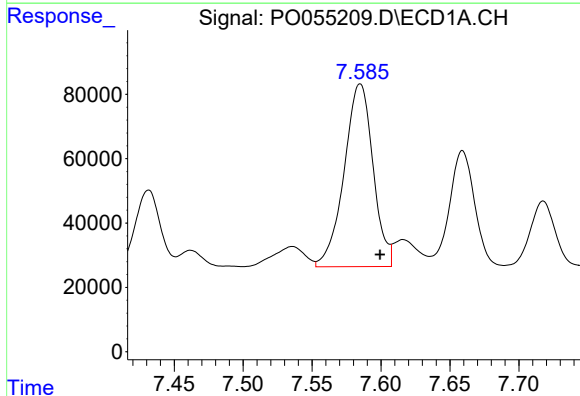


#30 AR-1254-5

R.T.: 7.585 min
Delta R.T.: -0.015 min
Response: 829295
Conc: 309.40 ng/ml

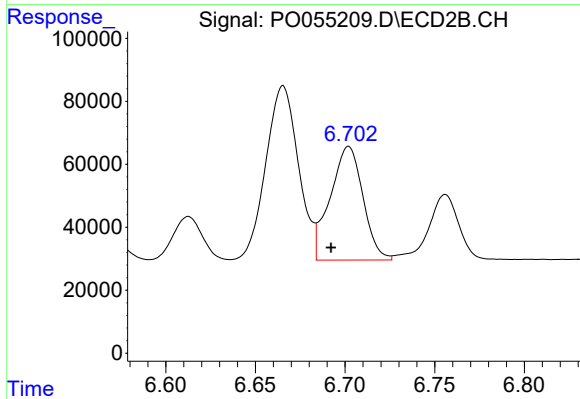

#30 AR-1254-5


R.T.: 6.702 min
Delta R.T.: 0.010 min
Response: 459065
Conc: 159.69 ng/ml

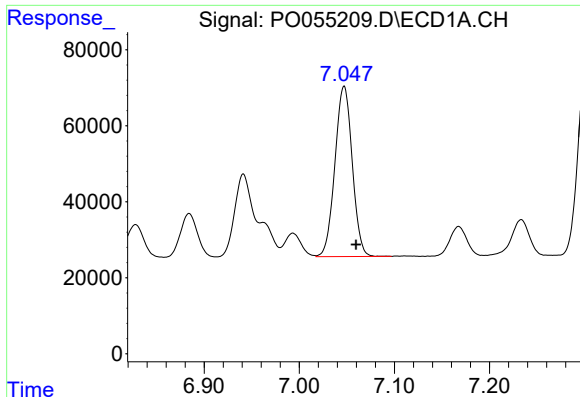

#31 AR-1260-1


R.T.: 7.047 min
Delta R.T.: -0.012 min
Response: 567506
Conc: 225.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

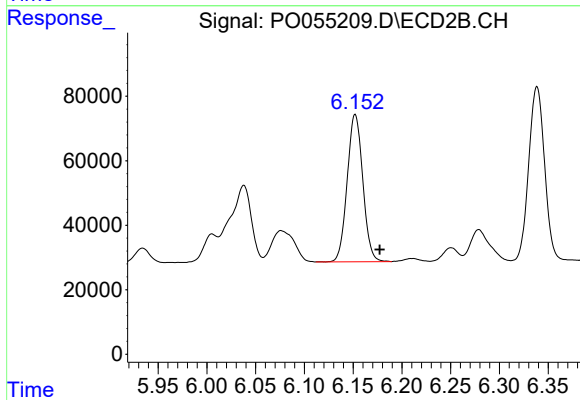


#31 AR-1260-1

R.T.: 6.152 min
Delta R.T.: -0.025 min
Response: 510162
Conc: 222.00 ng/ml

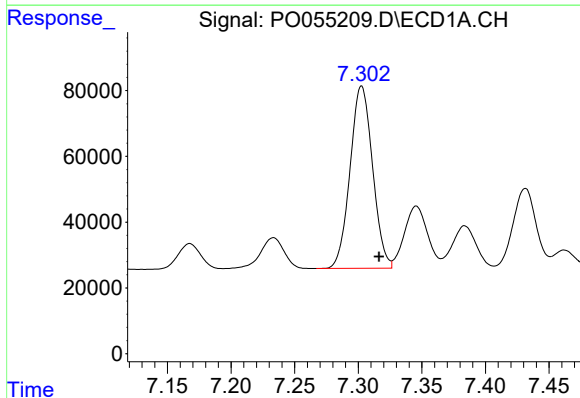


#32 AR-1260-2

R.T.: 7.303 min
Delta R.T.: -0.014 min
Response: 682723
Conc: 219.98 ng/ml

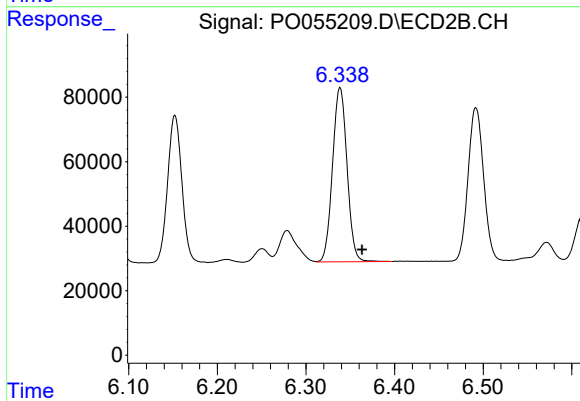

#32 AR-1260-2


R.T.: 6.339 min
Delta R.T.: -0.025 min
Response: 614310
Conc: 223.16 ng/ml

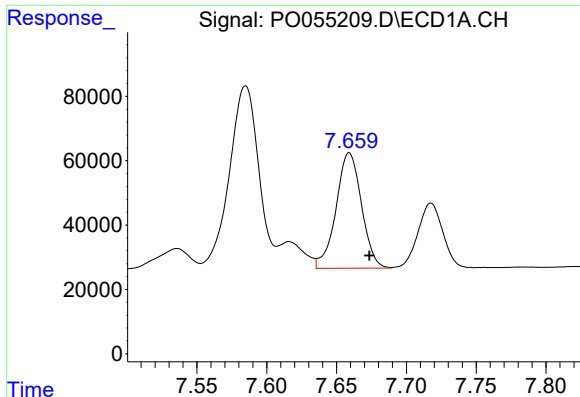

#33 AR-1260-3


R.T.: 7.659 min
Delta R.T.: -0.015 min
Response: 454952
Conc: 185.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

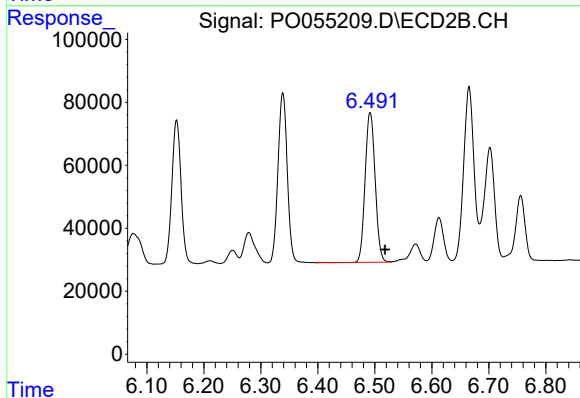


#33 AR-1260-3

R.T.: 6.492 min
Delta R.T.: -0.026 min
Response: 578966
Conc: 224.59 ng/ml

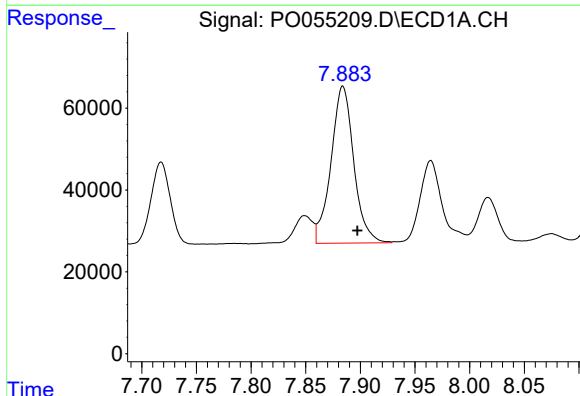


#34 AR-1260-4

R.T.: 7.884 min
Delta R.T.: -0.013 min
Response: 556431
Conc: 201.17 ng/ml

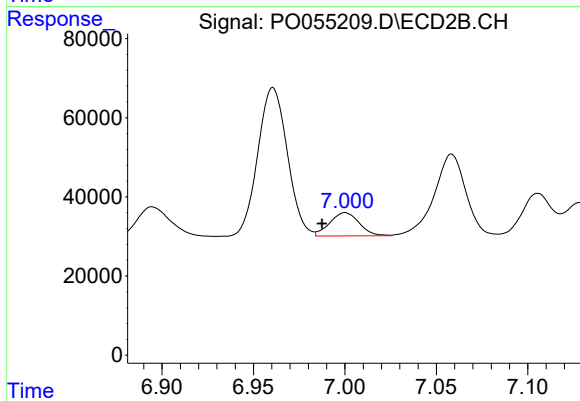

#34 AR-1260-4


R.T.: 7.000 min
Delta R.T.: 0.013 min
Response: 66126
Conc: 31.07 ng/ml

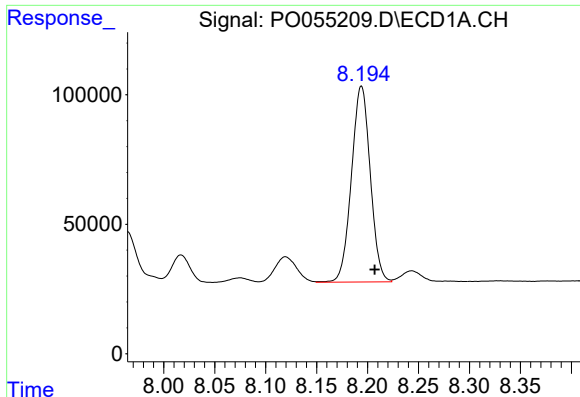

#35 AR-1260-5


R.T.: 8.194 min
Delta R.T.: -0.013 min
Response: 972526
Conc: 175.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

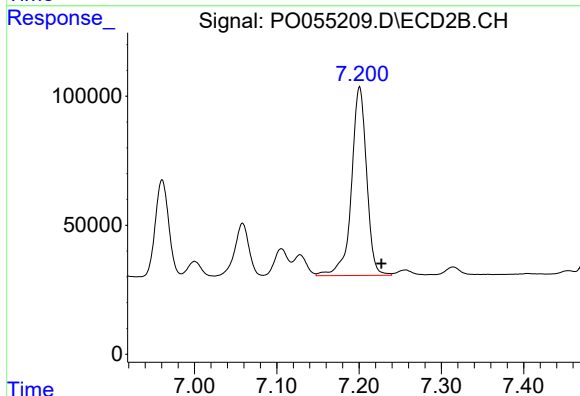


#35 AR-1260-5

R.T.: 7.201 min
Delta R.T.: -0.026 min
Response: 935724
Conc: 195.38 ng/ml

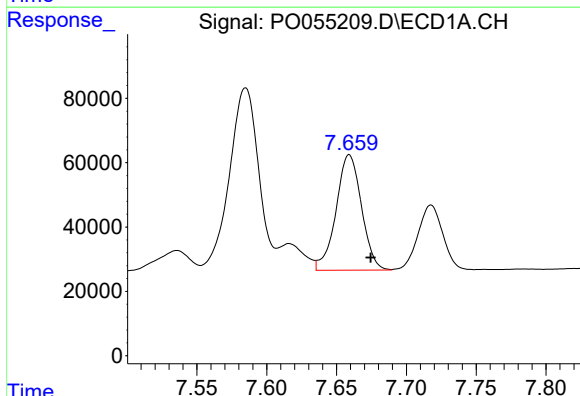


#36 AR-1262-1

R.T.: 7.659 min
Delta R.T.: -0.016 min
Response: 454952
Conc: 136.54 ng/ml

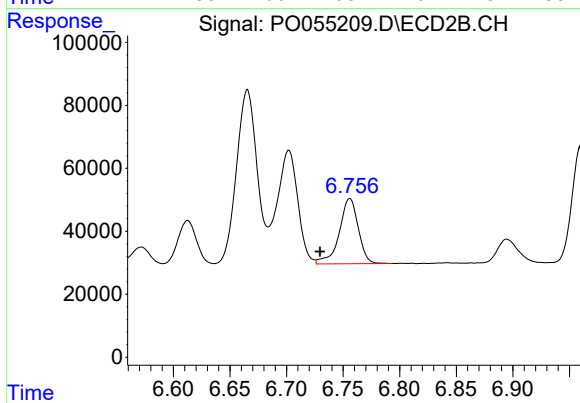

#36 AR-1262-1


R.T.: 6.756 min
Delta R.T.: 0.026 min
Response: 242469
Conc: 81.50 ng/ml

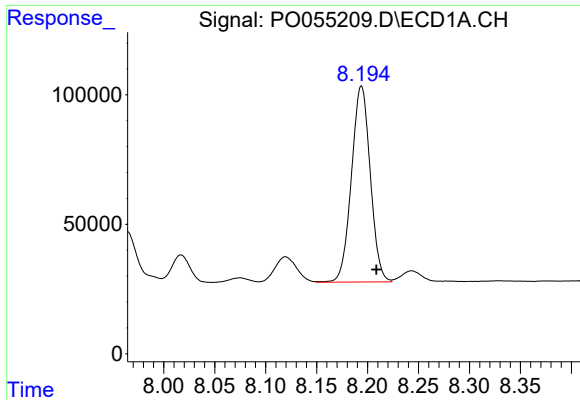

#37 AR-1262-2


R.T.: 8.194 min
Delta R.T.: -0.015 min
Response: 972526
Conc: 164.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

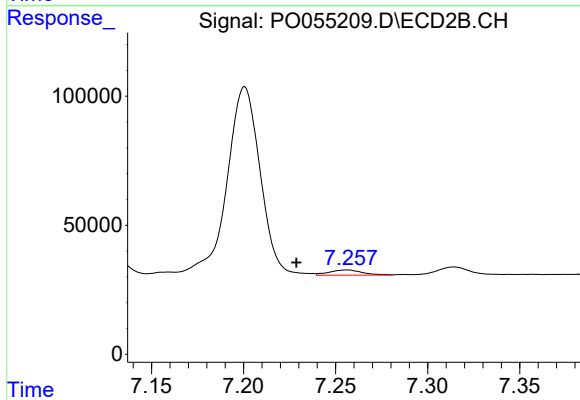


#37 AR-1262-2

R.T.: 7.256 min
Delta R.T.: 0.028 min
Response: 25528
Conc: 5.21 ng/ml

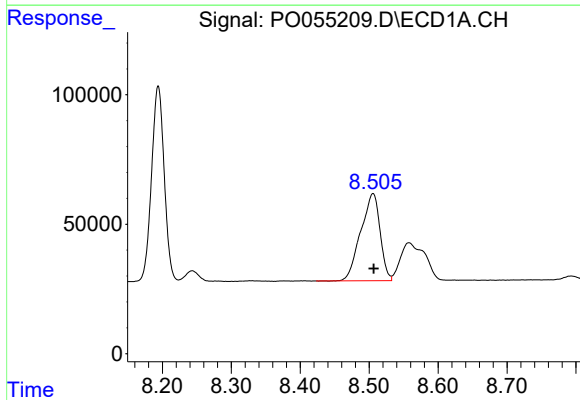


#38 AR-1262-3

R.T.: 8.506 min
Delta R.T.: -0.001 min
Response: 656347
Conc: 158.43 ng/ml

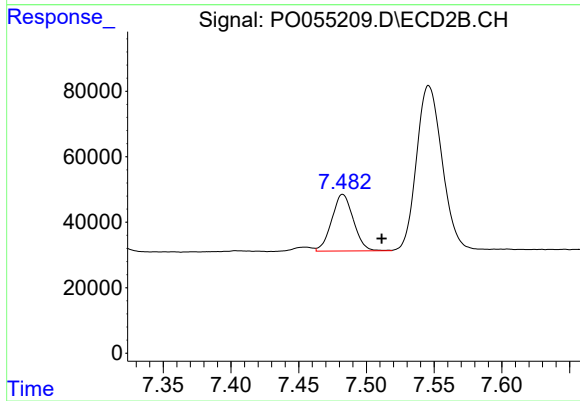

#38 AR-1262-3


R.T.: 7.483 min
Delta R.T.: -0.029 min
Response: 192336
Conc: 93.66 ng/ml

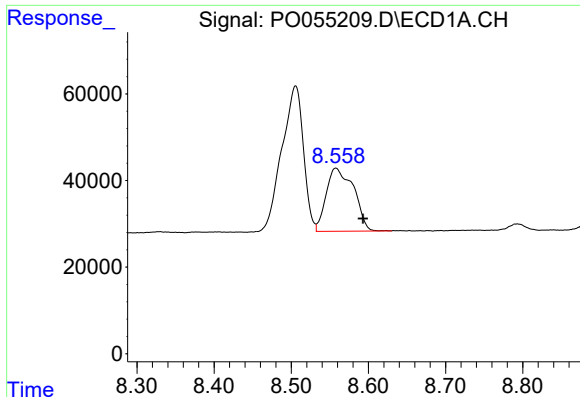

#39 AR-1262-4


R.T.: 8.558 min
Delta R.T.: -0.035 min
Response: 360756
Conc: 111.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

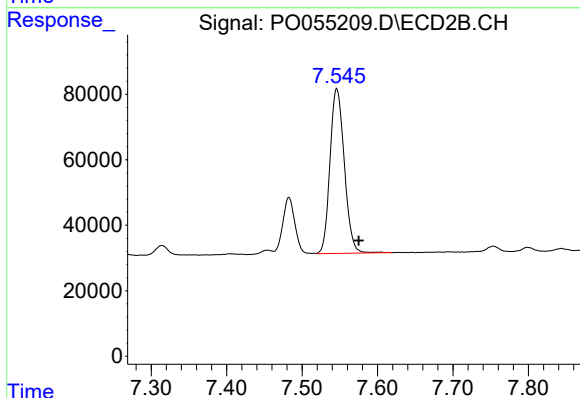


#39 AR-1262-4

R.T.: 7.546 min
Delta R.T.: -0.029 min
Response: 664115
Conc: 183.35 ng/ml

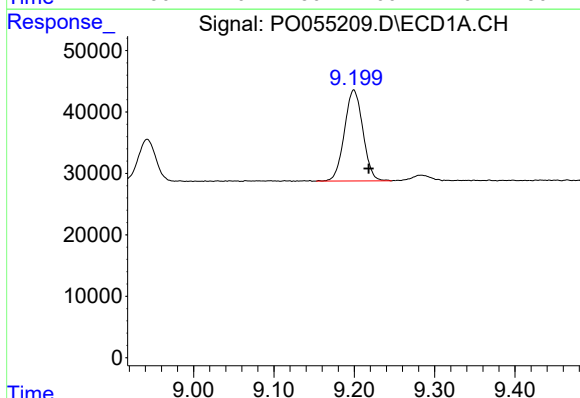


#40 AR-1262-5

R.T.: 9.199 min
Delta R.T.: -0.019 min
Response: 236903
Conc: 108.36 ng/ml

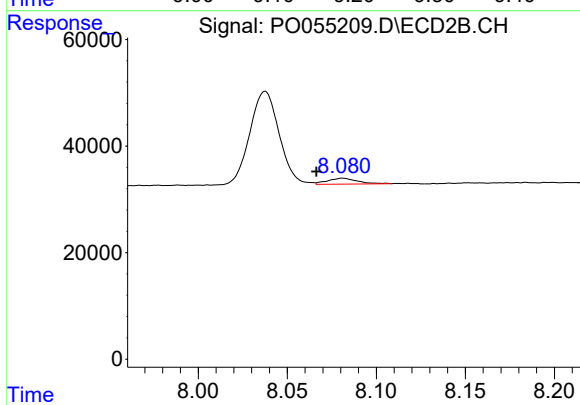

#40 AR-1262-5


R.T.: 8.081 min
Delta R.T.: 0.015 min
Response: 12925
Conc: 8.01 ng/ml

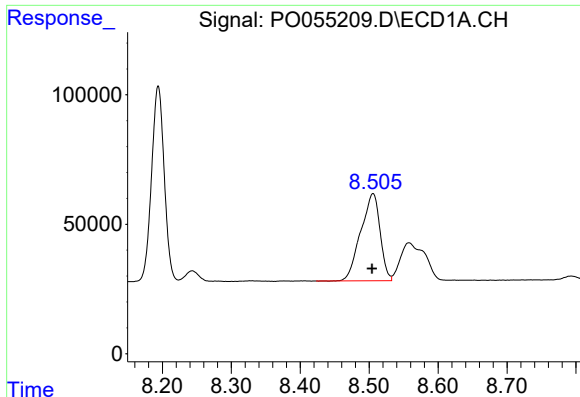

#41 AR-1268-1


R.T.: 8.506 min
Delta R.T.: 0.001 min
Response: 656347
Conc: 92.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

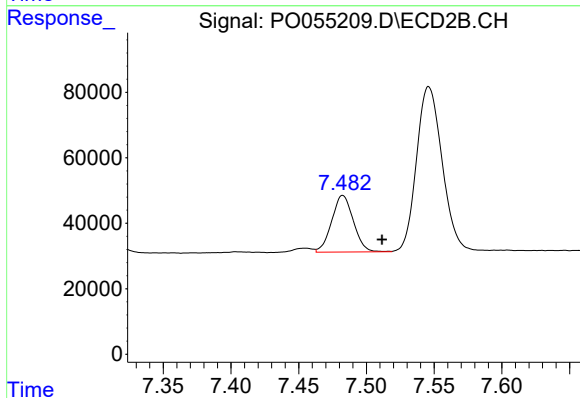


#41 AR-1268-1

R.T.: 7.483 min
Delta R.T.: -0.029 min
Response: 192336
Conc: 34.02 ng/ml

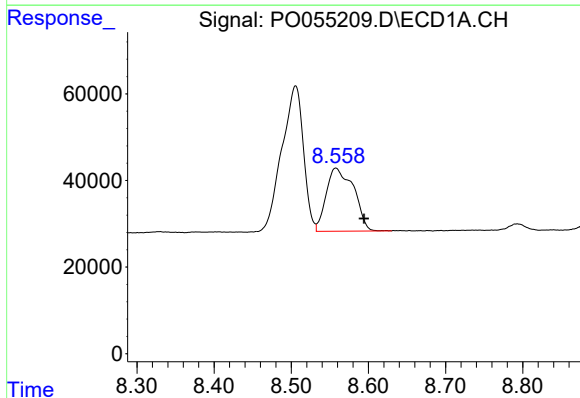


#42 AR-1268-2

R.T.: 8.558 min
Delta R.T.: -0.037 min
Response: 360756
Conc: 55.06 ng/ml

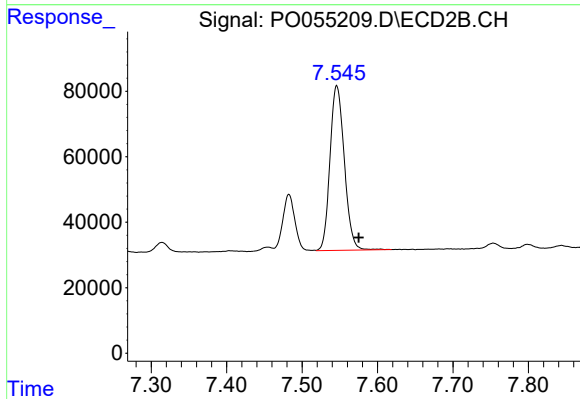

#42 AR-1268-2


R.T.: 7.546 min
Delta R.T.: -0.029 min
Response: 664115
Conc: 128.42 ng/ml

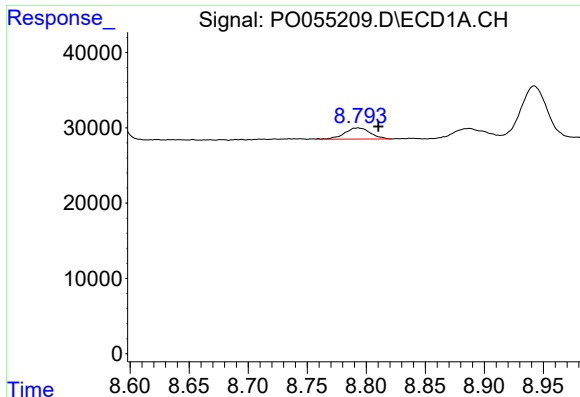

#43 AR-1268-3


R.T.: 8.793 min
Delta R.T.: -0.017 min
Response: 22634
Conc: 4.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

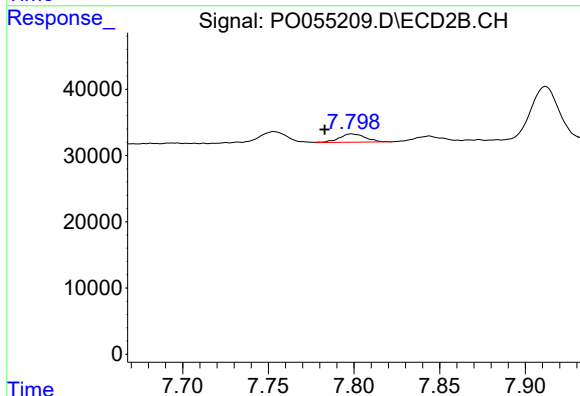


#43 AR-1268-3

R.T.: 7.799 min
Delta R.T.: 0.016 min
Response: 13532
Conc: 3.14 ng/ml

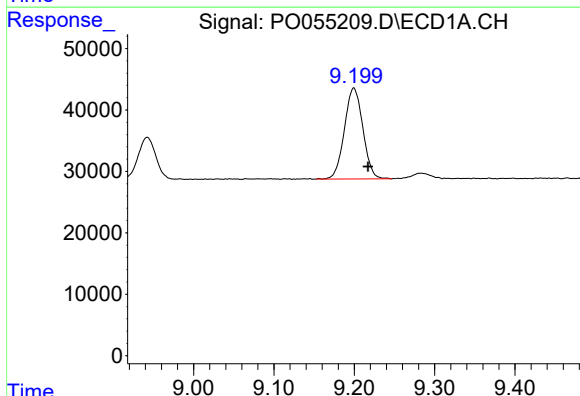


#44 AR-1268-4

R.T.: 9.199 min
Delta R.T.: -0.018 min
Response: 236903
Conc: 99.30 ng/ml

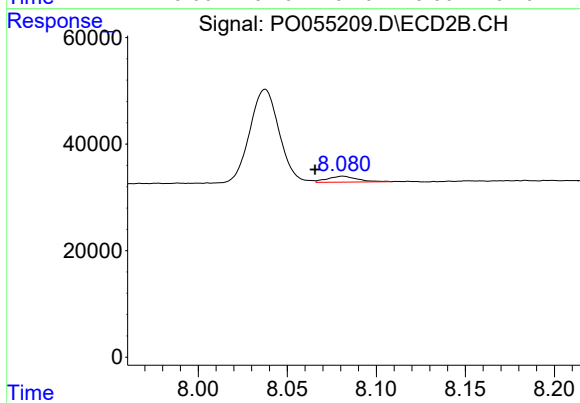

#44 AR-1268-4


R.T.: 8.081 min
Delta R.T.: 0.016 min
Response: 12925
Conc: 6.97 ng/ml

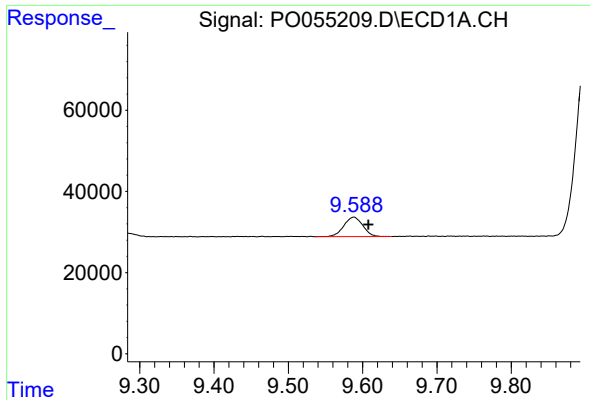

#45 AR-1268-5

R.T.: 9.588 min
Delta R.T.: -0.020 min
Response: 86622
Conc: 5.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-E1-E1A-F1-F1AMSD

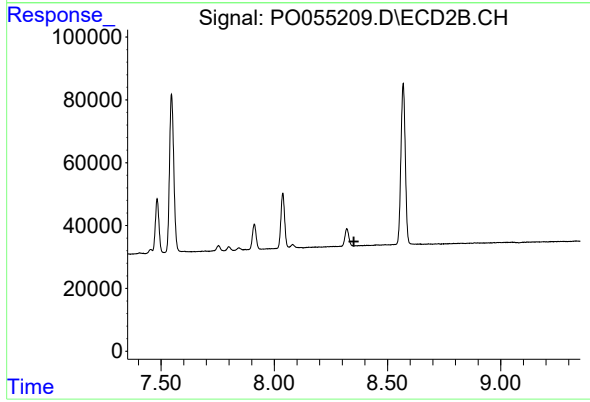

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 8.352 min
Response: 0
Conc: N.D.