

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041219\
 Data File : P0055222.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Apr 2019 13:23
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 13:49:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.292	3.605	626466	581602	18.051	18.225
2)	SA Decachlor...	9.903	8.570	940791	679602	19.084	21.339
Target Compounds							
7)	L1 AR-1016-5	5.929	0.000	81875	0	61.364	N.D. #
8)	L2 AR-1221-1	0.000	3.904	0	8563	N.D.	22.024 #
9)	L2 AR-1221-2	4.596	3.904	9416	8563	27.765	28.562
23)	L5 AR-1248-3	5.929	0.000	81875	0	51.263	N.D. #
27)	L6 AR-1254-2	6.474	0.000	13615	0	4.769	N.D. #
28)	L6 AR-1254-3	6.891	0.000	11587	0	3.685	N.D. #
29)	L6 AR-1254-4	0.000	6.328	0	7977	N.D.	4.074 #
32)	L7 AR-1260-2	0.000	6.328	0	7977	N.D.	2.898 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041219\
Data File : PO055222.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Apr 2019 13:23
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 13:49:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

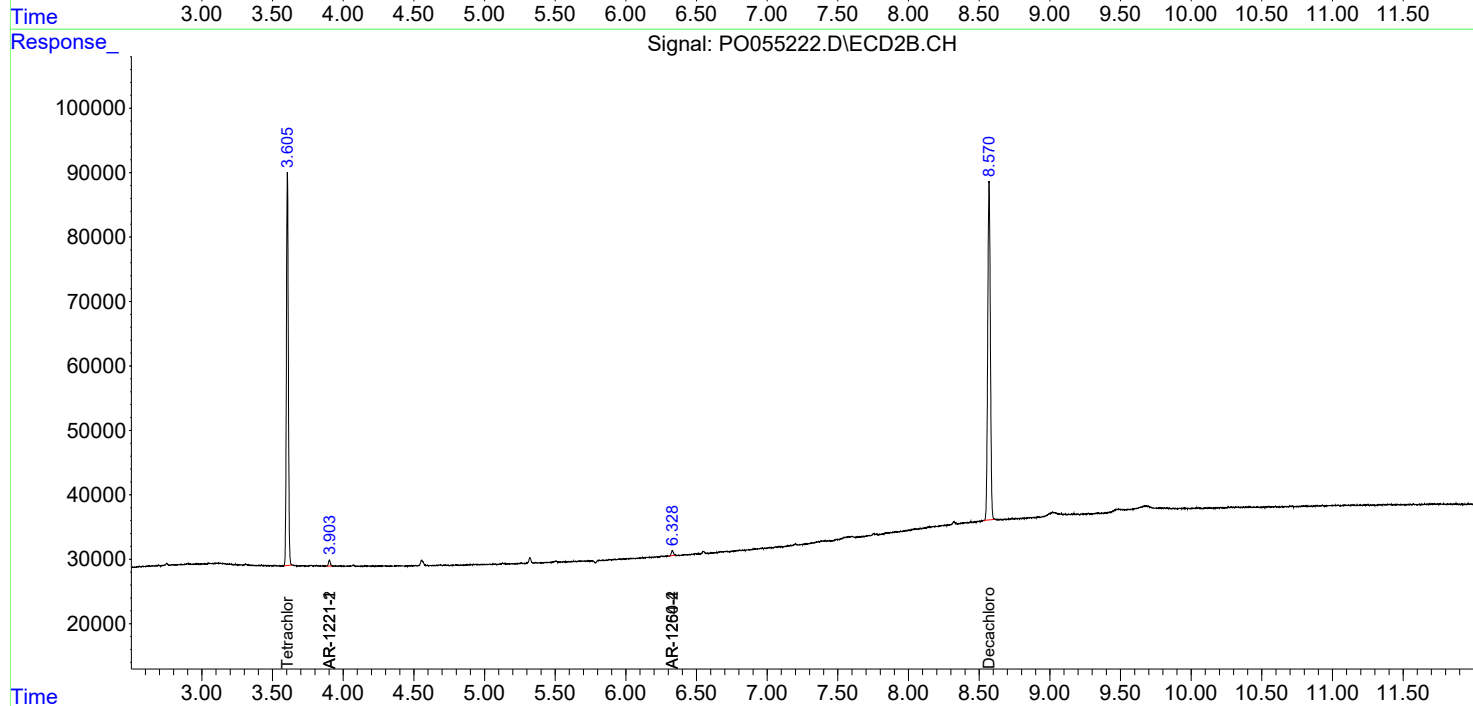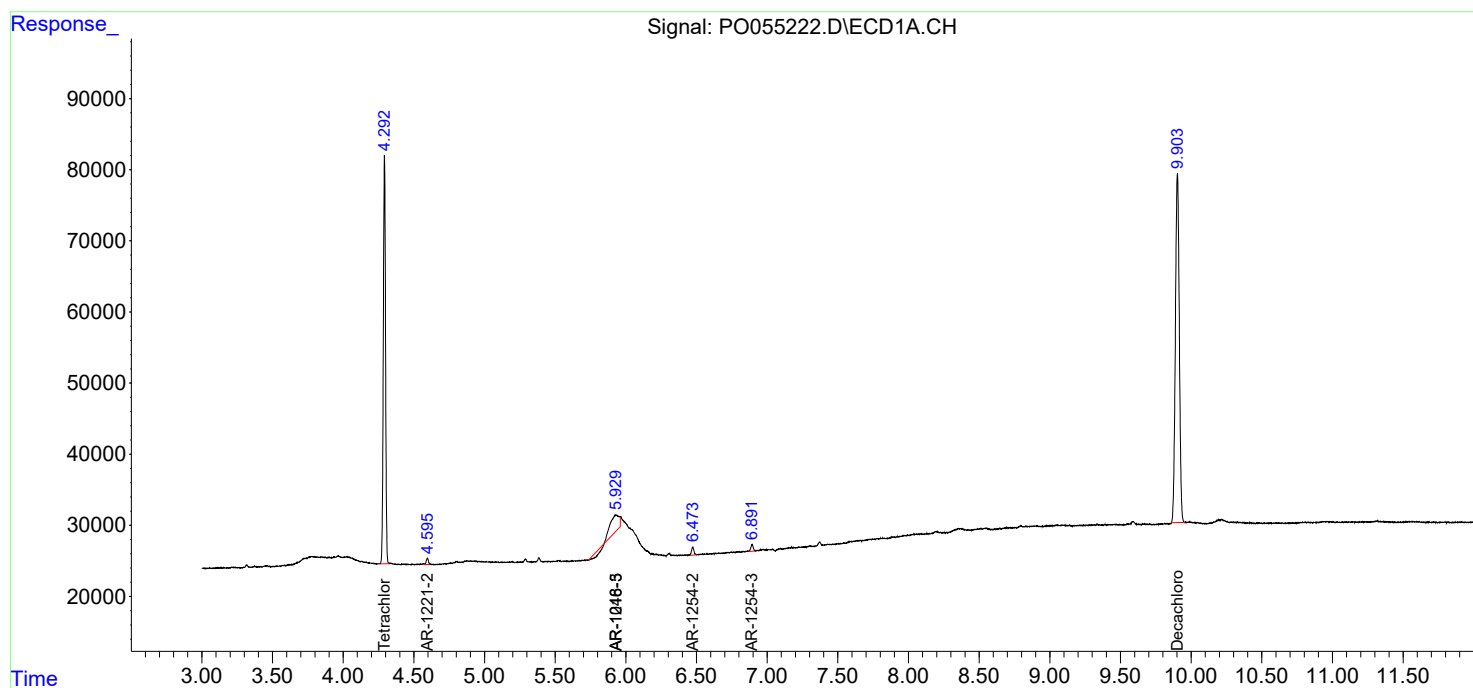


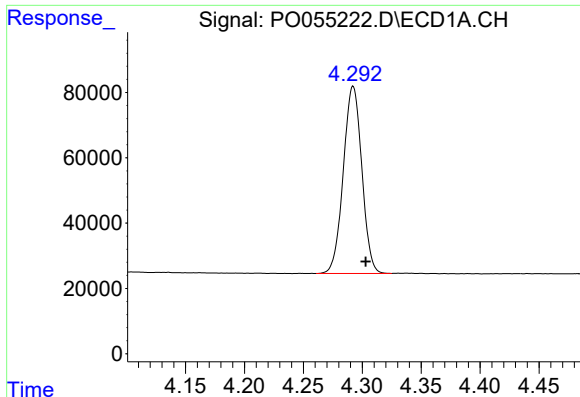

#1 Tetrachloro-m-xylene


R.T.: 4.292 min
Delta R.T.: -0.011 min
Response: 626466
Conc: 18.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

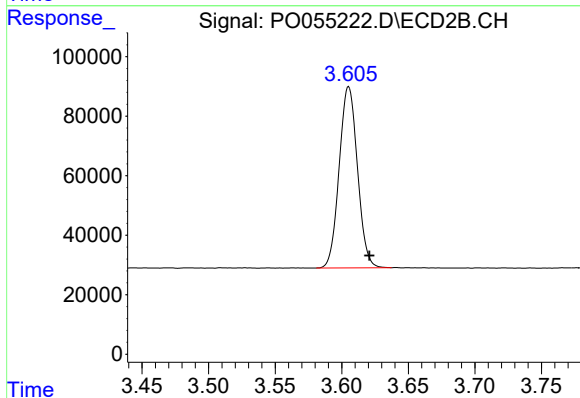


#1 Tetrachloro-m-xylene

R.T.: 3.605 min
Delta R.T.: -0.016 min
Response: 581602
Conc: 18.22 ng/ml

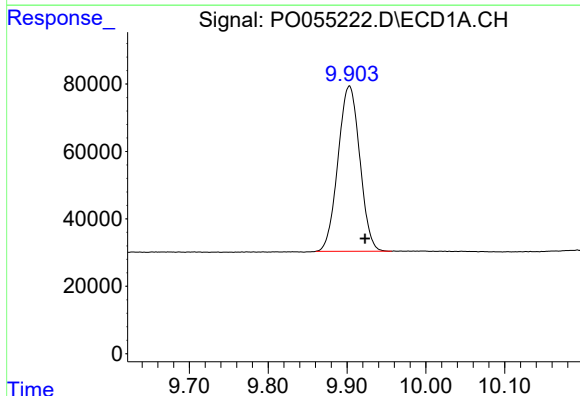


#2 Decachlorobiphenyl

R.T.: 9.903 min
Delta R.T.: -0.020 min
Response: 940791
Conc: 19.08 ng/ml

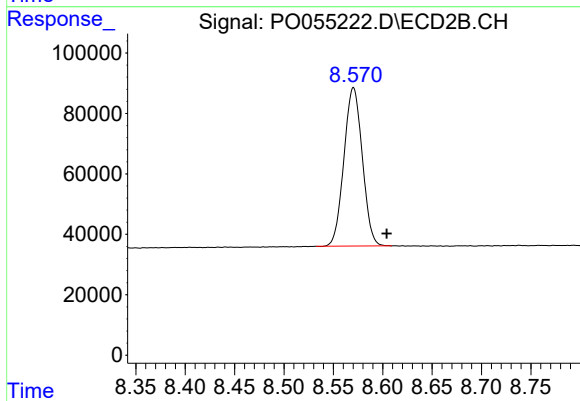

#2 Decachlorobiphenyl


R.T.: 8.570 min
Delta R.T.: -0.034 min
Response: 679602
Conc: 21.34 ng/ml

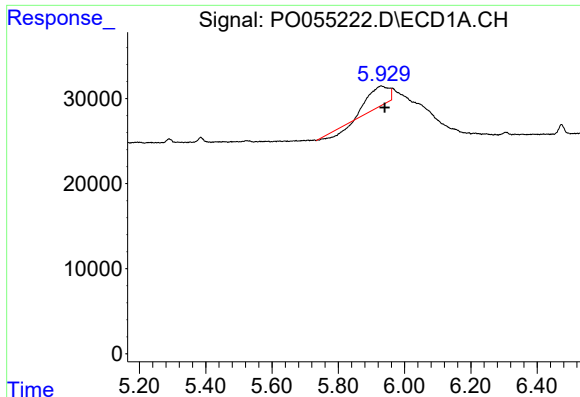

#7 AR-1016-5


R.T.: 5.929 min
Delta R.T.: -0.010 min
Response: 81875
Conc: 61.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

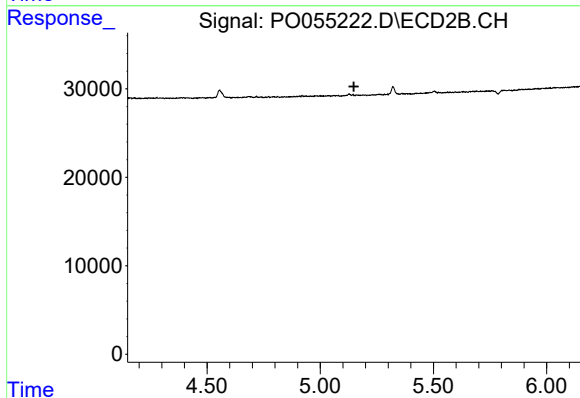


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 5.149 min
Response: 0
Conc: N.D.

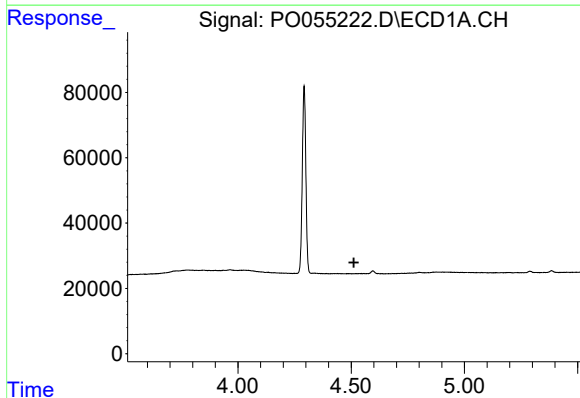


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.512 min
Response: 0
Conc: N.D.

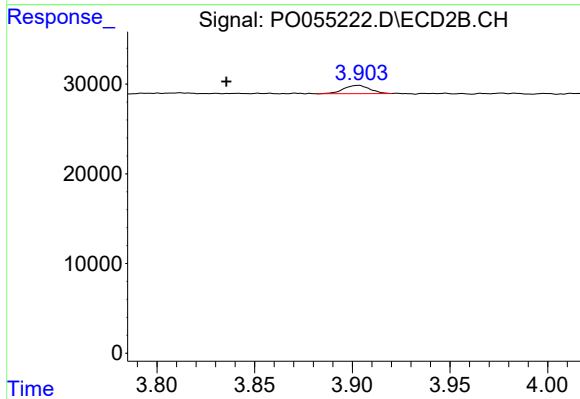

#8 AR-1221-1


R.T.: 3.904 min
Delta R.T.: 0.068 min
Response: 8563
Conc: 22.02 ng/ml

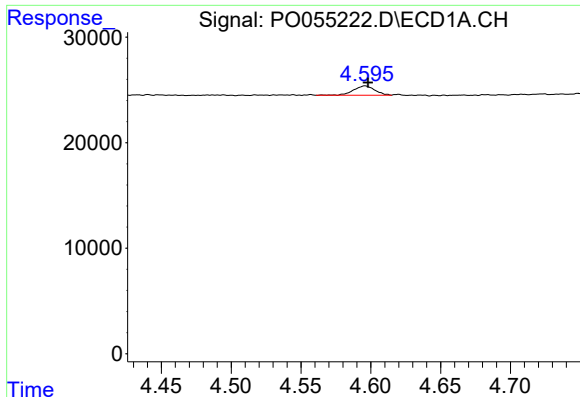

#9 AR-1221-2


R.T.: 4.596 min
Delta R.T.: -0.002 min
Response: 9416
Conc: 27.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

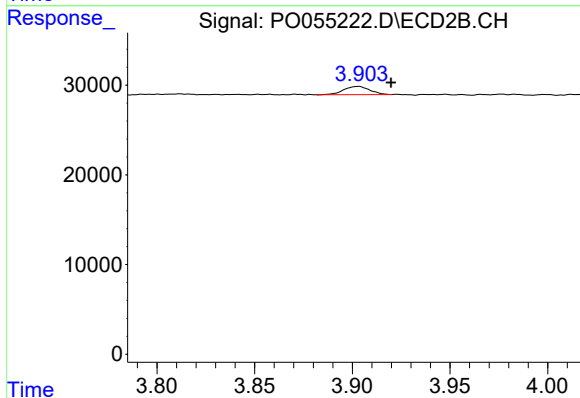


#9 AR-1221-2

R.T.: 3.904 min
Delta R.T.: -0.016 min
Response: 8563
Conc: 28.56 ng/ml

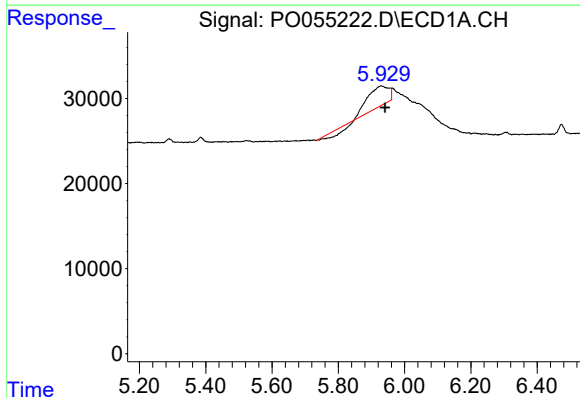


#23 AR-1248-3

R.T.: 5.929 min
Delta R.T.: -0.011 min
Response: 81875
Conc: 51.26 ng/ml

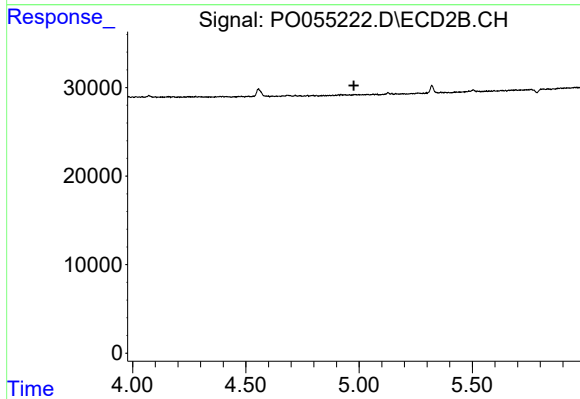

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 4.977 min
Response: 0
Conc: N.D.

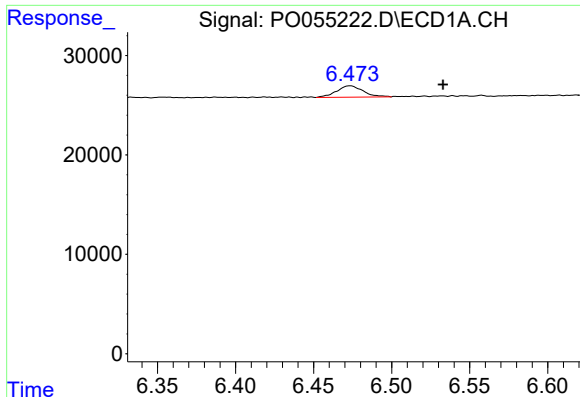

#27 AR-1254-2


R.T.: 6.474 min
Delta R.T.: -0.059 min
Response: 13615
Conc: 4.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

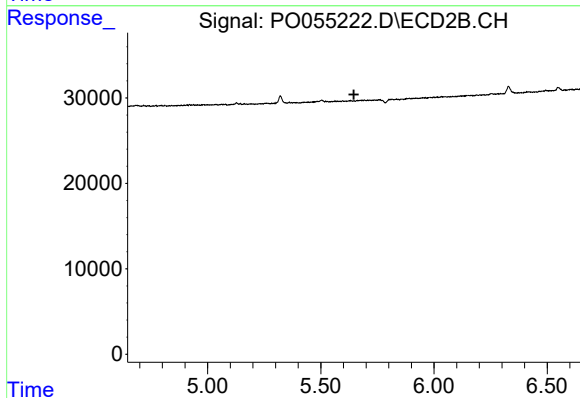


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 5.646 min
Response: 0
Conc: N.D.

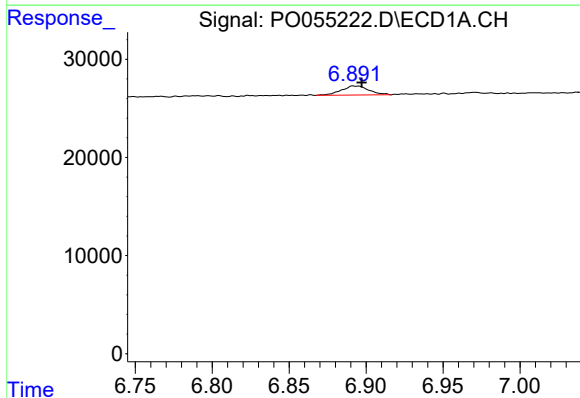


#28 AR-1254-3

R.T.: 6.891 min
Delta R.T.: -0.006 min
Response: 11587
Conc: 3.68 ng/ml

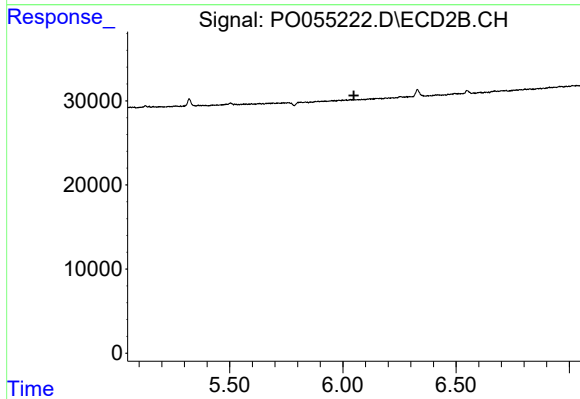

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.049 min
Response: 0
Conc: N.D.

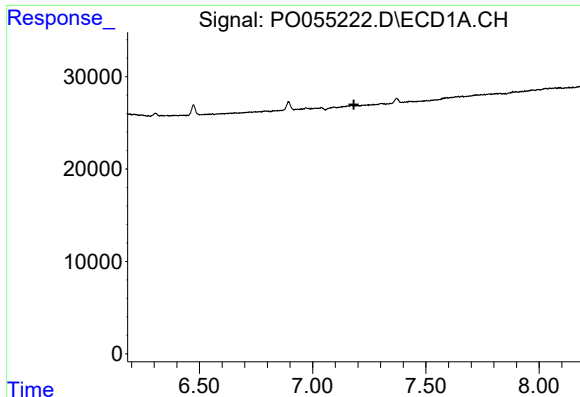

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

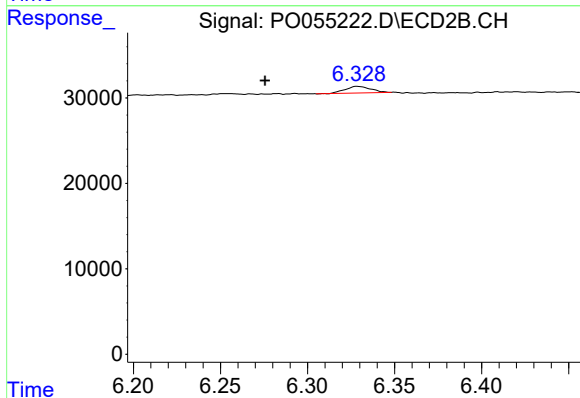


#29 AR-1254-4

R.T.: 6.328 min
Delta R.T.: 0.053 min
Response: 7977
Conc: 4.07 ng/ml

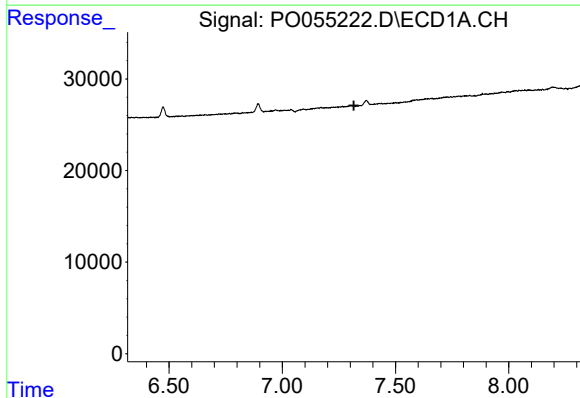

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.316 min
Response: 0
Conc: N.D.

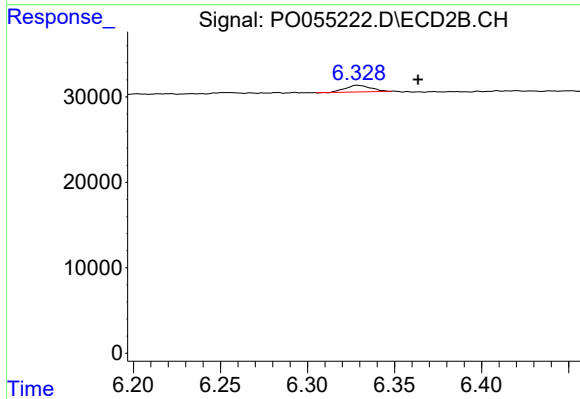

#32 AR-1260-2

R.T.: 6.328 min
Delta R.T.: -0.035 min
Response: 7977
Conc: 2.90 ng/ml