

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041219\
 Data File : P0055256.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Apr 2019 23:21
 Operator : SM/SJ
 Sample : PB118841BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB118841BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 00:50:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.292	3.604	642939	609831	18.526	19.110
2) SA Decachlor...	9.901	8.568	870530	650169	17.659	20.415
Target Compounds						
7) L1 AR-1016-5	5.927	0.000	24813	0	18.597	N.D. #
8) L2 AR-1221-1	0.000	3.901	0	9897	N.D.	25.456 #
9) L2 AR-1221-2	4.595	3.901	10226	9897	30.154	33.014
15) L3 AR-1232-5	5.776	0.000	406087	0	976.177	N.D. #
22) L5 AR-1248-2	5.776	0.000	406087	0	279.616	N.D. #
23) L5 AR-1248-3	5.927	0.000	24813	0	15.536	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041219\
Data File : PO055256.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Apr 2019 23:21
Operator : SM/SJ
Sample : PB118841BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB118841BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 00:50:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

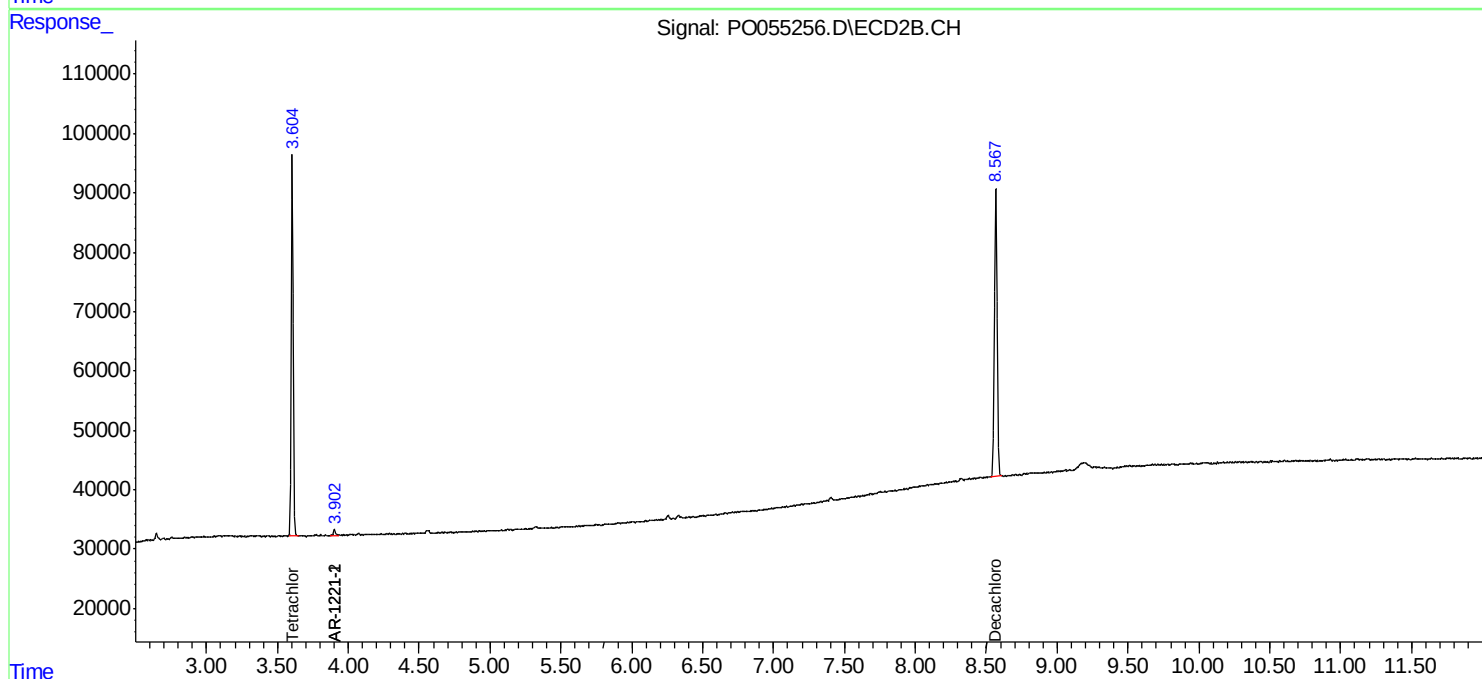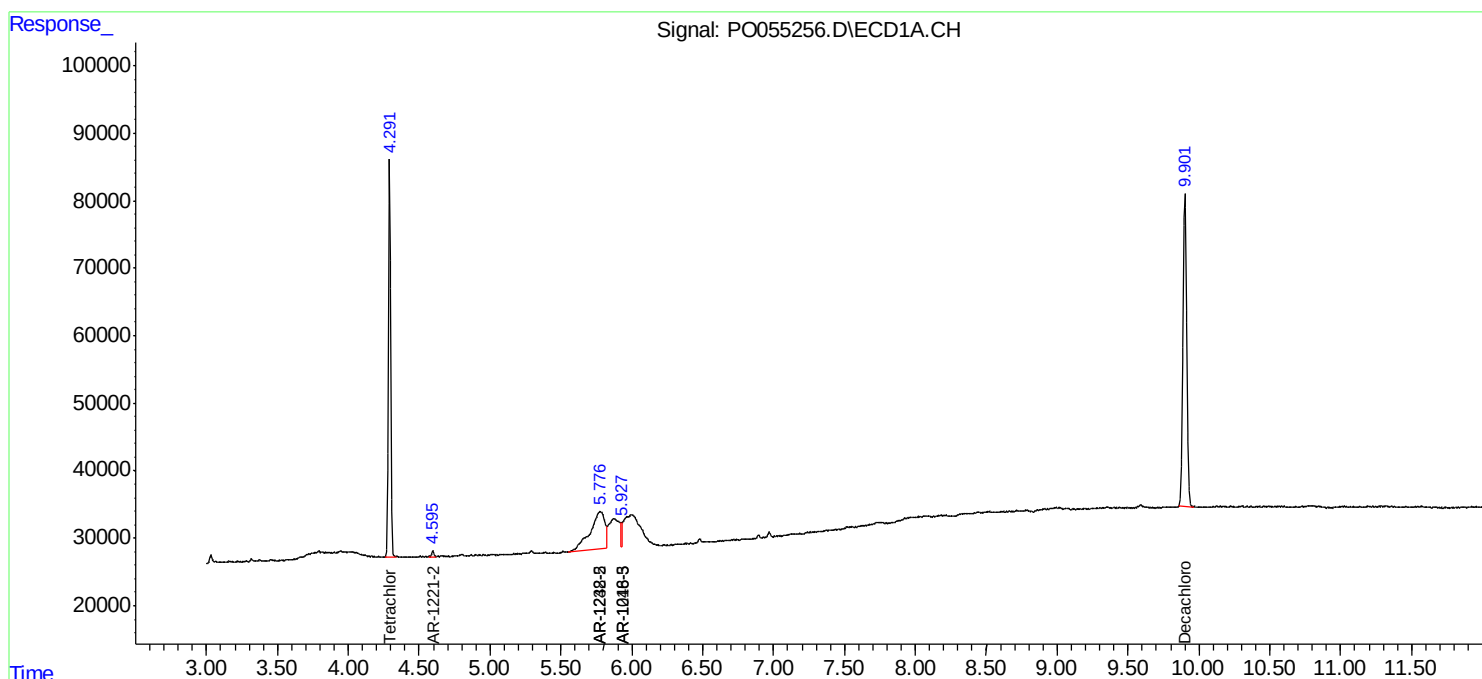


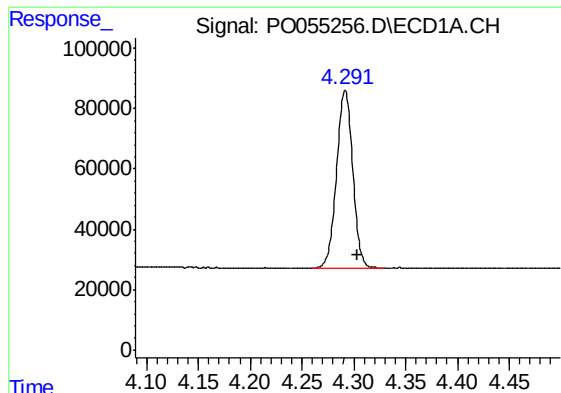

#1 Tetrachloro-m-xylene


R.T.: 4.292 min
Delta R.T.: -0.011 min
Response: 642939
Conc: 18.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB118841BL

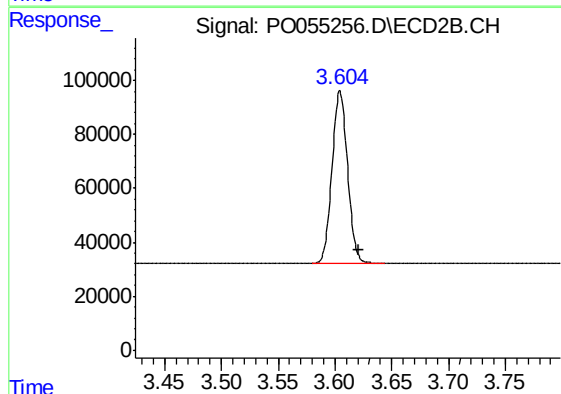


#1 Tetrachloro-m-xylene

R.T.: 3.604 min
Delta R.T.: -0.016 min
Response: 609831
Conc: 19.11 ng/ml

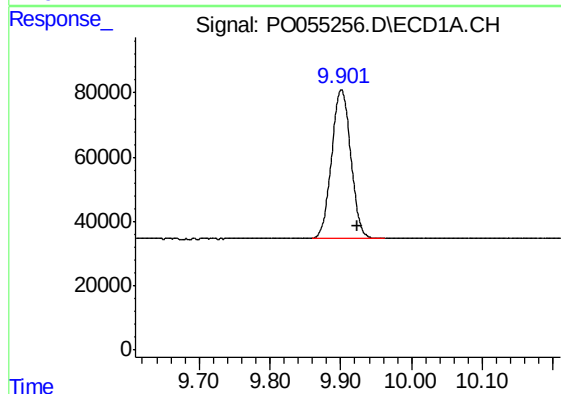


#2 Decachlorobiphenyl

R.T.: 9.901 min
Delta R.T.: -0.022 min
Response: 870530
Conc: 17.66 ng/ml

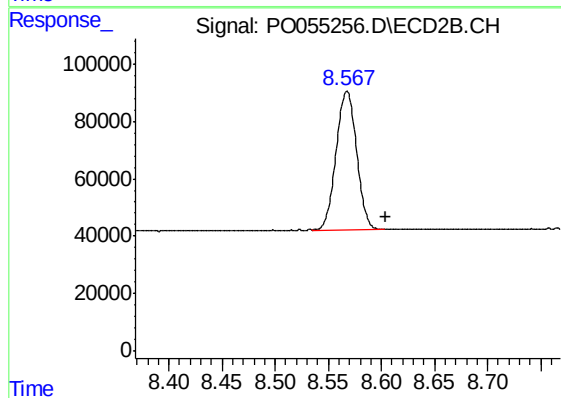

#2 Decachlorobiphenyl


R.T.: 8.568 min
Delta R.T.: -0.036 min
Response: 650169
Conc: 20.41 ng/ml

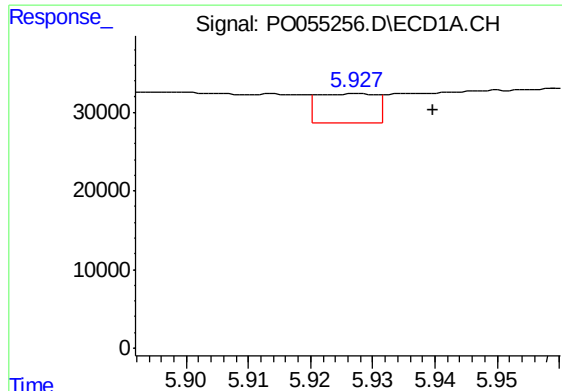

#7 AR-1016-5


R.T.: 5.927 min
Delta R.T.: -0.012 min
Response: 24813
Conc: 18.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB118841BL

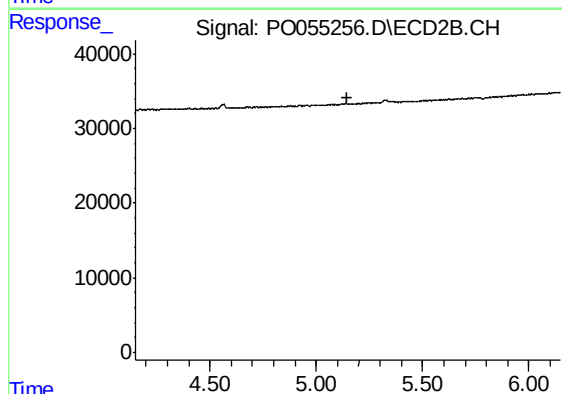


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 5.149 min
Response: 0
Conc: N.D.

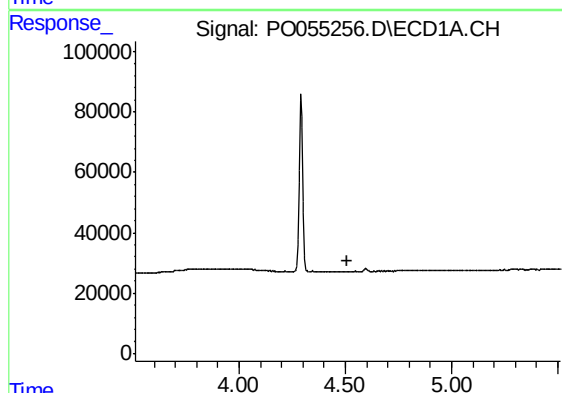


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.512 min
Response: 0
Conc: N.D.

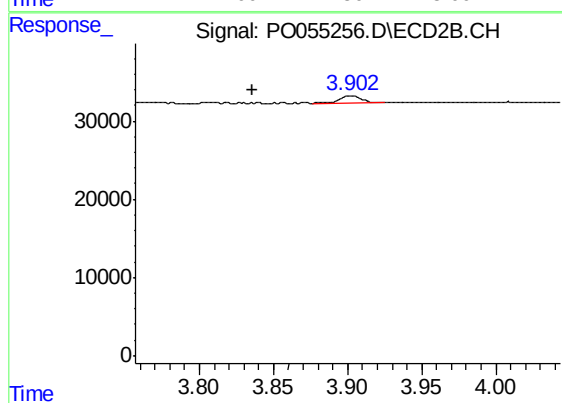

#8 AR-1221-1


R.T.: 3.901 min
Delta R.T.: 0.065 min
Response: 9897
Conc: 25.46 ng/ml

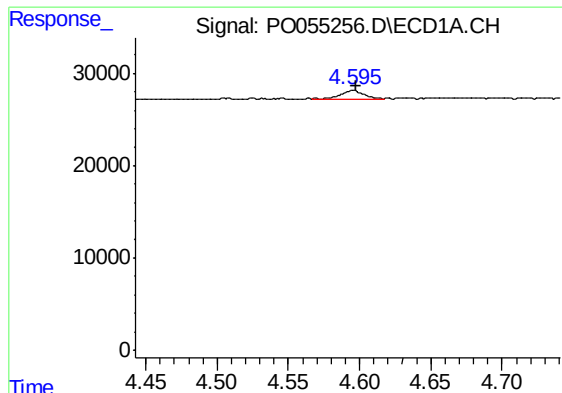

#9 AR-1221-2


R.T.: 4.595 min
Delta R.T.: -0.003 min
Response: 10226
Conc: 30.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB118841BL

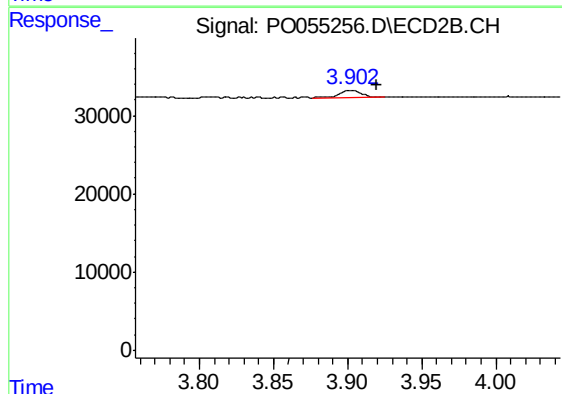


#9 AR-1221-2

R.T.: 3.901 min
Delta R.T.: -0.019 min
Response: 9897
Conc: 33.01 ng/ml

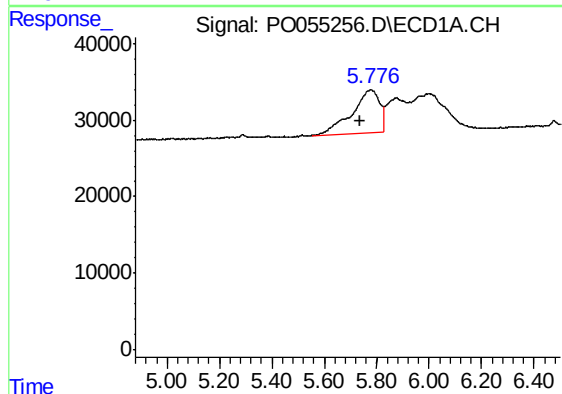


#15 AR-1232-5

R.T.: 5.776 min
Delta R.T.: 0.038 min
Response: 406087
Conc: 976.18 ng/ml

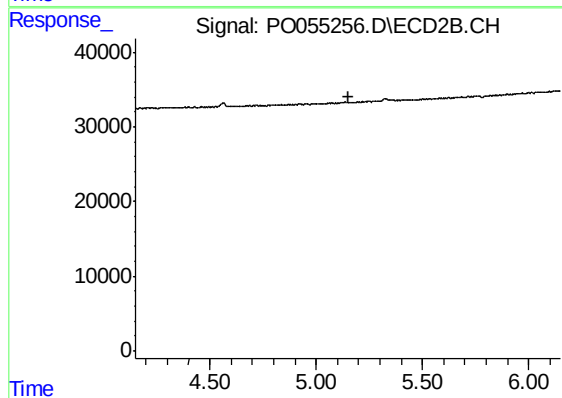

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T. : 5.150 min
Response: 0
Conc: N.D.

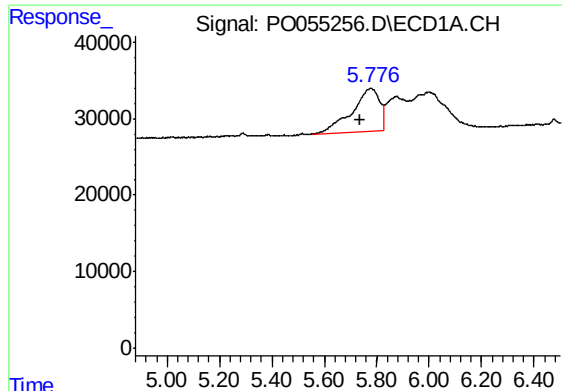

#22 AR-1248-2


R.T.: 5.776 min
Delta R.T.: 0.039 min
Response: 406087
Conc: 279.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB118841BL

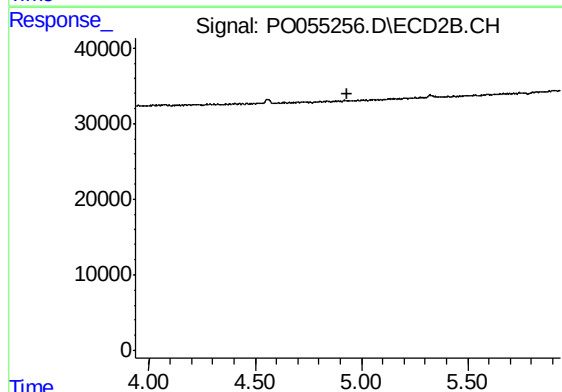


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 4.936 min
Response: 0
Conc: N.D.

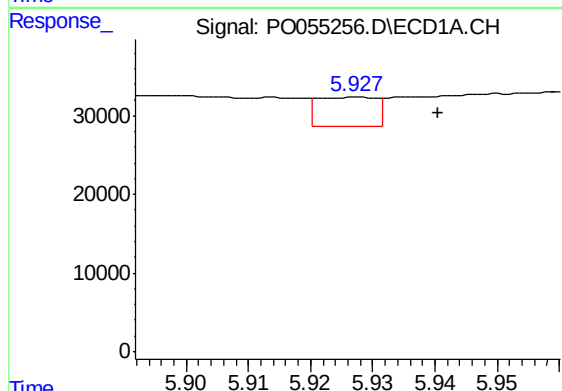

#23 AR-1248-3

R.T.: 5.927 min
Delta R.T.: -0.013 min
Response: 24813
Conc: 15.54 ng/ml

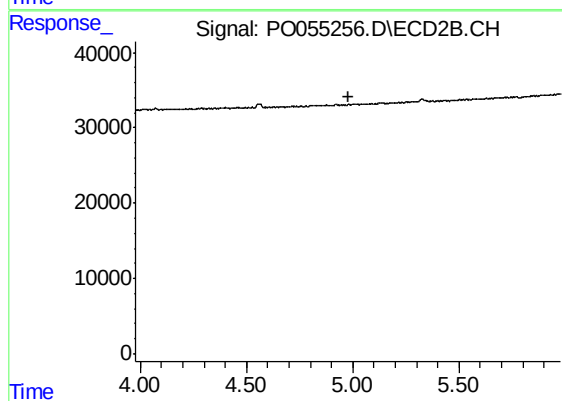

#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 4.977 min
Response: 0
Conc: N.D.