

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041219\
Data File : P0055220.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Apr 2019 12:49
Operator : SM/SJ
Sample : K2311-04RE
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
0237-COMP-CS-2-ELTRTRE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 15:59:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.293	3.605	538842	506780	15.526	15.880
2)	SA Decachlor...	9.903	8.569	450353	334798	9.135	10.512

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041219\
Data File : P0055220.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Apr 2019 12:49
Operator : SM/SJ
Sample : K2311-04RE
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
0237-COMP-CS-2-ELTRTRE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 15:59:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

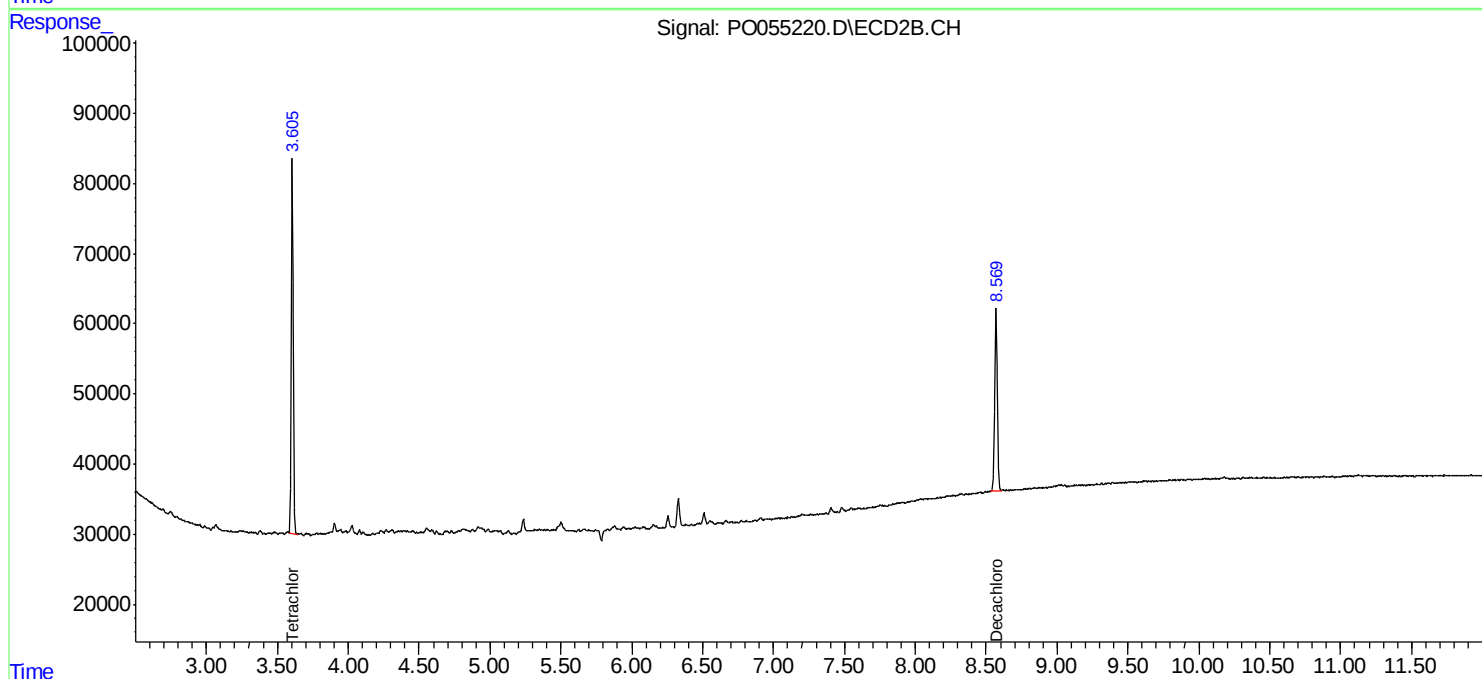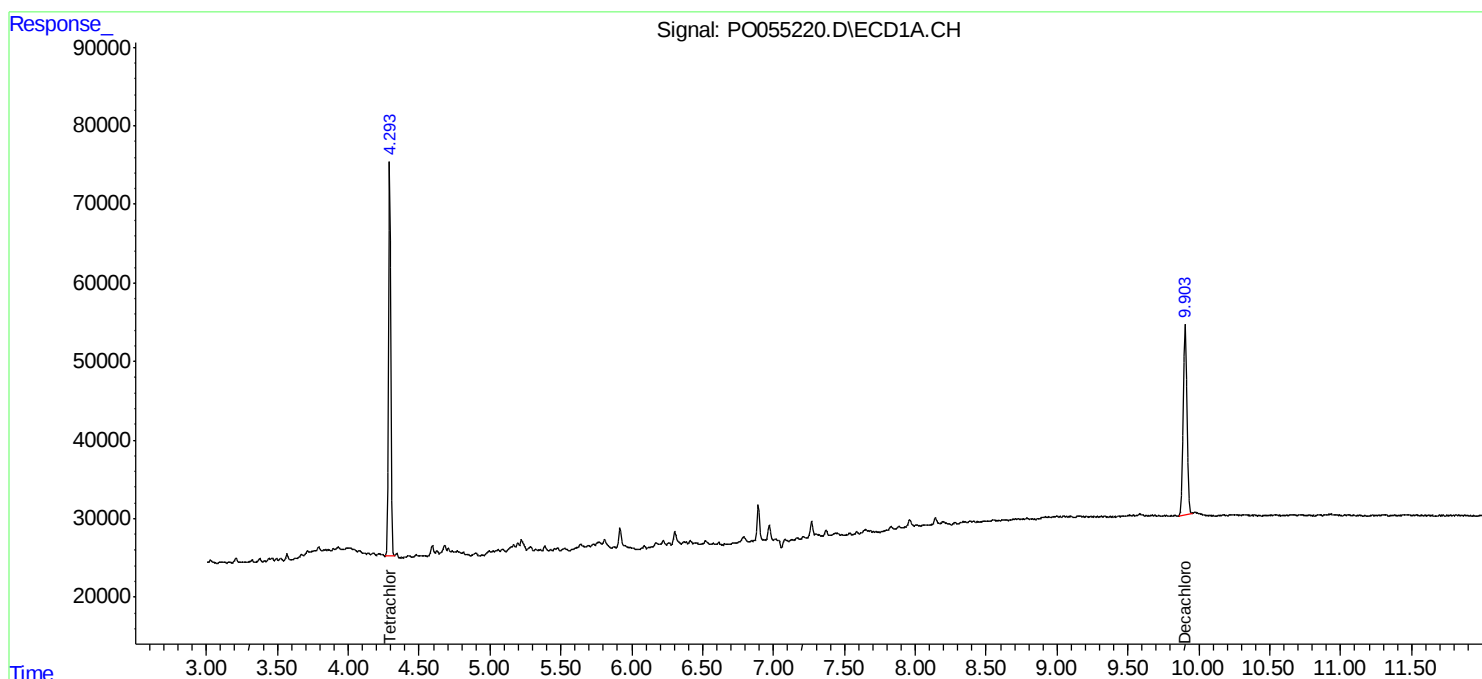


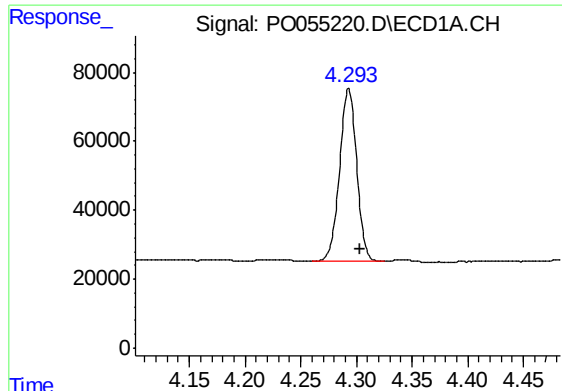

#1 Tetrachloro-m-xylene


R.T.: 4.293 min
Delta R.T.: -0.010 min
Response: 538842
Conc: 15.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
0237-COMP-CS-2-ELTRTRE

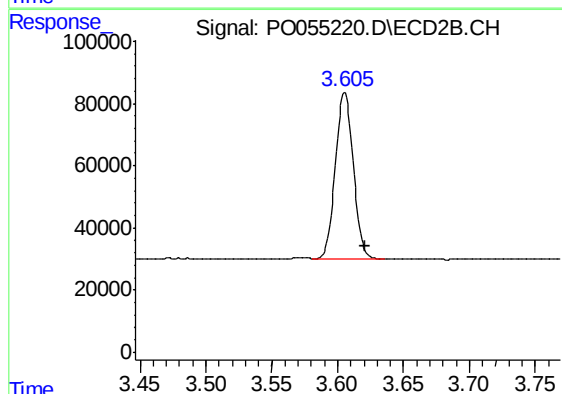


#1 Tetrachloro-m-xylene

R.T.: 3.605 min
Delta R.T.: -0.015 min
Response: 506780
Conc: 15.88 ng/ml

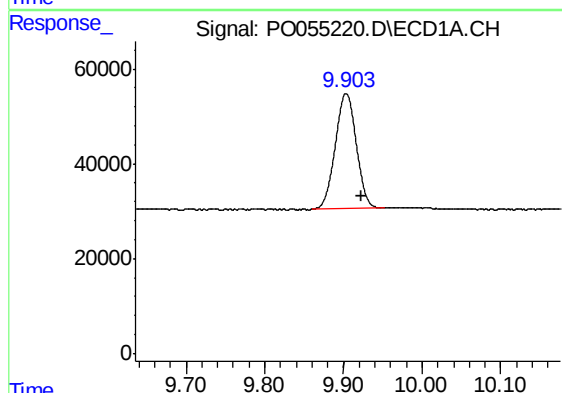

#2 Decachlorobiphenyl

R.T.: 9.903 min
Delta R.T.: -0.020 min
Response: 450353
Conc: 9.14 ng/ml

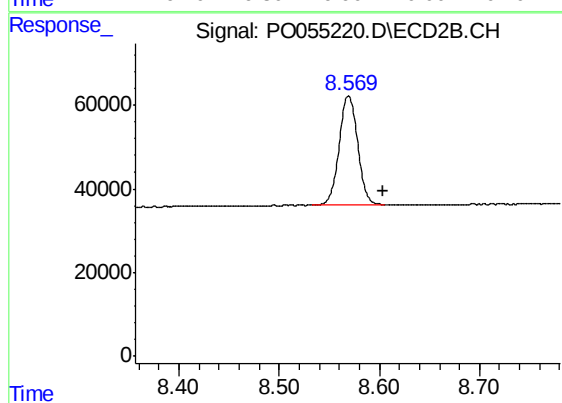

#2 Decachlorobiphenyl

R.T.: 8.569 min
Delta R.T.: -0.035 min
Response: 334798
Conc: 10.51 ng/ml