

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041219\
Data File : P0055245.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Apr 2019 20:14
Operator : SM/SJ
Sample : K2345-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 22:47:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.292	3.604	533270	514712	15.366	16.129
2)	SA Decachlor...	9.900	8.568	579455	456508	11.754	14.334

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041219\
Data File : P0055245.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Apr 2019 20:14
Operator : SM/SJ
Sample : K2345-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 22:47:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

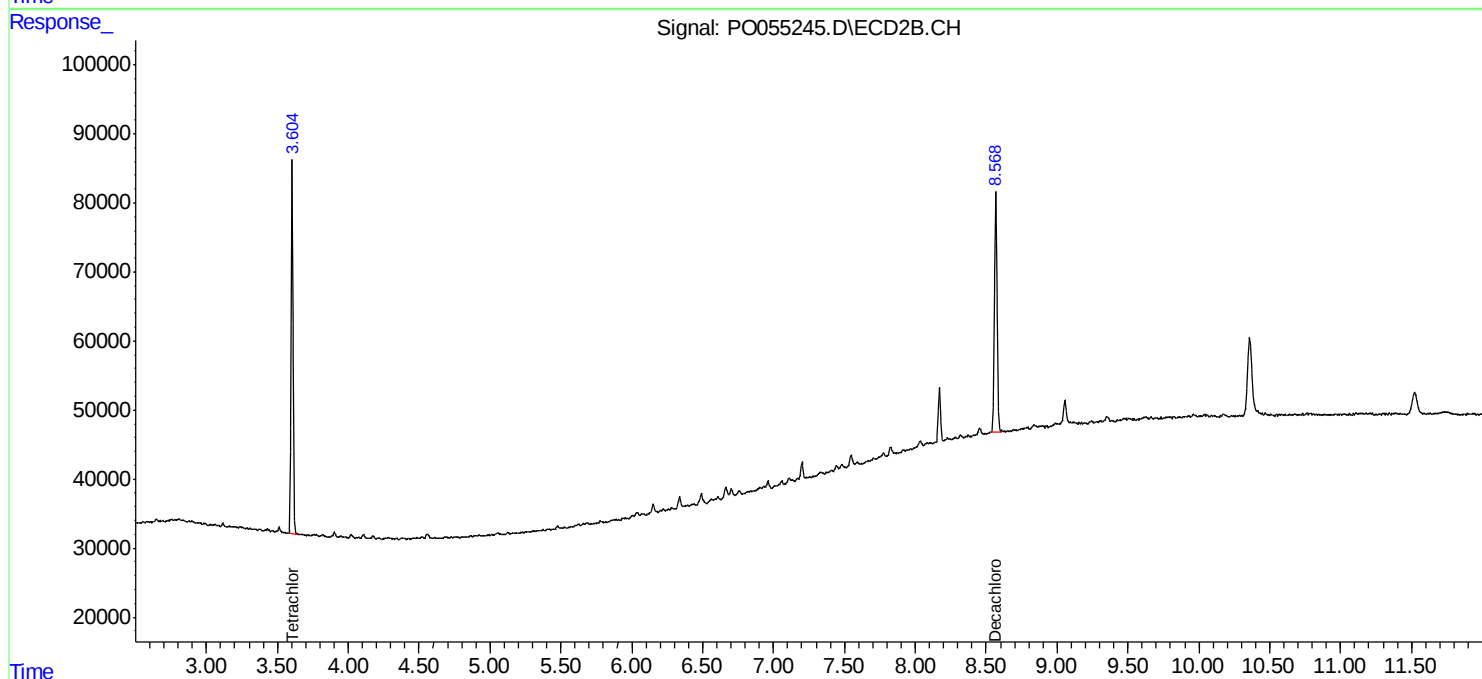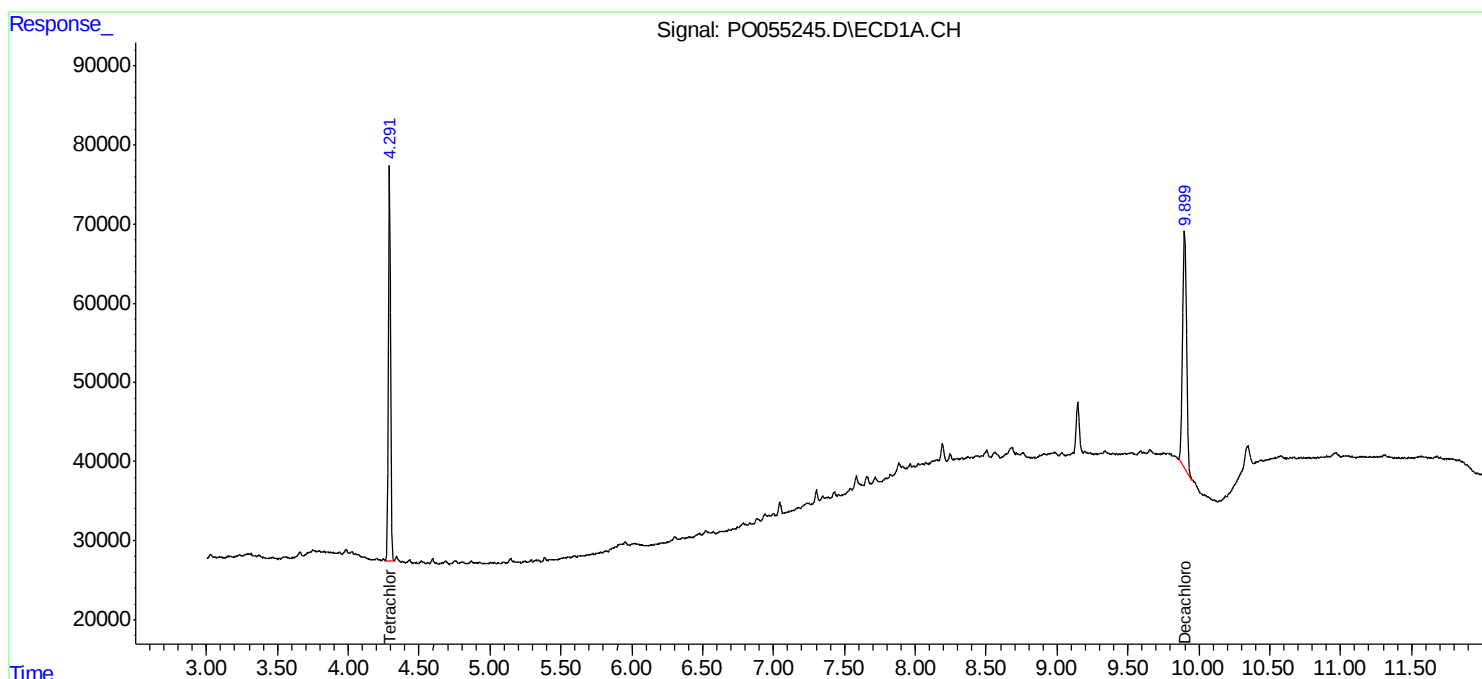


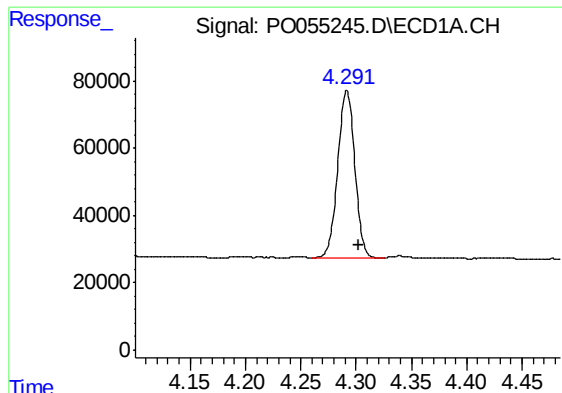

#1 Tetrachloro-m-xylene


R.T.: 4.292 min
Delta R.T.: -0.011 min
Response: 533270
Conc: 15.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-2

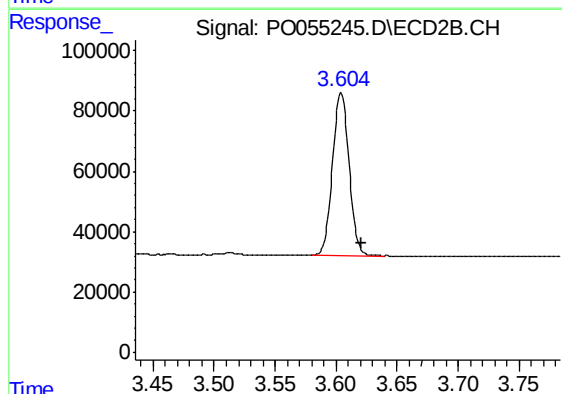


#1 Tetrachloro-m-xylene

R.T.: 3.604 min
Delta R.T.: -0.017 min
Response: 514712
Conc: 16.13 ng/ml

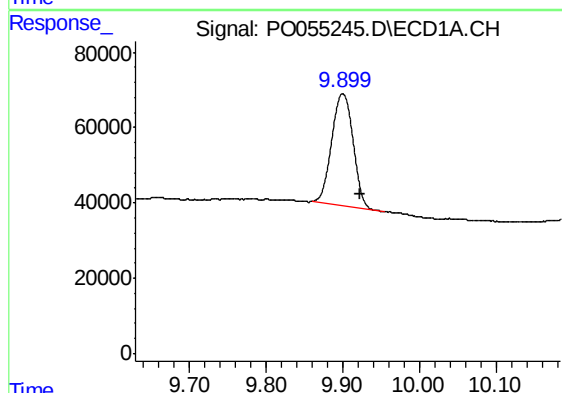

#2 Decachlorobiphenyl

R.T.: 9.900 min
Delta R.T.: -0.023 min
Response: 579455
Conc: 11.75 ng/ml

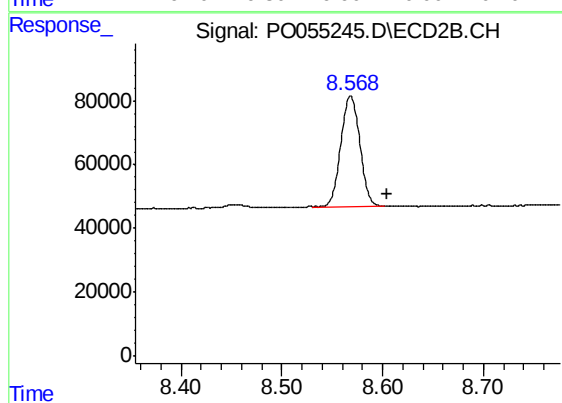

#2 Decachlorobiphenyl

R.T.: 8.568 min
Delta R.T.: -0.036 min
Response: 456508
Conc: 14.33 ng/ml