

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041219\
 Data File : P0055264.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Apr 2019 1:37
 Operator : SM/SJ
 Sample : K2376-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-4-S

Manual Integrations
 APPROVED

mohammad
 4/15/2019 4:47:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 02:28:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.277	3.605	3032710	700018	87.385m	21.936 #
2)	SA Decachlor...	9.904	8.568	545919	403863	11.074	12.681m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041219\
Data File : P0055264.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Apr 2019 1:37
Operator : SM/SJ
Sample : K2376-03
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-4-S


Manual Integrations
APPROVED

mohammad
4/15/2019 4:47:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 02:28:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

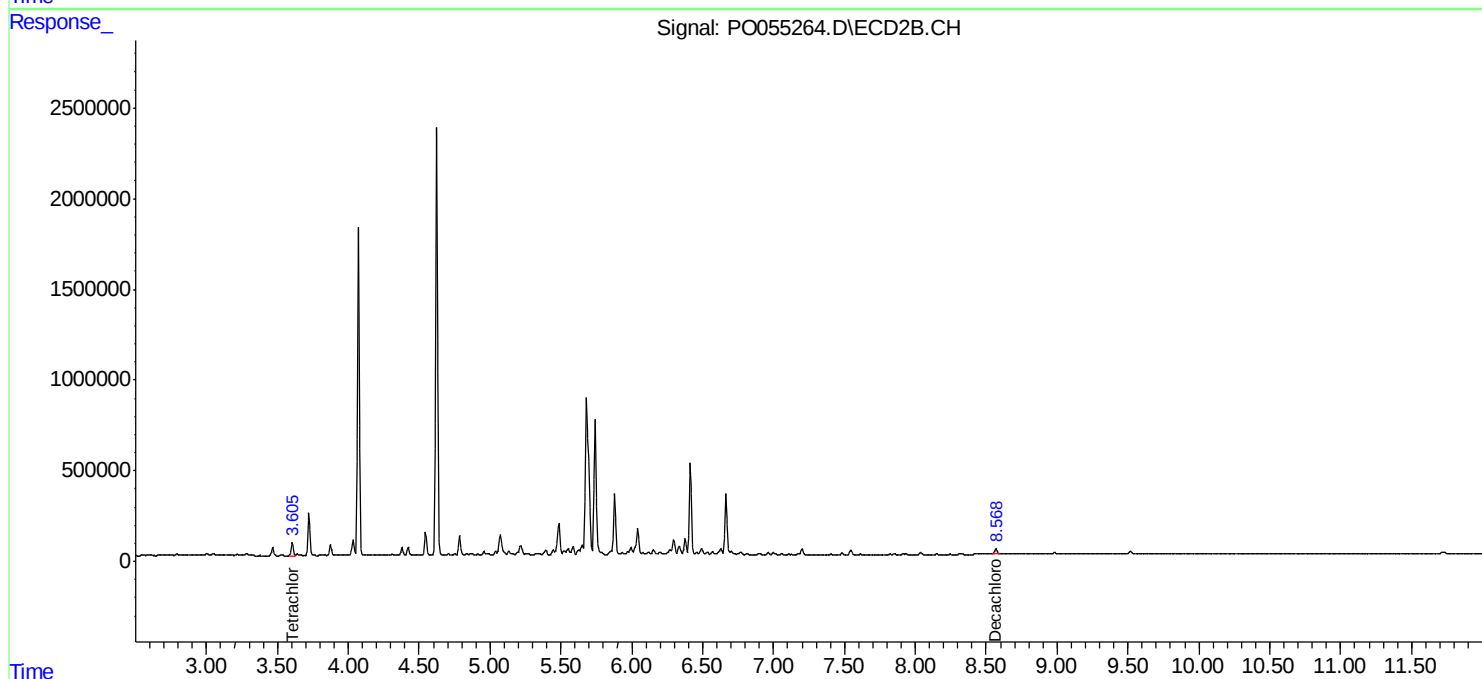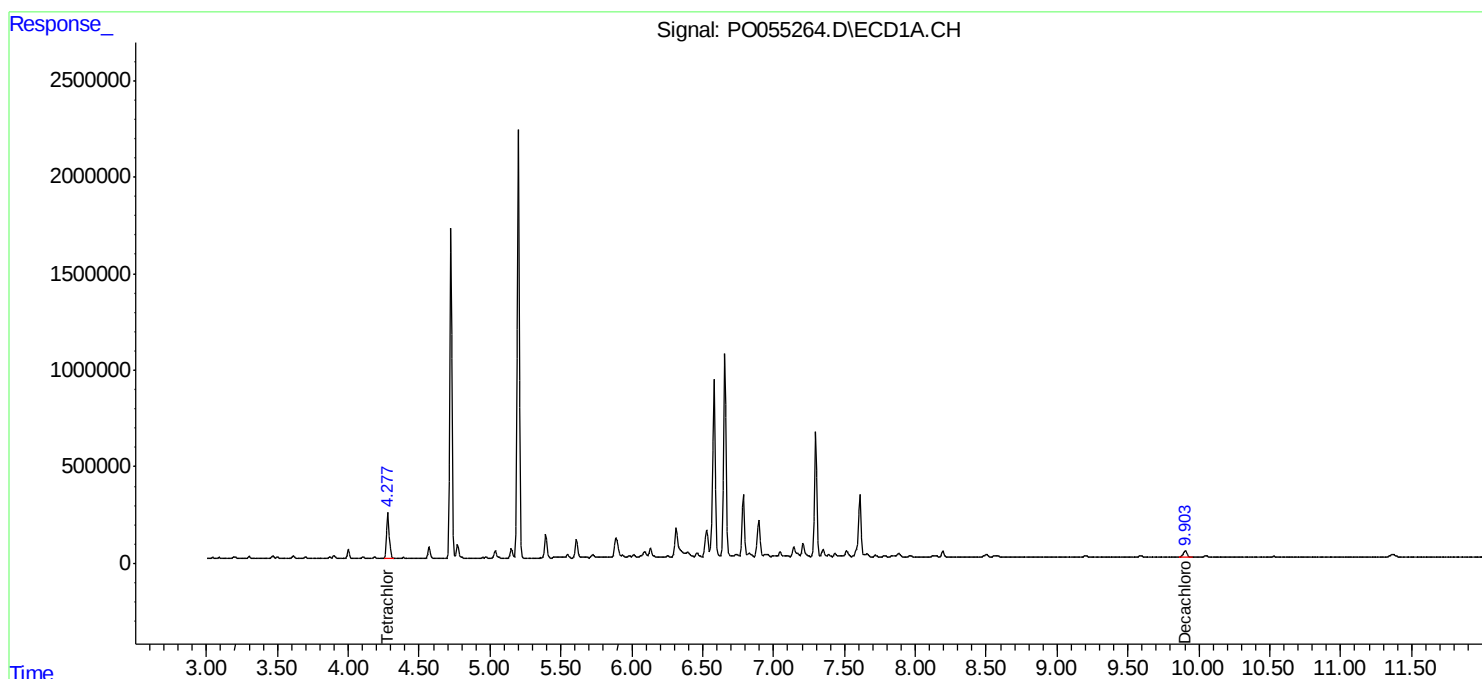

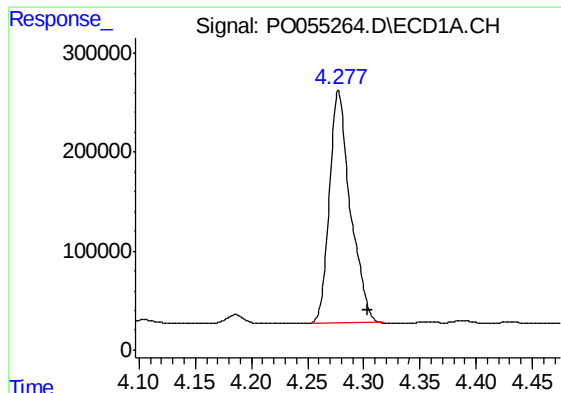


#1 Tetrachloro-m-xylene

R.T.: 4.277 min
Delta R.T.: -0.026 min
Response: 3032710
Conc: 87.39 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-4-S


Manual Integrations
APPROVED

mohammad
4/15/2019 4:47:13 PM

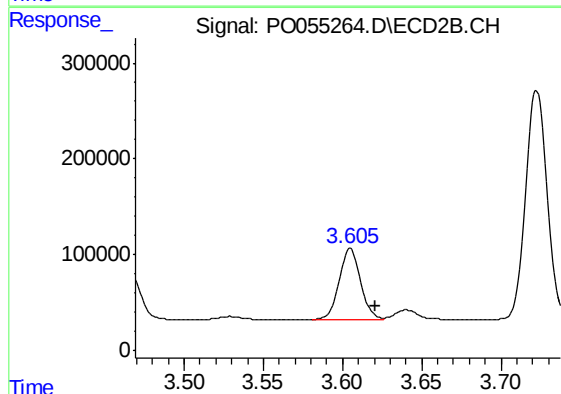


#1 Tetrachloro-m-xylene

R.T.: 3.605 min
Delta R.T.: -0.016 min
Response: 700018
Conc: 21.94 ng/ml

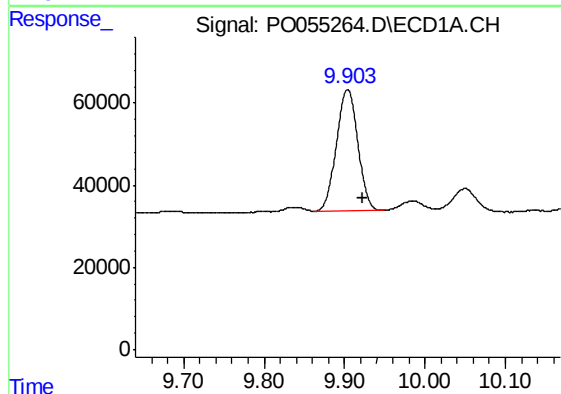

#2 Decachlorobiphenyl

R.T.: 9.904 min
Delta R.T.: -0.019 min
Response: 545919
Conc: 11.07 ng/ml

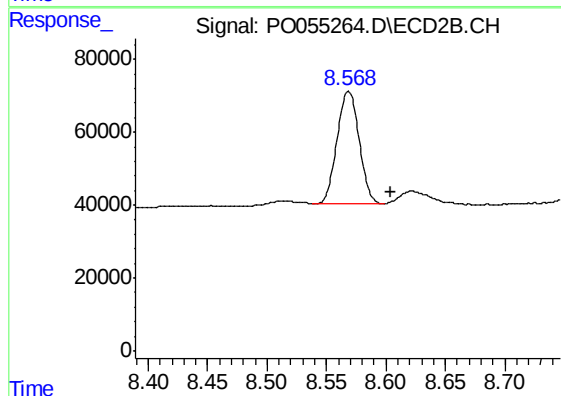

#2 Decachlorobiphenyl

R.T.: 8.568 min
Delta R.T.: -0.036 min
Response: 403863
Conc: 12.68 ng/ml m